

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012779.D
 Acq On : 26 Nov 2022 22:08
 Operator : CG/JU
 Sample : PB149078BL
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK078

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012779.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.399	32	36	42	rBV	157480	201936	1.24%	0.124%
2	3.816	104	107	129	rBV	1962562	3077295	18.88%	1.893%
3	4.163	161	166	173	rBV	43845	66024	0.41%	0.041%
4	7.163	669	676	685	rBV	2263795	3652324	22.41%	2.246%
5	7.340	699	706	716	rVB	2022223	3160784	19.40%	1.944%
6	7.546	734	741	754	rBV	2347257	3707767	22.75%	2.280%
7	8.016	814	821	830	rVB	2146722	3484423	21.38%	2.143%
8	8.716	932	940	957	rBV	2944429	4836523	29.68%	2.975%
9	9.187	1011	1020	1032	rBV	2188700	3611103	22.16%	2.221%
10	9.910	1135	1143	1151	rBV	1862080	2973686	18.25%	1.829%
11	10.445	1227	1234	1248	rBV	3134245	5097035	31.28%	3.135%
12	10.834	1292	1300	1309	rBV	3322727	5558039	34.11%	3.418%
13	10.969	1314	1323	1337	rBV	3121518	5315068	32.62%	3.269%
14	12.416	1562	1569	1574	rVB	53386	88478	0.54%	0.054%
15	13.628	1771	1775	1780	rVB3	12961	19874	0.12%	0.012%
16	14.057	1841	1848	1861	rBV	6024300	8459546	51.91%	5.203%
17	14.345	1890	1897	1910	rBV	6817889	10101351	61.99%	6.212%
18	14.651	1942	1949	1958	rBV	5366561	8259151	50.68%	5.079%
19	14.833	1972	1980	2000	rBV	2647935	3838144	23.55%	2.360%
20	15.057	2014	2018	2025	rVB6	15324	23886	0.15%	0.015%
21	15.645	2111	2118	2128	rBV	8913620	12949882	79.47%	7.964%
22	15.751	2130	2136	2148	rVV	2374220	3235815	19.86%	1.990%
23	15.886	2154	2159	2164	rVB	40312	57854	0.36%	0.036%
24	17.192	2376	2381	2387	rVB2	12460	21145	0.13%	0.013%
25	17.410	2411	2418	2427	rBV	7075910	9973604	61.21%	6.134%
26	17.510	2428	2435	2448	rVV	10078707	14080114	86.41%	8.659%
27	19.310	2736	2741	2747	rBV	115565	172815	1.06%	0.106%
28	19.380	2748	2753	2758	rVV	106474	156390	0.96%	0.096%
29	19.733	2807	2813	2825	rBV	12013178	16295094	100.00%	10.022%
30	21.492	3107	3112	3127	rBV	7458533	9848920	60.44%	6.057%
31	23.845	3505	3512	3520	rBV2	5959495	12133340	74.46%	7.462%
32	24.009	3533	3540	3554	rVB2	3958196	8142001	49.97%	5.007%


Sum of corrected areas: 162599411

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012779.D
Acq On : 26 Nov 2022 22:08
Operator : CG/JU
Sample : PB149078BL
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK078

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

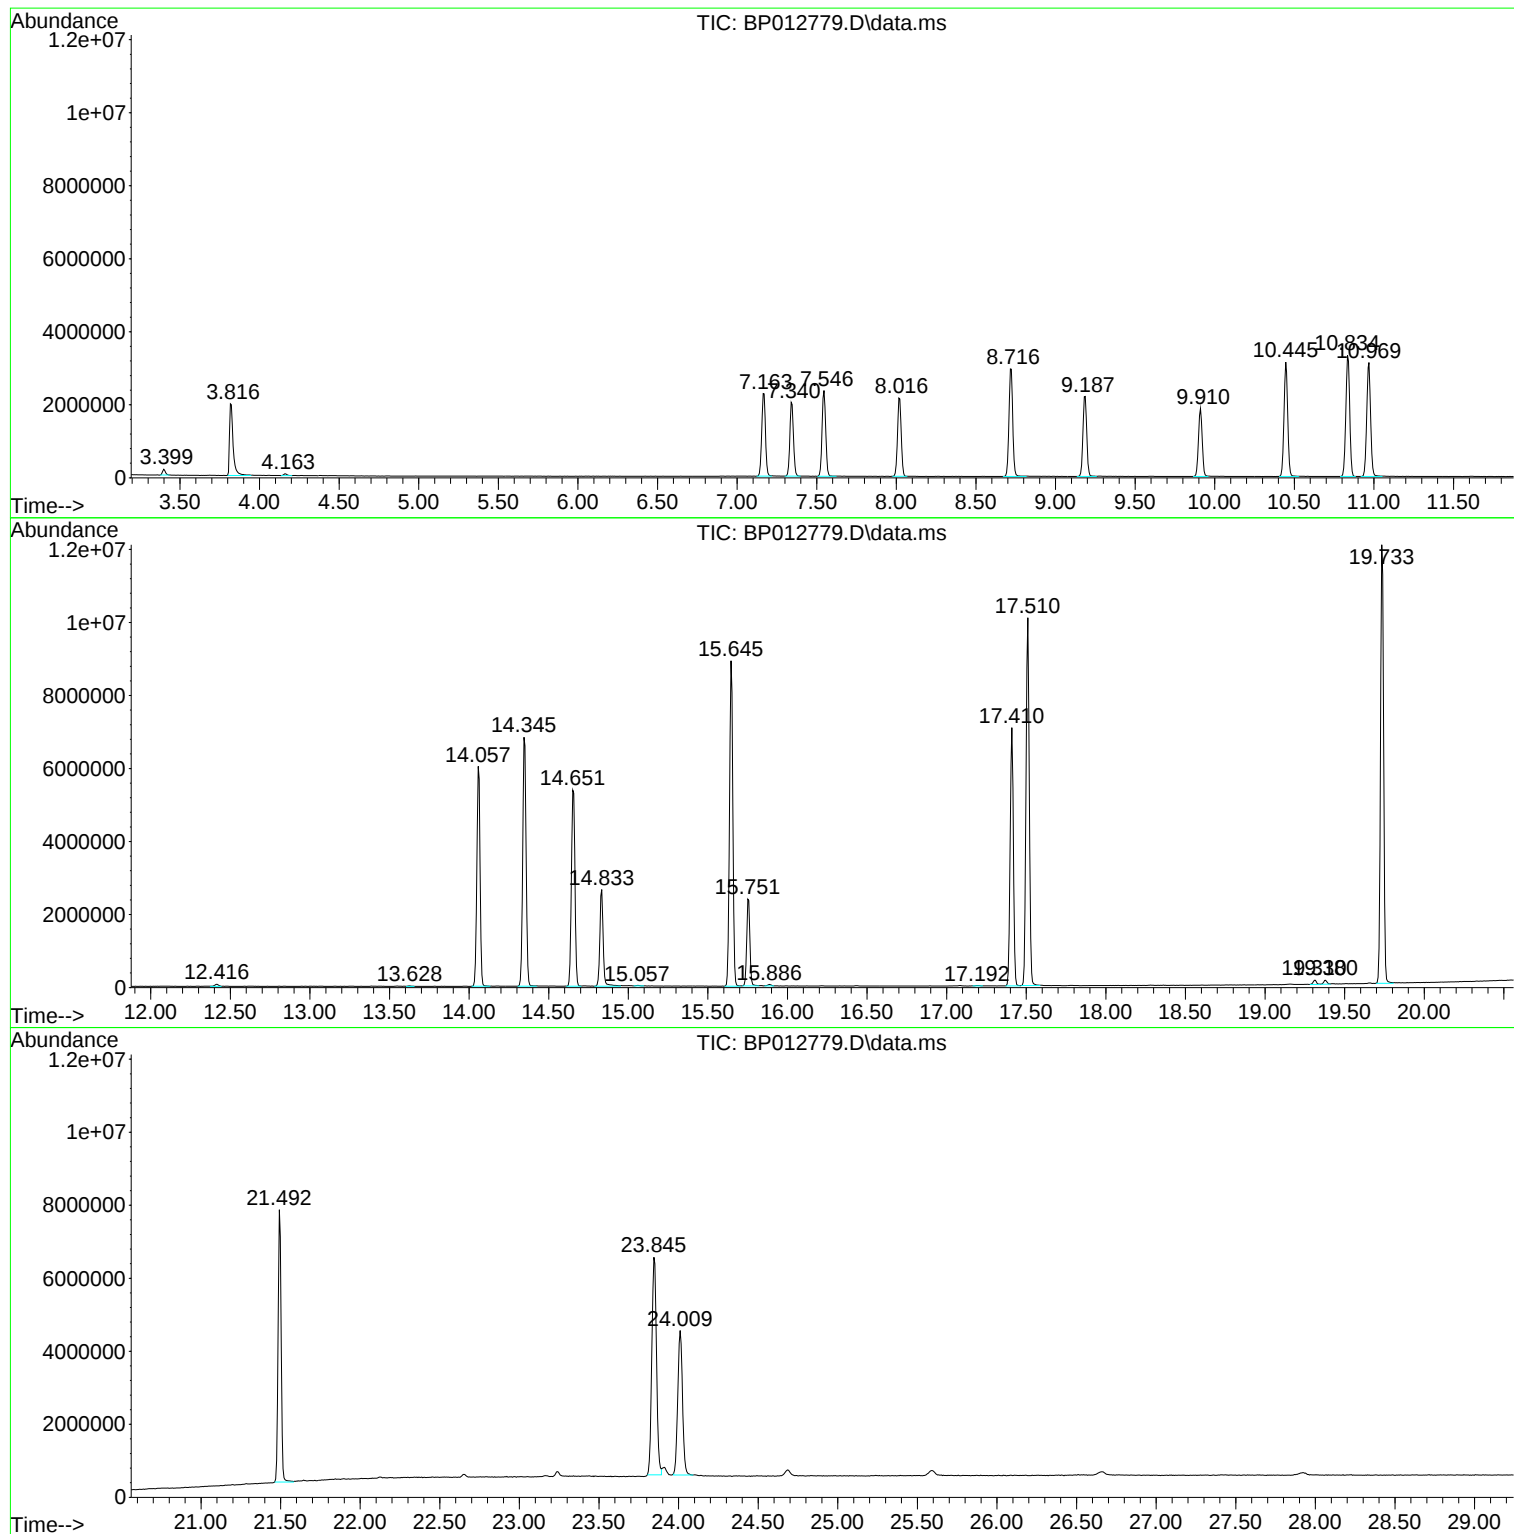

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012779.D
Acq On : 26 Nov 2022 22:08
Operator : CG/JU
Sample : PB149078BL
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK078

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012779.D
Acq On : 26 Nov 2022 22:08
Operator : CG/JU
Sample : PB149078BL
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK078

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc