

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012780.D
 Acq On : 26 Nov 2022 22:42
 Operator : CG/JU
 Sample : PB149205BL
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK205

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012780.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.393	32	35	45	rVB	121888	178048	1.20%	0.130%
2	3.816	105	107	124	rBV	879565	1501814	10.10%	1.095%
3	4.158	161	165	174	rVB	31408	51314	0.35%	0.037%
4	7.163	668	676	688	rBV	1916820	3033187	20.39%	2.212%
5	7.340	699	706	719	rVB	1705355	2641283	17.76%	1.926%
6	7.546	734	741	752	rBV	1930623	3056032	20.55%	2.228%
7	8.016	813	821	831	rBV	1582348	2564919	17.25%	1.870%
8	8.716	933	940	951	rBV	2452416	3919868	26.36%	2.858%
9	9.181	1012	1019	1031	rBV	1838603	2928424	19.69%	2.135%
10	9.910	1134	1143	1156	rBV	1461985	2369064	15.93%	1.728%
11	10.446	1226	1234	1248	rBV	2523746	4099243	27.56%	2.989%
12	10.834	1292	1300	1309	rBV	2399659	3987077	26.81%	2.907%
13	10.963	1315	1322	1337	rBV	1440602	2471679	16.62%	1.802%
14	11.604	1425	1431	1435	rBV9	10159	19439	0.13%	0.014%
15	12.416	1561	1569	1574	rBV	45028	72222	0.49%	0.053%
16	13.622	1768	1774	1781	rVB4	10132	19401	0.13%	0.014%
17	14.057	1841	1848	1859	rBV	5053423	7128329	47.93%	5.198%
18	14.345	1890	1897	1916	rBV	5705559	8464504	56.91%	6.172%
19	14.651	1942	1949	1957	rBV	3919399	5774564	38.83%	4.211%
20	14.834	1972	1980	1996	rBV	2237685	3280348	22.06%	2.392%
21	15.063	2015	2019	2025	rVB8	14816	22459	0.15%	0.016%
22	15.645	2110	2118	2129	rBV	7787218	11051331	74.31%	8.059%
23	15.751	2130	2136	2148	rVV	2012049	2717597	18.27%	1.982%
24	15.886	2153	2159	2164	rVB	33129	54693	0.37%	0.040%
25	16.428	2247	2251	2257	rBV6	10213	19465	0.13%	0.014%
26	17.192	2377	2381	2387	rBV3	10054	16479	0.11%	0.012%
27	17.410	2409	2418	2428	rBV	4936121	7129950	47.94%	5.199%
28	17.510	2428	2435	2454	rVV	8396914	12166940	81.81%	8.872%
29	18.280	2562	2566	2569	rBV6	13700	18228	0.12%	0.013%
30	19.310	2737	2741	2746	rBV	96173	134077	0.90%	0.098%
31	19.380	2748	2753	2757	rVV	93891	133087	0.89%	0.097%
32	19.733	2807	2813	2828	rBV	11437688	14771203	99.32%	10.771%
33	21.492	3107	3112	3125	rBV	6092684	8104828	54.49%	5.910%
34	23.851	3504	3513	3520	rBV2	7169268	14872815	100.00%	10.845%
35	24.010	3533	3540	3555	rVB2	4012033	8363121	56.23%	6.098%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012780.D
Acq On : 26 Nov 2022 22:42
Operator : CG/JU
Sample : PB149205BL
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK205

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Title : SVOA CALIBRATION




Sum of corrected areas: 137137032

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012780.D
Acq On : 26 Nov 2022 22:42
Operator : CG/JU
Sample : PB149205BL
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK205

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

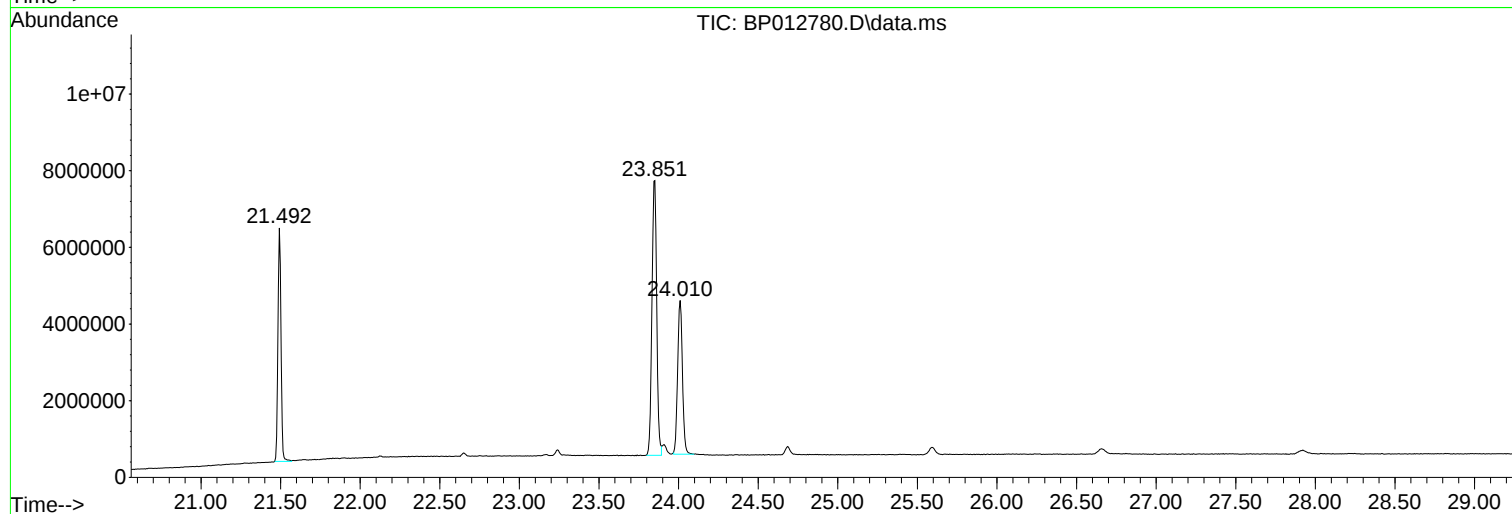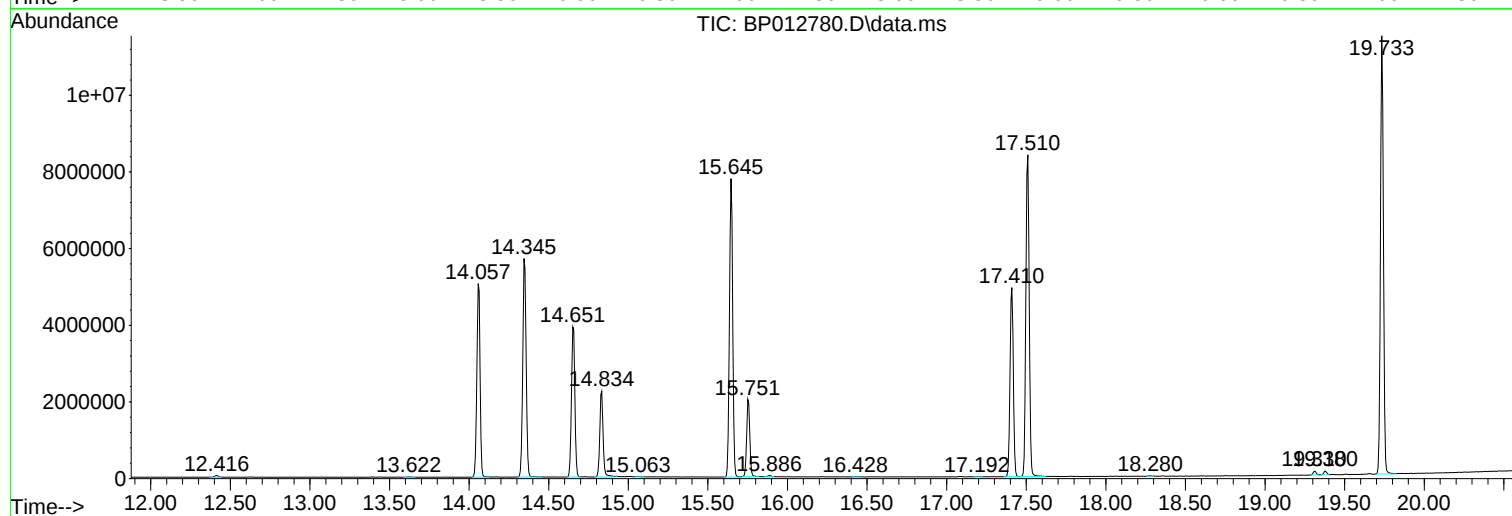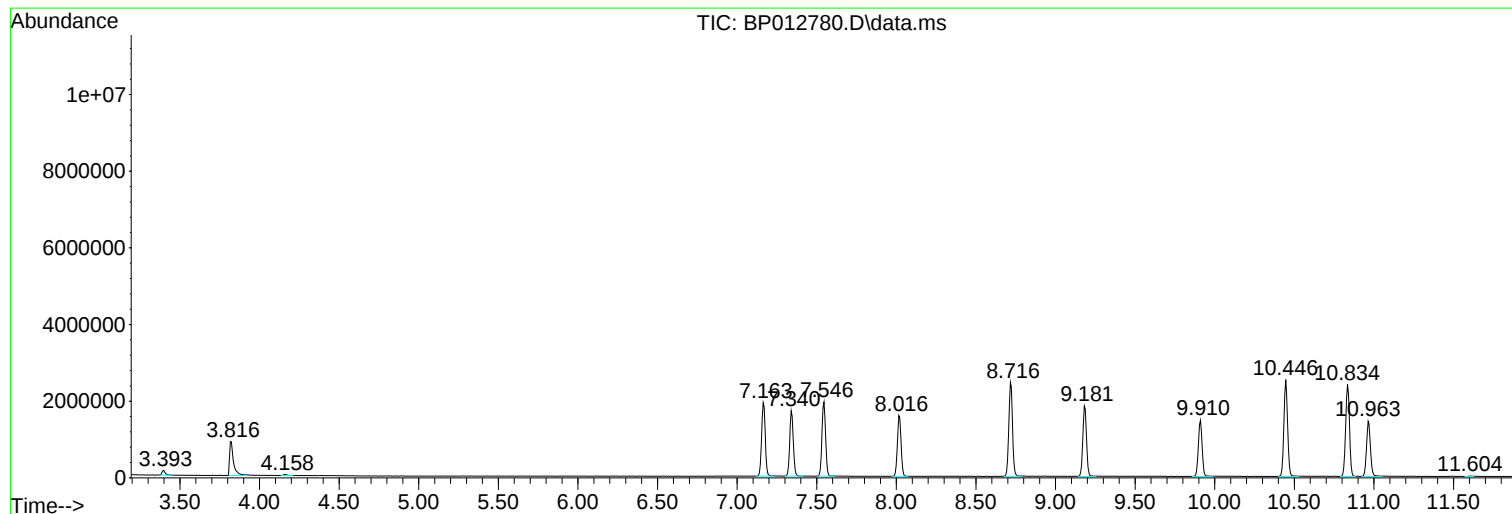

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012780.D
Acq On : 26 Nov 2022 22:42
Operator : CG/JU
Sample : PB149205BL
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK205

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012780.D
Acq On : 26 Nov 2022 22:42
Operator : CG/JU
Sample : PB149205BL
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK205

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc