

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012784.D
 Acq On : 27 Nov 2022 00:58
 Operator : CG/JU
 Sample : N5694-11
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHB47

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012784.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.364	27	30	32	rBV3	36586	42718	0.24%	0.029%
2	3.393	32	35	39	rVV	97382	134302	0.77%	0.090%
3	3.434	39	42	48	rVB	48821	72367	0.41%	0.048%
4	3.687	82	85	89	rVB3	12566	19548	0.11%	0.013%
5	3.822	105	108	121	rBV	297563	527603	3.02%	0.353%
6	4.064	143	149	158	rBV	46752	84730	0.48%	0.057%
7	4.158	161	165	171	rBV	35831	51797	0.30%	0.035%
8	5.105	321	326	331	rBV4	11676	20919	0.12%	0.014%
9	6.087	488	493	501	rVB4	10860	19894	0.11%	0.013%
10	7.163	669	676	689	rVB	572754	889402	5.09%	0.596%
11	7.340	699	706	714	rBV	1783227	2740271	15.68%	1.835%
12	7.546	732	741	748	rBV	1646527	2649645	15.16%	1.774%
13	7.610	748	752	760	rVB	70200	123103	0.70%	0.082%
14	8.016	813	821	828	rBV	1867844	2941158	16.83%	1.969%
15	8.075	828	831	837	rVB	65473	95634	0.55%	0.064%
16	8.716	929	940	952	rBV	1573294	2487954	14.24%	1.666%
17	9.181	1011	1019	1028	rBV	1925312	3070172	17.57%	2.056%
18	9.604	1087	1091	1096	rVB	30407	47667	0.27%	0.032%
19	9.910	1135	1143	1157	rBV	1436455	2387886	13.66%	1.599%
20	10.122	1174	1179	1186	rVB3	38013	64357	0.37%	0.043%
21	10.446	1225	1234	1249	rBV	2493984	4154844	23.77%	2.782%
22	10.834	1292	1300	1308	rBV	2845834	4691758	26.85%	3.141%
23	10.963	1314	1322	1335	rBV	1937584	3292017	18.84%	2.204%
24	11.069	1335	1340	1347	rVB5	38497	68060	0.39%	0.046%
25	11.234	1361	1368	1374	rVB5	26391	54190	0.31%	0.036%
26	11.387	1387	1394	1399	rBV5	22634	54082	0.31%	0.036%
27	11.657	1436	1440	1447	rVB	85547	139171	0.80%	0.093%
28	11.722	1447	1451	1455	rVV	37548	56751	0.32%	0.038%
29	11.769	1455	1459	1468	rVB	48807	90449	0.52%	0.061%
30	12.246	1533	1540	1545	rBV3	31533	50105	0.29%	0.034%
31	12.410	1563	1568	1575	rVB	47727	77084	0.44%	0.052%
32	13.475	1745	1749	1755	rVB	46080	62931	0.36%	0.042%
33	13.545	1755	1761	1769	rBV	206852	326312	1.87%	0.218%
34	13.622	1770	1774	1779	rVB5	9666	18897	0.11%	0.013%
35	14.057	1841	1848	1858	rBV	5776182	7852879	44.94%	5.258%
36	14.181	1865	1869	1875	rVB9	10778	21429	0.12%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012784.D
 Acq On : 27 Nov 2022 00:58
 Operator : CG/JU
 Sample : N5694-11
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHB47

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

37	14.345	1890	1897	1907	rBV	6177899	8797079	50.34%	5.890%
38	14.545	1928	1931	1936	rVB4	15181	20220	0.12%	0.014%
39	14.651	1940	1949	1958	rBV	4641682	6811378	38.98%	4.561%
40	14.722	1958	1961	1967	rVB7	13093	18599	0.11%	0.012%
41	14.828	1973	1979	1991	rBV	578107	891578	5.10%	0.597%
42	14.992	2003	2007	2012	rBV8	14170	27687	0.16%	0.019%
43	15.057	2013	2018	2024	rVB8	35490	59318	0.34%	0.040%
44	15.645	2111	2118	2129	rBV	8453998	12205374	69.84%	8.172%
45	15.751	2129	2136	2147	rBV	2370191	3143614	17.99%	2.105%
46	15.887	2153	2159	2165	rVB2	37643	64256	0.37%	0.043%
47	16.010	2175	2180	2185	rBV	34724	44480	0.25%	0.030%
48	17.198	2378	2382	2385	rBV4	12032	18503	0.11%	0.012%
49	17.410	2411	2418	2428	rBV	5774604	8321145	47.61%	5.572%
50	17.510	2428	2435	2445	rVV	9783670	14315280	81.91%	9.585%
51	17.592	2445	2449	2455	rVB2	82692	123026	0.70%	0.082%
52	17.781	2477	2481	2485	rBV3	27431	35408	0.20%	0.024%
53	18.069	2526	2530	2537	rVB8	29818	41342	0.24%	0.028%
54	18.275	2561	2565	2575	rBV	224818	318557	1.82%	0.213%
55	18.692	2632	2636	2642	rBV	168533	211236	1.21%	0.141%
56	18.751	2642	2646	2650	rVV5	29617	43279	0.25%	0.029%
57	19.310	2737	2741	2747	rBV	128967	175495	1.00%	0.118%
58	19.380	2748	2753	2758	rBV	135426	211252	1.21%	0.141%
59	19.510	2771	2775	2782	rBV	122034	165662	0.95%	0.111%
60	19.657	2797	2800	2807	rVB6	40231	47994	0.27%	0.032%
61	19.733	2807	2813	2826	rBV	13056495	17476052	100.00%	11.701%
62	21.186	3056	3060	3069	rBV	323062	438767	2.51%	0.294%
63	21.492	3107	3112	3123	rBV	7107588	9317621	53.32%	6.239%
64	23.851	3505	3513	3520	rBV2	8281898	17049074	97.56%	11.415%
65	24.010	3533	3540	3557	rVB2	4565879	9475579	54.22%	6.345%




Sum of corrected areas: 149350941

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012784.D
Acq On : 27 Nov 2022 00:58
Operator : CG/JU
Sample : N5694-11
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHB47

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

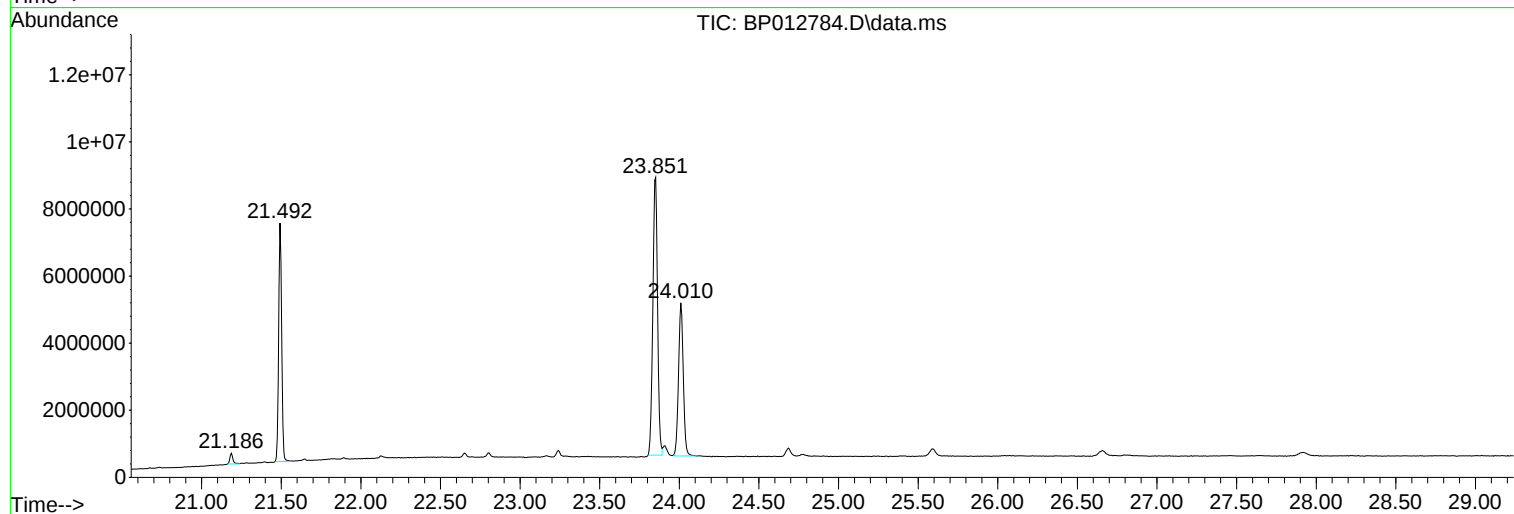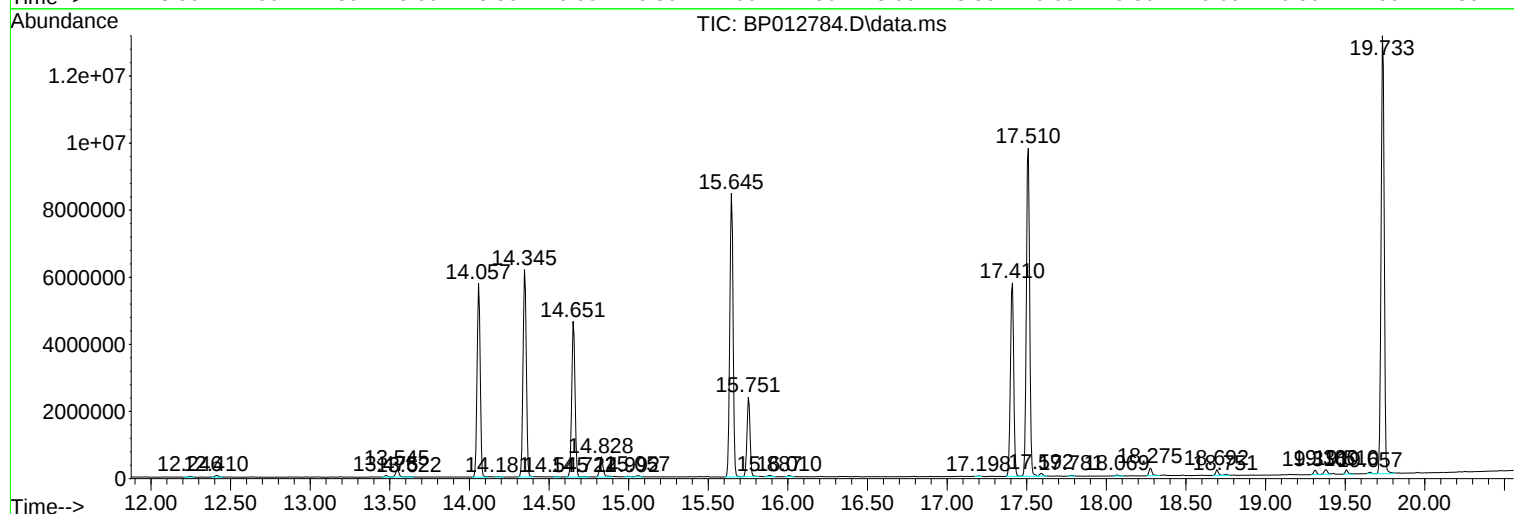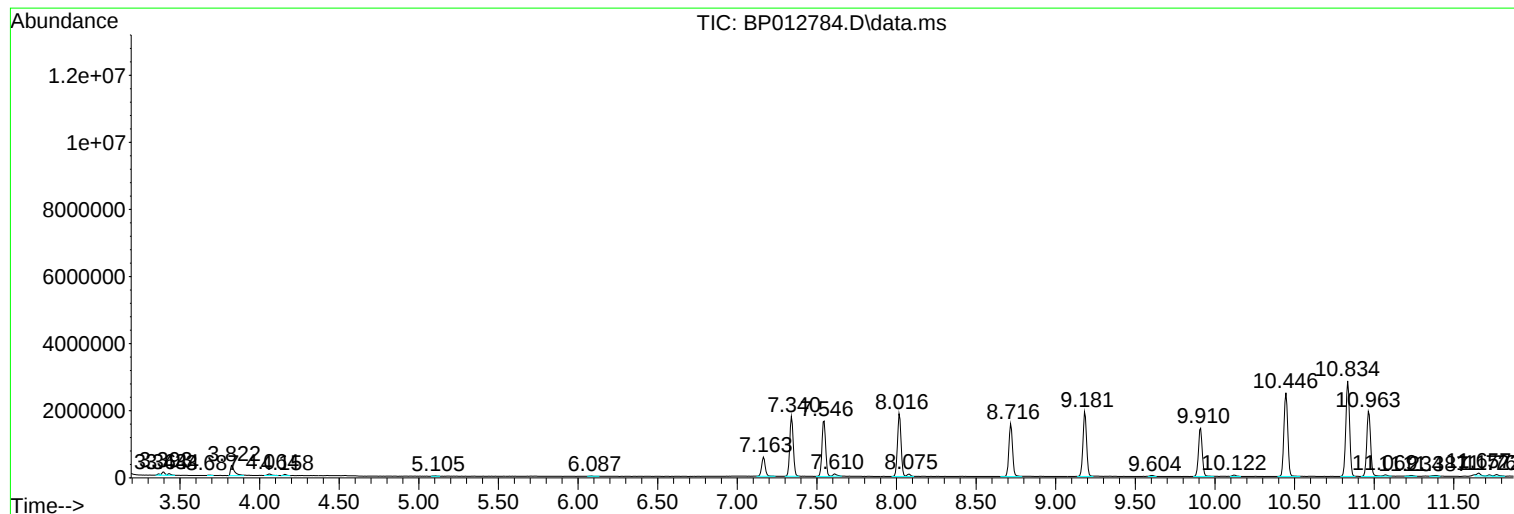

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012784.D
Acq On : 27 Nov 2022 00:58
Operator : CG/JU
Sample : N5694-11
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHB47

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012784.D
Acq On : 27 Nov 2022 00:58
Operator : CG/JU
Sample : N5694-11
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHB47

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc