

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012785.D
 Acq On : 27 Nov 2022 01:32
 Operator : CG/JU
 Sample : N5710-04
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COKY3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012785.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.364	25	30	39	rBV	2478192	4029626	15.57%	2.260%
2	3.429	39	41	51	rVB	184005	268807	1.04%	0.151%
3	3.823	105	108	125	rBV	453770	715368	2.76%	0.401%
4	4.058	144	148	153	rVB	48366	72522	0.28%	0.041%
5	4.158	161	165	171	rBV	34552	50459	0.20%	0.028%
6	4.699	250	257	272	rBV	15744117	25875211	100.00%	14.513%
7	5.305	352	360	367	rBV	90696	149086	0.58%	0.084%
8	7.164	668	676	685	rBV	409947	664944	2.57%	0.373%
9	7.340	699	706	716	rBV	1841116	2890438	11.17%	1.621%
10	7.546	733	741	750	rBV	1528951	2471107	9.55%	1.386%
11	7.634	751	756	760	rVV7	12956	26157	0.10%	0.015%
12	7.705	764	768	775	rVB4	23133	39403	0.15%	0.022%
13	8.017	814	821	839	rVB	1925561	3112563	12.03%	1.746%
14	8.716	933	940	951	rBV	1289014	2036142	7.87%	1.142%
15	9.181	1009	1019	1029	rBV	2047624	3260538	12.60%	1.829%
16	9.605	1083	1091	1098	rVB	71924	119290	0.46%	0.067%
17	9.911	1132	1143	1157	rBV	1465203	2439568	9.43%	1.368%
18	10.446	1225	1234	1248	rBV	2464835	4037826	15.60%	2.265%
19	10.834	1292	1300	1308	rBV	2850221	4779487	18.47%	2.681%
20	10.905	1308	1312	1315	rVV	25800	40272	0.16%	0.023%
21	10.963	1315	1322	1341	rVB	2328259	3966116	15.33%	2.224%
22	12.099	1512	1515	1520	rVB	29288	45260	0.17%	0.025%
23	12.246	1534	1540	1545	rBV2	42262	61271	0.24%	0.034%
24	12.416	1561	1569	1574	rBV	49852	82252	0.32%	0.046%
25	13.475	1744	1749	1756	rVB	71214	108216	0.42%	0.061%
26	14.057	1841	1848	1858	rBV	5509054	7661861	29.61%	4.297%
27	14.251	1875	1881	1887	rBV	64752	111170	0.43%	0.062%
28	14.346	1890	1897	1904	rVV	6568245	9284964	35.88%	5.208%
29	14.399	1904	1906	1918	rVB9	25351	46530	0.18%	0.026%
30	14.546	1927	1931	1937	rVB3	24017	33074	0.13%	0.019%
31	14.651	1942	1949	1957	rBV	4726866	6966018	26.92%	3.907%
32	14.828	1972	1979	1986	rBV	358957	532297	2.06%	0.299%
33	15.057	2013	2018	2024	rVB7	34409	57368	0.22%	0.032%
34	15.646	2111	2118	2130	rBV	8749300	12264867	47.40%	6.879%
35	15.751	2130	2136	2152	rVV	2087821	2785746	10.77%	1.562%
36	15.887	2152	2159	2166	rVB3	38176	79069	0.31%	0.044%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012785.D
 Acq On : 27 Nov 2022 01:32
 Operator : CG/JU
 Sample : N5710-04
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0KY3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

37	16.010	2175	2180	2185	rBV	35081	47987	0.19%	0.027%
38	16.434	2248	2252	2257	rVB7	13889	26153	0.10%	0.015%
39	17.192	2378	2381	2390	rVB4	19368	39618	0.15%	0.022%
40	17.410	2411	2418	2427	rBV	5987011	8605669	33.26%	4.827%
41	17.510	2428	2435	2445	rVV	9466848	13847996	53.52%	7.767%
42	17.592	2445	2449	2454	rVB	135753	183115	0.71%	0.103%
43	17.781	2477	2481	2485	rBV6	23049	30889	0.12%	0.017%
44	18.275	2561	2565	2575	rBV	402731	554162	2.14%	0.311%
45	18.487	2597	2601	2604	rVB5	18675	26606	0.10%	0.015%
46	18.692	2632	2636	2643	rBV2	177334	220080	0.85%	0.123%
47	19.310	2736	2741	2747	rBV2	126449	188252	0.73%	0.106%
48	19.375	2748	2752	2758	rBV	127033	216713	0.84%	0.122%
49	19.504	2770	2774	2783	rBV3	192178	277076	1.07%	0.155%
50	19.657	2797	2800	2803	rVB4	39836	41035	0.16%	0.023%
51	19.734	2807	2813	2828	rBV	12849181	16746524	64.72%	9.393%
52	21.186	3056	3060	3067	rBV	543144	710139	2.74%	0.398%
53	21.492	3106	3112	3125	rBV	7359828	9758756	37.71%	5.473%
54	23.845	3504	3512	3520	rBV2	8035154	16060003	62.07%	9.008%
55	24.010	3532	3540	3556	rVB2	4494252	9549731	36.91%	5.356%




Sum of corrected areas: 178295397

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012785.D
Acq On : 27 Nov 2022 01:32
Operator : CG/JU
Sample : N5710-04
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KY3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

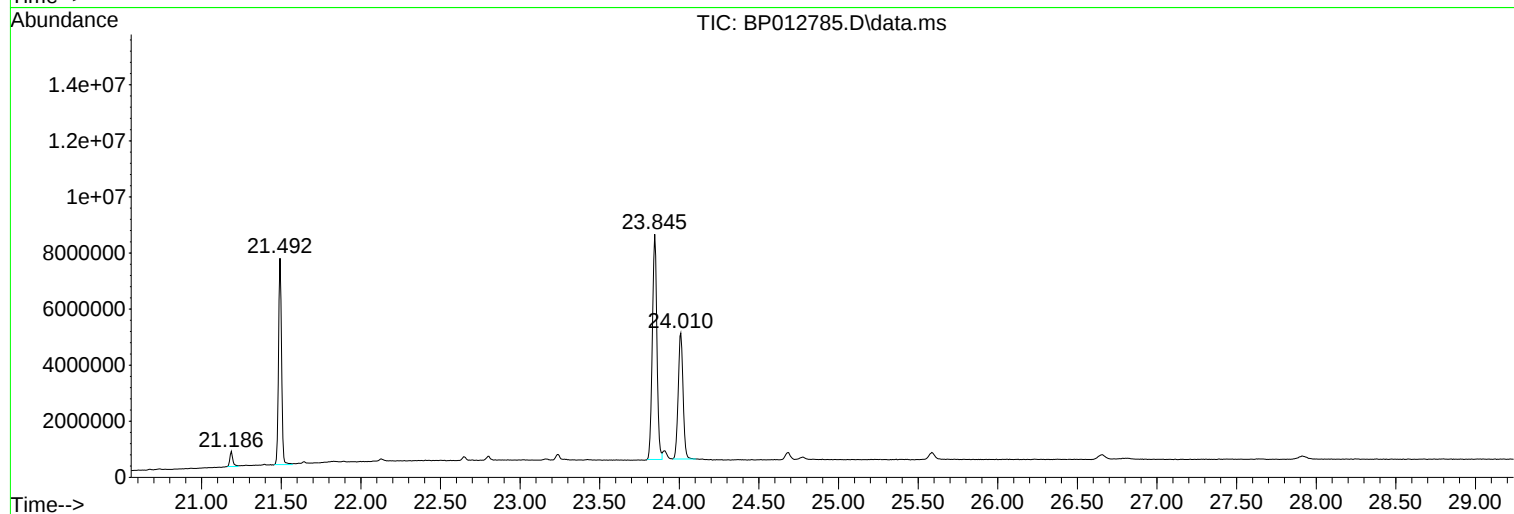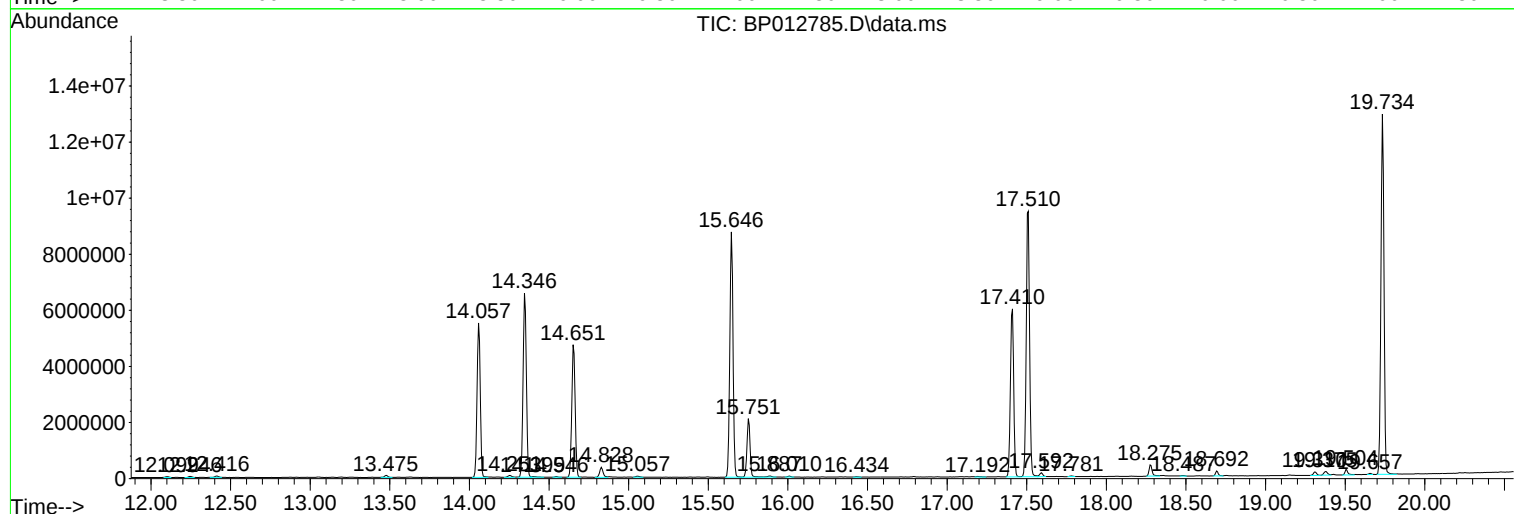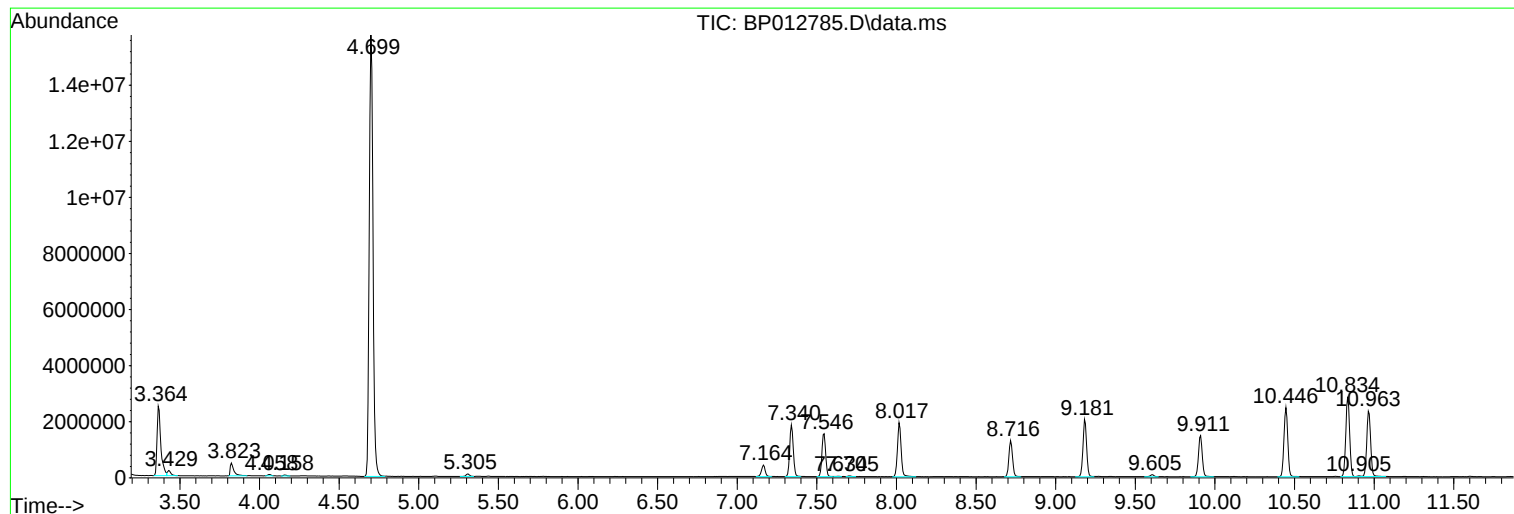

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012785.D
Acq On : 27 Nov 2022 01:32
Operator : CG/JU
Sample : N5710-04
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KY3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012785.D
Acq On : 27 Nov 2022 01:32
Operator : CG/JU
Sample : N5710-04
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KY3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc