

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012787.D
 Acq On : 27 Nov 2022 02:41
 Operator : CG/JU
 Sample : N5661-02
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C9803

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012787.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.393	31	35	45	rVB	107150	159840	0.93%	0.113%
2	3.681	82	84	93	rVB5	14034	23730	0.14%	0.017%
3	3.823	106	108	124	rBV	373413	627233	3.66%	0.442%
4	4.064	144	149	156	rVB	50475	78808	0.46%	0.056%
5	4.158	161	165	172	rVB	29355	44284	0.26%	0.031%
6	4.534	227	229	234	rVB6	11342	17565	0.10%	0.012%
7	5.099	322	325	330	rVB2	18488	26343	0.15%	0.019%
8	7.164	668	676	688	rVB	444803	701088	4.10%	0.495%
9	7.340	699	706	716	rBV	1842036	2849708	16.65%	2.010%
10	7.546	733	741	749	rBV	1315499	2101968	12.28%	1.483%
11	7.616	749	753	761	rVB4	18793	40480	0.24%	0.029%
12	8.016	814	821	828	rBV	1727551	2701095	15.78%	1.905%
13	8.716	932	940	951	rBV	1176956	1834646	10.72%	1.294%
14	9.181	1011	1019	1029	rBV	2003429	3219795	18.81%	2.271%
15	9.281	1031	1036	1044	rVB	57649	95983	0.56%	0.068%
16	9.605	1086	1091	1099	rVB2	31625	52200	0.30%	0.037%
17	9.910	1131	1143	1154	rBV	1281588	2127299	12.43%	1.500%
18	10.022	1157	1162	1166	rBV2	17477	29948	0.17%	0.021%
19	10.446	1226	1234	1243	rBV	2085954	3341963	19.53%	2.357%
20	10.834	1291	1300	1307	rBV	2602889	4300568	25.13%	3.033%
21	10.963	1314	1322	1333	rBV	2038706	3502177	20.46%	2.470%
22	12.246	1534	1540	1544	rBV	38400	61121	0.36%	0.043%
23	12.410	1561	1568	1574	rBV	47186	79802	0.47%	0.056%
24	13.057	1674	1678	1687	rVB8	11674	23498	0.14%	0.017%
25	13.193	1696	1701	1705	rBV5	14467	22537	0.13%	0.016%
26	13.475	1745	1749	1756	rVB2	56016	85737	0.50%	0.060%
27	13.546	1756	1761	1767	rVV4	17563	32978	0.19%	0.023%
28	13.628	1770	1775	1781	rVB5	13565	28202	0.16%	0.020%
29	14.057	1841	1848	1859	rBV	5290963	7103084	41.50%	5.010%
30	14.293	1883	1888	1890	rBV6	13300	22158	0.13%	0.016%
31	14.346	1890	1897	1906	rVV	5900950	8751515	51.13%	6.173%
32	14.428	1906	1911	1918	rVB	64678	99443	0.58%	0.070%
33	14.545	1927	1931	1934	rBV4	16612	22349	0.13%	0.016%
34	14.651	1942	1949	1958	rVB	4401271	6276138	36.67%	4.427%
35	14.828	1972	1979	1991	rBV	349629	565503	3.30%	0.399%
36	15.057	2014	2018	2025	rVB5	43458	71434	0.42%	0.050%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012787.D
 Acq On : 27 Nov 2022 02:41
 Operator : CG/JU
 Sample : N5661-02
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C9803

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

37	15.645	2111	2118	2129	rBV	8340794	11899063	69.52%	8.393%
38	15.751	2129	2136	2148	rVV	1837971	2434702	14.22%	1.717%
39	15.881	2155	2158	2171	rVB	38440	68745	0.40%	0.048%
40	16.010	2175	2180	2185	rVV	166391	227759	1.33%	0.161%
41	16.345	2232	2237	2244	rVV8	12951	35692	0.21%	0.025%
42	16.428	2249	2251	2257	rVB5	12761	17214	0.10%	0.012%
43	17.404	2411	2417	2428	rBV	5425311	7788429	45.50%	5.494%
44	17.504	2428	2434	2445	rVV	9771179	14023695	81.93%	9.892%
45	17.592	2446	2449	2453	rVB3	42380	56392	0.33%	0.040%
46	17.781	2478	2481	2486	rBV5	16333	20778	0.12%	0.015%
47	17.898	2498	2501	2504	rBV4	17818	23099	0.13%	0.016%
48	18.069	2526	2530	2536	rBV8	21740	29137	0.17%	0.021%
49	18.275	2561	2565	2573	rBV	265161	372238	2.17%	0.263%
50	18.563	2612	2614	2618	rBV4	20549	26259	0.15%	0.019%
51	18.692	2633	2636	2641	rVB5	35731	37091	0.22%	0.026%
52	19.310	2737	2741	2746	rBV2	138926	179748	1.05%	0.127%
53	19.375	2748	2752	2757	rBV	126535	185099	1.08%	0.131%
54	19.504	2770	2774	2784	rBV	137303	202648	1.18%	0.143%
55	19.651	2797	2799	2806	rVB3	47764	56495	0.33%	0.040%
56	19.733	2807	2813	2830	rVV	13155675	17115814	100.00%	12.073%
57	21.186	3056	3060	3065	rBV	324363	472564	2.76%	0.333%
58	21.492	3106	3112	3124	rVB	6572510	8785081	51.33%	6.196%
59	23.233	3405	3408	3414	rVB	229503	340026	1.99%	0.240%
60	23.845	3504	3512	3519	rBV2	8322302	16794873	98.12%	11.846%
61	24.010	3532	3540	3554	rVB2	4217679	8846723	51.69%	6.240%
62	24.680	3650	3654	3663	rVB2	298023	613550	3.58%	0.433%




Sum of corrected areas: 141775134

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012787.D
Acq On : 27 Nov 2022 02:41
Operator : CG/JU
Sample : N5661-02
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C9803

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

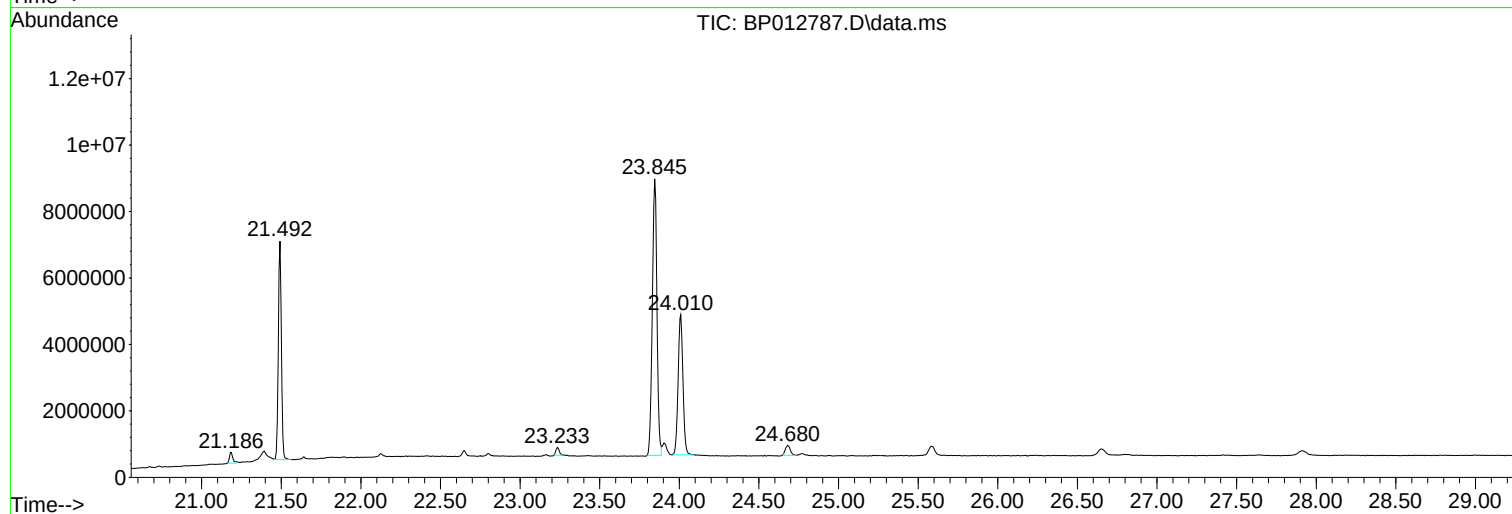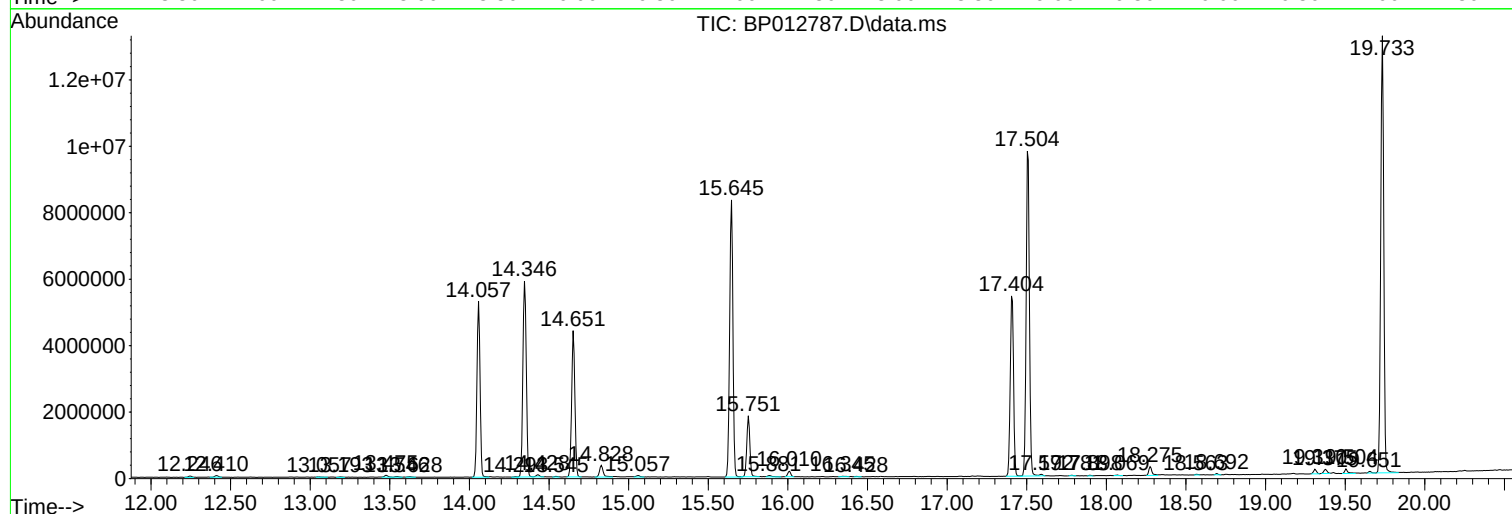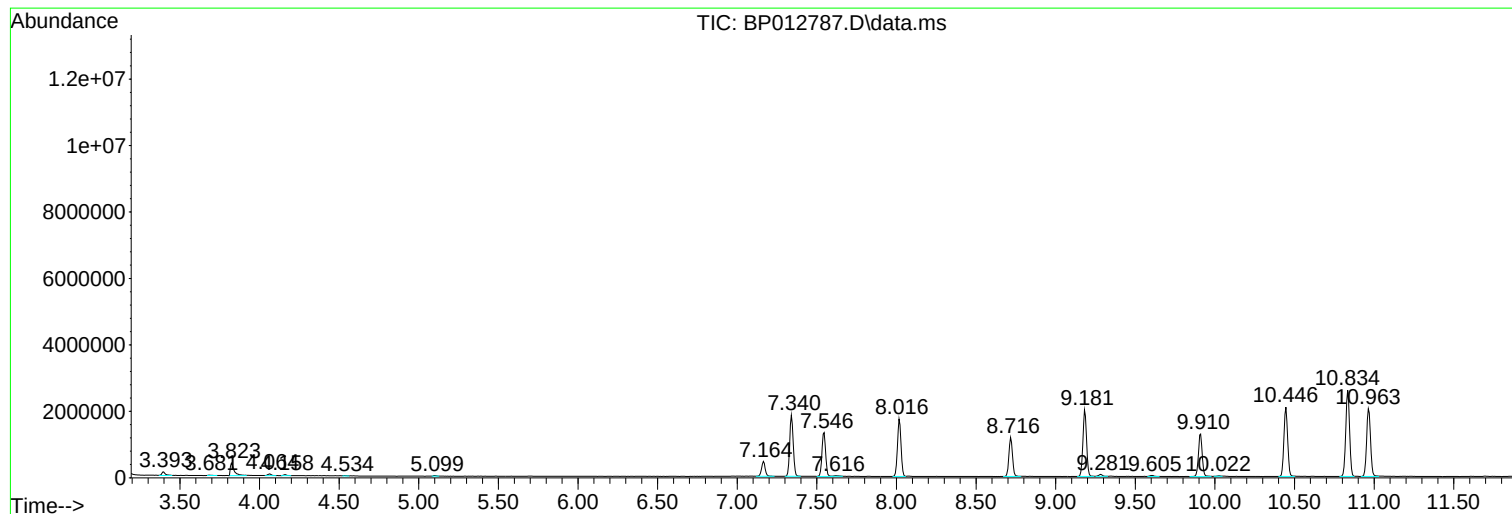

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012787.D
Acq On : 27 Nov 2022 02:41
Operator : CG/JU
Sample : N5661-02
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C9803

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012787.D
Acq On : 27 Nov 2022 02:41
Operator : CG/JU
Sample : N5661-02
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C9803

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc