

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012788.D
 Acq On : 27 Nov 2022 03:15
 Operator : CG/JU
 Sample : N5710-08
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COKY7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012788.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.364	26	30	38	rBV2	579537	1019276	5.69%	0.641%
2	3.434	38	42	51	rVB	207361	308497	1.72%	0.194%
3	3.681	81	84	88	rBV4	25668	39156	0.22%	0.025%
4	3.722	88	91	99	rVB	84470	128789	0.72%	0.081%
5	3.822	104	108	125	rBV	449968	703834	3.93%	0.443%
6	4.064	144	149	155	rVB	54248	80854	0.45%	0.051%
7	4.158	161	165	170	rVB	35693	47479	0.27%	0.030%
8	4.534	226	229	236	rVB6	12491	21929	0.12%	0.014%
9	4.699	250	257	268	rBV	2812751	4225754	23.60%	2.659%
10	5.111	320	327	331	rVB7	11401	23916	0.13%	0.015%
11	5.281	351	356	360	rBV	29139	50601	0.28%	0.032%
12	5.440	377	383	388	rBV	27900	43283	0.24%	0.027%
13	6.416	543	549	556	rBV	19250	38459	0.21%	0.024%
14	6.563	568	574	580	rVB2	11608	21367	0.12%	0.013%
15	6.975	639	644	648	rBV7	12955	25661	0.14%	0.016%
16	7.163	669	676	686	rVB	611535	969355	5.41%	0.610%
17	7.340	699	706	717	rBV	1903548	2943425	16.44%	1.852%
18	7.546	733	741	750	rBV	1780035	2825659	15.78%	1.778%
19	7.628	751	755	759	rVV5	16645	34015	0.19%	0.021%
20	7.704	763	768	773	rVB8	18409	32341	0.18%	0.020%
21	8.016	814	821	828	rBV	1929719	3060148	17.09%	1.926%
22	8.075	828	831	837	rVB	21271	31298	0.17%	0.020%
23	8.416	882	889	901	rBV	32895	62184	0.35%	0.039%
24	8.716	933	940	953	rBV	1603824	2564249	14.32%	1.614%
25	8.828	955	959	964	rVB6	11555	21116	0.12%	0.013%
26	9.181	1010	1019	1030	rBV	2049969	3306346	18.47%	2.081%
27	9.275	1030	1035	1040	rVV4	23225	43332	0.24%	0.027%
28	9.346	1042	1047	1052	rVB3	22952	34972	0.20%	0.022%
29	9.604	1085	1091	1095	rVB3	22760	34987	0.20%	0.022%
30	9.746	1110	1115	1119	rVB8	12171	21466	0.12%	0.014%
31	9.910	1134	1143	1151	rBV	1569778	2569874	14.35%	1.617%
32	10.187	1184	1190	1195	rBV6	13292	26336	0.15%	0.017%
33	10.446	1226	1234	1245	rBV	2601113	4337866	24.23%	2.730%
34	10.610	1259	1262	1270	rVB7	16181	28383	0.16%	0.018%
35	10.687	1270	1275	1281	rBV10	11119	19074	0.11%	0.012%
36	10.757	1281	1287	1292	rBV2	26608	46251	0.26%	0.029%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012788.D
 Acq On : 27 Nov 2022 03:15
 Operator : CG/JU
 Sample : N5710-08
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COKY7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

37	10.834	1292	1300	1308	rBV	2986617	4884606	27.28%	3.074%
38	10.963	1315	1322	1335	rBV	2055055	3466366	19.36%	2.181%
39	11.187	1356	1360	1364	rBV4	11093	19799	0.11%	0.012%
40	11.487	1405	1411	1418	rVB2	20327	39249	0.22%	0.025%
41	11.604	1427	1431	1437	rVV5	15712	25667	0.14%	0.016%
42	11.798	1454	1464	1468	rBV5	8991	22743	0.13%	0.014%
43	12.157	1520	1525	1532	rVB3	16896	31380	0.18%	0.020%
44	12.410	1562	1568	1575	rVB	58592	92930	0.52%	0.058%
45	12.828	1635	1639	1646	rBV3	21041	32978	0.18%	0.021%
46	13.016	1665	1671	1677	rBV	58364	90734	0.51%	0.057%
47	13.263	1705	1713	1719	rBV	85529	134394	0.75%	0.085%
48	13.539	1757	1760	1766	rBV4	14908	26200	0.15%	0.016%
49	13.610	1768	1772	1781	rVB6	25556	52934	0.30%	0.033%
50	14.057	1841	1848	1854	rBV	5774997	7903026	44.14%	4.973%
51	14.104	1854	1856	1862	rVV	33320	40513	0.23%	0.025%
52	14.251	1875	1881	1890	rBV	78288	159685	0.89%	0.100%
53	14.345	1890	1897	1910	rVB	6286956	9332695	52.13%	5.873%
54	14.604	1934	1941	1943	rBV	100776	154579	0.86%	0.097%
55	14.651	1943	1949	1959	rVB	4917171	7359417	41.11%	4.631%
56	14.828	1973	1979	1987	rBV	622433	931576	5.20%	0.586%
57	15.057	2013	2018	2023	rVB7	34859	56221	0.31%	0.035%
58	15.281	2053	2056	2063	rVB6	15217	22864	0.13%	0.014%
59	15.386	2069	2074	2078	rBV3	13820	22015	0.12%	0.014%
60	15.463	2081	2087	2092	rBV2	25194	45035	0.25%	0.028%
61	15.645	2111	2118	2128	rBV	8711466	12611876	70.45%	7.937%
62	15.751	2130	2136	2152	rVV	2453901	3323503	18.56%	2.091%
63	15.886	2155	2159	2166	rVB2	42447	73629	0.41%	0.046%
64	16.333	2230	2235	2242	rVB9	11759	19841	0.11%	0.012%
65	16.416	2245	2249	2251	rBV	24611	37076	0.21%	0.023%
66	17.080	2358	2362	2367	rBV6	14354	21774	0.12%	0.014%
67	17.192	2376	2381	2388	rVB2	14888	29260	0.16%	0.018%
68	17.286	2391	2397	2400	rVB3	14878	23046	0.13%	0.015%
69	17.410	2411	2418	2425	rBV	6096665	8788386	49.09%	5.530%
70	17.510	2428	2435	2445	rBV	9970108	14605897	81.58%	9.191%
71	17.775	2477	2480	2484	rVB4	11732	19094	0.11%	0.012%
72	18.063	2526	2529	2535	rVB8	18194	27952	0.16%	0.018%
73	18.275	2561	2565	2571	rBV3	74907	100589	0.56%	0.063%
74	18.357	2575	2579	2583	rVB	27937	36665	0.20%	0.023%
75	18.751	2642	2646	2651	rBV3	37376	52016	0.29%	0.033%
76	19.310	2736	2741	2746	rBV	143906	187148	1.05%	0.118%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012788.D
 Acq On : 27 Nov 2022 03:15
 Operator : CG/JU
 Sample : N5710-08
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0KY7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

77	19.374	2748	2752	2758	rVV	129221	184285	1.03%	0.116%
78	19.427	2758	2761	2764	rVB3	19043	22953	0.13%	0.014%
79	19.504	2771	2774	2779	rBV2	65943	77284	0.43%	0.049%
80	19.657	2797	2800	2804	rVB	39863	41266	0.23%	0.026%
81	19.733	2807	2813	2823	rBV	13928709	17902748	100.00%	11.266%
82	21.492	3106	3112	3124	rBV	7354905	9853435	55.04%	6.201%
83	23.845	3504	3512	3520	rBV2	8319278	16728853	93.44%	10.527%
84	24.010	3532	3540	3551	rBV2	4525737	9400737	52.51%	5.916%




Sum of corrected areas: 158908451

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012788.D
Acq On : 27 Nov 2022 03:15
Operator : CG/JU
Sample : N5710-08
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KY7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

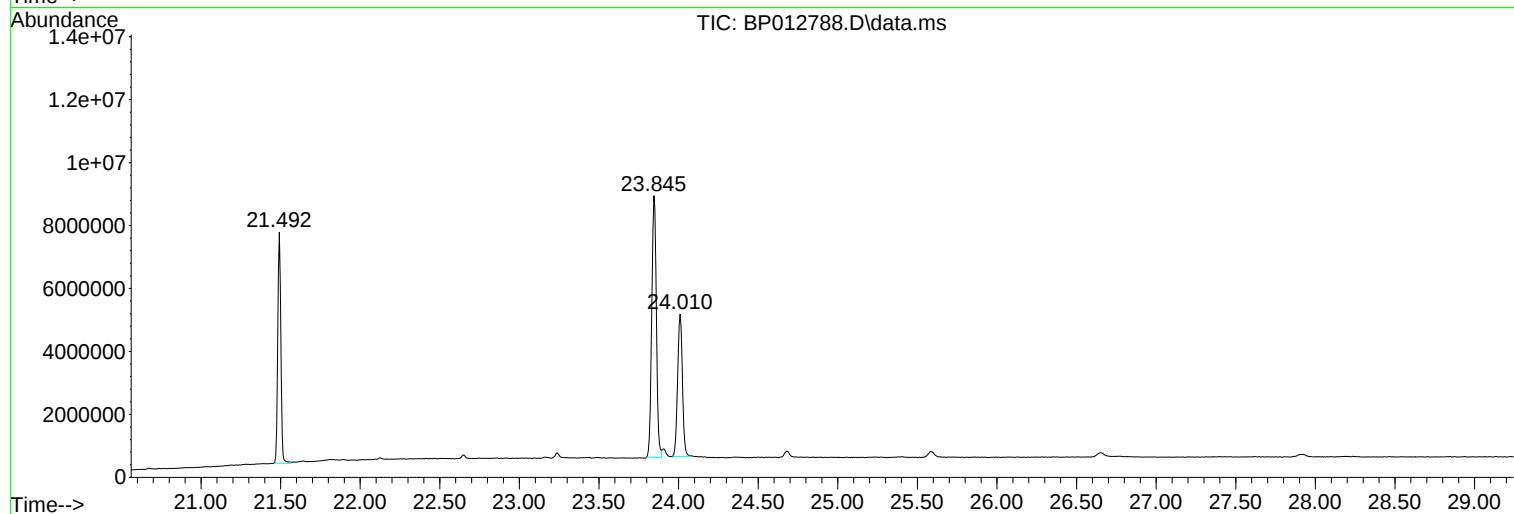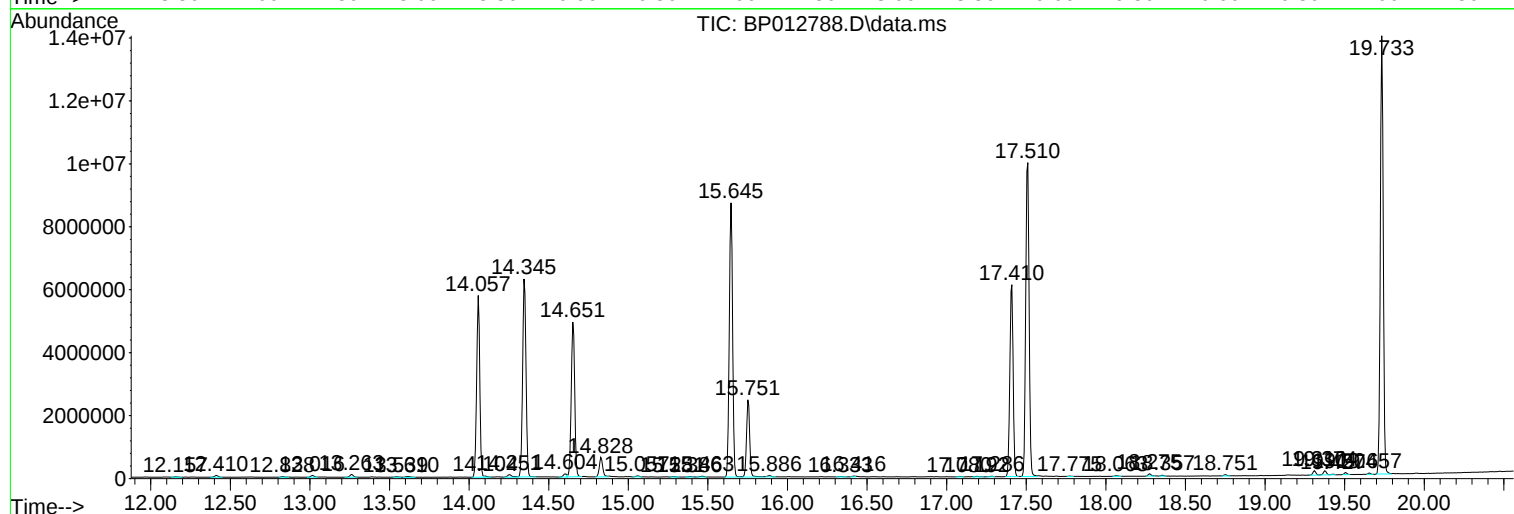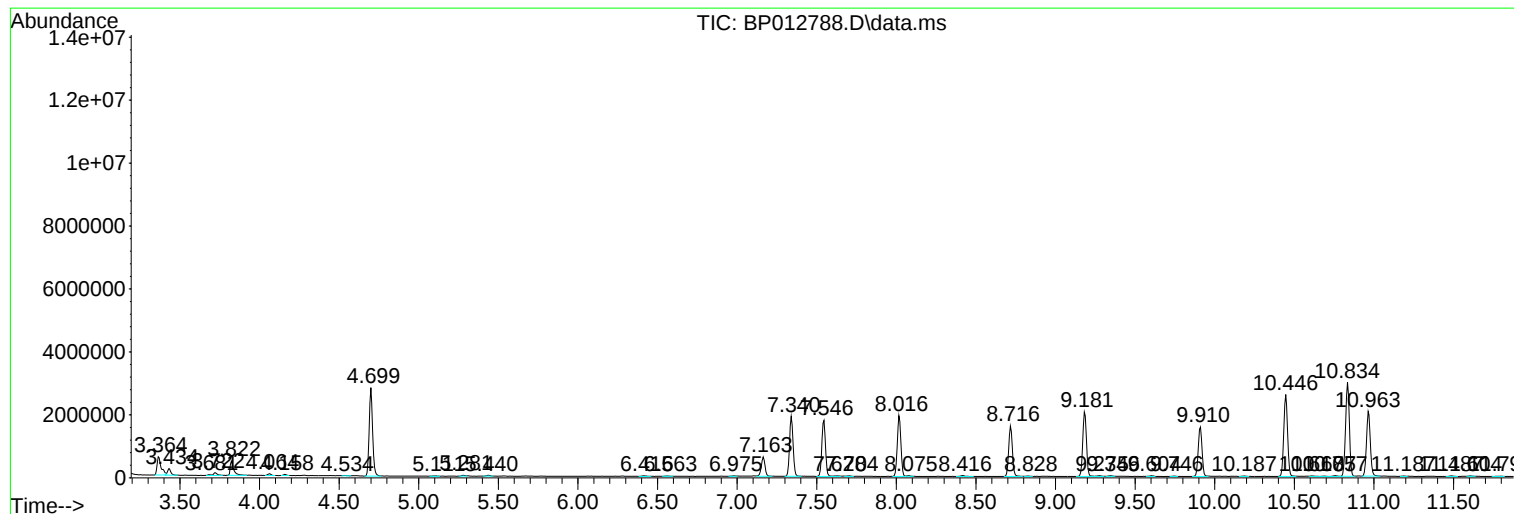

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012788.D
Acq On : 27 Nov 2022 03:15
Operator : CG/JU
Sample : N5710-08
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KY7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012788.D
Acq On : 27 Nov 2022 03:15
Operator : CG/JU
Sample : N5710-08
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KY7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc