

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012797.D
 Acq On : 27 Nov 2022 08:55
 Operator : CG/JU
 Sample : PB149251BL
 Misc :
 ALS Vial : 72 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK251

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012797.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.393	31	35	43	rVB	101852	142524	1.15%	0.121%
2	4.158	161	165	171	rBV	26948	42854	0.34%	0.036%
3	7.163	669	676	687	rBV	1612315	2523338	20.31%	2.144%
4	7.340	699	706	716	rVB	1448929	2217892	17.86%	1.884%
5	7.540	733	740	749	rBV	1618056	2576827	20.74%	2.189%
6	8.016	813	821	829	rVB	1620218	2517615	20.27%	2.139%
7	8.716	933	940	951	rBV	2117054	3282091	26.42%	2.788%
8	9.181	1010	1019	1028	rBV	1589711	2499202	20.12%	2.123%
9	9.904	1135	1142	1152	rBV	1242389	2015000	16.22%	1.712%
10	10.446	1225	1234	1246	rBV	2118453	3469549	27.93%	2.948%
11	10.834	1292	1300	1310	rVB	2421977	3985745	32.09%	3.386%
12	10.975	1316	1324	1326	rBV8	10867	21044	0.17%	0.018%
13	12.416	1563	1569	1574	rBV3	37303	64789	0.52%	0.055%
14	13.545	1755	1761	1769	rBV2	29431	51015	0.41%	0.043%
15	13.622	1769	1774	1781	rVB6	11401	17394	0.14%	0.015%
16	14.057	1841	1848	1860	rBV	4345613	5895327	47.46%	5.008%
17	14.345	1889	1897	1909	rBV	4878824	6927015	55.77%	5.885%
18	14.651	1942	1949	1957	rBV	4125665	5905628	47.54%	5.017%
19	14.828	1971	1979	1998	rBV	1820591	2656043	21.38%	2.256%
20	15.057	2014	2018	2024	rVB9	12483	18883	0.15%	0.016%
21	15.645	2111	2118	2130	rBV	6545920	9081465	73.11%	7.715%
22	15.751	2130	2136	2154	rVV	1631932	2171905	17.49%	1.845%
23	15.886	2154	2159	2164	rVB2	26825	39913	0.32%	0.034%
24	17.186	2376	2380	2385	rBV4	10920	21290	0.17%	0.018%
25	17.404	2411	2417	2427	rBV	5086040	7354126	59.20%	6.248%
26	17.504	2427	2434	2449	rBV	7034299	10179275	81.95%	8.648%
27	18.063	2526	2529	2534	rVB7	15697	22947	0.18%	0.019%
28	18.275	2562	2565	2570	rBV7	12742	19714	0.16%	0.017%
29	19.310	2737	2741	2747	rBV3	87219	118292	0.95%	0.100%
30	19.380	2749	2753	2757	rVV	72415	98240	0.79%	0.083%
31	19.651	2797	2799	2803	rVB4	22291	24910	0.20%	0.021%
32	19.733	2807	2813	2824	rBV	9603171	12421499	100.00%	10.553%
33	21.492	3106	3112	3122	rBV	6464309	8553113	68.86%	7.266%
34	23.845	3504	3512	3520	rBV2	6119324	12200201	98.22%	10.365%
35	24.004	3532	3539	3556	rVB2	4158168	8570661	69.00%	7.281%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012797.D
Acq On : 27 Nov 2022 08:55
Operator : CG/JU
Sample : PB149251BL
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK251

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Title : SVOA CALIBRATION




Sum of corrected areas: 117707326

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012797.D
Acq On : 27 Nov 2022 08:55
Operator : CG/JU
Sample : PB149251BL
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK251

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

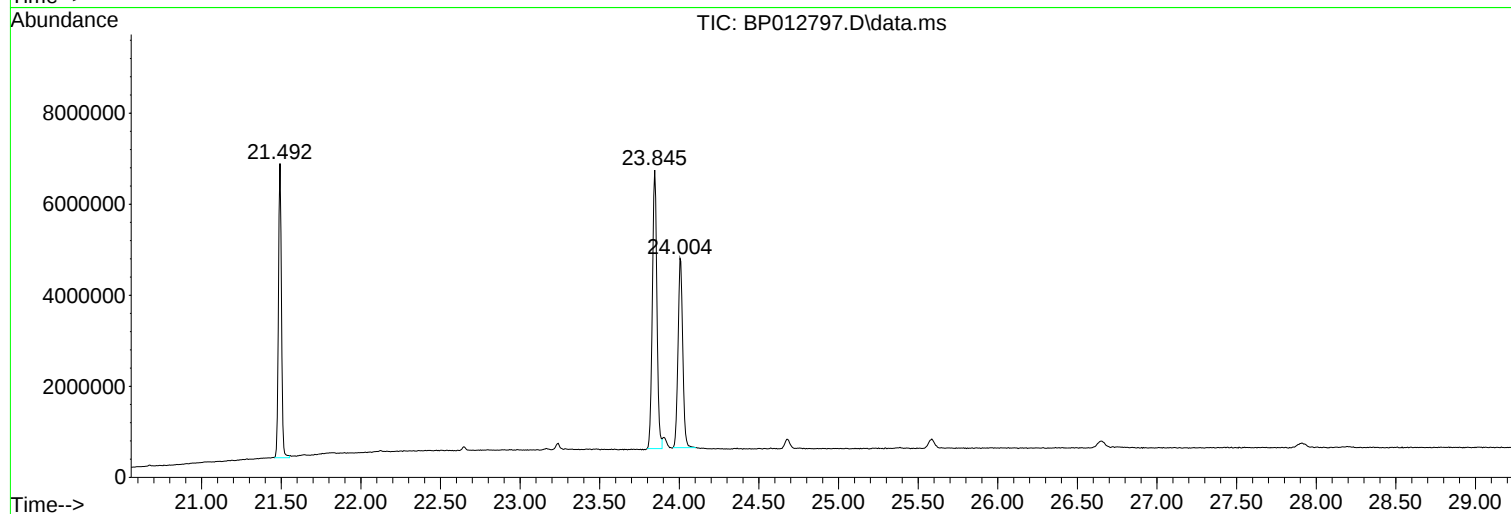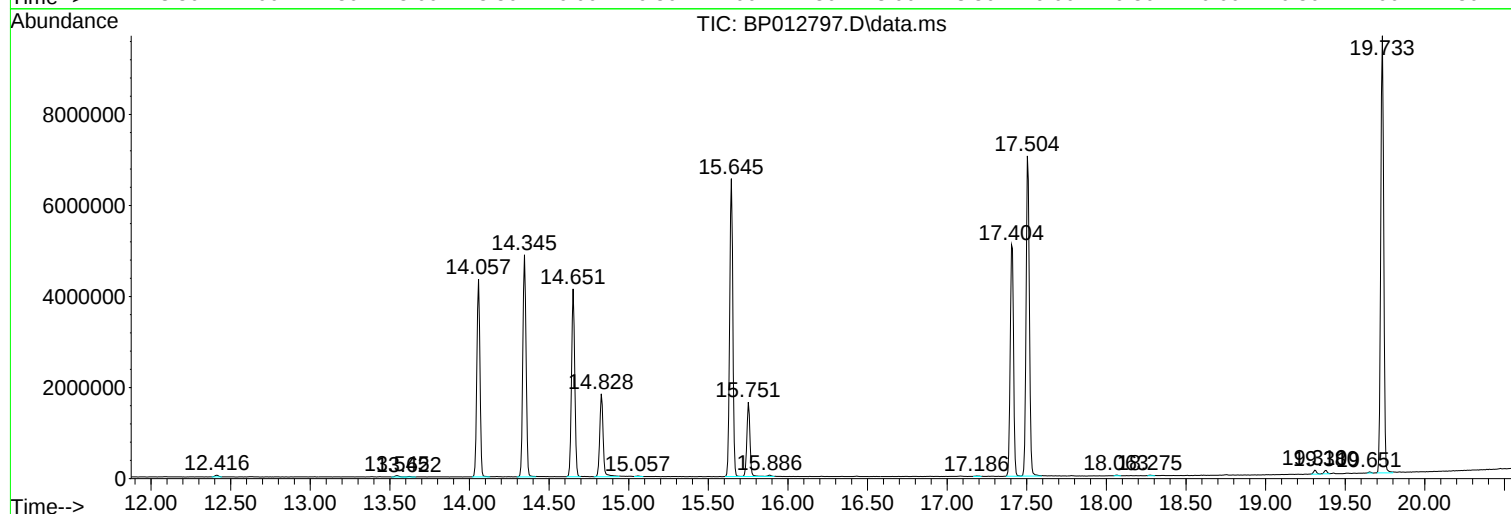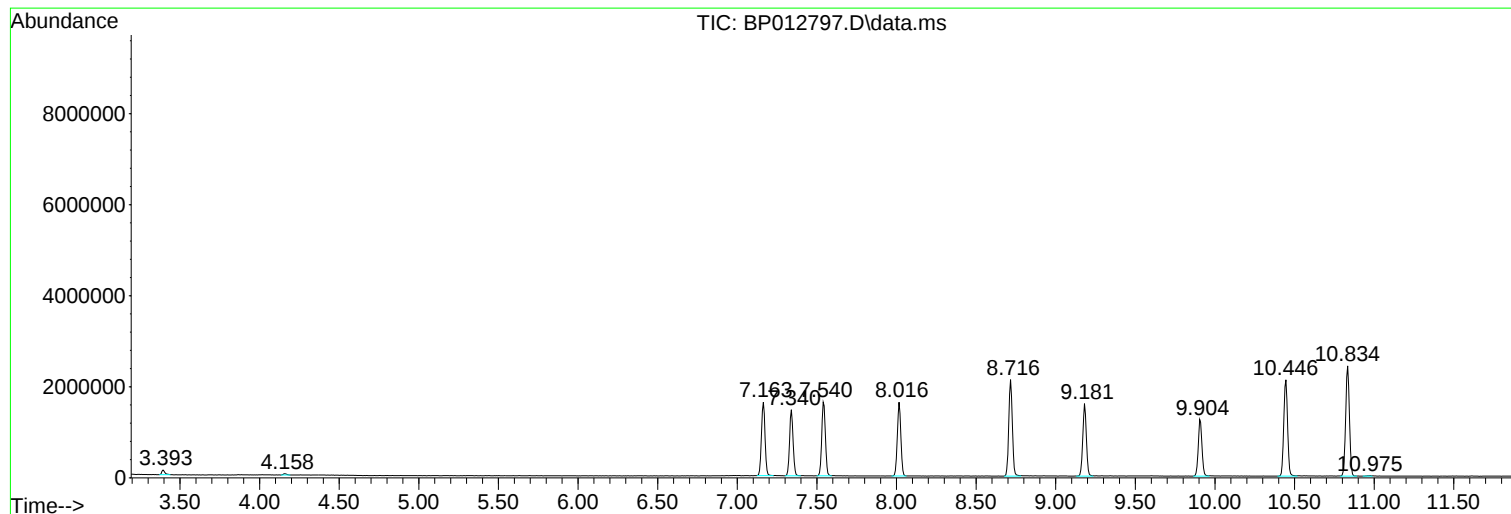

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012797.D
Acq On : 27 Nov 2022 08:55
Operator : CG/JU
Sample : PB149251BL
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK251

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012797.D
Acq On : 27 Nov 2022 08:55
Operator : CG/JU
Sample : PB149251BL
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK251

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc