

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012798.D
 Acq On : 27 Nov 2022 09:29
 Operator : CG/JU
 Sample : PB149206BL
 Misc :
 ALS Vial : 73 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK206

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012798.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.393	31	35	41	rBV	120483	159976	1.16%	0.122%
2	4.158	161	165	170	rBV	31946	43226	0.31%	0.033%
3	7.164	668	676	689	rBV	1873448	2924970	21.13%	2.224%
4	7.340	699	706	720	rVB	1668014	2591519	18.72%	1.970%
5	7.540	733	740	748	rBV	1873954	2960604	21.39%	2.251%
6	8.016	814	821	829	rVB	1818375	2805212	20.26%	2.132%
7	8.716	932	940	952	rBV	2449050	3809447	27.52%	2.896%
8	9.181	1010	1019	1030	rBV	1812776	2874935	20.77%	2.185%
9	9.905	1134	1142	1151	rBV	1425681	2327472	16.81%	1.769%
10	10.446	1224	1234	1247	rBV	2416803	3986130	28.79%	3.030%
11	10.834	1292	1300	1308	rBV	2696102	4474579	32.32%	3.402%
12	10.969	1317	1323	1329	rBV	7675	21182	0.15%	0.016%
13	12.410	1562	1568	1574	rBV	42990	76035	0.55%	0.058%
14	12.628	1599	1605	1610	rBV9	7497	14783	0.11%	0.011%
15	13.546	1756	1761	1764	rBV4	9980	15974	0.12%	0.012%
16	13.622	1771	1774	1782	rVB5	11666	19290	0.14%	0.015%
17	14.057	1841	1848	1861	rBV	5026975	6798019	49.10%	5.168%
18	14.346	1889	1897	1912	rBV	5428315	7937087	57.33%	6.034%
19	14.651	1942	1949	1958	rBV	4454880	6634818	47.93%	5.044%
20	14.828	1971	1979	1994	rBV	2097306	3006884	21.72%	2.286%
21	15.063	2014	2019	2024	rVB6	13397	21657	0.16%	0.016%
22	15.645	2111	2118	2129	rBV	7437676	10373518	74.93%	7.886%
23	15.751	2129	2136	2150	rVV	1836592	2492446	18.00%	1.895%
24	15.887	2153	2159	2166	rVB	33938	57189	0.41%	0.043%
25	17.081	2358	2362	2366	rBV7	11785	16482	0.12%	0.013%
26	17.192	2376	2381	2385	rBV3	12180	18247	0.13%	0.014%
27	17.410	2410	2418	2427	rBV	5638312	8218228	59.36%	6.247%
28	17.510	2428	2435	2455	rVB	8176361	11589021	83.71%	8.810%
29	18.063	2526	2529	2536	rVB9	13081	20013	0.14%	0.015%
30	18.275	2562	2565	2569	rBV6	15534	20400	0.15%	0.016%
31	19.310	2736	2741	2747	rBV	94836	145492	1.05%	0.111%
32	19.375	2748	2752	2758	rBV	84235	125634	0.91%	0.096%
33	19.733	2807	2813	2826	rBV	11231317	13844059	100.00%	10.524%
34	21.492	3106	3112	3125	rBV	6885033	9189165	66.38%	6.985%
35	23.845	3504	3512	3519	rBV2	6471913	13023856	94.08%	9.901%
36	24.010	3532	3540	3553	rVB2	4257496	8908970	64.35%	6.772%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012798.D
Acq On : 27 Nov 2022 09:29
Operator : CG/JU
Sample : PB149206BL
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK206

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Title : SVOA CALIBRATION




Sum of corrected areas: 131546519

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012798.D
Acq On : 27 Nov 2022 09:29
Operator : CG/JU
Sample : PB149206BL
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK206

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

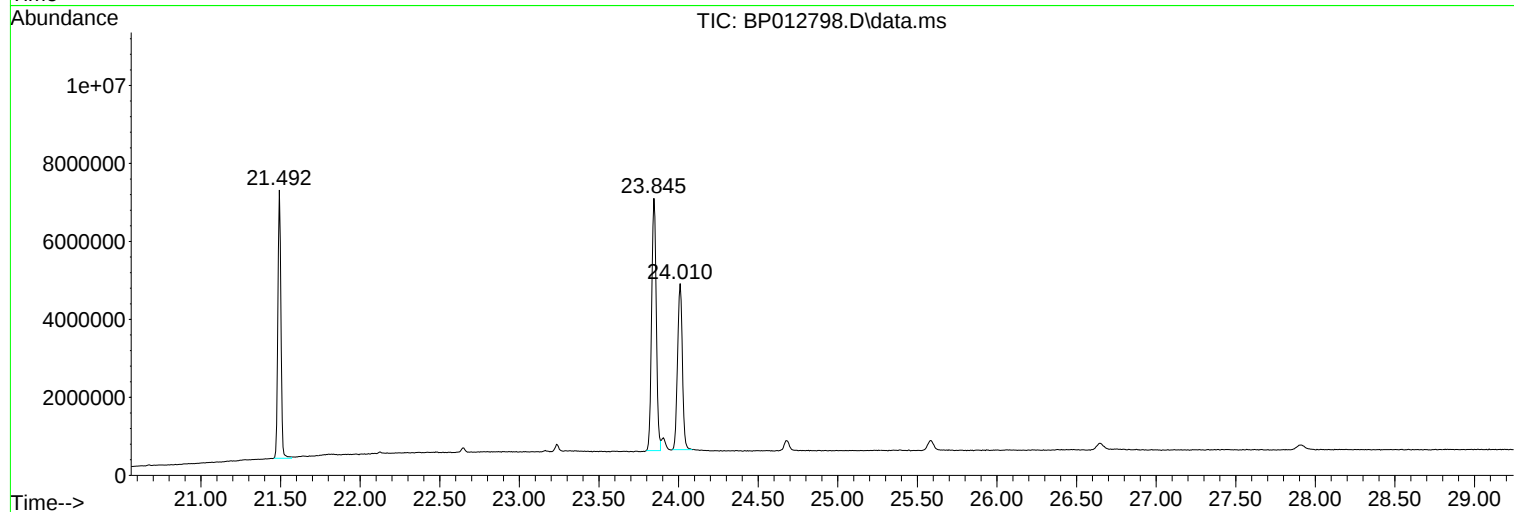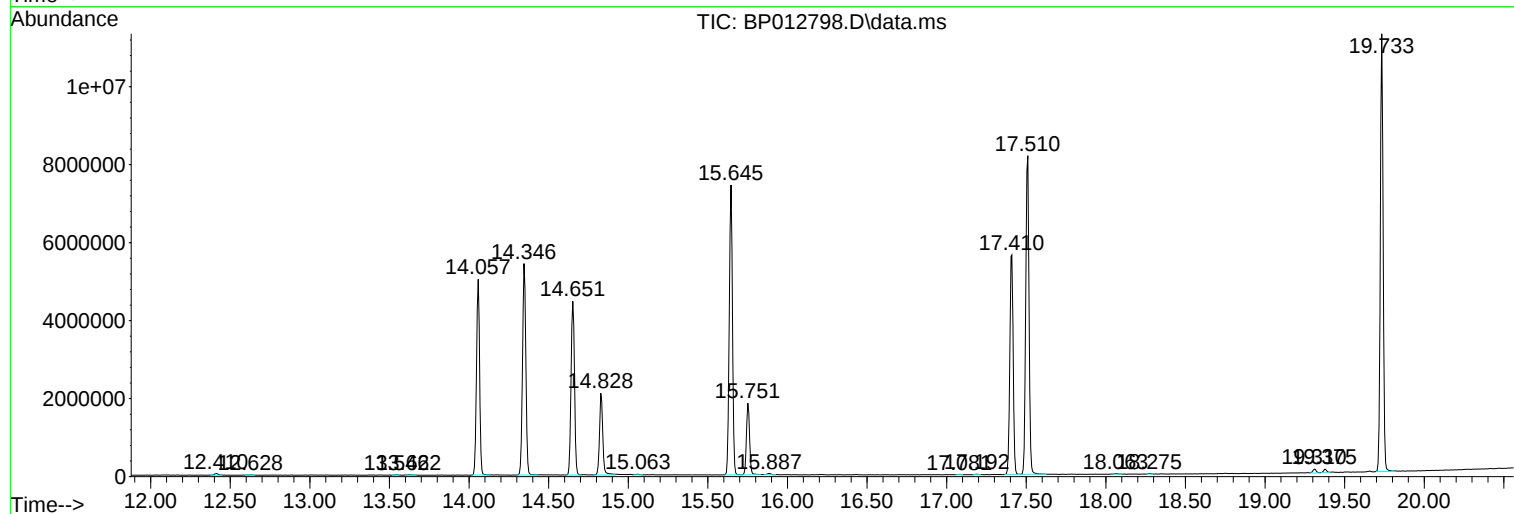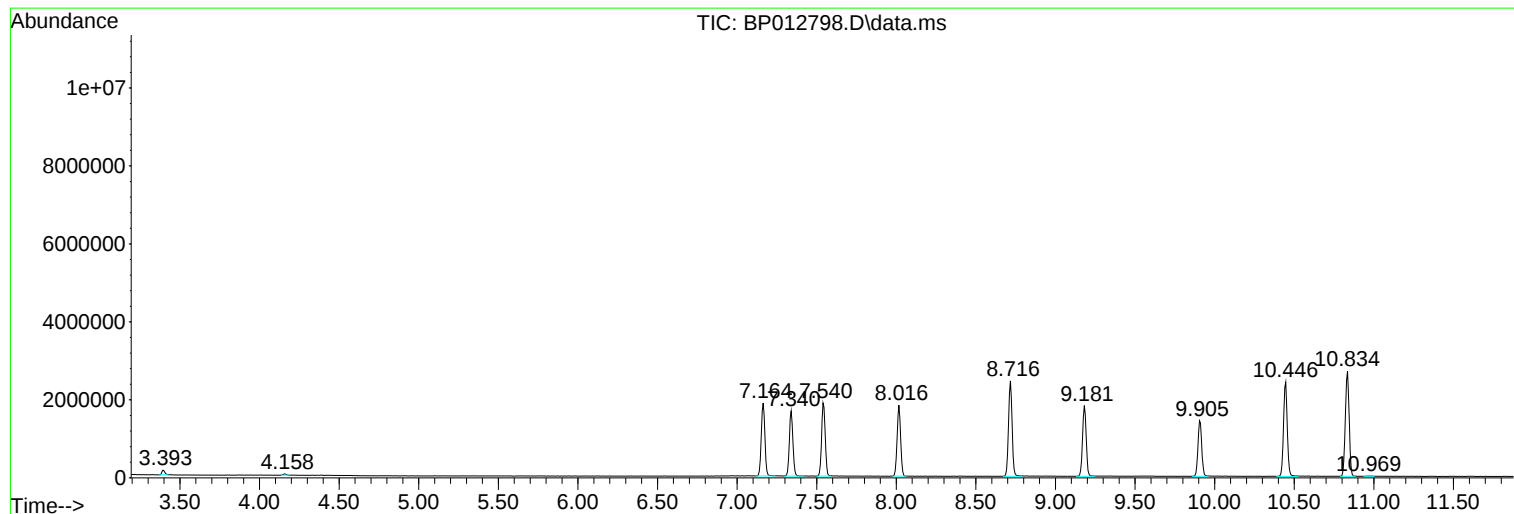

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012798.D
Acq On : 27 Nov 2022 09:29
Operator : CG/JU
Sample : PB149206BL
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK206

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012798.D
Acq On : 27 Nov 2022 09:29
Operator : CG/JU
Sample : PB149206BL
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK206

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc