

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012801.D
 Acq On : 27 Nov 2022 11:11
 Operator : CG/JU
 Sample : N5683-02
 Misc :
 ALS Vial : 76 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 ESQW0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012801.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.393	31	35	46	rVB	107880	156979	0.78%	0.099%
2	3.823	104	108	125	rBV	519756	874247	4.33%	0.549%
3	4.064	143	149	161	rVB	56744	104394	0.52%	0.066%
4	4.158	161	165	171	rBV	32021	49543	0.25%	0.031%
5	5.105	319	326	330	rBV5	12134	23864	0.12%	0.015%
6	7.164	669	676	686	rVB	458038	727740	3.60%	0.457%
7	7.340	697	706	714	rBV	1900593	2935282	14.53%	1.844%
8	7.540	733	740	750	rBV	1682518	2636522	13.05%	1.656%
9	8.016	813	821	828	rBV	1898033	2994294	14.82%	1.881%
10	8.716	930	940	952	rBV	1405604	2228311	11.03%	1.400%
11	9.181	1011	1019	1031	rBV	2103028	3343235	16.55%	2.100%
12	9.599	1086	1090	1096	rVB2	20566	32725	0.16%	0.021%
13	9.905	1132	1142	1154	rBV	1586084	2659665	13.16%	1.671%
14	10.234	1192	1198	1203	rVB7	11751	23346	0.12%	0.015%
15	10.446	1225	1234	1246	rBV	2504111	4248467	21.03%	2.669%
16	10.610	1257	1262	1267	rBV3	14274	26826	0.13%	0.017%
17	10.834	1289	1300	1313	rBV	2854853	4779620	23.66%	3.003%
18	10.963	1314	1322	1334	rBV	2216180	3694533	18.29%	2.321%
19	11.852	1468	1473	1478	rBV5	16993	28035	0.14%	0.018%
20	12.240	1537	1539	1547	rVB4	17544	23615	0.12%	0.015%
21	12.410	1564	1568	1573	rVB	50136	73395	0.36%	0.046%
22	12.487	1573	1581	1586	rVB	34226	60687	0.30%	0.038%
23	12.699	1611	1617	1622	rBV2	38824	73617	0.36%	0.046%
24	13.193	1696	1701	1707	rVB4	25980	40666	0.20%	0.026%
25	13.481	1738	1750	1755	rBV8	23437	67606	0.33%	0.042%
26	13.540	1756	1760	1764	rBV2	21556	32542	0.16%	0.020%
27	13.687	1781	1785	1793	rVB7	12753	29835	0.15%	0.019%
28	13.828	1799	1809	1818	rBV6	25057	74165	0.37%	0.047%
29	13.969	1823	1833	1838	rBV2	41911	80889	0.40%	0.051%
30	14.057	1838	1848	1857	rBV	5822943	7893571	39.07%	4.959%
31	14.128	1857	1860	1865	rVB2	37740	48792	0.24%	0.031%
32	14.346	1890	1897	1907	rBV	6581724	9344900	46.25%	5.871%
33	14.651	1938	1949	1956	rBV	4815961	6969717	34.50%	4.379%
34	14.828	1973	1979	1995	rBV	439981	712175	3.53%	0.447%
35	15.057	2012	2018	2025	rVB4	55963	107522	0.53%	0.068%
36	15.316	2058	2062	2066	rVB3	13971	21068	0.10%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012801.D
 Acq On : 27 Nov 2022 11:11
 Operator : CG/JU
 Sample : N5683-02
 Misc :
 ALS Vial : 76 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 ESQW0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

37	15.469	2085	2088	2095	rVB5	14767	23996	0.12%	0.015%
38	15.645	2111	2118	2130	rBV	8729529	12677442	62.75%	7.965%
39	15.751	2130	2136	2146	rBV	2736447	3574595	17.69%	2.246%
40	15.893	2154	2160	2167	rVB2	51704	136672	0.68%	0.086%
41	16.010	2174	2180	2185	rVB	218288	312680	1.55%	0.196%
42	16.381	2239	2243	2248	rVV2	49911	77284	0.38%	0.049%
43	16.422	2248	2250	2257	rVB8	14227	22522	0.11%	0.014%
44	17.216	2377	2385	2394	rVB3	36538	85146	0.42%	0.053%
45	17.404	2411	2417	2424	rBV	5940267	8577877	42.46%	5.389%
46	17.504	2428	2434	2446	rVV	10330246	15510613	76.77%	9.745%
47	17.592	2447	2449	2455	rVB7	26709	32965	0.16%	0.021%
48	18.275	2560	2565	2569	rBV2	203516	263054	1.30%	0.165%
49	19.310	2737	2741	2747	rVB	136238	184350	0.91%	0.116%
50	19.375	2748	2752	2758	rBV	151050	241095	1.19%	0.151%
51	19.504	2770	2774	2780	rBV	118653	152274	0.75%	0.096%
52	19.651	2797	2799	2803	rVB3	45024	46339	0.23%	0.029%
53	19.733	2807	2813	2825	rVV	14082896	19055527	94.32%	11.972%
54	21.186	3057	3060	3064	rBV2	148794	170489	0.84%	0.107%
55	21.492	3106	3112	3122	rBV	7615845	10175254	50.36%	6.393%
56	23.845	3504	3512	3520	rBV2	9839504	20203485	100.00%	12.693%
57	24.010	3532	3540	3555	rVB2	4972783	10424111	51.60%	6.549%




Sum of corrected areas: 159170160

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012801.D
Acq On : 27 Nov 2022 11:11
Operator : CG/JU
Sample : N5683-02
Misc :
ALS Vial : 76 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
ESQW0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

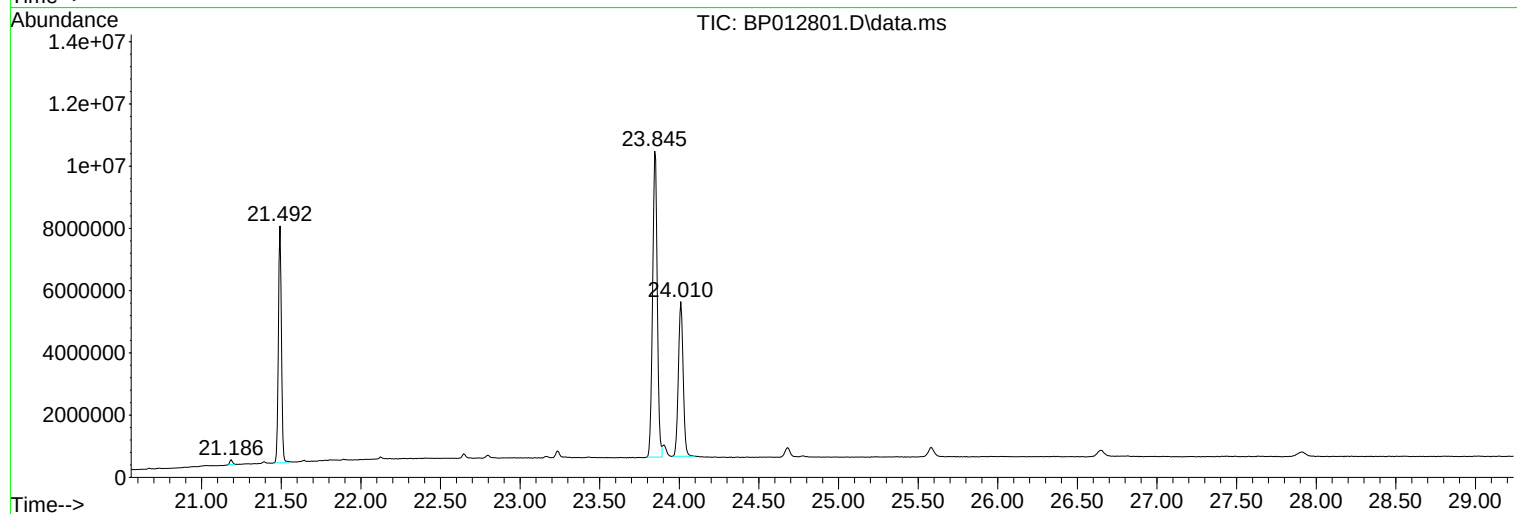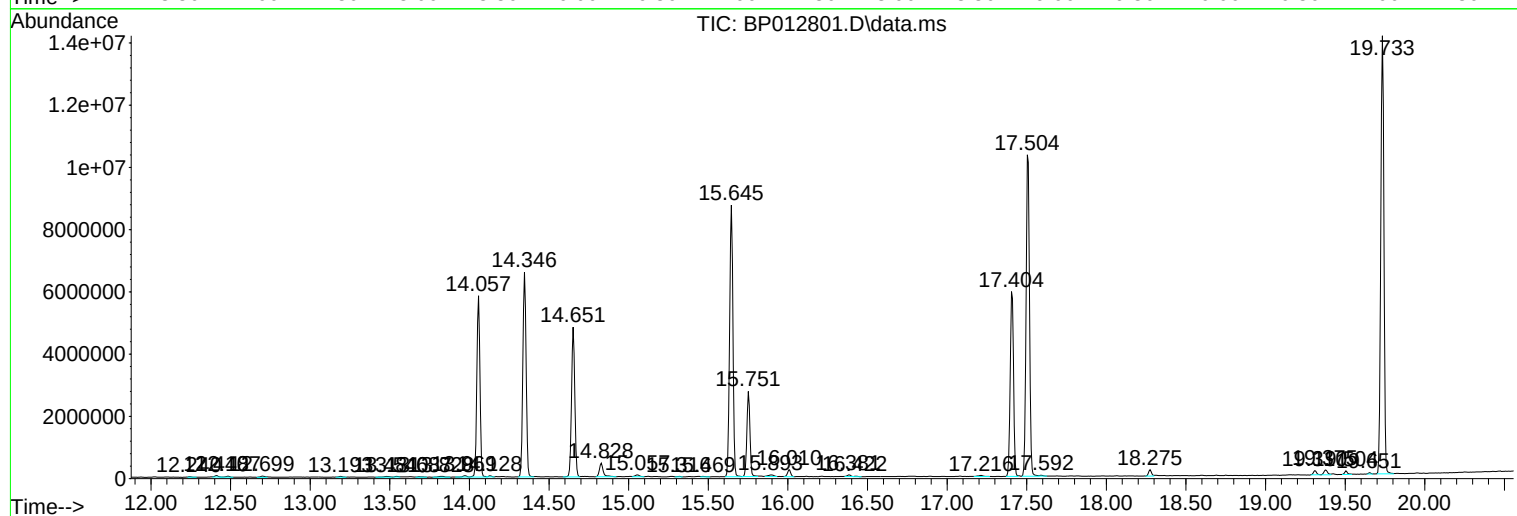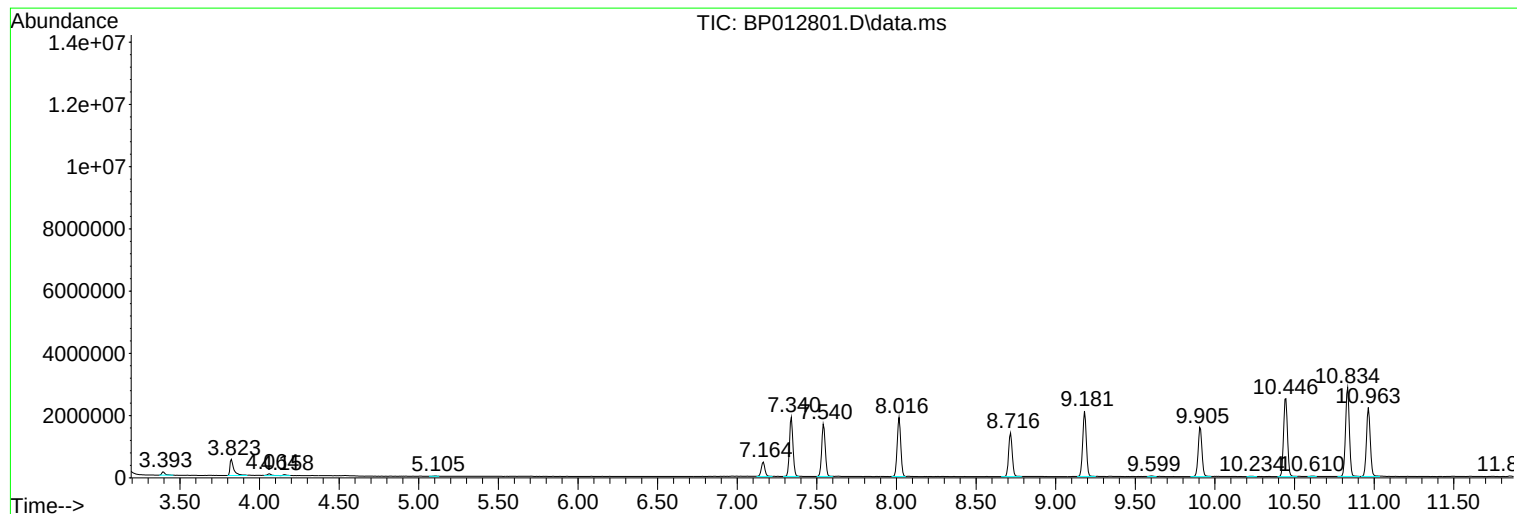

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012801.D
Acq On : 27 Nov 2022 11:11
Operator : CG/JU
Sample : N5683-02
Misc :
ALS Vial : 76 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
ESQW0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012801.D
Acq On : 27 Nov 2022 11:11
Operator : CG/JU
Sample : N5683-02
Misc :
ALS Vial : 76 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
ESQW0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
