

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012806.D
 Acq On : 27 Nov 2022 14:01
 Operator : CG/JU
 Sample : N5683-14
 Misc :
 ALS Vial : 81 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 ESQW7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012806.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.393	31	35	40	rBV	74242	101089	0.44%	0.057%
2	3.822	105	108	122	rBV	390703	631601	2.74%	0.359%
3	4.064	143	149	155	rBV	48672	83776	0.36%	0.048%
4	4.158	161	165	170	rVB	29761	40669	0.18%	0.023%
5	7.163	669	676	685	rBV	933540	1471473	6.39%	0.836%
6	7.340	699	706	715	rBV	2372061	3734881	16.22%	2.121%
7	7.540	733	740	751	rBV	2022331	3163328	13.74%	1.797%
8	8.016	812	821	829	rBV	1723330	2766233	12.02%	1.571%
9	8.716	931	940	954	rBV	1870434	3010388	13.08%	1.710%
10	9.181	1011	1019	1029	rBV	2769007	4455440	19.35%	2.531%
11	9.604	1086	1091	1096	rVB4	19260	32391	0.14%	0.018%
12	9.904	1135	1142	1151	rBV	1056180	1673814	7.27%	0.951%
13	10.446	1226	1234	1247	rBV	2862607	4843422	21.04%	2.751%
14	10.834	1291	1300	1313	rVB	2639969	4481250	19.47%	2.545%
15	10.963	1313	1322	1337	rBV	3243097	5466176	23.74%	3.105%
16	12.222	1530	1536	1542	rBV8	20673	39359	0.17%	0.022%
17	12.410	1561	1568	1576	rBV2	52389	88915	0.39%	0.051%
18	13.540	1754	1760	1768	rBV3	23490	40040	0.17%	0.023%
19	13.622	1770	1774	1782	rVB4	14336	23211	0.10%	0.013%
20	13.969	1827	1833	1840	rBV	95375	136634	0.59%	0.078%
21	14.057	1841	1848	1858	rBV	7579785	10183048	44.23%	5.784%
22	14.345	1890	1897	1915	rBV	8498296	12443592	54.05%	7.068%
23	14.651	1942	1949	1958	rBV	4663678	6654077	28.90%	3.780%
24	14.828	1973	1979	1995	rBV	456182	767452	3.33%	0.436%
25	15.063	2014	2019	2024	rVB6	34313	50047	0.22%	0.028%
26	15.645	2110	2118	2131	rBV	11157141	16067061	69.79%	9.126%
27	15.751	2131	2136	2141	rVV2	60479	92969	0.40%	0.053%
28	15.886	2151	2159	2167	rBV	65569	113079	0.49%	0.064%
29	16.428	2247	2251	2258	rBV5	22696	32202	0.14%	0.018%
30	17.192	2377	2381	2389	rVB6	13881	30196	0.13%	0.017%
31	17.404	2411	2417	2427	rBV	5896242	8430594	36.62%	4.789%
32	17.504	2427	2434	2445	rBV2	12114522	17967186	78.05%	10.205%
33	17.780	2476	2481	2485	rBV5	15652	36914	0.16%	0.021%
34	19.310	2736	2741	2746	rBV2	127174	186105	0.81%	0.106%
35	19.375	2748	2752	2757	rBV	117669	164989	0.72%	0.094%
36	19.622	2792	2794	2797	rBV	24882	26528	0.12%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012806.D
 Acq On : 27 Nov 2022 14:01
 Operator : CG/JU
 Sample : N5683-14
 Misc :
 ALS Vial : 81 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 ESQW7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

37	19.651	2797	2799	2805	rVB5	36321	46277	0.20%	0.026%
38	19.733	2807	2813	2827	rBV	15992947	22057184	95.81%	12.529%
39	21.492	3106	3112	3123	rBV	7481112	10051790	43.66%	5.709%
40	23.233	3404	3408	3413	rVB	227924	356475	1.55%	0.202%
41	23.851	3504	3513	3520	rBV2	10984377	23021234	100.00%	13.076%
42	24.010	3532	3540	3560	rVB2	4803236	10325616	44.85%	5.865%
43	24.674	3649	3653	3664	rVB2	335574	667178	2.90%	0.379%




Sum of corrected areas: 176055883

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012806.D
Acq On : 27 Nov 2022 14:01
Operator : CG/JU
Sample : N5683-14
Misc :
ALS Vial : 81 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
ESQW7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

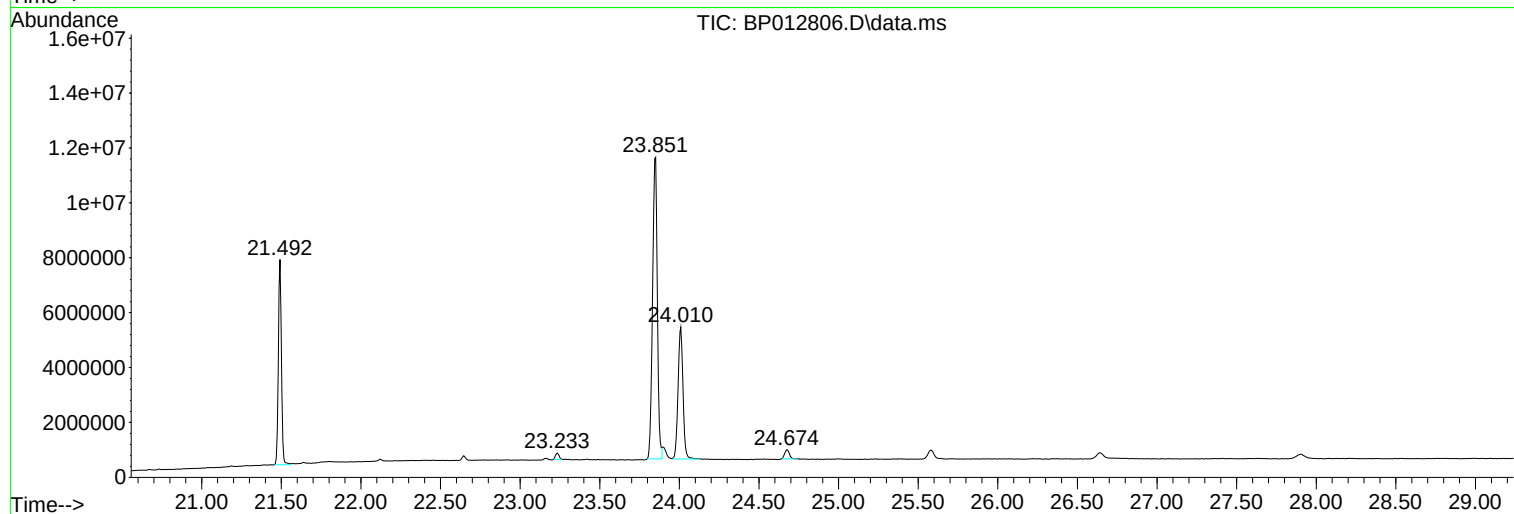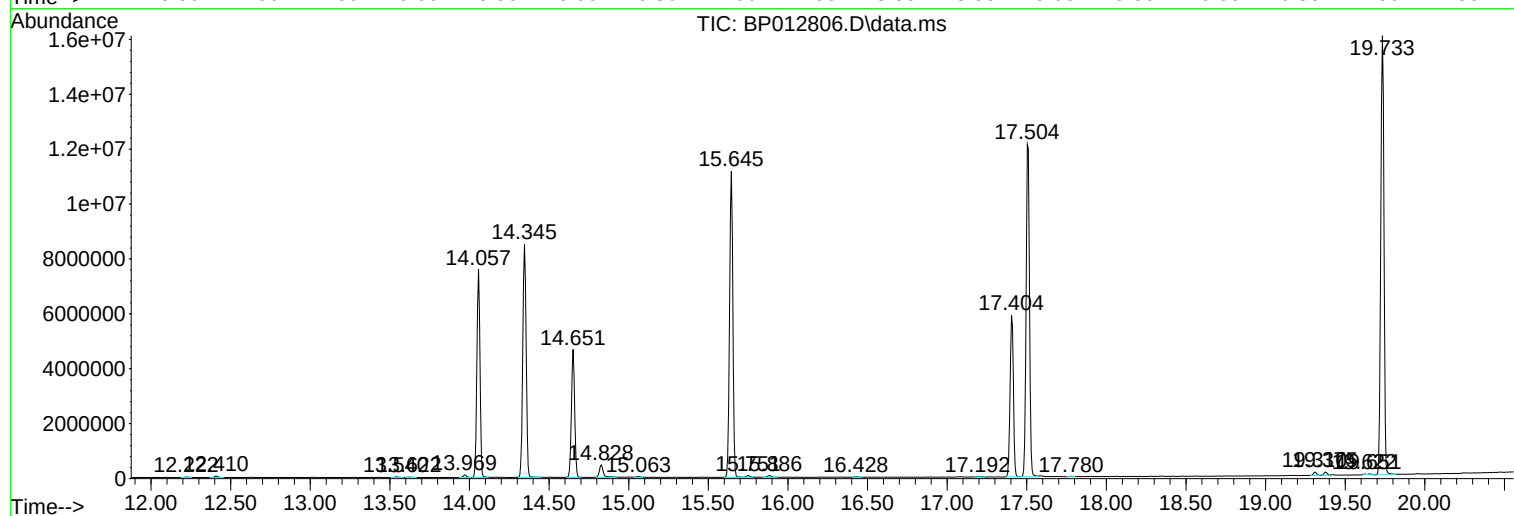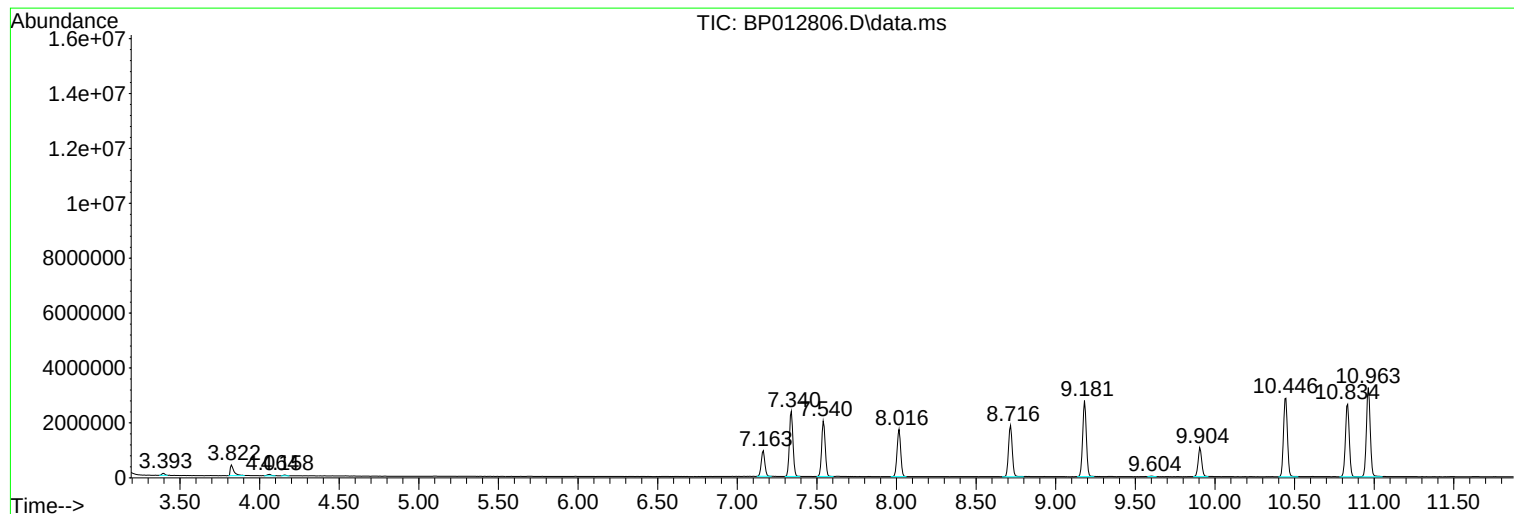

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012806.D
Acq On : 27 Nov 2022 14:01
Operator : CG/JU
Sample : N5683-14
Misc :
ALS Vial : 81 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
ESQW7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012806.D
Acq On : 27 Nov 2022 14:01
Operator : CG/JU
Sample : N5683-14
Misc :
ALS Vial : 81 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
ESQW7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
