

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112624\
 Data File : BP023320.D
 Acq On : 26 Nov 2024 11:34
 Operator : RC/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD020740

Quant Time: Nov 26 23:23:23 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 26 23:16:47 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.587	152	148	20.000	ng/ul	# 0.03
20) Naphthalene-d8	10.334	136	341	20.000	ng/ul	# 0.03
38) Acenaphthene-d10	14.140	164	247134	20.000	ng/ul	-0.03
64) Phenanthrene-d10	16.957	188	624538	20.000	ng/ul	-0.02
79) Chrysene-d12	21.421	240	723584	20.000	ng/ul	0.02
88) Perylene-d12	24.633	264	819942	20.000	ng/ul	0.04
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.099	96	16776	5448.505	ng/uL	-0.04
4) Pyridine-d5	3.505	84	108694	11881.886	ng/ul	-0.04
7) Phenol-d5	6.705	99	117212	10712.089	ng/ul	-0.06
9) Bis-(2-Chloroethyl)eth...	6.928	67	491	76.377	ng/ul	0.02
11) 2-Chlorophenol-d4	7.052	132	84070	10490.792	ng/ul	-0.05
15) 4-Methylphenol-d8	8.299	113	13155	1460.962	ng/ul	0.03
21) Nitrobenzene-d5	8.646	128	42616	17951.492	ng/ul	-0.06
24) 2-Nitrophenol-d4	9.363	143	49282	17413.078	ng/ul	-0.05
28) 2,4-Dichlorophenol-d3	10.028	165	300	50.617	ng/ul	0.07
31) 4-Chloroaniline-d4	10.410	131	122068	17263.661	ng/ul	-0.04
46) Dimethylphthalate-d6	13.557	166	369650	20.753	ng/ul	-0.01
49) Acenaphthylene-d8	13.834	160	386647	20.804	ng/ul	-0.02
54) 4-Nitrophenol-d4	14.416	143	37340	13.950	ng/ul	-0.02
60) Fluorene-d10	15.157	176	325280	20.829	ng/ul	-0.03
65) 4,6-Dinitro-2-methylph...	15.328	200	70846	18.936	ng/ul	0.00
73) Anthracene-d10	17.075	188	550360	20.813	ng/ul	0.00
81) Pyrene-d10	19.475	212	713083	21.395	ng/ul	0.01
92) Benzo(a)pyrene-d12	24.404	264	827577	21.189	ng/ul	0.03
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.187	88	209	58.746	ng/uL	87
5) Pyridine	3.522	79	111730	12161.686	ng/ul	97
6) Benzaldehyde	6.675	77	87801	13943.911	ng/ul	99
8) Phenol	6.728	94	120982	10588.081	ng/ul	97
10) Bis(2-Chloroethyl)ether	6.946	93	98093	11424.367	ng/ul	95
12) 2-Chlorophenol	7.081	128	87382	10502.633	ng/ul	97
13) 2-Methylphenol	7.957	108	88461	10371.537	ng/ul	97
14) 2,2'-oxybis(1-Chloropr...	8.010	45	121690	12519.514	ng/ul	97
16) Acetophenone	8.322	105	163030	10774.677	ng/ul	98
17) N-Nitroso-di-n-propyla...	8.393	70	94	12.442	ng/ul#	85
18) 4-Methylphenol	8.287	108	98591	10465.294	ng/ul	94
19) Hexachloroethane	8.546	117	42922	10666.975	ng/ul	93
22) Nitrobenzene	8.687	77	131189	19259.165	ng/ul	99
23) Isophorone	9.204	82	245290	20138.674	ng/ul	99
25) 2-Nitrophenol	9.399	139	54633	18288.870	ng/ul	94
26) 2,4-Dimethylphenol	9.463	107	122946	19059.663	ng/ul	98
27) Bis(2-Chloroethoxy)met...	9.681	93	135546	20225.519	ng/ul	98
29) 2,4-Dichlorophenol	9.934	162	98169	16721.925	ng/ul	97
30) Naphthalene	10.304	128	305518	18441.934	ng/ul	99
32) 4-Chloroaniline	10.440	127	116222	16965.714	ng/ul	98
33) Hexachlorobutadiene	10.581	225	89304	16811.817	ng/ul	98
34) Caprolactam	11.234	113	30906	17699.175	ng/ul	99
35) 4-Chloro-3-methylphenol	11.587	107	119060	18851.745	ng/ul	92
36) 2-Methylnaphthalene	11.928	142	228145	18241.385	ng/ul	99

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112624\
 Data File : BP023320.D
 Acq On : 26 Nov 2024 11:34
 Operator : RC/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1


Instrument :
 BNA_P
 ClientSampleId :
 SSTD020740


Quant Time: Nov 26 23:23:23 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 26 23:16:47 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.151	142	236097	18465.810	ng/ul	96
39) 1,2,4,5-Tetrachloroben...	12.298	216	163077	19.546	ng/ul	97
40) Hexachlorocyclopentadiene	12.263	237	68778	15.695	ng/ul	98
41) 2,4,6-Trichlorophenol	12.569	196	101773	20.032	ng/ul	98
42) 2,4,5-Trichlorophenol	12.657	196	110774	20.225	ng/ul	99
43) 1,1'-Biphenyl	12.957	154	331426	20.929	ng/ul	99
44) 2-Chloronaphthalene	12.998	162	269038	20.783	ng/ul	98
45) 2-Nitroaniline	13.240	65	81084	22.308	ng/ul	97
47) Dimethylphthalate	13.610	163	369987	21.063	ng/ul	99
48) 2,6-Dinitrotoluene	13.734	165	70683	20.686	ng/ul	91
50) Acenaphthylene	13.863	152	398215	21.197	ng/ul	99
51) 3-Nitroaniline	14.081	138	62006	21.069	ng/ul	95
52) Acenaphthene	14.210	153	288895	21.181	ng/ul	97
53) 2,4-Dinitrophenol	14.334	184	39029	16.098	ng/ul	95
55) 4-Nitrophenol	14.434	109	43717	13.959	ng/ul	96
56) Dibenzofuran	14.557	168	430901	20.448	ng/ul	100
57) 2,4-Dinitrotoluene	14.563	165	114472	21.020	ng/ul	94
58) 2,3,4,6-Tetrachlorophenol	14.798	232	108269	20.223	ng/ul	96
59) Diethylphthalate	15.004	149	362244	20.851	ng/ul	100
61) Fluorene	15.216	166	350060	20.296	ng/ul	100
62) 4-Chlorophenyl-phenyle...	15.216	204	200315	19.725	ng/ul	98
63) 4-Nitroaniline	15.292	138	58412	21.330	ng/ul	95
66) 4,6-Dinitro-2-methylph...	15.345	198	76763	19.207	ng/ul#	89
67) N-Nitrosodiphenylamine	15.445	169	308203	21.356	ng/ul	99
68) 4-Bromophenyl-phenylether	16.139	248	139412	19.713	ng/ul	97
69) Hexachlorobenzene	16.251	284	171973	19.316	ng/ul	95
70) Atrazine	16.433	200	140184	20.095	ng/ul	98
71) Pentachlorophenol	16.622	266	96111	17.388	ng/ul	94
72) Phenanthrene	17.010	178	616206	20.897	ng/ul	100
74) Anthracene	17.110	178	625975	21.114	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	12.928	216	162323	19.685	ng/uL	98
76) Pentachlorobenzene	14.475	250	186895	19.850	ng/uL	99
77) Carbazole	17.404	167	529273	20.462	ng/ul	98
78) Di-n-butylphthalate	17.975	149	639765	22.289	ng/ul	99
80) Fluoranthene	19.122	202	823312	21.442	ng/ul	100
82) Pyrene	19.504	202	881847	21.379	ng/ul	99
83) Butylbenzylphthalate	20.457	149	300358	22.117	ng/ul	95
84) 3,3'-Dichlorobenzidine	21.333	252	327546	20.166	ng/ul	100
85) Benzo(a)anthracene	21.404	228	936843	21.204	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.333	149	434090	22.493	ng/ul#	98
87) Chrysene	21.469	228	870287	20.934	ng/ul	100
89) Di-n-octyl phthalate	22.545	149	749896	22.543	ng/ul	100
90) Benzo(b)fluoranthene	23.615	252	978227	21.435	ng/ul	99
91) Benzo(k)fluoranthene	23.686	252	983349	21.888	ng/ul	99
93) Benzo(a)pyrene	24.480	252	873768	21.179	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	28.245	276	450337	7.835	ng/ul	98
95) Dibenzo(a,h)anthracene	28.309	278	880595	18.869	ng/ul	98
96) Benzo(g,h,i)perylene	29.368	276	807515	18.496	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Nov 26 23:23:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 26 23:16:47 2024
Response via : Initial Calibration







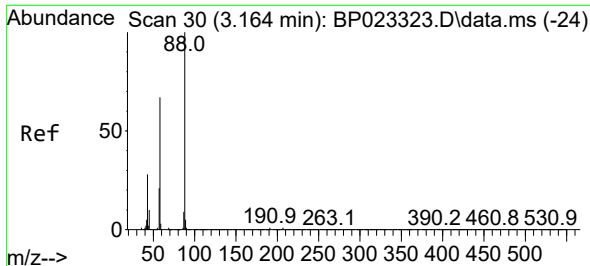

#2
1,4-Dioxane
Concen: 58.746 ng/uL
RT: 3.187 min Scan# 34
Delta R.T. 0.024 min
Lab File: BP023320.D
Acq: 26 Nov 2024 11:34




Instrument :
BNA_P
ClientSampleId :
SSTD020740


Tgt Ion: 88 Resp: 209
Ion Ratio Lower Upper
88 100
43 23.3 22.9 34.3
58 55.0 53.1 79.7

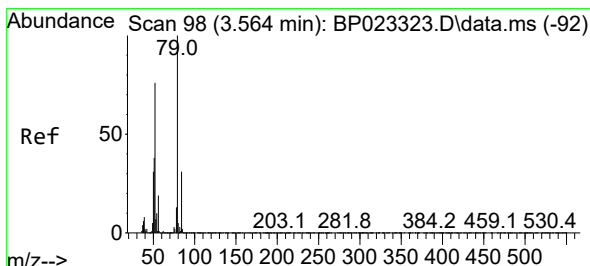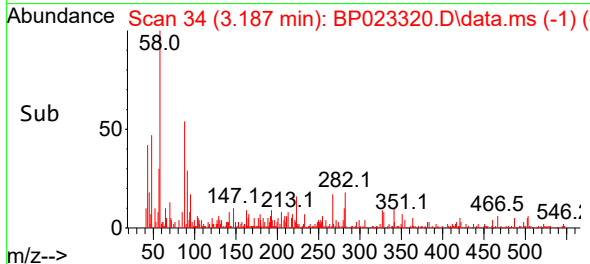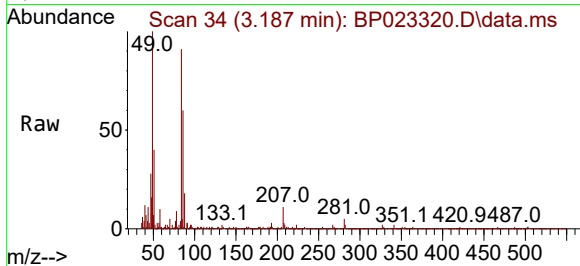

#5
Pyridine
Concen: 12161.686 ng/uL
RT: 3.522 min Scan# 91
Delta R.T. -0.041 min
Lab File: BP023320.D
Acq: 26 Nov 2024 11:34

Tgt Ion: 79 Resp: 111730
Ion Ratio Lower Upper
79 100
52 72.4 60.8 91.2
51 37.2 30.7 46.1


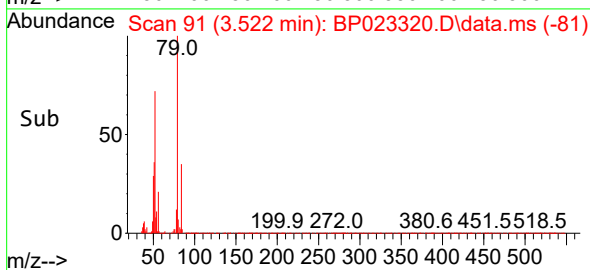

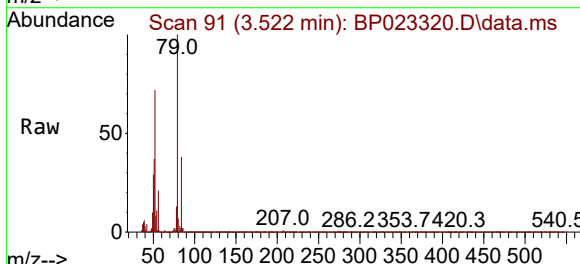




#6
Benzaldehyde
Concen: 13943.911 ng/ul
RT: 6.675 min Scan# 61
Delta R.T. -0.059 min
Lab File: BP023320.D
Acq: 26 Nov 2024 11:34




Instrument :
BNA_P
ClientSampleId :
SSTD020740


Tgt Ion: 77 Resp: 87801
Ion Ratio Lower Upper
77 100
105 87.1 70.6 106.0
106 83.7 67.4 101.0



#8
Phenol
Concen: 10588.081 ng/ul
RT: 6.728 min Scan# 636
Delta R.T. -0.065 min
Lab File: BP023320.D
Acq: 26 Nov 2024 11:34

Tgt Ion: 94 Resp: 120982
Ion Ratio Lower Upper
94 100
65 34.2 28.0 42.0
66 49.6 42.0 63.0



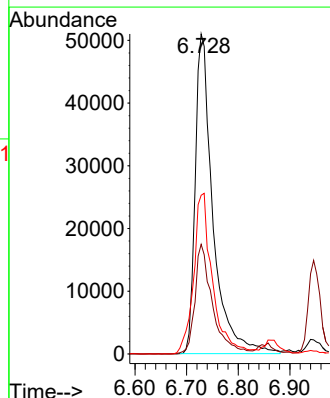





#10
Bis(2-Chloroethyl)ether
Concen: 11424.367 ng/ul
RT: 6.946 min Scan# 61
Delta R.T. -0.053 min
Lab File: BP023320.D
Acq: 26 Nov 2024 11:34




Instrument :
BNA_P
ClientSampleId :
SSTD020740


Tgt Ion: 93 Resp: 98093
Ion Ratio Lower Upper
93 100
63 81.0 61.3 91.9
95 34.0 25.4 38.0



#12
2-Chlorophenol
Concen: 10502.633 ng/ul
RT: 7.081 min Scan# 696
Delta R.T. -0.059 min
Lab File: BP023320.D
Acq: 26 Nov 2024 11:34

Tgt Ion: 128 Resp: 87382
Ion Ratio Lower Upper
128 100
64 54.1 44.8 67.2
130 33.2 24.7 37.1





#13

2-Methylphenol

Concen: 10371.537 ng/ul

RT: 7.957 min Scan# 84

Delta R.T. -0.053 min

Lab File: BP023320.D


Acq: 26 Nov 2024 11:34

Instrument :

BNA_P

ClientSampleId :

SSTD020740






Tgt Ion:108 Resp: 88461

Ion Ratio Lower Upper

108 100

107 94.8 73.8 110.8



#14

2,2'-oxybis(1-Chloropropane)

Concen: 12519.514 ng/ul

RT: 8.010 min Scan# 854

Delta R.T. -0.059 min

Lab File: BP023320.D

Acq: 26 Nov 2024 11:34




Tgt Ion: 45 Resp: 121690


Ion Ratio Lower Upper

45 100

77 18.8 13.9 20.9

79 13.3 11.3 16.9



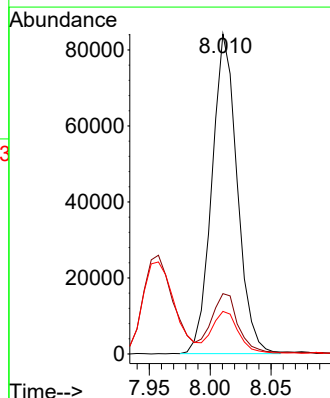





#16
Acetophenone
Concen: 10774.677 ng/ul
RT: 8.322 min Scan# 907
Delta R.T. -0.053 min
Lab File: BP023320.D
Acq: 26 Nov 2024 11:34




Instrument :
BNA_P
ClientSampleId :
SSTD020740


Tgt Ion:105 Resp: 163030
Ion Ratio Lower Upper
105 100
77 86.7 71.2 106.8
51 28.7 22.9 34.3



#17
N-Nitroso-di-n-propylamine
Concen: 12.442 ng/ul
RT: 8.393 min Scan# 919
Delta R.T. 0.041 min
Lab File: BP023320.D
Acq: 26 Nov 2024 11:34

Tgt Ion: 70 Resp: 94
Ion Ratio Lower Upper
70 100
42 64.2 43.5 65.3
101 0.3 6.8 10.2#
130 10.2 14.0 21.0#









#18
4-Methylphenol
Concen: 10465.294 ng/ul
RT: 8.287 min Scan# 901
Delta R.T. -0.047 min
Lab File: BP023320.D
Acq: 26 Nov 2024 11:34




Instrument :
BNA_P
ClientSampleId :
SSTD020740


Tgt Ion:108 Resp: 98591
Ion Ratio Lower Upper
108 100
107 112.6 95.1 142.7



#19
Hexachloroethane
Concen: 10666.975 ng/ul
RT: 8.546 min Scan# 945
Delta R.T. -0.053 min
Lab File: BP023320.D
Acq: 26 Nov 2024 11:34

Tgt Ion:117 Resp: 42922
Ion Ratio Lower Upper
117 100
201 127.5 107.0 160.6
199 85.5 62.1 93.1









#22
Nitrobenzene
Concen: 19259.165 ng/ul
RT: 8.687 min Scan# 90
Delta R.T. -0.059 min
Lab File: BP023320.D
Acq: 26 Nov 2024 11:34




Instrument :
BNA_P
ClientSampleId :
SSTD020740


Tgt Ion: 77 Resp: 131189
Ion Ratio Lower Upper
77 100
123 37.9 29.8 44.6
65 12.9 11.0 16.6



#23
Isophorone
Concen: 20138.674 ng/ul
RT: 9.204 min Scan# 1057
Delta R.T. -0.053 min
Lab File: BP023320.D
Acq: 26 Nov 2024 11:34

Tgt Ion: 82 Resp: 245290
Ion Ratio Lower Upper
82 100
95 8.1 7.0 10.4
138 15.5 12.0 18.0









#25
2-Nitrophenol
Concen: 18288.870 ng/ul
RT: 9.399 min Scan# 1100
Delta R.T. -0.047 min
Lab File: BP023320.D
Acq: 26 Nov 2024 11:34




Instrument :
BNA_P
ClientSampleId :
SSTD020740


Tgt Ion:139 Resp: 54633
Ion Ratio Lower Upper
139 100
65 64.2 55.1 82.7
109 44.1 39.1 58.7

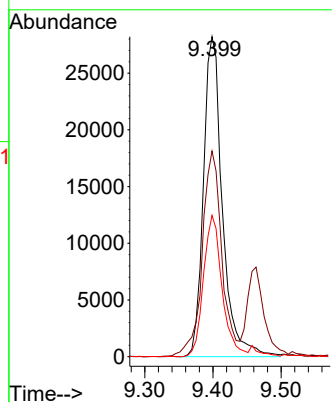

#26
2,4-Dimethylphenol
Concen: 19059.663 ng/ul
RT: 9.463 min Scan# 1101
Delta R.T. -0.047 min
Lab File: BP023320.D
Acq: 26 Nov 2024 11:34

Tgt Ion:107 Resp: 122946
Ion Ratio Lower Upper
107 100
121 42.8 36.6 55.0
122 73.2 58.6 87.8

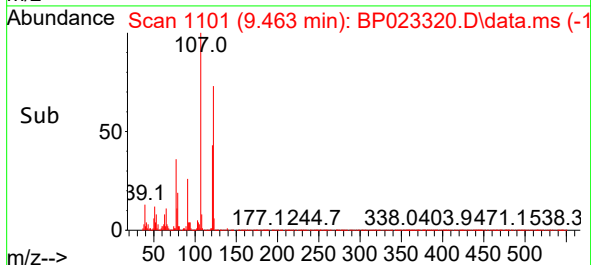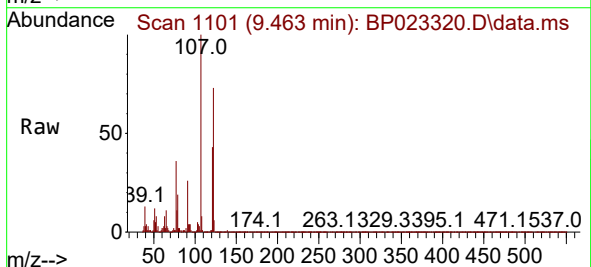



#27

Bis(2-Chloroethoxy)methane

Concen: 20225.519 ng/ul

RT: 9.681 min Scan# 1138

Delta R.T. -0.041 min

Lab File: BP023320.D

Acq: 26 Nov 2024 11:34

Instrument :

BNA_P

ClientSampleId :

SSTD020740





Tgt Ion: 93 Resp: 135546

Ion Ratio Lower Upper

93 100

95 30.4 25.0 37.4

123 10.7 7.8 11.6

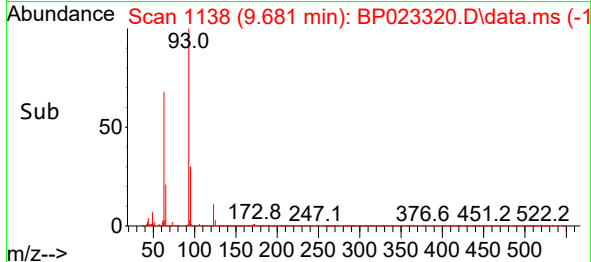

#29

2,4-Dichlorophenol

Concen: 16721.925 ng/ul

RT: 9.934 min Scan# 1181

Delta R.T. -0.047 min

Lab File: BP023320.D

Acq: 26 Nov 2024 11:34




Tgt Ion:162 Resp: 98169


Ion Ratio Lower Upper

162 100

164 68.3 53.0 79.6

98 39.7 30.3 45.5


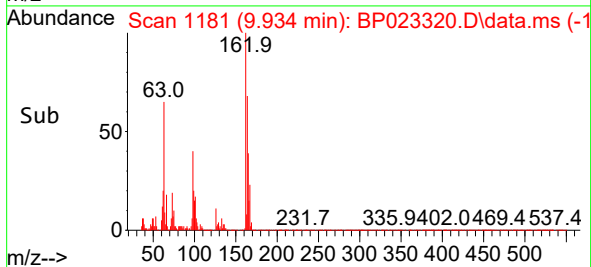

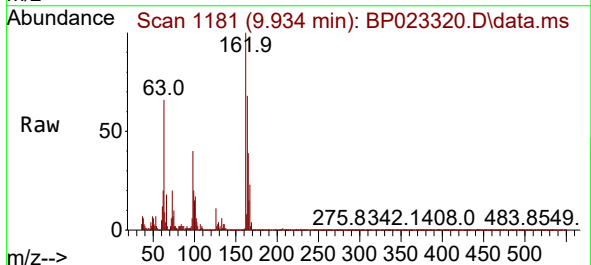




#30
Naphthalene
Concen: 18441.934 ng/ul
RT: 10.304 min Scan# 1244
Delta R.T. -0.047 min
Lab File: BP023320.D
Acq: 26 Nov 2024 11:34




Instrument :
BNA_P
ClientSampleId :
SSTD020740


Tgt Ion:128 Resp: 305518
Ion Ratio Lower Upper
128 100
129 11.1 8.5 12.7
127 13.4 10.5 15.7

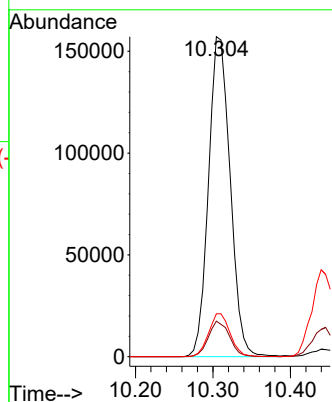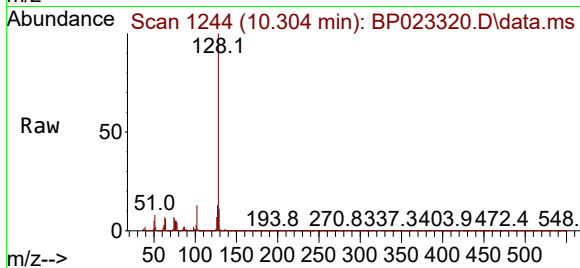

#32
4-Chloroaniline
Concen: 16965.714 ng/ul
RT: 10.440 min Scan# 1267
Delta R.T. -0.041 min
Lab File: BP023320.D
Acq: 26 Nov 2024 11:34

Tgt Ion:127 Resp: 116222
Ion Ratio Lower Upper
127 100
129 31.3 25.9 38.9









#33
Hexachlorobutadiene
Concen: 16811.817 ng/ul
RT: 10.581 min Scan# 11
Delta R.T. -0.041 min
Lab File: BP023320.D
Acq: 26 Nov 2024 11:34




Instrument :
BNA_P
ClientSampleId :
SSTD020740


Tgt Ion:225 Resp: 89304
Ion Ratio Lower Upper
225 100
223 61.6 51.4 77.2
227 66.5 53.0 79.4

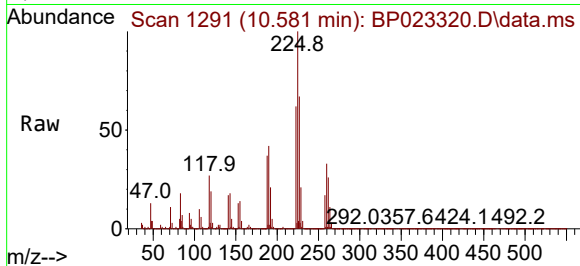

#34
Caprolactam
Concen: 17699.175 ng/ul
RT: 11.234 min Scan# 1402
Delta R.T. -0.041 min
Lab File: BP023320.D
Acq: 26 Nov 2024 11:34

Tgt Ion:113 Resp: 30906
Ion Ratio Lower Upper
113 100
55 162.5 127.5 191.3
56 126.0 100.7 151.1




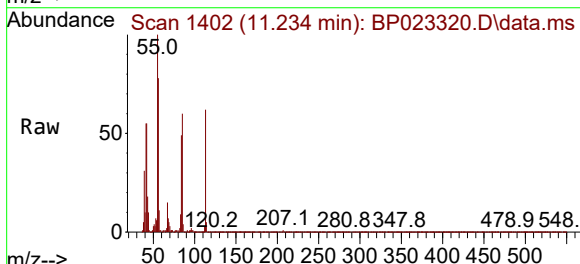




#35
4-Chloro-3-methylphenol
Concen: 18851.745 ng/ul
RT: 11.587 min Scan# 1468
Delta R.T. -0.035 min
Lab File: BP023320.D
Acq: 26 Nov 2024 11:34




Instrument :
BNA_P
ClientSampleId :
SSTD020740


Tgt Ion:107 Resp: 119060
Ion Ratio Lower Upper
107 100
144 24.0 17.9 26.9
142 73.6 53.0 79.4

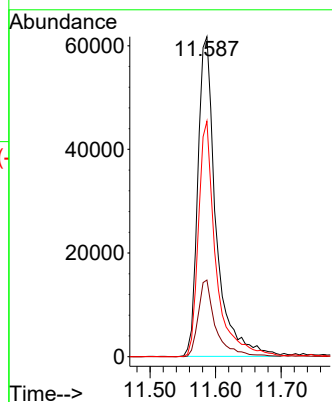

#36
2-Methylnaphthalene
Concen: 18241.385 ng/ul
RT: 11.928 min Scan# 1520
Delta R.T. -0.041 min
Lab File: BP023320.D
Acq: 26 Nov 2024 11:34

Tgt Ion:142 Resp: 228145
Ion Ratio Lower Upper
142 100
141 87.0 69.0 103.6





#37

1-Methylnaphthalene

Concen: 18465.810 ng/ul

RT: 12.151 min Scan# 1558

Delta R.T. -0.029 min

Lab File: BP023320.D

Acq: 26 Nov 2024 11:34

Instrument :

BNA_P

ClientSampleId :

SSTD020740





Tgt Ion:142 Resp: 236097

Ion Ratio Lower Upper

142 100

141 92.4 71.1 106.7

116 5.1 4.0 6.0

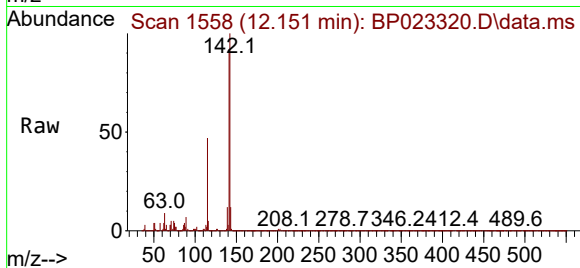

#39

1,2,4,5-Tetrachlorobenzene

Concen: 19.546 ng/ul

RT: 12.298 min Scan# 1583

Delta R.T. -0.047 min

Lab File: BP023320.D

Acq: 26 Nov 2024 11:34

Tgt Ion:216 Resp: 163077




Ion Ratio Lower Upper


216 100

214 77.3 64.4 96.6

179 21.4 16.4 24.6

108 15.8 13.2 19.8

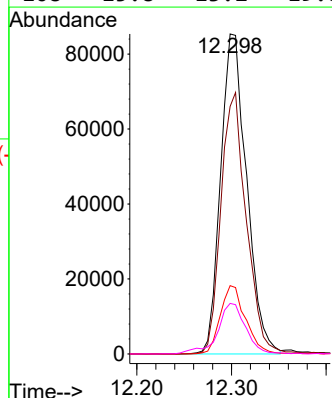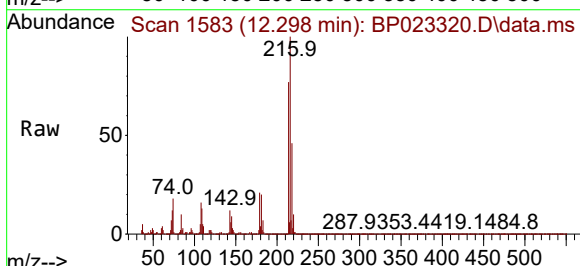



#40

Hexachlorocyclopentadiene

Concen: 15.695 ng/ul

RT: 12.263 min Scan# 1

Delta R.T. -0.041 min

Lab File: BP023320.D

Acq: 26 Nov 2024 11:34

Instrument :

BNA_P

ClientSampleId :

SSTD020740





Tgt Ion:237 Resp: 68778

Ion Ratio Lower Upper

237 100

235 64.8 50.5 75.7

272 12.6 9.5 14.3



#41

2,4,6-Trichlorophenol

Concen: 20.032 ng/ul

RT: 12.569 min Scan# 1629

Delta R.T. -0.029 min

Lab File: BP023320.D

Acq: 26 Nov 2024 11:34




Tgt Ion:196 Resp: 101773


Ion Ratio Lower Upper

196 100

198 98.8 77.5 116.3

200 31.1 25.0 37.4





#42

2,4,5-Trichlorophenol

Concen: 20.225 ng/ul

RT: 12.657 min Scan# 1

Delta R.T. -0.029 min

Lab File: BP023320.D

Acq: 26 Nov 2024 11:34

Instrument :

BNA_P

ClientSampleId :

SSTD020740





Tgt Ion:196 Resp: 110774

Ion Ratio Lower Upper

196 100

198 95.9 76.3 114.5

200 29.4 24.6 36.8

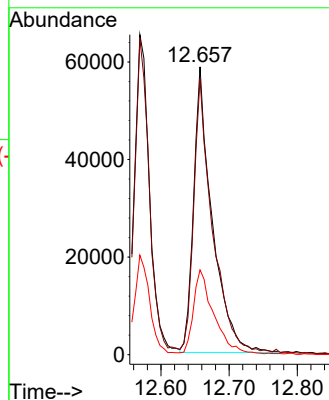

#43

1,1'-Biphenyl

Concen: 20.929 ng/ul

RT: 12.957 min Scan# 1695

Delta R.T. -0.029 min

Lab File: BP023320.D

Acq: 26 Nov 2024 11:34




Tgt Ion:154 Resp: 331426


Ion Ratio Lower Upper

154 100

153 40.6 32.8 49.2

76 11.3 10.0 15.0

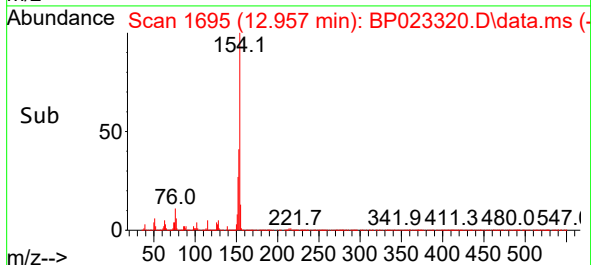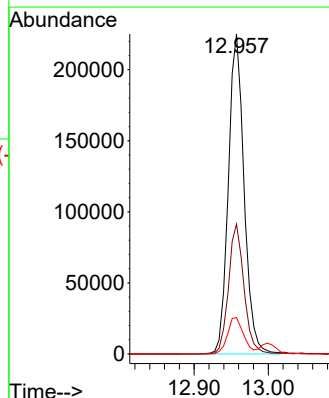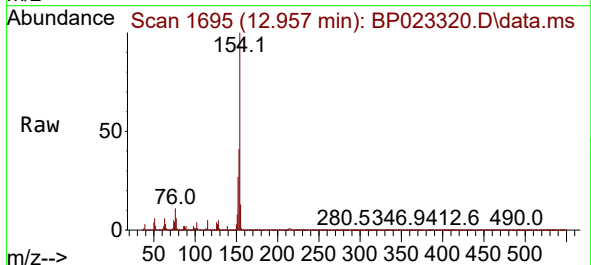



#44

2-Chloronaphthalene

Concen: 20.783 ng/ul

RT: 12.998 min Scan# 1

Delta R.T. -0.035 min

Lab File: BP023320.D

Acq: 26 Nov 2024 11:34

Instrument :

BNA_P

ClientSampleId :

SSTD020740





Tgt Ion:162 Resp: 269038

Ion Ratio Lower Upper

162 100

164 32.6 25.8 38.6

127 37.5 31.2 46.8



#45

2-Nitroaniline

Concen: 22.308 ng/ul

RT: 13.240 min Scan# 1743

Delta R.T. -0.024 min

Lab File: BP023320.D

Acq: 26 Nov 2024 11:34




Tgt Ion: 65 Resp: 81084


Ion Ratio Lower Upper

65 100

92 66.1 50.5 75.7

138 82.5 68.0 102.0









#47
Dimethylphthalate
Concen: 21.063 ng/ul
RT: 13.610 min Scan# 1806
Delta R.T. -0.012 min
Lab File: BP023320.D
Acq: 26 Nov 2024 11:34




Instrument :
BNA_P
ClientSampleId :
SSTD020740


Tgt Ion:163 Resp: 369987
Ion Ratio Lower Upper
163 100
194 4.3 3.3 4.9
164 10.3 8.6 13.0

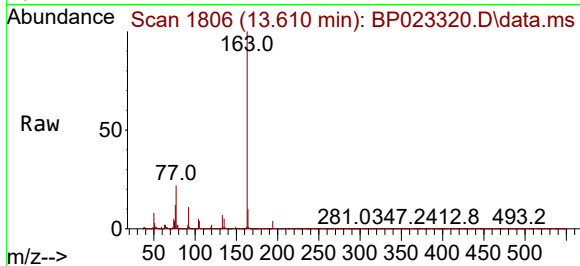

#48
2,6-Dinitrotoluene
Concen: 20.686 ng/ul
RT: 13.734 min Scan# 1827
Delta R.T. -0.035 min
Lab File: BP023320.D
Acq: 26 Nov 2024 11:34

Tgt Ion:165 Resp: 70683
Ion Ratio Lower Upper
165 100
89 61.0 55.4 83.0
121 20.5 18.2 27.2




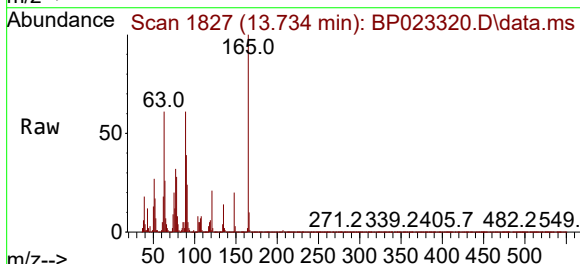




#50
Acenaphthylene
Concen: 21.197 ng/ul
RT: 13.863 min Scan# 1849
Delta R.T. -0.018 min
Lab File: BP023320.D
Acq: 26 Nov 2024 11:34




Instrument :
BNA_P
ClientSampleId :
SSTD020740


Tgt Ion:152 Resp: 398215
Ion Ratio Lower Upper
152 100
151 20.5 15.7 23.5
153 13.3 10.5 15.7



#51
3-Nitroaniline
Concen: 21.069 ng/ul
RT: 14.081 min Scan# 1886
Delta R.T. -0.035 min
Lab File: BP023320.D
Acq: 26 Nov 2024 11:34

Tgt Ion:138 Resp: 62006
Ion Ratio Lower Upper
138 100
108 13.1 9.8 14.8
92 137.9 105.8 158.8









#52
Acenaphthene
Concen: 21.181 ng/ul
RT: 14.210 min Scan# 1911
Delta R.T. -0.018 min
Lab File: BP023320.D
Acq: 26 Nov 2024 11:34




Instrument :
BNA_P
ClientSampleId :
SSTD020740


Tgt Ion:153 Resp: 288895
Ion Ratio Lower Upper
153 100
152 46.3 39.0 58.6
154 86.8 71.0 106.4



#53
2,4-Dinitrophenol
Concen: 16.098 ng/ul
RT: 14.334 min Scan# 1929
Delta R.T. -0.006 min
Lab File: BP023320.D
Acq: 26 Nov 2024 11:34

Tgt Ion:184 Resp: 39029
Ion Ratio Lower Upper
184 100
63 62.6 50.4 75.6
154 64.5 57.9 86.9









#55
4-Nitrophenol
Concen: 13.959 ng/ul
RT: 14.434 min Scan# 1946
Delta R.T. -0.029 min
Lab File: BP023320.D
Acq: 26 Nov 2024 11:34




Instrument :
BNA_P
ClientSampleId :
SSTD020740


Tgt Ion:109 Resp: 43717
Ion Ratio Lower Upper
109 100
139 87.6 66.7 100.1
65 110.8 86.1 129.1



#56
Dibenzofuran
Concen: 20.448 ng/ul
RT: 14.557 min Scan# 1967
Delta R.T. -0.018 min
Lab File: BP023320.D
Acq: 26 Nov 2024 11:34

Tgt Ion:168 Resp: 430901
Ion Ratio Lower Upper
168 100
139 38.7 31.0 46.4





#57

2,4-Dinitrotoluene

Concen: 21.020 ng/ul

RT: 14.563 min Scan# 1969

Delta R.T. -0.006 min

Lab File: BP023320.D

Acq: 26 Nov 2024 11:34

Instrument :

BNA_P

ClientSampleId :

SSTD020740





Tgt Ion:165 Resp: 114472

Ion Ratio Lower Upper

165 100

63 60.2 52.2 78.2

182 2.7 2.3 3.5

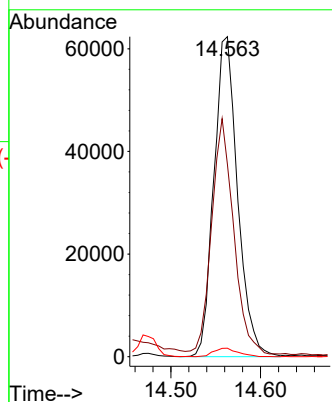

#58

2,3,4,6-Tetrachlorophenol

Concen: 20.223 ng/ul

RT: 14.798 min Scan# 2008

Delta R.T. -0.029 min

Lab File: BP023320.D

Acq: 26 Nov 2024 11:34

Tgt Ion:232 Resp: 108269




Ion Ratio Lower Upper


232 100

131 37.0 32.2 48.2

130 2.2 2.1 3.1

166 28.7 24.0 36.0





#59

Diethylphthalate

Concen: 20.851 ng/ul

RT: 15.004 min Scan# 2044

Delta R.T. -0.006 min

Lab File: BP023320.D

Acq: 26 Nov 2024 11:34

Instrument :

BNA_P

ClientSampleId :

SSTD020740





Tgt Ion:149 Resp: 362244

Ion Ratio Lower Upper

149 100

177 23.2 18.4 27.6

150 12.2 9.8 14.8

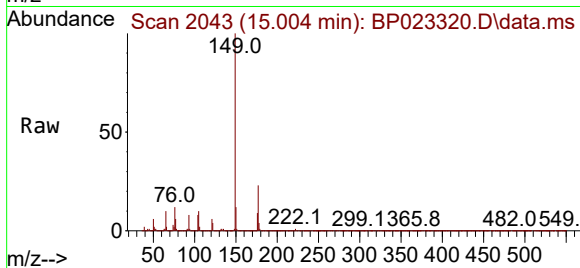

#61

Fluorene

Concen: 20.296 ng/ul

RT: 15.216 min Scan# 2079

Delta R.T. -0.024 min

Lab File: BP023320.D

Acq: 26 Nov 2024 11:34




Tgt Ion:166 Resp: 350060


Ion Ratio Lower Upper

166 100

165 98.2 78.5 117.7

167 13.3 11.1 16.7




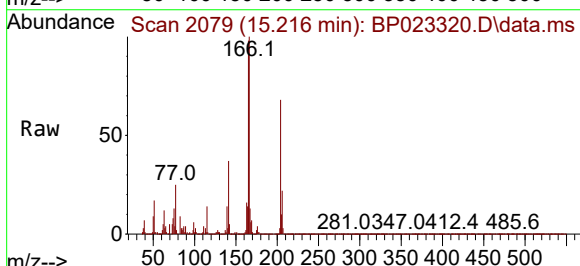




#62
4-Chlorophenyl-phenylether
Concen: 19.725 ng/ul
RT: 15.216 min Scan# 2081
Delta R.T. -0.012 min
Lab File: BP023320.D
Acq: 26 Nov 2024 11:34




Instrument :
BNA_P
ClientSampleId :
SSTD020740


Tgt Ion:204 Resp: 200315
Ion Ratio Lower Upper
204 100
206 31.9 26.9 40.3
141 54.5 42.4 63.6

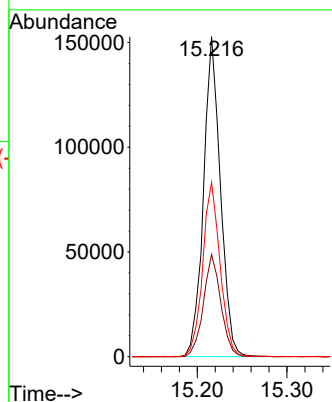

#63
4-Nitroaniline
Concen: 21.330 ng/ul
RT: 15.292 min Scan# 2092
Delta R.T. 0.006 min
Lab File: BP023320.D
Acq: 26 Nov 2024 11:34

Tgt Ion:138 Resp: 58412
Ion Ratio Lower Upper
138 100
92 59.2 53.0 79.4
108 116.7 96.2 144.2









#66
4,6-Dinitro-2-methylphenol
Concen: 19.207 ng/ul
RT: 15.345 min Scan# 2118
Delta R.T. -0.006 min
Lab File: BP023320.D
Acq: 26 Nov 2024 11:34




Instrument :
BNA_P
ClientSampleId :
SSTD020740


Tgt Ion:198 Resp: 76763
Ion Ratio Lower Upper
198 100
182 5.7 3.7 5.5#
77 30.1 19.1 28.7#

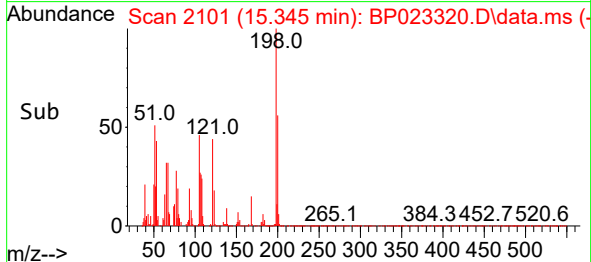

#67
N-Nitrosodiphenylamine
Concen: 21.356 ng/ul
RT: 15.445 min Scan# 2118
Delta R.T. -0.012 min
Lab File: BP023320.D
Acq: 26 Nov 2024 11:34

Tgt Ion:169 Resp: 308203
Ion Ratio Lower Upper
169 100
168 67.0 53.3 79.9
167 36.1 28.6 42.8


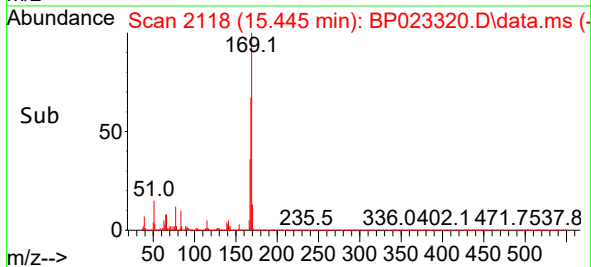

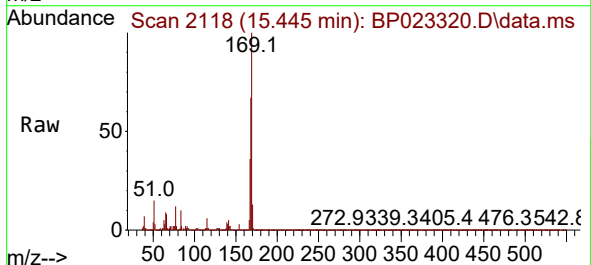




#68
4-Bromophenyl-phenylether
Concen: 19.713 ng/ul
RT: 16.139 min Scan# 21
Delta R.T. 0.000 min
Lab File: BP023320.D
Acq: 26 Nov 2024 11:34




Instrument :
BNA_P
ClientSampleId :
SSTD020740


Tgt Ion	Ratio	Lower	Upper
248	100		
250	101.5	78.5	117.7
141	68.0	52.5	78.7

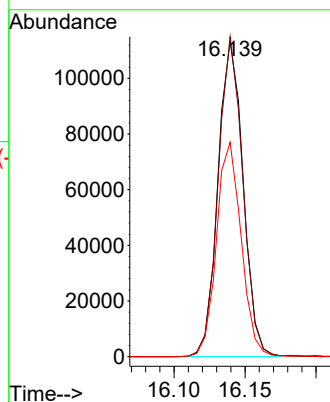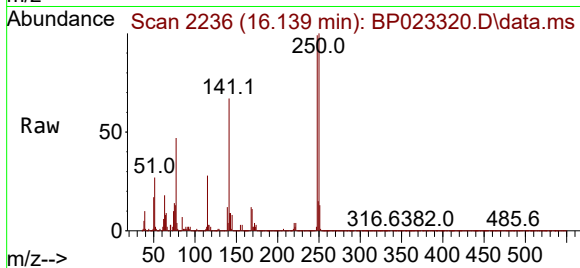

#69
Hexachlorobenzene
Concen: 19.316 ng/ul
RT: 16.251 min Scan# 2255
Delta R.T. -0.012 min
Lab File: BP023320.D
Acq: 26 Nov 2024 11:34

Tgt Ion	Ratio	Lower	Upper
284	100		
142	26.8	23.3	34.9
249	31.3	27.2	40.8

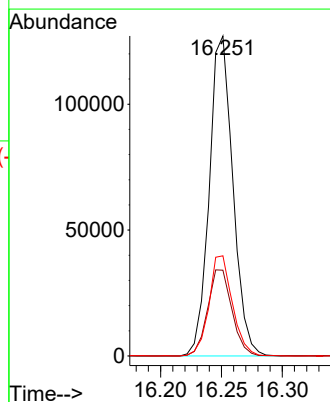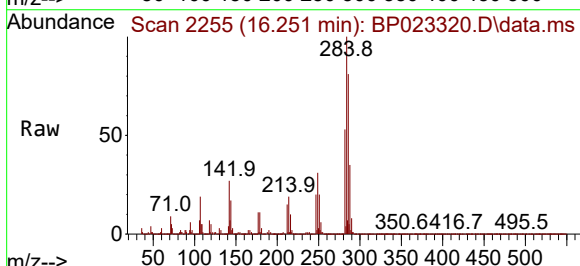



#70

Atrazine

Concen: 20.095 ng/ul

RT: 16.433 min Scan# 21

Delta R.T. 0.000 min

Lab File: BP023320.D

Acq: 26 Nov 2024 11:34

Instrument :

BNA_P

ClientSampleId :

SSTD020740





Tgt Ion:200 Resp: 140184

Ion Ratio Lower Upper

200 100

173 21.3 18.9 28.3

215 47.2 38.0 57.0



#71

Pentachlorophenol

Concen: 17.388 ng/ul

RT: 16.622 min Scan# 2318

Delta R.T. -0.018 min

Lab File: BP023320.D

Acq: 26 Nov 2024 11:34




Tgt Ion:266 Resp: 96111


Ion Ratio Lower Upper

266 100

264 64.6 47.9 71.9

268 65.4 48.2 72.4

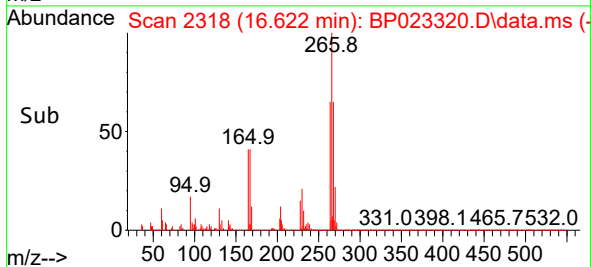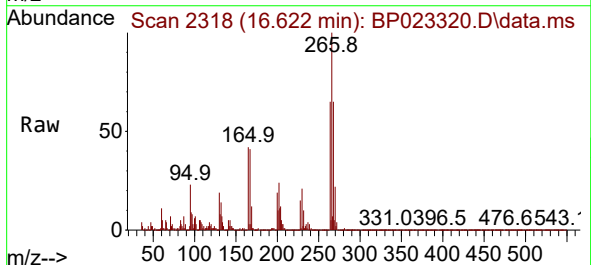



#72

Phenanthrene

Concen: 20.897 ng/ul

RT: 17.010 min Scan# 21

Delta R.T. -0.012 min

Lab File: BP023320.D

Acq: 26 Nov 2024 11:34

Instrument :

BNA_P

ClientSampleId :

SSTD020740





Tgt Ion:178 Resp: 616206

Ion Ratio Lower Upper

178 100

179 15.1 12.1 18.1

176 18.8 15.4 23.0

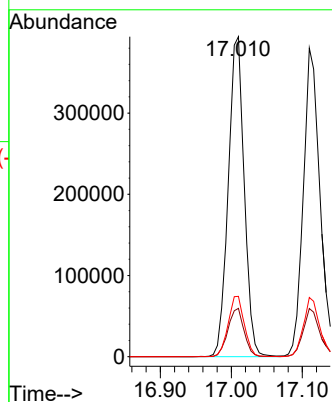

#74

Anthracene

Concen: 21.114 ng/ul

RT: 17.110 min Scan# 2401

Delta R.T. 0.000 min

Lab File: BP023320.D

Acq: 26 Nov 2024 11:34




Tgt Ion:178 Resp: 625975


Ion Ratio Lower Upper

178 100

179 15.6 12.3 18.5

176 19.2 14.7 22.1





#75

1,2,3,4-Tetrachlorobenzene

Concen: 19.685 ng/uL

RT: 12.928 min Scan# 1690

Delta R.T. -0.024 min

Lab File: BP023320.D

Acq: 26 Nov 2024 11:34

Instrument :

BNA_P

ClientSampleId :

SSTD020740





Tgt Ion:216 Resp: 162323

Ion Ratio Lower Upper

216 100

214 77.3 62.9 94.3

218 47.3 39.2 58.8

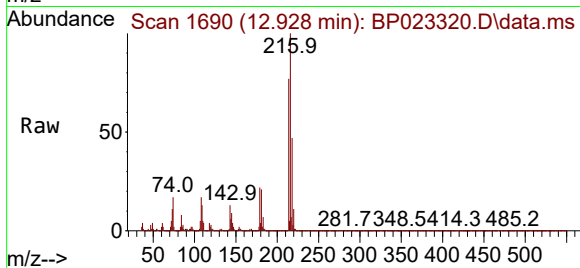

#76

Pentachlorobenzene

Concen: 19.850 ng/uL

RT: 14.475 min Scan# 1953

Delta R.T. -0.024 min

Lab File: BP023320.D

Acq: 26 Nov 2024 11:34




Tgt Ion:250 Resp: 186895


Ion Ratio Lower Upper

250 100

248 63.1 50.1 75.1

252 62.8 51.0 76.4


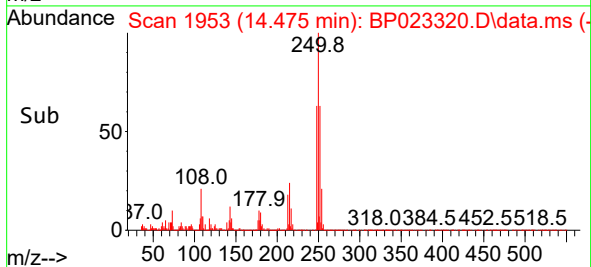

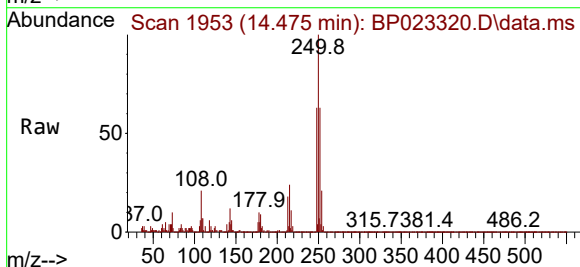




#77
 Carbazole
 Concen: 20.462 ng/ul
 RT: 17.404 min Scan# 2452
 Delta R.T. -0.006 min
 Lab File: BP023320.D
 Acq: 26 Nov 2024 11:34




Instrument :
 BNA_P
 ClientSampleId :
 SSTD020740


Tgt Ion:167 Resp: 529273
 Ion Ratio Lower Upper
 167 100
 166 22.4 17.3 25.9
 139 12.3 10.3 15.5

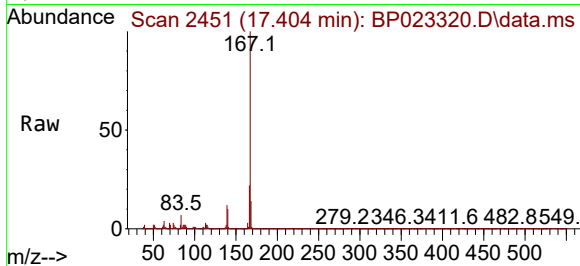

#78
 Di-n-butylphthalate
 Concen: 22.289 ng/ul
 RT: 17.975 min Scan# 2548
 Delta R.T. -0.006 min
 Lab File: BP023320.D
 Acq: 26 Nov 2024 11:34

Tgt Ion:149 Resp: 639765
 Ion Ratio Lower Upper
 149 100
 150 9.4 7.4 11.0
 104 6.3 5.2 7.8

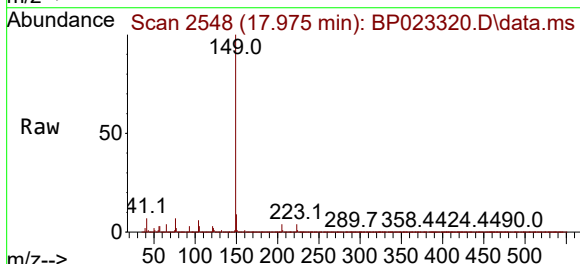




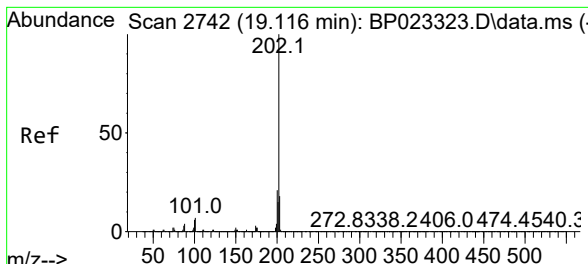


#80
 Fluoranthene
 Concen: 21.442 ng/ul
 RT: 19.122 min Scan# 21
 Delta R.T. 0.006 min
 Lab File: BP023320.D
 Acq: 26 Nov 2024 11:34

Instrument :
 BNA_P
 ClientSampleId :
 SSTD020740

Tgt Ion:202 Resp: 823312




Ion	Ratio	Lower	Upper
202	100		
101	7.0	5.6	8.4
100	5.6	4.6	7.0

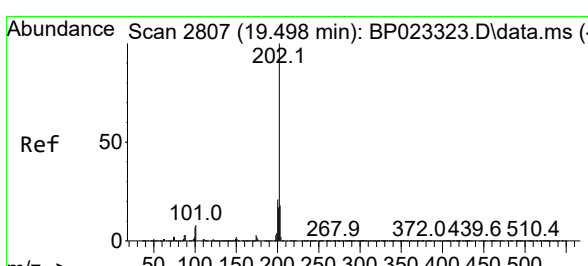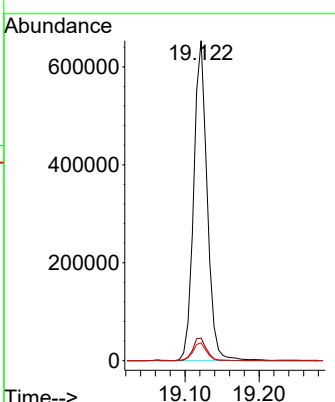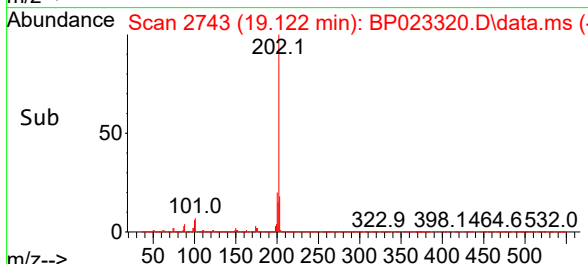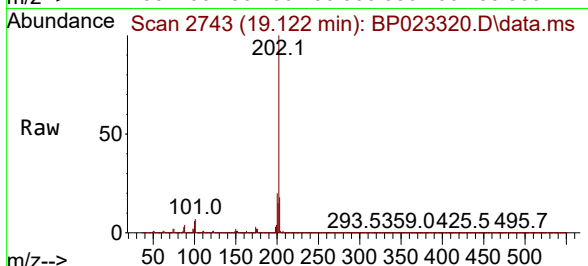


#82
 Pyrene
 Concen: 21.379 ng/ul
 RT: 19.504 min Scan# 2808
 Delta R.T. 0.006 min
 Lab File: BP023320.D
 Acq: 26 Nov 2024 11:34

Tgt Ion:202 Resp: 881847

Ion	Ratio	Lower	Upper
202	100		
101	8.3	6.7	10.1
100	6.9	5.8	8.8

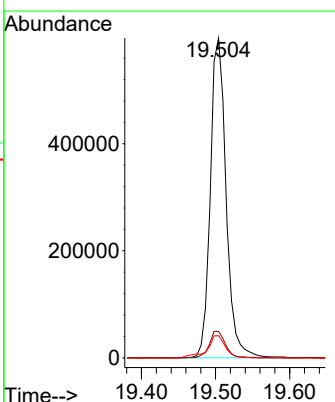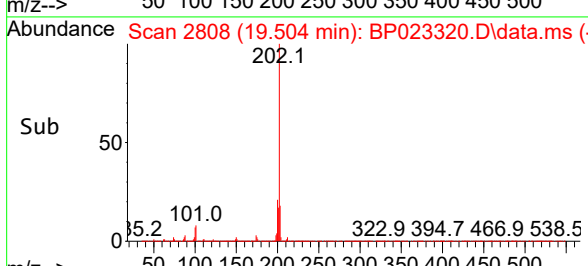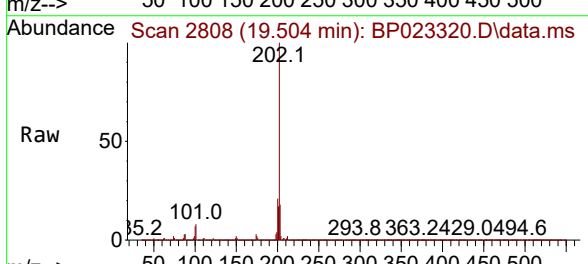



#83

Butylbenzylphthalate

Concen: 22.117 ng/ul

RT: 20.457 min Scan# 2968

Delta R.T. 0.012 min

Lab File: BP023320.D

Acq: 26 Nov 2024 11:34

Instrument :

BNA_P

ClientSampleId :

SSTD020740





Tgt Ion:149 Resp: 300358

Ion Ratio Lower Upper

149 100

91 78.0 59.0 88.4

206 24.0 20.7 31.1

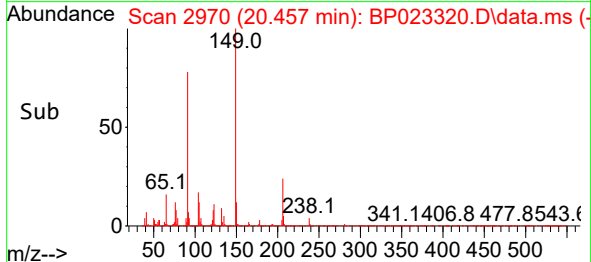

#84

3,3'-Dichlorobenzidine

Concen: 20.166 ng/ul

RT: 21.333 min Scan# 3119

Delta R.T. 0.024 min

Lab File: BP023320.D

Acq: 26 Nov 2024 11:34




Tgt Ion:252 Resp: 327546


Ion Ratio Lower Upper

252 100

254 64.5 51.8 77.8

126 6.6 5.0 7.6

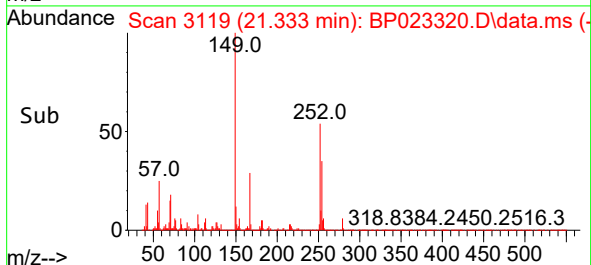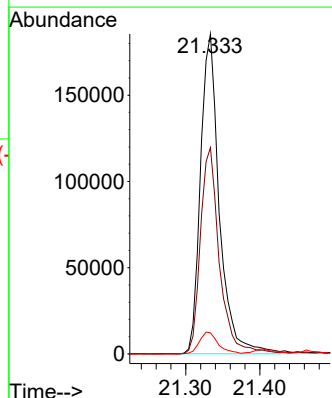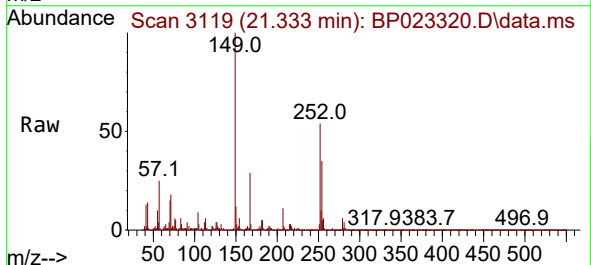



#85

Benzo(a)anthracene

Concen: 21.204 ng/ul

RT: 21.404 min Scan# 3119

Delta R.T. 0.018 min

Lab File: BP023320.D

Acq: 26 Nov 2024 11:34

Instrument :

BNA_P

ClientSampleId :

SSTD020740





Tgt Ion:228 Resp: 936843

Ion Ratio Lower Upper

228 100

229 19.3 15.7 23.5

226 26.1 21.6 32.4

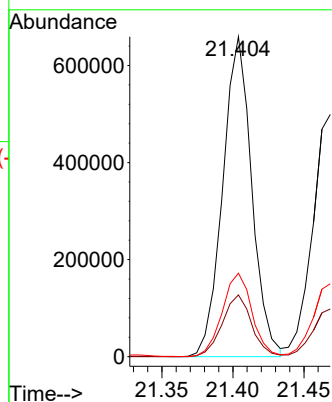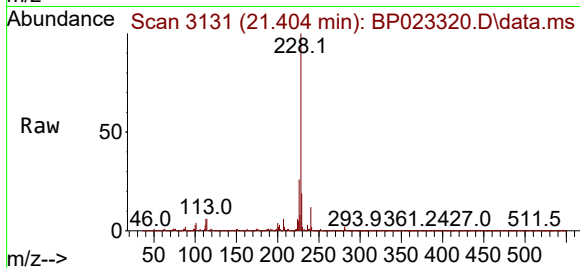

#86

Bis(2-ethylhexyl)phthalate

Concen: 22.493 ng/ul

RT: 21.333 min Scan# 3119

Delta R.T. 0.029 min

Lab File: BP023320.D

Acq: 26 Nov 2024 11:34




Tgt Ion:149 Resp: 434090


Ion Ratio Lower Upper

149 100

167 28.8 22.5 33.7

279 6.1 3.7 5.5#

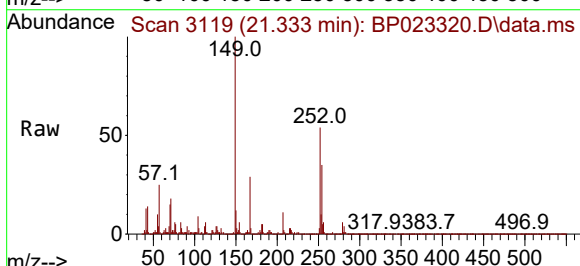



#87

Chrysene

Concen: 20.934 ng/ul

RT: 21.469 min Scan# 3142

Delta R.T. 0.018 min

Lab File: BP023320.D

Acq: 26 Nov 2024 11:34

Instrument :

BNA_P

ClientSampleId :

SSTD020740





Tgt Ion:228 Resp: 870287

Ion Ratio Lower Upper

228 100

226 30.1 24.2 36.2

229 19.7 15.6 23.4

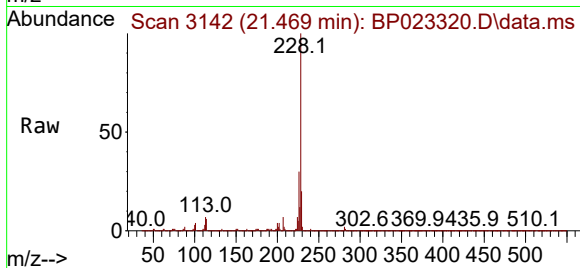

#89

Di-n-octyl phthalate

Concen: 22.543 ng/ul




RT: 22.545 min Scan# 3325


Delta R.T. 0.024 min

Lab File: BP023320.D

Acq: 26 Nov 2024 11:34

Tgt Ion:149 Resp: 749896

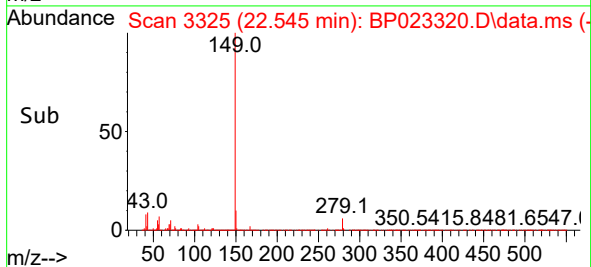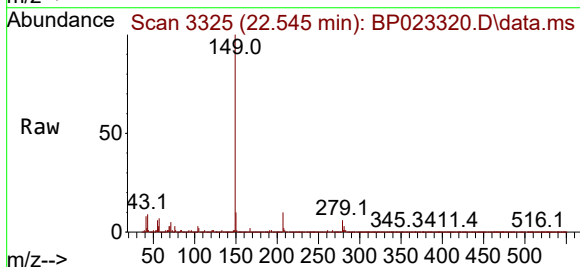



#90

Benzo(b)fluoranthene

Concen: 21.435 ng/ul

RT: 23.615 min Scan# 3507

Delta R.T. 0.029 min

Lab File: BP023320.D

Acq: 26 Nov 2024 11:34

Instrument :

BNA_P

ClientSampleId :

SSTD020740





Tgt Ion:252 Resp: 978227

Ion Ratio Lower Upper

252 100

253 22.2 17.3 25.9

125 5.4 4.4 6.6

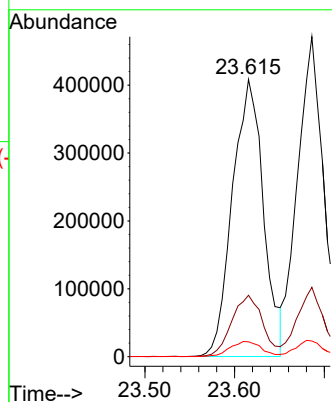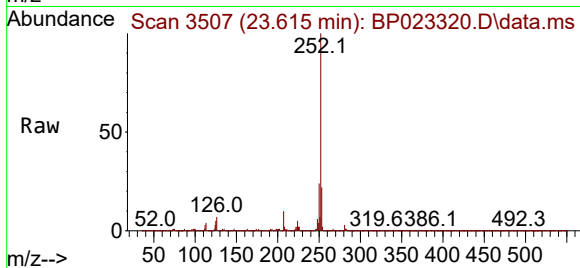

#91

Benzo(k)fluoranthene

Concen: 21.888 ng/ul

RT: 23.686 min Scan# 3519

Delta R.T. 0.029 min

Lab File: BP023320.D

Acq: 26 Nov 2024 11:34




Tgt Ion:252 Resp: 983349


Ion Ratio Lower Upper

252 100

253 21.7 17.5 26.3

125 4.9 4.3 6.5



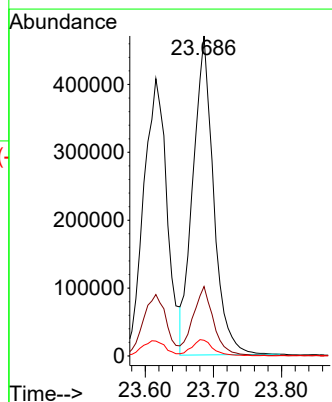
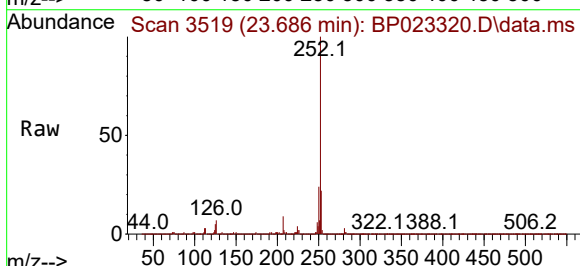




#93
Benzo(a)pyrene
Concen: 21.179 ng/ul
RT: 24.480 min Scan# 30
Delta R.T. 0.035 min
Lab File: BP023320.D
Acq: 26 Nov 2024 11:34




Instrument :
BNA_P
ClientSampleId :
SSTD020740


Tgt Ion:252 Resp: 873768
Ion Ratio Lower Upper
252 100
253 22.1 17.4 26.0
125 6.1 5.0 7.4



#94
Indeno(1,2,3-cd)pyrene
Concen: 7.835 ng/ul
RT: 28.245 min Scan# 4294
Delta R.T. 0.041 min
Lab File: BP023320.D
Acq: 26 Nov 2024 11:34

Tgt Ion:276 Resp: 450337
Ion Ratio Lower Upper
276 100
138 9.6 7.8 11.6
277 23.7 19.8 29.8





#95

Dibenzo(a,h)anthracene

Concen: 18.869 ng/ul

RT: 28.309 min Scan# 41

Delta R.T. 0.029 min

Lab File: BP023320.D

Acq: 26 Nov 2024 11:34

Instrument :

BNA_P

ClientSampleId :

SSTD020740





Tgt Ion:278 Resp: 880595

Ion Ratio Lower Upper

278 100

139 7.6 6.0 9.0

279 22.8 19.2 28.8

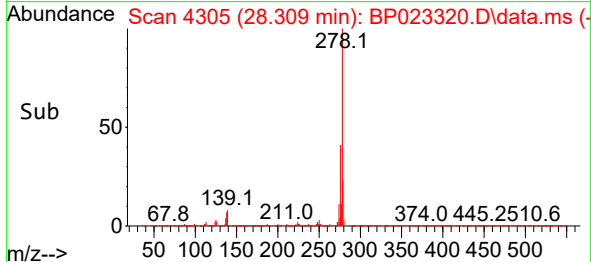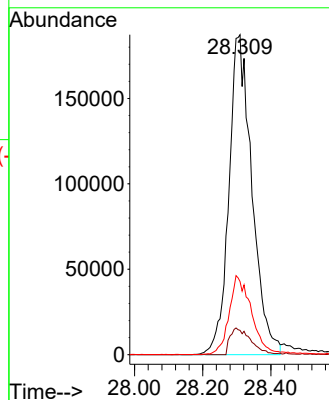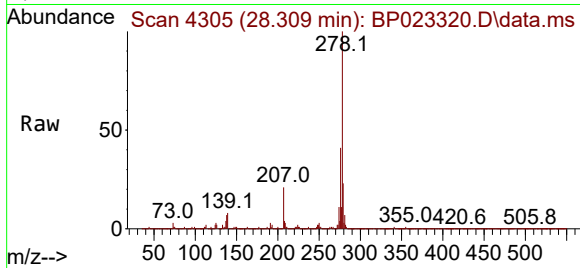

#96

Benzo(g,h,i)perylene

Concen: 18.496 ng/ul

RT: 29.368 min Scan# 4485

Delta R.T. 0.018 min

Lab File: BP023320.D

Acq: 26 Nov 2024 11:34

Tgt Ion:276 Resp: 807515

Ion Ratio Lower Upper

276 100

138 11.5 8.5 12.7

277 24.1 18.9 28.3

