




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112624\
Data File : BP023322.D
Acq On : 26 Nov 2024 14:16
Operator : RC/JU
Sample : SSTD01056
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SSTD010636

Manual IntegrationsAPPROVED

Quant Time: Nov 26 23:24:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 26 23:16:47 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/27/2024
Supervised By :mohammad ahmed 11/27/2024

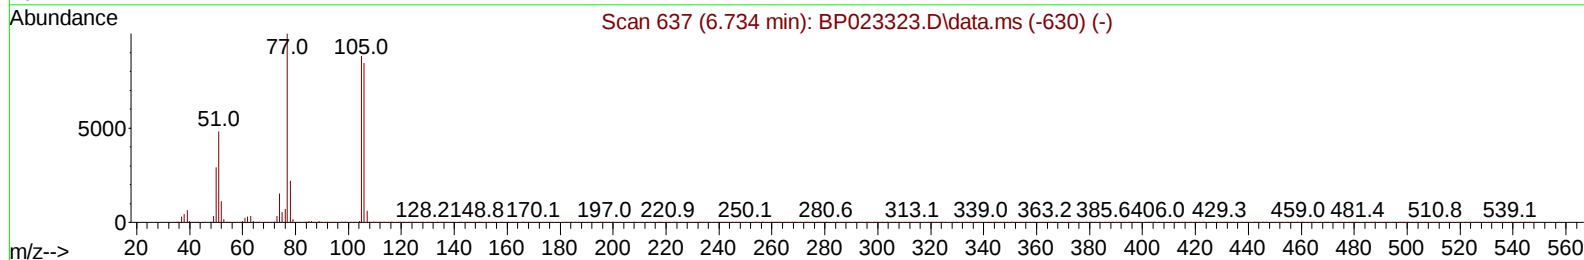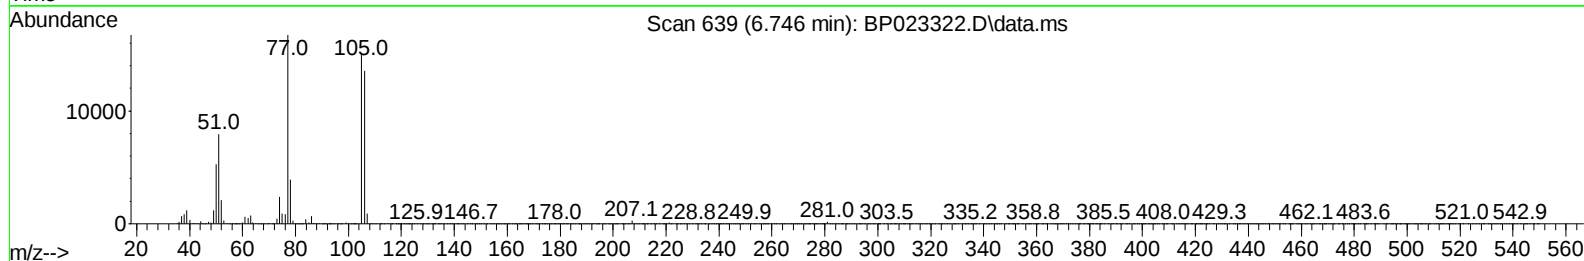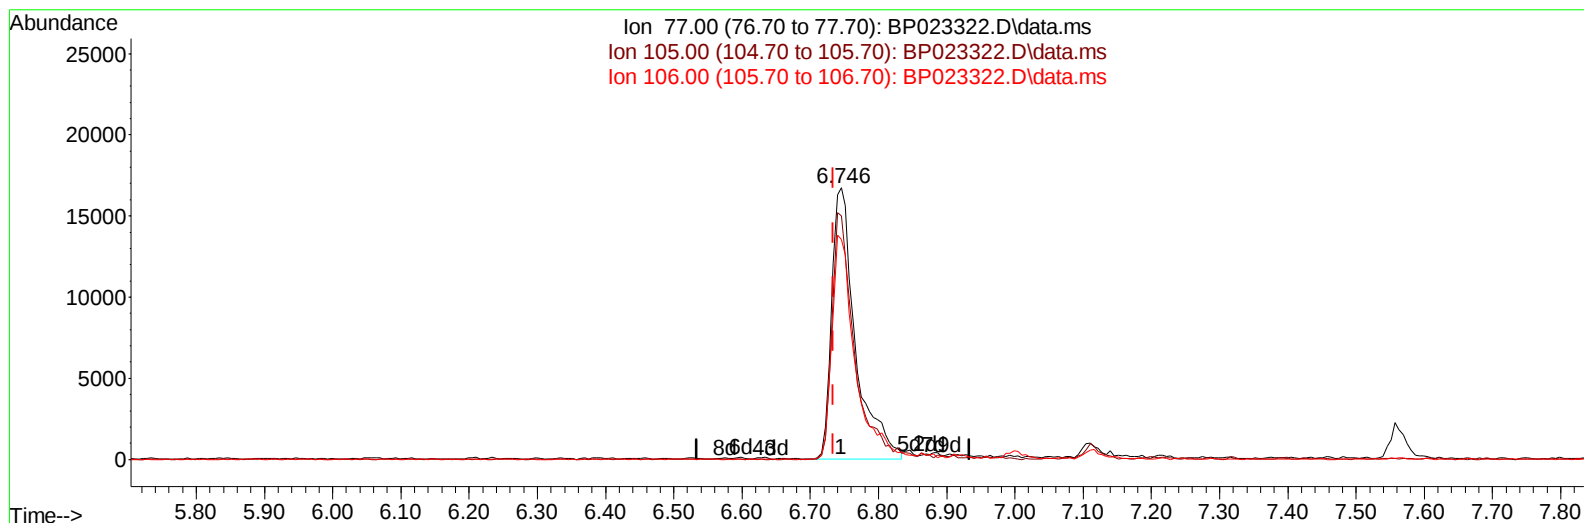

TIC: BP023322.D\data.ms

(6) Benzaldehyde

6.746min (+ 0.012) 13.62 ng/u1

response 40649

Ion	Exp%	Act%
77.00	100.00	100.00
105.00	88.30	89.71
106.00	84.20	80.98
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112624\
Data File : BP023322.D
Acq On : 26 Nov 2024 14:16
Operator : RC/JU
Sample : SSTD01056
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SSTD010636

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/27/2024
Supervised By :mohammad ahmed 11/27/2024

Quant Time: Nov 26 23:24:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 26 23:16:47 2024
Response via : Initial Calibration

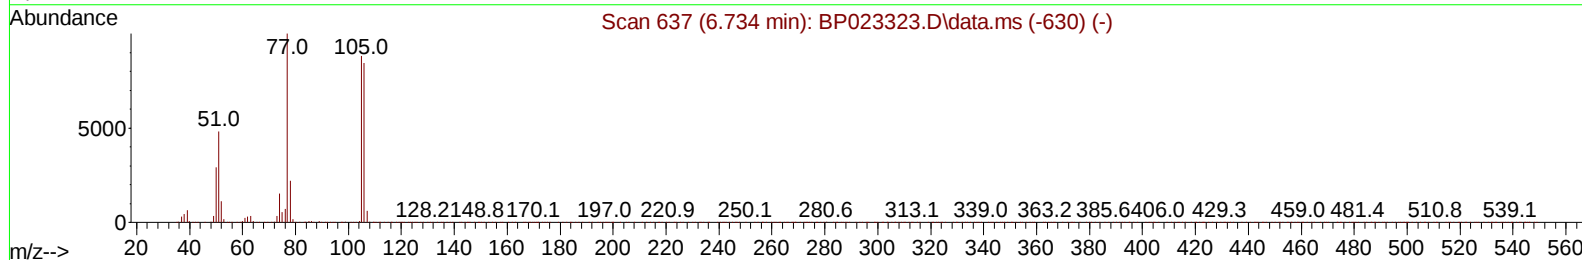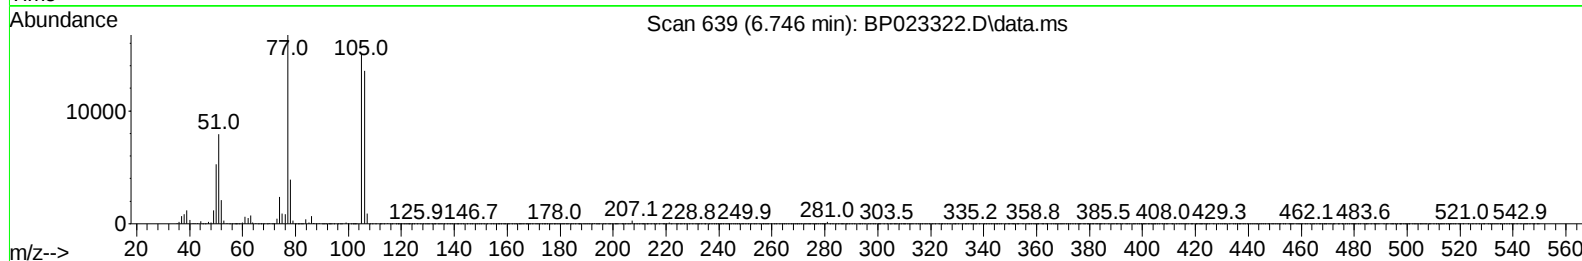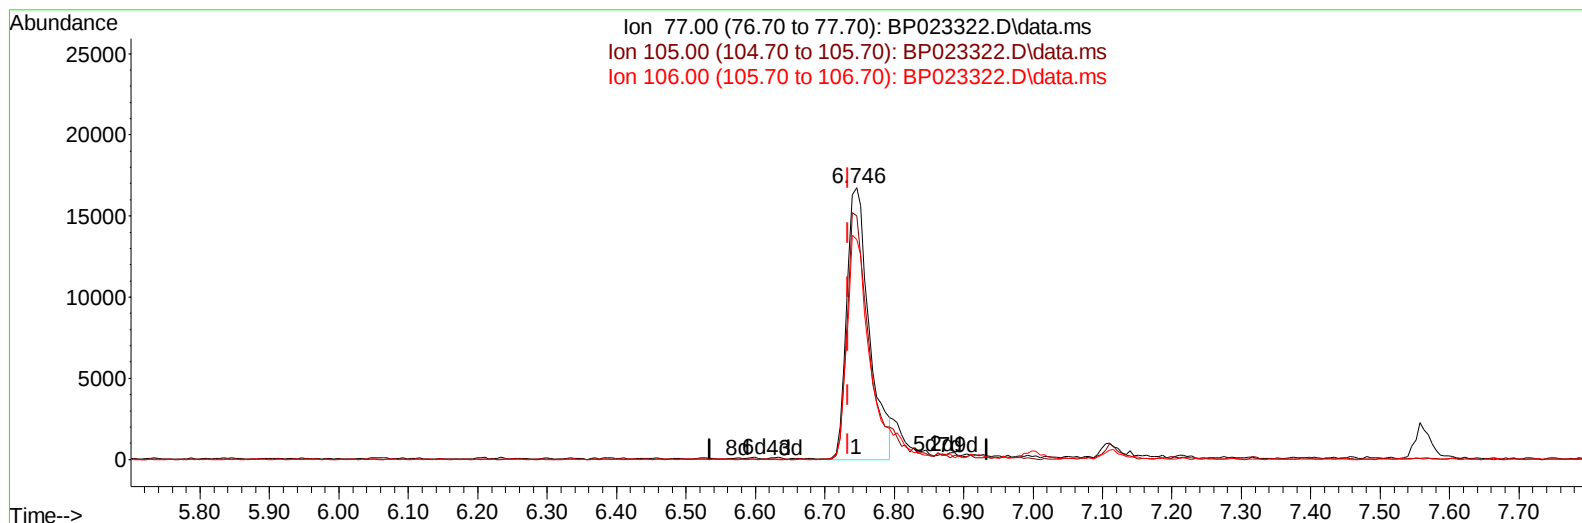

TIC: BP023322.D\data.ms

(6) Benzaldehyde

6.746min (+ 0.012) 12.62 ng/ul m

response 37674

Ion	Exp%	Act%
77.00	100.00	100.00
105.00	88.30	89.71
106.00	84.20	80.98
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112624\
Data File : BP023322.D
Acq On : 26 Nov 2024 14:16
Operator : RC/JU
Sample : SSTD01056
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SSTD010636

Manual IntegrationsAPPROVED

Quant Time: Nov 26 23:24:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 26 23:16:47 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/27/2024
Supervised By :mohammad ahmed 11/27/2024

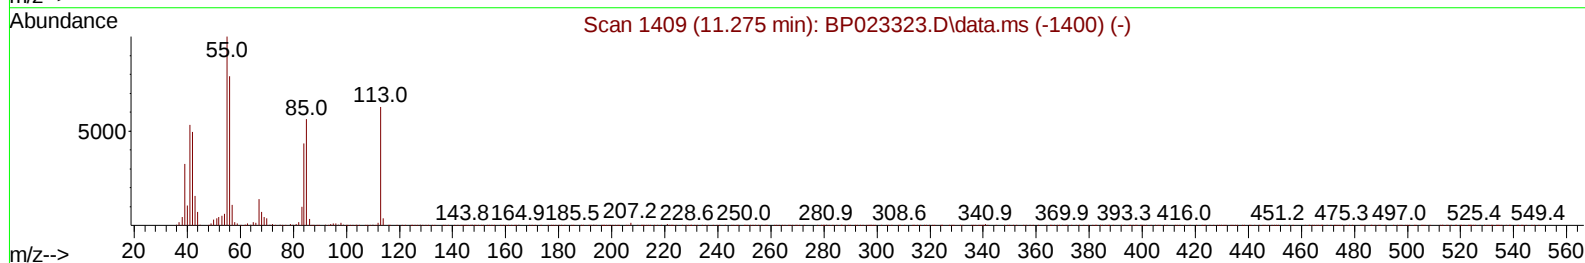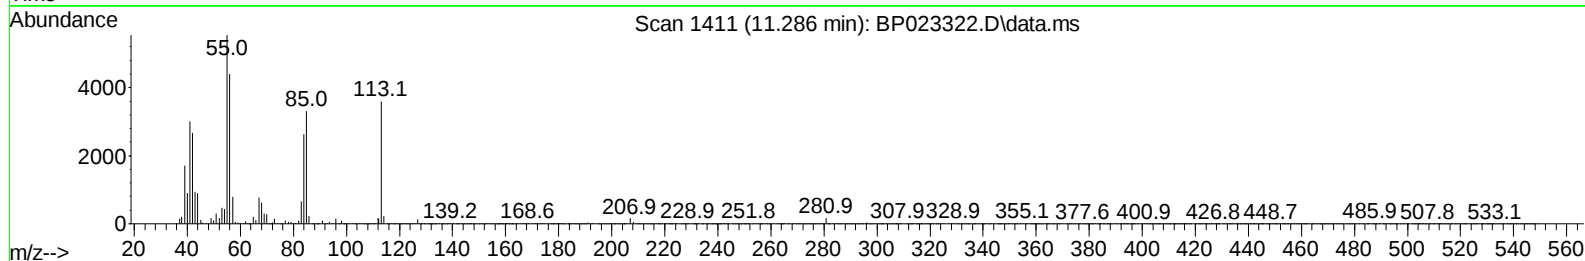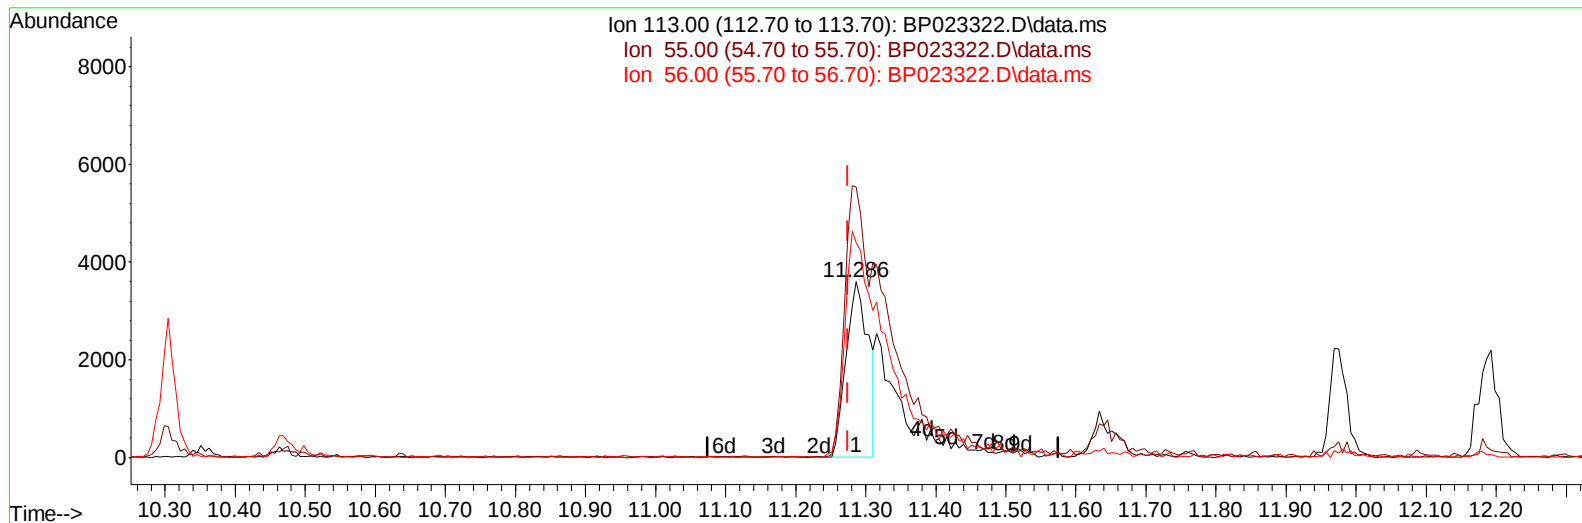

TIC: BP023322.D\data.ms

(34) Caprolactam

11.286min (+ 0.012) 5.55 ng/ul

response 7914

Ion	Exp%	Act%
113.00	100.00	100.00
55.00	159.40	154.28
56.00	125.90	122.26
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112624\
Data File : BP023322.D
Acq On : 26 Nov 2024 14:16
Operator : RC/JU
Sample : SST01056
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SSTD010636

Manual IntegrationsAPPROVED

Quant Time: Nov 26 23:24:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 26 23:16:47 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/27/2024
Supervised By :mohammad ahmed 11/27/2024

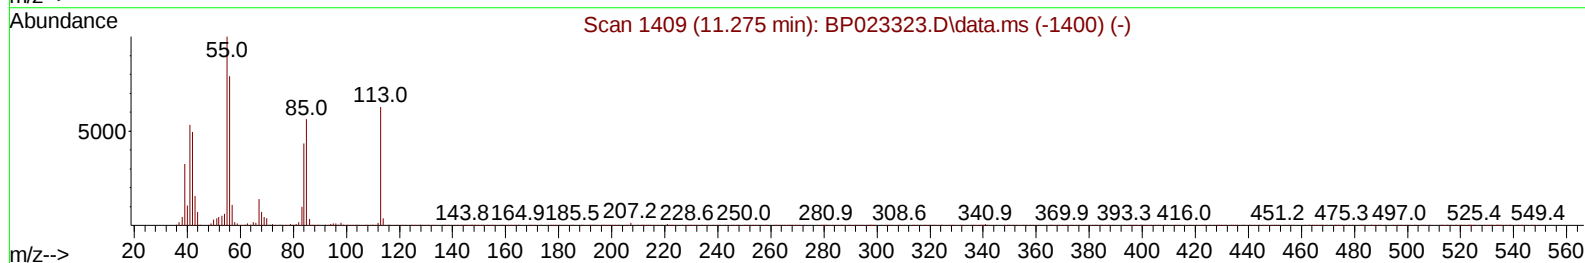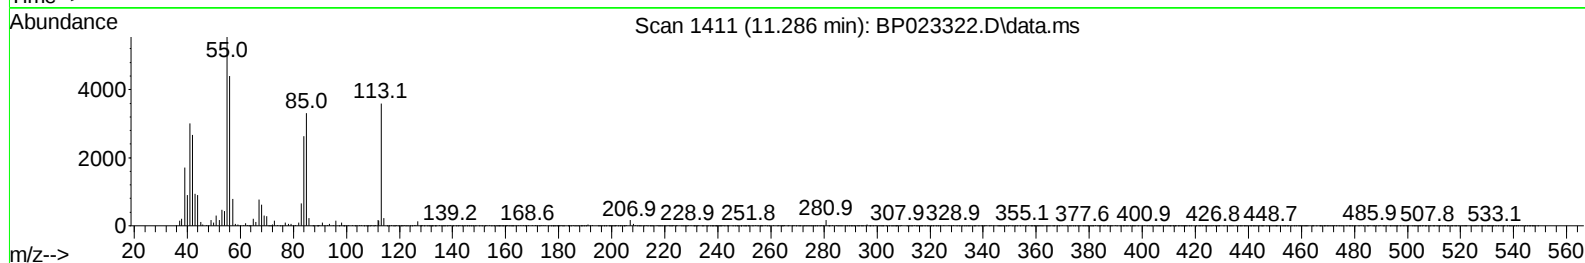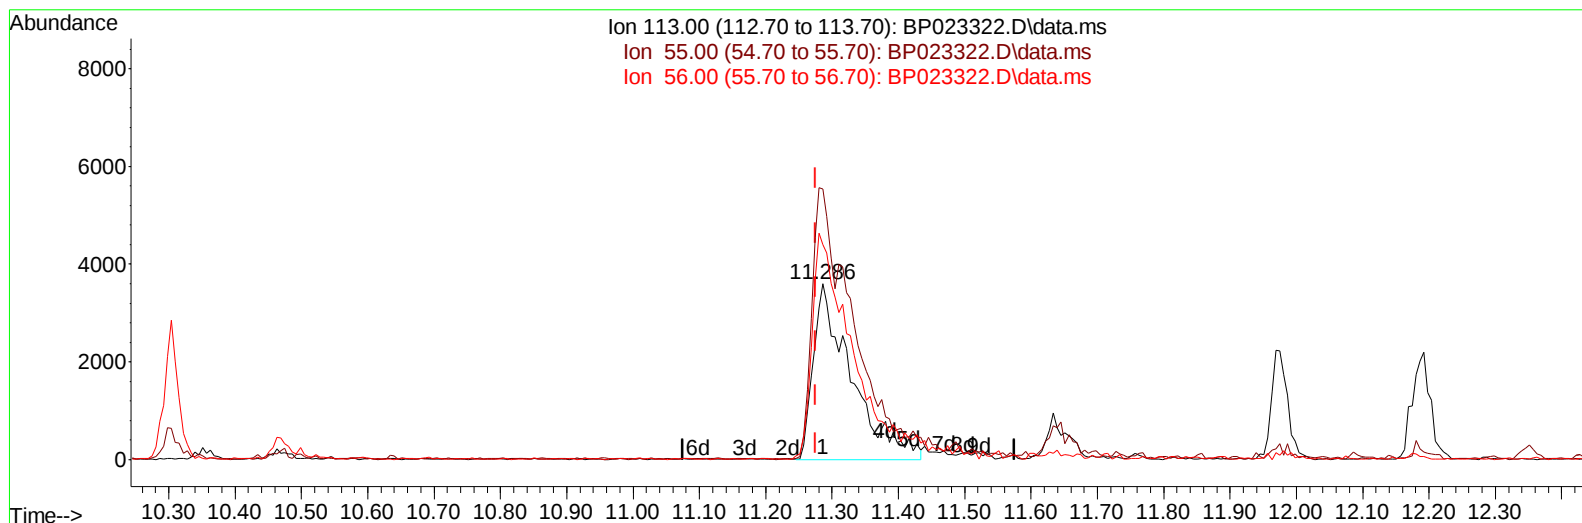

TIC: BP023322.D\data.ms

(34) Caprolactam

11.286min (+ 0.012) 10.02 ng/ul m

response 14283

Ion	Exp%	Act%
113.00	100.00	100.00
55.00	159.40	154.28
56.00	125.90	122.26
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112624\
Data File : BP023322.D
Acq On : 26 Nov 2024 14:16
Operator : RC/JU
Sample : SSTD01056
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SSTD010636

Manual IntegrationsAPPROVED

Quant Time: Nov 26 23:24:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 26 23:16:47 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/27/2024
Supervised By :mohammad ahmed 11/27/2024

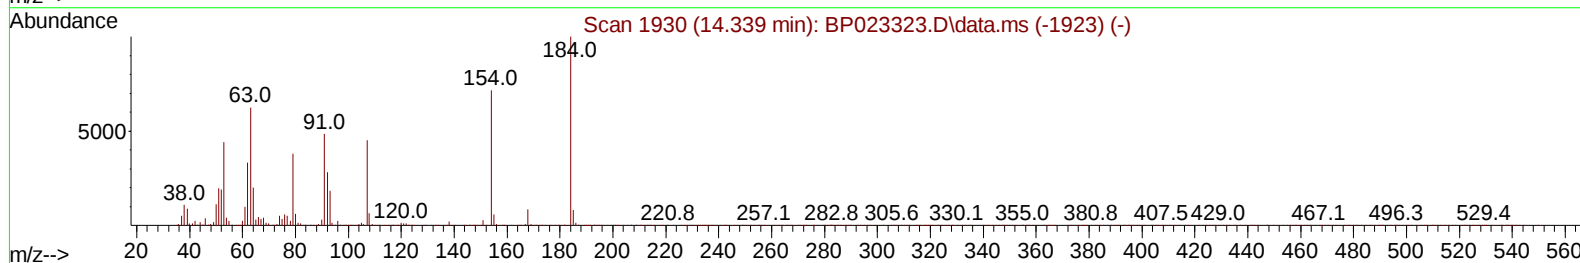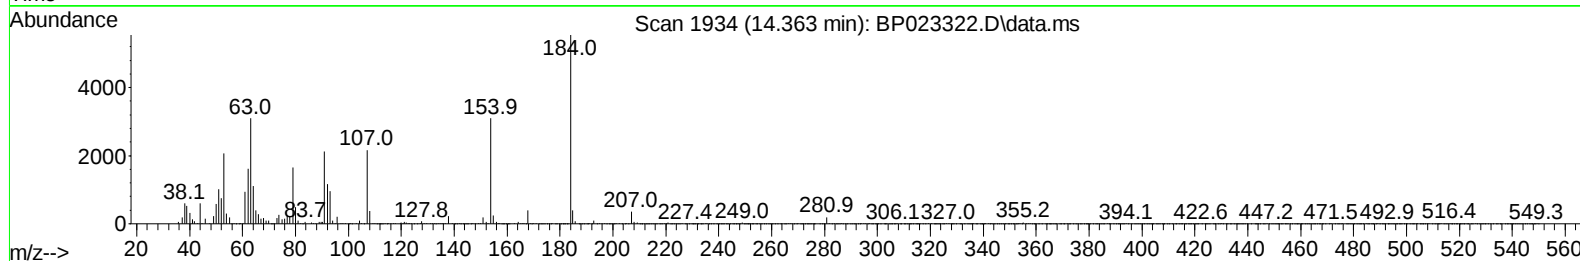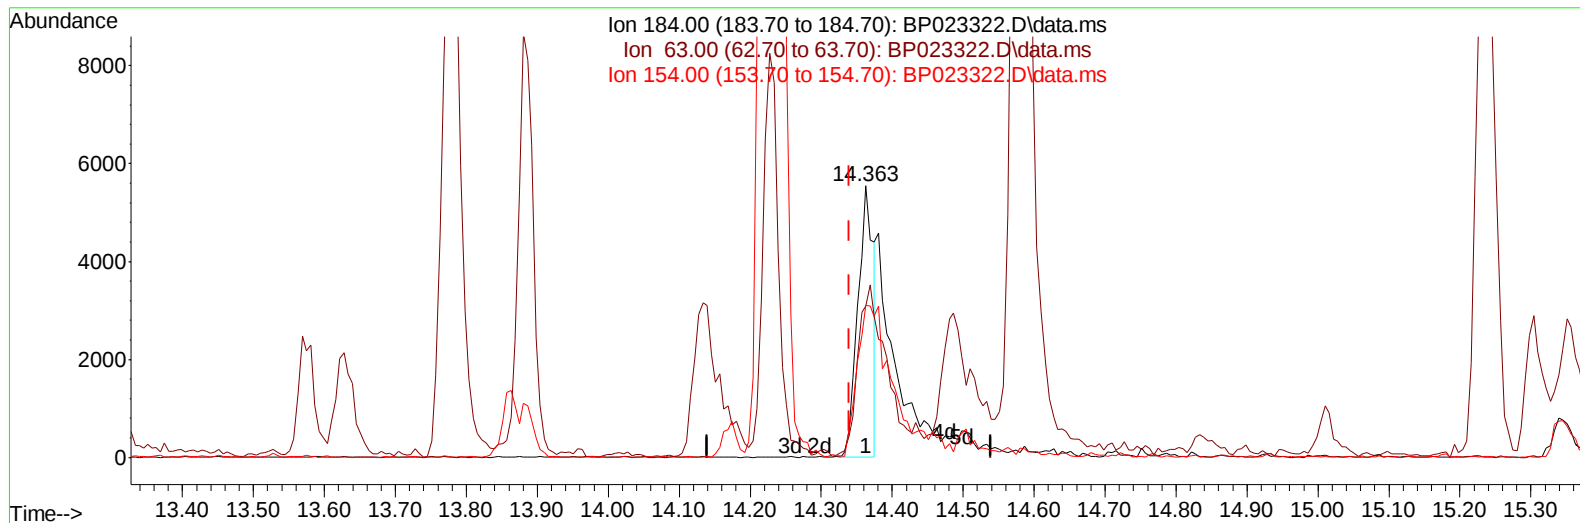

TIC: BP023322.D\data.ms

(53) 2,4-Dinitrophenol

14.363min (+ 0.023) 3.90 ng/ul

response 8407

Ion	Exp%	Act%
184.00	100.00	100.00
63.00	63.00	55.86
154.00	72.40	55.92#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112624\
Data File : BP023322.D
Acq On : 26 Nov 2024 14:16
Operator : RC/JU
Sample : SSTD01056
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SSTD010636

Manual IntegrationsAPPROVED

Quant Time: Nov 26 23:24:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 26 23:16:47 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/27/2024
Supervised By :mohammad ahmed 11/27/2024

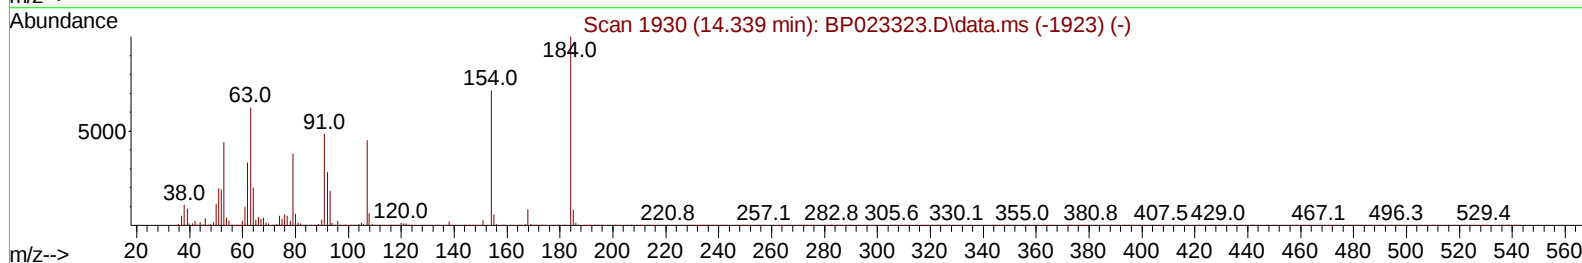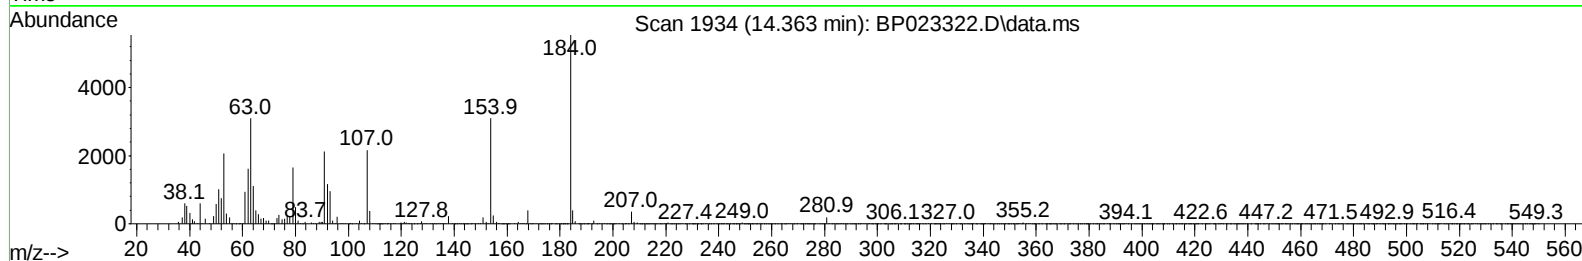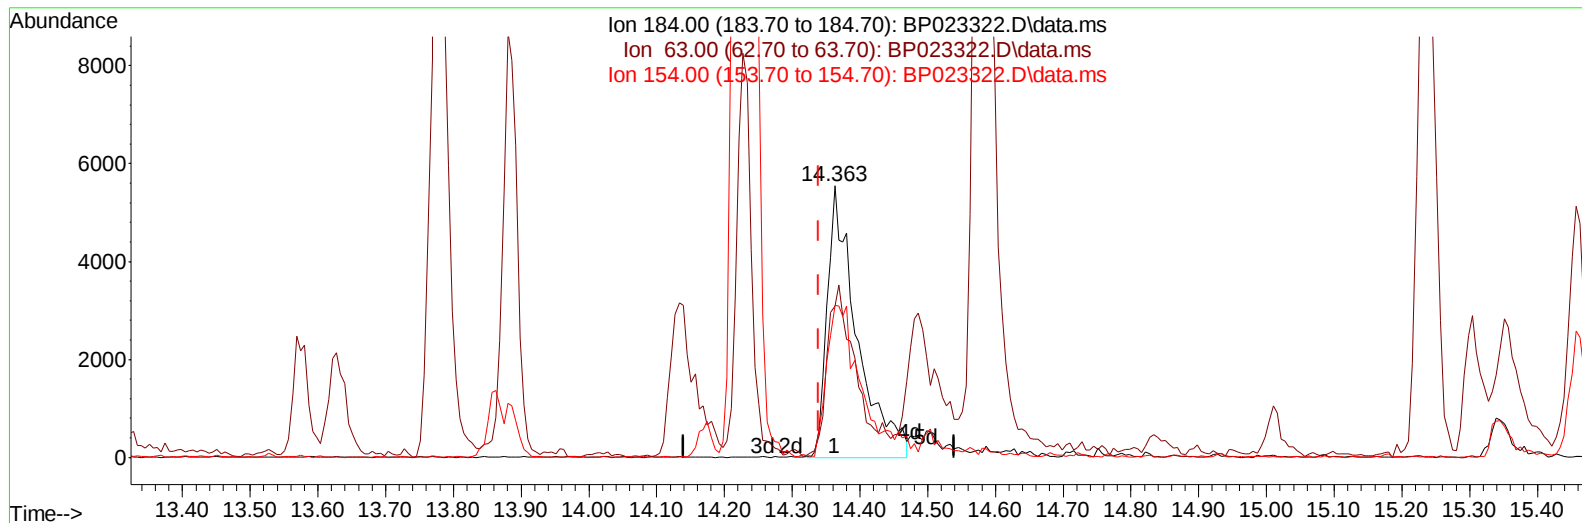

TIC: BP023322.D\data.ms

(53) 2,4-Dinitrophenol

14.363min (+ 0.023) 7.78 ng/ul m

response 16792

Ion	Exp%	Act%
184.00	100.00	100.00
63.00	63.00	55.86
154.00	72.40	55.92#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112624\
Data File : BP023322.D
Acq On : 26 Nov 2024 14:16
Operator : RC/JU
Sample : SSTD01056
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SSTD010636

Manual IntegrationsAPPROVED

Quant Time: Nov 26 23:24:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 26 23:16:47 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/27/2024
Supervised By :mohammad ahmed 11/27/2024

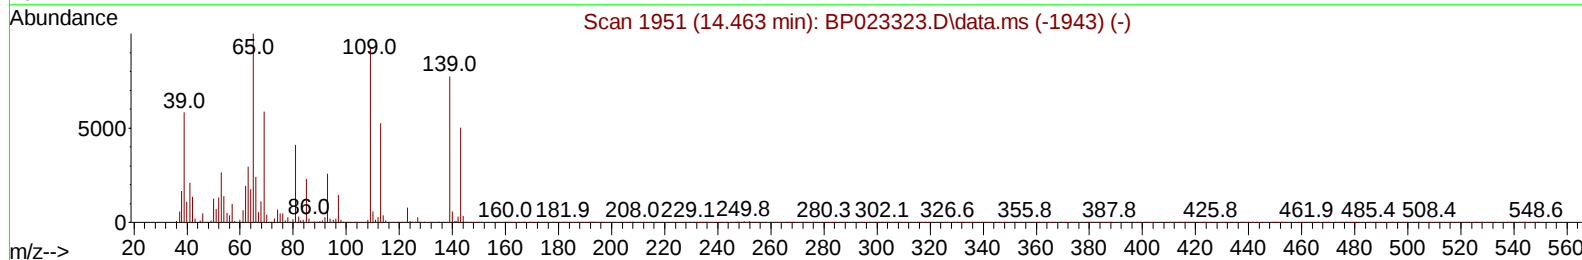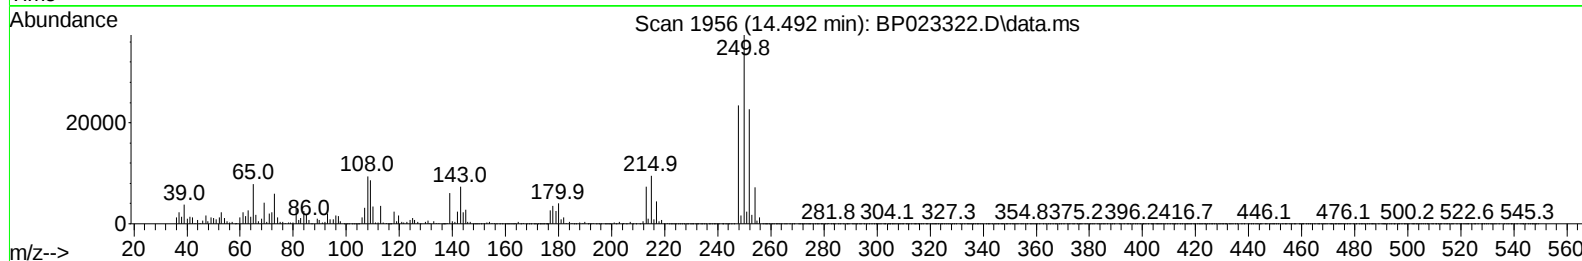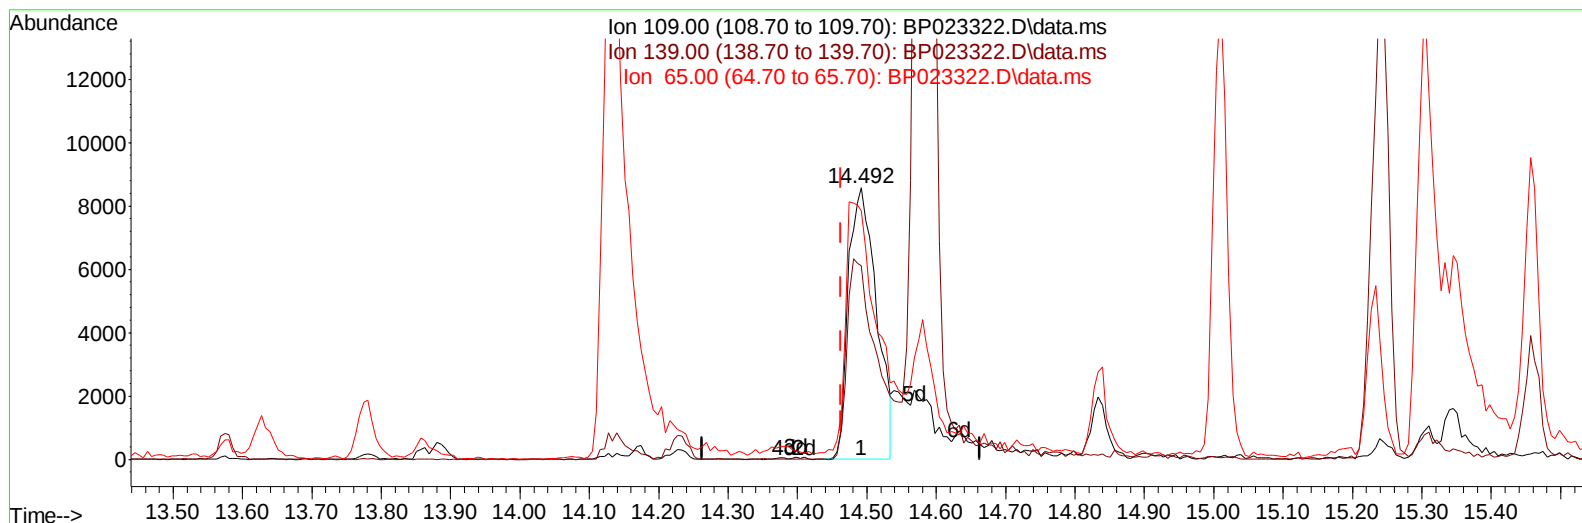

TIC: BP023322.D\data.ms

(55) 4-Nitrophenol

14.492min (+ 0.029) 8.61 ng/u1

response 24002

Ion	Exp%	Act%
109.00	100.00	100.00
139.00	83.40	71.30
65.00	107.60	91.70
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112624\
Data File : BP023322.D
Acq On : 26 Nov 2024 14:16
Operator : RC/JU
Sample : SSTD01056
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SSTD010636

Manual IntegrationsAPPROVED

Quant Time: Nov 26 23:24:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 26 23:16:47 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/27/2024
Supervised By :mohammad ahmed 11/27/2024

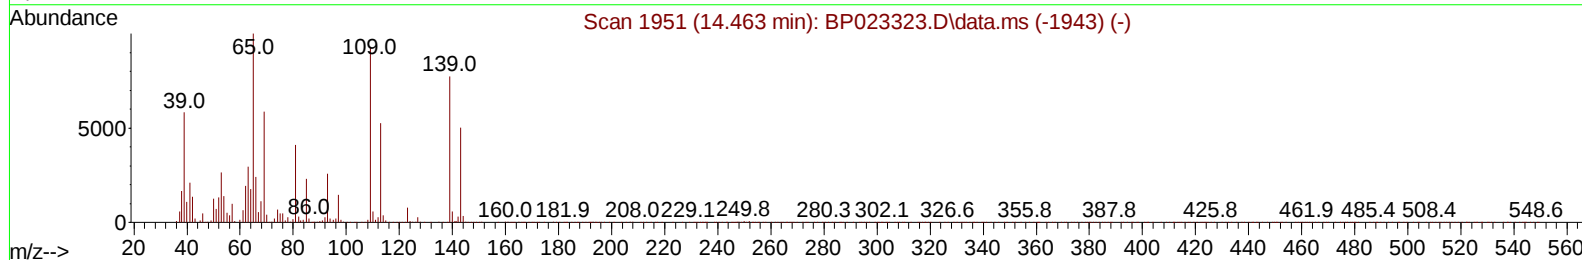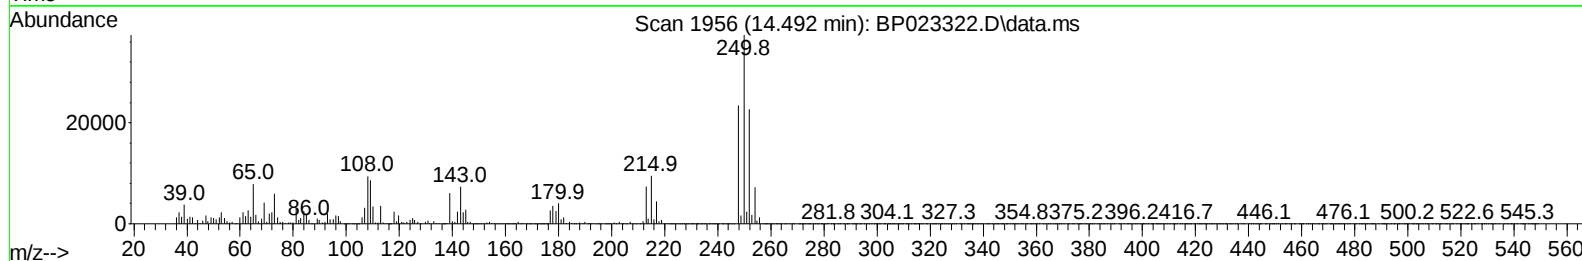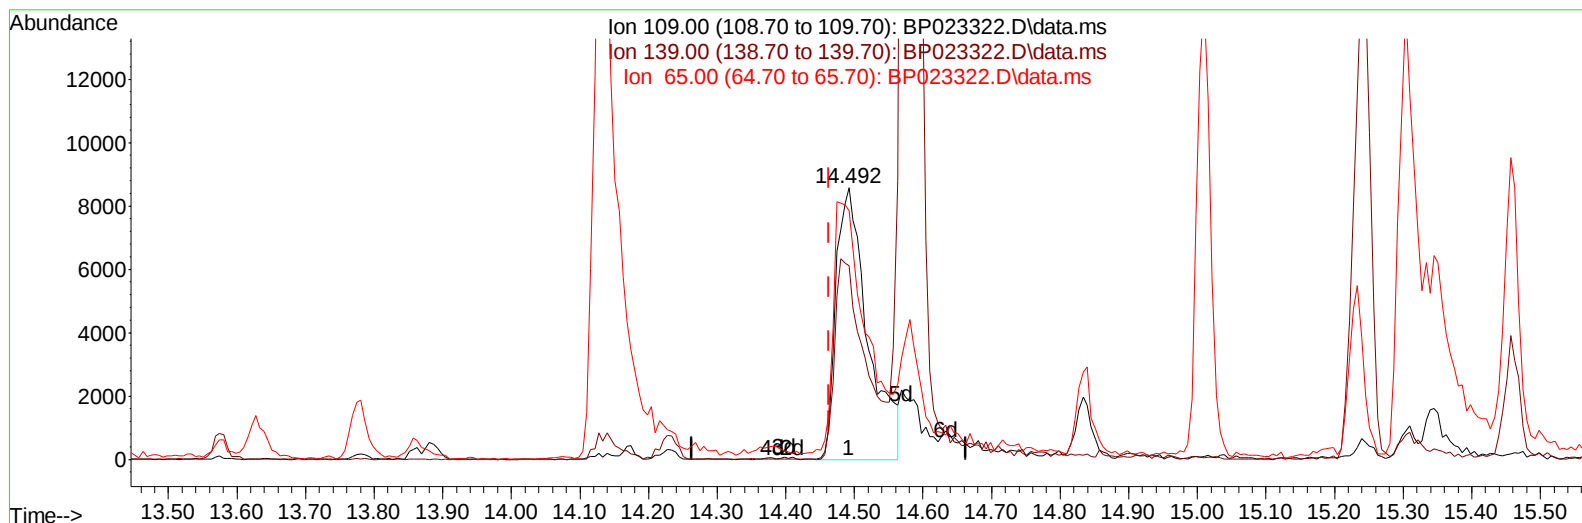

TIC: BP023322.D\data.ms

(55) 4-Nitrophenol

14.492min (+ 0.029) 9.86 ng/ul m

response 27485

Ion	Exp%	Act%
109.00	100.00	100.00
139.00	83.40	71.30
65.00	107.60	91.70
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112624\
Data File : BP023322.D
Acq On : 26 Nov 2024 14:16
Operator : RC/JU
Sample : SSTD01056
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SSTD010636

Manual IntegrationsAPPROVED

Quant Time: Nov 26 23:24:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 26 23:16:47 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/27/2024
Supervised By :mohammad ahmed 11/27/2024

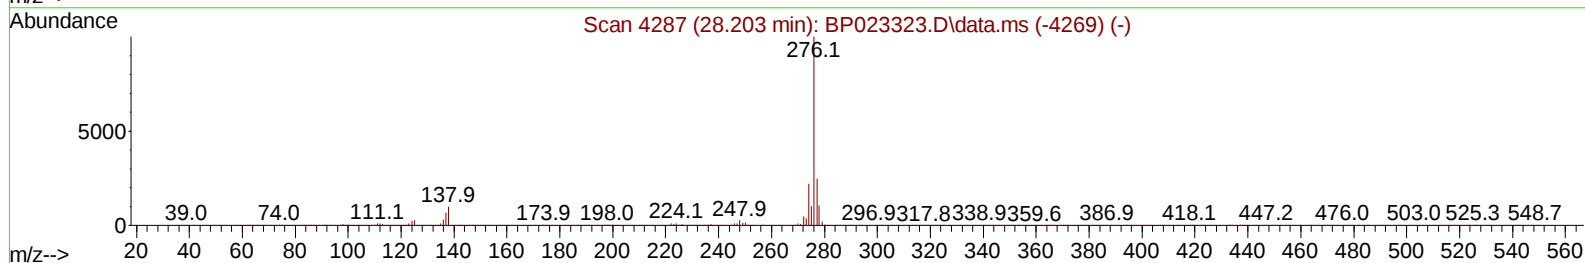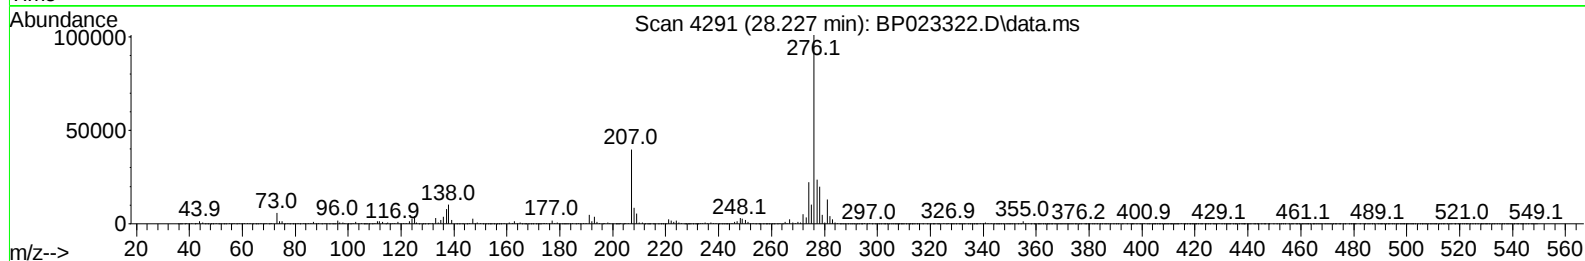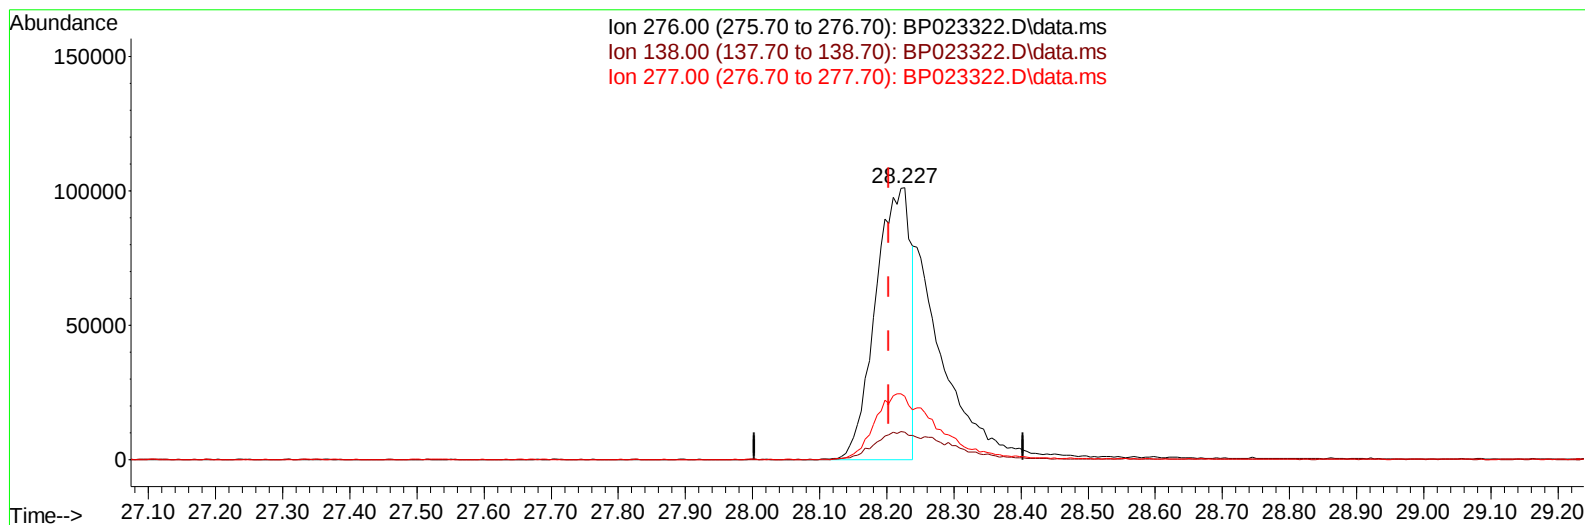

TIC: BP023322.D\data.ms

(94) Indeno(1,2,3-cd)pyrene

28.227min (+ 0.023) 6.73 ng/u1

response 369196

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	9.70	10.10
277.00	24.80	23.25
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112624\
Data File : BP023322.D
Acq On : 26 Nov 2024 14:16
Operator : RC/JU
Sample : SSTD01056
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SSTD010636

Manual IntegrationsAPPROVED

Quant Time: Nov 26 23:24:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 26 23:16:47 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/27/2024
Supervised By :mohammad ahmed 11/27/2024

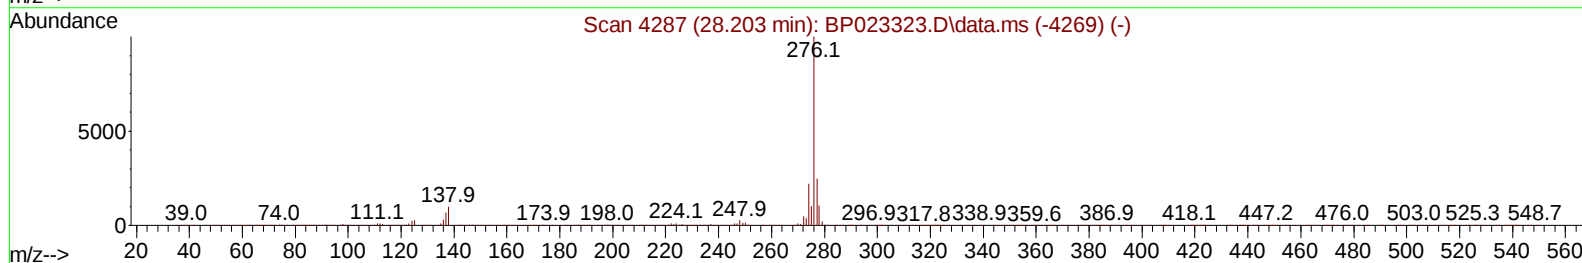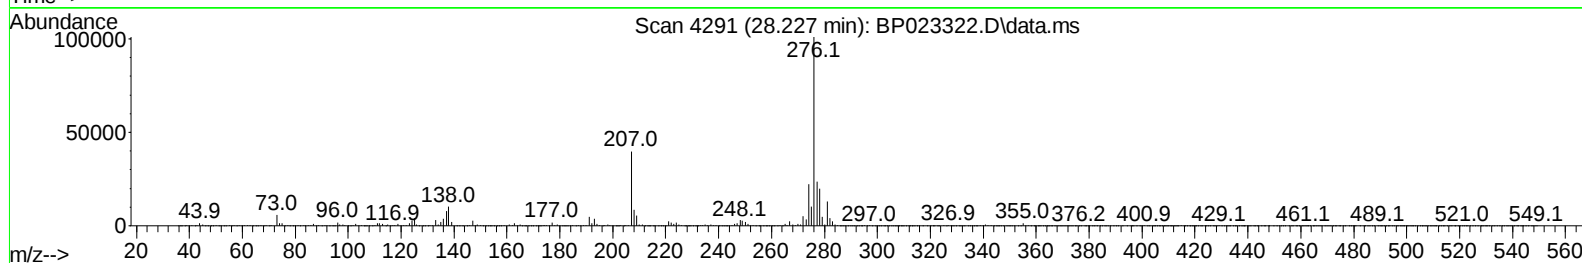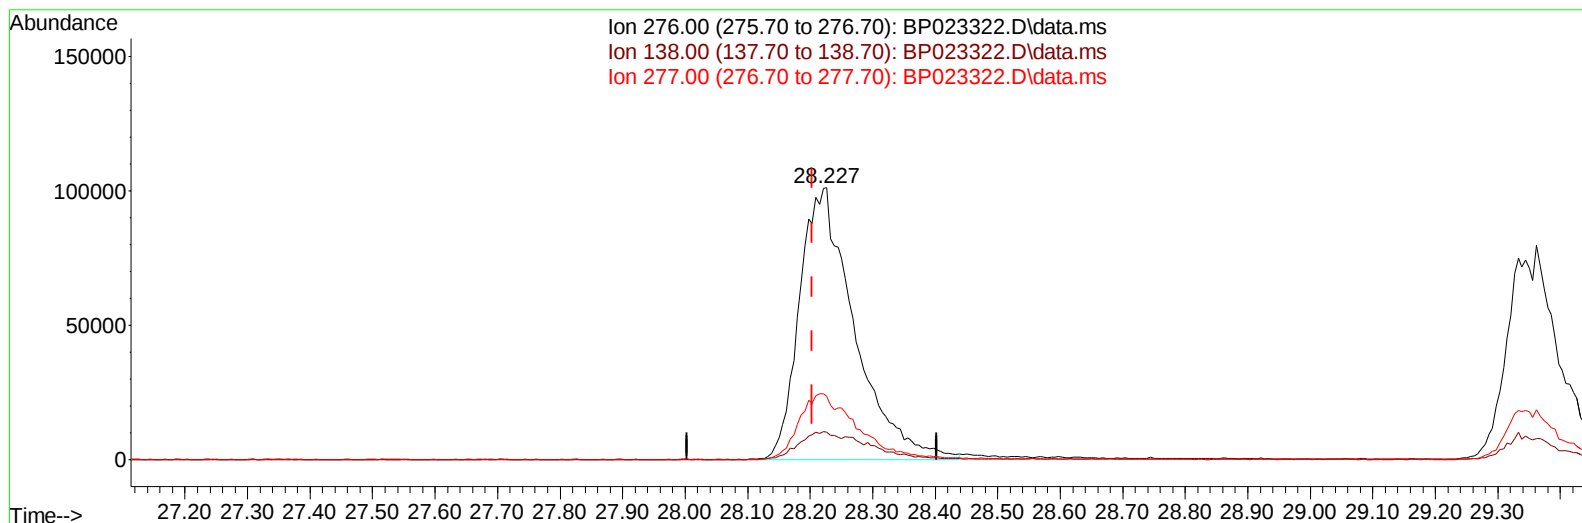

TIC: BP023322.D\data.ms

(94) Indeno(1,2,3-cd)pyrene

28.227min (+ 0.023) 11.25 ng/ul m

response 616859

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	9.70	10.10
277.00	24.80	23.25
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112624\
 Data File : BP023322.D
 Acq On : 26 Nov 2024 14:16
 Operator : RC/JU
 Sample : SSTD010636
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD010636

Manual IntegrationsAPPROVED

Quant Time: Nov 26 23:24:52 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 26 23:16:47 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/27/2024
 Supervised By :mohammad ahmed 11/27/2024

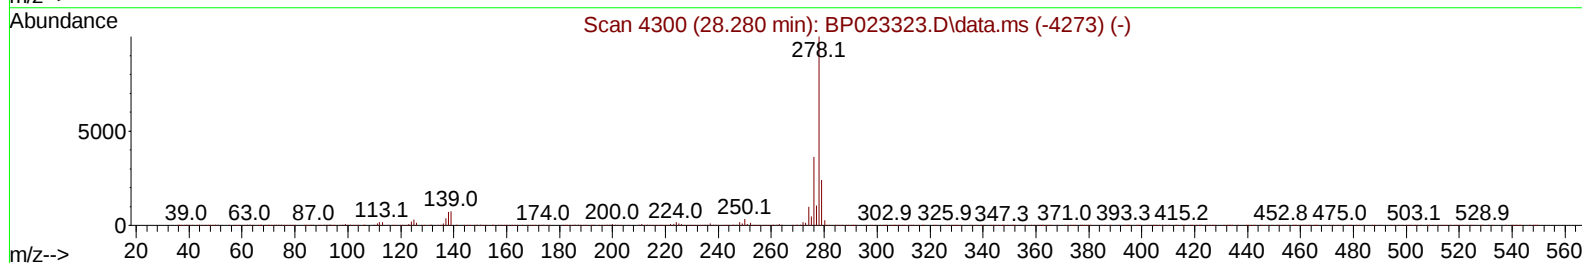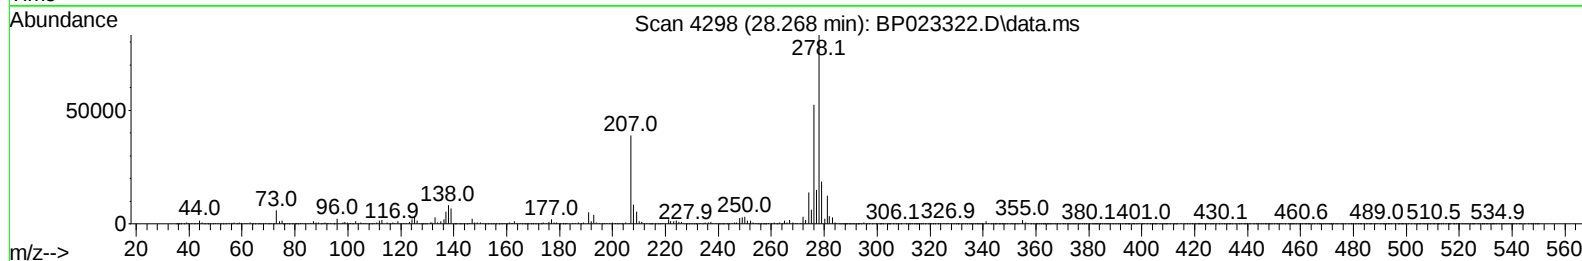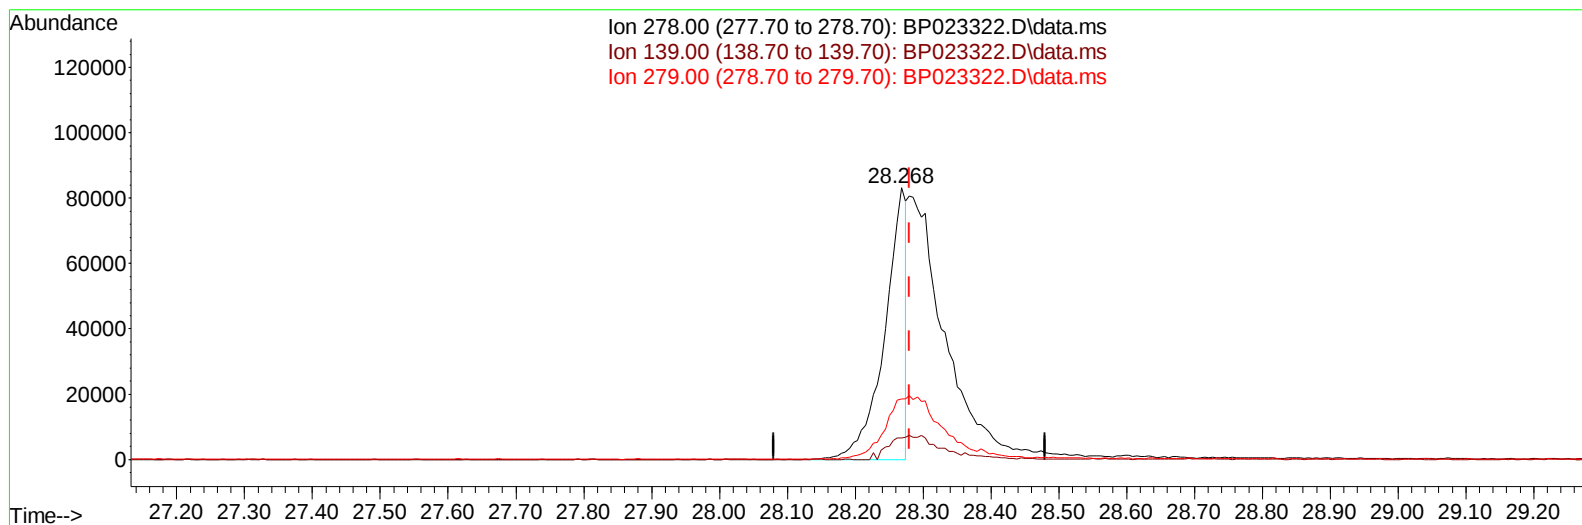

TIC: BP023322.D\data.ms

(95) Dibenzo(a,h)anthracene

28.268min (-0.012) 4.09 ng/u1

response 181972

Ion	Exp%	Act%
278.00	100.00	100.00
139.00	7.50	7.98
279.00	24.00	22.38
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112624\
Data File : BP023322.D
Acq On : 26 Nov 2024 14:16
Operator : RC/JU
Sample : SSTD01056
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SSTD010636

Manual IntegrationsAPPROVED

Quant Time: Nov 26 23:24:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 26 23:16:47 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/27/2024
Supervised By :mohammad ahmed 11/27/2024

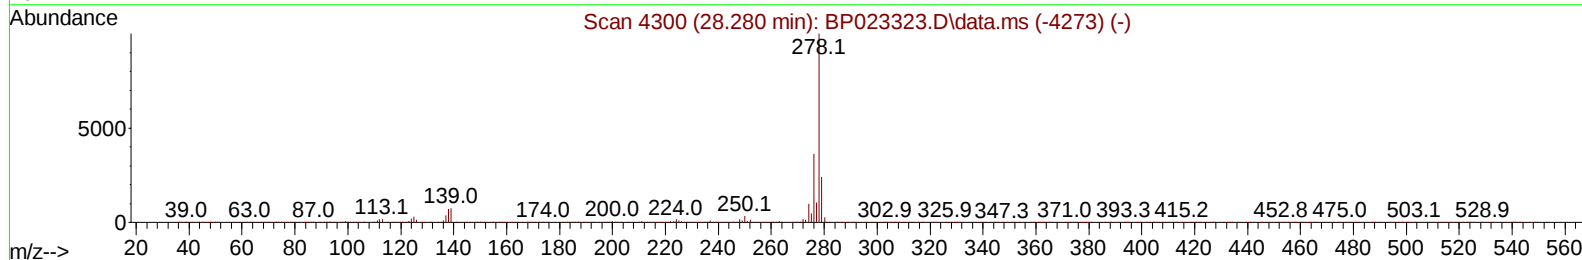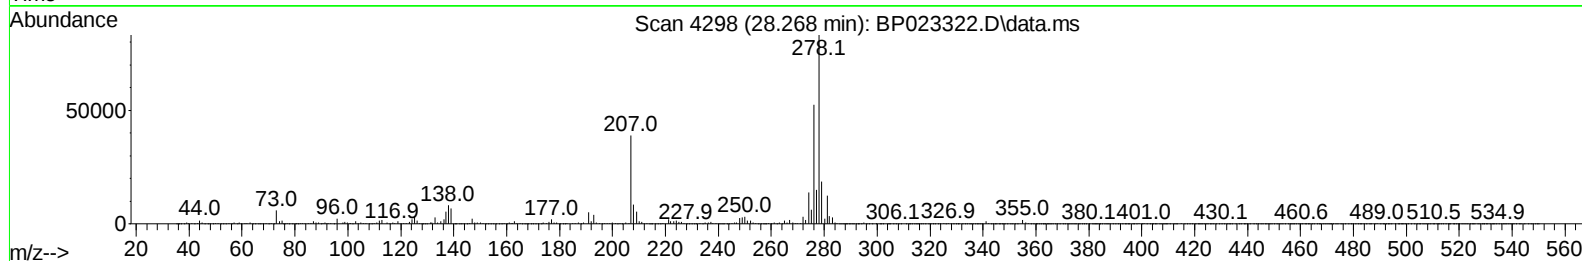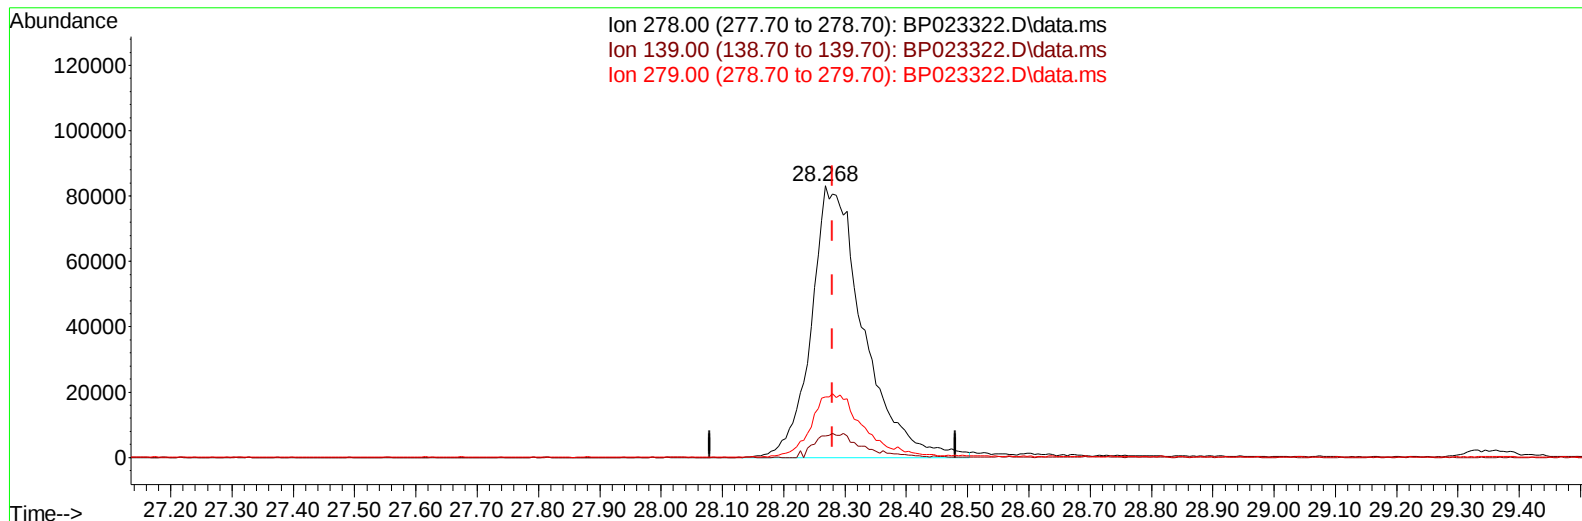

TIC: BP023322.D\data.ms

(95) Dibenzo(a,h)anthracene

28.268min (-0.012) 10.99 ng/ul m

response 489391

Ion	Exp%	Act%
278.00	100.00	100.00
139.00	7.50	7.98
279.00	24.00	22.38
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112624\
Data File : BP023322.D
Acq On : 26 Nov 2024 14:16
Operator : RC/JU
Sample : SSTD01056
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SSTD010636

Manual IntegrationsAPPROVED

Quant Time: Nov 26 23:24:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 26 23:16:47 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/27/2024
Supervised By :mohammad ahmed 11/27/2024

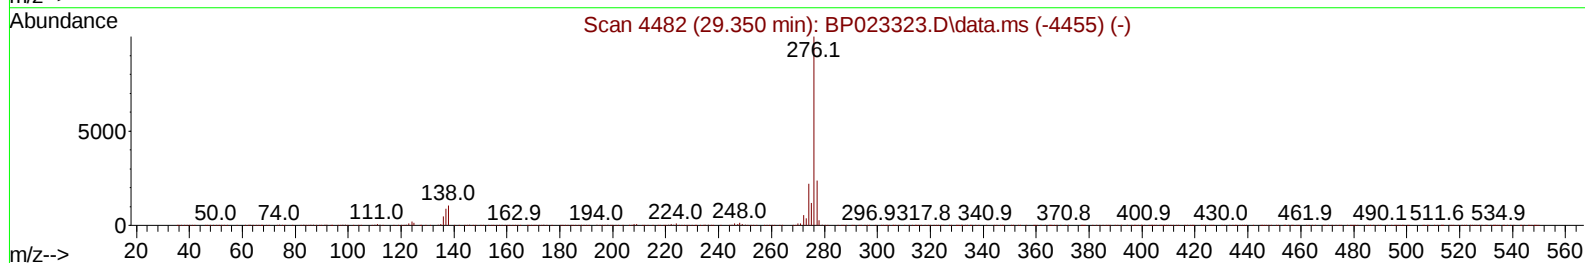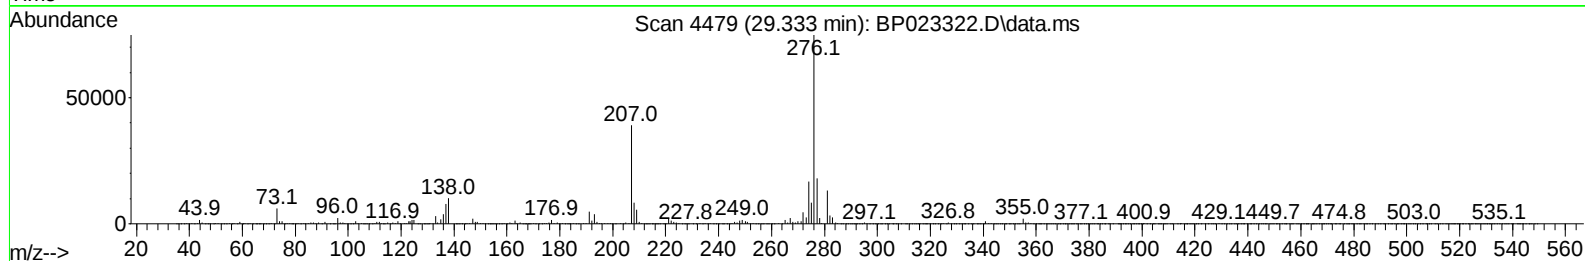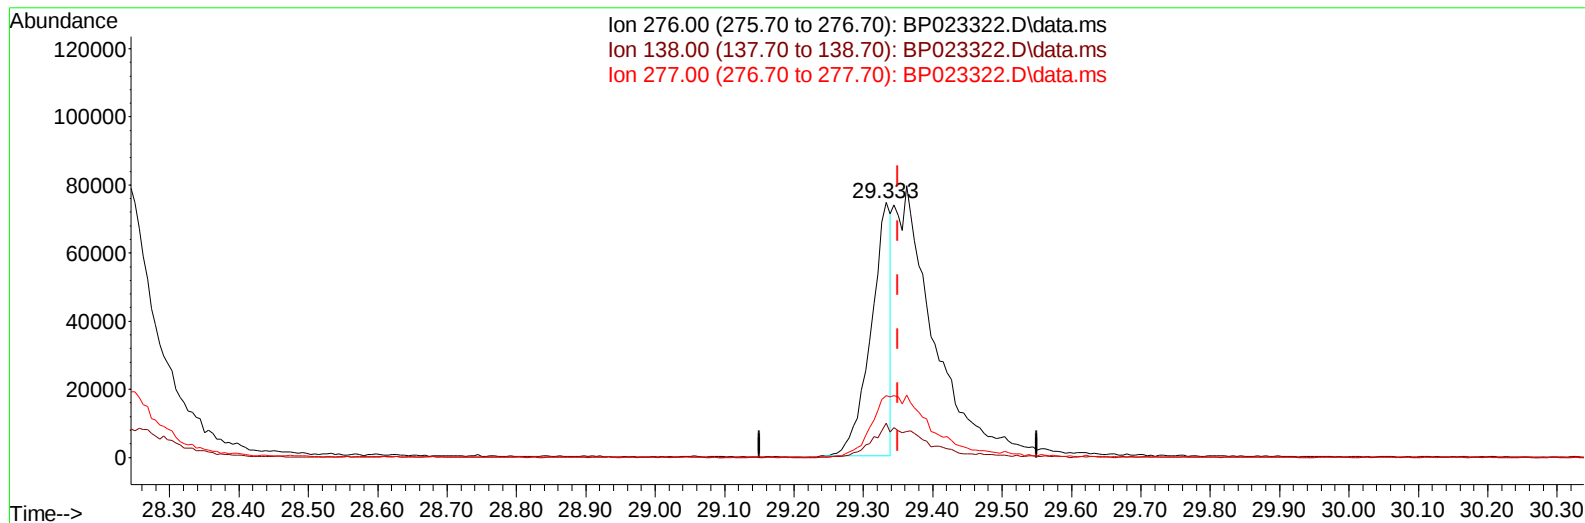

TIC: BP023322.D\data.ms

(96) Benzo(g,h,i)perylene

29.333min (-0.018) 3.57 ng/u1

response 148718

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	10.60	13.55#
277.00	23.60	24.23
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112624\
Data File : BP023322.D
Acq On : 26 Nov 2024 14:16
Operator : RC/JU
Sample : SSTD01056
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SSTD010636

Manual IntegrationsAPPROVED

Quant Time: Nov 26 23:24:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 26 23:16:47 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/27/2024
Supervised By :mohammad ahmed 11/27/2024

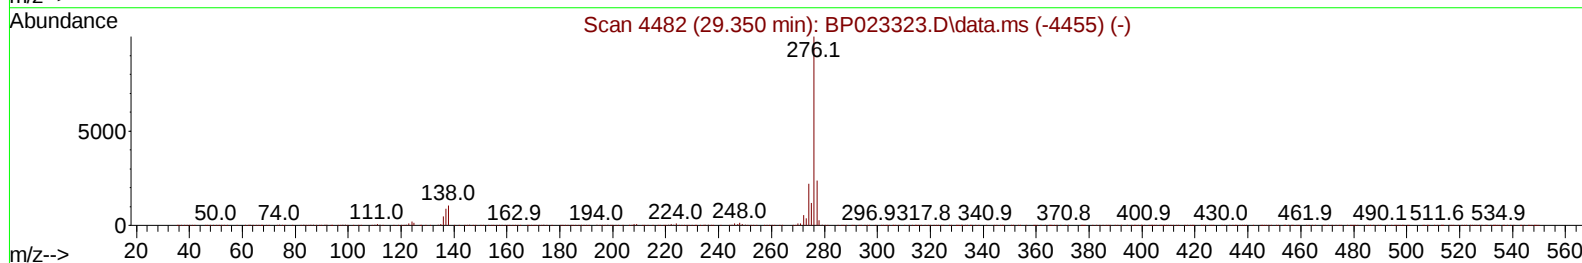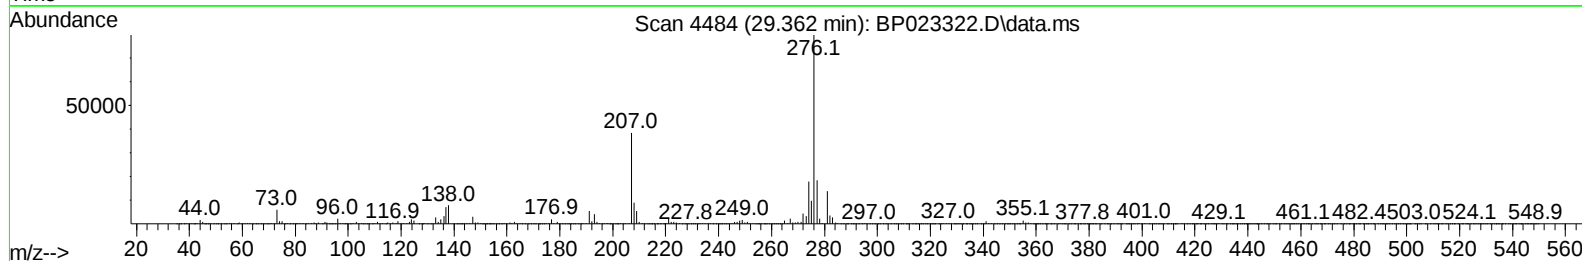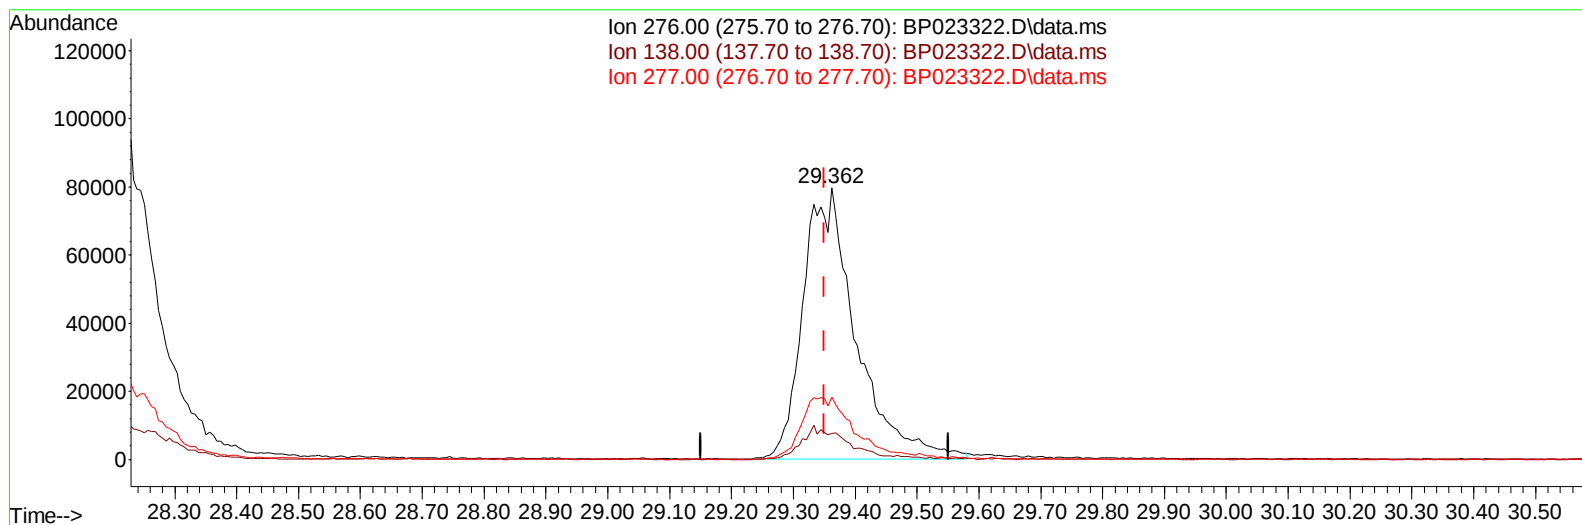

TIC: BP023322.D\data.ms

(96) Benzo(g,h,i)perylene

29.362min (+ 0.012) 11.35 ng/ul m

response 472760

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	10.60	9.69
277.00	23.60	23.12
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112624\
 Data File : BP023322.D
 Acq On : 26 Nov 2024 14:16
 Operator : RC/JU
 Sample : SSTD01056
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD010636

Manual IntegrationsAPPROVED

Quant Time: Nov 26 23:44:24 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 26 23:16:47 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/27/2024
 Supervised By :mohammad ahmed 11/27/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.563	152	70159	20.000	ng/ul	0.00
20) Naphthalene-d8	10.304	136	278454	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.175	164	219919	20.000	ng/ul	0.00
64) Phenanthrene-d10	16.980	188	567852	20.000	ng/ul	0.00
79) Chrysene-d12	21.404	240	661949	20.000	ng/ul	0.00
88) Perylene-d12	24.609	264	782287	20.000	ng/ul	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.128	96	8376	5.739	ng/uL	0.00
4) Pyridine-d5	3.552	84	50757	11.705	ng/ul	0.00
7) Phenol-d5	6.775	99	55098	10.622	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.916	67	38361	12.588	ng/ul	0.00
11) 2-Chlorophenol-d4	7.116	132	41910	11.032	ng/ul	0.01
15) 4-Methylphenol-d8	8.281	113	45347	10.624	ng/ul	0.01
21) Nitrobenzene-d5	8.704	128	21782	11.236	ng/ul	0.00
24) 2-Nitrophenol-d4	9.422	143	24961	10.801	ng/ul	0.01
28) 2,4-Dichlorophenol-d3	9.969	165	51698	10.682	ng/ul	0.01
31) 4-Chloroaniline-d4	10.469	131	56993	9.871	ng/ul	0.02
46) Dimethylphthalate-d6	13.575	166	178712	11.275	ng/ul	0.00
49) Acenaphthylene-d8	13.857	160	194275	11.747	ng/ul	0.00
54) 4-Nitrophenol-d4	14.469	143	13340	5.600	ng/ul	0.03
60) Fluorene-d10	15.186	176	163448	11.762	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.345	200	31698	9.318	ng/ul	0.01
73) Anthracene-d10	17.074	188	270868	11.266	ng/ul	0.00
81) Pyrene-d10	19.468	212	353101	11.581	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.374	264	432396	11.604	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.163	88	9289	5.508	ng/uL	95
5) Pyridine	3.569	79	51774	11.888	ng/ul	97
6) Benzaldehyde	6.746	77	37674m	12.621	ng/ul	
8) Phenol	6.804	94	57840	10.678	ng/ul	97
10) Bis(2-Chloroethyl)ether	6.998	93	49577	12.180	ng/ul	99
12) 2-Chlorophenol	7.146	128	45585	11.558	ng/ul	98
13) 2-Methylphenol	8.016	108	43987	10.879	ng/ul	94
14) 2,2'-oxybis(1-Chloropr...	8.063	45	63145	13.704	ng/ul	97
16) Acetophenone	8.375	105	82301	11.474	ng/ul	92
17) N-Nitroso-di-n-propyla...	8.351	70	44363	12.387	ng/ul	97
18) 4-Methylphenol	8.345	108	47194	10.568	ng/ul	92
19) Hexachloroethane	8.604	117	22398	11.742	ng/ul	94
22) Nitrobenzene	8.745	77	68252	12.270	ng/ul	94
23) Isophorone	9.263	82	120676	12.133	ng/ul	100
25) 2-Nitrophenol	9.451	139	27101	11.110	ng/ul	99
26) 2,4-Dimethylphenol	9.522	107	60442	11.475	ng/ul	96
27) Bis(2-Chloroethoxy)met...	9.734	93	66432	12.139	ng/ul	98
29) 2,4-Dichlorophenol	9.992	162	52167	10.882	ng/ul	99
30) Naphthalene	10.351	128	157913	11.673	ng/ul	99
32) 4-Chloroaniline	10.492	127	57442	10.269	ng/ul	99
33) Hexachlorobutadiene	10.628	225	48118	11.093	ng/ul	96
34) Caprolactam	11.286	113	14283m	10.017	ng/ul	
35) 4-Chloro-3-methylphenol	11.634	107	56300	10.917	ng/ul	98

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112624\
 Data File : BP023322.D
 Acq On : 26 Nov 2024 14:16
 Operator : RC/JU
 Sample : SST001056
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SST0010636

Manual IntegrationsAPPROVED

Quant Time: Nov 26 23:44:24 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 26 23:16:47 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/27/2024
 Supervised By :mohammad ahmed 11/27/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
36) 2-Methylnaphthalene	11.975	142	114536	11.215	ng/ul	99
37) 1-Methylnaphthalene	12.186	142	117773	11.280	ng/ul	96
39) 1,2,4,5-Tetrachloroben...	12.351	216	87502	11.786	ng/ul	93
40) Hexachlorocyclopentadiene	12.316	237	32478	8.328	ng/ul	97
41) 2,4,6-Trichlorophenol	12.610	196	49298	10.904	ng/ul	97
42) 2,4,5-Trichlorophenol	12.704	196	52188	10.708	ng/ul	98
43) 1,1'-Biphenyl	12.998	154	166783	11.835	ng/ul	97
44) 2-Chloronaphthalene	13.045	162	134209	11.651	ng/ul	98
45) 2-Nitroaniline	13.269	65	36309	11.226	ng/ul	94
47) Dimethylphthalate	13.628	163	179614	11.490	ng/ul	99
48) 2,6-Dinitrotoluene	13.780	165	32610	10.725	ng/ul	98
50) Acenaphthylene	13.886	152	195273	11.681	ng/ul	99
51) 3-Nitroaniline	14.133	138	26457	10.102	ng/ul	97
52) Acenaphthene	14.227	153	144395	11.897	ng/ul	95
53) 2,4-Dinitrophenol	14.363	184	16792m	7.783	ng/ul	
55) 4-Nitrophenol	14.492	109	27485m	9.862	ng/ul	
56) Dibenzofuran	14.580	168	219729	11.718	ng/ul	98
57) 2,4-Dinitrotoluene	14.580	165	53385	11.016	ng/ul#	84
58) 2,3,4,6-Tetrachlorophenol	14.833	232	53384	11.205	ng/ul	96
59) Diethylphthalate	15.010	149	178232	11.529	ng/ul	99
61) Fluorene	15.245	166	179016	11.664	ng/ul	99
62) 4-Chlorophenyl-phenyle...	15.233	204	105332	11.655	ng/ul	97
63) 4-Nitroaniline	15.304	138	23169	9.507	ng/ul	88
66) 4,6-Dinitro-2-methylph...	15.357	198	33817	9.306	ng/ul#	88
67) N-Nitrosodiphenylamine	15.457	169	154296	11.759	ng/ul	98
68) 4-Bromophenyl-phenylether	16.145	248	71822	11.169	ng/ul	99
69) Hexachlorobenzene	16.269	284	87795	10.846	ng/ul	99
70) Atrazine	16.433	200	67137	10.585	ng/ul	99
71) Pentachlorophenol	16.639	266	44678	8.890	ng/ul	93
72) Phenanthrene	17.021	178	315246	11.758	ng/ul	99
74) Anthracene	17.110	178	311094	11.541	ng/ul	100
75) 1,2,3,4-Tetrachloroben...	12.957	216	86591	11.549	ng/uL	95
76) Pentachlorobenzene	14.504	250	96595	11.284	ng/uL	100
77) Carbazole	17.410	167	249906	10.626	ng/ul	99
78) Di-n-butylphthalate	17.986	149	303641	11.635	ng/ul	99
80) Fluoranthene	19.121	202	403118	11.476	ng/ul	99
82) Pyrene	19.504	202	435596	11.544	ng/ul	99
83) Butylbenzylphthalate	20.439	149	143916	11.584	ng/ul	93
84) 3,3'-Dichlorobenzidine	21.321	252	150670	10.140	ng/ul#	98
85) Benzo(a)anthracene	21.386	228	463369	11.464	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.315	149	207646	11.761	ng/ul	99
87) Chrysene	21.457	228	454827	11.959	ng/ul	100
89) Di-n-octyl phthalate	22.527	149	370979	11.689	ng/ul	100
90) Benzo(b)fluoranthene	23.592	252	491700	11.293	ng/ul	99
91) Benzo(k)fluoranthene	23.656	252	526075	12.273	ng/ul	99
93) Benzo(a)pyrene	24.451	252	462305	11.745	ng/ul#	98
94) Indeno(1,2,3-cd)pyrene	28.227	276	616859m	11.249	ng/ul	
95) Dibenzo(a,h)anthracene	28.268	278	489391m	10.991	ng/ul	
96) Benzo(g,h,i)perylene	29.362	276	472760m	11.350	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Instrument :

BNA_P

ClientSampleId :

SSTD010636

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/27/2024

Supervised By :mohammad ahmed 11/27/2024

