

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112921\
 Data File : BP008150.D
 Acq On : 29 Nov 2021 19:54
 Operator : CG/JU
 Sample : M4818-01 5X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 TR-04-112321

Quant Time: Nov 30 00:06:26 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 25 01:13:46 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.805	152	114910	20.000	ng	-0.01
21) Naphthalene-d8	10.605	136	438897	20.000	ng	0.00
39) Acenaphthene-d10	14.451	164	285389	20.000	ng	0.00
64) Phenanthrene-d10	17.210	188	611313	20.000	ng	0.00
76) Chrysene-d12	21.310	240	594261	20.000	ng	0.00
86) Perylene-d12	23.704	264	630374	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.399	112	138958	19.470	ng	0.00
7) Phenol-d6	6.987	99	182195	18.911	ng	-0.01
23) Nitrobenzene-d5	8.963	82	118833	12.312	ng	-0.01
42) 2,4,6-Tribromophenol	15.945	330	68840	18.872	ng	-0.01
45) 2-Fluorobiphenyl	13.069	172	264683	13.471	ng	-0.01
79) Terphenyl-d14	19.775	244	423400	14.890	ng	-0.01
Target Compounds						
9) Benzaldehyde	6.946	77	255	Below Cal	#	35
78) Pyrene	19.580	202	4737	Below Cal	#	66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112921\
Data File : BP008150.D
Acq On : 29 Nov 2021 19:54
Operator : CG/JU
Sample : M4818-01 5X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
TR-04-112321

Quant Time: Nov 30 00:06:26 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 25 01:13:46 2021
Response via : Initial Calibration




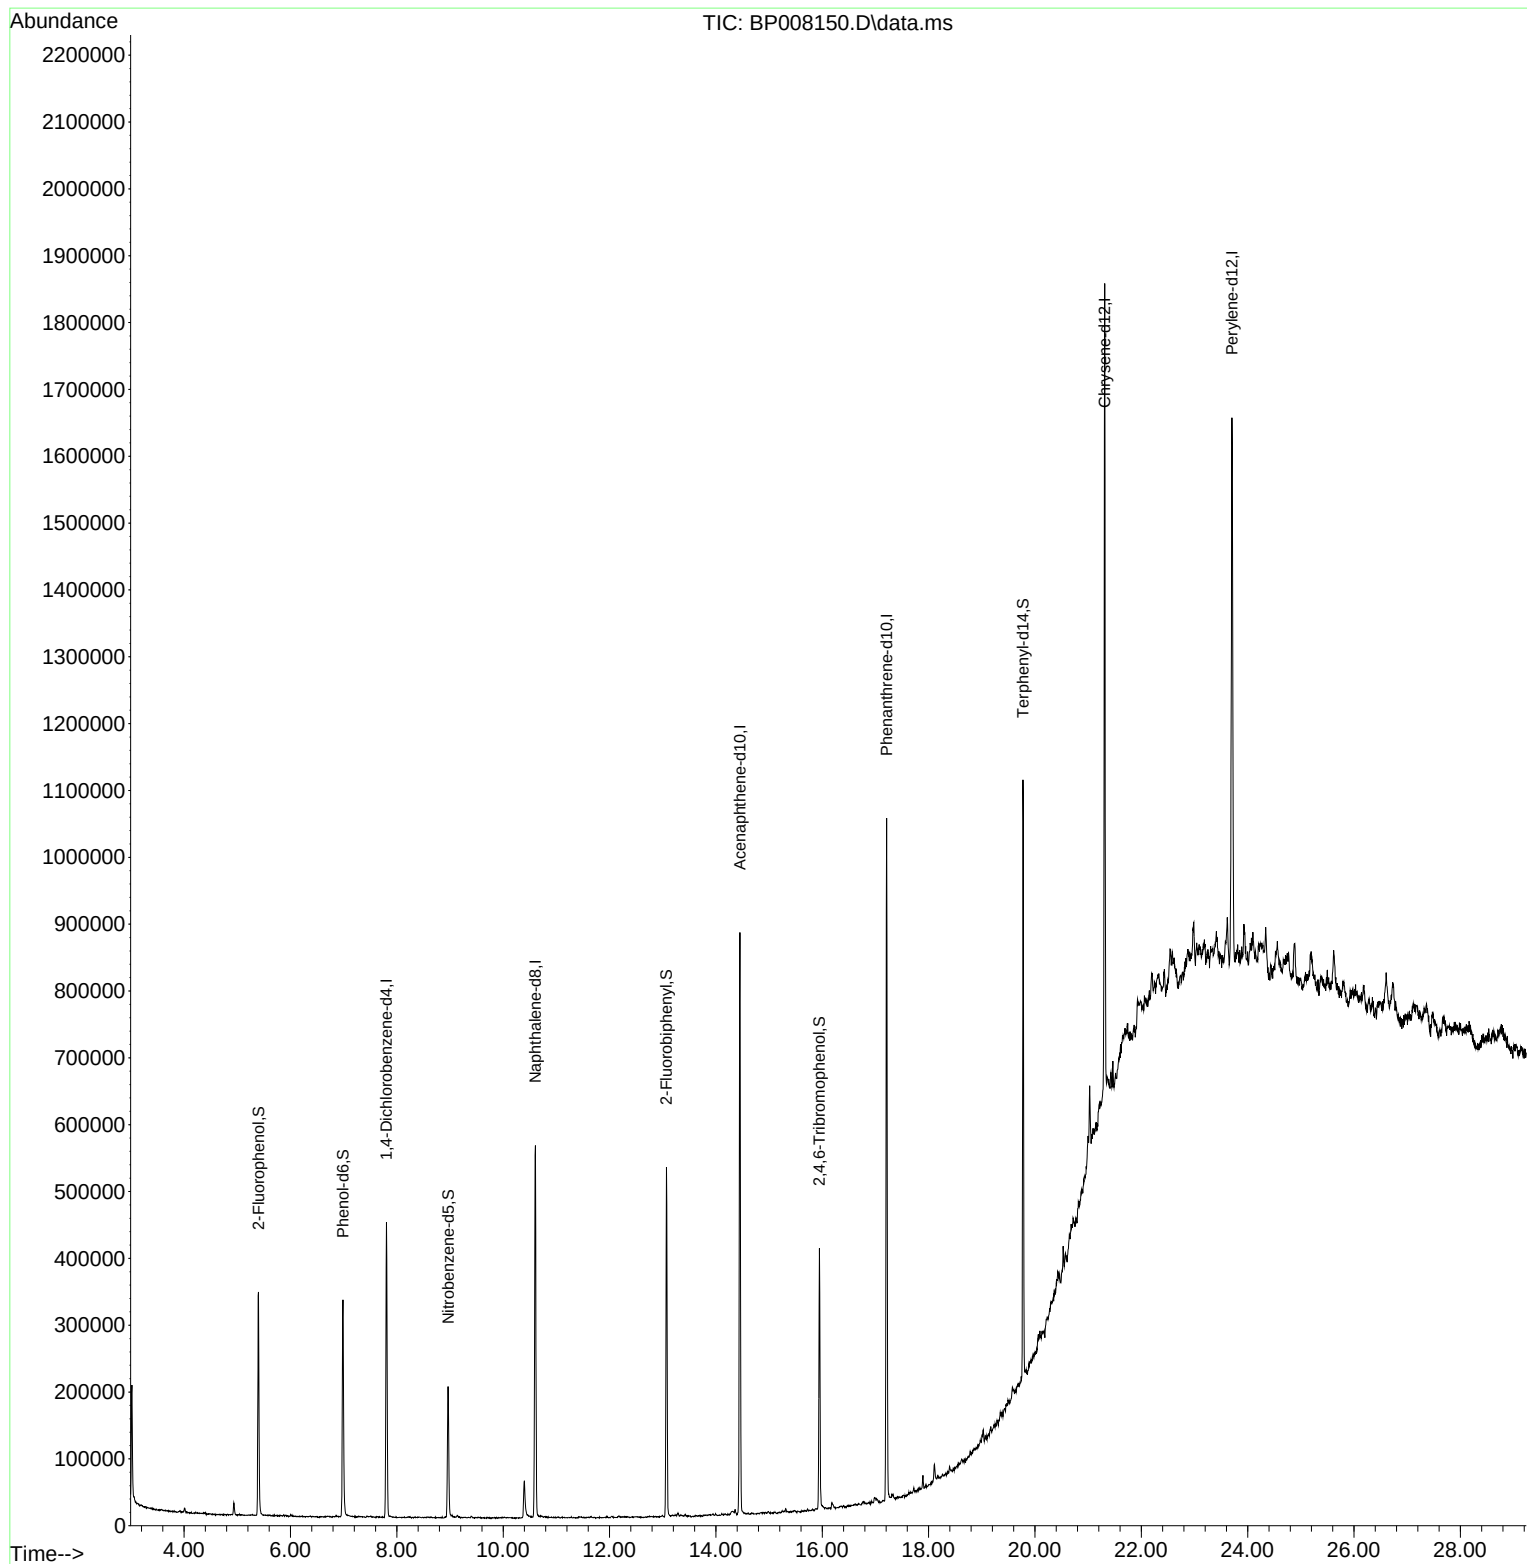


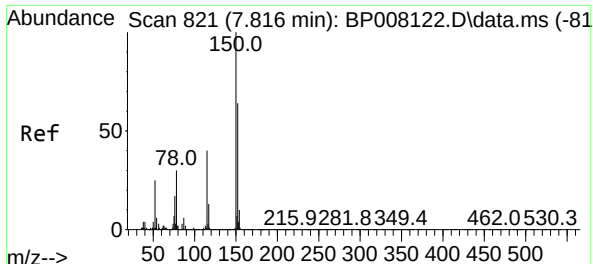

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.805 min Scan# 81
Delta R.T. -0.011 min
Lab File: BP008150.D
Acq: 29 Nov 2021 19:54




Instrument :
BNA_P
ClientSampleId :
TR-04-112321


Tgt Ion:152 Resp: 114910
Ion Ratio Lower Upper
152 100
150 156.2 125.7 188.5
115 63.7 50.7 76.1

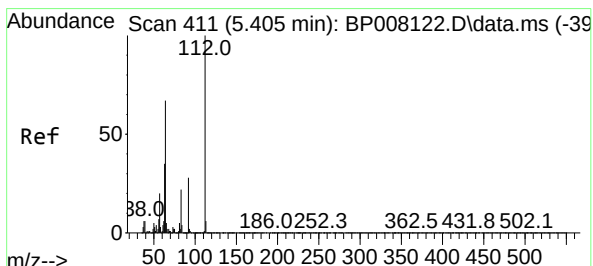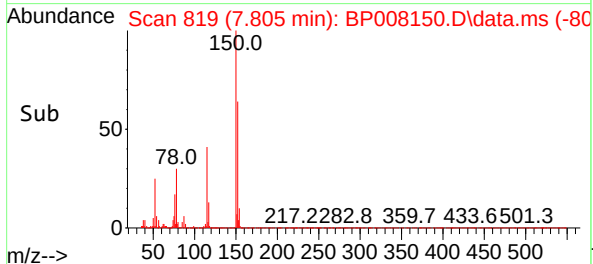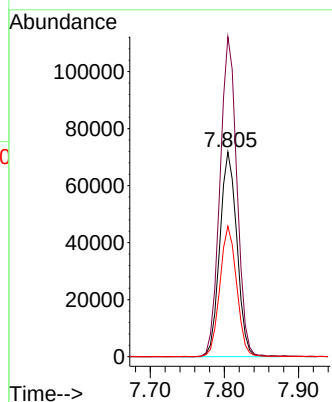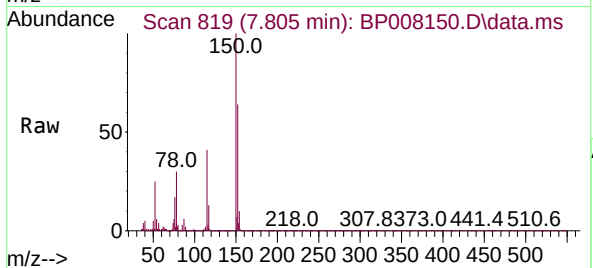

#5
2-Fluorophenol
Concen: 19.470 ng
RT: 5.399 min Scan# 410
Delta R.T. -0.006 min
Lab File: BP008150.D
Acq: 29 Nov 2021 19:54

Tgt Ion:112 Resp: 138958
Ion Ratio Lower Upper
112 100
64 67.9 53.4 80.2
63 35.5 27.8 41.8


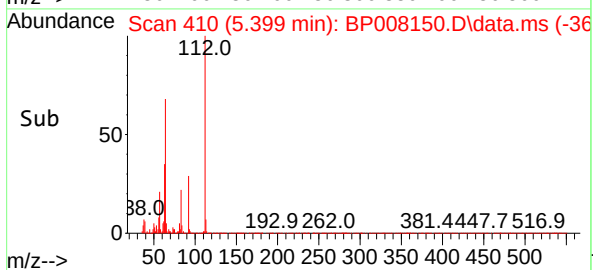
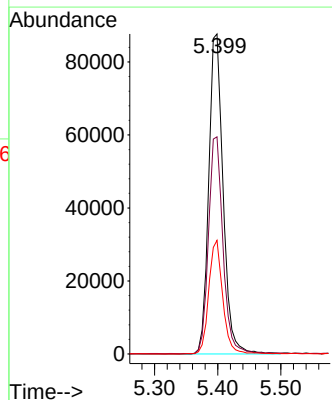
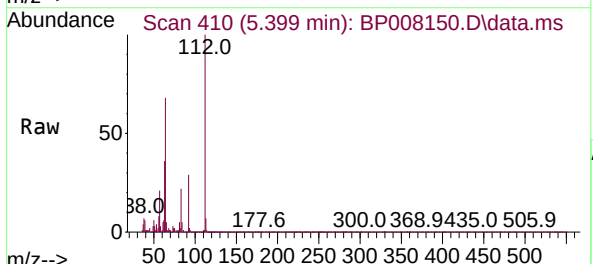


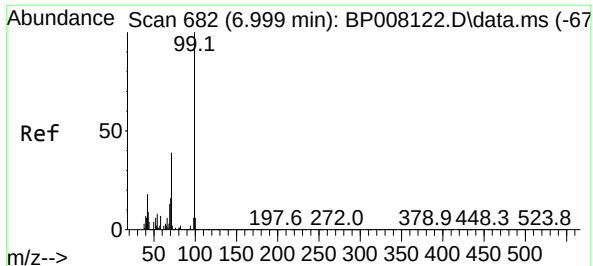

#7
Phenol-d6
Concen: 18.911 ng
RT: 6.987 min Scan# 61
Delta R.T. -0.012 min
Lab File: BP008150.D
Acq: 29 Nov 2021 19:54




Instrument :
BNA_P
ClientSampleId :
TR-04-112321


Tgt Ion: 99 Resp: 182195
Ion Ratio Lower Upper
99 100
42 19.3 14.6 22.0
71 41.2 31.1 46.7

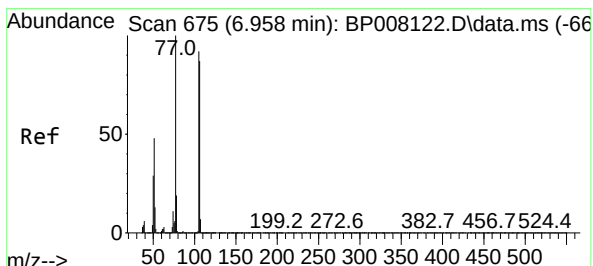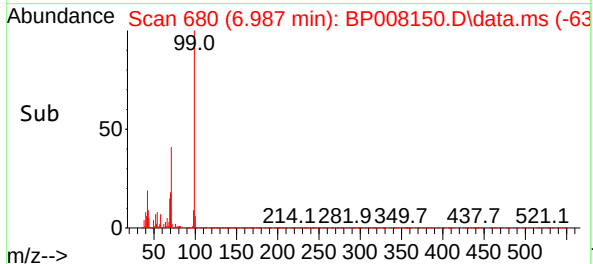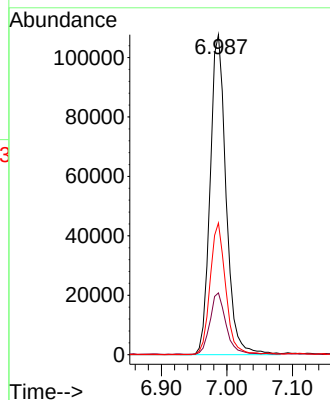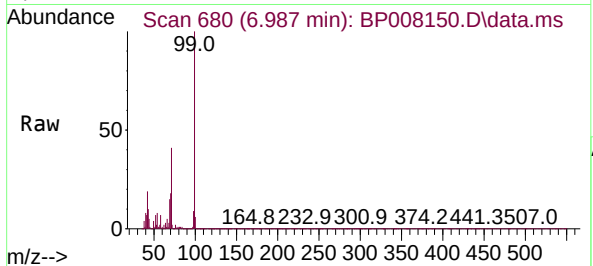

#9
Benzaldehyde
Concen: Below Cal
RT: 6.946 min Scan# 673
Delta R.T. -0.012 min
Lab File: BP008150.D
Acq: 29 Nov 2021 19:54

Tgt Ion: 77 Resp: 255
Ion Ratio Lower Upper
77 100
105 36.6 71.8 111.8#
106 19.5 67.3 107.3#


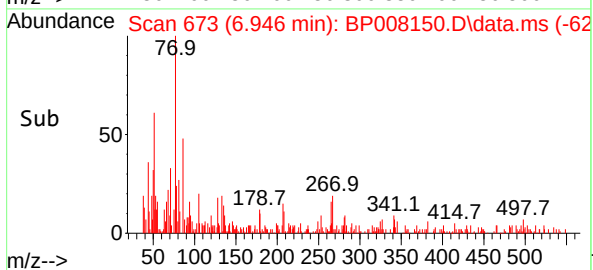
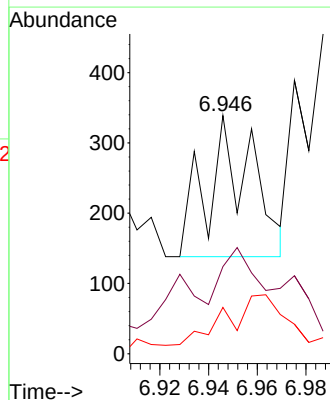
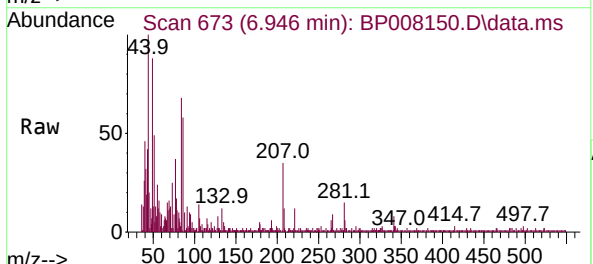


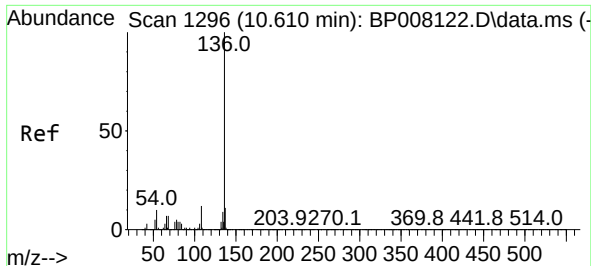

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.605 min Scan# 1016
Delta R.T. -0.006 min
Lab File: BP008150.D
Acq: 29 Nov 2021 19:54




Instrument :
BNA_P
ClientSampleId :
TR-04-112321


Tgt Ion:	136	Resp:	438897
Ion	Ratio	Lower	Upper
136	100		
137	11.0	9.0	13.6
54	9.6	8.2	12.4
68	6.6	5.8	8.8

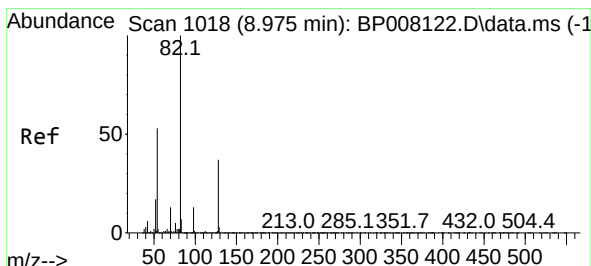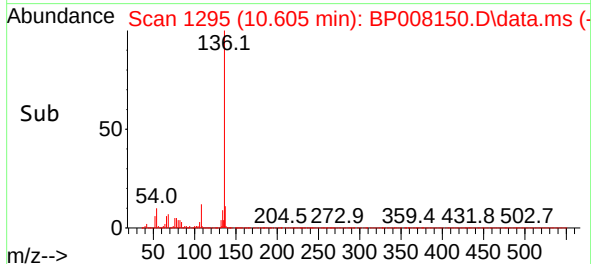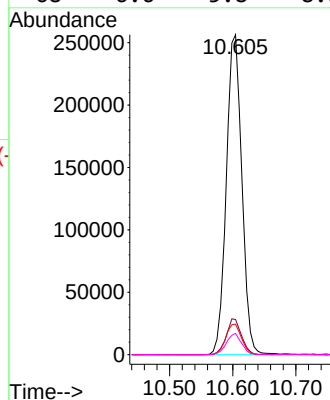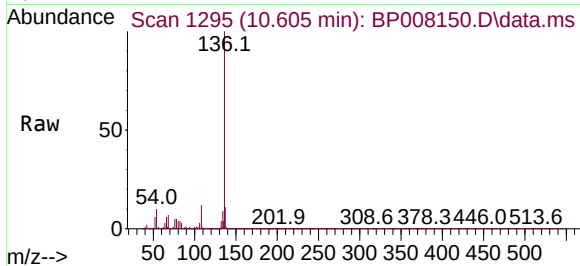

#23
Nitrobenzene-d5
Concen: 12.312 ng
RT: 8.963 min Scan# 1016
Delta R.T. -0.012 min
Lab File: BP008150.D
Acq: 29 Nov 2021 19:54

Tgt Ion:	82	Resp:	118833
Ion	Ratio	Lower	Upper
82	100		
128	36.1	29.6	44.4
54	55.6	42.7	64.1


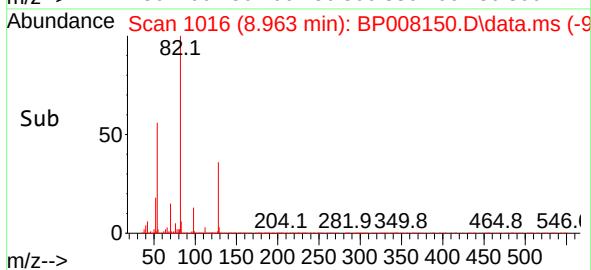
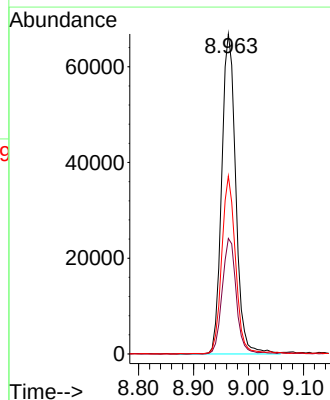
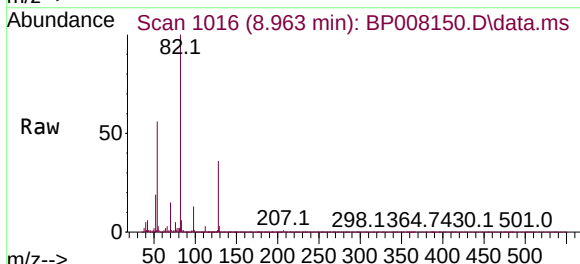


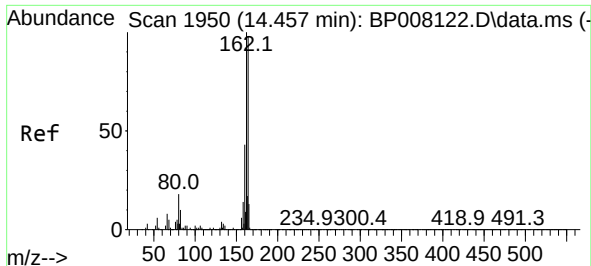

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.451 min Scan# 1949
Delta R.T. -0.006 min
Lab File: BP008150.D
Acq: 29 Nov 2021 19:54




Instrument :
BNA_P
ClientSampleId :
TR-04-112321


Tgt Ion:164 Resp: 285389
Ion Ratio Lower Upper
164 100
162 104.4 81.9 122.9
160 46.2 35.4 53.0

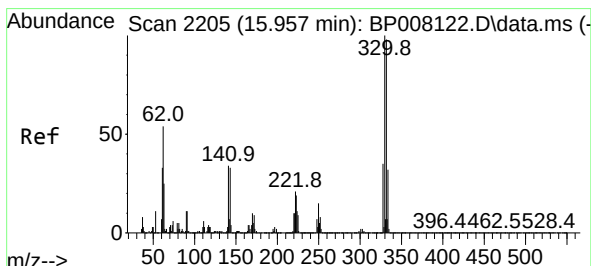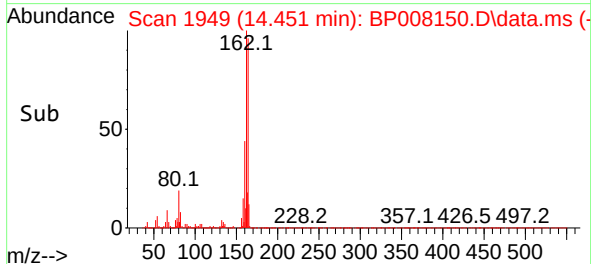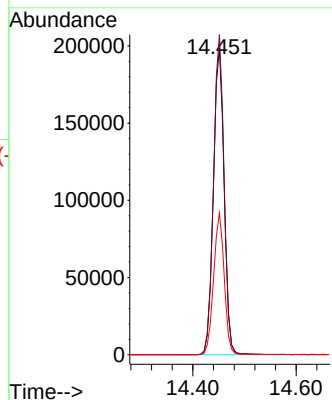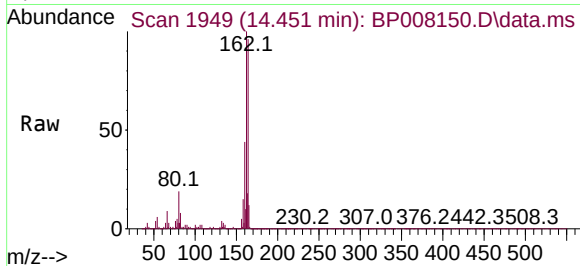

#42
2,4,6-Tribromophenol
Concen: 18.872 ng
RT: 15.945 min Scan# 2203
Delta R.T. -0.012 min
Lab File: BP008150.D
Acq: 29 Nov 2021 19:54

Tgt Ion:330 Resp: 68840
Ion Ratio Lower Upper
330 100
332 96.4 77.0 115.4
141 35.4 28.4 42.6


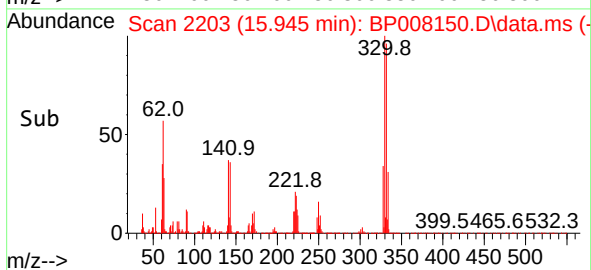
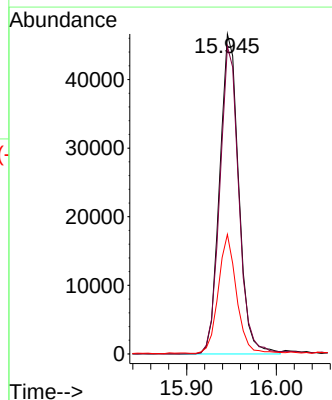
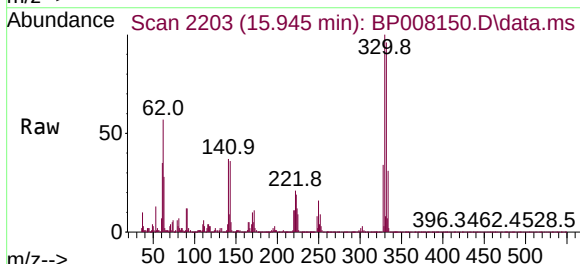


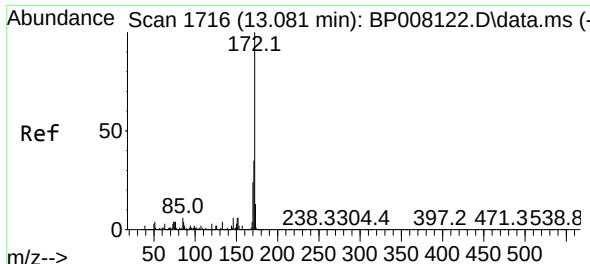

#45
2-Fluorobiphenyl
Concen: 13.471 ng
RT: 13.069 min Scan# 1
Delta R.T. -0.012 min
Lab File: BP008150.D
Acq: 29 Nov 2021 19:54




Instrument :
BNA_P
ClientSampleId :
TR-04-112321


Tgt Ion:172 Resp: 264683
Ion Ratio Lower Upper
172 100
171 34.4 28.0 42.0
170 23.6 18.9 28.3

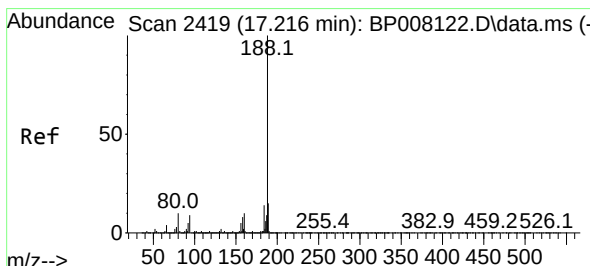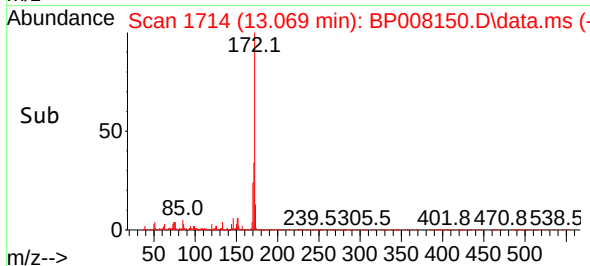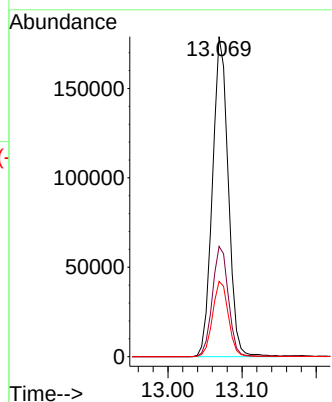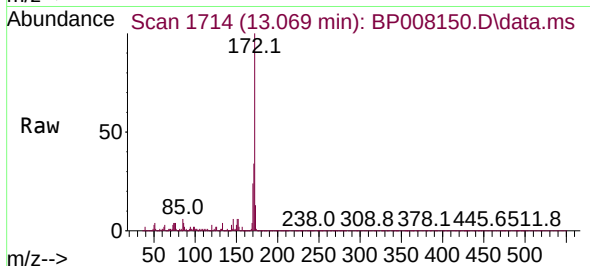

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.210 min Scan# 2418
Delta R.T. -0.006 min
Lab File: BP008150.D
Acq: 29 Nov 2021 19:54

Tgt Ion:188 Resp: 611313
Ion Ratio Lower Upper
188 100
94 8.5 7.2 10.8
80 9.4 8.2 12.4


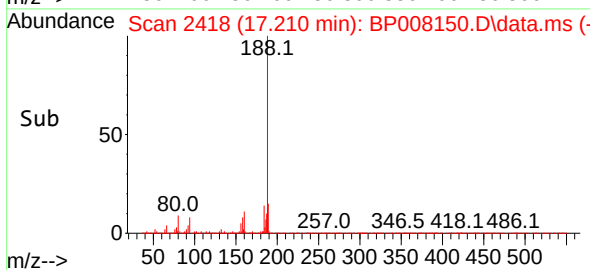
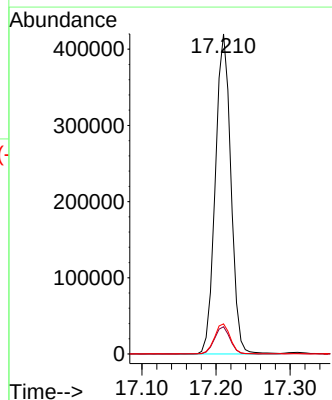
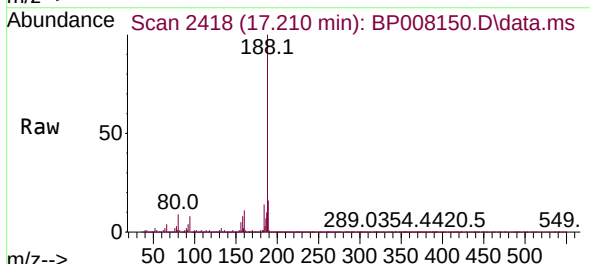


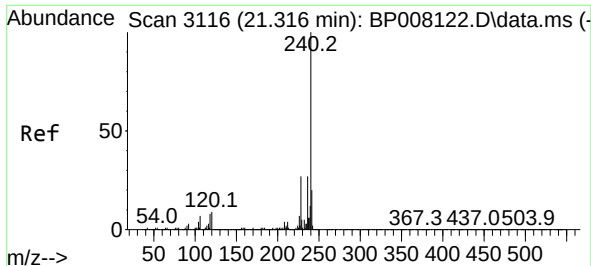

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.310 min Scan# 3115
Delta R.T. -0.006 min
Lab File: BP008150.D
Acq: 29 Nov 2021 19:54




Instrument :
BNA_P
ClientSampleId :
TR-04-112321


Tgt Ion:240 Resp: 594261
Ion Ratio Lower Upper
240 100
120 7.8 7.3 10.9
236 27.1 21.4 32.2

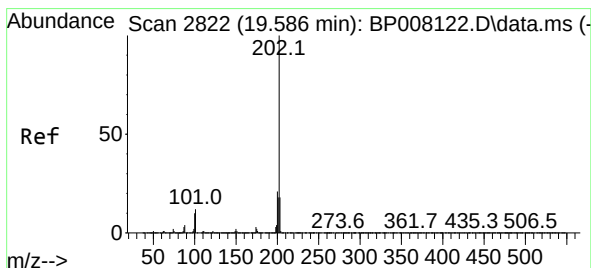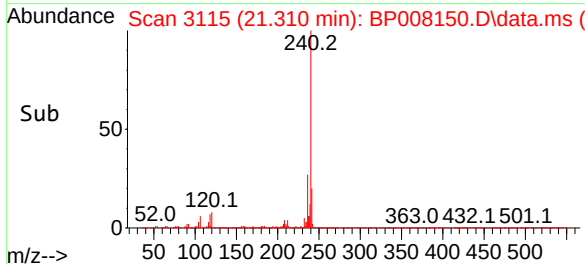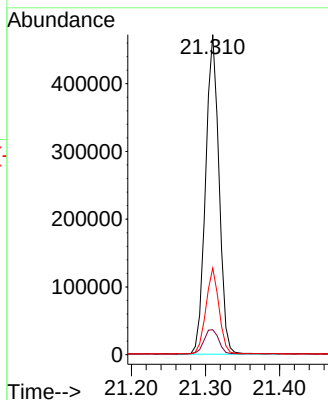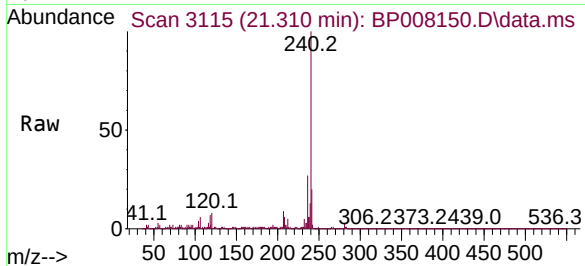

#78
Pyrene
Concen: Below Cal
RT: 19.580 min Scan# 2821
Delta R.T. -0.006 min
Lab File: BP008150.D
Acq: 29 Nov 2021 19:54

Tgt Ion:202 Resp: 4737
Ion Ratio Lower Upper
202 100
200 30.8 17.1 25.7#
203 40.4 14.2 21.2#


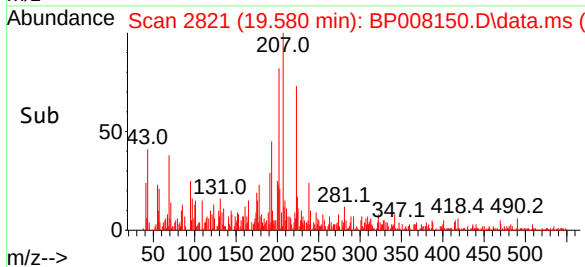
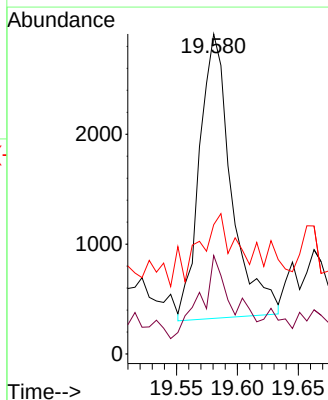
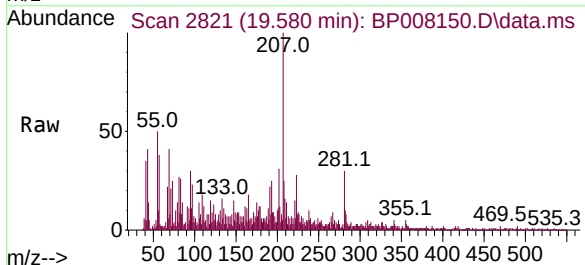


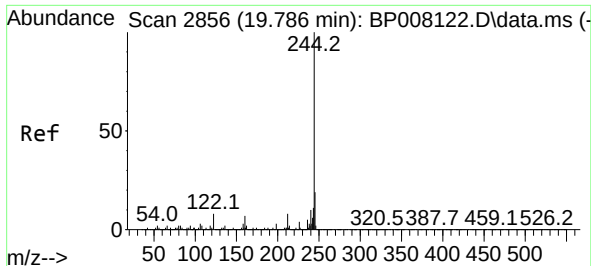

#79
 Terphenyl-d14
 Concen: 14.890 ng
 RT: 19.775 min Scan# 21
 Delta R.T. -0.011 min
 Lab File: BP008150.D
 Acq: 29 Nov 2021 19:54

Instrument :
 BNA_P
 ClientSampleId :
 TR-04-112321

Tgt Ion:	244	Resp:	423400
Ion Ratio	Lower	Upper	
244	100		
212	7.9	6.0	9.0
122	8.9	6.6	9.8

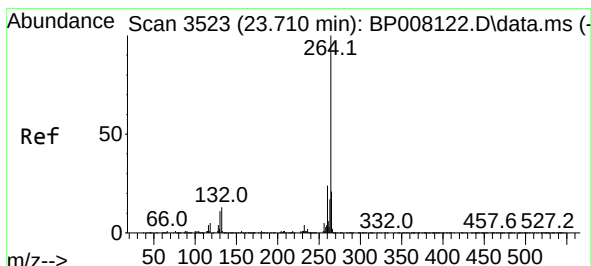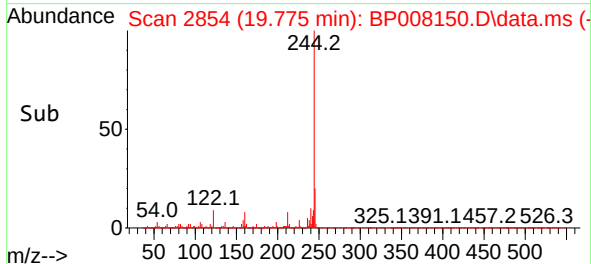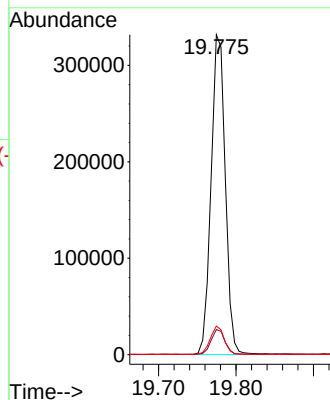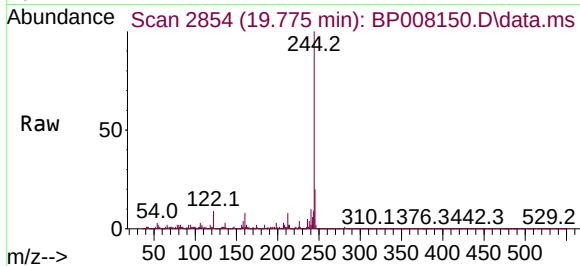

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 23.704 min Scan# 3522
 Delta R.T. -0.006 min
 Lab File: BP008150.D
 Acq: 29 Nov 2021 19:54

Tgt Ion:	264	Resp:	630374
Ion Ratio	Lower	Upper	
264	100		
260	24.4	19.4	29.2
265	22.1	17.6	26.4

