
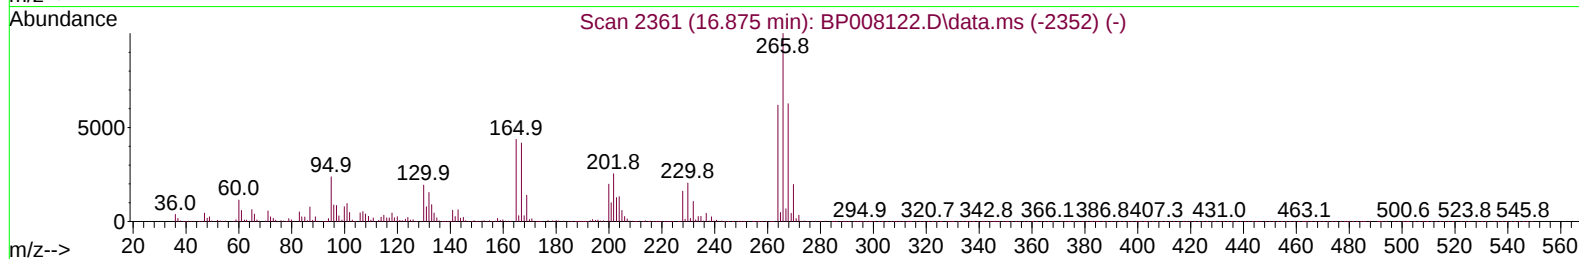
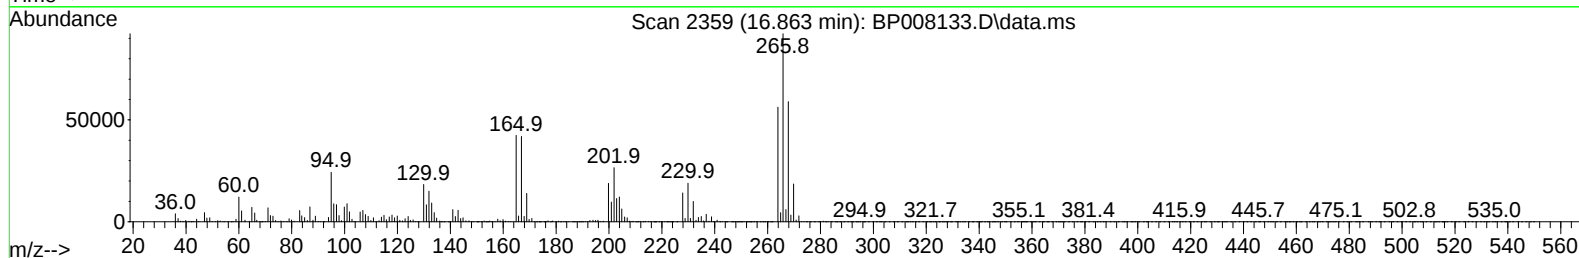


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112921\
Data File : BP008133.D
Acq On : 29 Nov 2021 09:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 29 10:57:48 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 25 01:13:46 2021
Response via : Initial Calibration

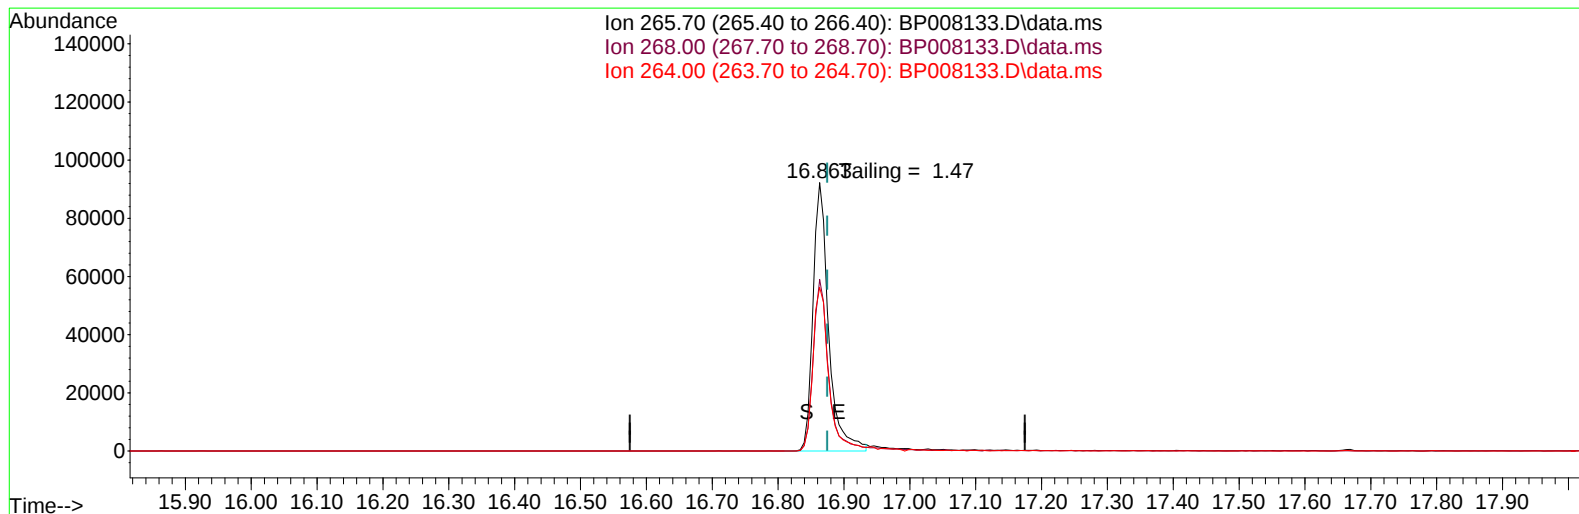

TIC: BP008133.D\data.ms

(70) Pentachlorophenol (C)




16.863min (-0.012) 712860.42 ng

response 156195

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	63.89
264.00	61.90	60.91
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112921\
 Data File : BP008133.D
 Acq On : 29 Nov 2021 09:53
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 29 10:57:48 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 25 01:13:46 2021
 Response via : Initial Calibration

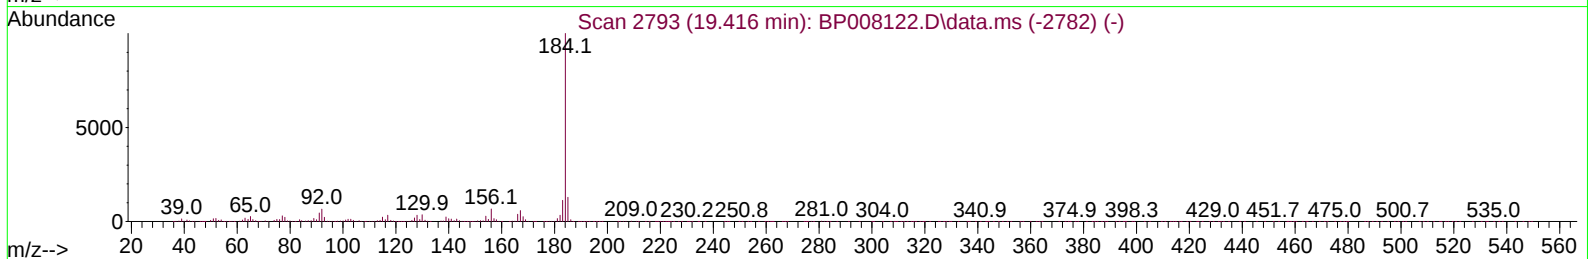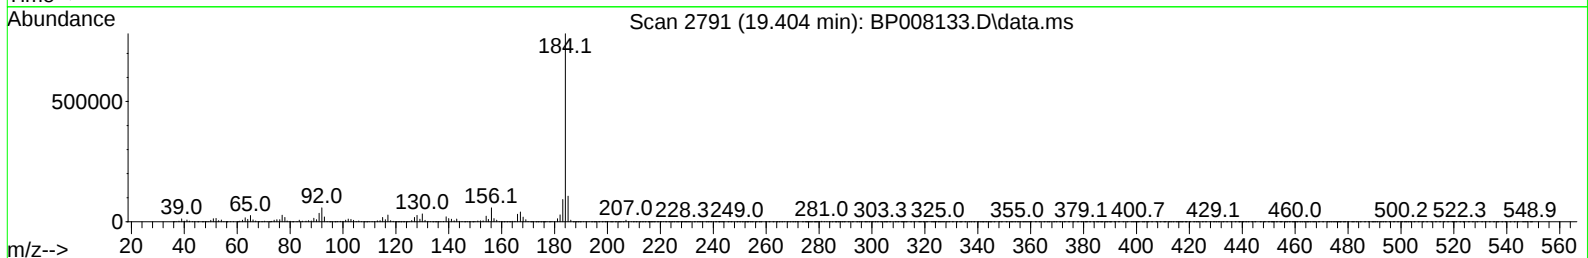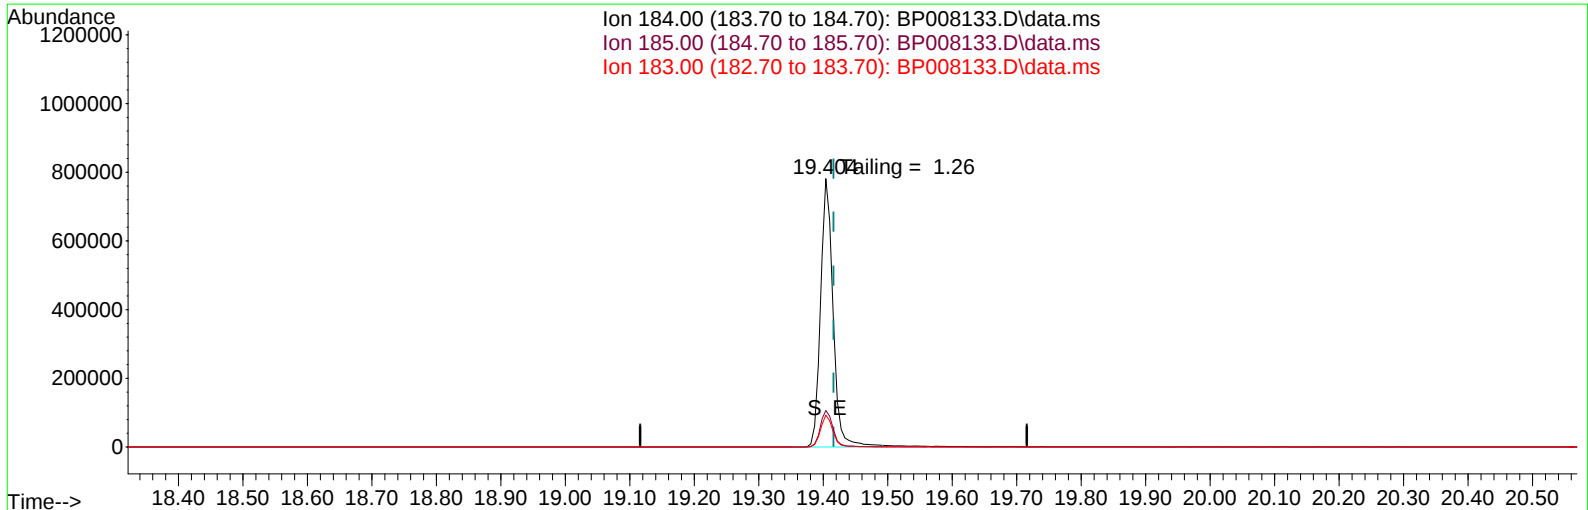

TIC: BP008133.D\data.ms

(77) Benzidine

19.404min (-0.012) 1159072.55 ng

response 1065250

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	12.90	13.62
183.00	11.40	11.86
0.00	0.00	0.00