
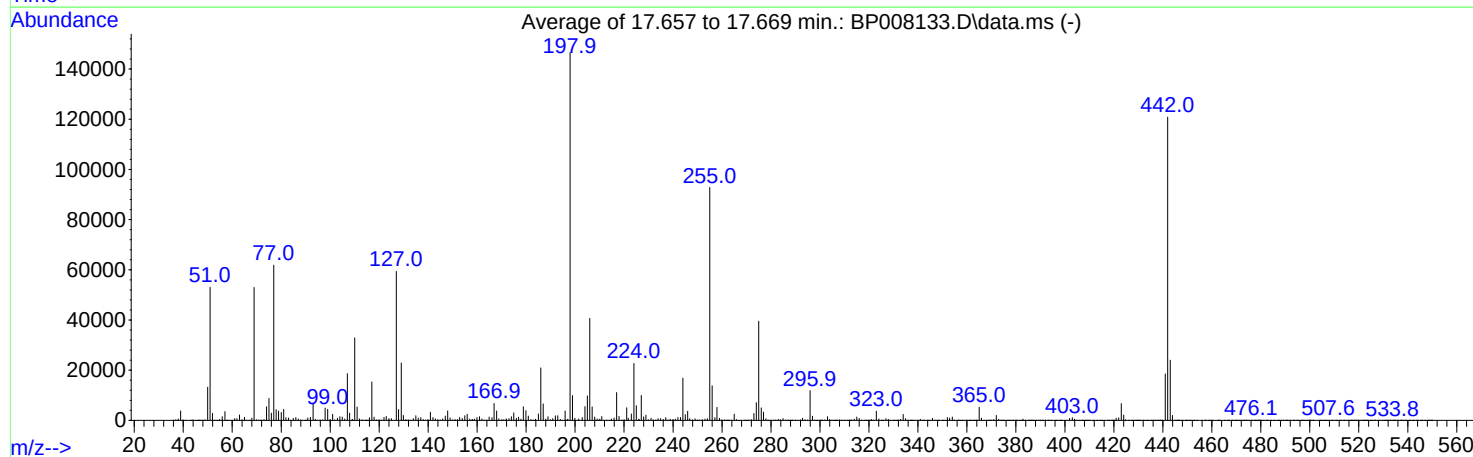


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112921\
 Data File : BP008133.D
 Acq On : 29 Nov 2021 09:53
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 01 12:06:05 2021

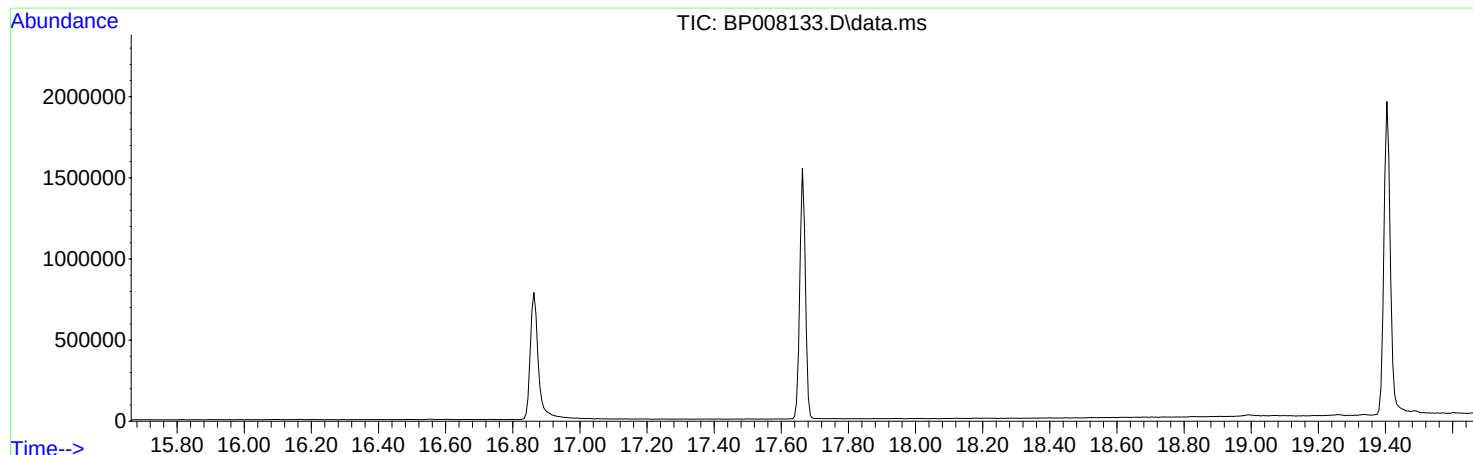




AutoFind: Scans 2494, 2495, 2496; Background Corrected with Scan 2484

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.2	53081	PASS
68	69	0.00	2	1.7	907	PASS
69	198	0.00	100	36.1	52992	PASS
70	69	0.00	2	0.5	280	PASS
127	198	10	80	40.5	59368	PASS
197	198	0.00	2	0.3	479	PASS
198	198	100	100	100.0	146603	PASS
199	198	5	9	6.8	9898	PASS
275	198	10	60	27.0	39539	PASS
365	198	1	100	3.6	5248	PASS
441	198	0.01	100	12.6	18513	PASS
442	442	100	100	100.0	120845	PASS
443	442	15	24	19.8	23964	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112921\
Data File : BP008133.D
Acq On : 29 Nov 2021 09:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Nov 29 10:57:48 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 25 01:13:46 2021
Response via : Initial Calibration

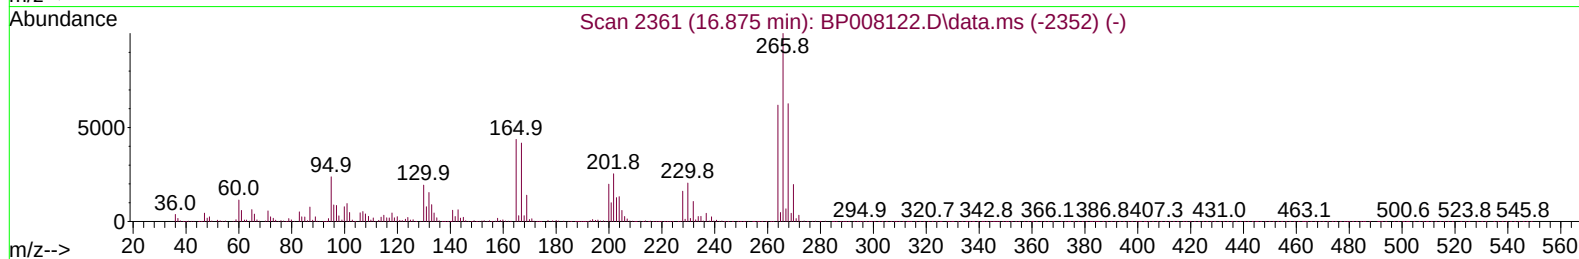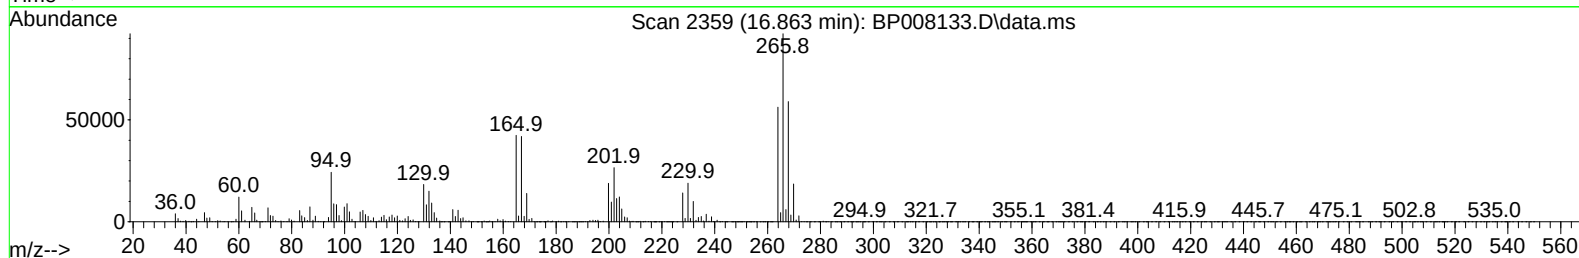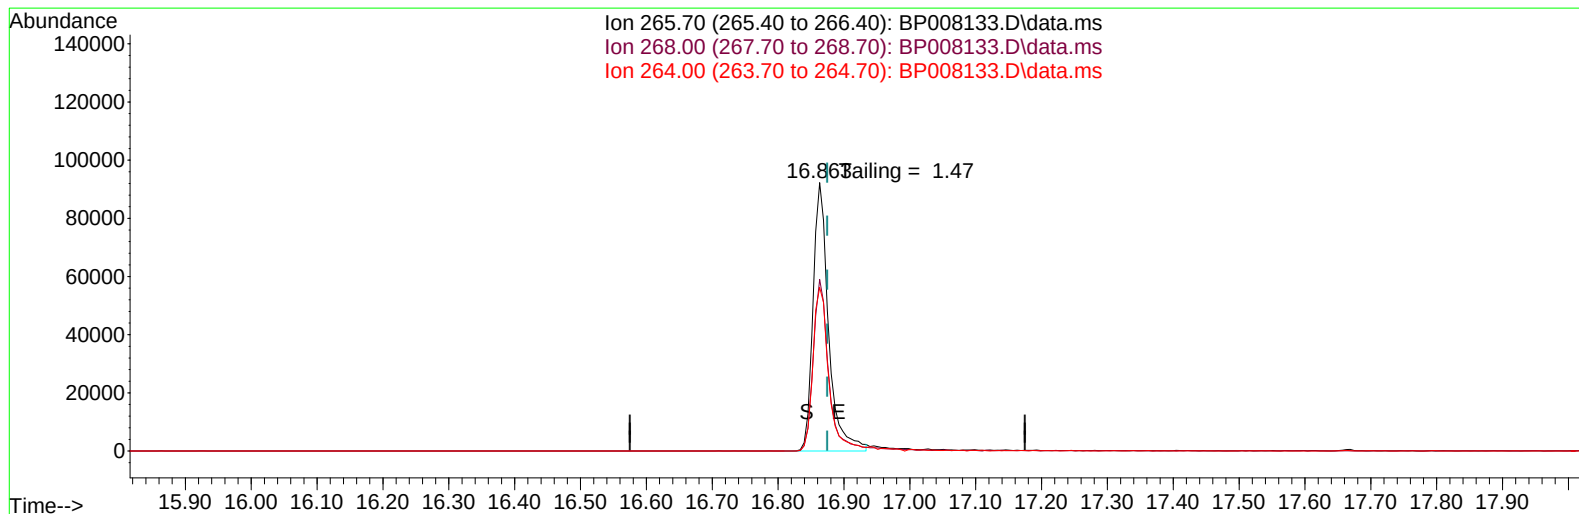

TIC: BP008133.D\data.ms

(70) Pentachlorophenol (C)

16.863min (-0.012) 712860.42 ng




response 156195

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	63.89
264.00	61.90	60.91
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112921\
Data File : BP008133.D
Acq On : 29 Nov 2021 09:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Nov 29 10:57:48 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 25 01:13:46 2021
Response via : Initial Calibration

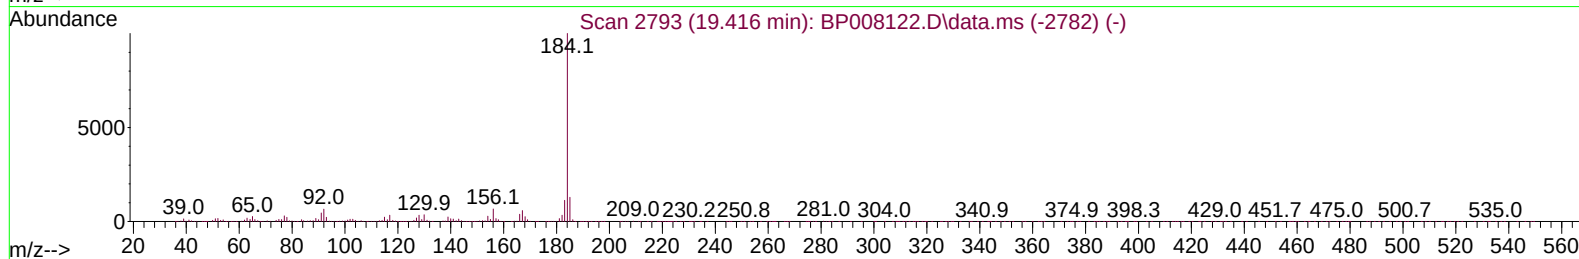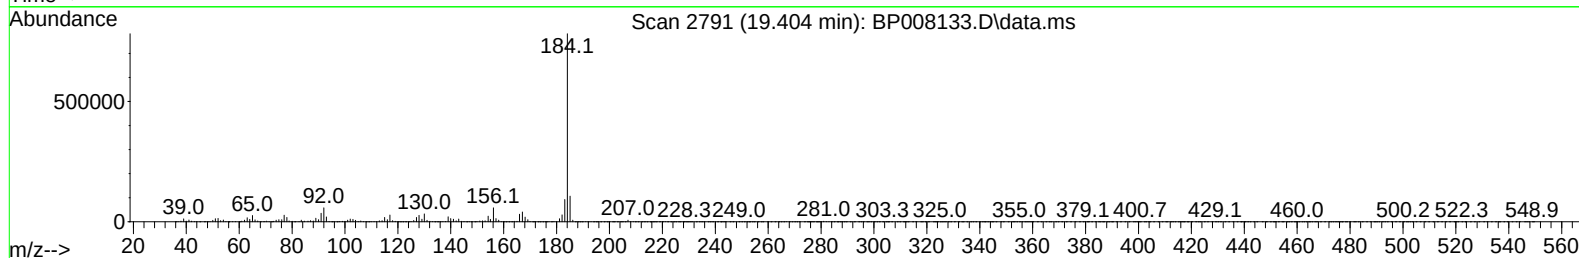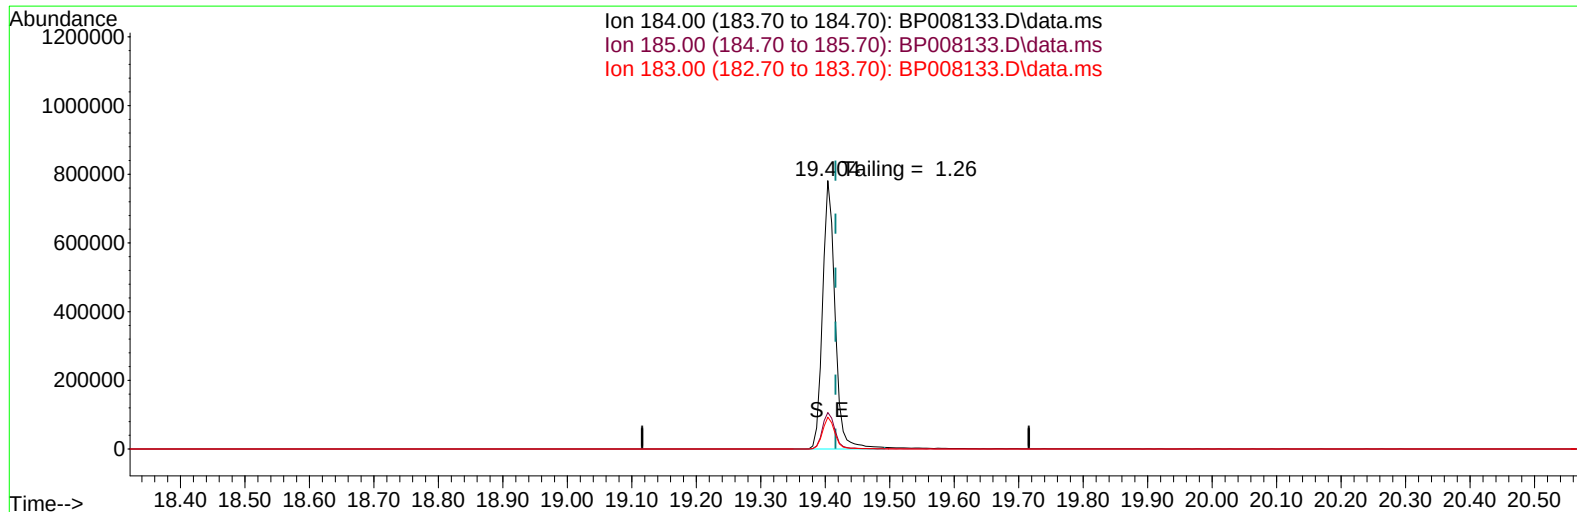

TIC: BP008133.D\data.ms

(77) Benzidine

19.404min (-0.012) 1159072.55 ng

response 1065250

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	12.90	13.62
183.00	11.40	11.86
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/29/2021	BNA_P	BP008133.D
Compound Name	Response	Retention Time
DDT	535683	20.61
DDD	1277	20.18
DDE	615	19.69
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1892	537575	0.35

Instrument :
BNA_P
ClientSampleId :
DFTPP