
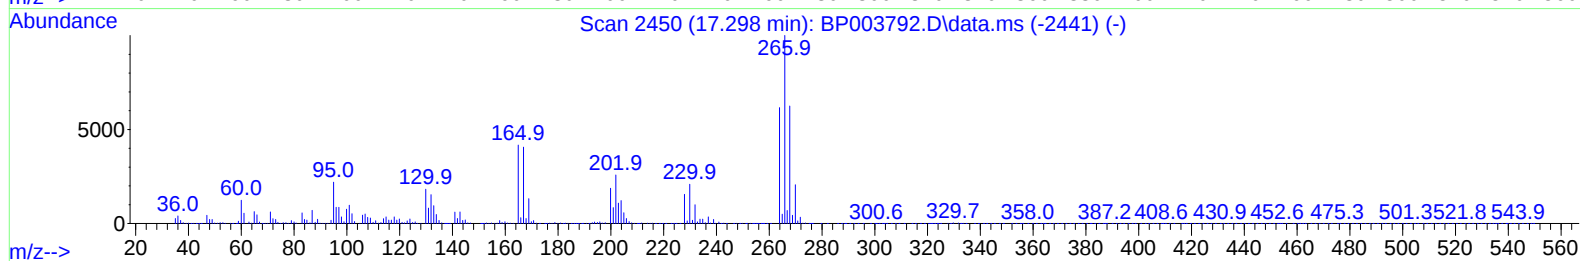
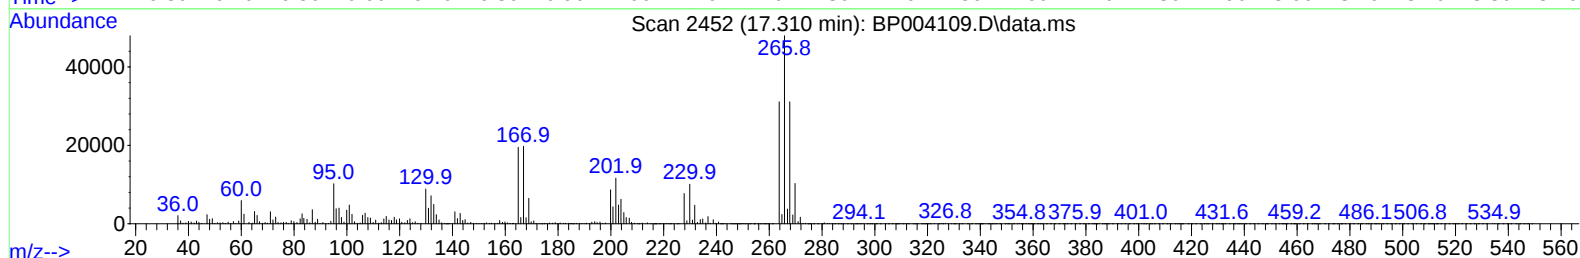


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113020\
Data File : BP004109.D
Acq On : 30 Nov 2020 12:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 01 01:19:39 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 23 16:42:41 2020
Response via : Initial Calibration

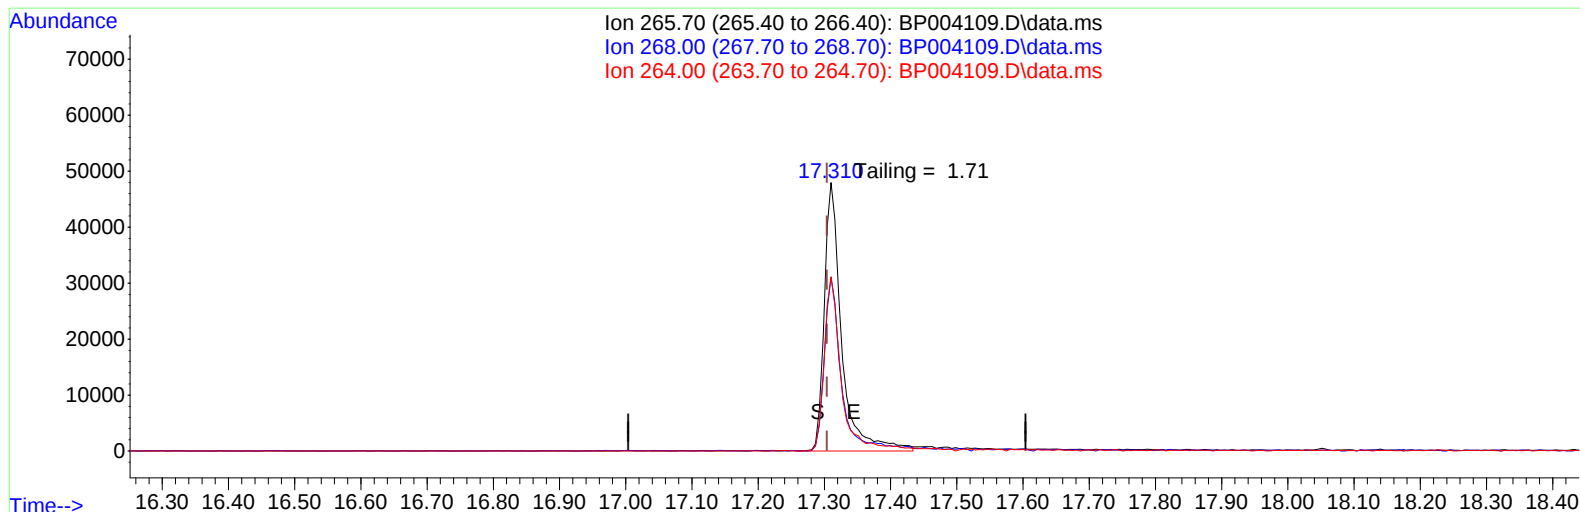

TIC: BP004109.D\data.ms

(70) Pentachlorophenol (C)




17.310min (+ 0.006) 187300.10 ng

response 87321

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	64.81
264.00	63.30	64.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113020\
Data File : BP004109.D
Acq On : 30 Nov 2020 12:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 01 01:19:39 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 23 16:42:41 2020
Response via : Initial Calibration

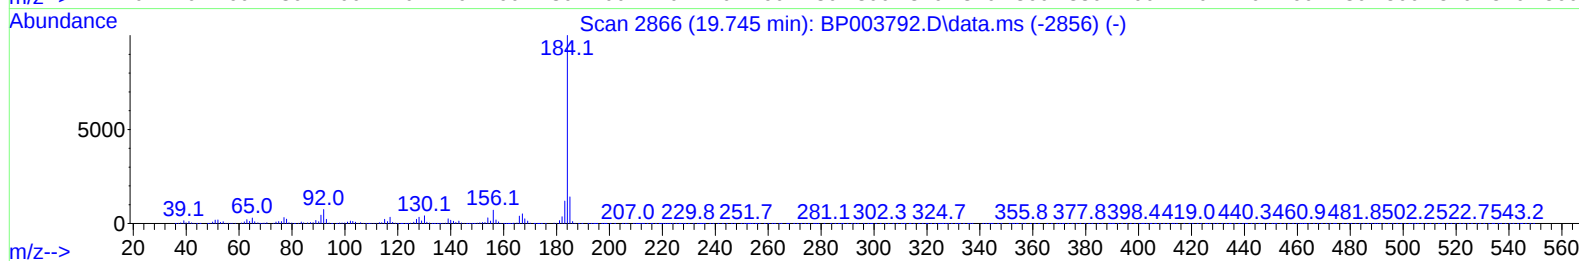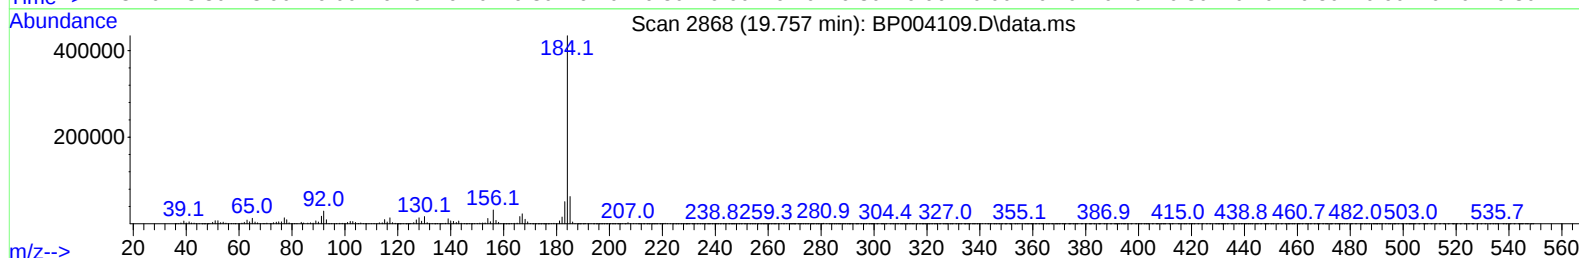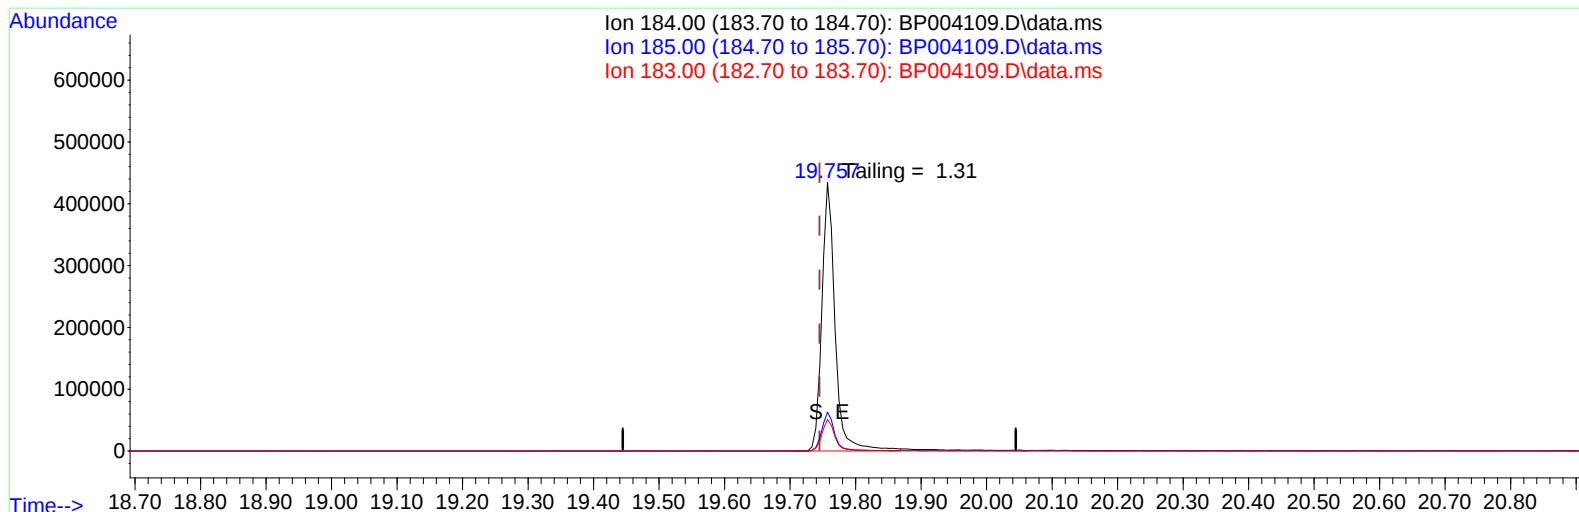

TIC: BP004109.D\data.ms

(77) Benzidine

19.757min (+ 0.012) 1518.31 ng

response 613015

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.47
183.00	12.00	11.79
0.00	0.00	0.00