
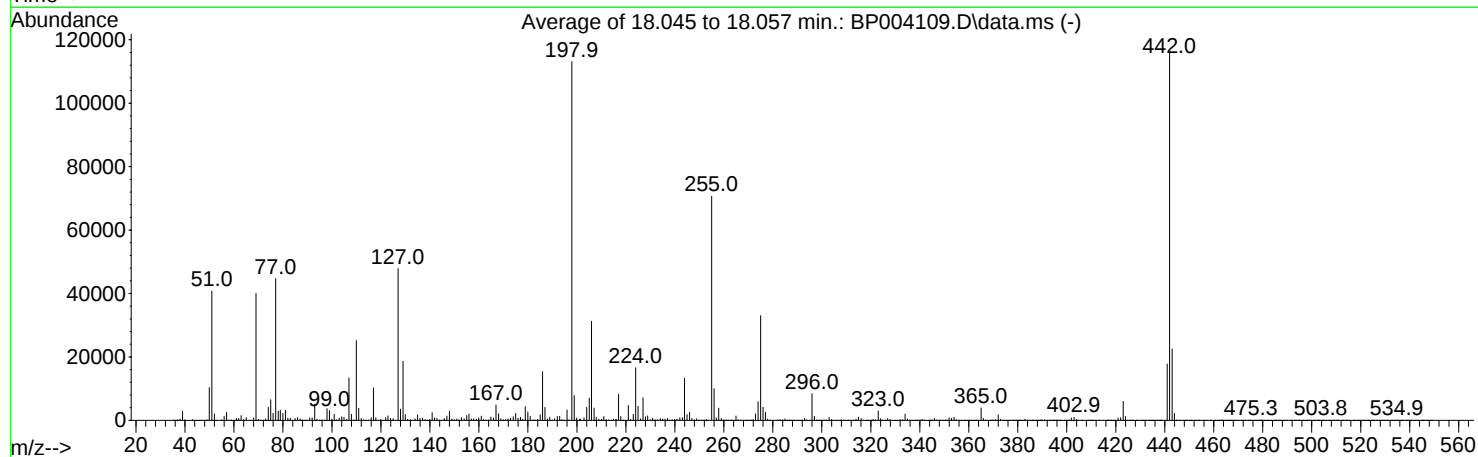


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113020\
 Data File : BP004109.D
 Acq On : 30 Nov 2020 12:08
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP110320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Nov 23 16:42:41 2020

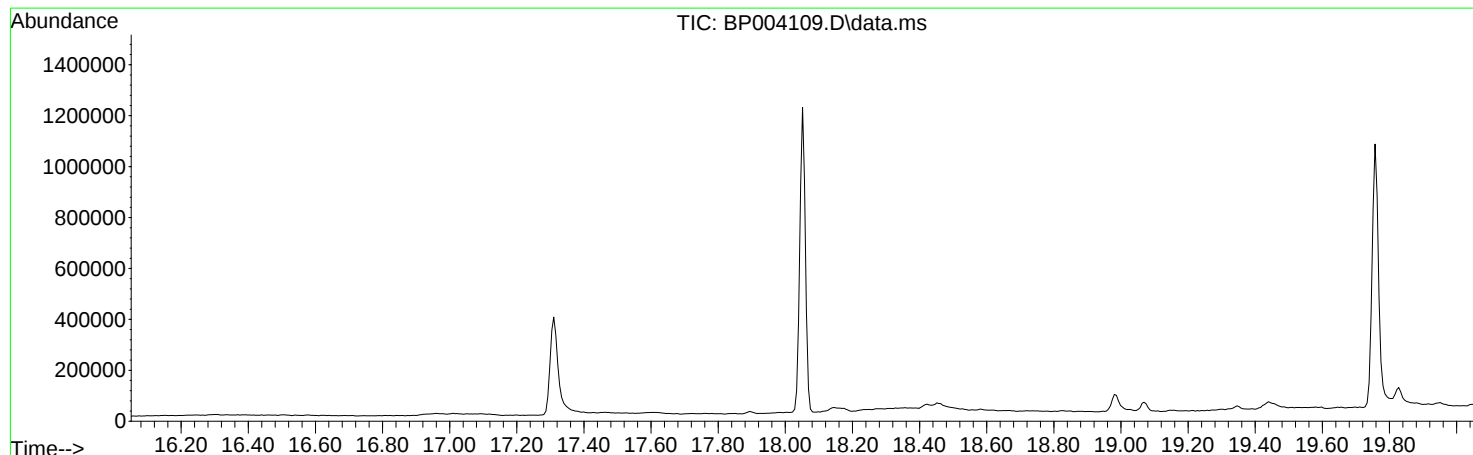

AutoFind: Scans 2577, 2578, 2579; Background Corrected with Scan 2571

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.1	40789	PASS
68	69	0.00	2	1.9	762	PASS
69	198	0.00	100	35.4	40055	PASS
70	69	0.00	2	0.8	322	PASS
127	198	10	80	42.3	47895	PASS
197	198	0.00	2	0.1	163	PASS
198	198	100	100	100.0	113117	PASS
199	198	5	9	6.9	7839	PASS
275	198	10	60	29.1	32973	PASS
365	198	1	100	3.4	3902	PASS
441	198	0.01	100	15.7	17756	PASS
442	442	100	100	100.0	115988	PASS
443	442	15	24	19.4	22500	PASS