
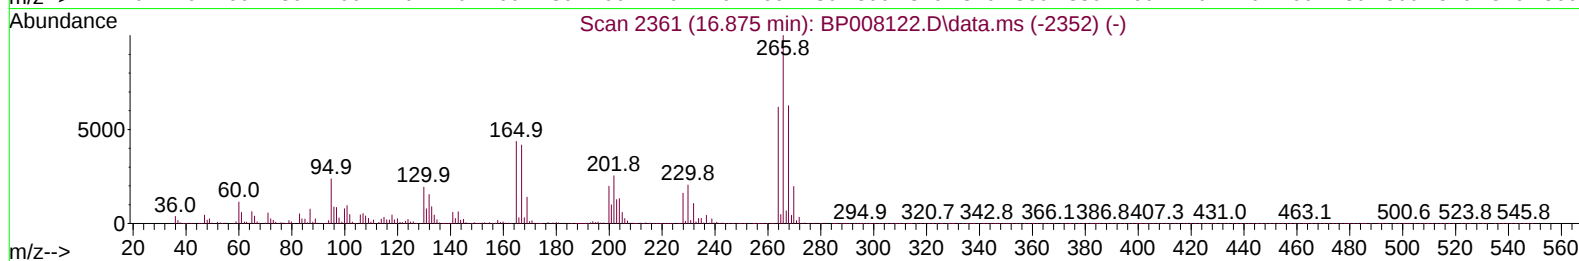
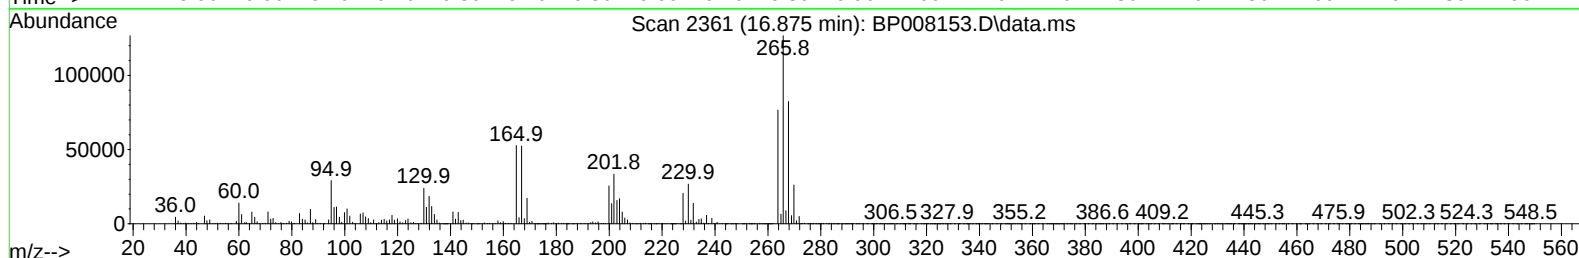


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113021\
 Data File : BP008153.D
 Acq On : 30 Nov 2021 09:35
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 30 11:18:44 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 25 01:13:46 2021
 Response via : Initial Calibration

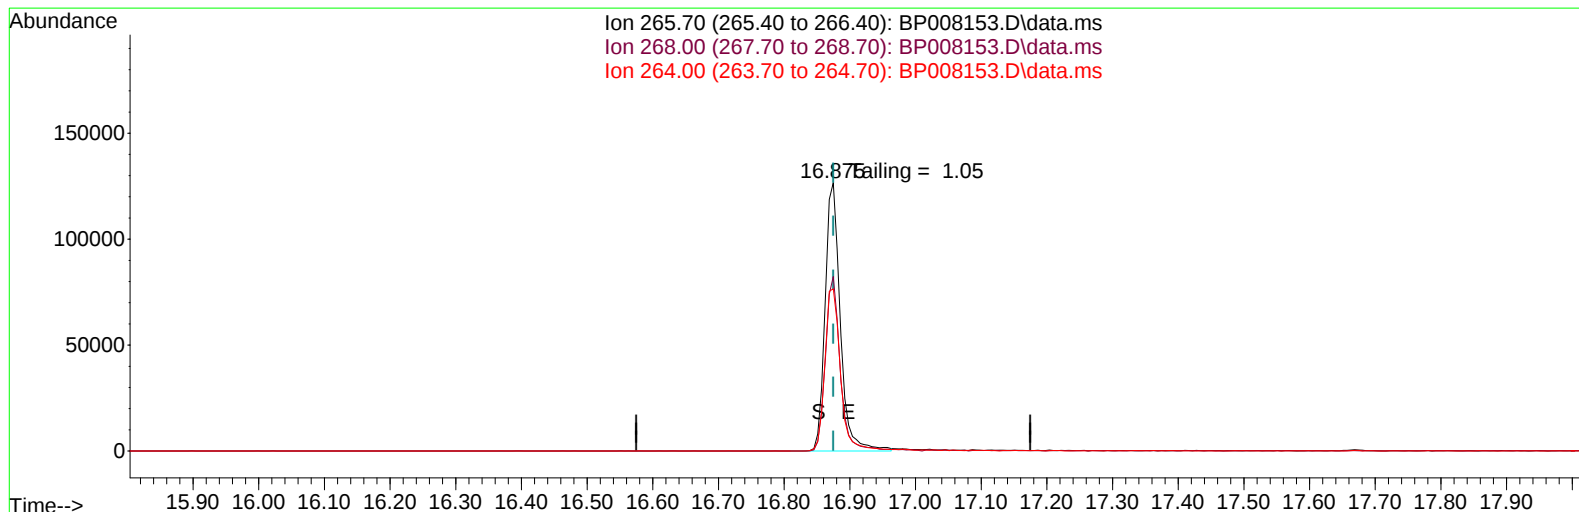

TIC: BP008153.D\data.ms

(70) Pentachlorophenol (C)




16.875min (-0.000) 692456.69 ng

response 205562

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	64.98
264.00	61.90	60.46
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113021\
 Data File : BP008153.D
 Acq On : 30 Nov 2021 09:35
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 30 11:18:44 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 25 01:13:46 2021
 Response via : Initial Calibration

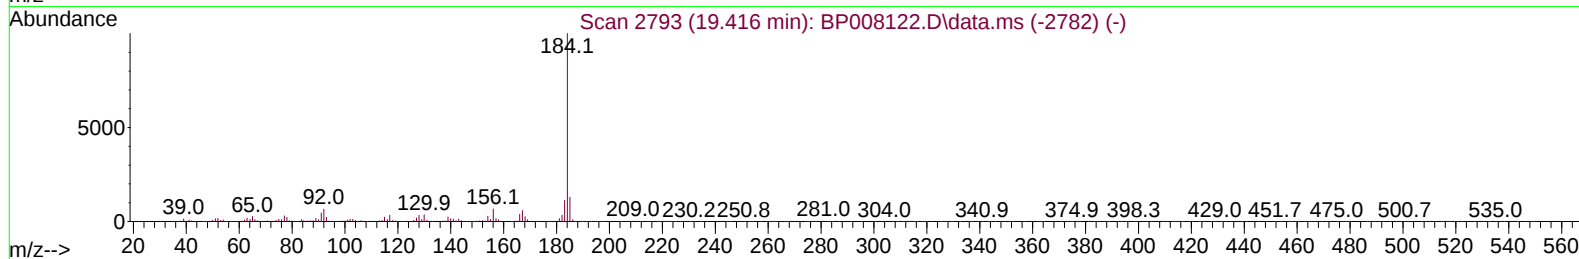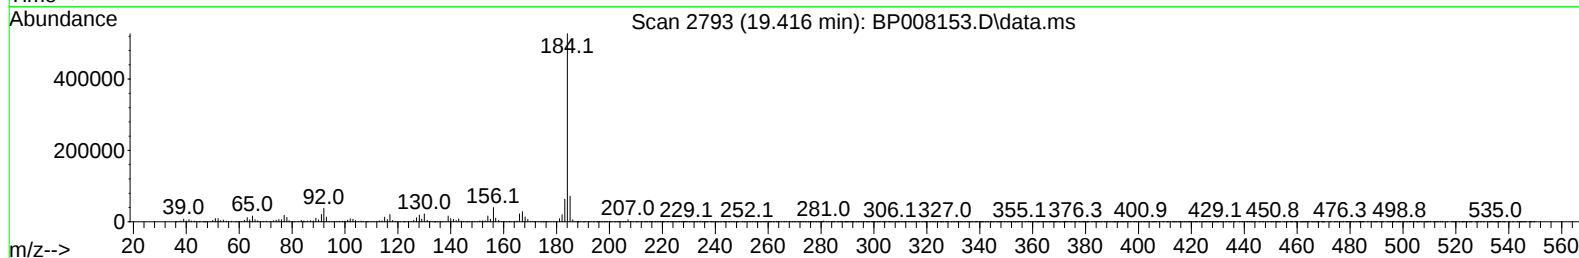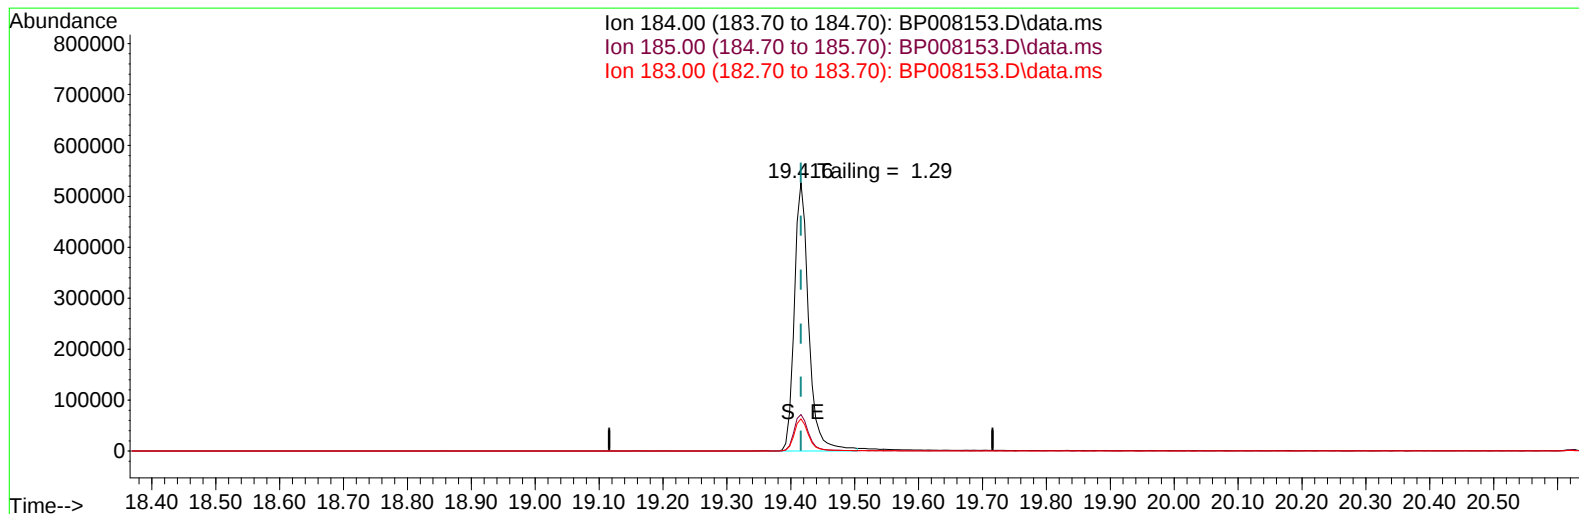

TIC: BP008153.D\data.ms

(77) Benzidine**19.416min (-0.000) 259219.58 ng****response 842718**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	12.90	13.63
183.00	11.40	12.00
0.00	0.00	0.00