


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113021\
 Data File : BP008153.D
 Acq On : 30 Nov 2021 09:35
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 01 12:06:05 2021

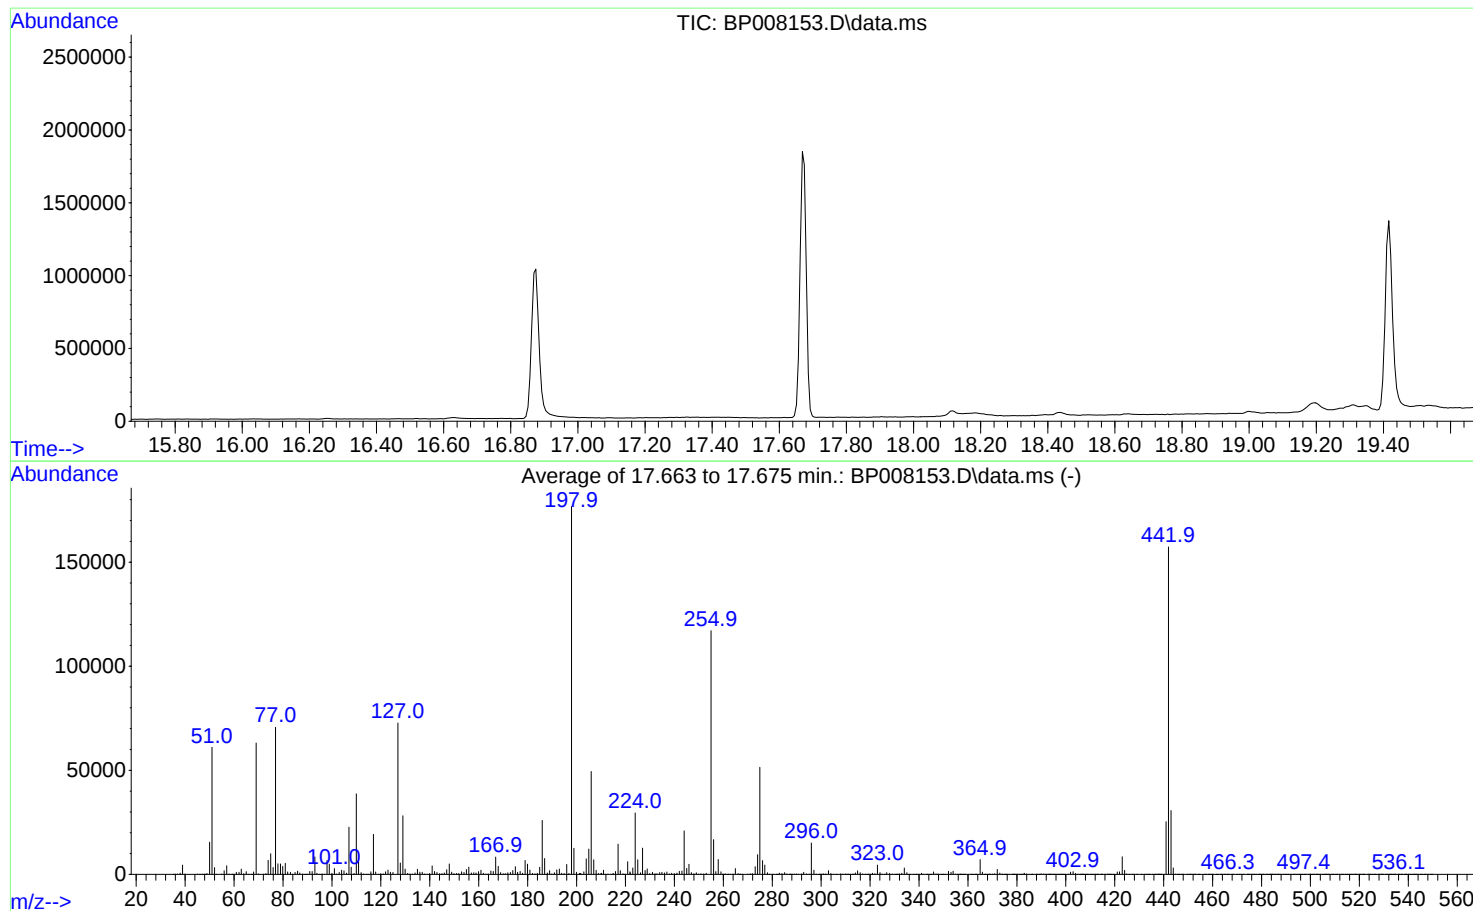




AutoFind: Scans 2495, 2496, 2497; Background Corrected with Scan 2487

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.5	61013	PASS
68	69	0.00	2	1.8	1158	PASS
69	198	0.00	100	35.7	63135	PASS
70	69	0.00	2	0.4	238	PASS
127	198	10	80	41.1	72695	PASS
197	198	0.00	2	0.3	461	PASS
198	198	100	100	100.0	176731	PASS
199	198	5	9	7.1	12524	PASS
275	198	10	60	29.1	51434	PASS
365	198	1	100	4.0	7092	PASS
441	198	0.01	100	14.3	25298	PASS
442	442	100	100	100.0	157313	PASS
443	442	15	24	19.5	30712	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113021\
Data File : BP008153.D
Acq On : 30 Nov 2021 09:35
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Nov 30 11:18:44 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 25 01:13:46 2021
Response via : Initial Calibration

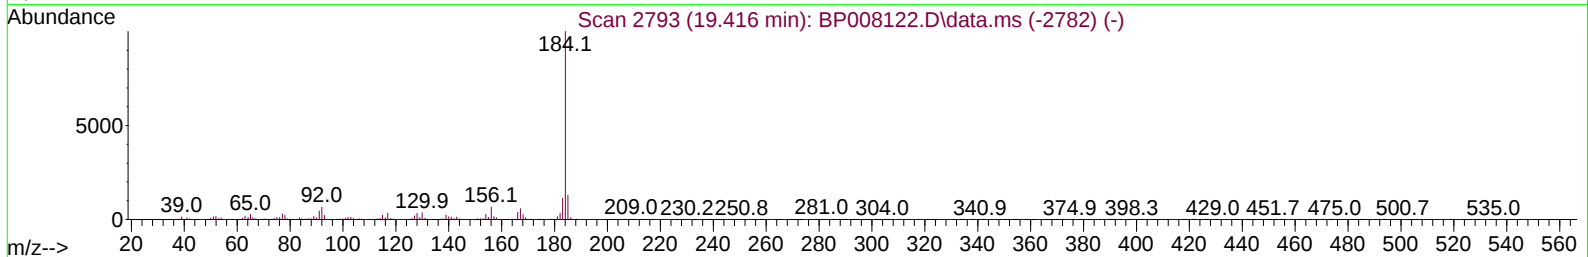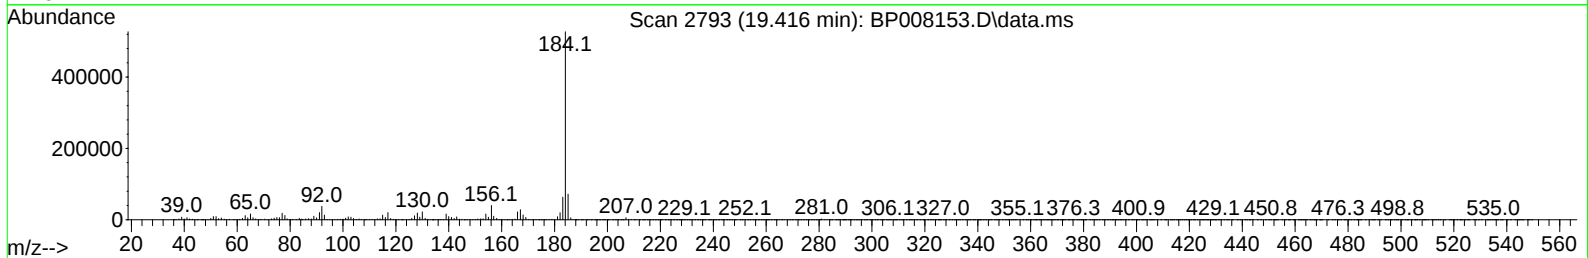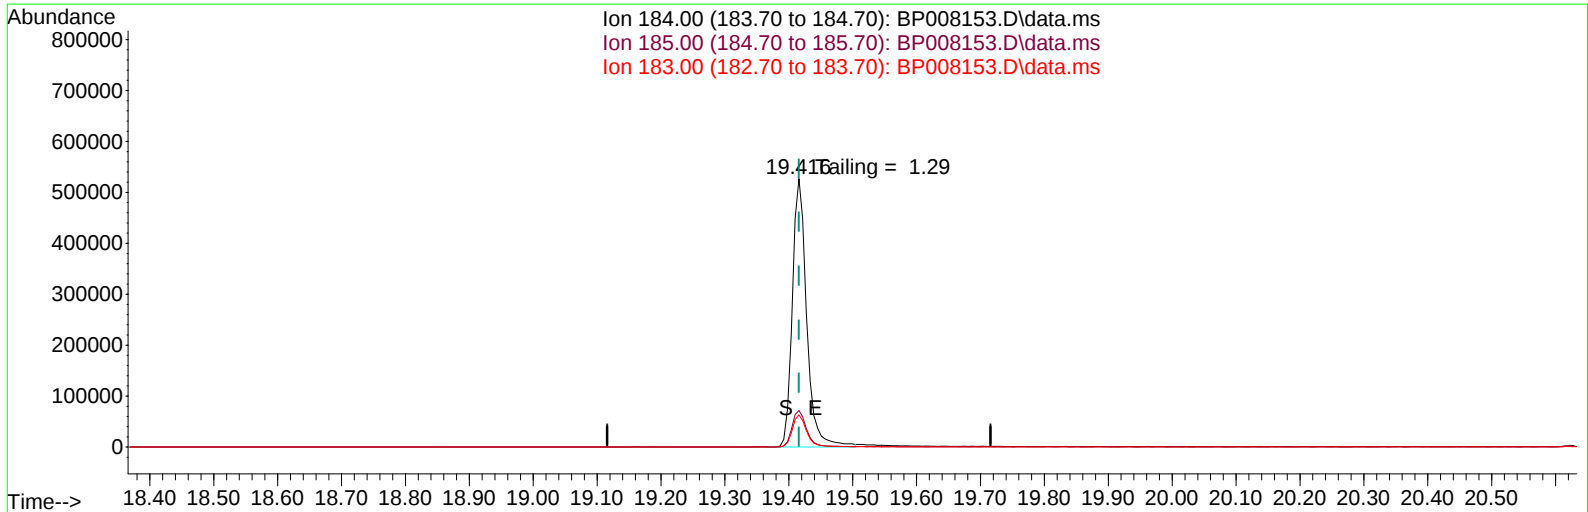

TIC: BP008153.D\data.ms

(77) Benzidine

19.416min (-0.000) 259219.58 ng

response 842718

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	12.90	13.63
183.00	11.40	12.00
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/30/2021	BNA_P	BP008153.D
Compound Name	Response	Retention Time
DDT	584192	20.62
DDD	4029	20.19
DDE	493	19.99
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4522	588714	0.77

Instrument :
BNA_P
ClientSampleId :
DFTPP