
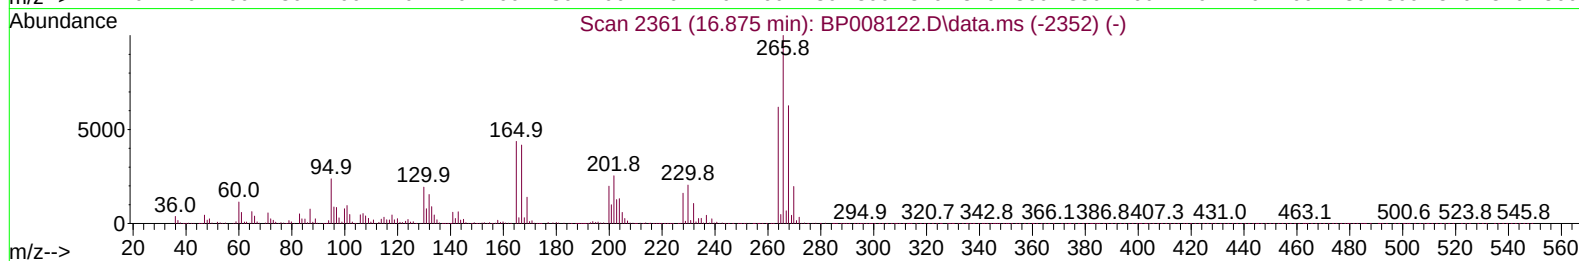
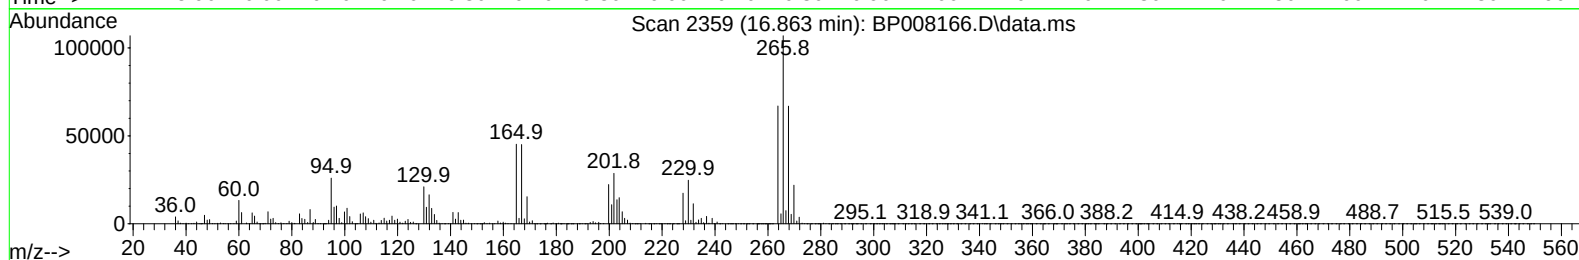


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120121\
 Data File : BP008166.D
 Acq On : 01 Dec 2021 10:12
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 01 12:02:36 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 25 01:13:46 2021
 Response via : Initial Calibration

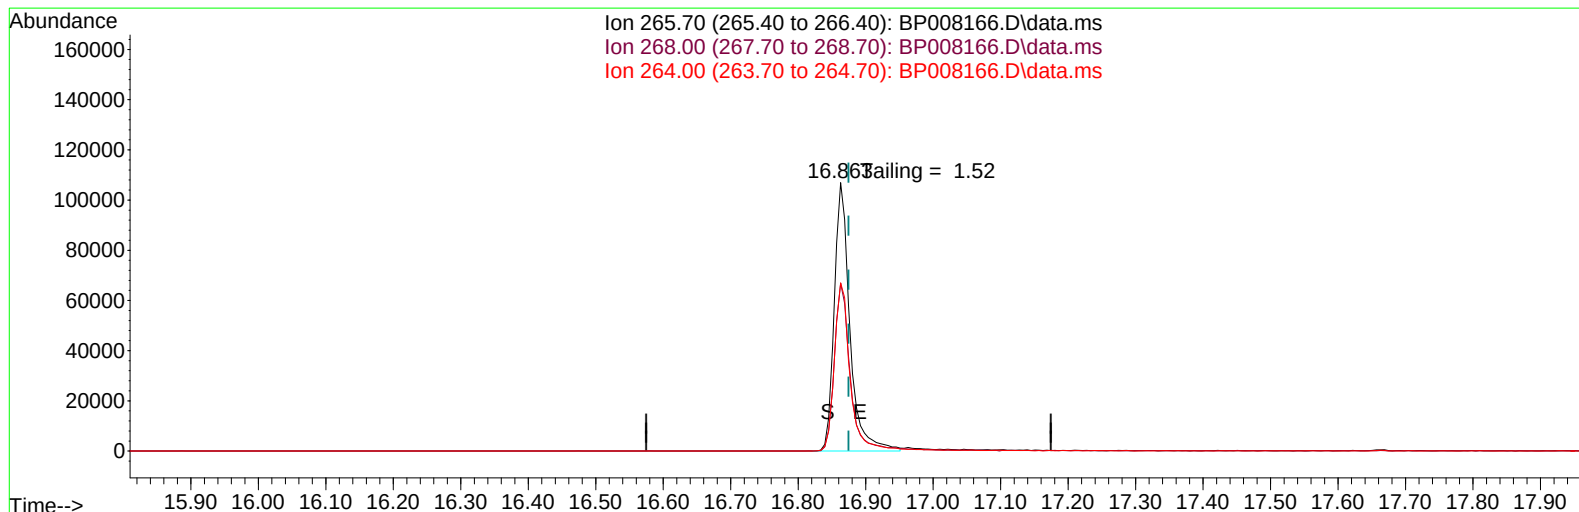

TIC: BP008166.D\data.ms

(70) Pentachlorophenol (C)




16.863min (-0.012) 1165779.04 ng

response 173036

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	62.56
264.00	61.90	62.68
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120121\
 Data File : BP008166.D
 Acq On : 01 Dec 2021 10:12
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 01 12:02:36 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 25 01:13:46 2021
 Response via : Initial Calibration

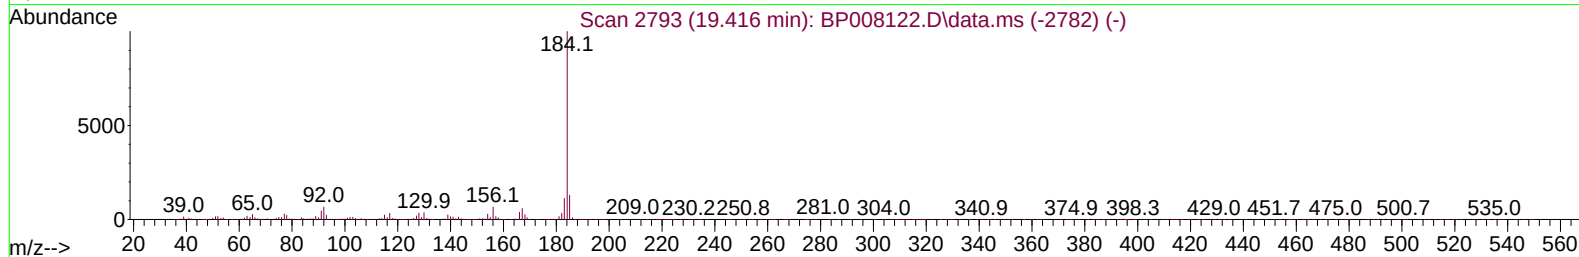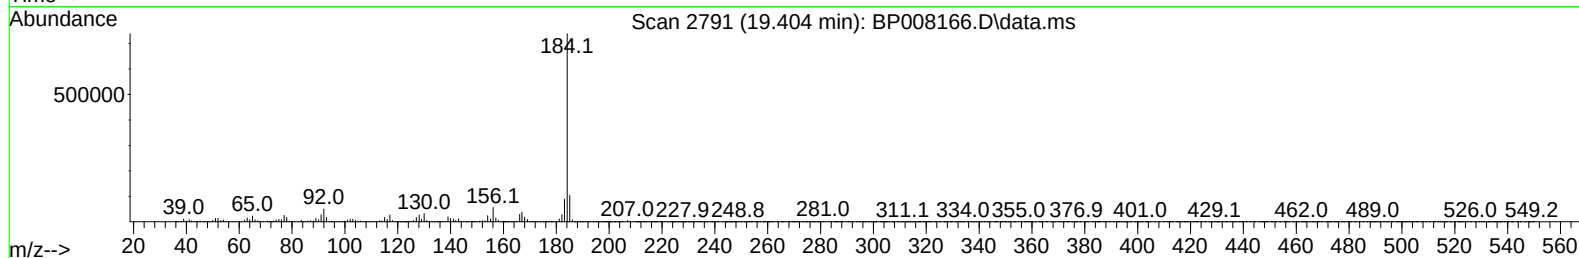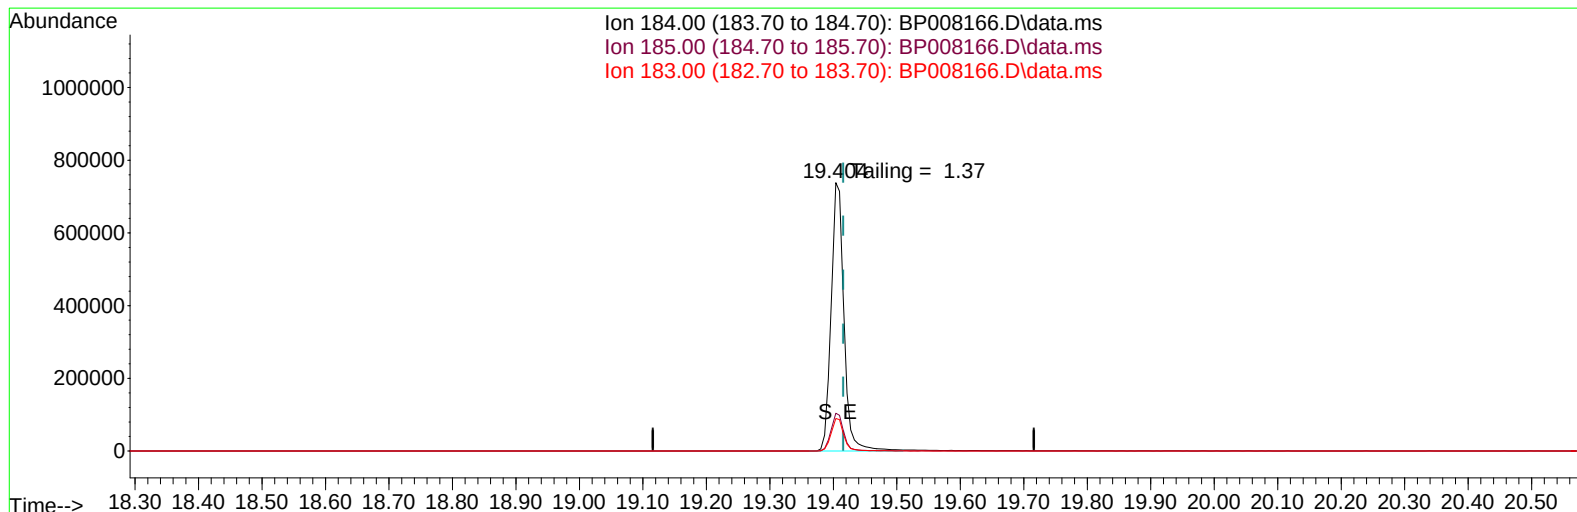

TIC: BP008166.D\data.ms

(77) Benzidine**19.404min (-0.012) 670026.67 ng****response 1047763**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	12.90	14.10
183.00	11.40	12.11
0.00	0.00	0.00