

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120121\
 Data File : BP008173.D
 Acq On : 01 Dec 2021 14:34
 Operator : CG/JU
 Sample : M4856-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 332

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP008173.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.322	222	227	241	rBV	512890	702777	1.32%	0.524%
2	4.928	322	330	344	rBV	2173591	3295554	6.17%	2.455%
3	6.981	672	679	689	rBV	413984	690547	1.29%	0.514%
4	7.799	811	818	826	rBV	349776	542449	1.02%	0.404%
5	8.957	1008	1015	1024	rBV	801487	1350141	2.53%	1.006%
6	10.598	1287	1294	1302	rBV	390846	653842	1.22%	0.487%
7	13.069	1707	1714	1722	rBV	1695613	2552561	4.78%	1.901%
8	14.445	1943	1948	1955	rVB	532827	769288	1.44%	0.573%
9	16.604	2310	2315	2331	rVB2	258216	552433	1.03%	0.412%
10	16.998	2374	2382	2402	rVB4	121494	549561	1.03%	0.409%
11	17.210	2412	2418	2424	rBV	593023	835744	1.56%	0.623%
12	18.327	2591	2608	2620	rBV	4961497	22706285	42.50%	16.914%
13	18.480	2620	2634	2643	rVV	6993643	26009487	48.68%	19.375%
14	18.651	2644	2663	2667	rVB	13959736	53425590	100.00%	39.797%
15	18.763	2674	2682	2692	rVB	1994544	4615955	8.64%	3.438%
16	19.510	2803	2809	2817	rBV	266808	553244	1.04%	0.412%
17	19.780	2849	2855	2860	rBV	2571439	3144212	5.89%	2.342%
18	20.339	2944	2950	2957	rVB	440420	739335	1.38%	0.551%
19	21.027	3062	3067	3073	rVB	586002	963033	1.80%	0.717%
20	21.174	3088	3092	3099	rVB2	382616	583149	1.09%	0.434%
21	21.310	3110	3115	3120	rBV	789484	999898	1.87%	0.745%
22	21.680	3172	3178	3184	rBV	491782	973254	1.82%	0.725%
23	22.392	3293	3299	3318	rVB	503097	1043235	1.95%	0.777%
24	23.174	3427	3432	3438	rVB	448583	813084	1.52%	0.606%
25	23.257	3441	3446	3457	rVB2	507995	1094934	2.05%	0.816%
26	23.704	3517	3522	3531	rVB2	575637	1169605	2.19%	0.871%
27	23.892	3550	3554	3563	rVB6	238735	586606	1.10%	0.437%
28	24.074	3581	3585	3596	rVB3	337739	765315	1.43%	0.570%
29	25.109	3757	3761	3771	rVB2	228932	571644	1.07%	0.426%
30	25.992	3905	3911	3925	rVB4	300235	992592	1.86%	0.739%




Sum of corrected areas: 134245354

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120121\
Data File : BP008173.D
Acq On : 01 Dec 2021 14:34
Operator : CG/JU
Sample : M4856-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
332

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

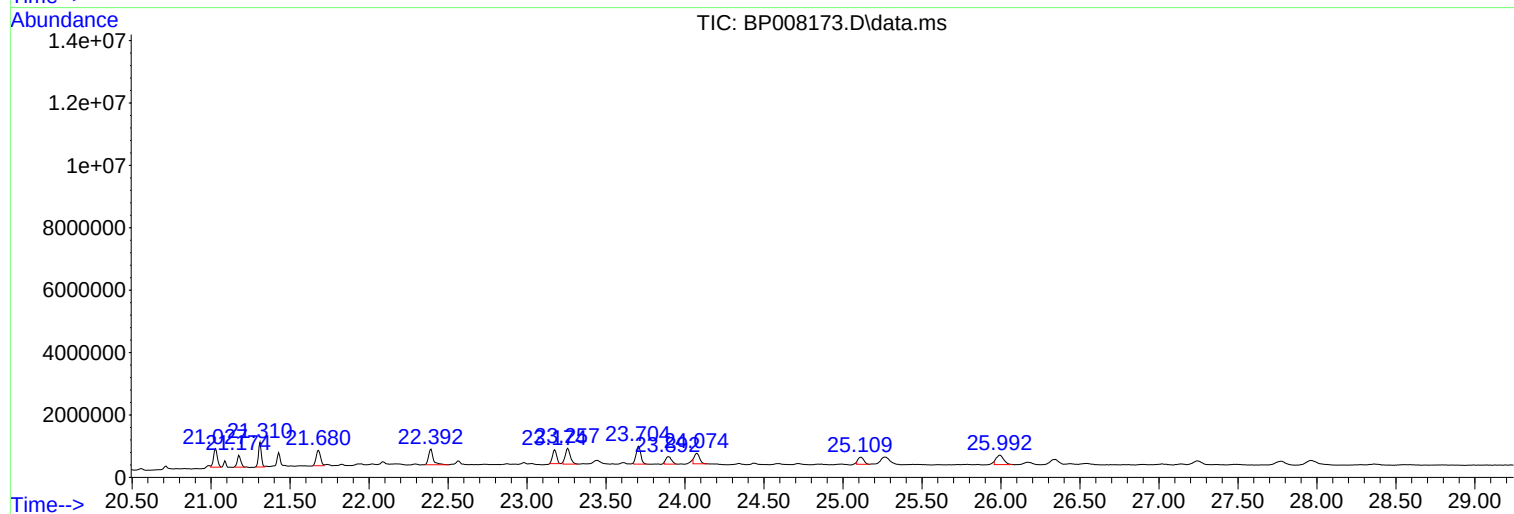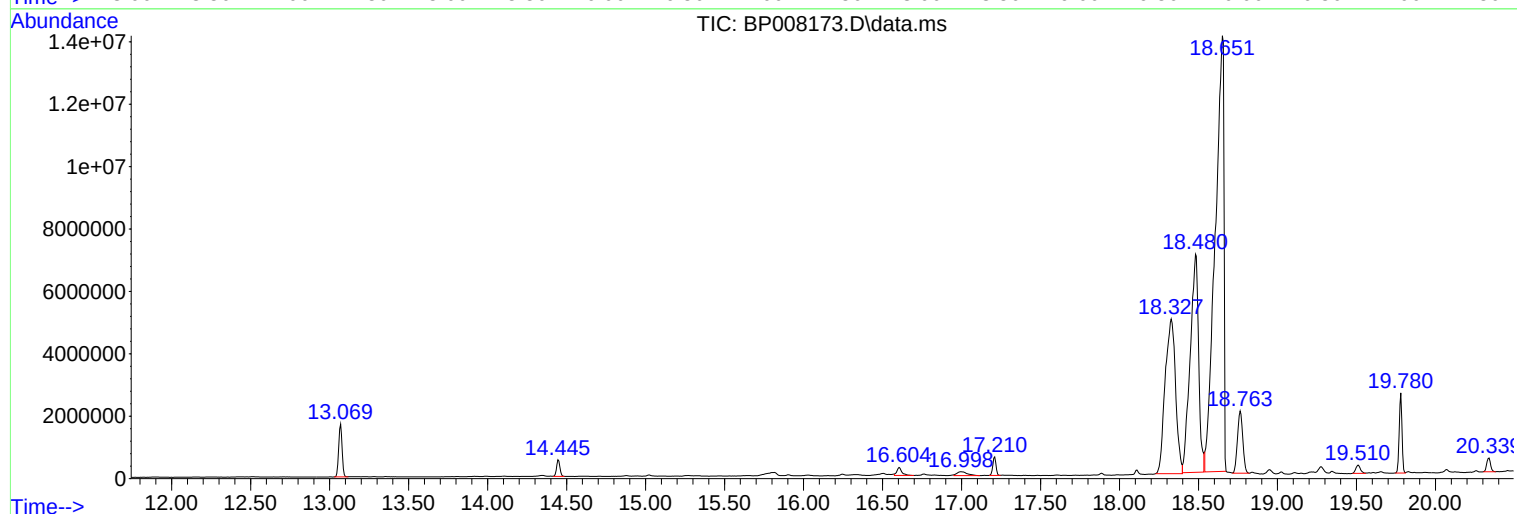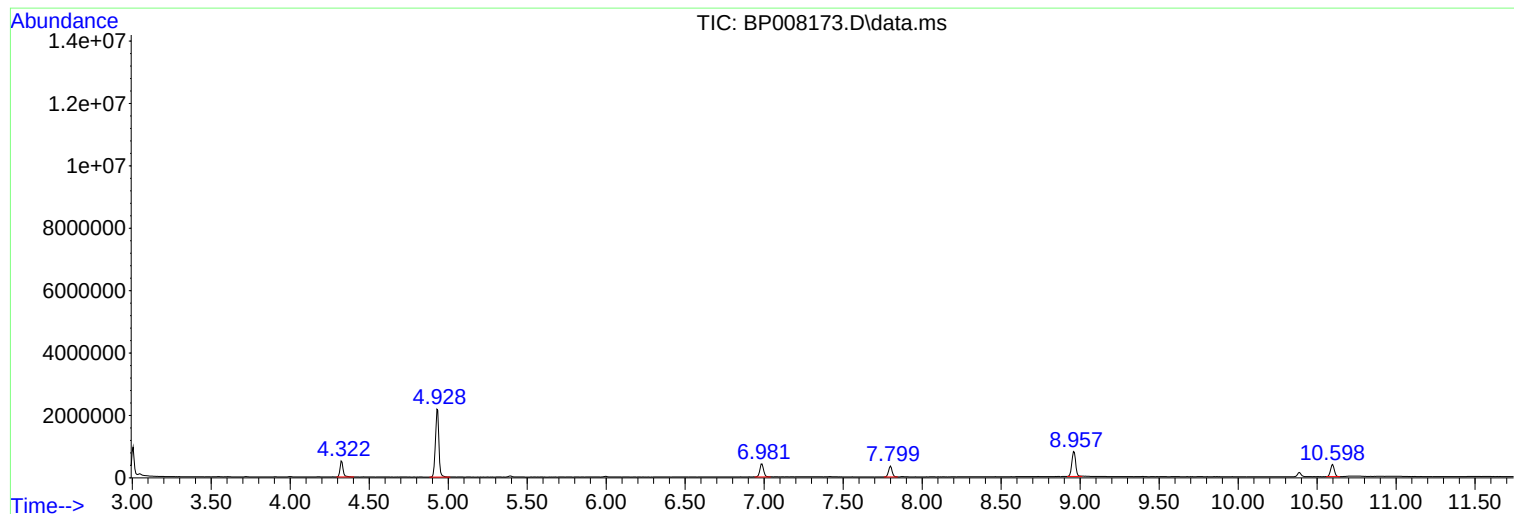

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120121\
Data File : BP008173.D
Acq On : 01 Dec 2021 14:34
Operator : CG/JU
Sample : M4856-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
332

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120121\
Data File : BP008173.D
Acq On : 01 Dec 2021 14:34
Operator : CG/JU
Sample : M4856-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
332

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------