


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120121\
 Data File : BP008166.D
 Acq On : 01 Dec 2021 10:12
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 03 14:39:24 2021

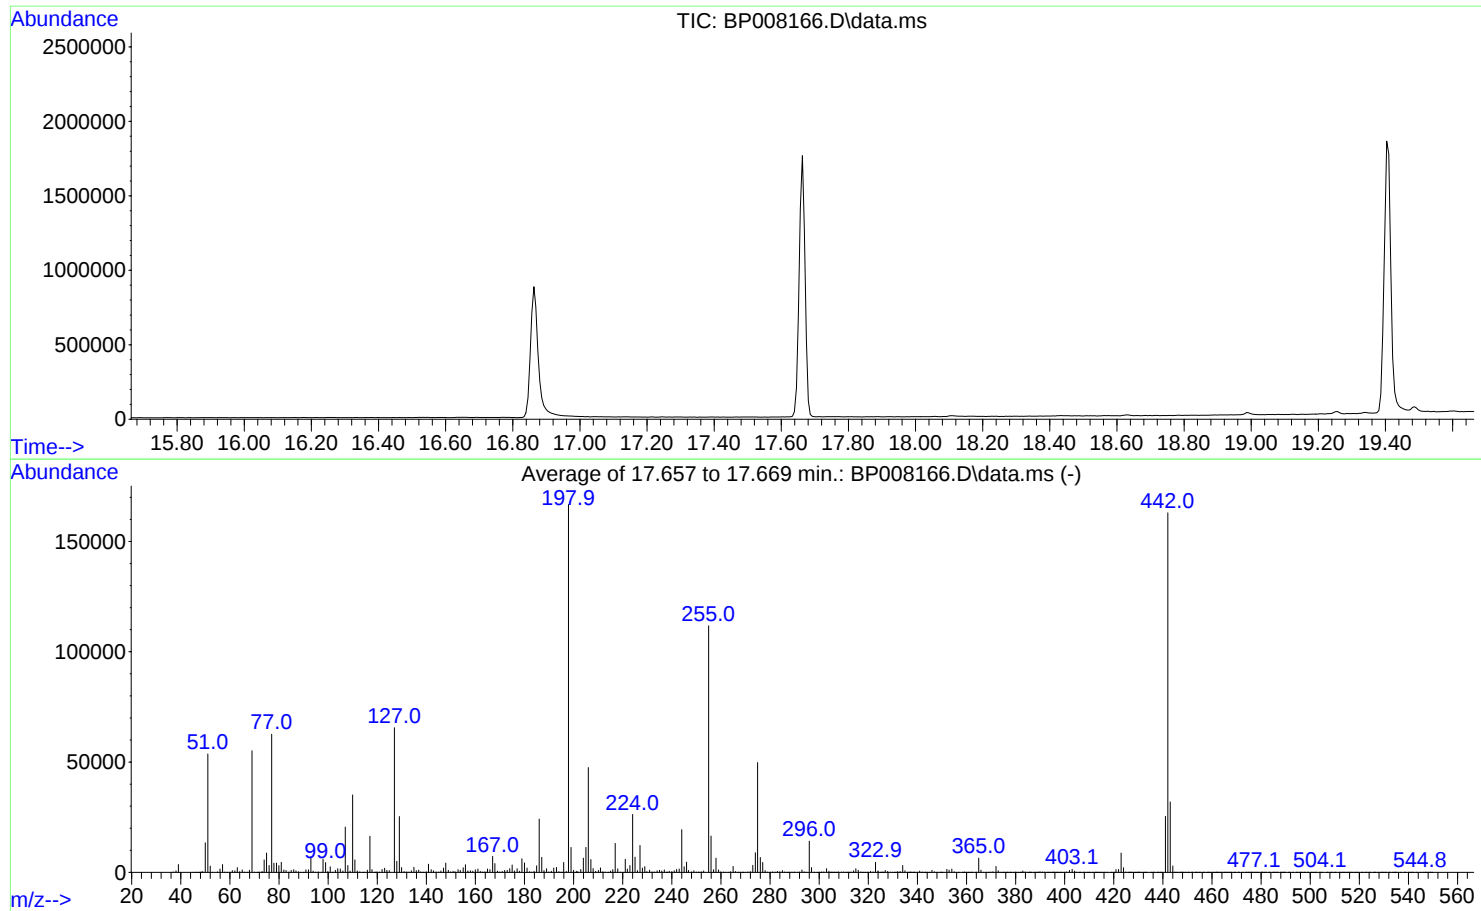




AutoFind: Scans 2494, 2495, 2496; Background Corrected with Scan 2487

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.2	53666	PASS
68	69	0.00	2	1.7	945	PASS
69	198	0.00	100	33.1	55141	PASS
70	69	0.00	2	0.2	127	PASS
127	198	10	80	39.3	65612	PASS
197	198	0.00	2	0.3	476	PASS
198	198	100	100	100.0	166758	PASS
199	198	5	9	6.8	11348	PASS
275	198	10	60	29.9	49795	PASS
365	198	1	100	3.9	6455	PASS
441	198	0.01	100	15.2	25405	PASS
442	442	100	100	100.0	163000	PASS
443	442	15	24	19.6	31909	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120121\
 Data File : BP008166.D
 Acq On : 01 Dec 2021 10:12
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Dec 01 12:02:36 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 25 01:13:46 2021
 Response via : Initial Calibration

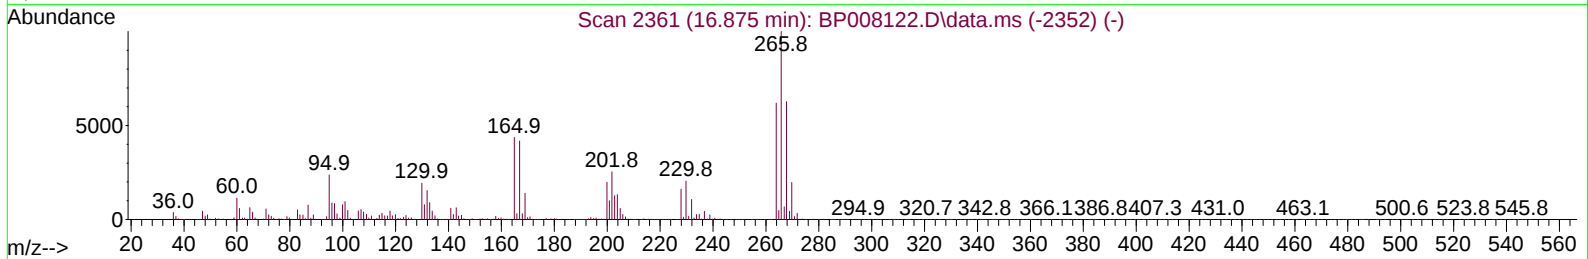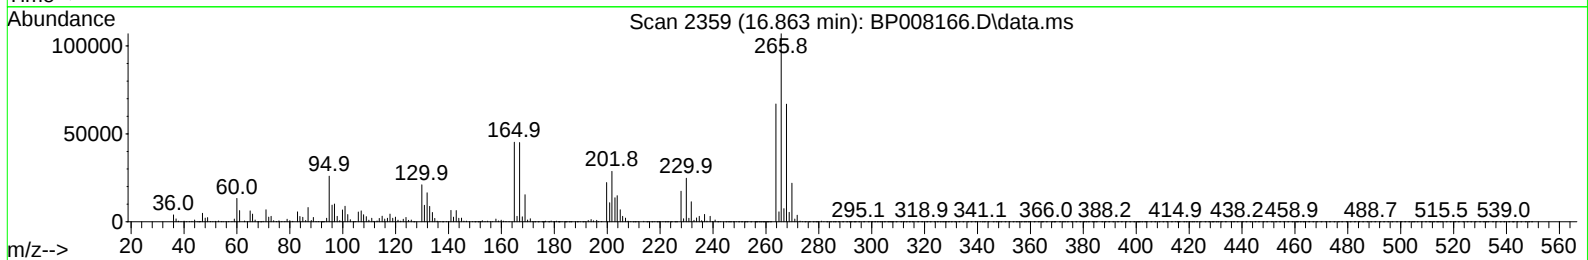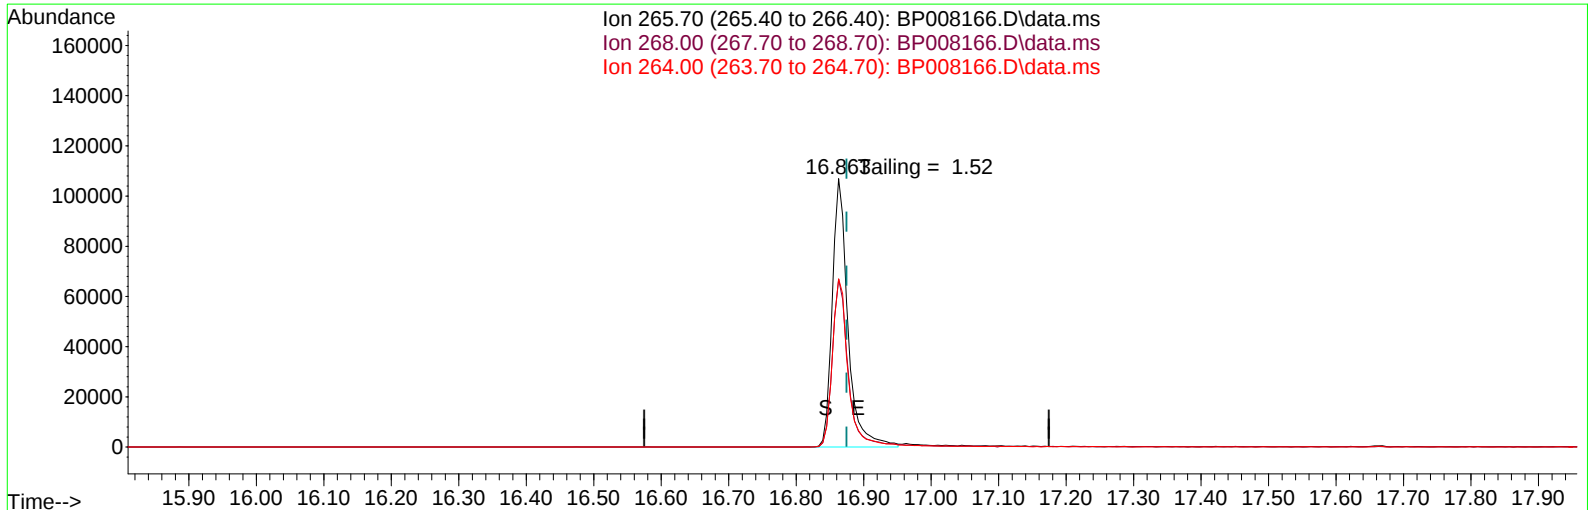

TIC: BP008166.D\data.ms

(70) Pentachlorophenol (C)

16.863min (-0.012) 1165779.04 ng




response 173036

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	62.56
264.00	61.90	62.68
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120121\
Data File : BP008166.D
Acq On : 01 Dec 2021 10:12
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Dec 01 12:02:36 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 25 01:13:46 2021
Response via : Initial Calibration

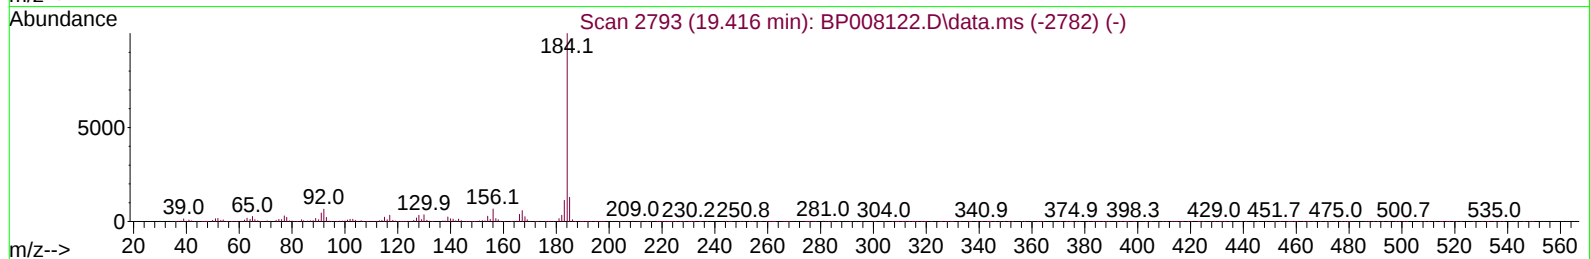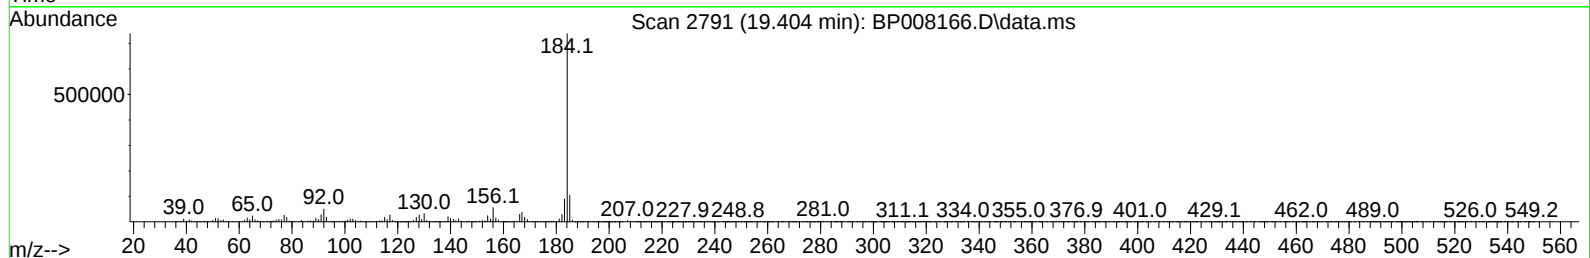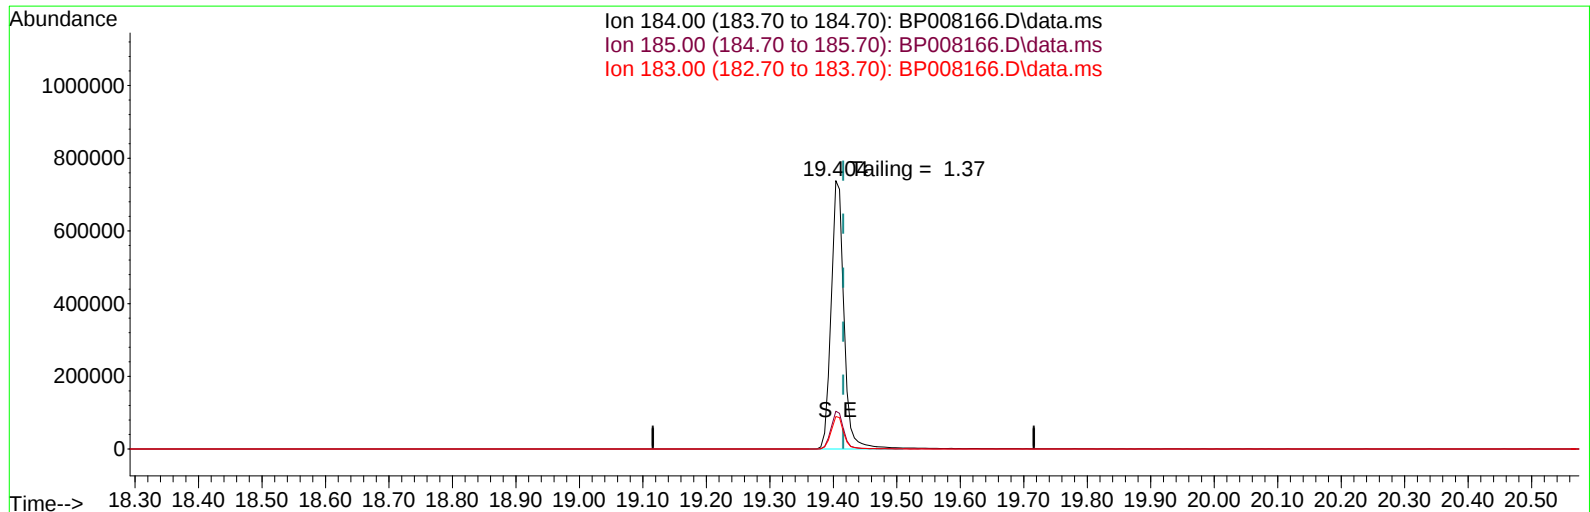

TIC: BP008166.D\data.ms

(77) Benzidine

19.404min (-0.012) 670026.67 ng

response 1047763

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	12.90	14.10
183.00	11.40	12.11
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_P
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
12/1/2021	BNA_P	<u>BP008166.D</u>
Compound Name	Response	Retention Time
DDT	606601	20.61
DDD	3679	20.18
DDE	881	19.69
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4560	611161	0.75