
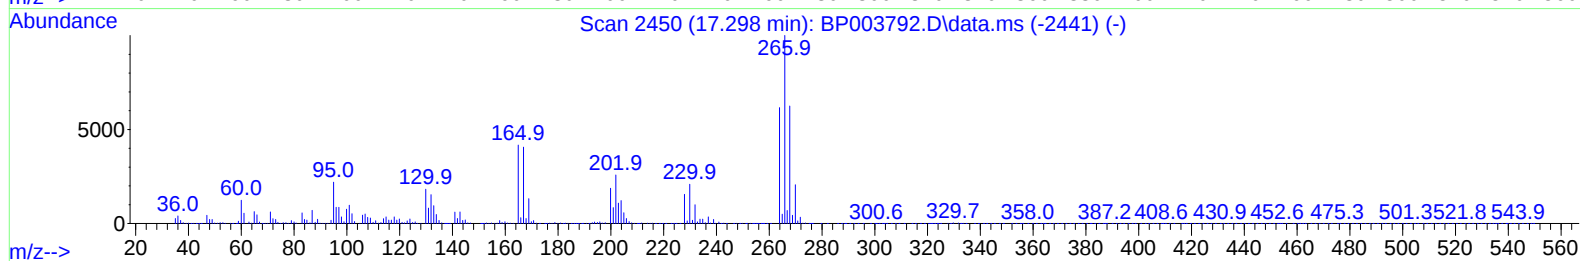
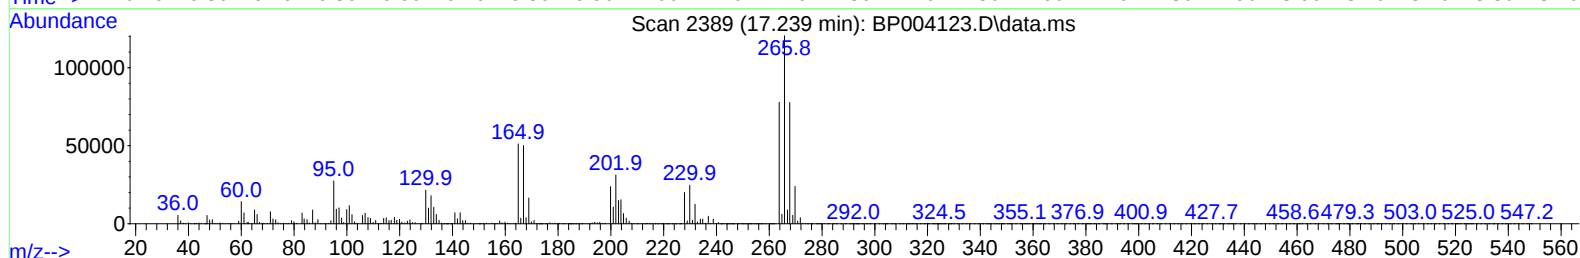


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120220\
 Data File : BP004123.D
 Acq On : 02 Dec 2020 09:50
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 03 00:16:09 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP110320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 02 11:39:42 2020
 Response via : Initial Calibration

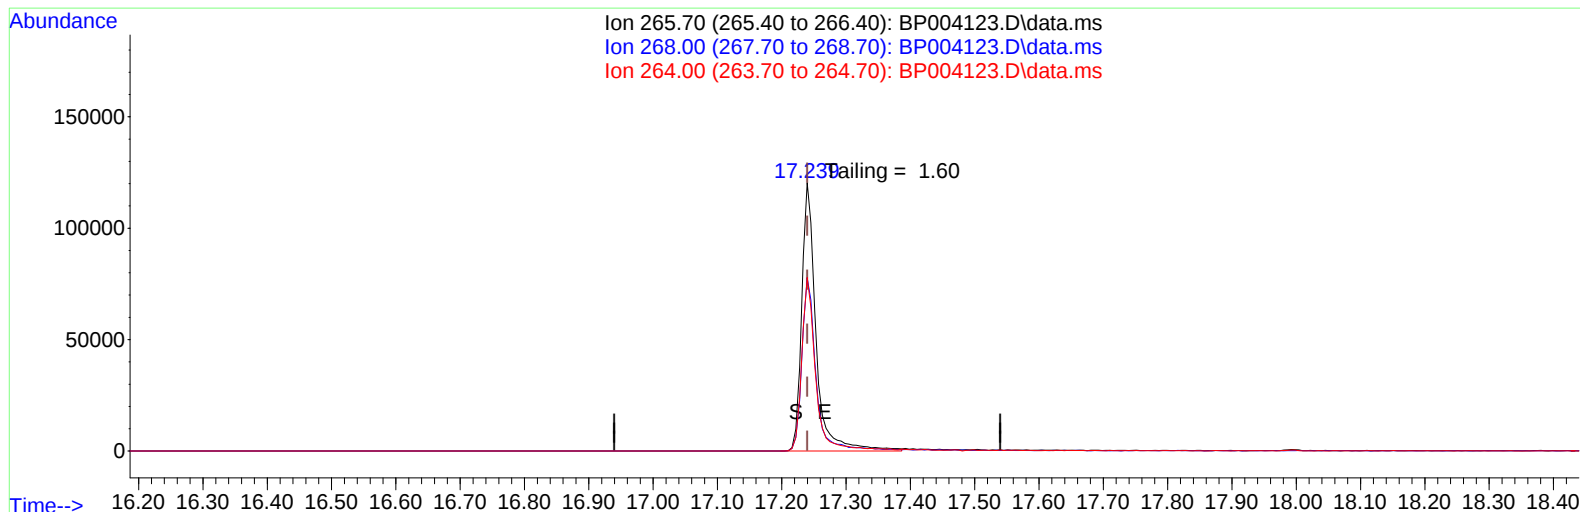

TIC: BP004123.D\data.ms

(70) Pentachlorophenol (C)




17.239min (-0.000) 3304369.87 ng

response 189928

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	64.55
264.00	63.30	64.63
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120220\
 Data File : BP004123.D
 Acq On : 02 Dec 2020 09:50
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 03 00:16:09 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP110320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 02 11:39:42 2020
 Response via : Initial Calibration

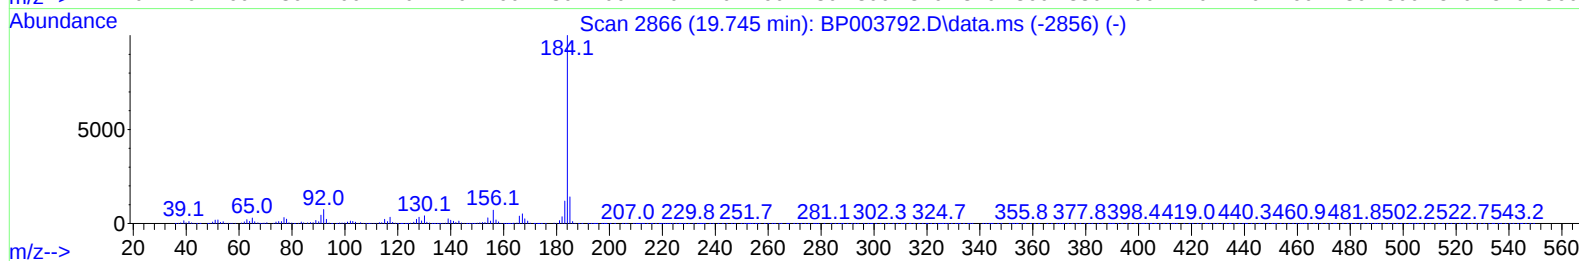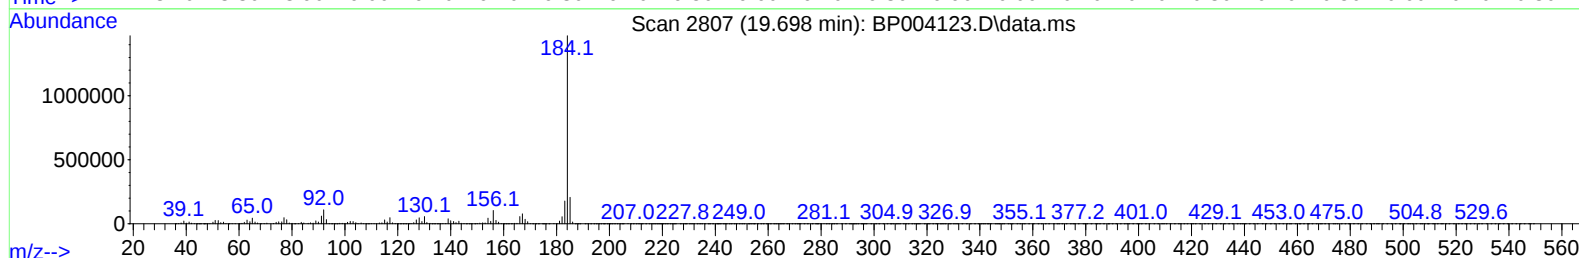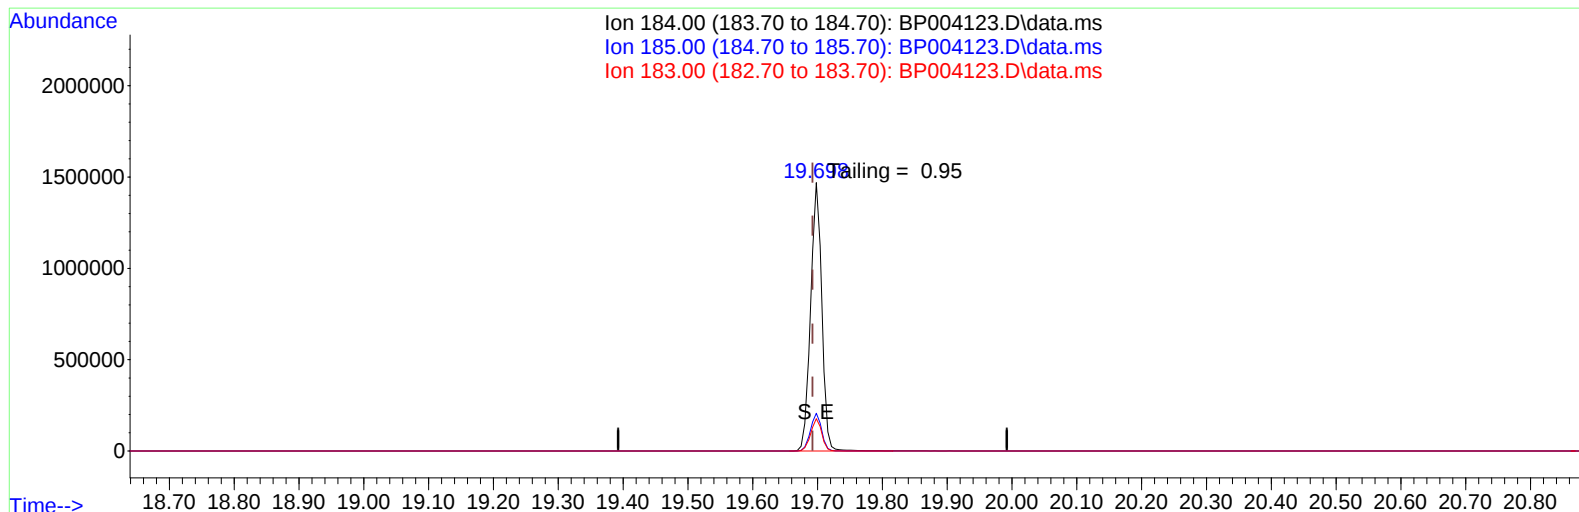

TIC: BP004123.D\data.ms

(77) Benzidine

19.698min (+ 0.006) 2149091.92 ng

response 1774216

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.08
183.00	12.00	12.08
0.00	0.00	0.00