
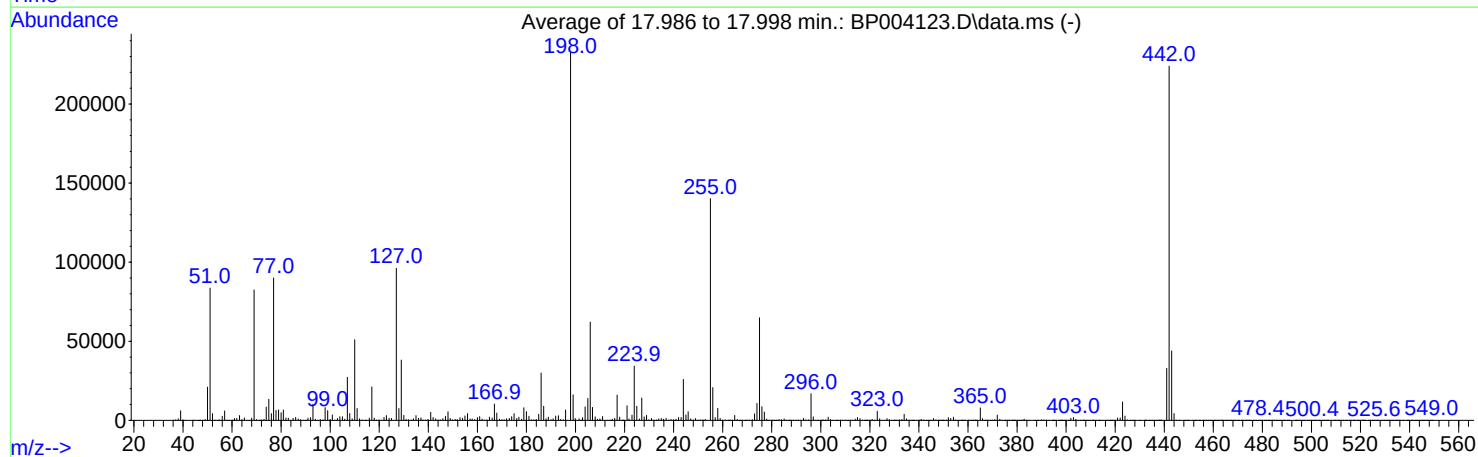


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120220\
 Data File : BP004123.D
 Acq On : 02 Dec 2020 09:50
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP110320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 02 11:39:42 2020

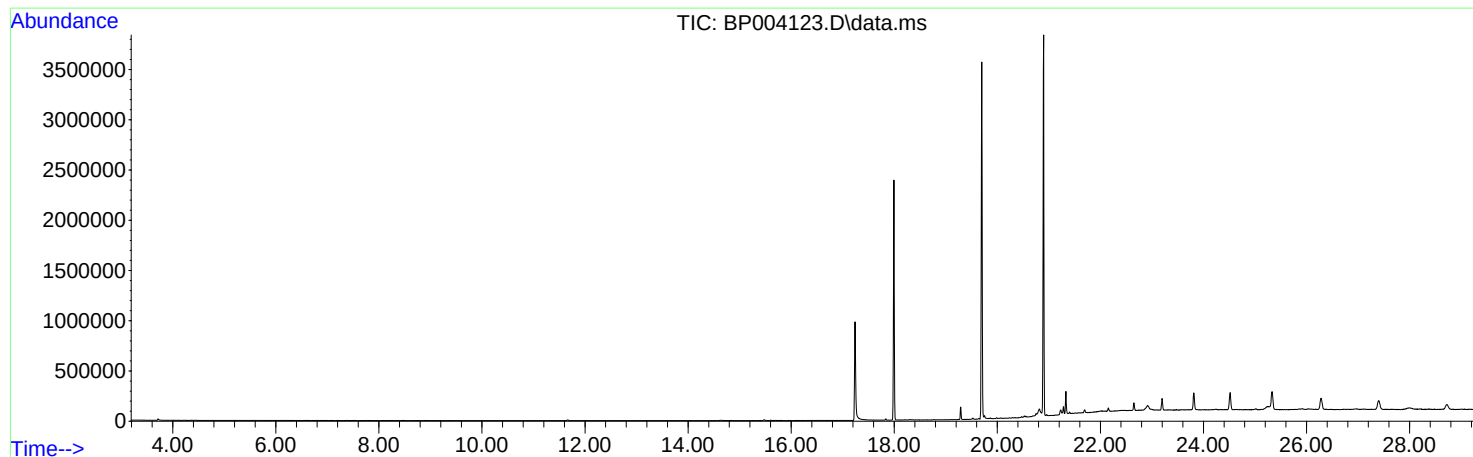

Spectrum Information: Average of 17.986 to 17.998 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.0	83613	PASS
68	69	0.00	2	1.8	1460	PASS
69	198	0.00	100	35.5	82440	PASS
70	69	0.00	2	0.6	479	PASS
127	198	10	80	41.3	96109	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	232533	PASS
199	198	5	9	6.9	16157	PASS
275	198	10	60	27.9	64864	PASS
365	198	1	100	3.4	7903	PASS
441	198	0.01	100	14.1	32863	PASS
442	442	100	100	100.0	223893	PASS
443	442	15	24	19.6	43915	PASS