
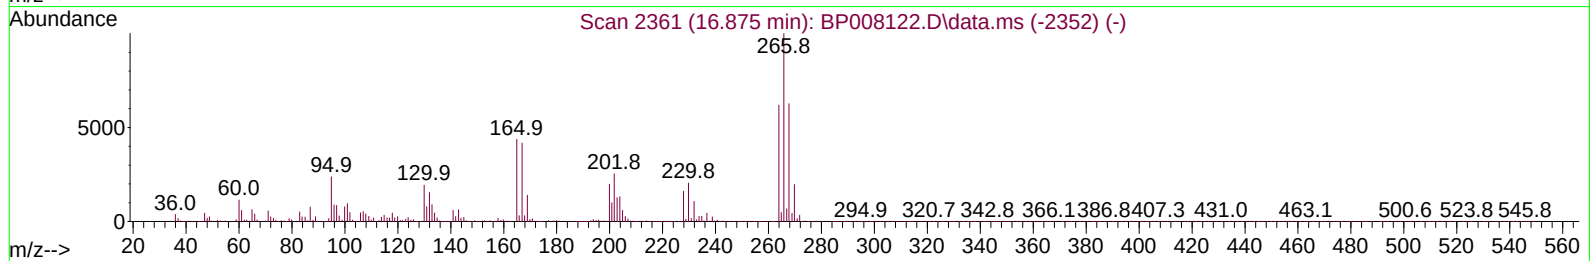
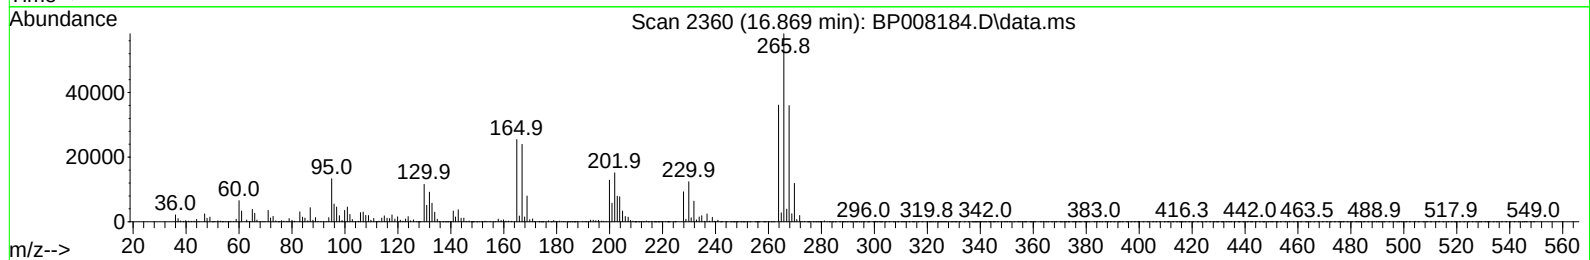


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120221\
 Data File : BP008184.D
 Acq On : 02 Dec 2021 09:58
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 02 11:25:28 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 01 12:06:05 2021
 Response via : Initial Calibration

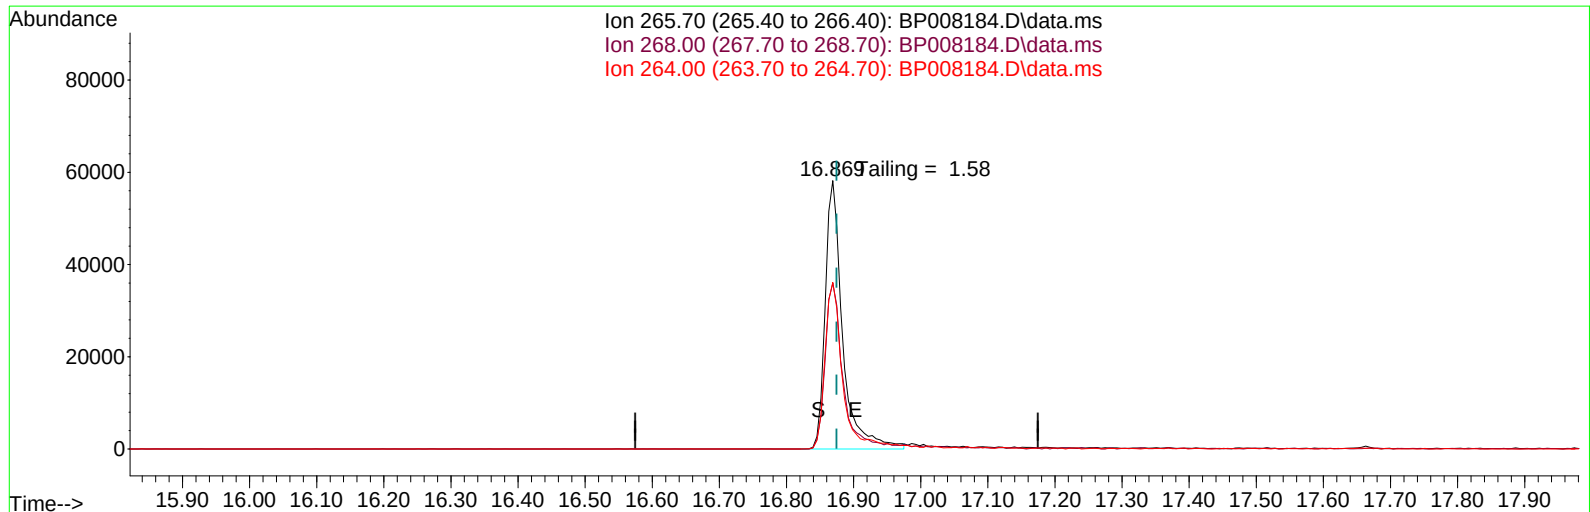

TIC: BP008184.D\data.ms

(70) Pentachlorophenol (C)




16.869min (-0.006) 783247.97 ng

response 105185

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	61.80
264.00	61.90	62.06
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120221\
 Data File : BP008184.D
 Acq On : 02 Dec 2021 09:58
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 02 11:25:28 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 01 12:06:05 2021
 Response via : Initial Calibration

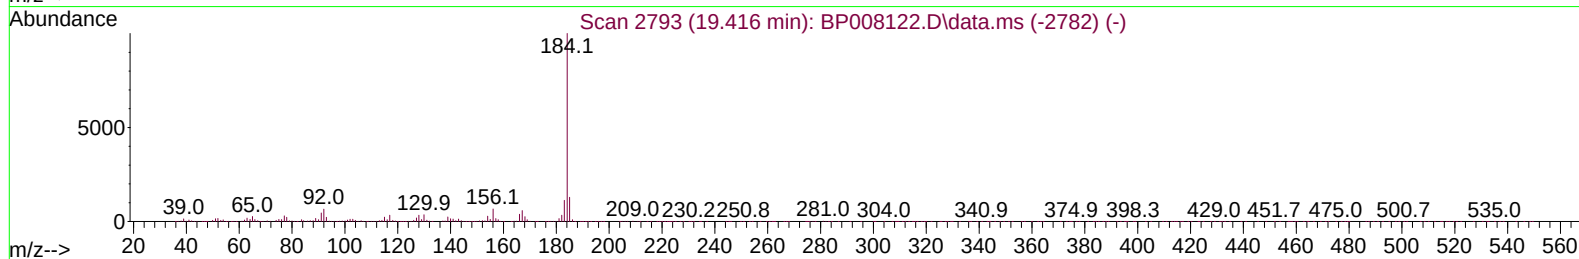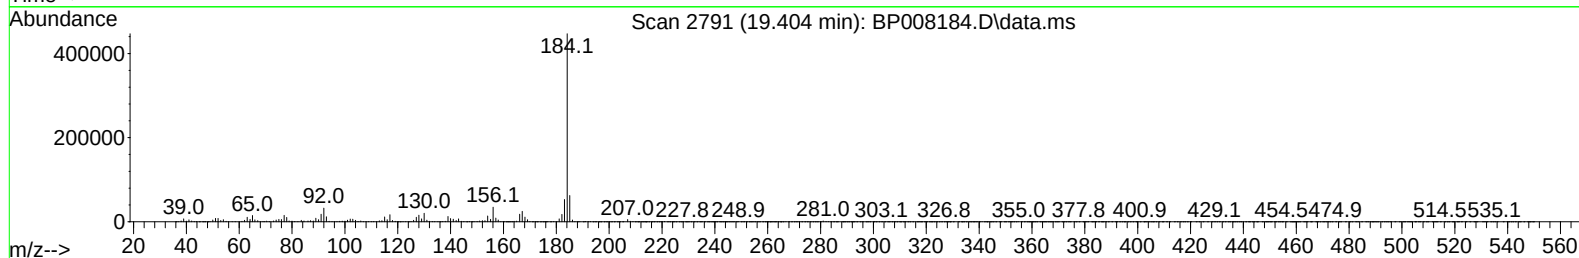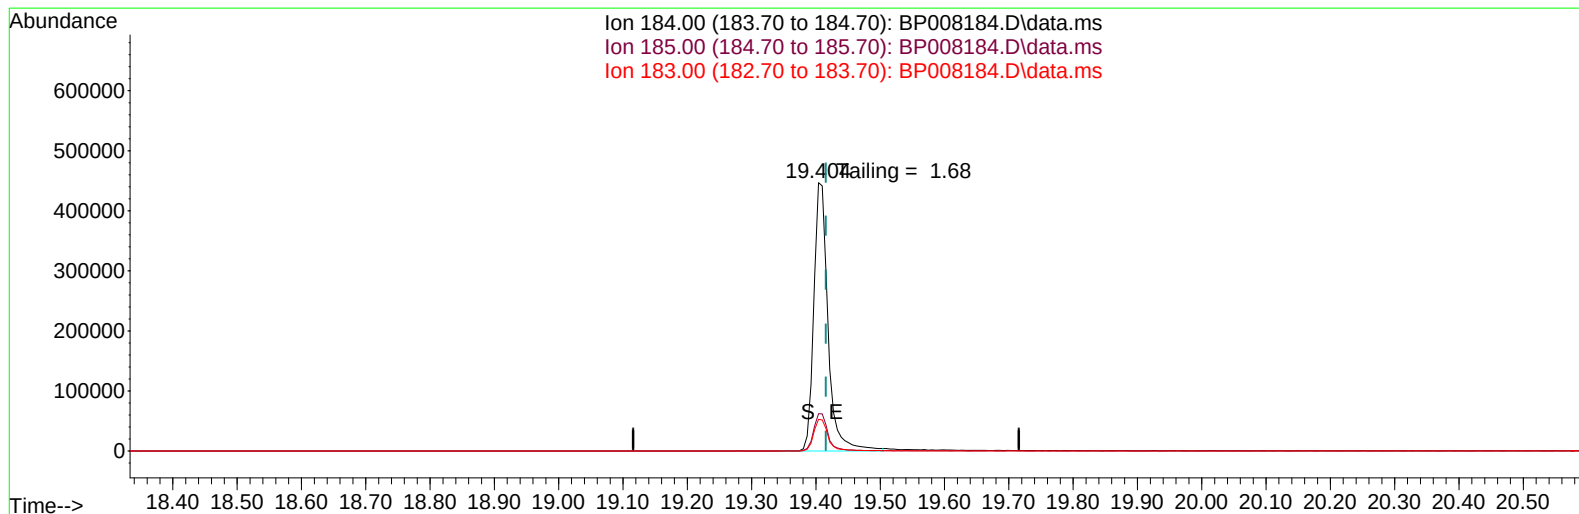

TIC: BP008184.D\data.ms

(77) Benzidine**19.404min (-0.012) 261680.61 ng****response 703548**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	12.90	13.92
183.00	11.40	11.83
0.00	0.00	0.00