


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120221\
 Data File : BP008184.D
 Acq On : 02 Dec 2021 09:58
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 03 14:39:24 2021

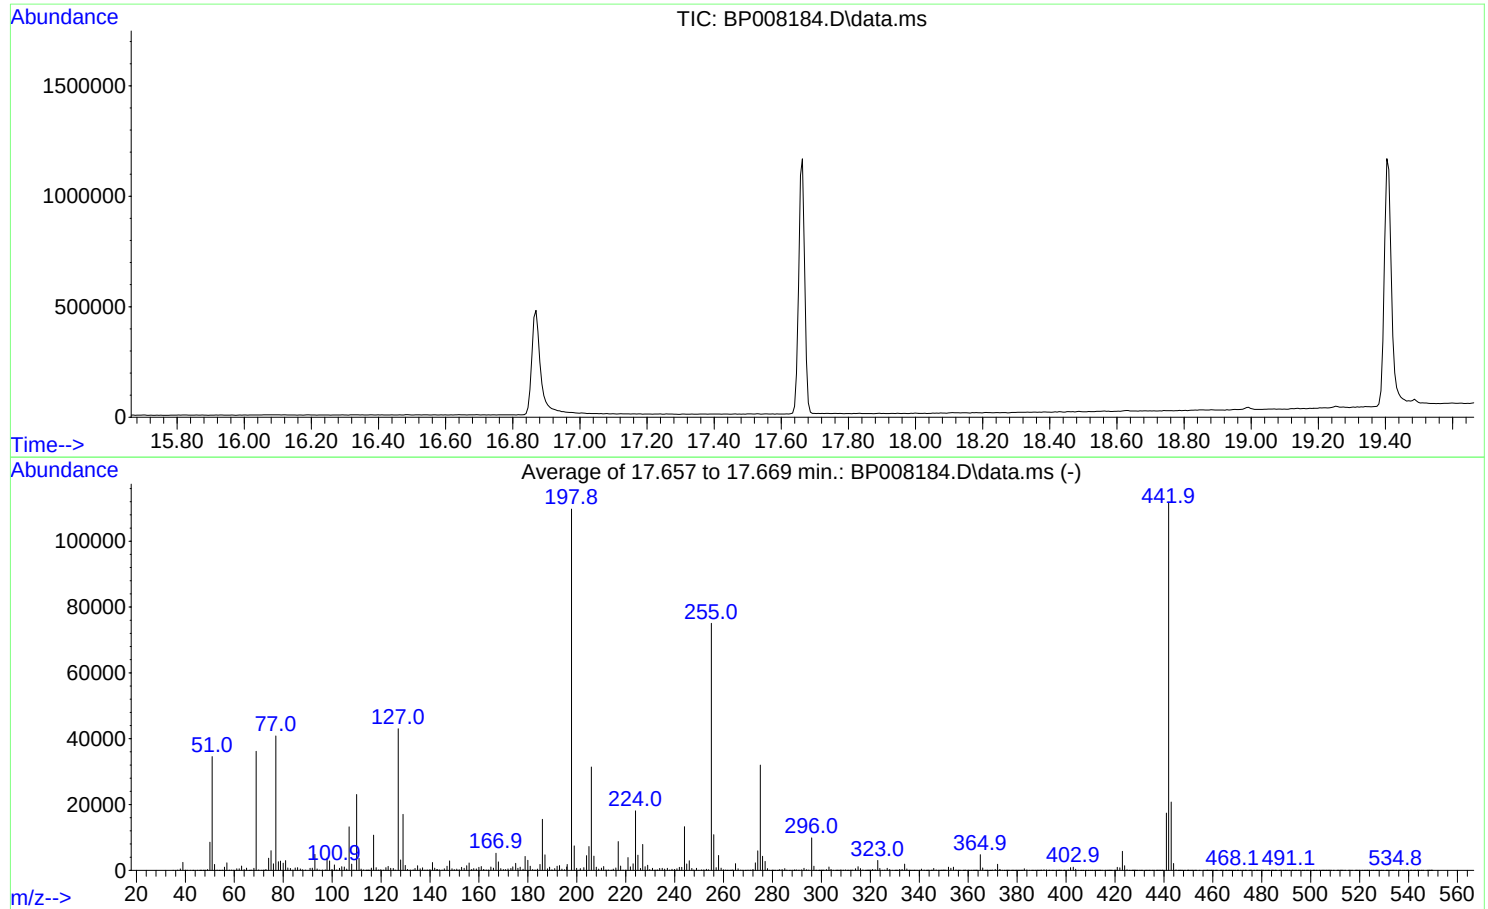




AutoFind: Scans 2494, 2495, 2496; Background Corrected with Scan 2485

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.5	34541	PASS
68	69	0.00	2	1.8	645	PASS
69	198	0.00	100	33.0	36173	PASS
70	69	0.00	2	0.5	171	PASS
127	198	10	80	39.2	43016	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	109770	PASS
199	198	5	9	6.8	7450	PASS
275	198	10	60	29.1	31987	PASS
365	198	1	100	4.3	4753	PASS
441	198	0.01	100	15.9	17399	PASS
442	442	100	100	100.0	111760	PASS
443	442	15	24	18.6	20773	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120221\
Data File : BP008184.D
Acq On : 02 Dec 2021 09:58
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Dec 02 11:25:28 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 01 12:06:05 2021
Response via : Initial Calibration

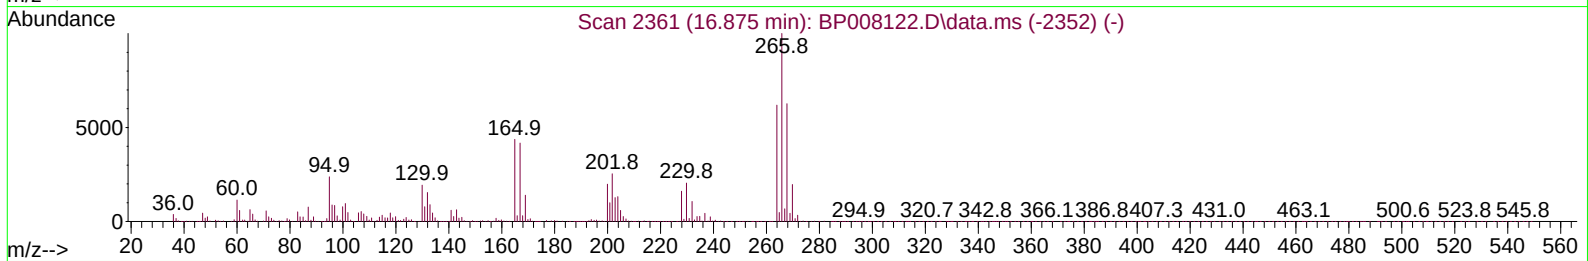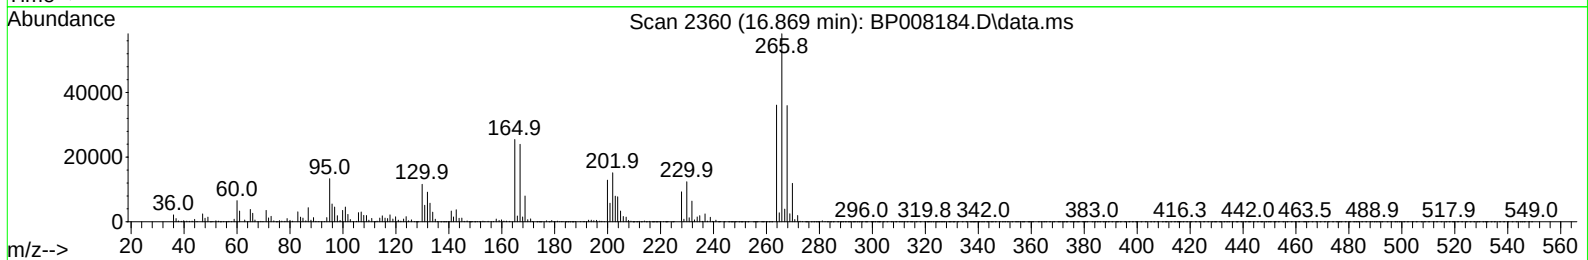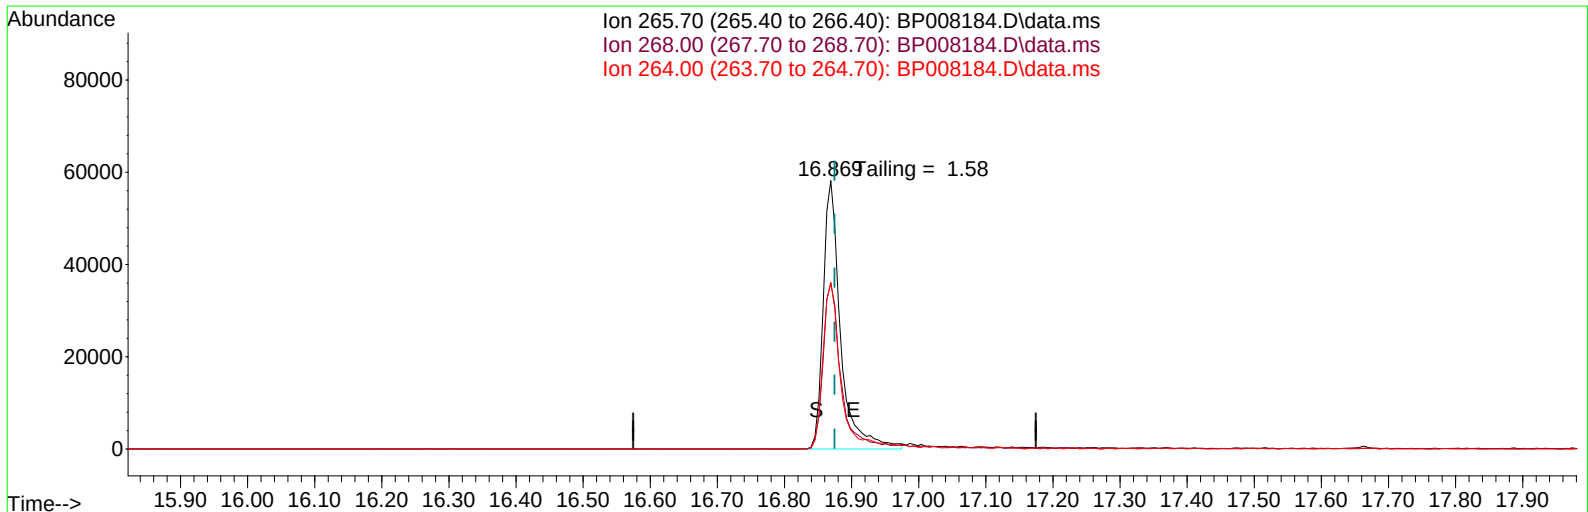

TIC: BP008184.D\data.ms

(70) Pentachlorophenol (C)

16.869min (-0.006) 783247.97 ng




response 105185

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	61.80
264.00	61.90	62.06
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120221\
 Data File : BP008184.D
 Acq On : 02 Dec 2021 09:58
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Dec 02 11:25:28 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 01 12:06:05 2021
 Response via : Initial Calibration

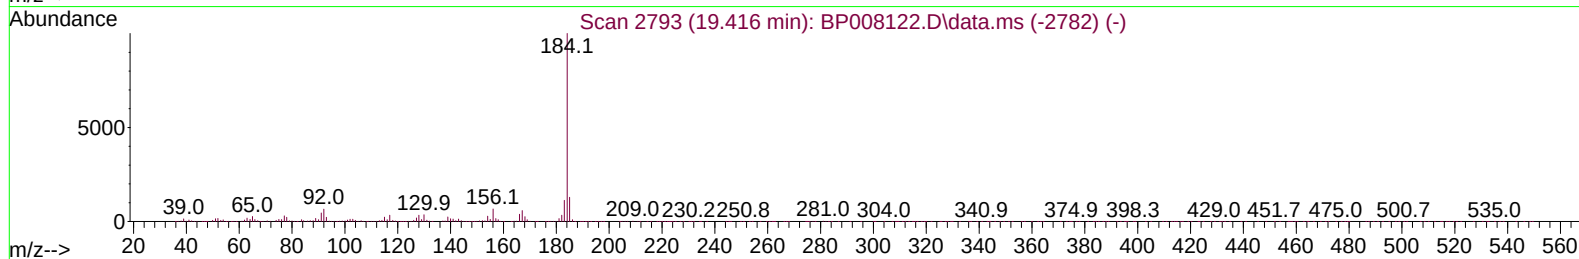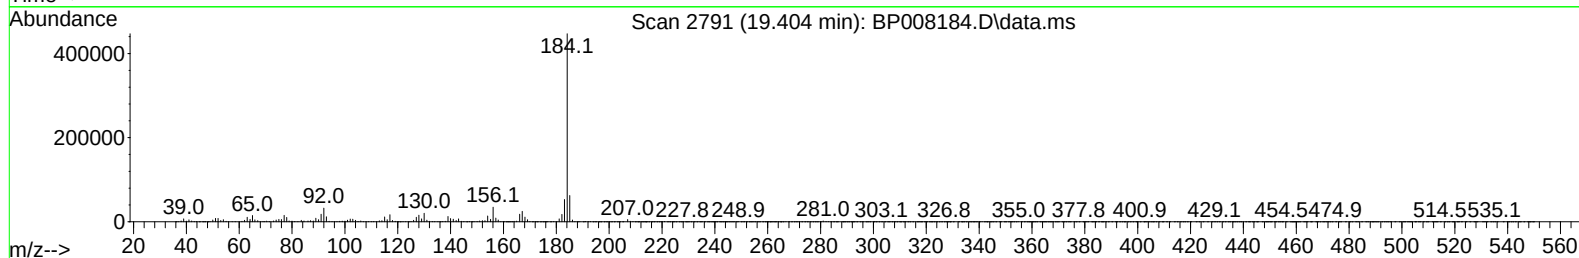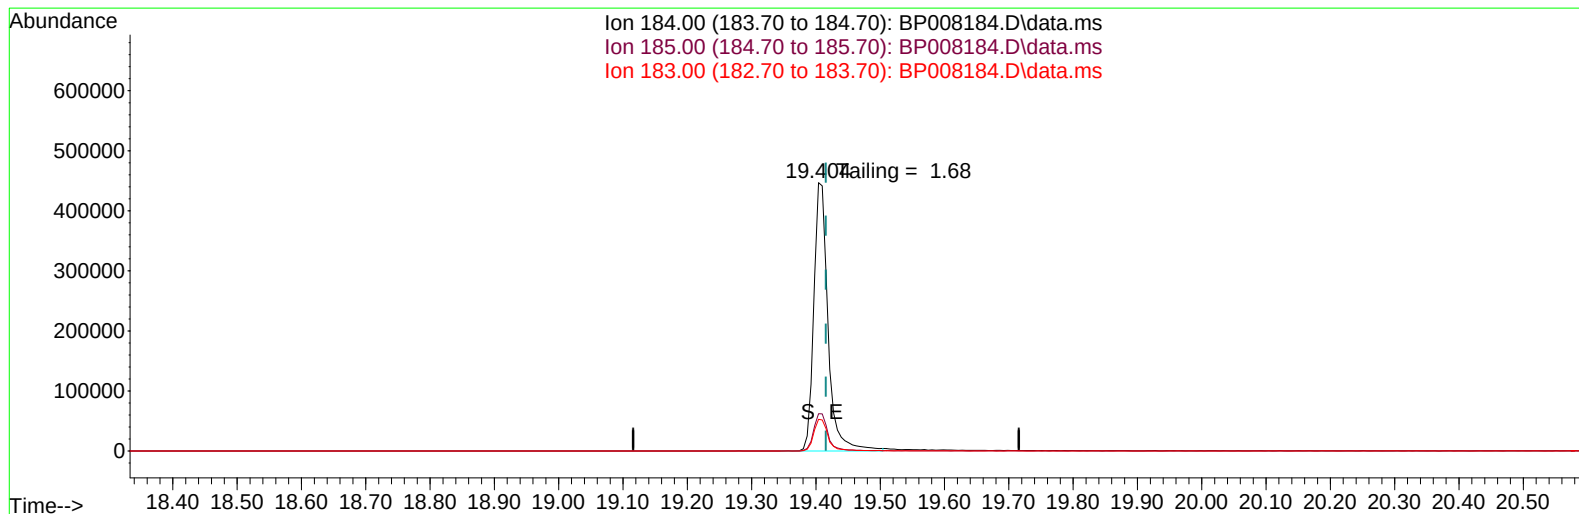

TIC: BP008184.D\data.ms

(77) Benzidine

19.404min (-0.012) 261680.61 ng

response 703548

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	12.90	13.92
183.00	11.40	11.83
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_P
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
12/2/2021	BNA_P	BP008184.D
Compound Name	Response	Retention Time
DDT	397522	20.61
DDD	3118	20.18
DDE	882	19.69
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4000	401522	1.00