

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120222\
 Data File : BP012939.D
 Acq On : 02 Dec 2022 14:52
 Operator : CG/JU
 Sample : N5738-21
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBNK0

Quant Time: Dec 03 01:30:11 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 01 23:46:27 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.005	152	315962	20.000	ng/ul	0.00
20) Naphthalene-d8	10.822	136	1690603	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.639	164	1332313	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.398	188	3119030	20.000	ng/ul	0.00
79) Chrysene-d12	21.480	240	3450474	20.000	ng/ul	0.00
88) Perylene-d12	23.992	264	3751333	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.387	96	35678	5.025	ng/uL	0.00
4) Pyridine-d5	3.822	84	179316	7.825	ng/ul	0.00
7) Phenol-d5	7.158	99	876551	30.041	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.328	67	484512	29.330	ng/ul	0.00
11) 2-Chlorophenol-d4	7.534	132	667017	31.189	ng/ul	0.00
15) 4-Methylphenol-d8	8.710	113	681756	28.456	ng/ul	0.00
21) Nitrobenzene-d5	9.169	128	359806	29.928	ng/ul	0.00
24) 2-Nitrophenol-d4	9.899	143	425272	30.909	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.434	165	838003	30.424	ng/ul	0.00
31) 4-Chloroaniline-d4	10.957	131	866331	22.261	ng/ul	0.00
46) Dimethylphthalate-d6	14.045	166	2918128	30.368	ng/ul	0.00
49) Acenaphthylene-d8	14.334	160	3270266	30.823	ng/ul	0.00
54) 4-Nitrophenol-d4	14.828	143	497406	25.307	ng/ul	0.00
60) Fluorene-d10	15.634	176	2649407	31.368	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.745	200	436622	23.860	ng/ul	0.00
73) Anthracene-d10	17.498	188	4325410	31.374	ng/ul	0.00
81) Pyrene-d10	19.722	212	5347660	31.530	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.827	264	5776578	31.516	ng/ul	0.00
Target Compounds						
8) Phenol	7.187	94	37266	1.230	ng/ul	95
16) Acetophenone	8.834	105	135682	3.656	ng/ul	99
71) Pentachlorophenol	17.039	266	195434	7.824	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120222\
Data File : BP012939.D
Acq On : 02 Dec 2022 14:52
Operator : CG/JU
Sample : N5738-21
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBNK0

Quant Time: Dec 03 01:30:11 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120122.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 01 23:46:27 2022
Response via : Initial Calibration




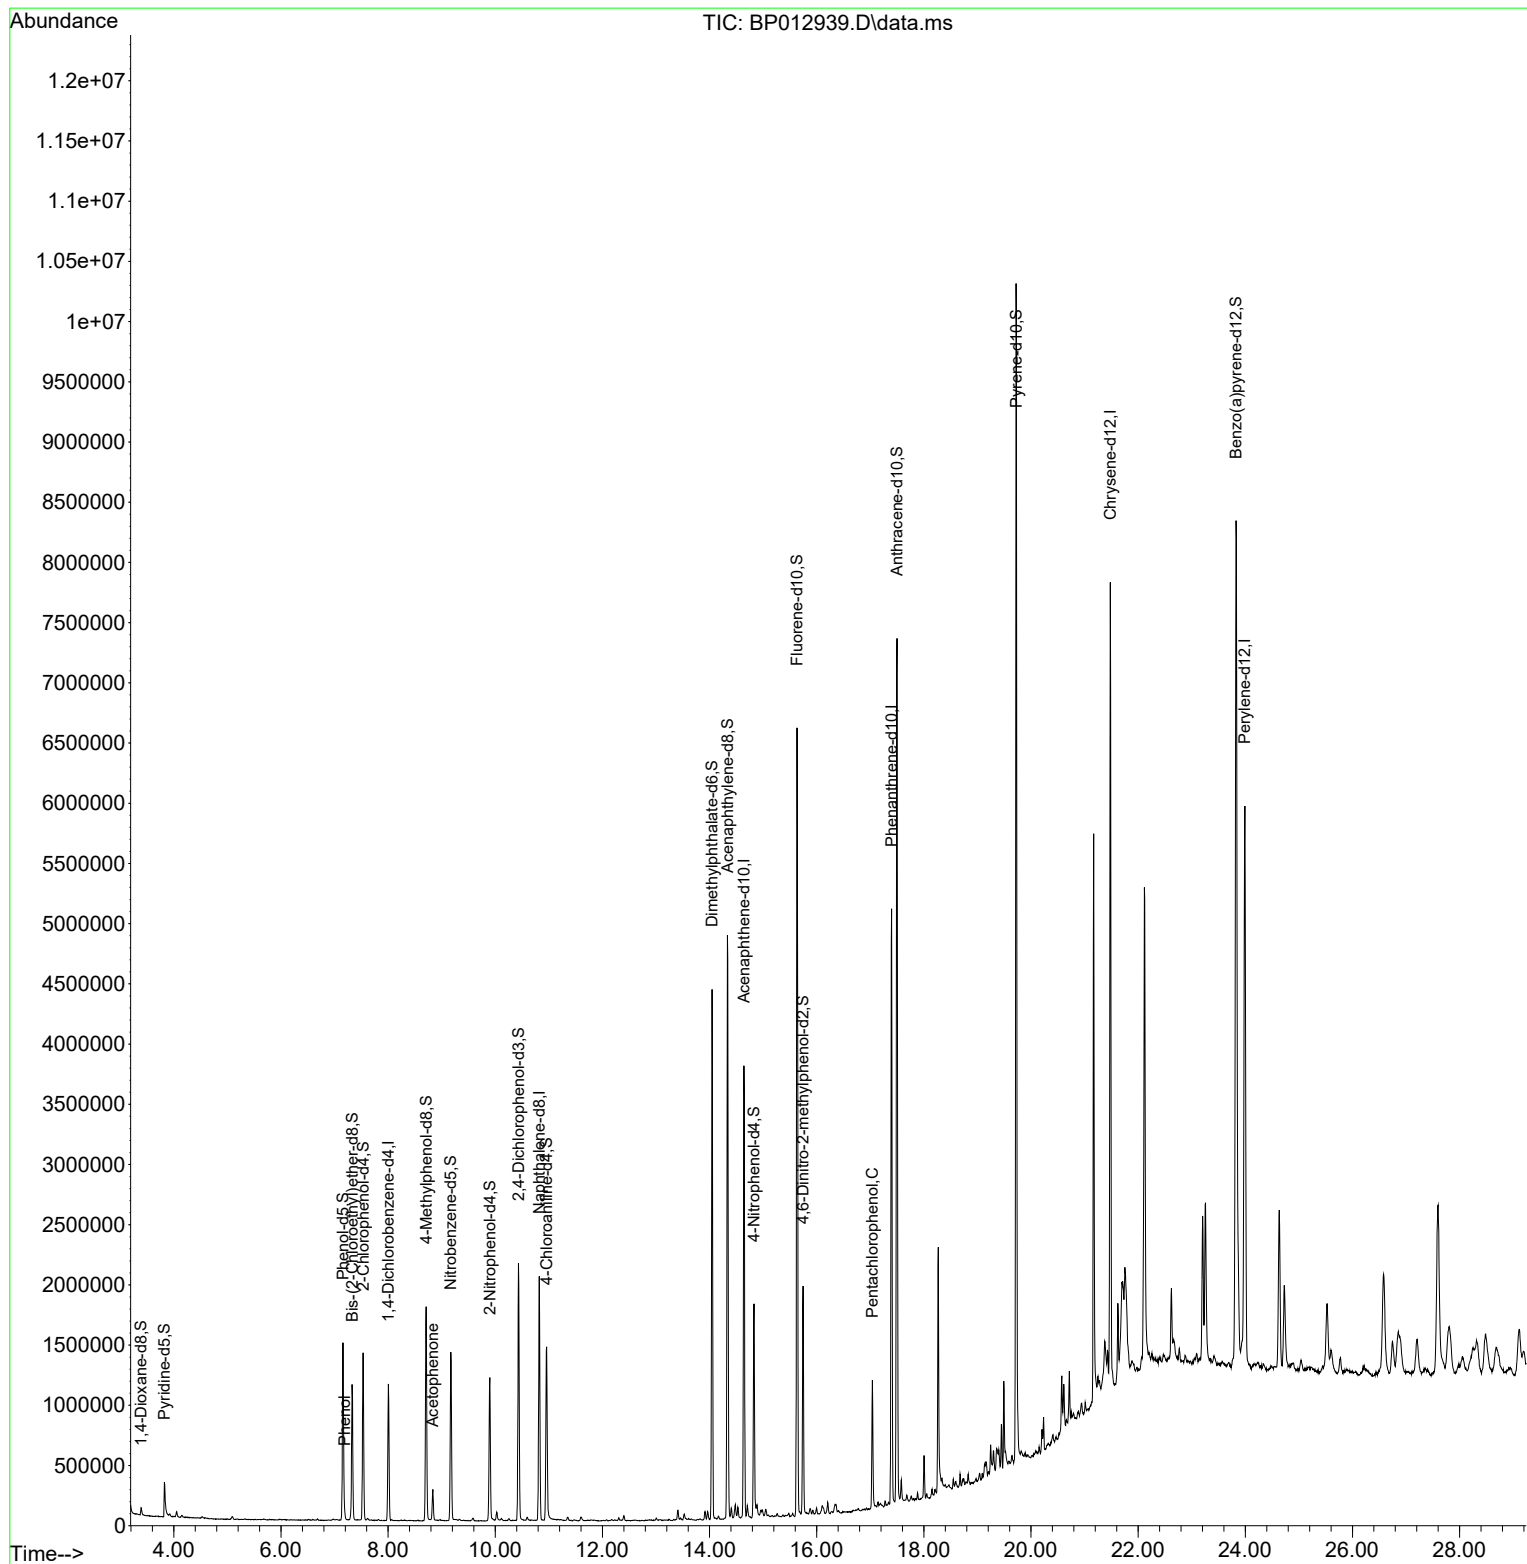


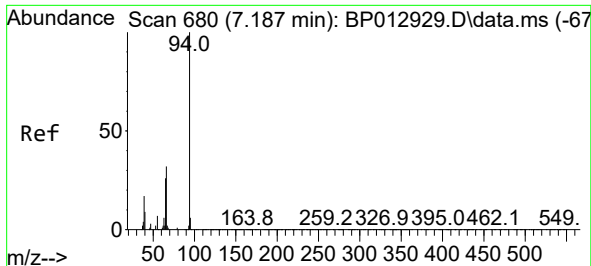

#8
Phenol
Concen: 1.230 ng/ul
RT: 7.187 min Scan# 61
Delta R.T. 0.000 min
Lab File: BP012939.D
Acq: 02 Dec 2022 14:52




Instrument :
BNA_P
ClientSampleId :
GBNK0


Tgt Ion: 94 Resp: 37266
Ion Ratio Lower Upper
94 100
65 27.3 21.8 32.6
66 38.1 26.6 39.8

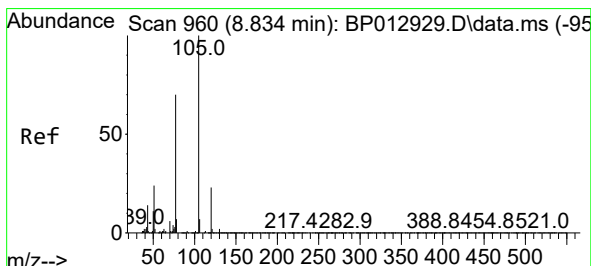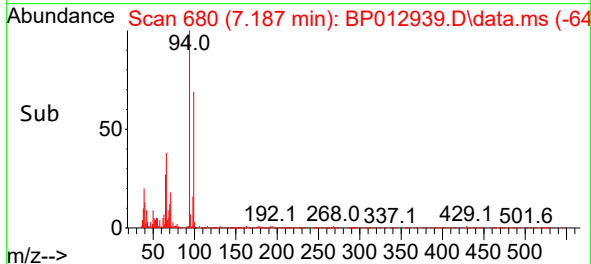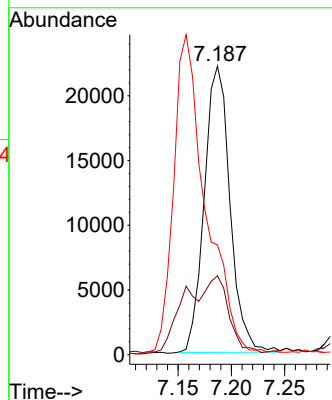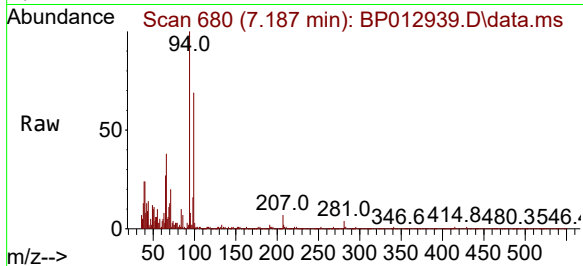

#16
Acetophenone
Concen: 3.656 ng/ul
RT: 8.834 min Scan# 960
Delta R.T. 0.000 min
Lab File: BP012939.D
Acq: 02 Dec 2022 14:52

Tgt Ion: 105 Resp: 135682
Ion Ratio Lower Upper
105 100
77 74.8 60.4 90.6
51 26.1 20.7 31.1

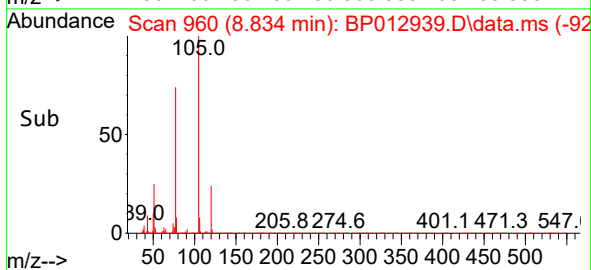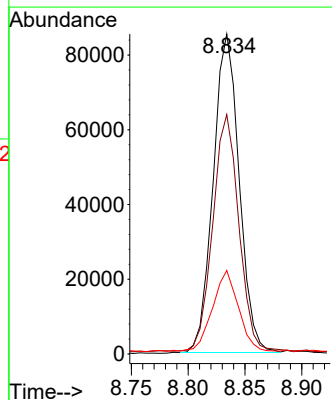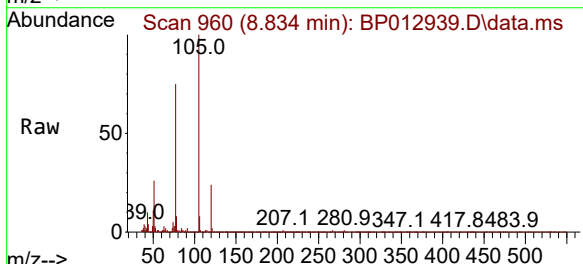

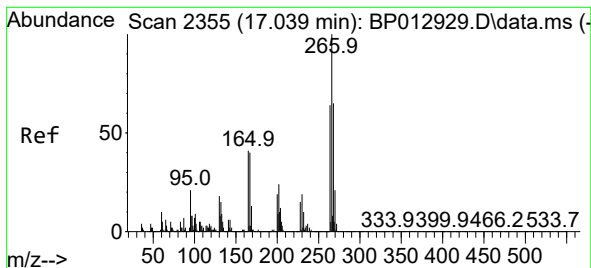

#71

Pentachlorophenol

Concen: 7.824 ng/ul

RT: 17.039 min Scan# 21

Delta R.T. 0.000 min

Lab File: BP012939.D


Acq: 02 Dec 2022 14:52

Instrument :

BNA_P

ClientSampleId :

GBNK0

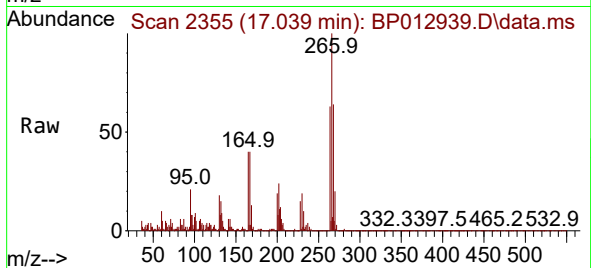

Tgt Ion:266 Resp: 195434

Ion Ratio Lower Upper

266 100

264 63.0 50.5 75.7

268 64.0 51.2 76.8

