
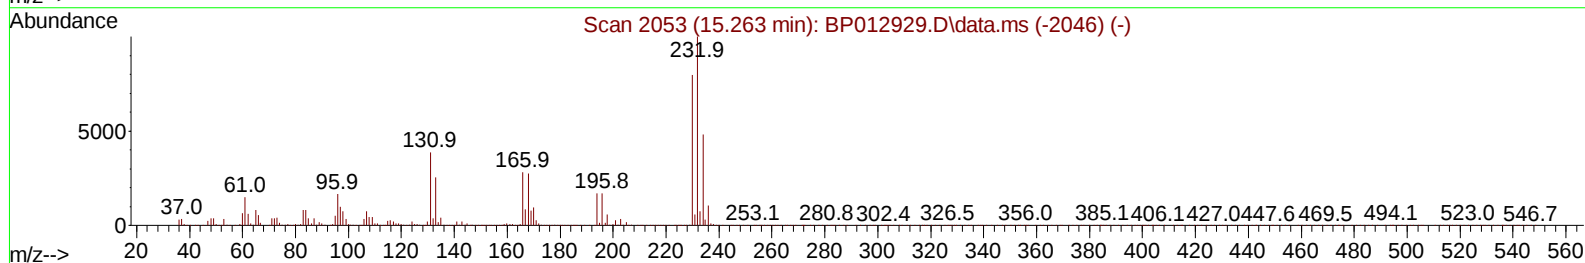
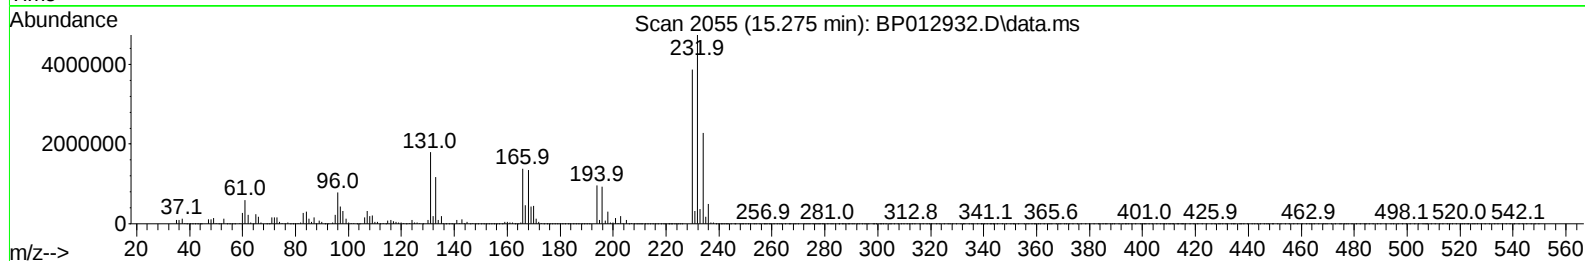


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120222\
Data File : BP012932.D
Acq On : 02 Dec 2022 10:54
Operator : CG/JU
Sample : N5738-15
Misc :
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Dec 03 01:28:40 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120122.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 01 23:46:27 2022
Response via : Initial Calibration

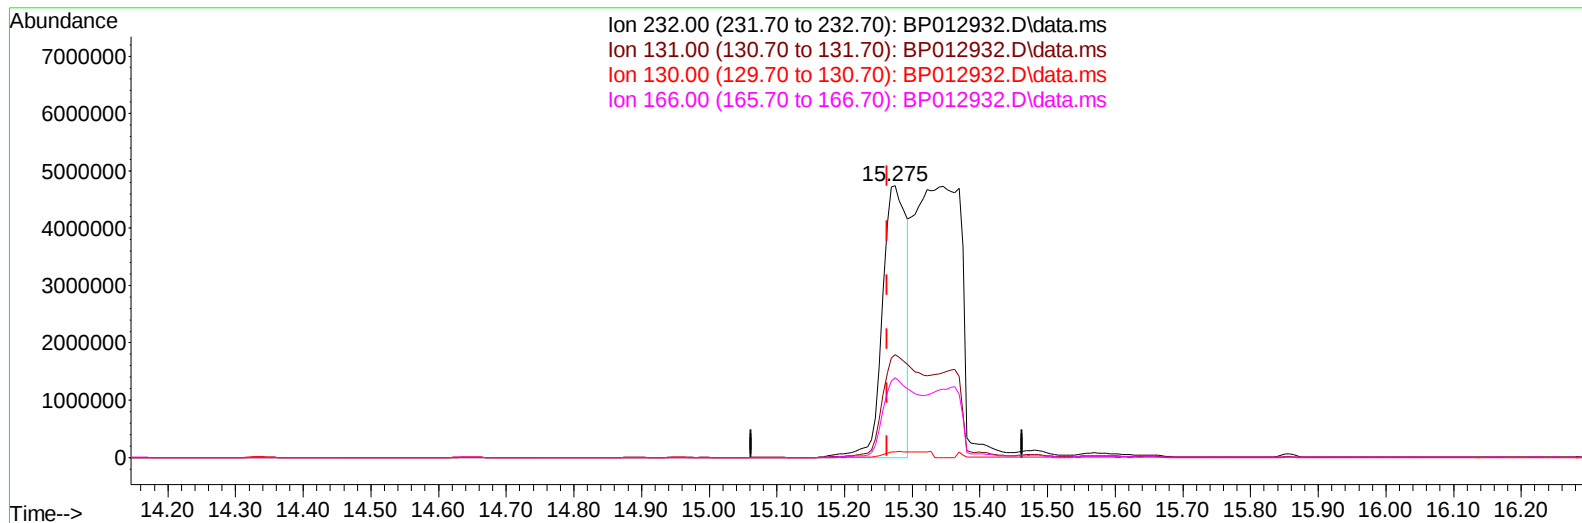

TIC: BP012932.D\data.ms

(58) 2,3,4,6-Tetrachlorophenol




15.275min (+ 0.012) 274.30 ng/u1

response 11643501

Ion	Exp%	Act%
232.00	100.00	100.00
131.00	38.80	37.92
130.00	2.20	2.15
166.00	28.10	29.26

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120222\
Data File : BP012932.D
Acq On : 02 Dec 2022 10:54
Operator : CG/JU
Sample : N5738-15
Misc :
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Dec 03 01:28:40 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120122.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 01 23:46:27 2022
Response via : Initial Calibration

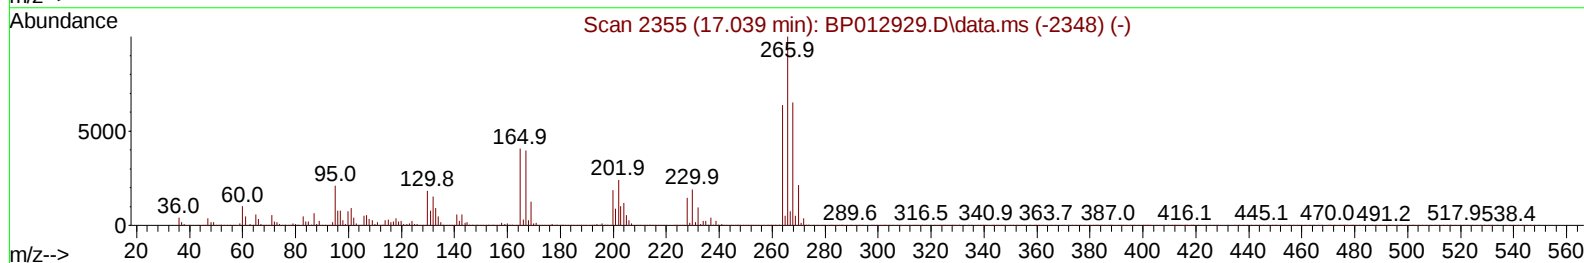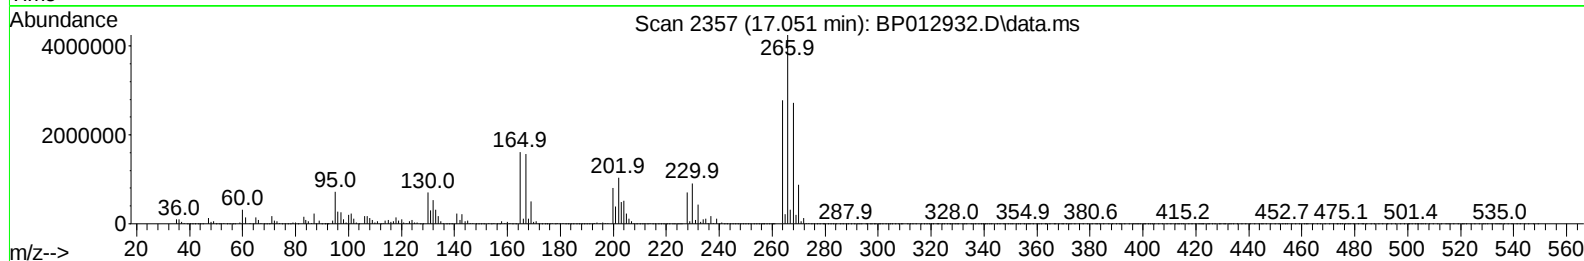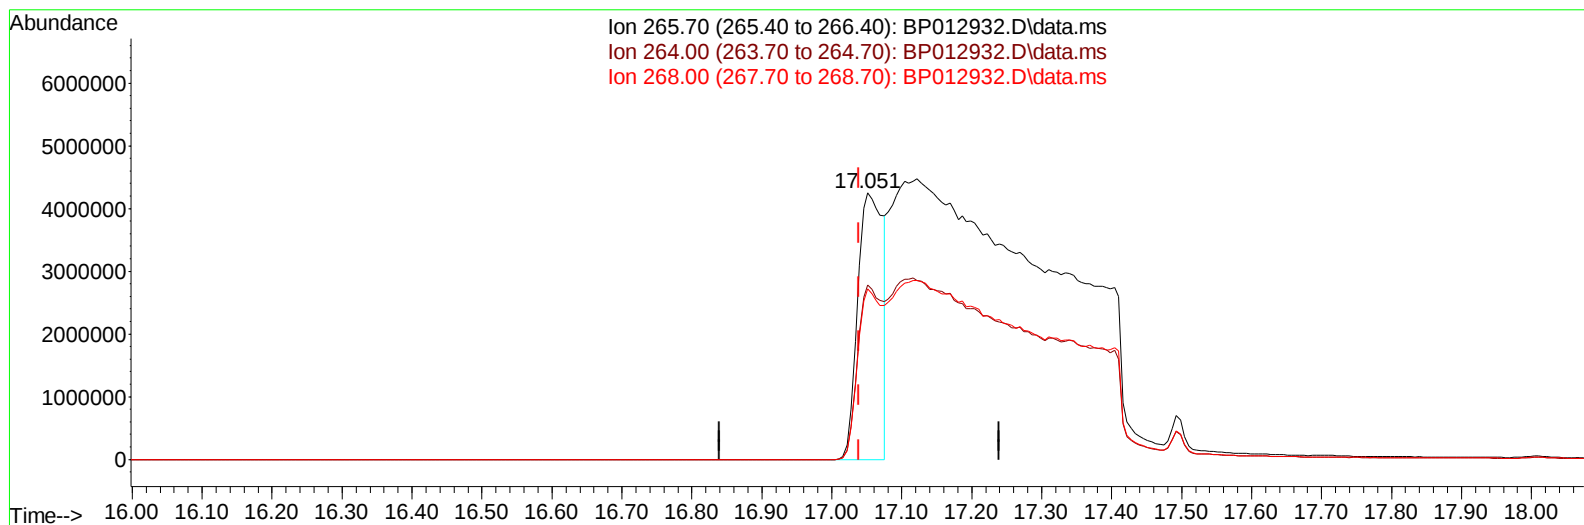

TIC: BP012932.D\data.ms

(71) Pentachlorophenol (C)

17.051min (+ 0.012) 389.39 ng/u1

response 10676041

Ion	Exp%	Act%
265.70	100.00	100.00
264.00	63.10	65.49
268.00	64.00	63.95
0.00	0.00	0.00