

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120222\
 Data File : BP012944.D
 Acq On : 02 Dec 2022 17:43
 Operator : CG/JU
 Sample : N5785-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COL70

Quant Time: Dec 03 01:31:12 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 01 23:46:27 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.005	152	304642	20.000	ng/u1	0.00
20) Naphthalene-d8	10.822	136	1602087	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.640	164	1290038	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.398	188	3127685	20.000	ng/u1	0.00
79) Chrysene-d12	21.480	240	3547720	20.000	ng/u1	0.00
88) Perylene-d12	23.986	264	3473655	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	24778	3.619	ng/uL	0.00
4) Pyridine-d5	3.828	84	198346	8.978	ng/u1	0.01
7) Phenol-d5	7.158	99	15034	0.534	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.328	67	386565	24.270	ng/u1	0.00
11) 2-Chlorophenol-d4	7.534	132	46437	2.252	ng/u1	0.00
15) 4-Methylphenol-d8	8.710	113	28595	1.238	ng/u1	0.00
21) Nitrobenzene-d5	9.175	128	268591	23.575	ng/u1	0.00
24) 2-Nitrophenol-d4	9.899	143	21633	1.659	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.434	165	65645	2.515	ng/u1	0.00
31) 4-Chloroaniline-d4	10.957	131	625623	16.964	ng/u1	0.00
46) Dimethylphthalate-d6	14.045	166	2546652	27.370	ng/u1	0.00
49) Acenaphthylene-d8	14.334	160	2594972	25.260	ng/u1	0.00
54) 4-Nitrophenol-d4	14.840	143	530	0.028	ng/u1	0.01
60) Fluorene-d10	15.634	176	2316873	28.330	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.763	200	832	0.045	ng/u1	0.02
73) Anthracene-d10	17.498	188	4415939	31.942	ng/u1	0.00
81) Pyrene-d10	19.722	212	5427973	31.126	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.827	264	5422849	31.951	ng/u1	0.00
Target Compounds						
					Qvalue	
22) Nitrobenzene	9.216	77	163449	5.948	ng/u1	99
75) 1,2,3,4-Tetrachloroben...	13.440	216	272371	6.537	ng/uL	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120222\
Data File : BP012944.D
Acq On : 02 Dec 2022 17:43
Operator : CG/JU
Sample : N5785-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COL70

Quant Time: Dec 03 01:31:12 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120122.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 01 23:46:27 2022
Response via : Initial Calibration




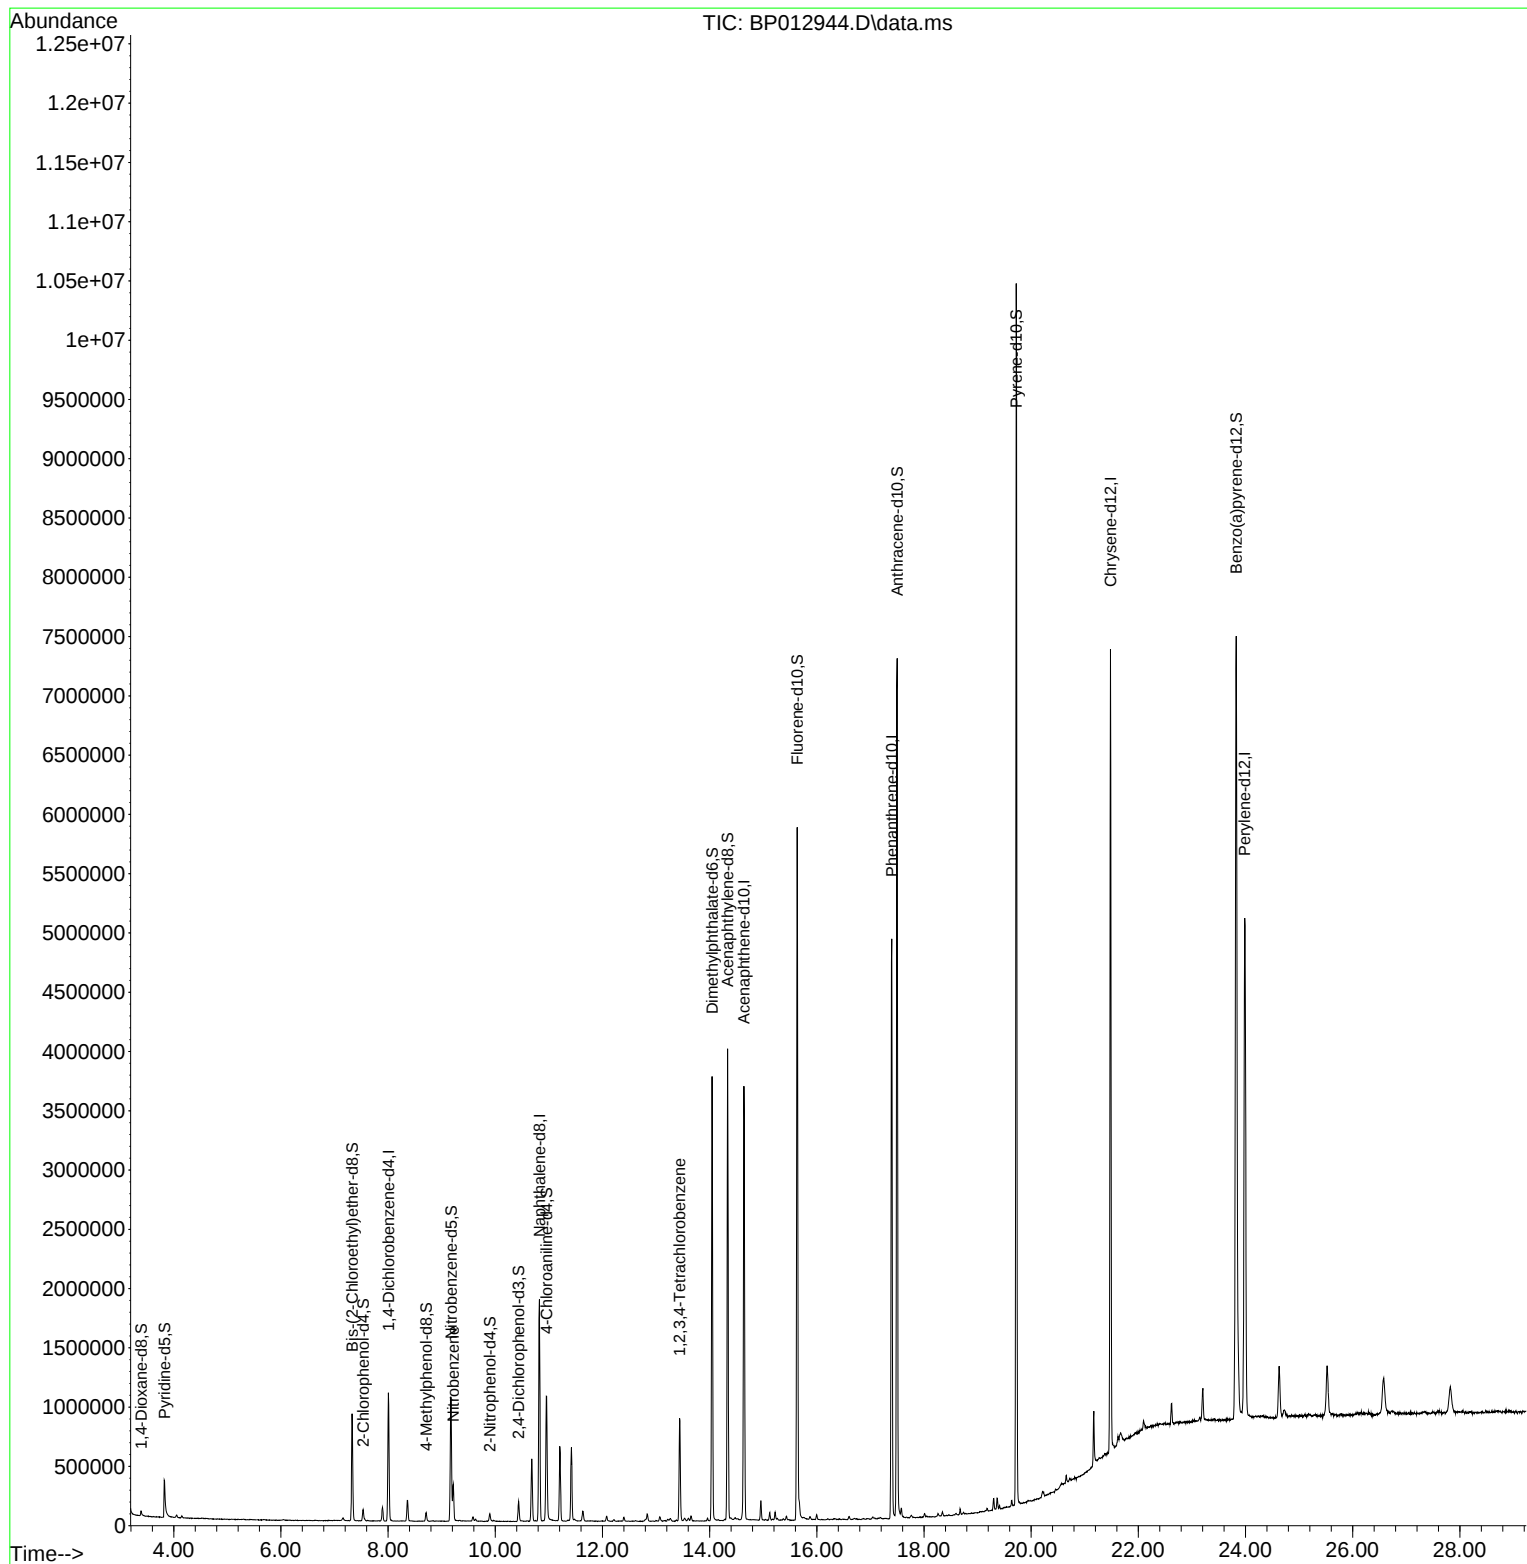


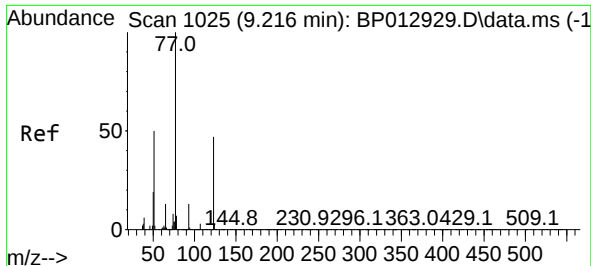

#22
Nitrobenzene
Concen: 5.948 ng/ul
RT: 9.216 min Scan# 1025
Delta R.T. 0.000 min
Lab File: BP012944.D
Acq: 02 Dec 2022 17:43

Instrument :
BNA_P
ClientSampleId :
COL70

Tgt Ion: 77 Resp: 163449
Ion Ratio Lower Upper
77 100
123 47.7 37.6 56.4
65 11.9 9.9 14.9

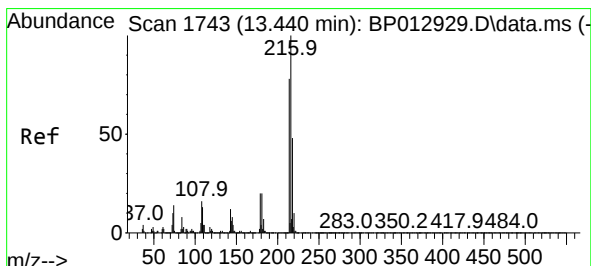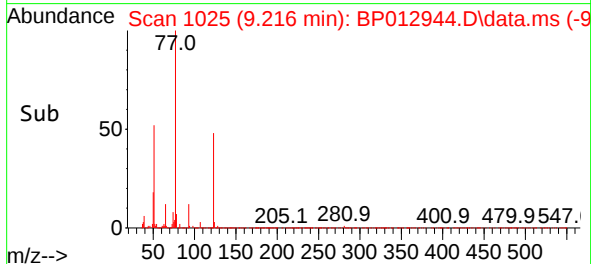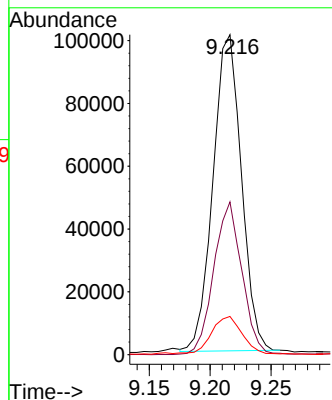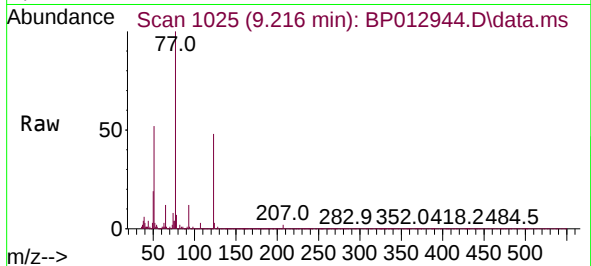

#75
1,2,3,4-Tetrachlorobenzene
Concen: 6.537 ng/uL
RT: 13.440 min Scan# 1743
Delta R.T. -0.006 min
Lab File: BP012944.D
Acq: 02 Dec 2022 17:43

Tgt Ion: 216 Resp: 272371
Ion Ratio Lower Upper
216 100
214 79.5 62.2 93.2
218 47.3 39.4 59.2

