

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120222\
 Data File : BP012930.D
 Acq On : 02 Dec 2022 09:12
 Operator : CG/JU
 Sample : PB149301BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK301

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012930.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.393	31	35	46	rVB	65483	101586	0.77%	0.089%
2	3.817	103	107	129	rBV	888140	1501050	11.39%	1.320%
3	4.152	160	164	170	rVB2	18821	30080	0.23%	0.026%
4	7.158	667	675	684	rBV	1165191	1844486	14.00%	1.622%
5	7.328	697	704	715	rVB	1020834	1597217	12.12%	1.405%
6	7.534	731	739	748	rBV	1119617	1820385	13.82%	1.601%
7	8.005	812	819	829	rVB	1170949	1854650	14.08%	1.631%
8	8.705	928	938	951	rBV	1522307	2481945	18.84%	2.183%
9	9.169	1008	1017	1025	rBV	1164230	1890402	14.35%	1.663%
10	9.893	1133	1140	1148	rBV	939518	1567622	11.90%	1.379%
11	10.434	1224	1232	1245	rBV	1579462	2627946	19.95%	2.311%
12	10.822	1290	1298	1307	rBV	1932640	3298933	25.04%	2.902%
13	10.951	1312	1320	1337	rBV	1625206	2849525	21.63%	2.506%
14	11.475	1405	1409	1416	rVB8	8402	16705	0.13%	0.015%
15	11.598	1424	1430	1434	rBV9	7780	15367	0.12%	0.014%
16	12.398	1560	1566	1575	rVB2	35314	62217	0.47%	0.055%
17	13.534	1753	1759	1762	rBV7	9334	18389	0.14%	0.016%
18	13.610	1766	1772	1776	rVV4	8989	14930	0.11%	0.013%
19	14.045	1839	1846	1858	rBV	3503872	4946657	37.55%	4.351%
20	14.334	1888	1895	1907	rBV	3894210	5581213	42.36%	4.909%
21	14.469	1912	1918	1932	rVV2	62935	161484	1.23%	0.142%
22	14.640	1940	1947	1955	rBV	3750697	5435163	41.25%	4.781%
23	14.822	1971	1978	2001	rBV	1635717	2594138	19.69%	2.282%
24	15.039	2012	2015	2020	rVB6	9873	17138	0.13%	0.015%
25	15.634	2109	2116	2128	rBV	5214169	7635876	57.96%	6.716%
26	15.739	2128	2134	2146	rVB	1690254	2285473	17.35%	2.010%
27	15.869	2152	2156	2165	rVB4	26152	49958	0.38%	0.044%
28	16.410	2246	2248	2255	rVB8	11029	16566	0.13%	0.015%
29	17.181	2374	2379	2385	rBV	11490	23186	0.18%	0.020%
30	17.392	2408	2415	2426	rBV	5196783	7431252	56.41%	6.536%
31	17.492	2426	2432	2450	rVB	6611238	9207828	69.89%	8.099%
32	17.763	2475	2478	2485	rBV5	6368	14317	0.11%	0.013%
33	18.257	2558	2562	2568	rBV5	39128	61975	0.47%	0.055%
34	19.298	2735	2739	2743	rBV2	82263	104377	0.79%	0.092%
35	19.363	2746	2750	2755	rBV	74274	111042	0.84%	0.098%
36	19.486	2769	2771	2775	rBV5	21806	24978	0.19%	0.022%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120222\
Data File : BP012930.D
Acq On : 02 Dec 2022 09:12
Operator : CG/JU
Sample : PB149301BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK301

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120122.M
Title : SVOA CALIBRATION

37	19.639	2794	2797	2802	rVB4	32650	40468	0.31%	0.036%
38	19.722	2805	2811	2820	rBV	8825359	11559543	87.74%	10.167%
39	21.480	3104	3110	3119	rBV	7049293	9471187	71.89%	8.331%
40	23.821	3500	3508	3522	rBV2	6328743	13174737	100.00%	11.588%
41	23.986	3528	3536	3551	rVB	4902534	10150204	77.04%	8.928%




Sum of corrected areas: 113692195

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120222\
Data File : BP012930.D
Acq On : 02 Dec 2022 09:12
Operator : CG/JU
Sample : PB149301BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK301

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

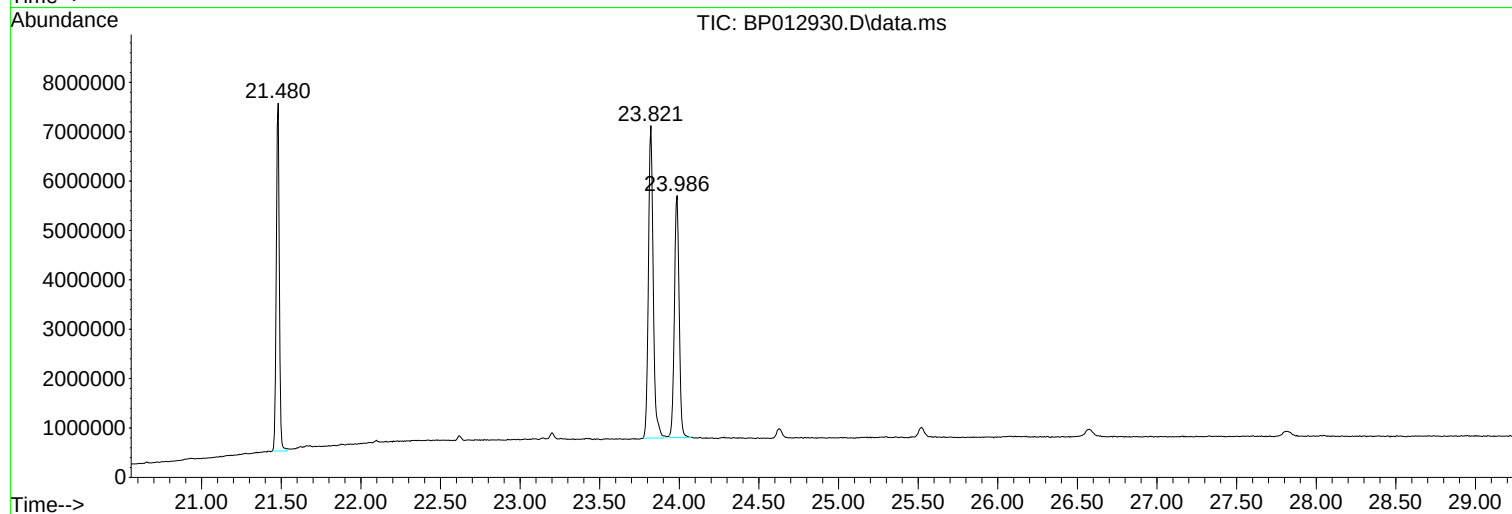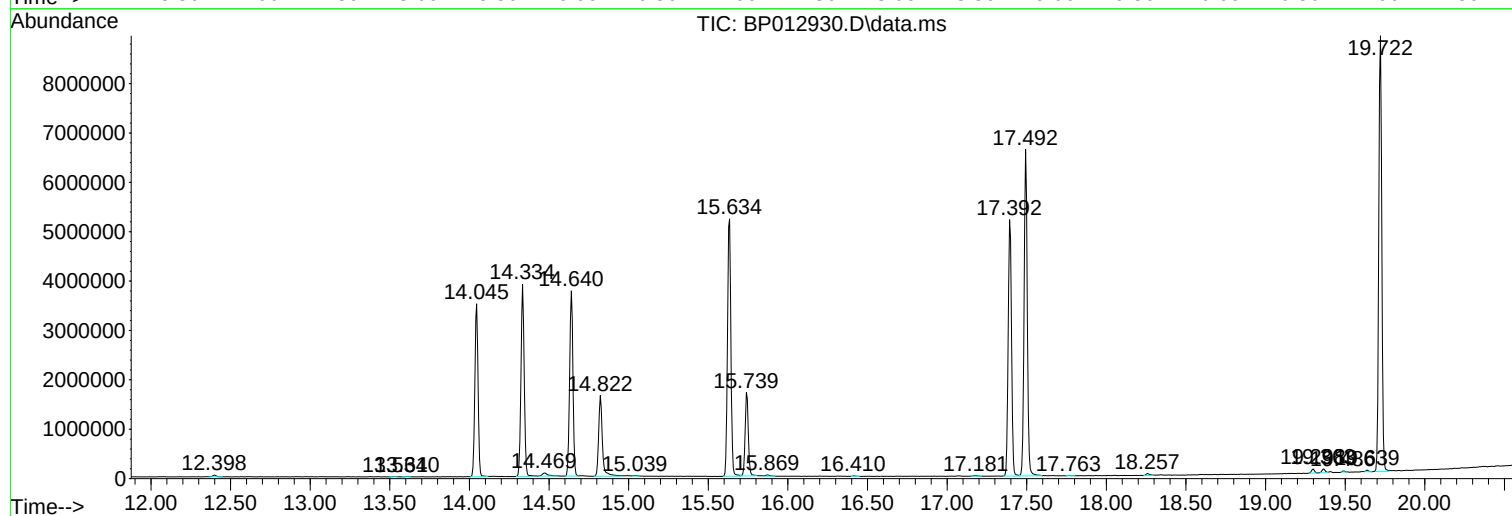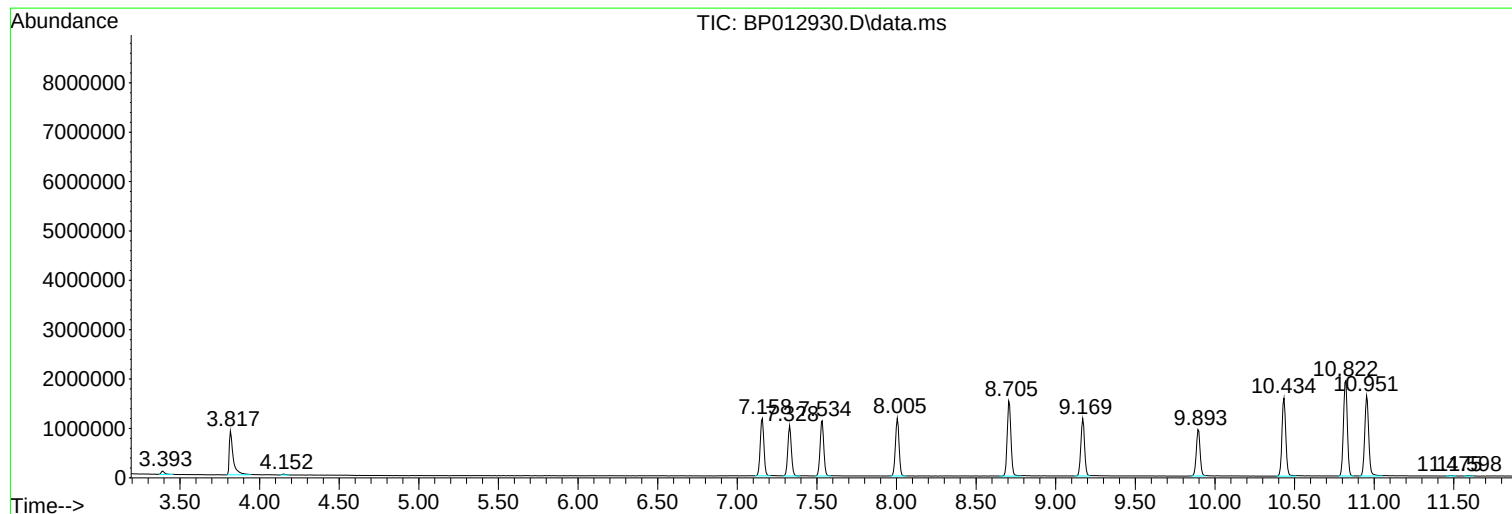

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120222\
Data File : BP012930.D
Acq On : 02 Dec 2022 09:12
Operator : CG/JU
Sample : PB149301BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK301

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120222\
Data File : BP012930.D
Acq On : 02 Dec 2022 09:12
Operator : CG/JU
Sample : PB149301BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK301

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc