

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120222\
 Data File : BP012931.D
 Acq On : 02 Dec 2022 09:46
 Operator : CG/JU
 Sample : PB149337BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK337

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012931.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.387	30	34	44	rBV	92904	137253	0.71%	0.096%
2	3.817	103	107	129	rBV	1256206	2180100	11.28%	1.524%
3	4.146	160	163	170	rBV	14935	22940	0.12%	0.016%
4	7.158	668	675	684	rBV	1732667	2739701	14.17%	1.915%
5	7.328	697	704	713	rVB	1507844	2311739	11.96%	1.616%
6	7.534	732	739	749	rBV	1673107	2660710	13.76%	1.860%
7	8.005	812	819	826	rBV	1073755	1682318	8.70%	1.176%
8	8.711	929	939	957	rBV	2260645	3684311	19.06%	2.575%
9	9.169	1009	1017	1031	rBV	1733838	2818586	14.58%	1.970%
10	9.899	1130	1141	1148	rBV	1395587	2339826	12.10%	1.635%
11	10.434	1224	1232	1246	rBV	2333371	3856222	19.95%	2.695%
12	10.822	1288	1298	1307	rBV	1755385	2947785	15.25%	2.060%
13	10.952	1312	1320	1335	rBV	2317378	4033147	20.86%	2.819%
14	12.399	1560	1566	1571	rVB	41655	70498	0.36%	0.049%
15	13.534	1752	1759	1765	rBV3	19162	36426	0.19%	0.025%
16	13.604	1767	1771	1778	rVB5	10674	22950	0.12%	0.016%
17	14.046	1839	1846	1854	rBV	5141001	7062925	36.54%	4.937%
18	14.334	1887	1895	1906	rBV	5736287	8051350	41.65%	5.627%
19	14.475	1914	1919	1929	rBV3	52773	115499	0.60%	0.081%
20	14.640	1940	1947	1955	rBV	3323512	4779670	24.72%	3.341%
21	14.822	1971	1978	1998	rBV	2559452	3931110	20.34%	2.748%
22	15.634	2109	2116	2128	rBV	7520122	10895280	56.36%	7.615%
23	15.740	2128	2134	2152	rVV	2728213	3664317	18.96%	2.561%
24	15.869	2152	2156	2164	rVB2	35287	64867	0.34%	0.045%
25	16.416	2244	2249	2256	rVB2	13714	25377	0.13%	0.018%
26	17.069	2355	2360	2365	rBV7	13289	20713	0.11%	0.014%
27	17.392	2408	2415	2425	rBV	4454266	6429867	33.26%	4.494%
28	17.492	2425	2432	2451	rVV	9240210	13293727	68.77%	9.291%
29	18.257	2559	2562	2569	rBV4	34004	44984	0.23%	0.031%
30	19.298	2734	2739	2745	rBV2	124412	172284	0.89%	0.120%
31	19.363	2746	2750	2755	rVV	117185	164681	0.85%	0.115%
32	19.404	2755	2757	2762	rVB6	18076	22248	0.12%	0.016%
33	19.634	2794	2796	2801	rVB3	26521	30157	0.16%	0.021%
34	19.722	2805	2811	2821	rVV	12870513	16714956	86.46%	11.683%
35	21.475	3104	3109	3118	rBV	5983366	8105986	41.93%	5.666%
36	23.822	3500	3508	3523	rBV2	9376198	19331621	100.00%	13.512%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120222\
Data File : BP012931.D
Acq On : 02 Dec 2022 09:46
Operator : CG/JU
Sample : PB149337BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK337

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120122.M
Title : SVOA CALIBRATION

37 23.986 3528 3536 3547 rVB2 4028731 8608135 44.53% 6.017%




Sum of corrected areas: 143074266

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120222\
Data File : BP012931.D
Acq On : 02 Dec 2022 09:46
Operator : CG/JU
Sample : PB149337BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK337

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

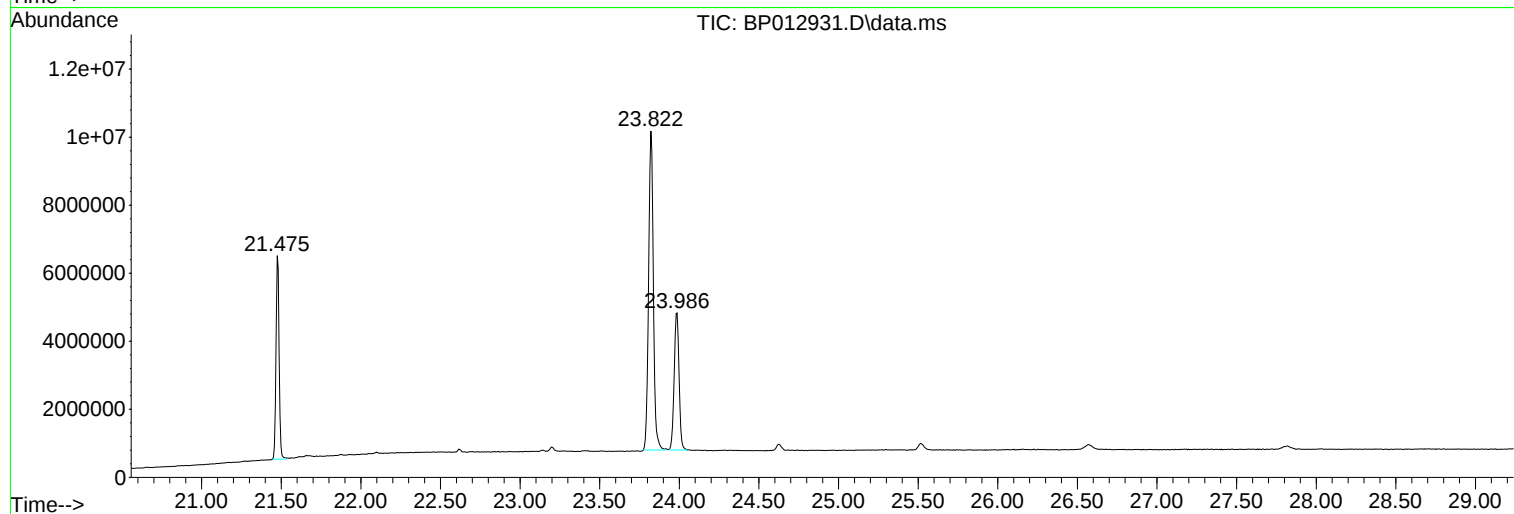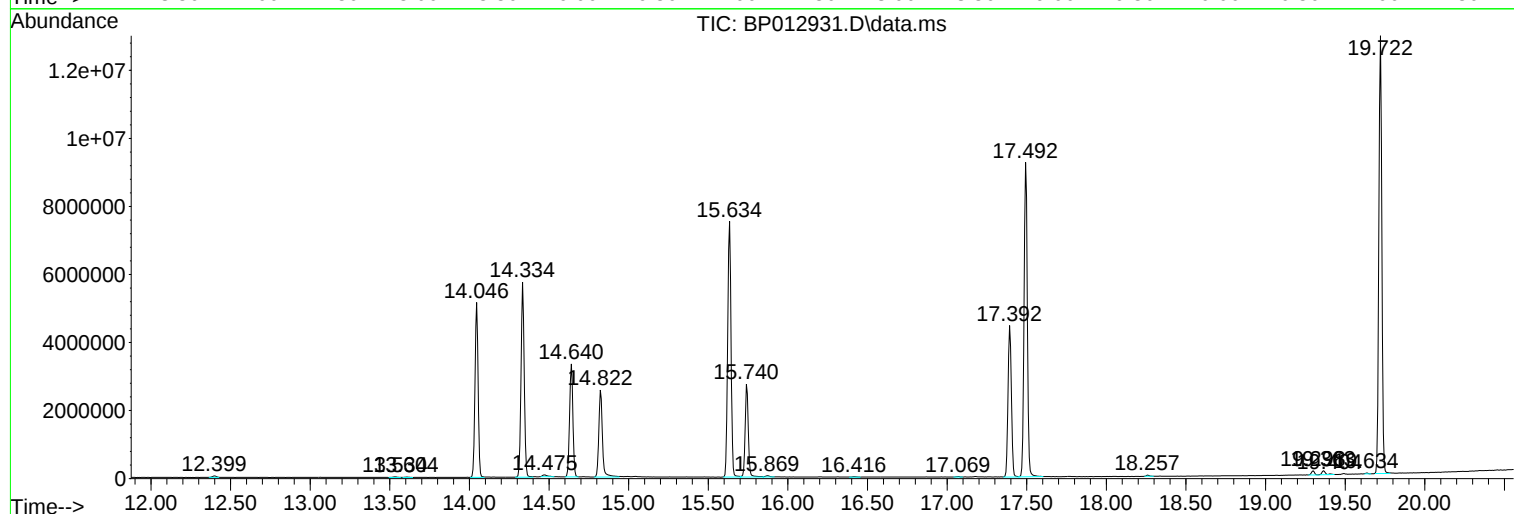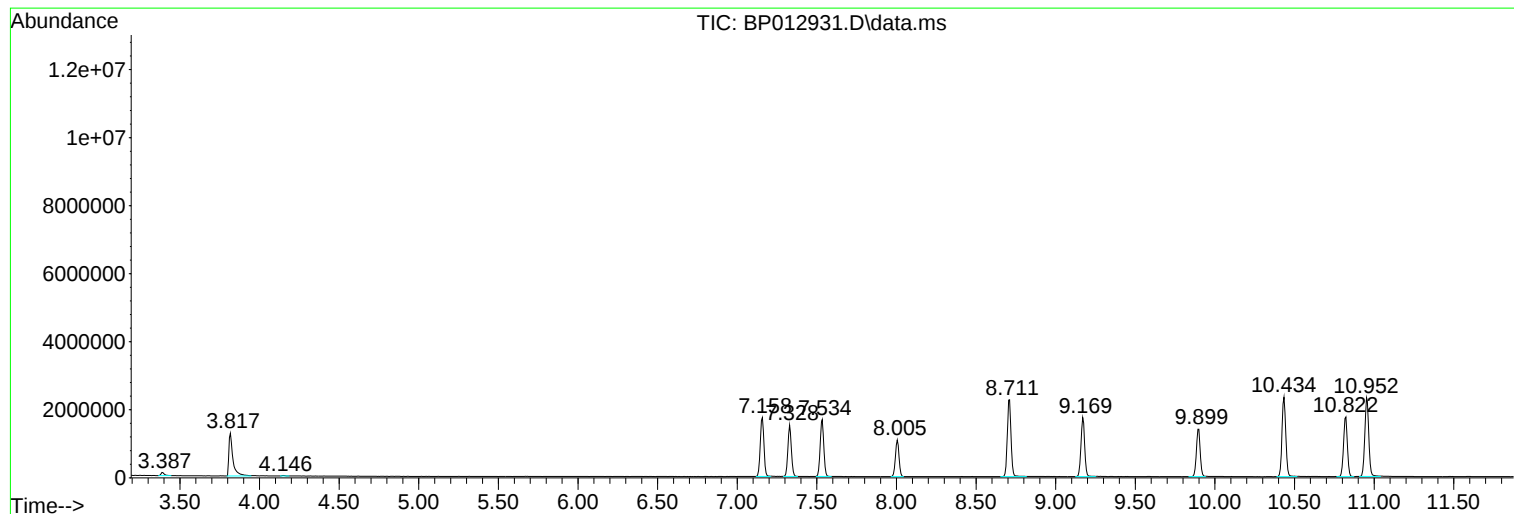

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120222\
Data File : BP012931.D
Acq On : 02 Dec 2022 09:46
Operator : CG/JU
Sample : PB149337BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK337

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120222\
Data File : BP012931.D
Acq On : 02 Dec 2022 09:46
Operator : CG/JU
Sample : PB149337BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK337

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc