

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120222\
 Data File : BP012941.D
 Acq On : 02 Dec 2022 16:00
 Operator : CG/JU
 Sample : N5785-04
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COL74

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012941.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.393	31	35	45	rVB	40681	63437	0.44%	0.059%
2	3.828	107	109	126	rBV	182070	324496	2.24%	0.301%
3	4.052	144	147	151	rVB	19040	25676	0.18%	0.024%
4	4.152	159	164	171	rVB	19288	28580	0.20%	0.027%
5	5.093	320	324	331	rBV	84406	119669	0.83%	0.111%
6	5.299	355	359	365	rVB4	12825	18409	0.13%	0.017%
7	7.157	669	675	685	rVB	191066	309832	2.14%	0.288%
8	7.328	698	704	714	rVB	921693	1442363	9.97%	1.339%
9	7.534	731	739	748	rBV	766368	1237676	8.56%	1.149%
10	8.005	812	819	831	rBV	1125565	1786637	12.35%	1.658%
11	8.710	931	939	950	rBV	658923	1059528	7.32%	0.983%
12	9.169	1010	1017	1029	rBV	1131755	1870796	12.93%	1.736%
13	9.581	1083	1087	1092	rVV	22325	34751	0.24%	0.032%
14	9.899	1129	1141	1151	rBV	585035	989161	6.84%	0.918%
15	10.434	1225	1232	1246	rBV	1337047	2232519	15.43%	2.072%
16	10.822	1290	1298	1309	rBV	1956372	3243504	22.42%	3.010%
17	10.957	1314	1321	1336	rBV	630902	1146750	7.93%	1.064%
18	11.628	1431	1435	1440	rVB8	10163	16705	0.12%	0.016%
19	12.081	1506	1512	1521	rVB	33153	55794	0.39%	0.052%
20	12.404	1561	1567	1570	rBV3	28745	47674	0.33%	0.044%
21	13.263	1707	1713	1720	rVB	24038	40361	0.28%	0.037%
22	13.451	1739	1745	1753	rVB8	22017	40014	0.28%	0.037%
23	13.616	1767	1773	1776	rBV6	10402	17483	0.12%	0.016%
24	13.963	1827	1832	1836	rBV5	18471	26369	0.18%	0.024%
25	14.045	1839	1846	1861	rBV	3726022	5059107	34.97%	4.695%
26	14.334	1888	1895	1910	rBV	3990748	5975305	41.30%	5.545%
27	14.475	1914	1919	1932	rVB3	26925	76529	0.53%	0.071%
28	14.639	1941	1947	1957	rBV	3741741	5545276	38.33%	5.146%
29	14.834	1974	1980	1987	rBV6	23435	48780	0.34%	0.045%
30	15.051	2013	2017	2021	rVB7	14815	20225	0.14%	0.019%
31	15.375	2067	2072	2078	rBV	72303	108079	0.75%	0.100%
32	15.434	2078	2082	2087	rVB	29520	37121	0.26%	0.034%
33	15.634	2109	2116	2122	rBV	5725115	8285277	57.27%	7.689%
34	15.739	2130	2134	2142	rVB	116786	172622	1.19%	0.160%
35	15.875	2152	2157	2163	rVB2	29159	46961	0.32%	0.044%
36	15.998	2174	2178	2182	rBV	22153	32536	0.22%	0.030%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120222\
 Data File : BP012941.D
 Acq On : 02 Dec 2022 16:00
 Operator : CG/JU
 Sample : N5785-04
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COL74

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120122.M
 Title : SVOA CALIBRATION

37	17.039	2351	2355	2358	rBV6	18583	30002	0.21%	0.028%
38	17.180	2375	2379	2386	rBV3	15050	30698	0.21%	0.028%
39	17.398	2409	2416	2426	rBV	5332336	7546840	52.16%	7.004%
40	17.498	2426	2433	2442	rVV	7572616	10847192	74.98%	10.067%
41	17.580	2443	2447	2456	rVB3	129619	198709	1.37%	0.184%
42	17.769	2477	2479	2486	rVB4	13810	17815	0.12%	0.017%
43	18.010	2516	2520	2523	rBV6	19051	23864	0.16%	0.022%
44	18.263	2560	2563	2570	rBV5	33797	52440	0.36%	0.049%
45	18.675	2631	2633	2636	rVB4	25631	26465	0.18%	0.025%
46	19.298	2736	2739	2745	rVB2	95770	127586	0.88%	0.118%
47	19.369	2747	2751	2755	rVV	103703	139368	0.96%	0.129%
48	19.410	2756	2758	2761	rVB2	32989	30947	0.21%	0.029%
49	19.639	2794	2797	2802	rVB3	58355	67618	0.47%	0.063%
50	19.722	2806	2811	2824	rVV	9653540	13490058	93.25%	12.519%
51	21.169	3054	3057	3063	rBV3	166465	220826	1.53%	0.205%
52	21.480	3105	3110	3121	rBV	7080037	9504814	65.70%	8.821%
53	23.827	3501	3509	3523	rBV2	6684612	14467256	100.00%	13.426%
54	23.992	3530	3537	3548	rVB2	4510932	9346655	64.61%	8.674%




Sum of corrected areas: 107755155

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120222\
Data File : BP012941.D
Acq On : 02 Dec 2022 16:00
Operator : CG/JU
Sample : N5785-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COL74

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

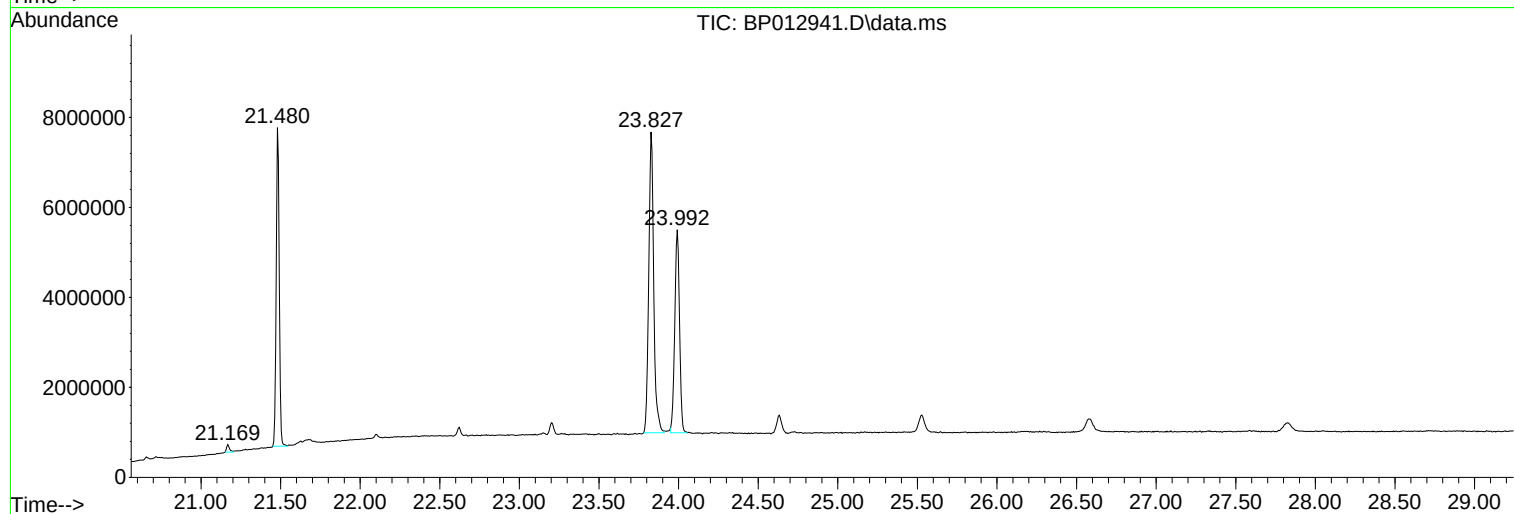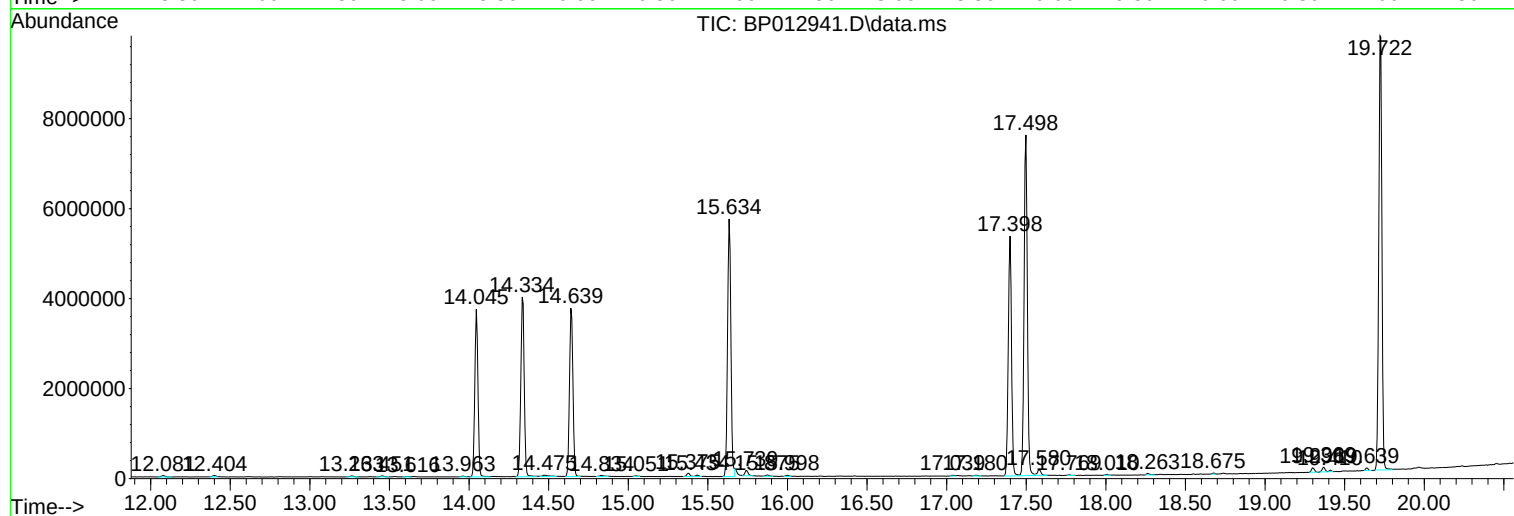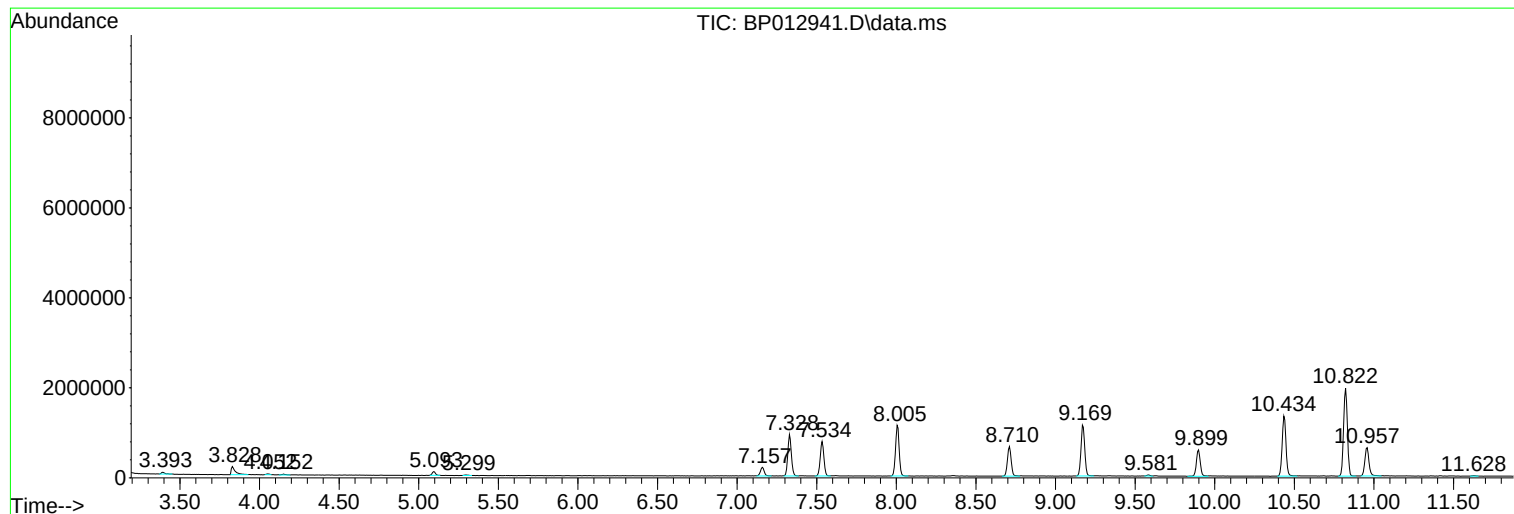

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120222\
Data File : BP012941.D
Acq On : 02 Dec 2022 16:00
Operator : CG/JU
Sample : N5785-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COL74

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120222\
Data File : BP012941.D
Acq On : 02 Dec 2022 16:00
Operator : CG/JU
Sample : N5785-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COL74

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
