

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120222\
 Data File : BP012943.D
 Acq On : 02 Dec 2022 17:09
 Operator : CG/JU
 Sample : N5785-03
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COL73

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012943.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.393	31	35	40	rBV	38797	56313	0.40%	0.055%
2	3.828	106	109	124	rBV	200356	353789	2.52%	0.345%
3	4.058	144	148	155	rVB2	22036	35796	0.25%	0.035%
4	4.152	160	164	169	rVB	20376	30776	0.22%	0.030%
5	5.093	319	324	335	rVB	103207	153625	1.09%	0.150%
6	5.299	354	359	368	rVB	49270	87013	0.62%	0.085%
7	7.158	667	675	685	rBV	187769	311128	2.21%	0.304%
8	7.328	696	704	712	rBV	874945	1389605	9.89%	1.357%
9	7.534	730	739	747	rBV	728125	1172934	8.35%	1.145%
10	8.005	810	819	832	rBV	1065312	1751591	12.46%	1.710%
11	8.363	870	880	885	rBV	52272	91887	0.65%	0.090%
12	8.710	930	939	950	rBV	667479	1079384	7.68%	1.054%
13	9.169	1010	1017	1027	rBV	1061694	1755882	12.50%	1.714%
14	9.581	1083	1087	1095	rVB2	21968	35603	0.25%	0.035%
15	9.899	1133	1141	1149	rBV	369352	623207	4.43%	0.608%
16	10.434	1224	1232	1245	rBV	1231911	2049667	14.59%	2.001%
17	10.681	1269	1274	1281	rVB	21769	34115	0.24%	0.033%
18	10.822	1290	1298	1308	rBV	1841219	3068271	21.83%	2.996%
19	10.957	1313	1321	1336	rBV	696944	1233527	8.78%	1.204%
20	11.628	1428	1435	1443	rBV	8165	19758	0.14%	0.019%
21	12.075	1505	1511	1518	rBV3	31858	53390	0.38%	0.052%
22	12.398	1559	1566	1571	rVB2	29432	50059	0.36%	0.049%
23	13.263	1707	1713	1719	rVB4	16336	28507	0.20%	0.028%
24	13.528	1753	1758	1764	rBV6	15448	28046	0.20%	0.027%
25	13.963	1828	1832	1835	rBV6	16906	24655	0.18%	0.024%
26	14.045	1840	1846	1858	rBV	3304908	4557397	32.43%	4.450%
27	14.334	1887	1895	1904	rBV	3679269	5501143	39.15%	5.371%
28	14.481	1915	1920	1924	rBV6	16733	32384	0.23%	0.032%
29	14.639	1940	1947	1956	rBV	3561704	5234977	37.25%	5.111%
30	14.828	1974	1979	1985	rBV9	10573	23008	0.16%	0.022%
31	15.051	2012	2017	2023	rVB9	15303	25929	0.18%	0.025%
32	15.434	2077	2082	2088	rVB	34864	49281	0.35%	0.048%
33	15.634	2108	2116	2130	rBV	5223918	7731951	55.02%	7.549%
34	15.745	2130	2135	2142	rVB	62823	109579	0.78%	0.107%
35	15.875	2153	2157	2164	rVB3	26225	45168	0.32%	0.044%
36	17.039	2351	2355	2359	rBV7	18160	29167	0.21%	0.028%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120222\
 Data File : BP012943.D
 Acq On : 02 Dec 2022 17:09
 Operator : CG/JU
 Sample : N5785-03
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COL73

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120122.M
 Title : SVOA CALIBRATION

37	17.398	2409	2416	2426	rBV	5121640	7180351	51.10%	7.010%
38	17.498	2426	2433	2444	rVV	7281462	10481759	74.59%	10.234%
39	17.581	2444	2447	2457	rVB3	79864	129394	0.92%	0.126%
40	18.004	2515	2519	2524	rBV5	50590	69276	0.49%	0.068%
41	18.263	2560	2563	2572	rBV8	23520	37809	0.27%	0.037%
42	18.339	2573	2576	2580	rBV	14408	18430	0.13%	0.018%
43	19.298	2735	2739	2745	rBV2	97352	141240	1.01%	0.138%
44	19.369	2746	2751	2755	rBV	99802	148499	1.06%	0.145%
45	19.410	2755	2758	2763	rVB6	28046	37342	0.27%	0.036%
46	19.639	2794	2797	2801	rVB3	52032	54092	0.38%	0.053%
47	19.722	2805	2811	2825	rBV	9381420	13172980	93.74%	12.861%
48	21.480	3105	3110	3122	rBV	6708553	9213599	65.57%	8.996%
49	23.827	3501	3509	3522	rBV2	6349054	14052616	100.00%	13.720%
50	23.992	3530	3537	3546	rVB2	4239133	8828313	62.82%	8.619%




Sum of corrected areas: 102424212

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120222\
Data File : BP012943.D
Acq On : 02 Dec 2022 17:09
Operator : CG/JU
Sample : N5785-03
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COL73

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

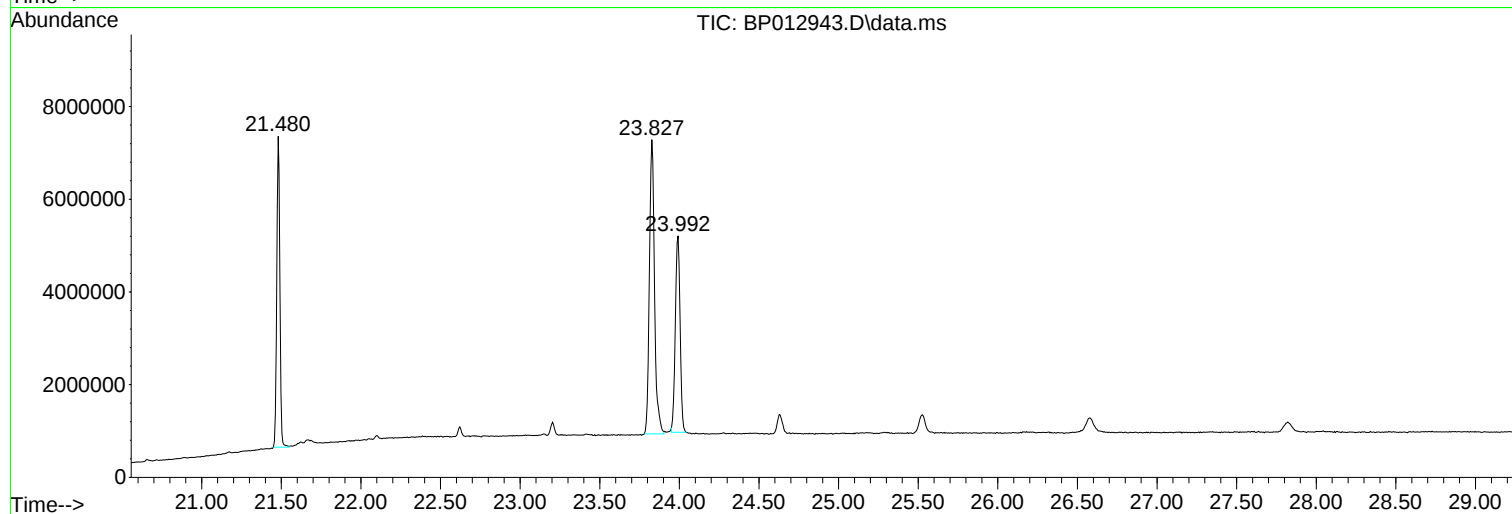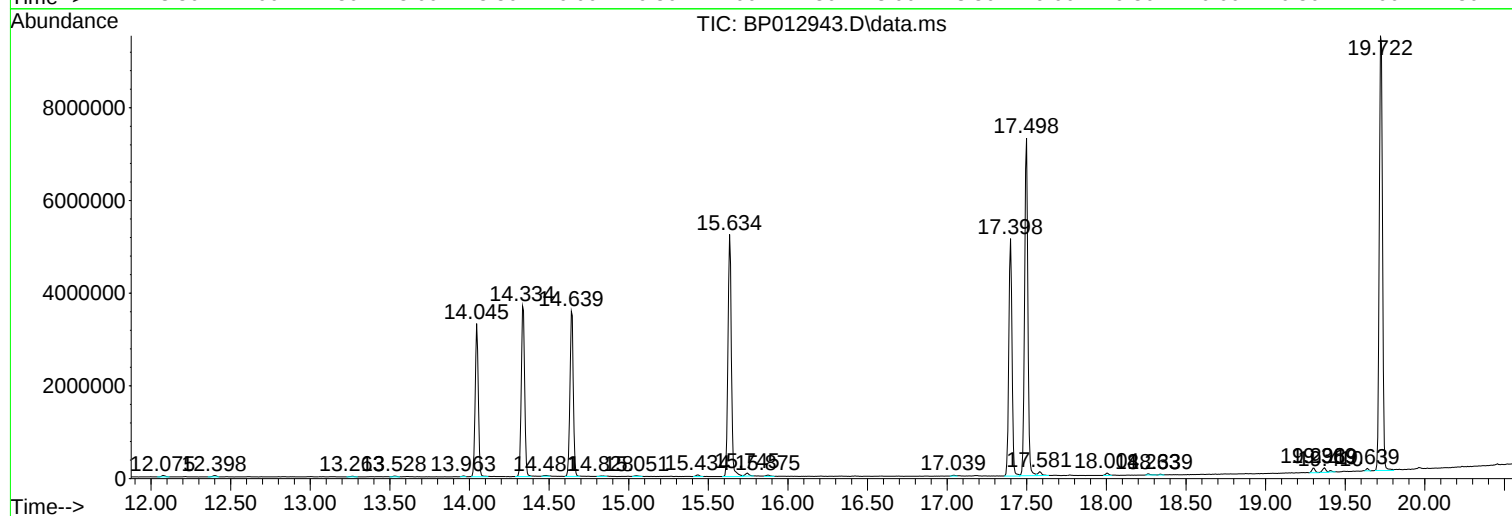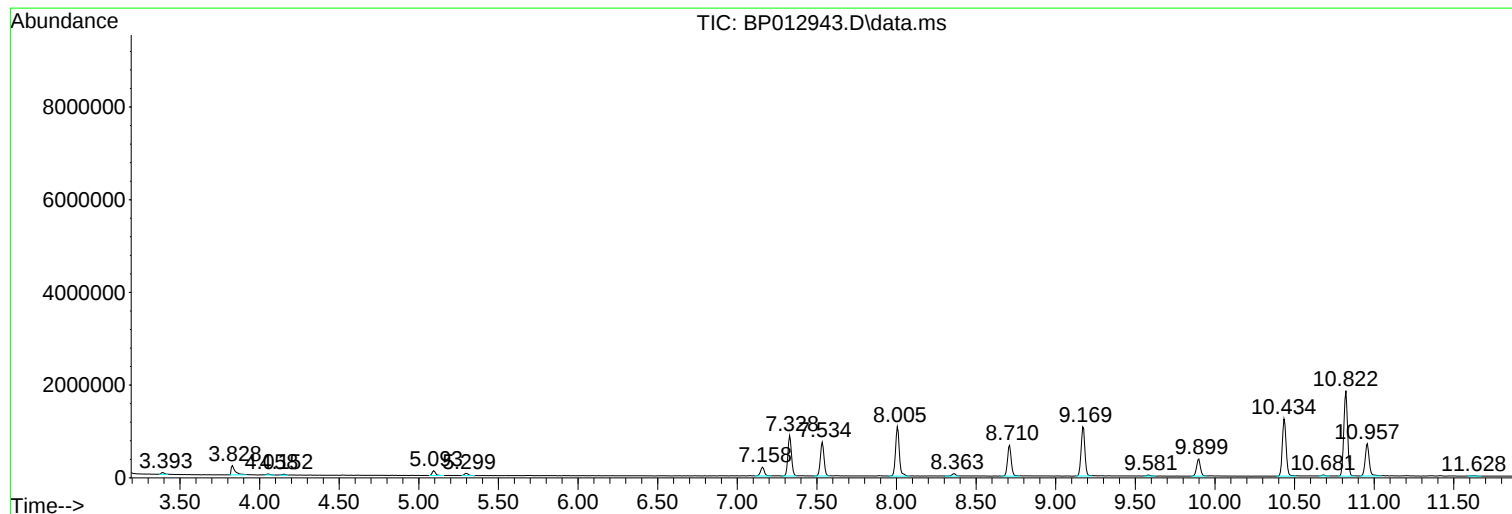

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120222\
Data File : BP012943.D
Acq On : 02 Dec 2022 17:09
Operator : CG/JU
Sample : N5785-03
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0L73

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120222\
Data File : BP012943.D
Acq On : 02 Dec 2022 17:09
Operator : CG/JU
Sample : N5785-03
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0L73

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc