

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP120420\
 Data File : BP004152.D
 Acq On : 04 Dec 2020 21:09
 Operator : CG/JU
 Sample : SSTDICV020
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SICV001

Quant Time: Dec 05 03:42:25 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP120420.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Dec 05 03:41:01 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.85	152	355483	20.00	ng/ul	0.00
20) Naphthalene-d8	10.65	136	1499826	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.49	164	959202	20.00	ng/ul	0.00
64) Phenanthrene-d10	17.26	188	2122764	20.00	ng/ul	0.00
79) Chrysene-d12	21.34	240	2215766	20.00	ng/ul	0.00
88) Perylene-d12	23.70	264	2447502	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.34	96	74575	8.06	ng/uL	0.00
4) Pyridine-d5	3.74	84	525129	19.98	ng/ul	0.00
7) Phenol-d5	7.00	99	641599	20.19	ng/ul	0.00
9) Bis-(2-Chloroethyl)ether-d	7.18	67	377060	20.52	ng/ul	0.00
11) 2-Chlorophenol-d4	7.38	132	500788	20.25	ng/ul	0.00
15) 4-Methylphenol-d8	8.55	113	513501	20.51	ng/ul	0.00
21) Nitrobenzene-d5	9.00	128	253503	20.73	ng/ul	0.00
24) 2-Nitrophenol-d4	9.72	143	236178	21.15	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.26	165	505451	20.57	ng/ul	0.00
31) 4-Chloroaniline-d4	10.77	131	743280	20.62	ng/ul	0.00
46) Dimethylphthalate-d6	13.90	166	1551312	20.36	ng/ul	0.00
49) Acenaphthylene-d8	14.19	160	1908643	20.39	ng/ul	0.00
54) 4-Nitrophenol-d4	14.67	143	255599	20.50	ng/ul	0.00
60) Fluorene-d10	15.49	176	1359492	20.41	ng/ul	0.00
65) 4,6-Dinitro-2-methylphenol	15.60	200	164825	19.11	ng/ul	0.00
73) Anthracene-d10	17.35	188	2126962	20.39	ng/ul	0.00
81) Pyrene-d10	19.59	212	2420712	20.77	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.56	264	2664078	20.26	ng/ul	0.00

Target Compounds

					Ovalue
2) 1,4-Dioxane	3.38	88	80713	8.050	ng/uL# 90
5) Pyridine	3.76	79	537719	20.232	ng/ul 95
6) Benzaldehyde	6.99	77	316231	22.392	ng/ul 96
8) Phenol	7.03	94	663572	20.408	ng/ul 100
10) Bis(2-Chloroethyl)ether	7.28	93	532468	20.407	ng/ul 98
12) 2-Chlorophenol	7.41	128	509755	20.388	ng/ul 99
13) 2-Methylphenol	8.28	108	506437	20.466	ng/ul 99
14) 2,2'-oxybis(1-Chloropropan	8.38	45	643900	20.714	ng/ul 97
16) Acetophenone	8.67	105	810423	20.892	ng/ul 99
17) N-Nitroso-di-n-propylamine	8.66	70	419706	20.601	ng/ul 97
18) 4-Methylphenol	8.61	108	539966	20.473	ng/ul 100
19) Hexachloroethane	8.93	117	218261	20.385	ng/ul 97
22) Nitrobenzene	9.05	77	612974	20.567	ng/ul 99
23) Isophorone	9.57	82	1224050	20.328	ng/ul 98
25) 2-Nitrophenol	9.76	139	258746	21.630	ng/ul 95
26) 2,4-Dimethylphenol	9.82	107	585547	20.183	ng/ul 100
27) Bis(2-Chloroethoxy)methane	10.06	93	725966	20.263	ng/ul 99
29) 2,4-Dichlorophenol	10.29	162	487092	20.523	ng/ul 100
30) Naphthalene	10.70	128	1709484	20.384	ng/ul 100
32) 4-Chloroaniline	10.80	127	712580	20.696	ng/ul 100
33) Hexachlorobutadiene	10.99	225	340533	19.992	ng/ul 99
34) Caprolactam	11.55	113	113288	12.936	ng/ul 96

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP120420\
 Data File : BP004152.D
 Acq On : 04 Dec 2020 21:09
 Operator : CG/JU
 Sample : SSTDICV020
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SICV001

Quant Time: Dec 05 03:42:25 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP120420.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Dec 05 03:41:01 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
35) 4-Chloro-3-methylphenol	11.92	107	539436	20.472	ng/ul	98
36) 2-Methylnaphthalene	12.31	142	1199840	20.311	ng/ul	100
37) 1-Methylnaphthalene	12.53	142	1160248	20.431	ng/ul	100
39) 1,2,4,5-Tetrachlorobenzene	12.68	216	654179	20.309	ng/ul	99
40) Hexachlorocyclopentadiene	12.67	237	393987	19.567	ng/ul	100
41) 2,4,6-Trichlorophenol	12.92	196	389803	21.016	ng/ul	99
42) 2,4,5-Trichlorophenol	12.99	196	415721	20.812	ng/ul	98
43) 1,1'-Biphenyl	13.33	154	1567151	20.430	ng/ul	99
44) 2-Chloronaphthalene	13.36	162	1246641	20.496	ng/ul	100
45) 2-Nitroaniline	13.56	65	322600	21.601	ng/ul	99
47) Dimethylphthalate	13.95	163	1572179	20.329	ng/ul	100
48) 2,6-Dinitrotoluene	14.06	165	304572	21.699	ng/ul	98
50) Acenaphthylene	14.22	152	1903588	20.522	ng/ul	100
51) 3-Nitroaniline	14.39	138	272354	20.791	ng/ul	97
52) Acenaphthene	14.56	153	1328697	20.304	ng/ul	99
53) 2,4-Dinitrophenol	14.59	184	103554	19.138	ng/ul	97
55) 4-Nitrophenol	14.69	109	192107	20.484	ng/ul	95
56) Dibenzofuran	14.90	168	1863563	20.544	ng/ul	99
57) 2,4-Dinitrotoluene	14.85	165	424386	22.135	ng/ul	100
58) 2,3,4,6-Tetrachlorophenol	15.12	232	346324	21.255	ng/ul	97
59) Diethylphthalate	15.33	149	1584168	20.293	ng/ul	100
61) Fluorene	15.55	166	1546273	20.544	ng/ul	99
62) 4-Chlorophenyl-phenylether	15.55	204	792952	20.194	ng/ul	98
63) 4-Nitroaniline	15.56	138	279588	22.575	ng/ul	98
66) 4,6-Dinitro-2-methylphenol	15.62	198	190136	19.754	ng/ul	99
67) N-Nitrosodiphenylamine	15.76	169	1328678	20.339	ng/ul	99
68) 4-Bromophenyl-phenylether	16.45	248	512728	20.181	ng/ul	97
69) Hexachlorobenzene	16.56	284	577819	20.393	ng/ul	98
70) Atrazine	16.72	200	528198	20.699	ng/ul	99
71) Pentachlorophenol	16.90	266	273770	20.229	ng/ul	97
72) Phenanthrene	17.30	178	2498936	20.465	ng/ul	100
74) Anthracene	17.39	178	2553202	20.524	ng/ul	99
75) 1,2,3,4-Tetrachlorobenzene	13.29	216	649412	20.153	ng/uL	100
76) Pentachlorobenzene	14.82	250	662094	20.328	ng/uL	99
77) Carbazole	17.66	167	2246407	21.262	ng/ul	100
78) Di-n-butylphthalate	18.23	149	2783943	20.215	ng/ul	100
80) Fluoranthene	19.27	202	3048300	20.651	ng/ul	99
82) Pyrene	19.62	202	3106181	20.716	ng/ul	100
83) Butylbenzylphthalate	20.50	149	1240611	20.366	ng/ul	97
84) 3,3'-Dichlorobenzidine	21.26	252	1030810	20.505	ng/ul	99
85) Benzo(a)anthracene	21.33	228	3093743	20.756	ng/ul	100
86) Bis(2-ethylhexyl)phthalate	21.27	149	1868312	20.328	ng/ul	100
87) Chrysene	21.38	228	2936572	20.571	ng/ul	99
89) Di-n-octyl phthalate	22.19	149	3170659	21.680	ng/ul	100
90) Benzo(b)fluoranthene	22.99	252	3254466	20.650	ng/ul	100
91) Benzo(k)fluoranthene	23.04	252	3143072	20.589	ng/ul	99
93) Benzo(a)pyrene	23.60	252	2964071	20.478	ng/ul	100
94) Indeno(1,2,3-cd)pyrene	26.14	276	3763246	20.300	ng/ul	99
95) Dibenzo(a,h)anthracene	26.16	278	3164288	20.450	ng/ul	100
96) Benzo(g,h,i)perylene	26.87	276	3129738	20.119	ng/ul	99


Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP120420\
Data File : BP004152.D
Acq On : 04 Dec 2020 21:09
Operator : CG/JU
Sample : SSTDICV020
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SICV001

Quant Time: Dec 05 03:42:25 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP120420.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 05 03:41:01 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
--------------------	------	------	----------	------	-------	----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed



#2

1,4-Dioxane

Concen: 8.050 ng/uL

RT: 3.38 min Scan# 32

Delta R.T. 0.00 min

Lab File: BP004152.D

Acq: 04 Dec 2020 21:09

Instrument :

BNA_P

ClientSampleId :

SICV001





Tot Ion: 88 Resp: 80713

Ion Ratio Lower Upper

88 100

43 36.8 42.5 63.7#

58 70.6 57.0 85.4

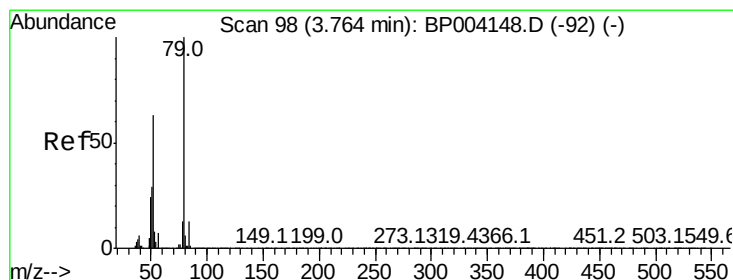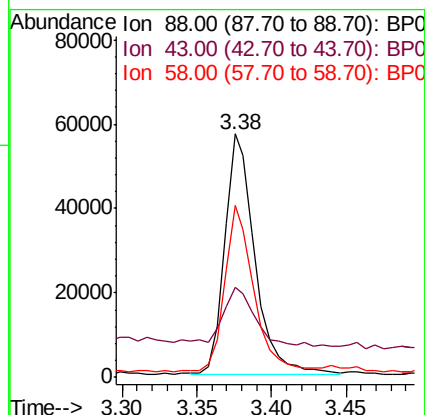

#5

Pyridine

Concen: 20.232 ng/uL

RT: 3.76 min Scan# 97

Delta R.T. -0.01 min

Lab File: BP004152.D

Acq: 04 Dec 2020 21:09




Tgt Ion: 79 Resp: 537719


Ion Ratio Lower Upper

79 100

52 69.6 51.4 77.0

51 30.5 24.0 36.0

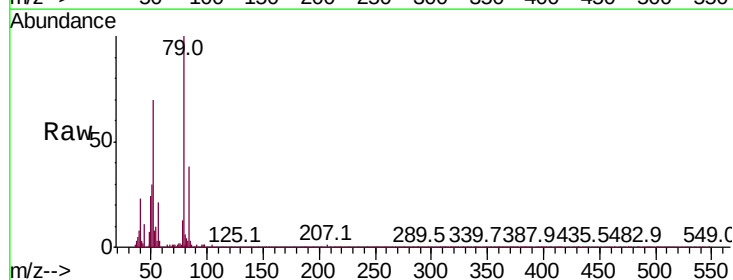



#6

Benzaldehyde

Concen: 22.392 ng/ul

RT: 6.99 min Scan# 646

Delta R.T. -0.01 min

Lab File: BP004152.D

Acq: 04 Dec 2020 21:09

Instrument :

BNA_P

ClientSampleId :

SICV001





Tot Ion: 77 Resp: 316231

Ion Ratio Lower Upper

77 100

105 94.7 79.8 119.8

106 91.8 75.2 112.8

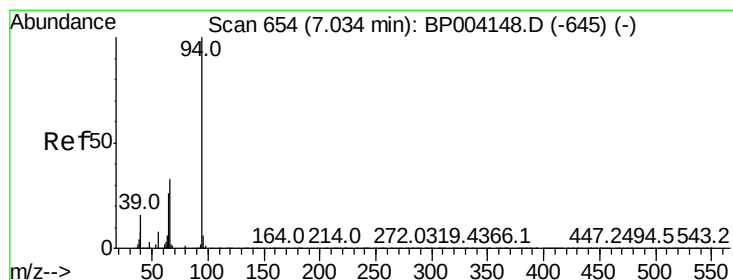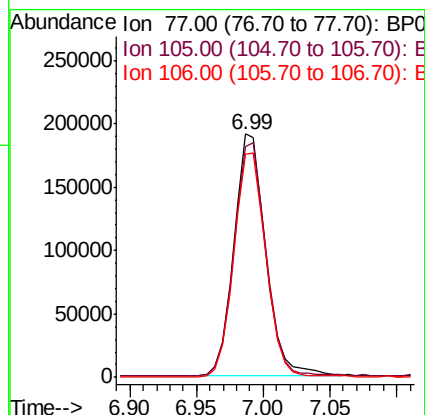

#8

Phenol

Concen: 20.408 ng/ul

RT: 7.03 min Scan# 654

Delta R.T. -0.00 min

Lab File: BP004152.D

Acq: 04 Dec 2020 21:09




Tgt Ion: 94 Resp: 663572


Ion Ratio Lower Upper

94 100

65 26.1 20.8 31.2

66 34.1 27.0 40.6

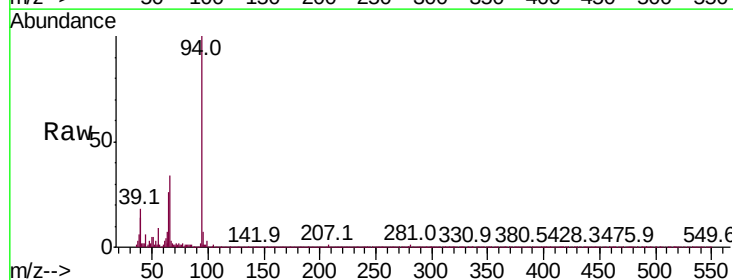

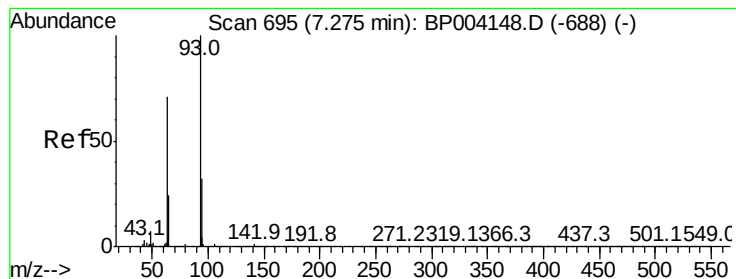

#10

Bis(2-Chloroethyl)ether

Concen: 20.407 ng/ul

RT: 7.28 min Scan# 695

Delta R.T. -0.00 min

Lab File: BP004152.D

Acq: 04 Dec 2020 21:09

Instrument :

BNA_P

ClientSampleId :

SICV001





Tot Ion: 93 Resp: 532468

Ion Ratio Lower Upper

93 100

63 72.3 57.0 85.4

95 32.1 26.8 40.2

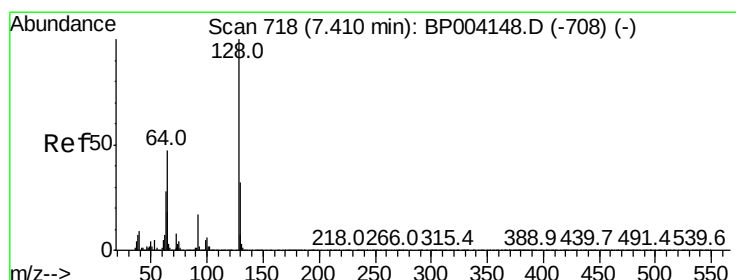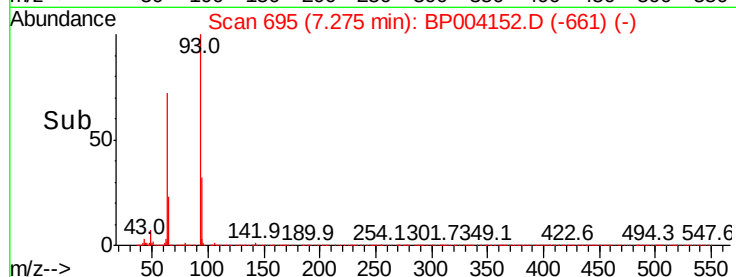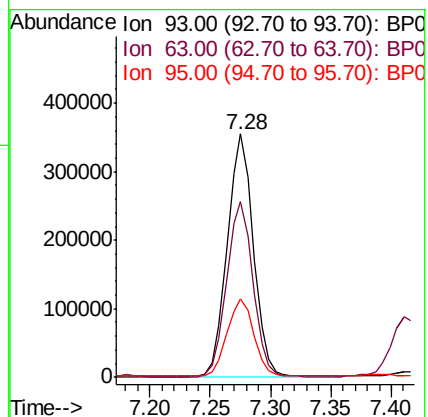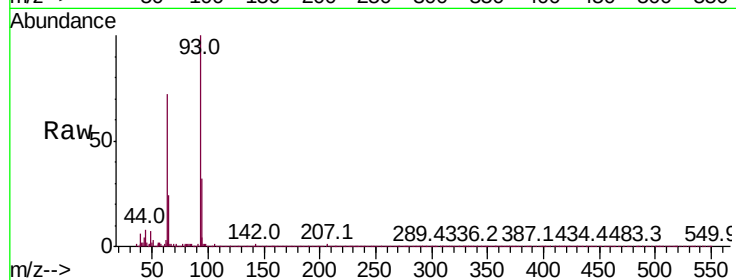

#12

2-Chlorophenol

Concen: 20.388 ng/ul

RT: 7.41 min Scan# 718

Delta R.T. -0.00 min

Lab File: BP004152.D

Acq: 04 Dec 2020 21:09




Tgt Ion: 128 Resp: 509755


Ion Ratio Lower Upper

128 100

64 45.7 37.4 56.0

130 32.5 25.4 38.2

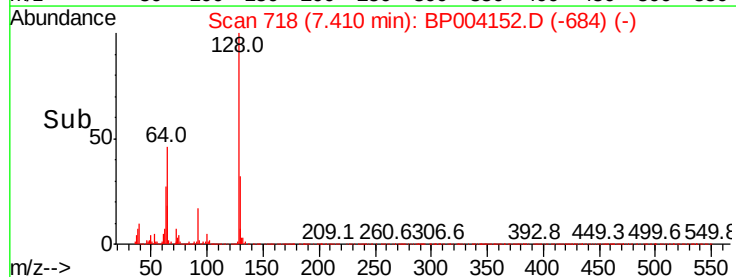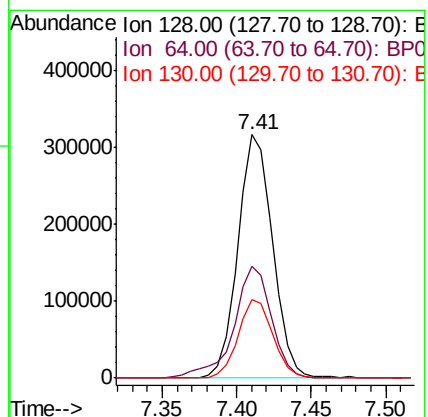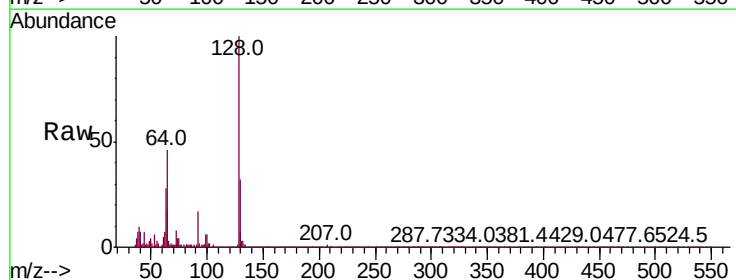



#13

2-Methylphenol

Concen: 20.466 ng/ul

RT: 8.28 min Scan# 866

Delta R.T. -0.01 min

Lab File: BP004152.D

Acq: 04 Dec 2020 21:09

Instrument :

BNA_P

ClientSampleId :


SICV001

Tot Ion:108 Resp: 506437

Ion Ratio Lower Upper

108 100

107 90.0 72.7 109.1



Abundance Ion 108.00 (107.70 to 108.70): E

Ion 107.00 (106.70 to 107.70): E

8.28

300000



200000

100000

0

8.20 8.25 8.30 8.35

Time-->



#14

2,2'-oxybis(1-Chloropropane)

Concen: 20.714 ng/ul

RT: 8.38 min Scan# 883

Delta R.T. -0.01 min

Lab File: BP004152.D

Acq: 04 Dec 2020 21:09


Tgt Ion: 45 Resp: 643900

Ion Ratio Lower Upper

45 100

77 16.7 14.2 21.4

79 13.3 11.4 17.2



Abundance Ion 45.00 (44.70 to 45.70): BP0

Ion 77.00 (76.70 to 77.70): BP0

Ion 79.00 (78.70 to 79.70): BP0

8.38

300000


200000


100000

0

8.30 8.35 8.40 8.45

Time-->





#16

Acetophenone

Concen: 20.892 ng/ul

RT: 8.67 min Scan# 932





Delta R.T. -0.00 min

Lab File: BP004152.D

Acq: 04 Dec 2020 21:09

Instrument :
BNA_P
ClientSampleId :
SICV001

Tot Ion:	105	Resp:	810423
Ion	Ratio	Lower	Upper
105	100		
77	77.1	60.9	91.3
51	22.9	18.2	27.4

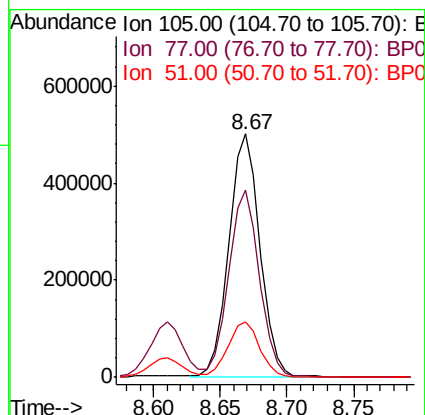

#17

N-Nitroso-di-n-propylamine

Concen: 20.601 ng/ul




RT: 8.66 min Scan# 930


Delta R.T. -0.00 min

Lab File: BP004152.D

Acq: 04 Dec 2020 21:09

Tgt Ion:	70	Resp:	419706
Ion	Ratio	Lower	Upper
70	100		
42	49.1	41.4	62.0
101	9.9	8.2	12.2
130	21.6	17.5	26.3



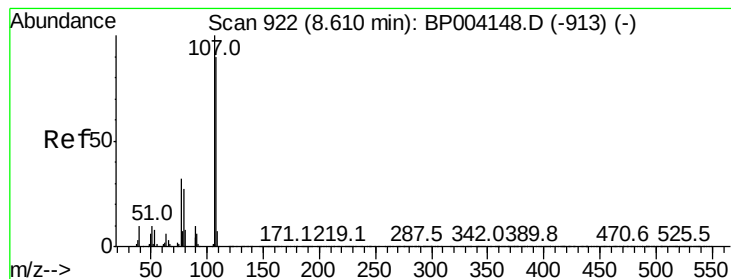

#18

4-Methylphenol

Concen: 20.473 ng/ul

RT: 8.61 min Scan# 922

Delta R.T. -0.00 min

Lab File: BP004152.D

Acq: 04 Dec 2020 21:09

Instrument :

BNA_P

ClientSampleId :





SICV001

Tot Ion:108 Resp: 539966

Ion Ratio Lower Upper

108 100

107 111.6 89.3 133.9

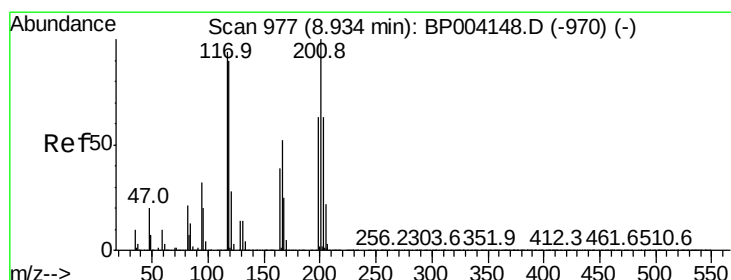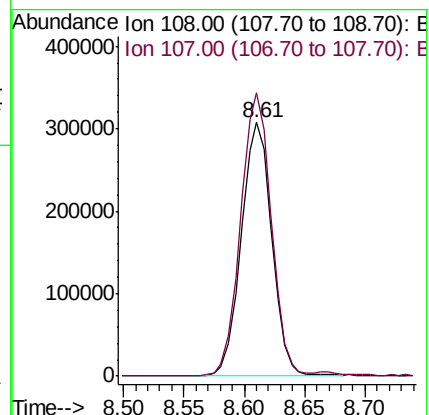

#19

Hexachloroethane

Concen: 20.385 ng/ul

RT: 8.93 min Scan# 977

Delta R.T. -0.00 min

Lab File: BP004152.D

Acq: 04 Dec 2020 21:09




Tgt Ion:117 Resp: 218261


Ion Ratio Lower Upper

117 100

201 108.6 84.3 126.5

199 64.3 53.0 79.4



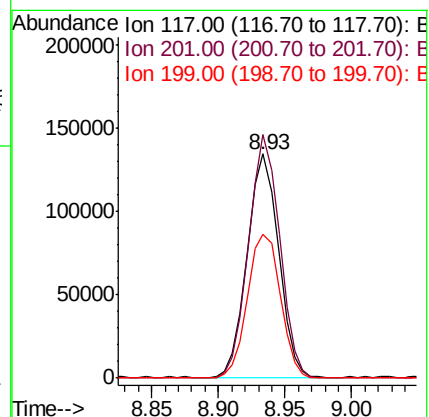





#22
Nitrobenzene
Concen: 20.567 ng/ul
RT: 9.05 min Scan# 996
Delta R.T. -0.00 min
Lab File: BP004152.D
Acq: 04 Dec 2020 21:09




Instrument :
BNA_P
ClientSampled :
SICV001


Tot Ion	Ratio	Lower	Upper
77	100		
123	45.7	37.4	56.2
65	12.3	9.9	14.9

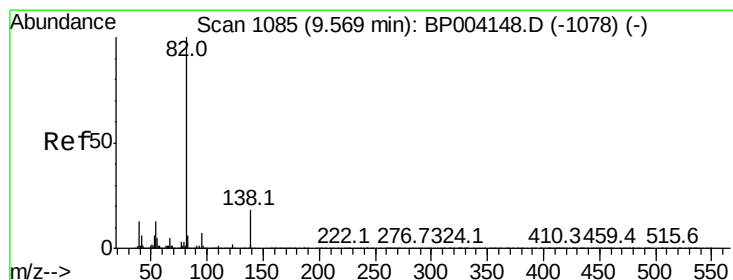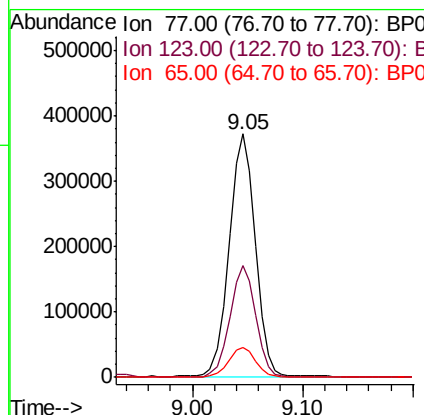

#23
Isophorone
Concen: 20.328 ng/ul
RT: 9.57 min Scan# 1085
Delta R.T. -0.00 min
Lab File: BP004152.D
Acq: 04 Dec 2020 21:09

Tgt Ion	Ratio	Lower	Upper
82	100		
95	7.3	6.0	9.0
138	17.3	14.6	21.8

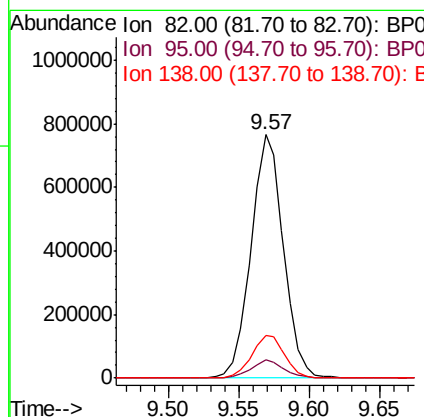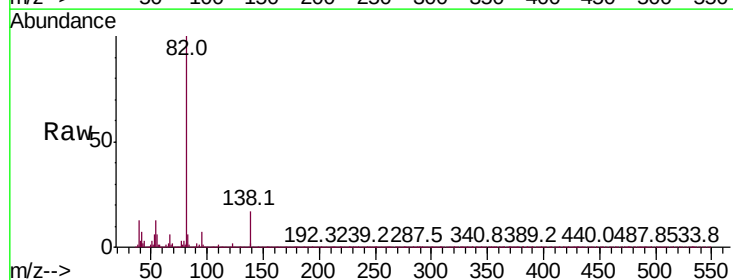



#25

2-Nitrophenol

Concen: 21.630 ng/ul

RT: 9.76 min Scan# 1117

Delta R.T. -0.00 min

Lab File: BP004152.D

Acq: 04 Dec 2020 21:09

Instrument :

BNA_P

ClientSampleId :

SICV001


Tot Ion:139 Resp: 258746

Ion Ratio Lower Upper

139 100

65 46.6 39.8 59.6




109 27.2 24.5 36.7



Abundance Ion 139.00 (138.70 to 139.70): E

Ion 65.00 (64.70 to 65.70): BP0

Ion 109.00 (108.70 to 109.70): E

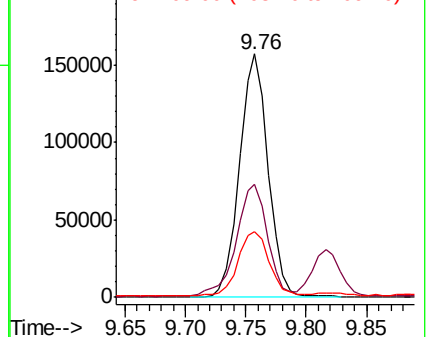

#26

2,4-Dimethylphenol

Concen: 20.183 ng/ul

RT: 9.82 min Scan# 1127

Delta R.T. -0.00 min

Lab File: BP004152.D

Acq: 04 Dec 2020 21:09


Tgt Ion:107 Resp: 585547

Ion Ratio Lower Upper

107 100

121 50.5 40.4 60.6



122 84.6 67.6 101.4




Abundance Ion 107.00 (106.70 to 107.70): E

Ion 121.00 (120.70 to 121.70): E

Ion 122.00 (121.70 to 122.70): E




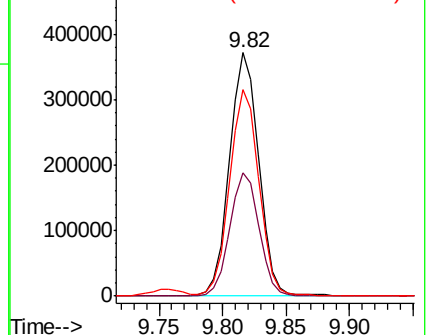


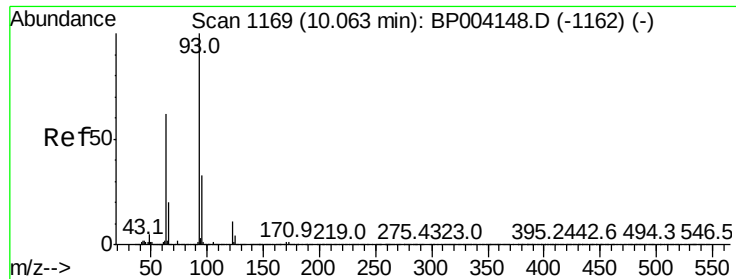

#27
 Bis(2-Chloroethoxy)methane
 Concen: 20.263 ng/ul
 RT: 10.06 min Scan# 1168
 Delta R.T. -0.01 min
 Lab File: BP004152.D
 Acq: 04 Dec 2020 21:09




Instrument :
 BNA_P
 ClientSampleId :
 SICV001


Tot Ion	Ratio	Lower	Upper
93	100		
95	33.1	27.0	40.4
123	11.3	8.8	13.2

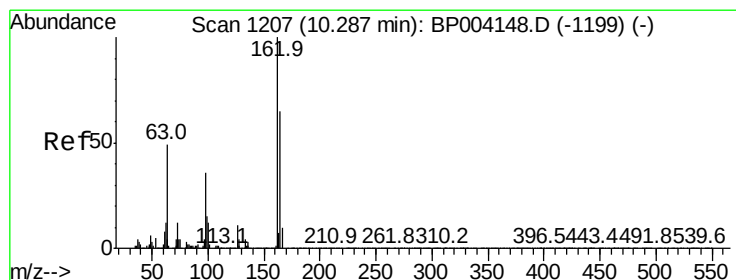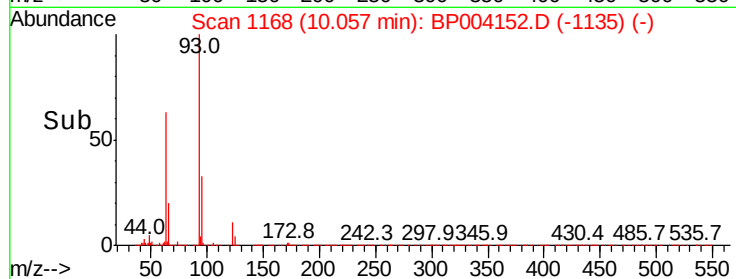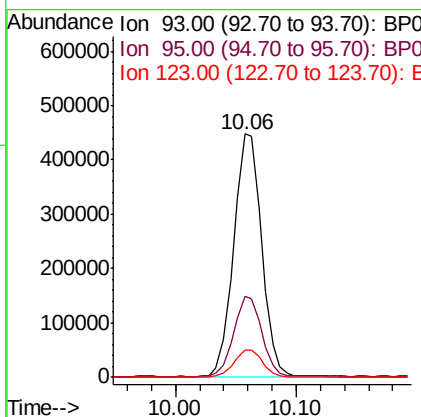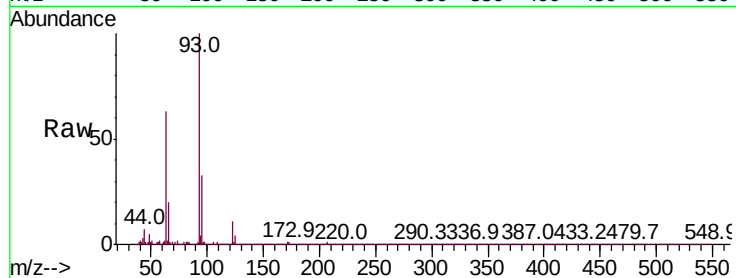

#29
 2,4-Dichlorophenol
 Concen: 20.523 ng/ul
 RT: 10.29 min Scan# 1207
 Delta R.T. -0.00 min
 Lab File: BP004152.D
 Acq: 04 Dec 2020 21:09

Tgt Ion	Ratio	Lower	Upper
162	100		
164	65.5	51.9	77.9
98	38.1	30.4	45.6

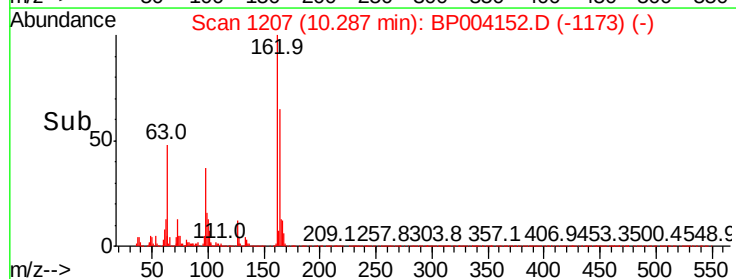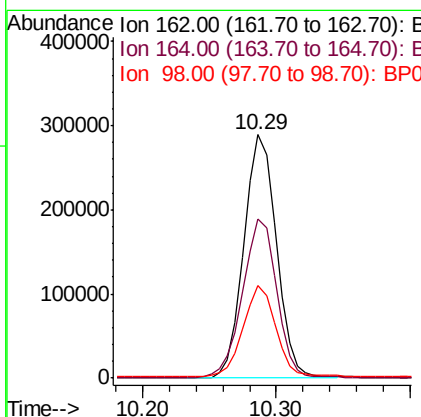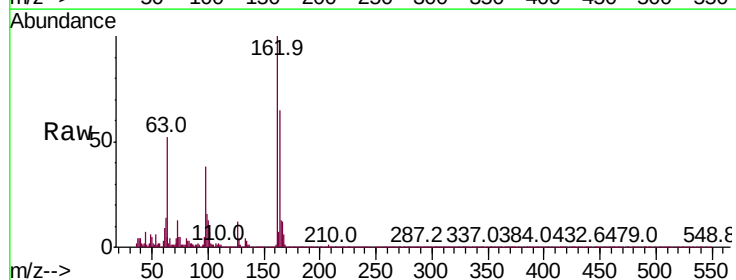

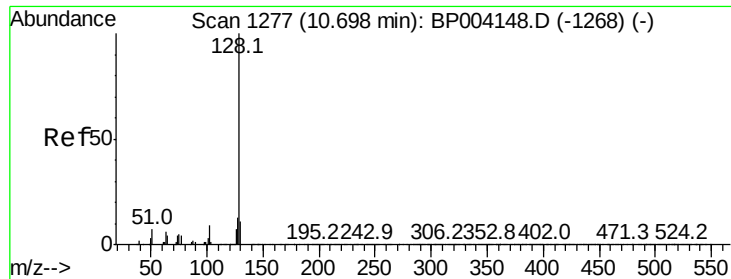

#30

Naphthalene

Concen: 20.384 ng/ul

RT: 10.70 min Scan# 1277

Delta R.T. -0.00 min

Lab File: BP004152.D

Acq: 04 Dec 2020 21:09

Instrument :

BNA_P

ClientSampled :

SICV001





Tot Ion:128 Resp: 1709484

Ion Ratio Lower Upper

128 100

129 11.1 8.9 13.3

127 13.1 10.4 15.6

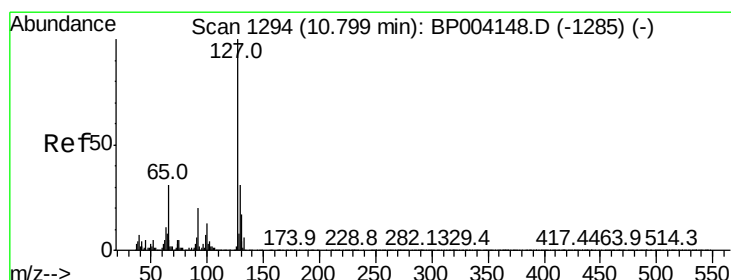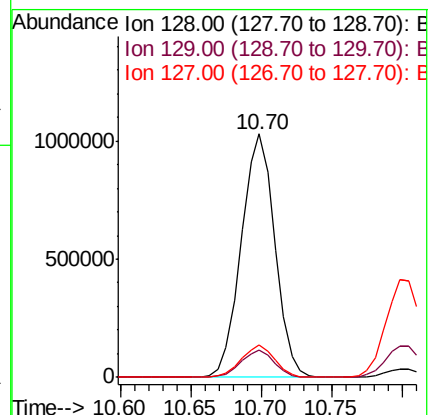

#32

4-Chloroaniline

Concen: 20.696 ng/ul

RT: 10.80 min Scan# 1294

Delta R.T. -0.00 min

Lab File: BP004152.D




Acq: 04 Dec 2020 21:09


Tgt Ion:127 Resp: 712580

Ion Ratio Lower Upper

127 100

129 31.5 25.3 37.9



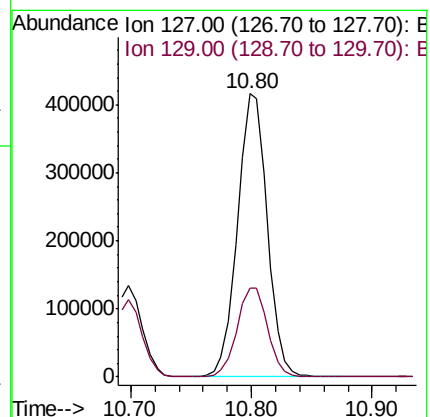
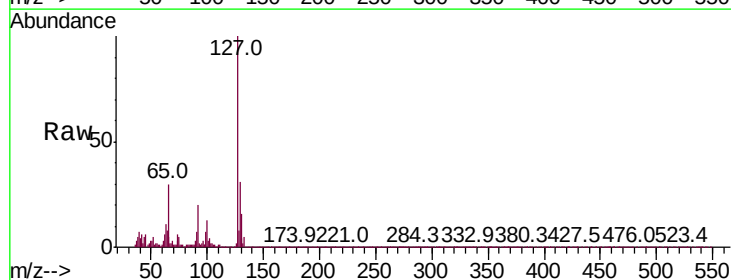




#33
Hexachlorobutadiene
Concen: 19.992 ng/ul
RT: 10.99 min Scan# 1327
Delta R.T. -0.00 min
Lab File: BP004152.D
Acq: 04 Dec 2020 21:09




Instrument :
BNA_P
ClientSampled :
SICV001


Tot Ion	Ratio	Lower	Upper
225	100		
223	63.0	49.9	74.9
227	62.3	50.9	76.3

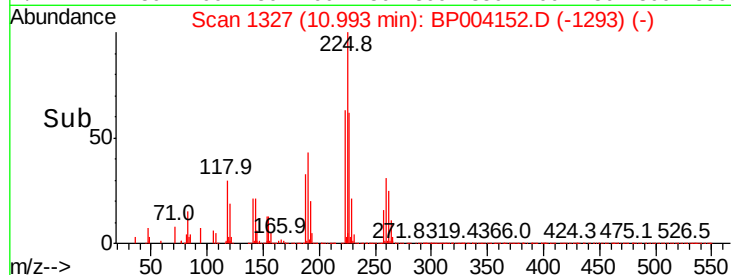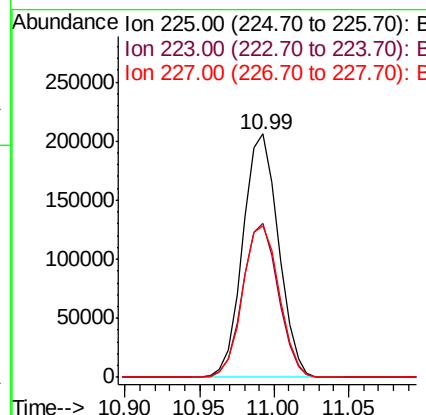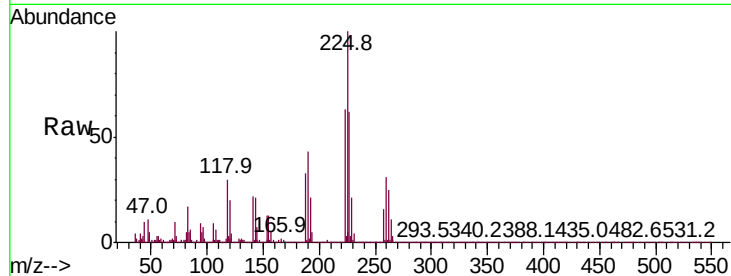

#34
Caprolactam
Concen: 12.936 ng/ul
RT: 11.55 min Scan# 1421
Delta R.T. -0.00 min
Lab File: BP004152.D
Acq: 04 Dec 2020 21:09

Tgt Ion	Ratio	Lower	Upper
113	100		
55	164.8	136.3	204.5
56	119.8	93.2	139.8


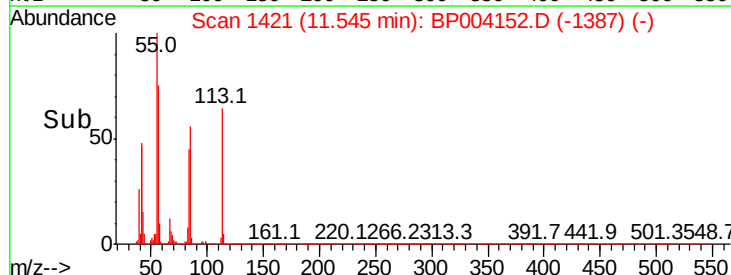
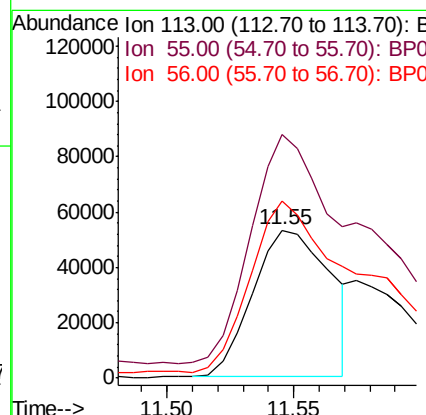
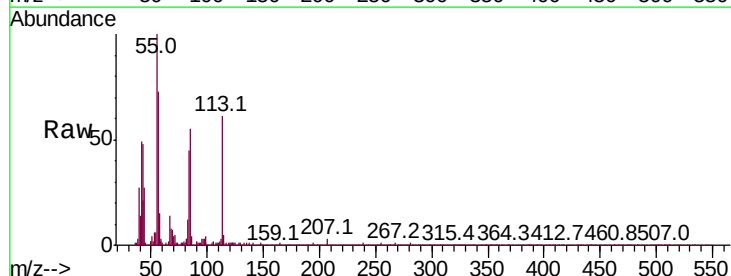




#35
4-Chloro-3-methylphenol
Concen: 20.472 ng/ul
RT: 11.92 min Scan# 1485
Delta R.T. -0.00 min
Lab File: BP004152.D
Acq: 04 Dec 2020 21:09




Instrument :
BNA_P
ClientSampleId :
SICV001


Tot Ion	Ratio	Lower	Upper
107	100		
144	26.4	20.1	30.1
142	80.2	63.4	95.0

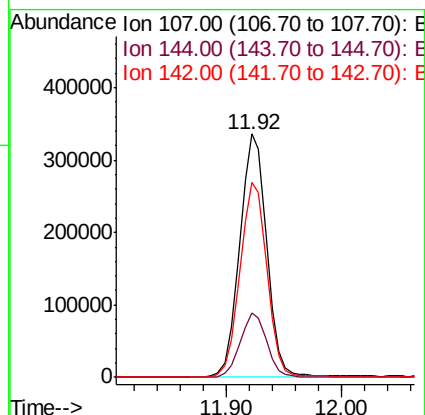

#36
2-Methylnaphthalene
Concen: 20.311 ng/ul
RT: 12.31 min Scan# 1551
Delta R.T. -0.01 min
Lab File: BP004152.D
Acq: 04 Dec 2020 21:09

Tgt Ion	Ratio	Lower	Upper
142	100		
141	88.7	71.1	106.7





#37

1-Methylnaphthalene

Concen: 20.431 ng/ul

RT: 12.53 min Scan# 1589

Delta R.T. -0.00 min

Lab File: BP004152.D

Acq: 04 Dec 2020 21:09

Instrument :

BNA_P

ClientSampleId :

SICV001


Tot Ion:142 Resp: 1160248

Ion Ratio Lower Upper

142 100

141 93.7 74.6 112.0

116 3.7 3.0 4.4






Abundance

Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

Ion 116.00 (115.70 to 116.70): E

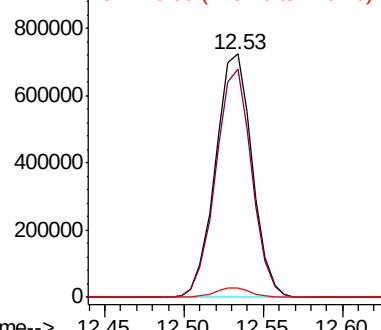

#39

1,2,4,5-Tetrachlorobenzene

Concen: 20.309 ng/ul

RT: 12.68 min Scan# 1614

Delta R.T. -0.00 min

Lab File: BP004152.D

Acq: 04 Dec 2020 21:09

Tgt Ion:216 Resp: 654179


Ion Ratio Lower Upper

216 100

214 77.7 62.4 93.6

179 19.8 16.6 25.0

108 15.6 13.0 19.4





Abundance


Ion 216.00 (215.70 to 216.70): E

Ion 214.00 (213.70 to 214.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 108.00 (107.70 to 108.70): E




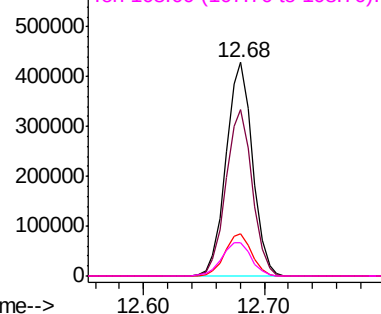




#40
Hexachlorocyclopentadiene
Concen: 19.567 ng/ul
RT: 12.67 min Scan# 1612
Delta R.T. -0.00 min
Lab File: BP004152.D
Acq: 04 Dec 2020 21:09




Instrument :
BNA_P
ClientSampleId :
SICV001


Tot Ion	Ratio	Lower	Upper
237	100		
235	62.9	50.6	75.8
272	13.0	10.3	15.5

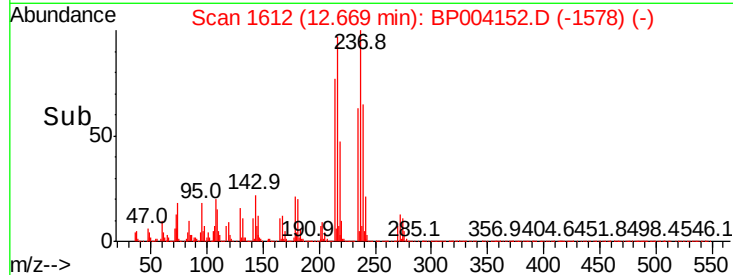

#41
2,4,6-Trichlorophenol
Concen: 21.016 ng/ul
RT: 12.92 min Scan# 1654
Delta R.T. -0.00 min
Lab File: BP004152.D
Acq: 04 Dec 2020 21:09

Tgt Ion	Ratio	Lower	Upper
196	100		
198	96.3	75.9	113.9
200	31.3	24.6	36.8


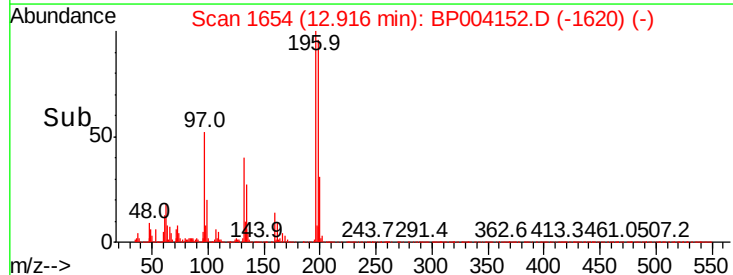






#42
 2,4,5-Trichlorophenol
 Concen: 20.812 ng/ul
 RT: 12.99 min Scan# 1666
 Delta R.T. -0.00 min
 Lab File: BP004152.D
 Acq: 04 Dec 2020 21:09




Instrument :
 BNA_P
 ClientSampleId :
 SICV001


Tot Ion	Ratio	Lower	Upper
196	100		
198	96.2	78.2	117.4
200	30.6	25.1	37.7

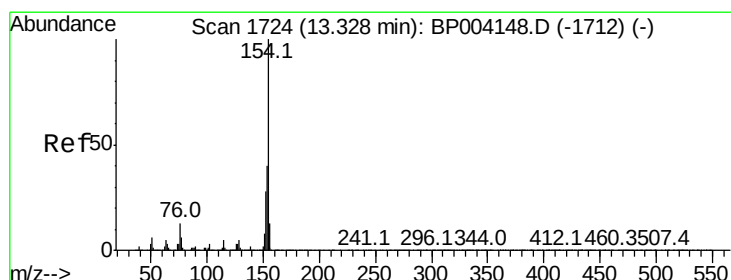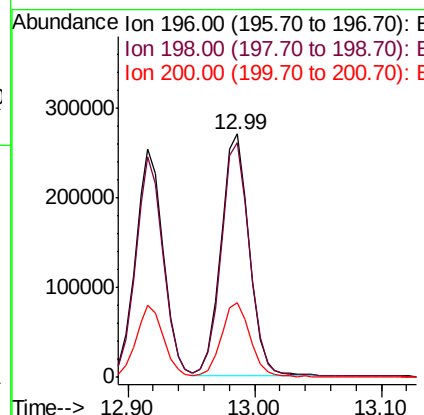

#43
 1,1'-Biphenyl
 Concen: 20.430 ng/ul
 RT: 13.33 min Scan# 1724
 Delta R.T. -0.00 min
 Lab File: BP004152.D
 Acq: 04 Dec 2020 21:09

Tgt Ion	Ratio	Lower	Upper
154	100		
153	40.3	32.2	48.2
76	12.8	10.8	16.2


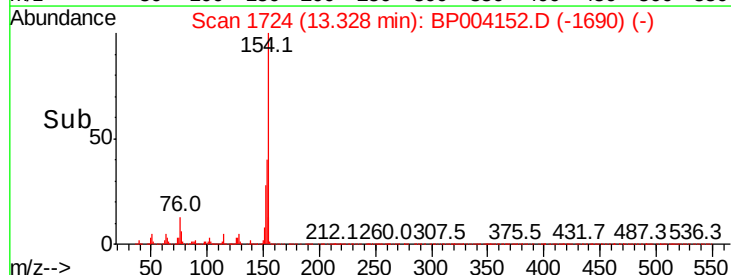
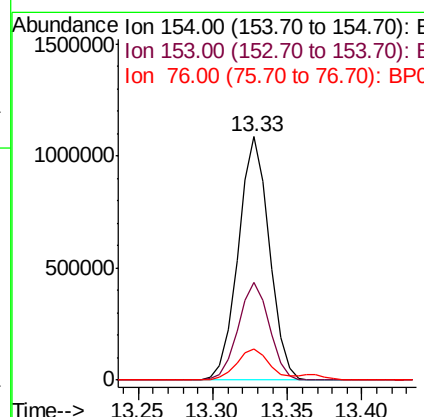





#44
2-Chloronaphthalene
Concen: 20.496 ng/ul
RT: 13.36 min Scan# 1730
Delta R.T. -0.01 min
Lab File: BP004152.D
Acq: 04 Dec 2020 21:09




Instrument :
BNA_P
ClientSampleId :
SICV001


Tot Ion:162 Resp: 1246641
Ion Ratio Lower Upper
162 100
164 33.1 26.2 39.4
127 38.0 30.4 45.6

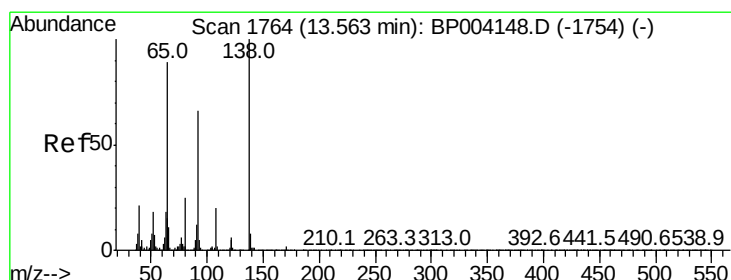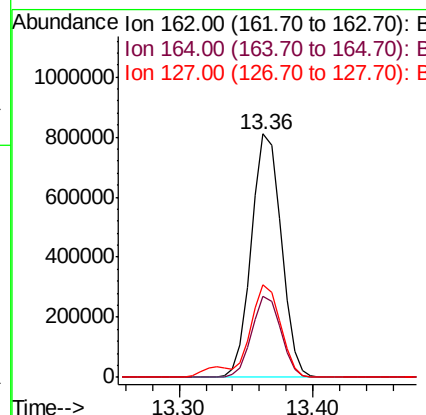

#45
2-Nitroaniline
Concen: 21.601 ng/ul
RT: 13.56 min Scan# 1764
Delta R.T. -0.00 min
Lab File: BP004152.D
Acq: 04 Dec 2020 21:09

Tgt Ion: 65 Resp: 322600
Ion Ratio Lower Upper
65 100
92 73.6 59.4 89.2
138 111.2 89.6 134.4

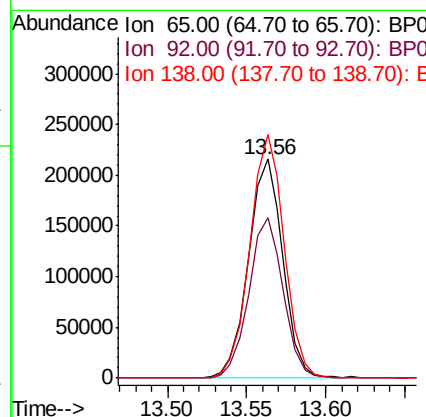



#47

Dimethylphthalate

Concen: 20.329 ng/ul

RT: 13.95 min Scan# 1830

Delta R.T. -0.00 min

Lab File: BP004152.D

Acq: 04 Dec 2020 21:09

Instrument :

BNA_P

ClientSampleId :

SICV001


Tot Ion:163 Resp: 1572179

Ion Ratio Lower Upper

163 100

194 4.2 3.4 5.0




164 10.2 8.1 12.1



Abundance Ion 163.00 (162.70 to 163.70): E

1500000 Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

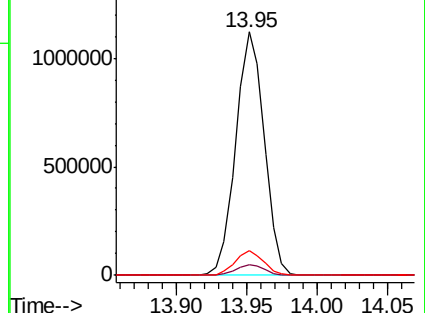

#48

2,6-Dinitrotoluene

Concen: 21.699 ng/ul

RT: 14.06 min Scan# 1849

Delta R.T. -0.00 min

Lab File: BP004152.D

Acq: 04 Dec 2020 21:09


Tgt Ion:165 Resp: 304572

Ion Ratio Lower Upper

165 100

89 55.0 45.2 67.8



121 20.9 17.9 26.9




Abundance Ion 165.00 (164.70 to 165.70): E

Ion 89.00 (88.70 to 89.70): BP0

Ion 121.00 (120.70 to 121.70): E

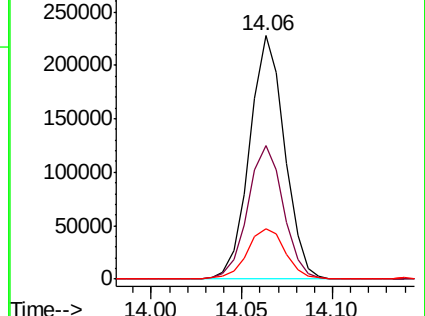



#50

Acenaphthylene

Concen: 20.522 ng/ul

RT: 14.22 min Scan# 1875

Delta R.T. -0.00 min

Lab File: BP004152.D

Acq: 04 Dec 2020 21:09

Instrument :


BNA_P

ClientSampleId :

SICV001

Tot Ion:152 Resp: 1903588

Ion	Ratio	Lower	Upper
152	100		
151	20.1	16.1	24.1
153	13.1	10.5	15.7






Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E

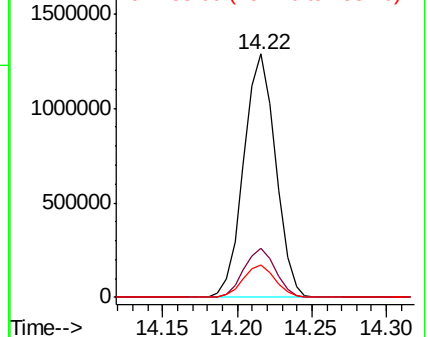

#51

3-Nitroaniline

Concen: 20.791 ng/ul

RT: 14.39 min Scan# 1904


Delta R.T. -0.01 min

Lab File: BP004152.D

Acq: 04 Dec 2020 21:09

Tgt Ion:138 Resp: 272354

Ion	Ratio	Lower	Upper
138	100		
108	13.1	12.6	19.0
92	119.1	93.3	139.9






Abundance

Ion 138.00 (137.70 to 138.70): E

Ion 108.00 (107.70 to 108.70): E

Ion 92.00 (91.70 to 92.70): BPO

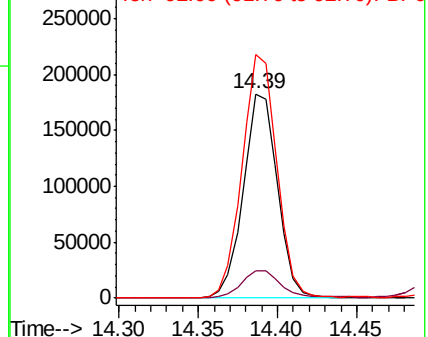



#52

Acenaphthene

Concen: 20.304 ng/ul

RT: 14.56 min Scan# 1933

Delta R.T. -0.01 min

Lab File: BP004152.D

Acq: 04 Dec 2020 21:09

Instrument :

BNA_P

ClientSampleId :

SICV001





Tot Ion:153 Resp: 1328697

Ion Ratio Lower Upper

153 100

152 47.4 38.0 57.0

154 89.4 70.5 105.7

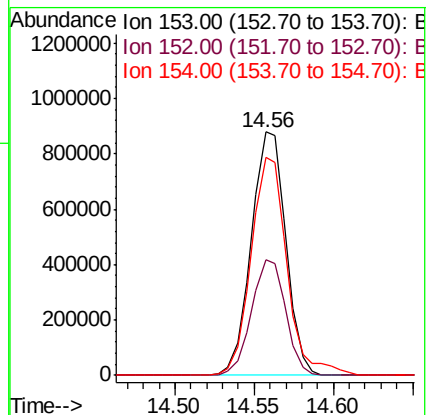

#53

2,4-Dinitrophenol

Concen: 19.138 ng/ul

RT: 14.59 min Scan# 1939

Delta R.T. -0.00 min

Lab File: BP004152.D

Acq: 04 Dec 2020 21:09




Tgt Ion:184 Resp: 103554


Ion Ratio Lower Upper

184 100

63 55.5 43.6 65.4

154 62.2 46.9 70.3



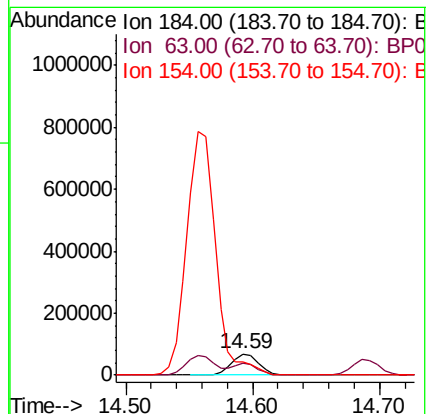





#55
4-Nitrophenol
Concen: 20.484 ng/ul
RT: 14.69 min Scan# 1956
Delta R.T. -0.00 min
Lab File: BP004152.D
Acq: 04 Dec 2020 21:09




Instrument :
BNA_P
ClientSampleId :
SICV001


Tot Ion	Ratio	Lower	Upper
109	100		
139	145.0	111.9	167.9
65	131.1	99.2	148.8

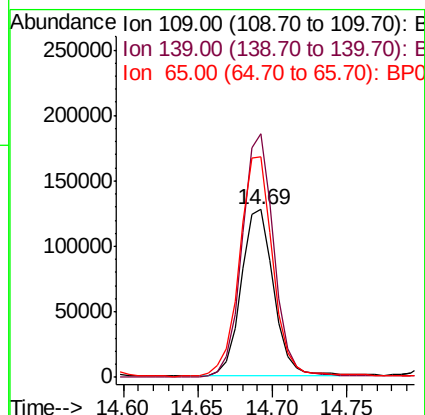

#56
Dibenzofuran
Concen: 20.544 ng/ul
RT: 14.90 min Scan# 1991
Delta R.T. -0.00 min
Lab File: BP004152.D
Acq: 04 Dec 2020 21:09

Tgt Ion	Ratio	Lower	Upper
168	100		
139	35.3	28.6	42.8


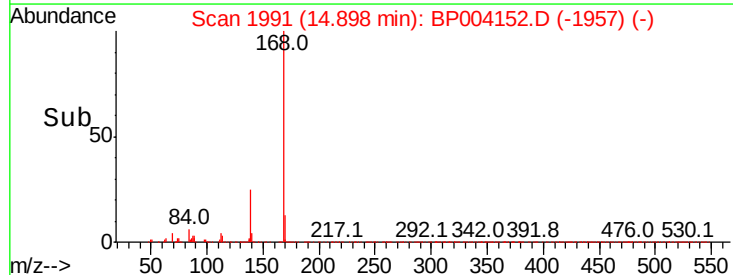






#57
2,4-Dinitrotoluene
Concen: 22.135 ng/ul
RT: 14.85 min Scan# 1983
Delta R.T. -0.00 min
Lab File: BP004152.D
Acq: 04 Dec 2020 21:09




Instrument :
BNA_P
ClientSampleId :
SICV001


Tot Ion	Ratio	Lower	Upper
165	100		
63	40.0	32.1	48.1
182	3.0	2.4	3.6

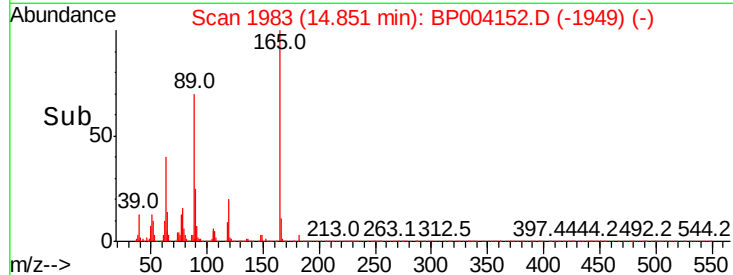

#58
2,3,4,6-Tetrachlorophenol
Concen: 21.255 ng/ul
RT: 15.12 min Scan# 2028
Delta R.T. -0.01 min
Lab File: BP004152.D
Acq: 04 Dec 2020 21:09

Tgt Ion	Ratio	Lower	Upper
232	100		
131	41.5	31.5	47.3
130	2.4	1.7	2.5
166	29.6	22.7	34.1

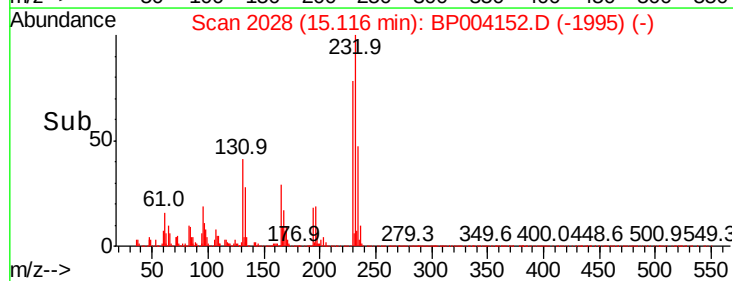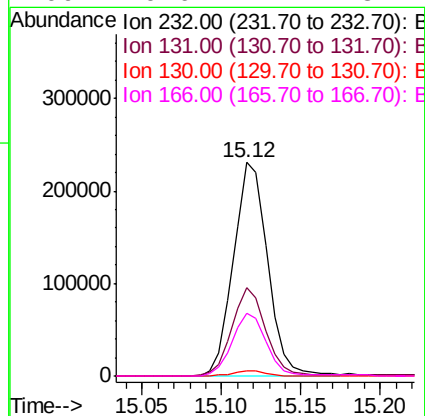



#59

Diethylphthalate

Concen: 20.293 ng/ul

RT: 15.33 min Scan# 2064

Delta R.T. -0.00 min

Lab File: BP004152.D

Acq: 04 Dec 2020 21:09

Instrument :

BNA_P

ClientSampleId :

SICV001


Tot Ion:149 Resp: 1584168

Ion Ratio Lower Upper

149 100

177 23.1 18.5 27.7




150 12.7 10.1 15.1



Abundance Ion 149.00 (148.70 to 149.70): E

Ion 177.00 (176.70 to 177.70): E

Ion 150.00 (149.70 to 150.70): E

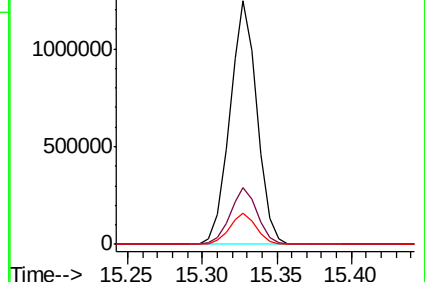

#61

Fluorene

Concen: 20.544 ng/ul

RT: 15.55 min Scan# 2102

Delta R.T. -0.00 min

Lab File: BP004152.D

Acq: 04 Dec 2020 21:09


Tgt Ion:166 Resp: 1546273

Ion Ratio Lower Upper

166 100

165 96.5 77.8 116.6



167 13.6 11.0 16.4




Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E




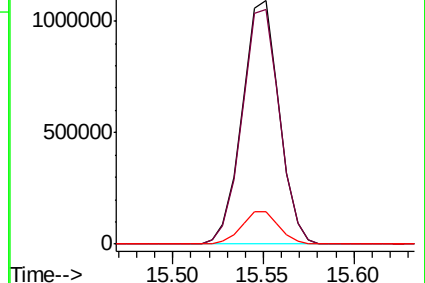


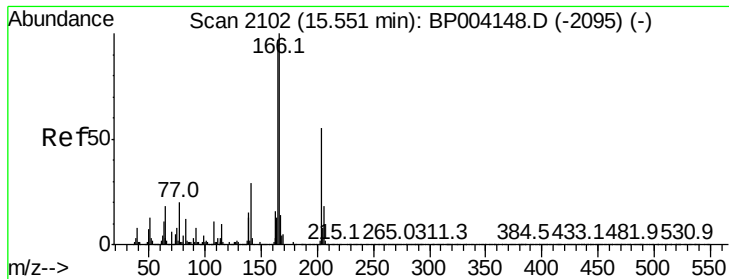

#62
4-Chlorophenyl-phenylether
Concen: 20.194 ng/ul
RT: 15.55 min Scan# 2101
Delta R.T. -0.01 min
Lab File: BP004152.D
Acq: 04 Dec 2020 21:09




Instrument :
BNA_P
ClientSampleId :
SICV001


Tot Ion	Ratio	Lower	Upper
204	100		
206	32.8	26.7	40.1
141	54.7	42.2	63.2

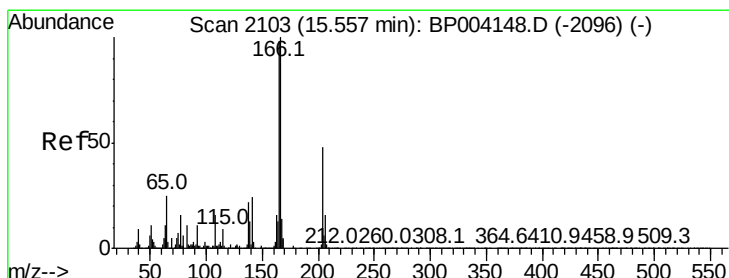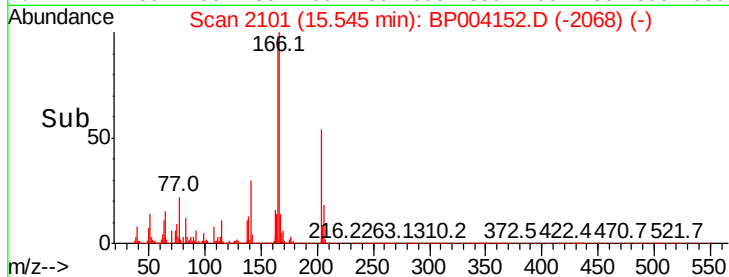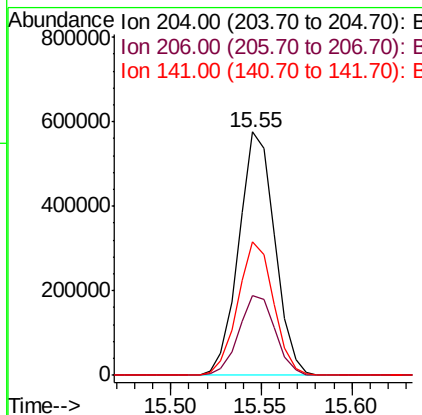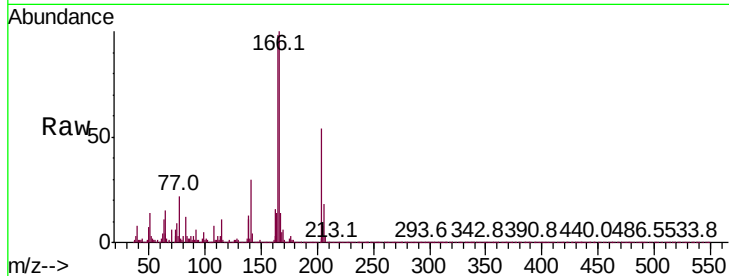

#63
4-Nitroaniline
Concen: 22.575 ng/ul
RT: 15.56 min Scan# 2103
Delta R.T. -0.00 min
Lab File: BP004152.D
Acq: 04 Dec 2020 21:09

Tgt Ion	Ratio	Lower	Upper
138	100		
92	52.5	42.3	63.5
108	72.5	60.2	90.2


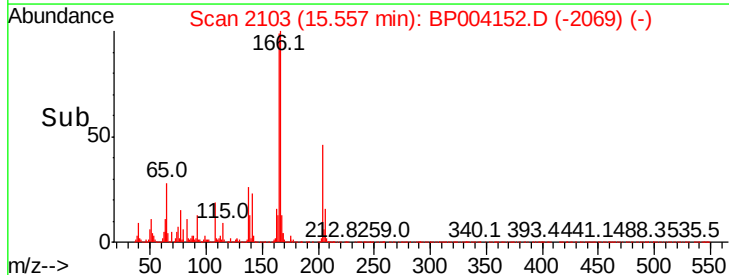
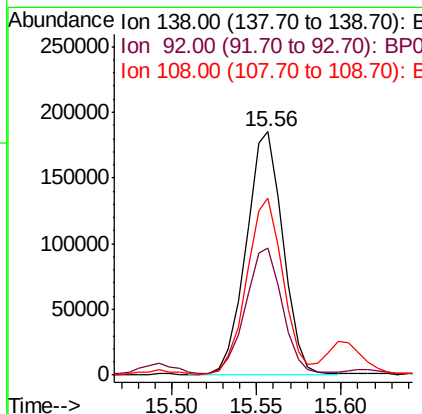
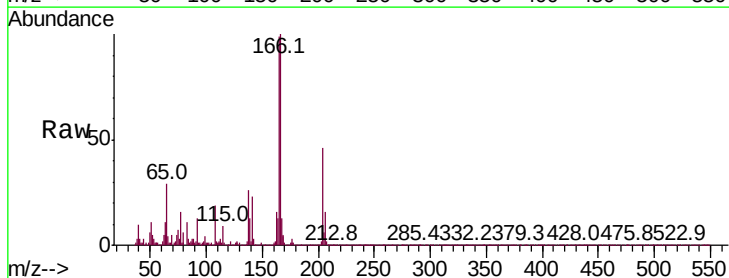




#66
4,6-Dinitro-2-methylphenol
Concen: 19.754 ng/ul
RT: 15.62 min Scan# 2113
Delta R.T. -0.00 min
Lab File: BP004152.D
Acq: 04 Dec 2020 21:09




Instrument :
BNA_P
ClientSampleId :
SICV001


Tot Ion	Ratio	Lower	Upper
198	100		
182	3.9	3.8	5.6
77	24.0	19.7	29.5

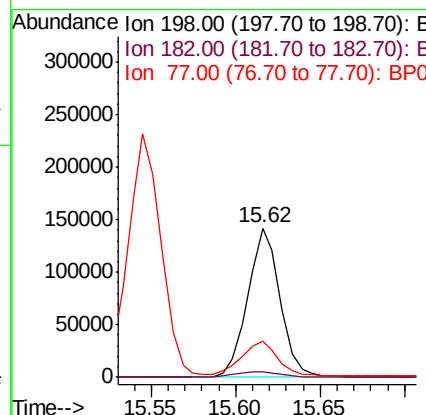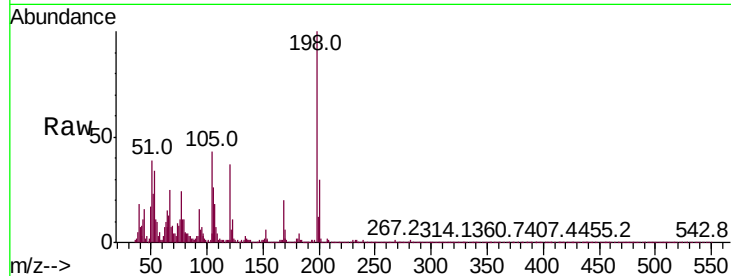

#67
N-Nitrosodiphenylamine
Concen: 20.339 ng/ul
RT: 15.76 min Scan# 2137
Delta R.T. -0.00 min
Lab File: BP004152.D
Acq: 04 Dec 2020 21:09

Tgt Ion	Ratio	Lower	Upper
169	100		
168	66.1	52.7	79.1
167	36.2	28.2	42.2


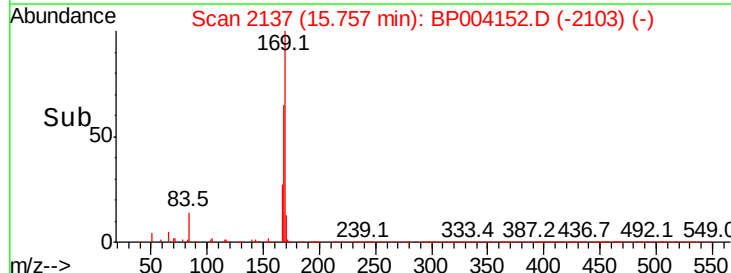
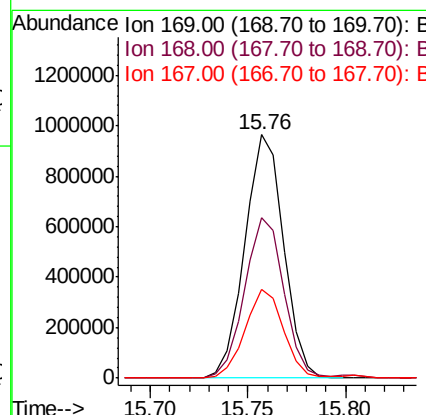





#68
4-Bromophenyl-phenylether
Concen: 20.181 ng/ul
RT: 16.45 min Scan# 2254
Delta R.T. -0.00 min
Lab File: BP004152.D
Acq: 04 Dec 2020 21:09




Instrument :
BNA_P
ClientSampled :
SICV001


Tot Ion:248 Resp: 512728
Ion Ratio Lower Upper
248 100
250 98.0 75.5 113.3
141 67.1 53.2 79.8

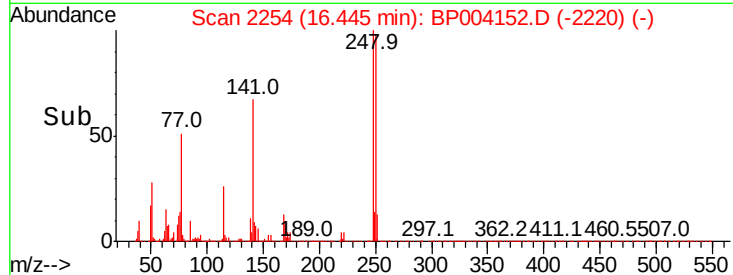

#69
Hexachlorobenzene
Concen: 20.393 ng/ul
RT: 16.56 min Scan# 2273
Delta R.T. -0.00 min
Lab File: BP004152.D
Acq: 04 Dec 2020 21:09

Tgt Ion:284 Resp: 577819
Ion Ratio Lower Upper
284 100
142 30.3 25.4 38.0
249 31.2 25.4 38.2


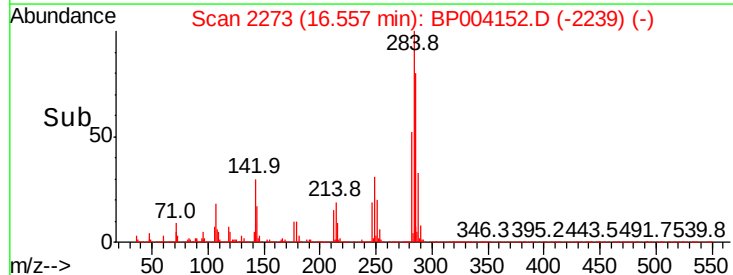






#70
Atrazine
Concen: 20.699 ng/ul
RT: 16.72 min Scan# 2300
Delta R.T. -0.00 min
Lab File: BP004152.D
Acq: 04 Dec 2020 21:09




Instrument :
BNA_P
ClientSampled :
SICV001


Tot Ion	Ratio	Lower	Upper
200	100		
173	25.9	21.4	32.0
215	49.9	39.9	59.9

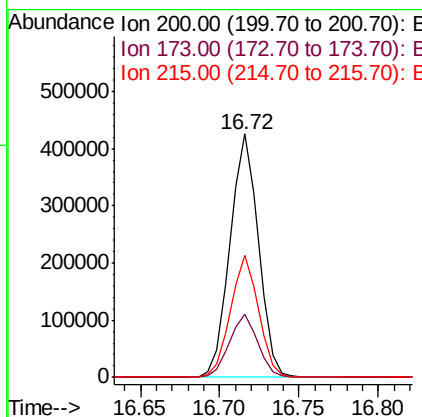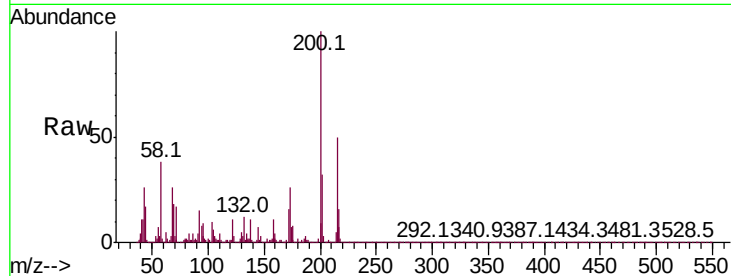

#71
Pentachlorophenol
Concen: 20.229 ng/ul
RT: 16.90 min Scan# 2331
Delta R.T. -0.00 min
Lab File: BP004152.D
Acq: 04 Dec 2020 21:09

Tgt Ion	Ratio	Lower	Upper
266	100		
264	64.5	49.2	73.8
268	64.1	50.0	75.0

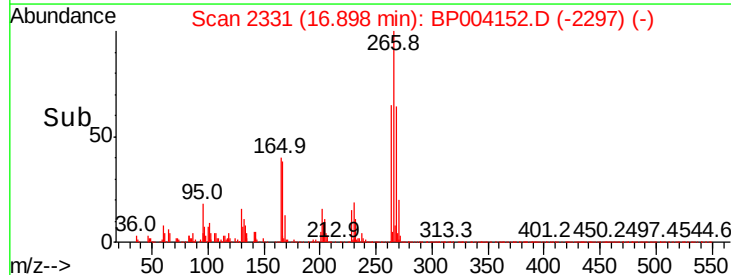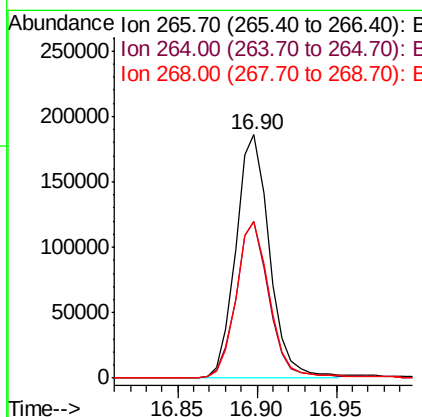



#72

Phenanthrene

Concen: 20.465 ng/ul

RT: 17.30 min Scan# 2399

Delta R.T. -0.00 min

Lab File: BP004152.D

Acq: 04 Dec 2020 21:09

Instrument :


BNA_P

ClientSampleId :

SICV001

Tot Ion:178 Resp: 2498936

Ion	Ratio	Lower	Upper
178	100		
179	15.4	12.1	18.1
176	19.4	15.4	23.2






Abundance

Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

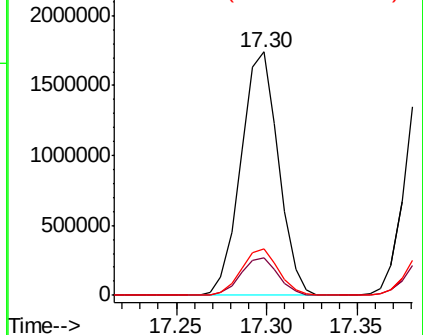

#74

Anthracene

Concen: 20.524 ng/ul

RT: 17.39 min Scan# 2414


Delta R.T. -0.01 min

Lab File: BP004152.D

Acq: 04 Dec 2020 21:09

Tgt Ion:178 Resp: 2553202

Ion	Ratio	Lower	Upper
178	100		
179	15.6	12.2	18.2
176	18.9	14.6	22.0






Abundance

Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

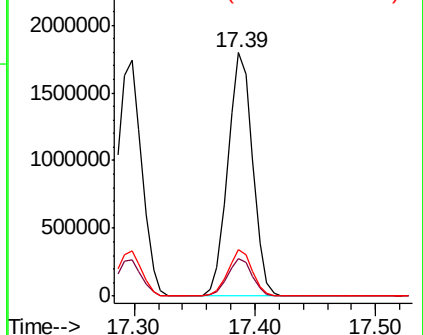

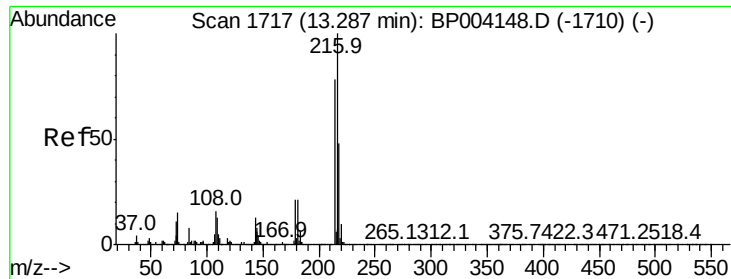

#75

1,2,3,4-Tetrachlorobenzene

Concen: 20.153 ng/uL

RT: 13.29 min Scan# 1717

Delta R.T. -0.00 min

Lab File: BP004152.D

Acq: 04 Dec 2020 21:09

Instrument :

BNA_P

ClientSampled :

SICV001


Tot Ion:216 Resp: 649412

Ion Ratio Lower Upper

216 100

214 78.0 62.5 93.7




218 47.8 38.3 57.5



Abundance Ion 216.00 (215.70 to 216.70): E

Ion 214.00 (213.70 to 214.70): E

Ion 218.00 (217.70 to 218.70): E

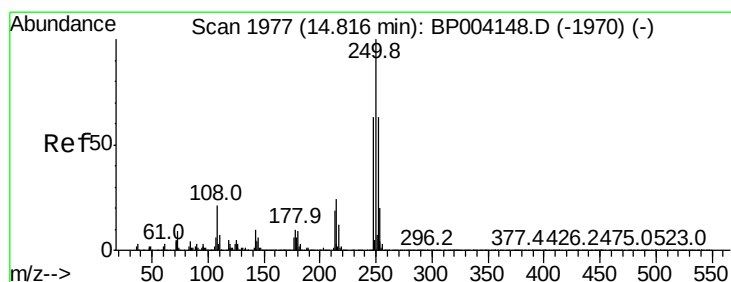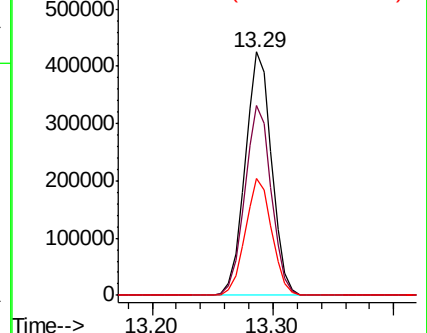

#76

Pentachlorobenzene

Concen: 20.328 ng/uL

RT: 14.82 min Scan# 1977

Delta R.T. -0.00 min

Lab File: BP004152.D

Acq: 04 Dec 2020 21:09


Tgt Ion:250 Resp: 662094

Ion Ratio Lower Upper

250 100

248 62.9 50.5 75.7



252 64.1 50.4 75.6

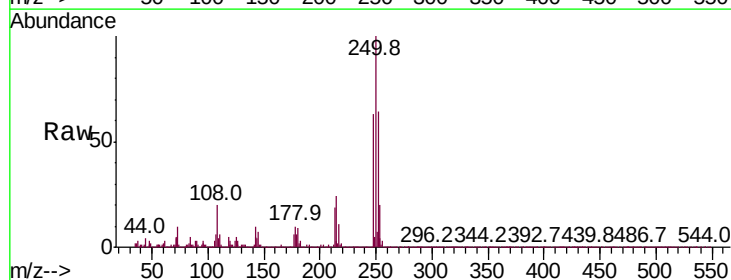


Abundance Ion 250.00 (249.70 to 250.70): E

Ion 248.00 (247.70 to 248.70): E

Ion 252.00 (251.70 to 252.70): E

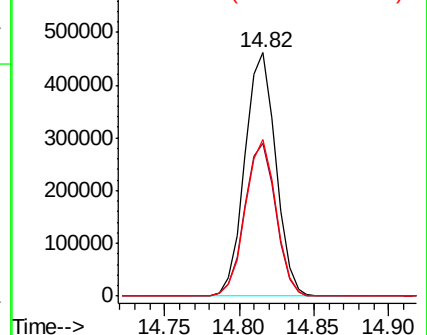



#77

Carbazole

Concen: 21.262 ng/ul

RT: 17.66 min Scan# 2460

Delta R.T. -0.00 min

Lab File: BP004152.D

Acq: 04 Dec 2020 21:09

Instrument :


BNA_P

ClientSampleId :

SICV001

Tot Ion:167 Resp: 2246407

Ion	Ratio	Lower	Upper
167	100		
166	21.6	17.2	25.8
139	12.6	9.8	14.8






Abundance

Ion 167.00 (166.70 to 167.70): E

Ion 166.00 (165.70 to 166.70): E

Ion 139.00 (138.70 to 139.70): E

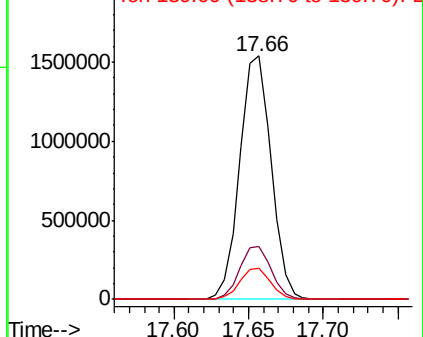

#78

Di-n-butylphthalate

Concen: 20.215 ng/ul

RT: 18.23 min Scan# 2557


Delta R.T. -0.00 min

Lab File: BP004152.D

Acq: 04 Dec 2020 21:09

Tgt Ion:149 Resp: 2783943

Ion	Ratio	Lower	Upper
149	100		
150	9.2	7.4	11.0
104	4.6	3.8	5.8






Abundance

Ion 149.00 (148.70 to 149.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 104.00 (103.70 to 104.70): E




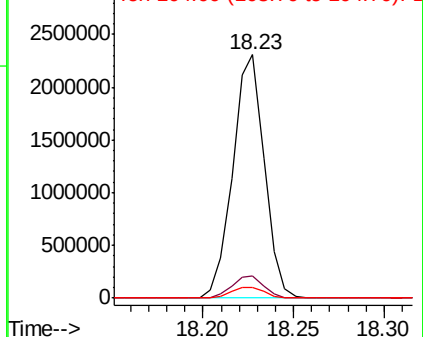


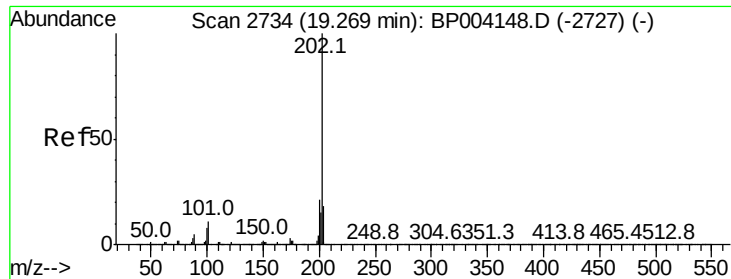

#80
Fluoranthene
Concen: 20.651 ng/ul
RT: 19.27 min Scan# 2734
Delta R.T. -0.00 min
Lab File: BP004152.D
Acq: 04 Dec 2020 21:09




Instrument :
BNA_P
ClientSampleId :
SICV001


Tot Ion:202 Resp: 3048300
Ion Ratio Lower Upper
202 100
101 11.3 8.6 12.8
100 8.5 6.6 9.8

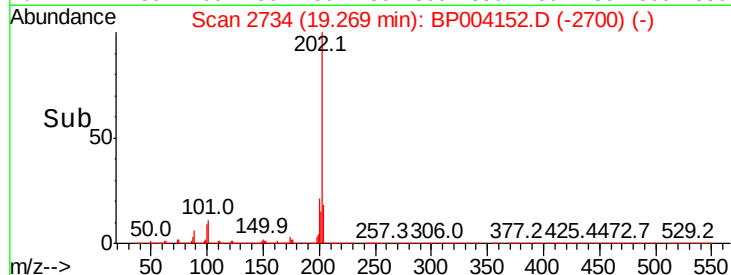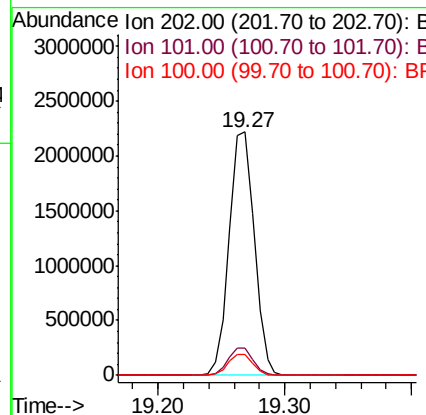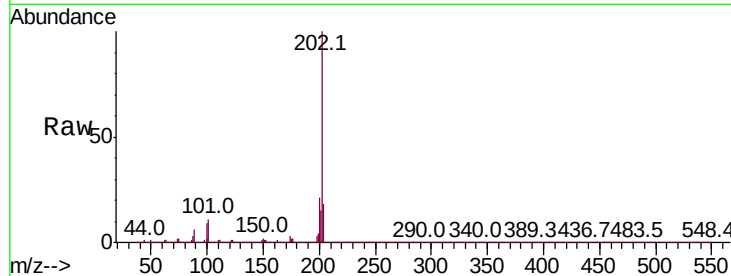

#82
Pyrene
Concen: 20.716 ng/ul
RT: 19.62 min Scan# 2794
Delta R.T. -0.00 min
Lab File: BP004152.D
Acq: 04 Dec 2020 21:09

Tgt Ion:202 Resp: 3106181
Ion Ratio Lower Upper
202 100
101 12.5 10.0 15.0
100 9.8 8.2 12.2



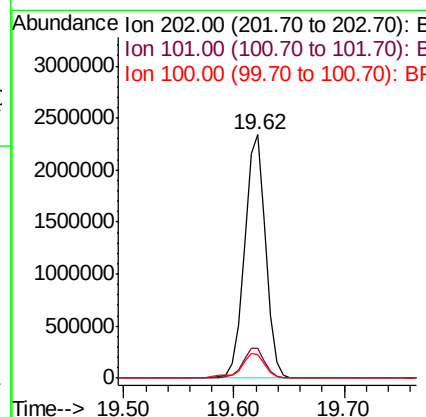





#83
Butylbenzylphthalate
Concen: 20.366 ng/ul
RT: 20.50 min Scan# 2944
Delta R.T. -0.00 min
Lab File: BP004152.D
Acq: 04 Dec 2020 21:09




Instrument :
BNA_P
ClientSampleId :
SICV001


Tot Ion:149 Resp: 1240611
Ion Ratio Lower Upper
149 100
91 68.3 56.8 85.2
206 23.0 17.9 26.9

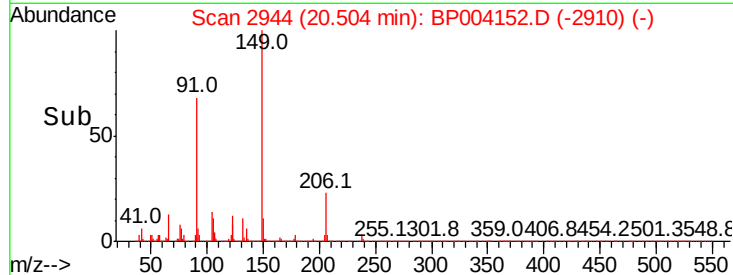

#84
3,3'-Dichlorobenzidine
Concen: 20.505 ng/ul
RT: 21.26 min Scan# 3073
Delta R.T. -0.00 min
Lab File: BP004152.D
Acq: 04 Dec 2020 21:09

Tgt Ion:252 Resp: 1030810
Ion Ratio Lower Upper
252 100
254 63.9 51.8 77.8
126 10.1 8.5 12.7









#85
 Benzo(a)anthracene
 Concen: 20.756 ng/ul
 RT: 21.33 min Scan# 3084
 Delta R.T. -0.00 min
 Lab File: BP004152.D
 Acq: 04 Dec 2020 21:09

Instrument :
 BNA_P
 ClientSampleId :
 SICV001

Tot Ion:228 Resp: 3093743




Ion	Ratio	Lower	Upper
228	100		
229	19.8	15.9	23.9
226	27.3	22.0	33.0

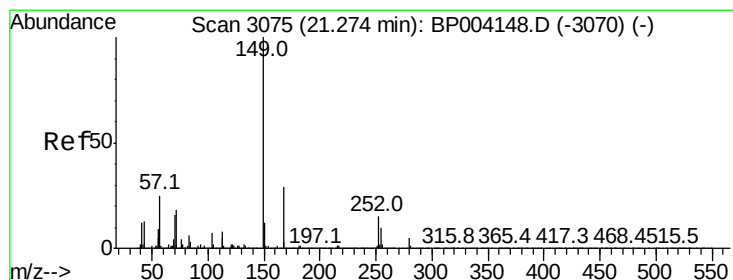


#86
 Bis(2-ethylhexyl)phthalate
 Concen: 20.328 ng/ul
 RT: 21.27 min Scan# 3075
 Delta R.T. -0.00 min
 Lab File: BP004152.D
 Acq: 04 Dec 2020 21:09

Tgt Ion:149 Resp: 1868312

Ion	Ratio	Lower	Upper
149	100		
167	28.6	22.9	34.3
279	5.0	3.8	5.6

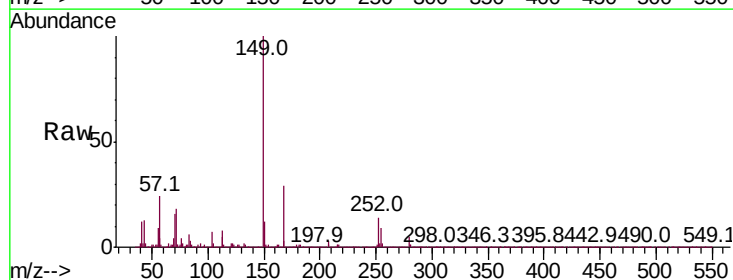



#87

Chrysene

Concen: 20.571 ng/ul

RT: 21.38 min Scan# 3093

Delta R.T. -0.01 min

Lab File: BP004152.D

Acq: 04 Dec 2020 21:09

Instrument :

BNA_P

ClientSampleId :

SICV001


Tot Ion:228 Resp: 2936572

Ion	Ratio	Lower	Upper
228	100		
226	30.7	24.1	36.1
229	20.0	15.7	23.5

228 100

226 30.7 24.1 36.1




229 20.0 15.7 23.5



Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

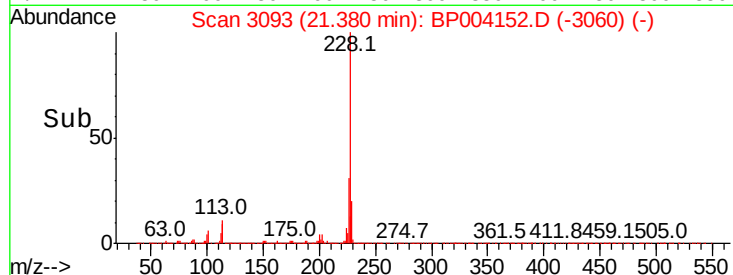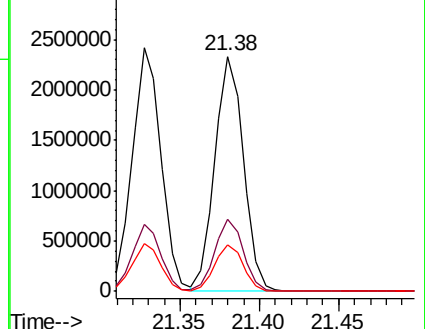

#89

Di-n-octyl phthalate

Concen: 21.680 ng/ul


RT: 22.19 min Scan# 3231

Delta R.T. -0.01 min



Lab File: BP004152.D


Acq: 04 Dec 2020 21:09

Tgt Ion:149 Resp: 3170659



Abundance Ion 149.00 (148.70 to 149.70): E

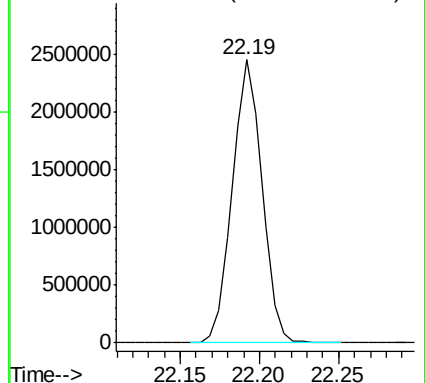

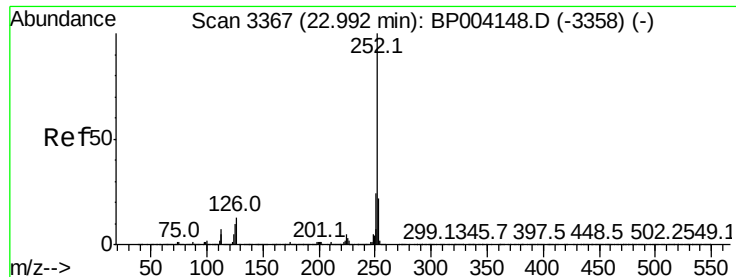

#90

Benzo(b)fluoranthene

Concen: 20.650 ng/ul

RT: 22.99 min Scan# 3367

Delta R.T. -0.00 min

Lab File: BP004152.D

Acq: 04 Dec 2020 21:09

Instrument :

BNA_P

ClientSampled :

SICV001


Tot Ion:252 Resp: 3254466

Ion Ratio Lower Upper

252 100

253 21.9 17.6 26.4




125 9.4 7.9 11.9

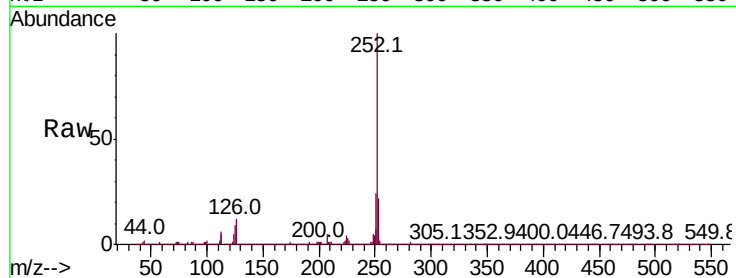

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

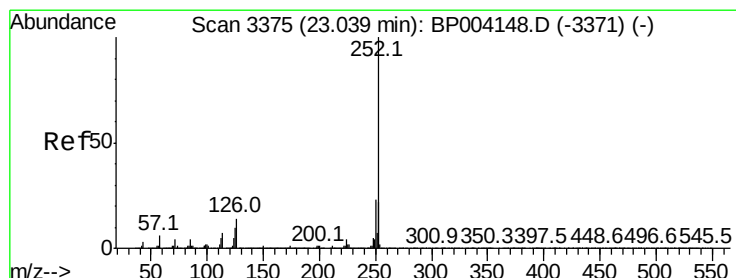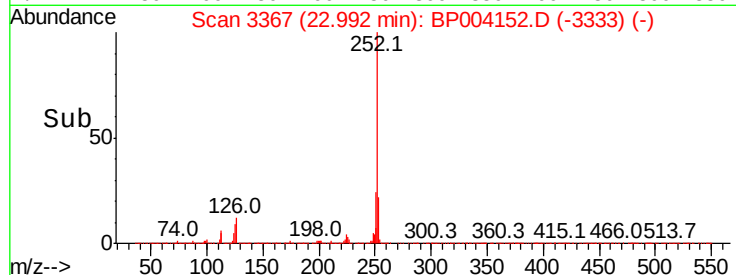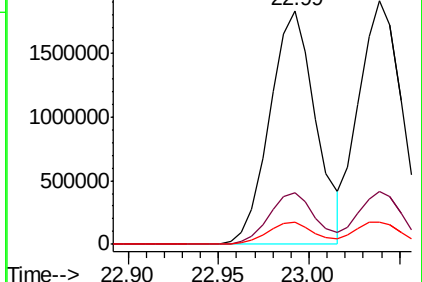

#91

Benzo(k)fluoranthene

Concen: 20.589 ng/ul

RT: 23.04 min Scan# 3375

Delta R.T. -0.00 min

Lab File: BP004152.D

Acq: 04 Dec 2020 21:09


Tgt Ion:252 Resp: 3143072

Ion Ratio Lower Upper

252 100

253 22.0 17.9 26.9



125 9.4 7.8 11.8

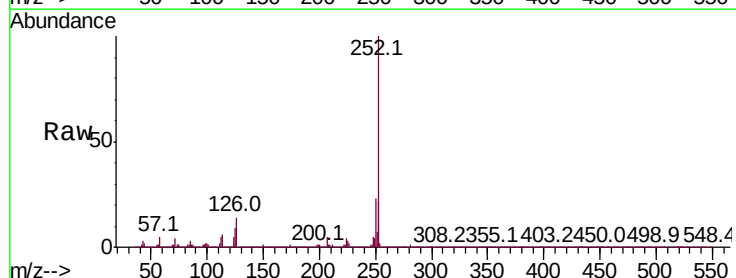


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

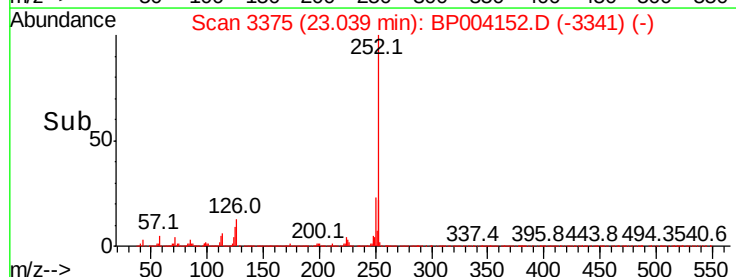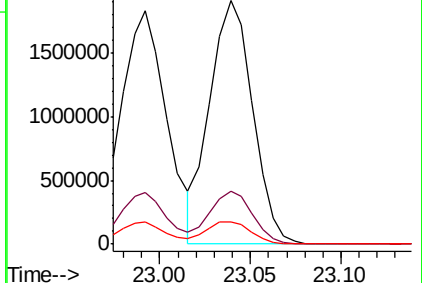



#93

Benzo(a)pyrene

Concen: 20.478 ng/ul

RT: 23.60 min Scan# 3471

Delta R.T. -0.01 min

Lab File: BP004152.D

Acq: 04 Dec 2020 21:09

Instrument :

BNA_P

ClientSampleId :

SICV001


Tot Ion:252 Resp: 2964071

Ion Ratio Lower Upper

252 100

253 21.9 17.5 26.3




125 10.2 8.3 12.5



Abundance Ion 252.00 (251.70 to 252.70): E

2000000 Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

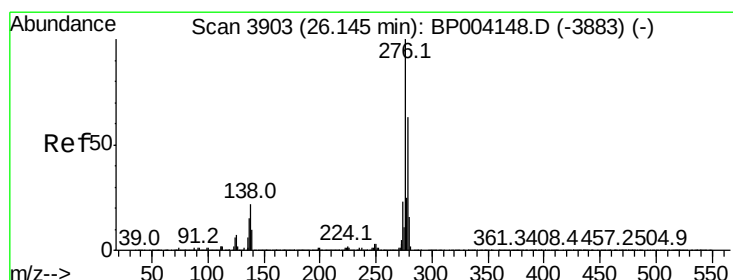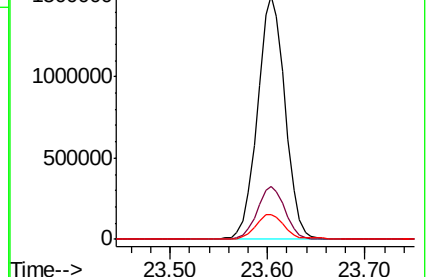

#94

Indeno(1,2,3-cd)pyrene

Concen: 20.300 ng/ul

RT: 26.14 min Scan# 3902

Delta R.T. -0.01 min

Lab File: BP004152.D

Acq: 04 Dec 2020 21:09


Tgt Ion:276 Resp: 3763246

Ion Ratio Lower Upper

276 100

138 22.4 17.4 26.0



277 25.0 20.1 30.1




Abundance Ion 276.00 (275.70 to 276.70): E

1500000 Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E



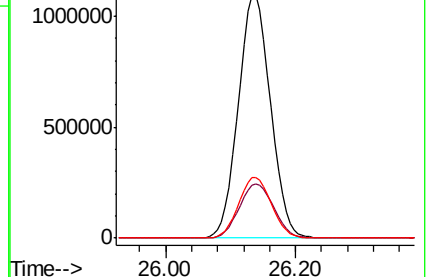





#95
Dibenzo(a,h)anthracene
Concen: 20.450 ng/ul
RT: 26.16 min Scan# 3905
Delta R.T. -0.01 min
Lab File: BP004152.D
Acq: 04 Dec 2020 21:09

Instrument :
BNA_P
ClientSampleId :
SICV001

Tot Ion:278 Resp: 3164288
Ion Ratio Lower Upper
278 100
139 15.1 12.3 18.5
279 24.0 19.1 28.7

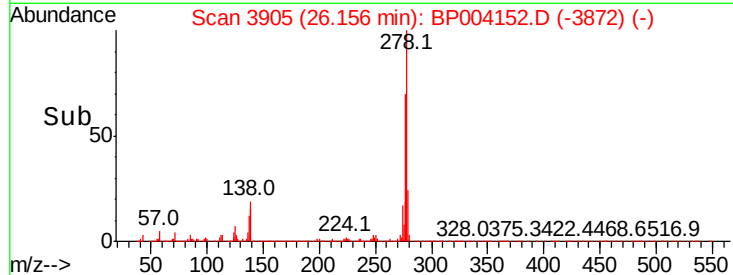

#96
Benzo(g,h,i)perylene
Concen: 20.119 ng/ul
RT: 26.87 min Scan# 4027
Delta R.T. -0.01 min
Lab File: BP004152.D
Acq: 04 Dec 2020 21:09

Tgt Ion:276 Resp: 3129738
Ion Ratio Lower Upper
276 100
138 21.0 16.2 24.4
277 23.9 19.0 28.6

