
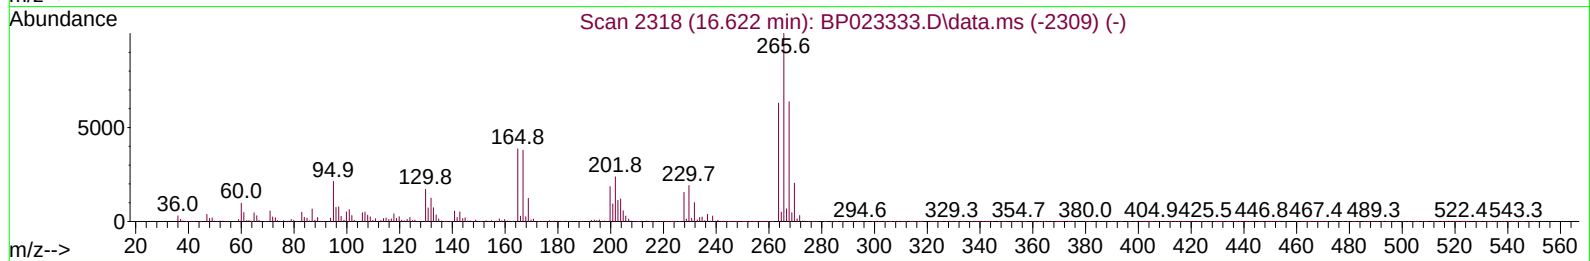
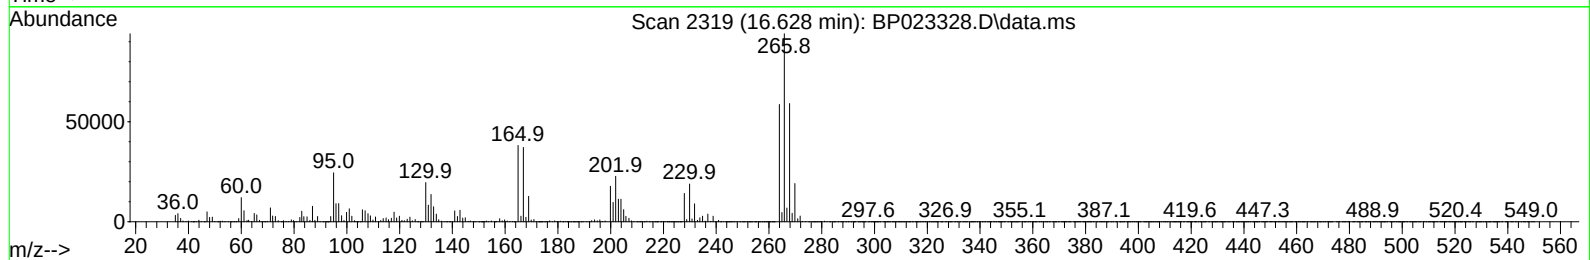


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120424\
Data File : BP023328.D
Acq On : 04 Dec 2024 11:20
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 05 02:07:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP120424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 05 01:54:03 2024
Response via : Initial Calibration

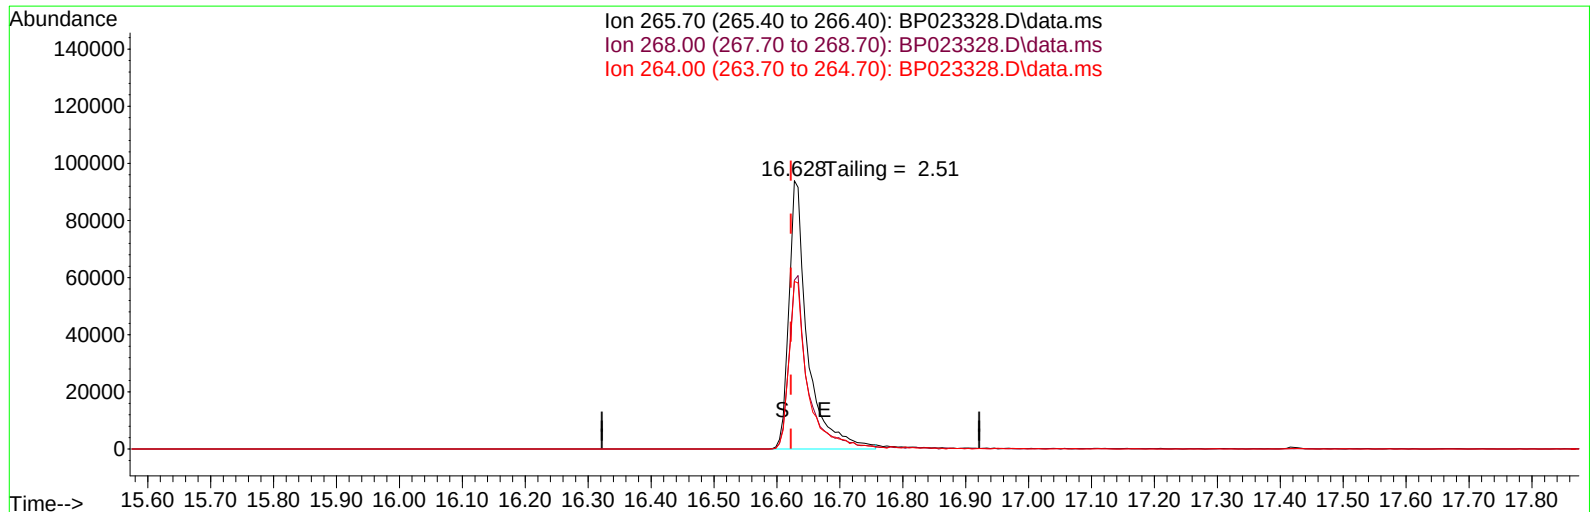

TIC: BP023328.D\data.ms

(70) Pentachlorophenol (C)




16.628min (+ 0.006) 2245019.36 ng

response 198497

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	68.30	62.94
264.00	67.90	62.41
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120424\
Data File : BP023328.D
Acq On : 04 Dec 2024 11:20
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 05 02:07:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP120424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 05 01:54:03 2024
Response via : Initial Calibration

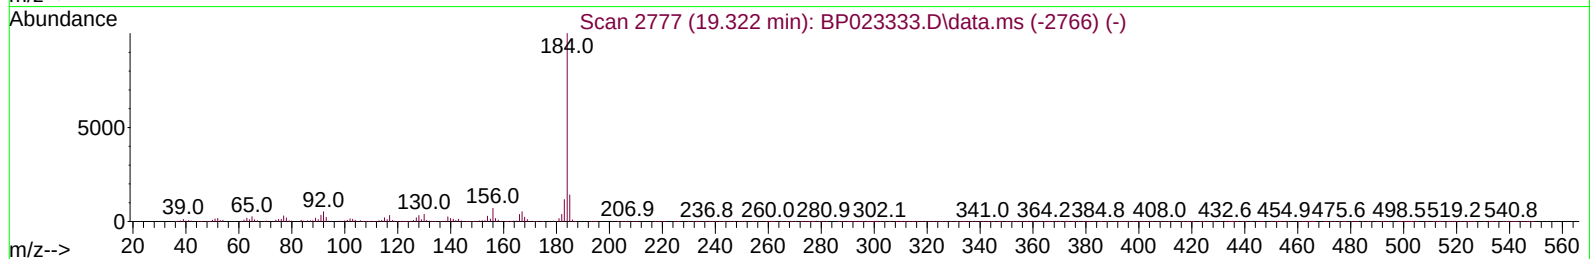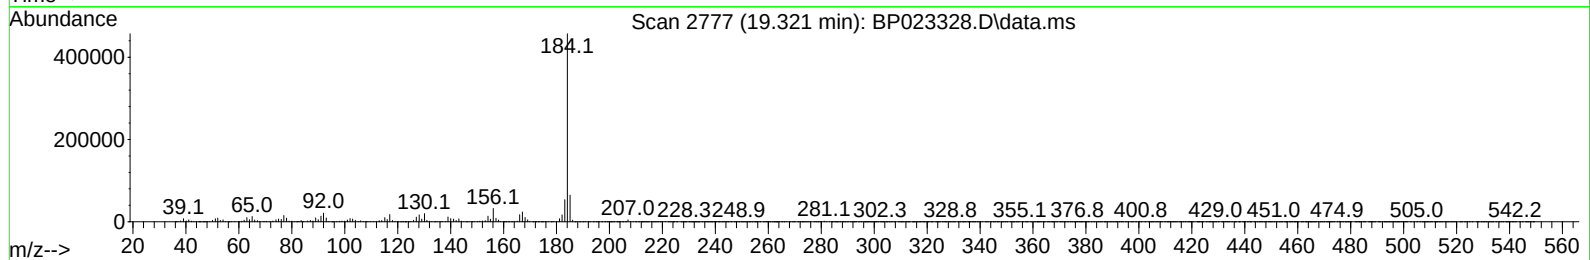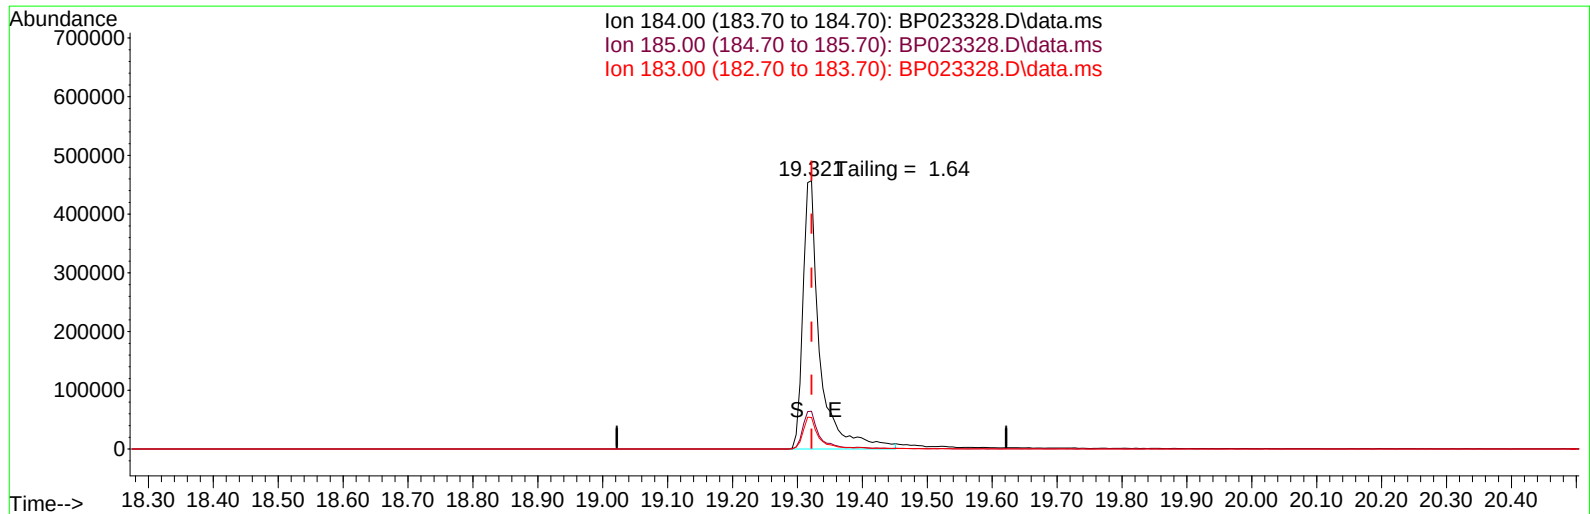

TIC: BP023328.D\data.ms

(77) Benzidine

19.321min (-0.000) 4177557.51 ng

response 848195

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.09
183.00	11.70	11.74
0.00	0.00	0.00