
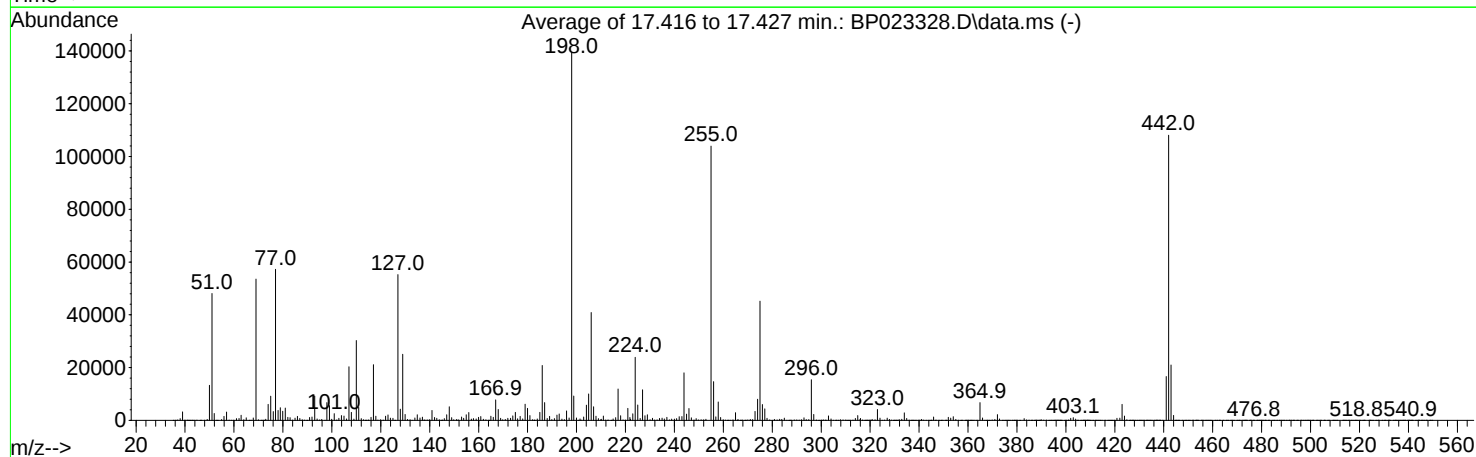


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120424\
Data File : BP023328.D
Acq On : 04 Dec 2024 11:20
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP120424.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Dec 05 01:54:03 2024

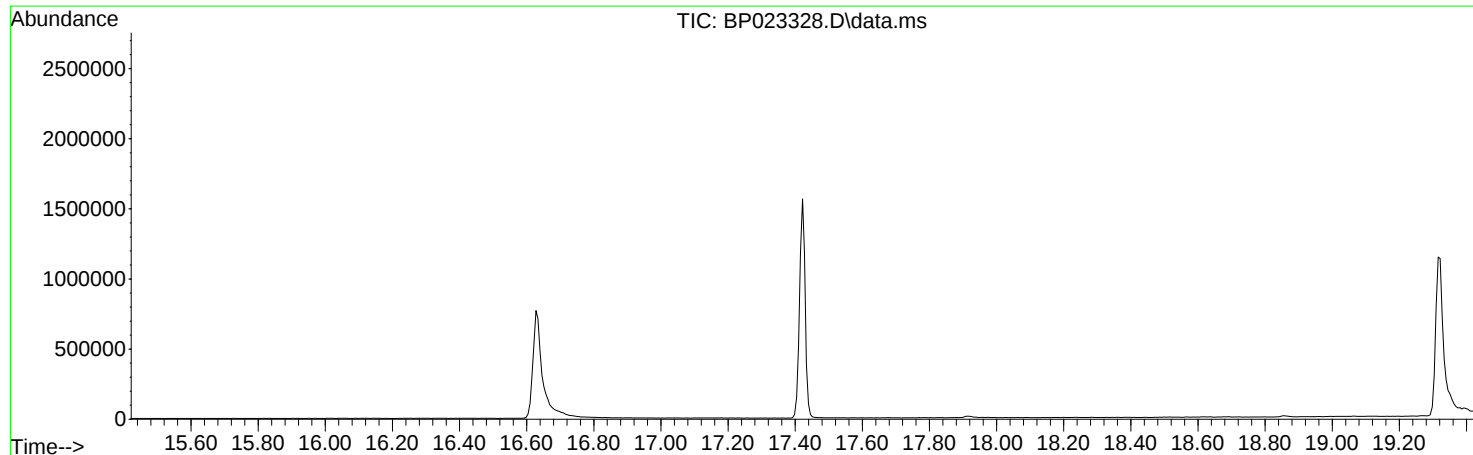




AutoFind: Scans 2453, 2454, 2455; Background Corrected with Scan 2445

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.5	48064	PASS
68	69	0.00	2	1.7	889	PASS
69	198	0.00	100	38.4	53575	PASS
70	69	0.00	2	0.5	270	PASS
127	198	10	80	39.6	55275	PASS
197	198	0.00	2	0.6	905	PASS
198	198	100	100	100.0	139422	PASS
199	198	5	9	6.6	9240	PASS
275	198	10	60	32.4	45176	PASS
365	198	1	100	4.8	6744	PASS
441	198	0.01	100	11.9	16596	PASS
442	442	100	100	100.0	108091	PASS
443	442	15	24	19.4	21003	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120424\
Data File : BP023328.D
Acq On : 04 Dec 2024 11:20
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Dec 05 02:07:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP120424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 05 01:54:03 2024
Response via : Initial Calibration

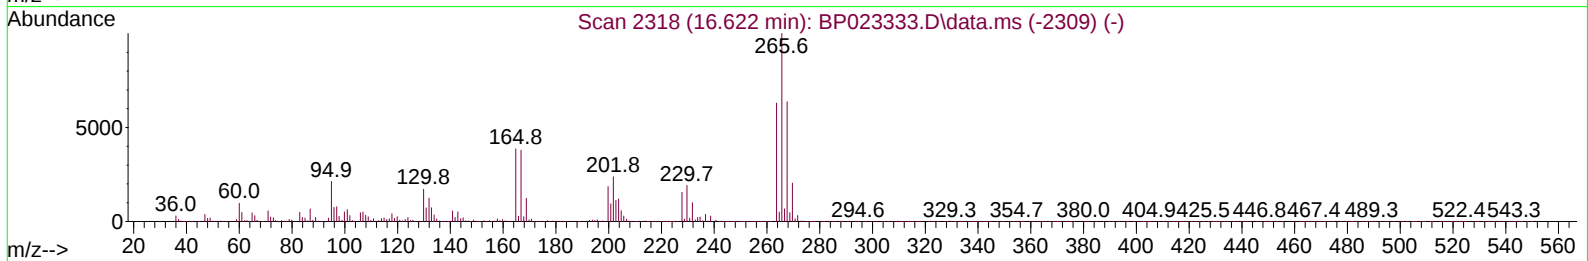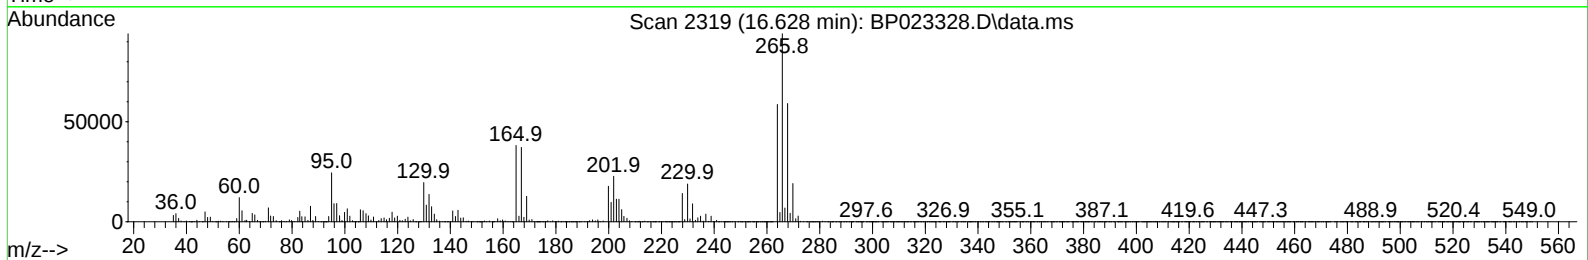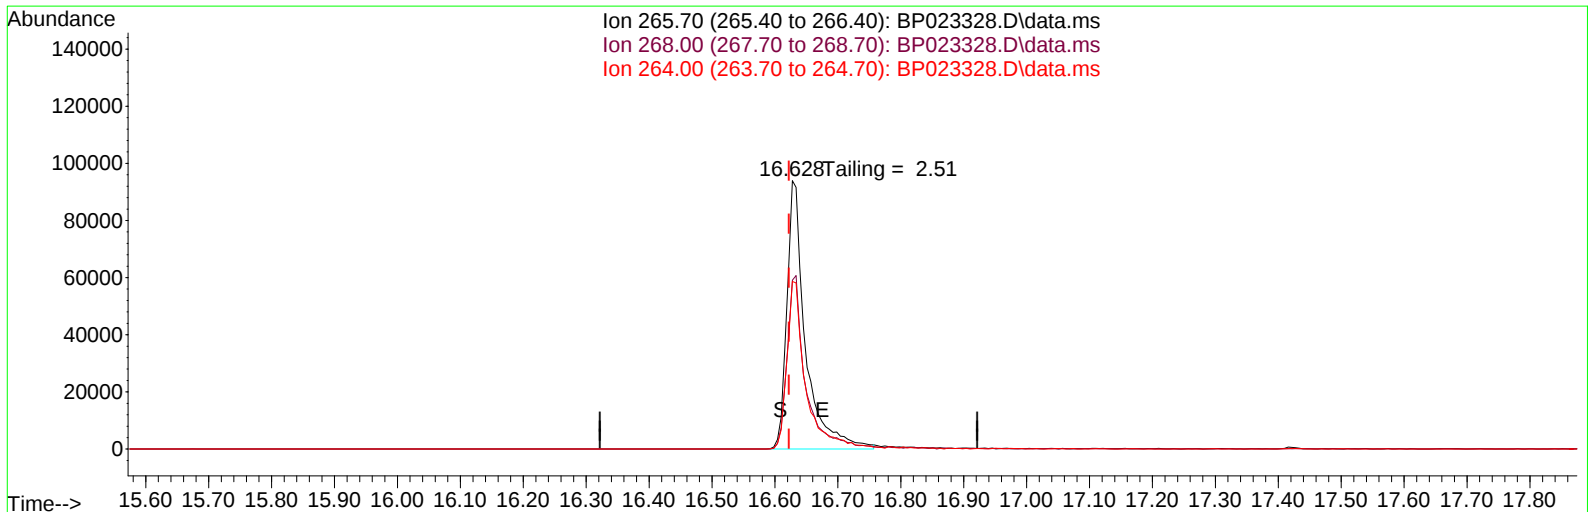

TIC: BP023328.D\data.ms

(70) Pentachlorophenol (C)

16.628min (+ 0.006) 2245019.36 ng




response 198497

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	68.30	62.94
264.00	67.90	62.41
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120424\
Data File : BP023328.D
Acq On : 04 Dec 2024 11:20
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Dec 05 02:07:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP120424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 05 01:54:03 2024
Response via : Initial Calibration

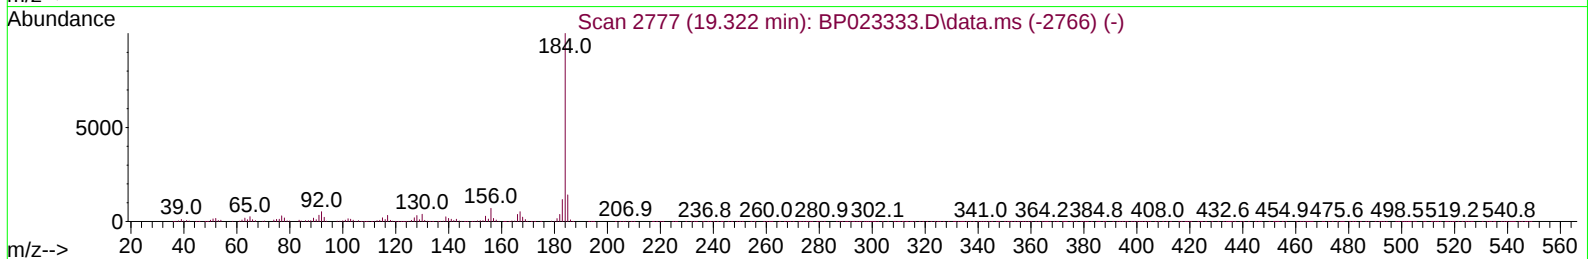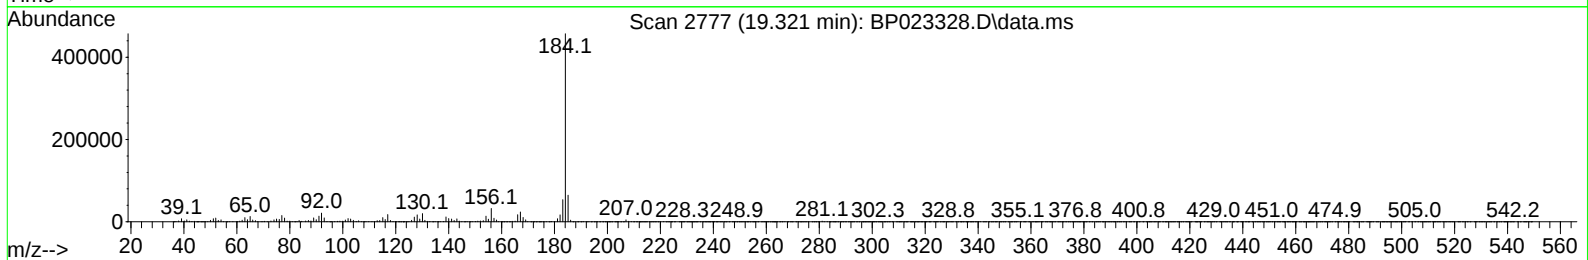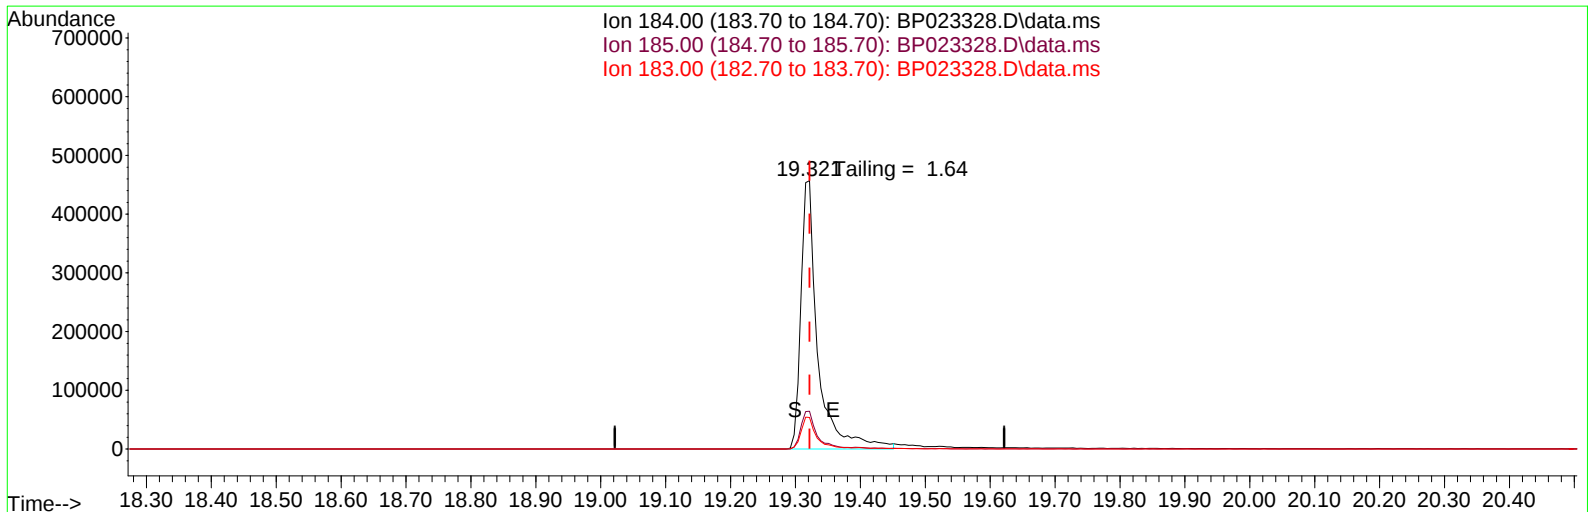

TIC: BP023328.D\data.ms

(77) Benzidine

19.321min (-0.000) 4177557.51 ng

response 848195

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.09
183.00	11.70	11.74
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/4/2024	BNA_P	<u>BP023328.D</u>
Compound Name	Response	Retention Time
DDT	539365	20.598
DDD	5519	20.192
DDE	624	19.604
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6143	545508	1.13

Instrument :
BNA_P
ClientSampleId :
DFTPP