

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP120719\
 Data File : BP001263.D
 Acq On : 07 Dec 2019 19:34
 Operator : JU
 Sample : K6147-19
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: Dec 09 00:44:16 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP112719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 05 12:34:47 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.31	152	67679	20.00	ng	0.00
21) Naphthalene-d8	10.34	136	250623	20.00	ng	-0.01
39) Acenaphthene-d10	13.20	164	147770	20.00	ng	0.00
64) Phenanthrene-d10	15.60	188	297068	20.00	ng	-0.01
76) Chrysene-d12	19.24	240	238683	20.00	ng	-0.02
87) Perylene-d12	21.02	264	230494	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	6.24	112	600629	147.24	ng	0.03
7) Phenol-d6	7.77	99	800938	147.38	ng	0.00
23) Nitrobenzene-d5	9.19	82	576744	99.84	ng	0.00
42) 2,4,6-Tribromophenol	14.50	330	238438	168.34	ng	0.00
45) 2-Fluorobiphenyl	12.12	172	968969	95.97	ng	-0.01
79) Terphenyl-d14	17.89	244	1302549	100.96	ng	0.00
Target Compounds						
9) Benzaldehyde	7.62	77	83	Below Cal	Qvalue	# 82
15) Benzyl Alcohol	8.55	79	10818	2.425 ng	#	59
19) n-Nitroso-di-n-propylamine	9.19	70	83913	21.398 ng	#	76
54) 2,4-Dinitrophenol	13.32	184	16	7.124 ng	#	62
65) 4,6-Dinitro-2-methylphenol	14.15	198	28	6.296 ng	#	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP120719\
Data File : BP001263.D
Acq On : 07 Dec 2019 19:34
Operator : JU
Sample : K6147-19
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :

Quant Time: Dec 09 00:44:16 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP112719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 05 12:34:47 2019
Response via : Initial Calibration




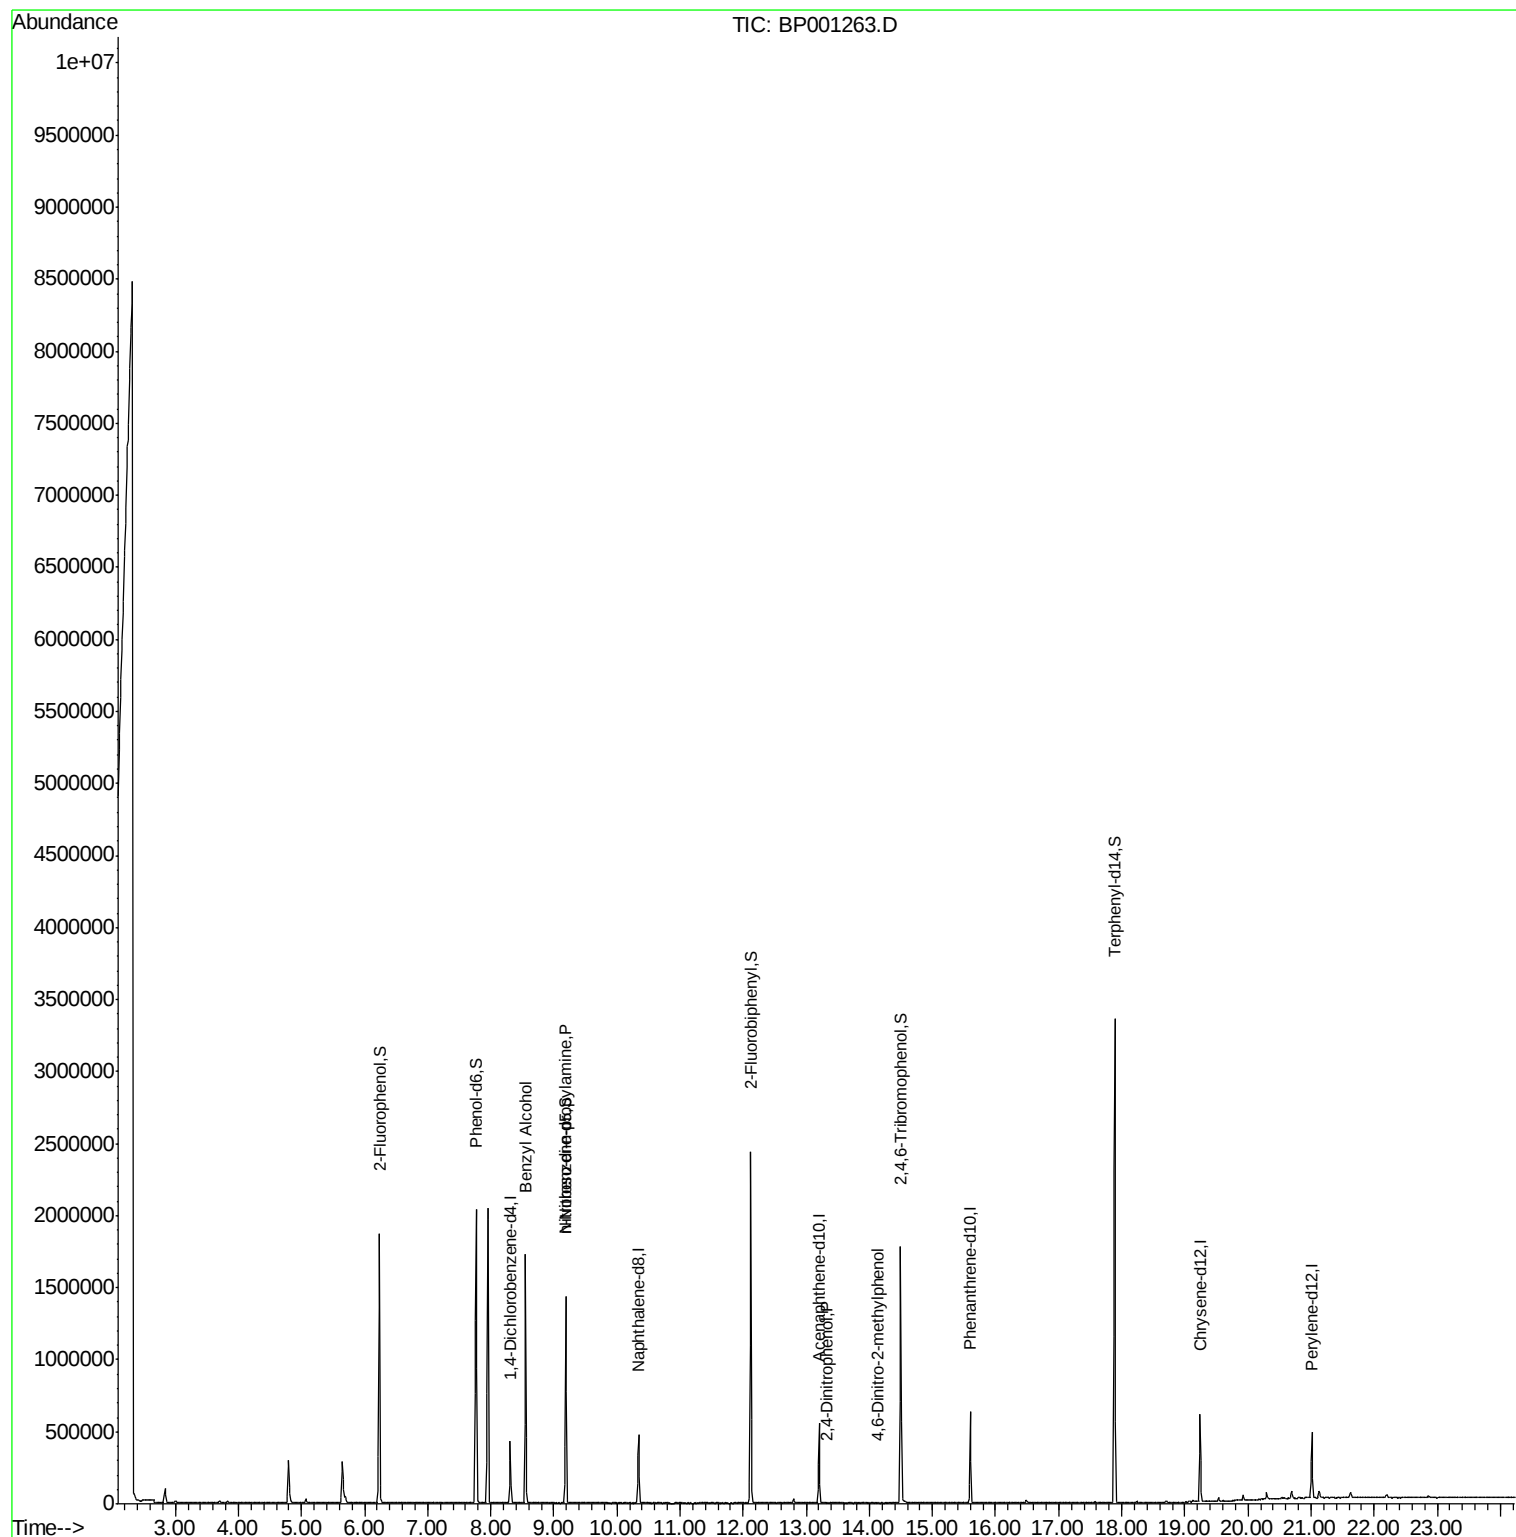




#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 8.31 min Scan# 1058
 Delta R.T. 0.00 min
 Lab File: BP001263.D
 Acq: 07 Dec 2019 19:34




Instrument :
 BNA_P
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
152	100		
150	153.3	127.3	190.9
115	69.8	56.0	84.0

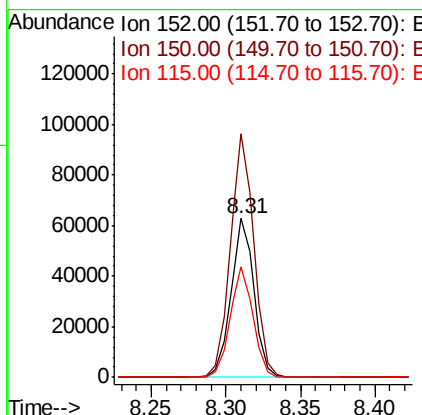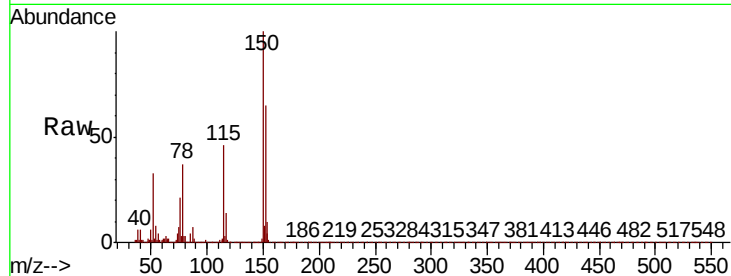

#5
 2-Fluorophenol
 Concen: 147.238 ng
 RT: 6.24 min Scan# 706
 Delta R.T. 0.03 min
 Lab File: BP001263.D
 Acq: 07 Dec 2019 19:34

Tgt Ion	Ratio	Lower	Upper
112	100		
64	67.2	56.8	85.2
63	40.1	32.2	48.2

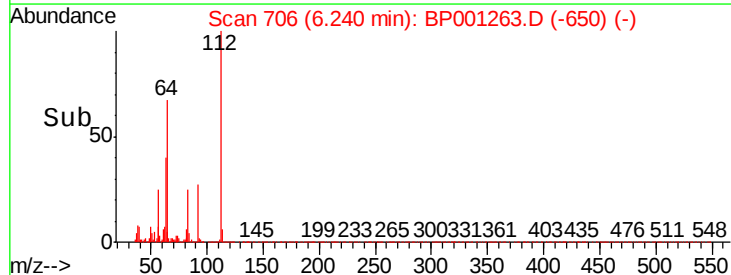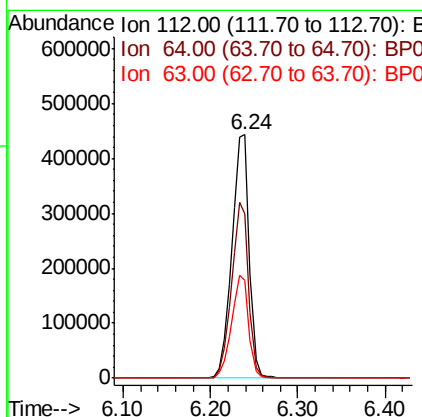



#7

Phenol-d6

Concen: 147.376 ng

RT: 7.77 min Scan# 966

Delta R.T. 0.01 min

Lab File: BP001263.D

Acq: 07 Dec 2019 19:34

Instrument :

BNA_P

ClientSampleId :





Tot Ion: 99 Resp: 800938

Ion Ratio Lower Upper

99 100

42 23.1 17.6 26.4

71 45.4 33.8 50.8

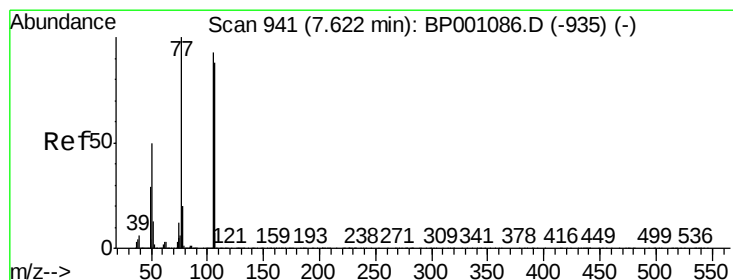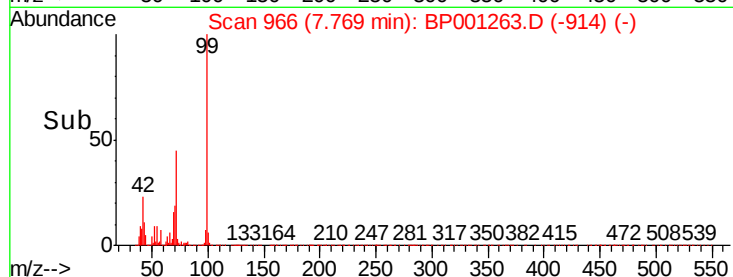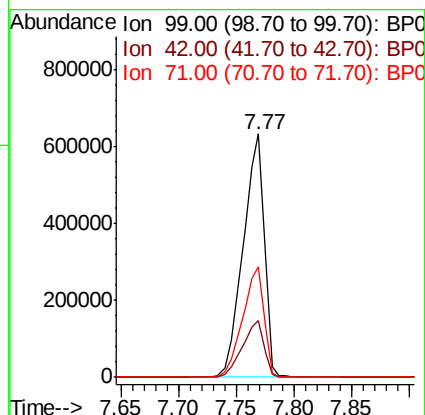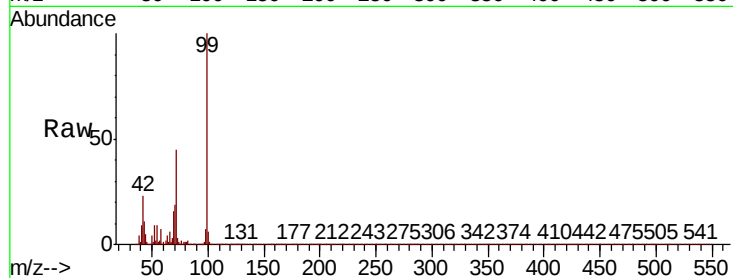

#9

Benzaldehyde

Concen: Below Cal

RT: 7.62 min Scan# 940

Delta R.T. 0.01 min

Lab File: BP001263.D

Acq: 07 Dec 2019 19:34




Tgt Ion: 77 Resp: 83


Ion Ratio Lower Upper

77 100

105 56.1 69.7 109.7#

106 87.7 67.1 107.1


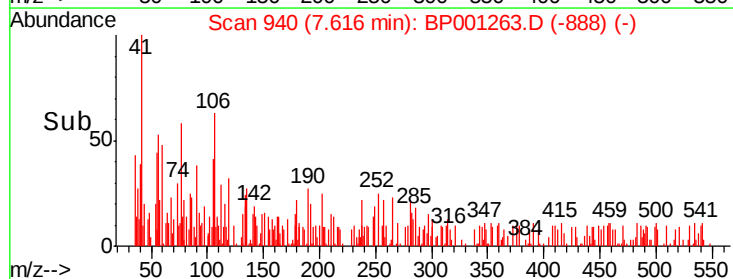
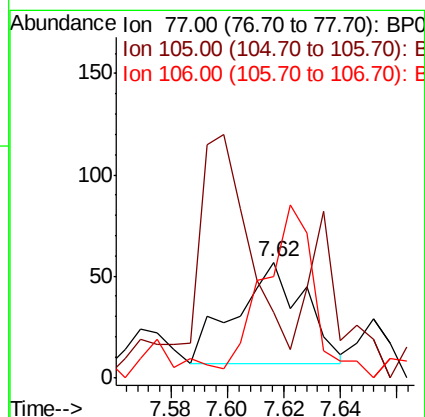
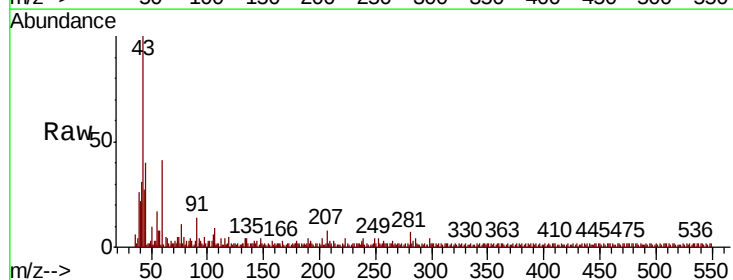


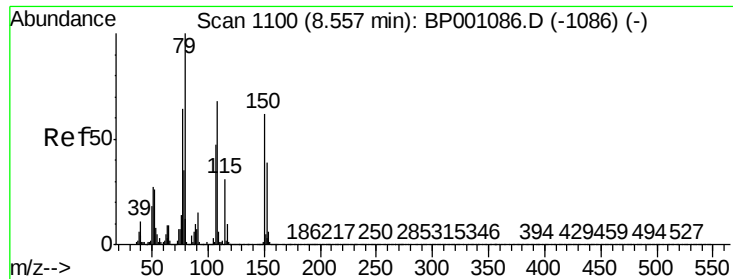

#15
Benzyl Alcohol
Concen: 2.425 ng
RT: 8.55 min Scan# 1099
Delta R.T. 0.01 min
Lab File: BP001263.D
Acq: 07 Dec 2019 19:34




Instrument :
BNA_P
ClientSampleId :


Tot Ion	Ratio	Lower	Upper
79	100		
108	31.5	51.6	77.4#
77	98.7	53.5	80.3#

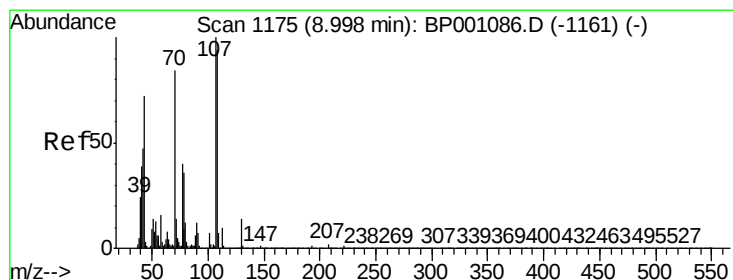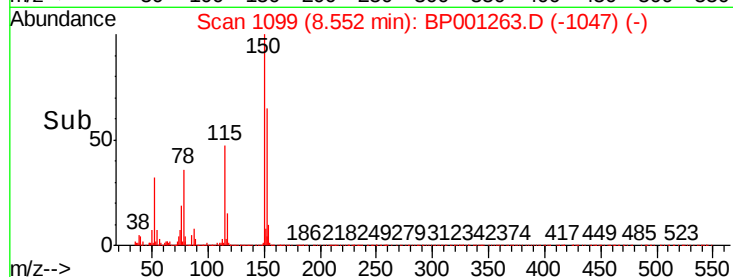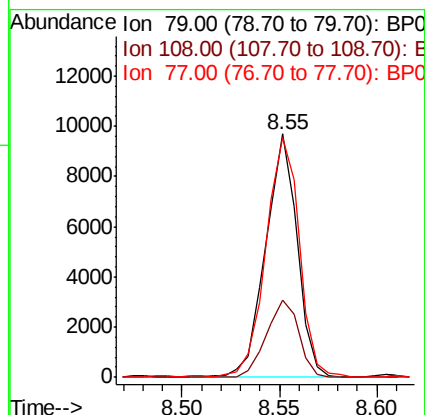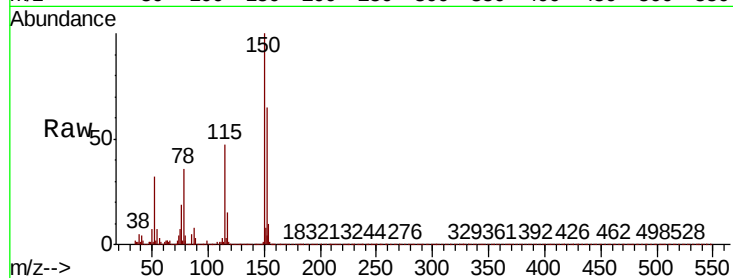

#19
n-Nitroso-di-n-propylamine
Concen: 21.398 ng
RT: 9.19 min Scan# 1208
Delta R.T. 0.21 min
Lab File: BP001263.D
Acq: 07 Dec 2019 19:34

Tgt Ion	Ratio	Lower	Upper
70	100		
42	47.1	50.6	76.0#
101	0.0	7.1	10.7#
130	1.5	13.6	20.4#


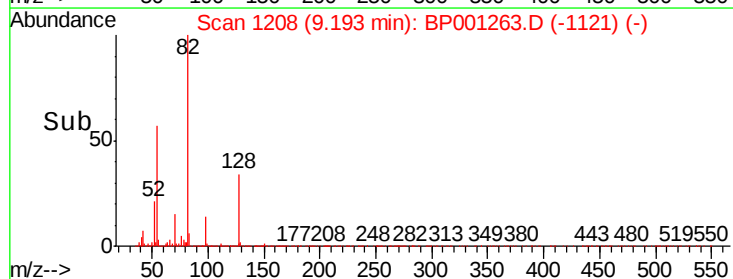
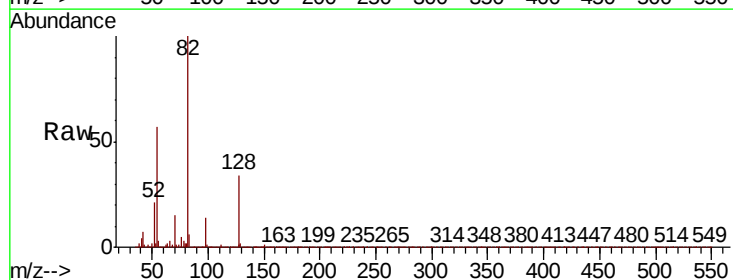
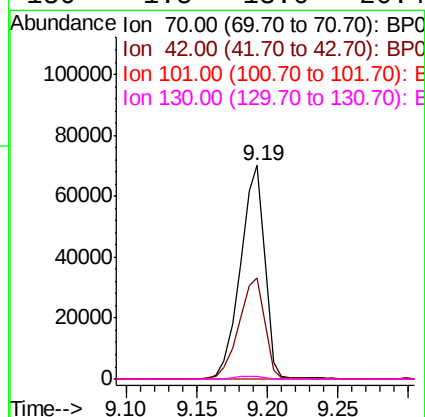


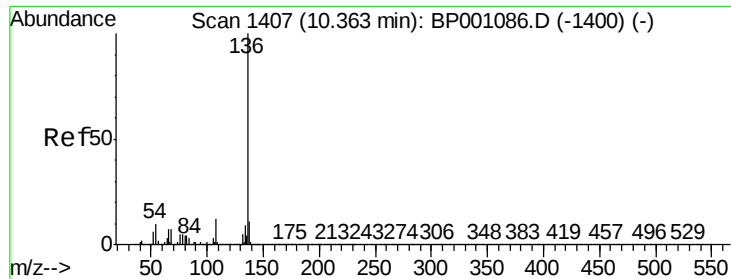

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.34 min Scan# 1403
Delta R.T. -0.01 min
Lab File: BP001263.D
Acq: 07 Dec 2019 19:34




Instrument :
BNA_P
ClientSampleId :


Tot Ion:136	Resp:	250623	
Ion Ratio	Lower	Upper	
136 100			
137 11.2	8.4	12.6	
54 10.3	7.4	11.0	
68 5.8	4.6	7.0	

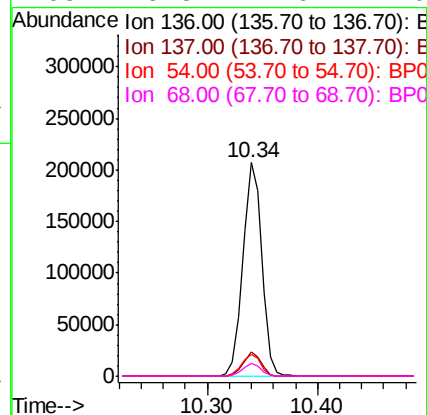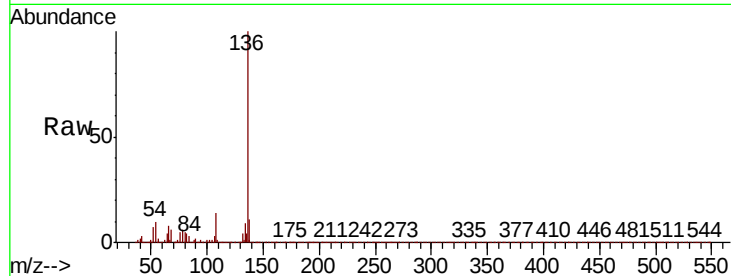

#23
Nitrobenzene-d5
Concen: 99.841 ng
RT: 9.19 min Scan# 1208
Delta R.T. -0.01 min
Lab File: BP001263.D
Acq: 07 Dec 2019 19:34

Tgt Ion: 82	Resp: 576744
Ion Ratio	Lower Upper
82 100	
128 34.1	27.5 41.3
54 57.3	45.7 68.5


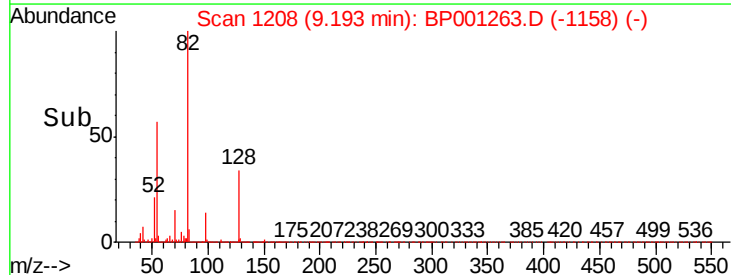
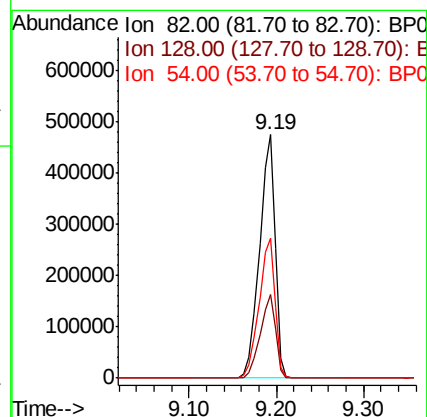



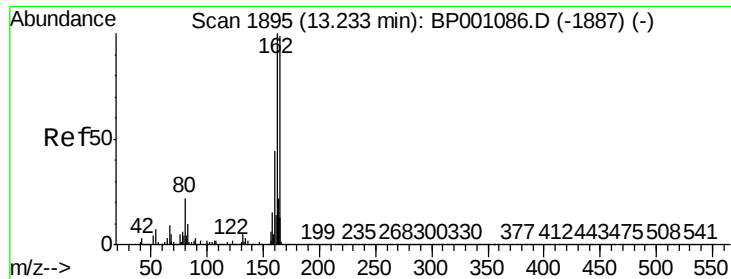

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 13.20 min Scan# 1890
Delta R.T. -0.01 min
Lab File: BP001263.D
Acq: 07 Dec 2019 19:34




Instrument :
BNA_P
ClientSampleId :


Tot Ion:164 Resp: 147770
Ion Ratio Lower Upper
164 100
162 100.9 80.7 121.1
160 46.9 36.3 54.5

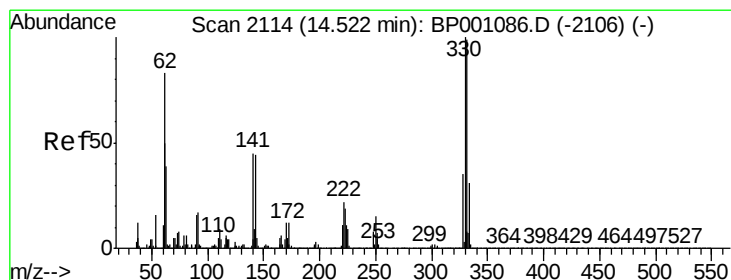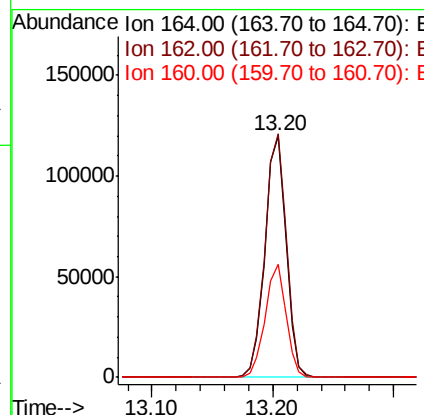

#42
2,4,6-Tribromophenol
Concen: 168.344 ng
RT: 14.50 min Scan# 2110
Delta R.T. -0.01 min
Lab File: BP001263.D
Acq: 07 Dec 2019 19:34

Tgt Ion:330 Resp: 238438
Ion Ratio Lower Upper
330 100
332 98.3 79.1 118.7
141 45.5 35.9 53.9


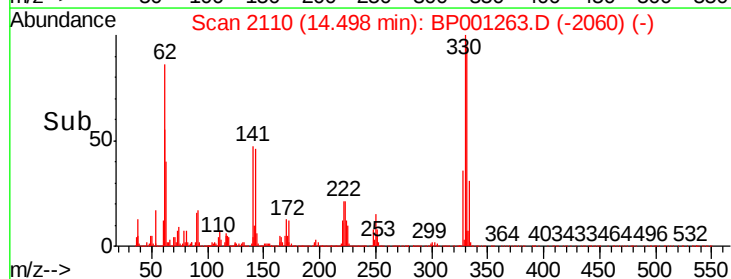
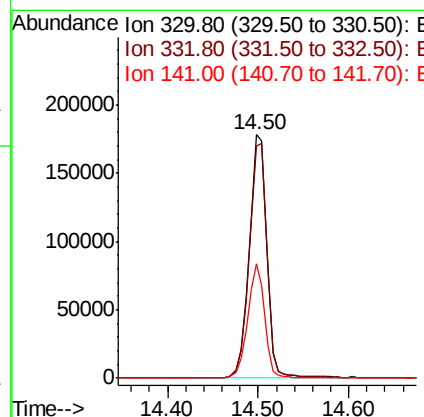
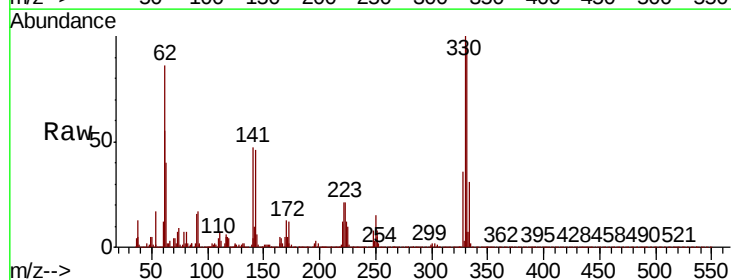


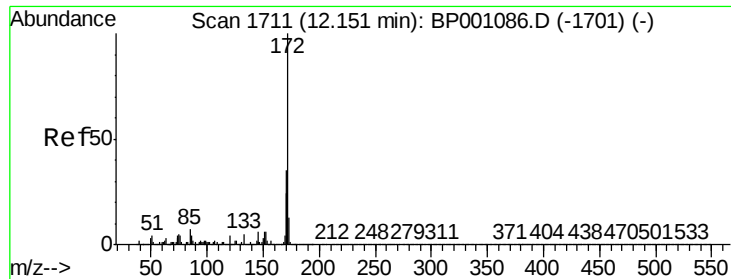

#45
2-Fluorobiphenyl
Concen: 95.971 ng
RT: 12.12 min Scan# 1706
Delta R.T. -0.01 min
Lab File: BP001263.D
Acq: 07 Dec 2019 19:34




Instrument :
BNA_P
ClientSampleId :


Tot Ion	Ratio	Lower	Upper
172	100		
171	35.4	28.7	43.1
170	23.4	19.2	28.8

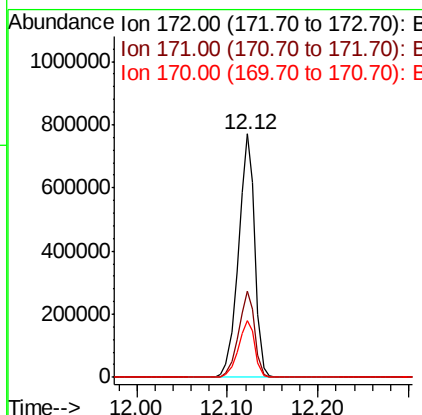

#54
2,4-Dinitrophenol
Concen: 7.124 ng
RT: 13.32 min Scan# 1909
Delta R.T. -0.01 min
Lab File: BP001263.D
Acq: 07 Dec 2019 19:34

Tgt Ion	Ratio	Lower	Upper
184	100		
63	80.8	69.4	104.0
154	7.7	57.4	86.2#

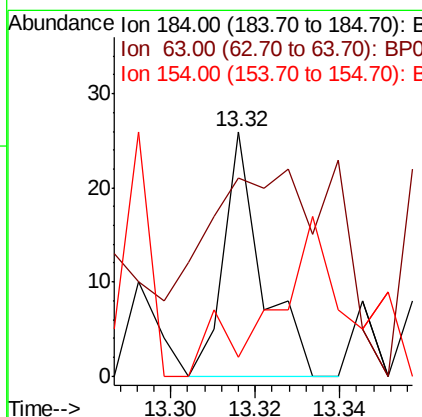



#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 15.60 min Scan# 2297

Delta R.T. -0.01 min

Lab File: BP001263.D

Acq: 07 Dec 2019 19:34

Instrument :

BNA_P

ClientSampleId :


Tot Ion:188 Resp: 297068

Ion Ratio Lower Upper

188 100

94 9.2 7.1 10.7




80 10.0 7.8 11.6



Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BP0

Ion 80.00 (79.70 to 80.70): BP0

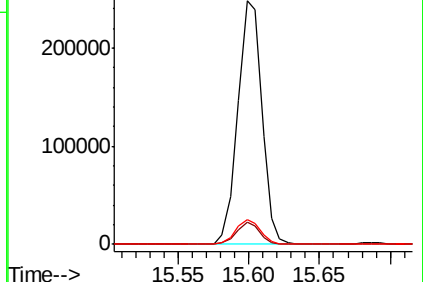

#65

4,6-Dinitro-2-methylphenol

Concen: 6.296 ng

RT: 14.15 min Scan# 2050

Delta R.T. -0.06 min

Lab File: BP001263.D

Acq: 07 Dec 2019 19:34


Tgt Ion:198 Resp: 28

Ion Ratio Lower Upper

198 100

51 38.2 36.2 76.2



105 50.0 30.2 70.2




Abundance Ion 198.00 (197.70 to 198.70): E

Ion 51.00 (50.70 to 51.70): BP0

Ion 105.00 (104.70 to 105.70): E

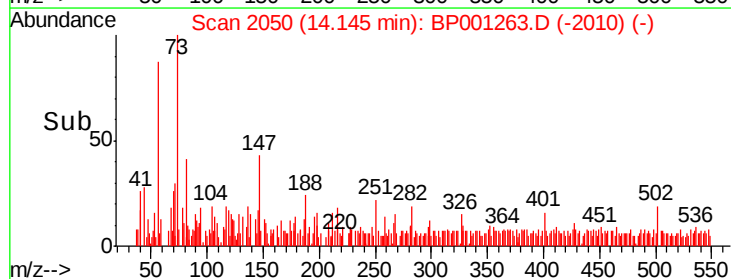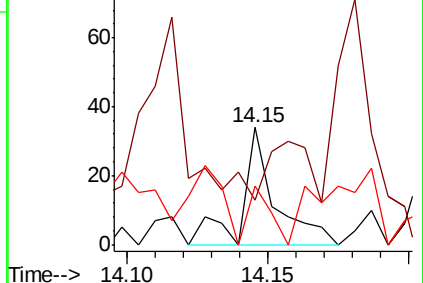



#76

Chrysene-d12

Concen: 20.000 ng

RT: 19.24 min Scan# 2916

Delta R.T. -0.02 min

Lab File: BP001263.D

Acq: 07 Dec 2019 19:34

Instrument :

BNA_P

ClientSampleId :


Tot Ion:240 Resp: 238683

Ion Ratio Lower Upper

240 100

120 10.4 7.0 10.6




236 25.9 21.7 32.5



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

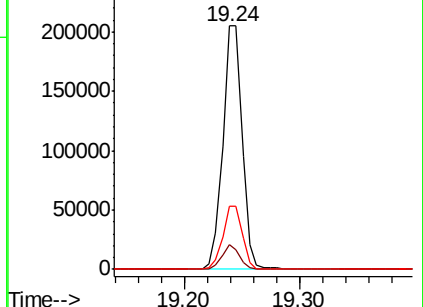

#79

Terphenyl-d14

Concen: 100.964 ng

RT: 17.89 min Scan# 2686

Delta R.T. -0.01 min

Lab File: BP001263.D

Acq: 07 Dec 2019 19:34


Tgt Ion:244 Resp: 1302549

Ion Ratio Lower Upper

244 100

212 8.4 6.6 9.8



122 11.5 9.2 13.8




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

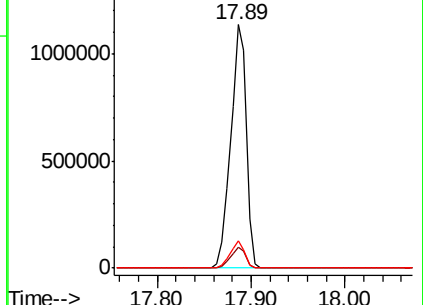




#87
Pervlene-d12
Concen: 20.000 ng
RT: 21.02 min Scan# 3218
Delta R.T. -0.01 min
Lab File: BP001263.D
Acq: 07 Dec 2019 19:34

Instrument :
BNA_P
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.9	19.4	29.0
265	21.3	17.1	25.7



Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

