

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP120719\
 Data File : BP001258.D
 Acq On : 07 Dec 2019 17:05
 Operator : JU
 Sample : K6147-14
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P001-WC003

Quant Time: Dec 09 02:19:36 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP112719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 05 12:34:47 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.31	152	82330	20.00	ng	0.00
21) Naphthalene-d8	10.34	136	299968	20.00	ng	-0.01
39) Acenaphthene-d10	13.20	164	170973	20.00	ng	0.00
64) Phenanthrene-d10	15.60	188	334439	20.00	ng	0.00
76) Chrysene-d12	19.24	240	261490	20.00	ng	-0.02
87) Perylene-d12	21.02	264	263967	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	6.23	112	616570	124.25	ng	0.02
7) Phenol-d6	7.77	99	759496	114.88	ng	0.00
23) Nitrobenzene-d5	9.19	82	659781	95.43	ng	0.00
42) 2,4,6-Tribromophenol	14.50	330	254862	155.52	ng	0.00
45) 2-Fluorobiphenyl	12.12	172	1078279	92.30	ng	-0.01
79) Terphenyl-d14	17.89	244	1389042	98.28	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP120719\
Data File : BP001258.D
Acq On : 07 Dec 2019 17:05
Operator : JU
Sample : K6147-14
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P001-WC003

Quant Time: Dec 09 02:19:36 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP112719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 05 12:34:47 2019
Response via : Initial Calibration

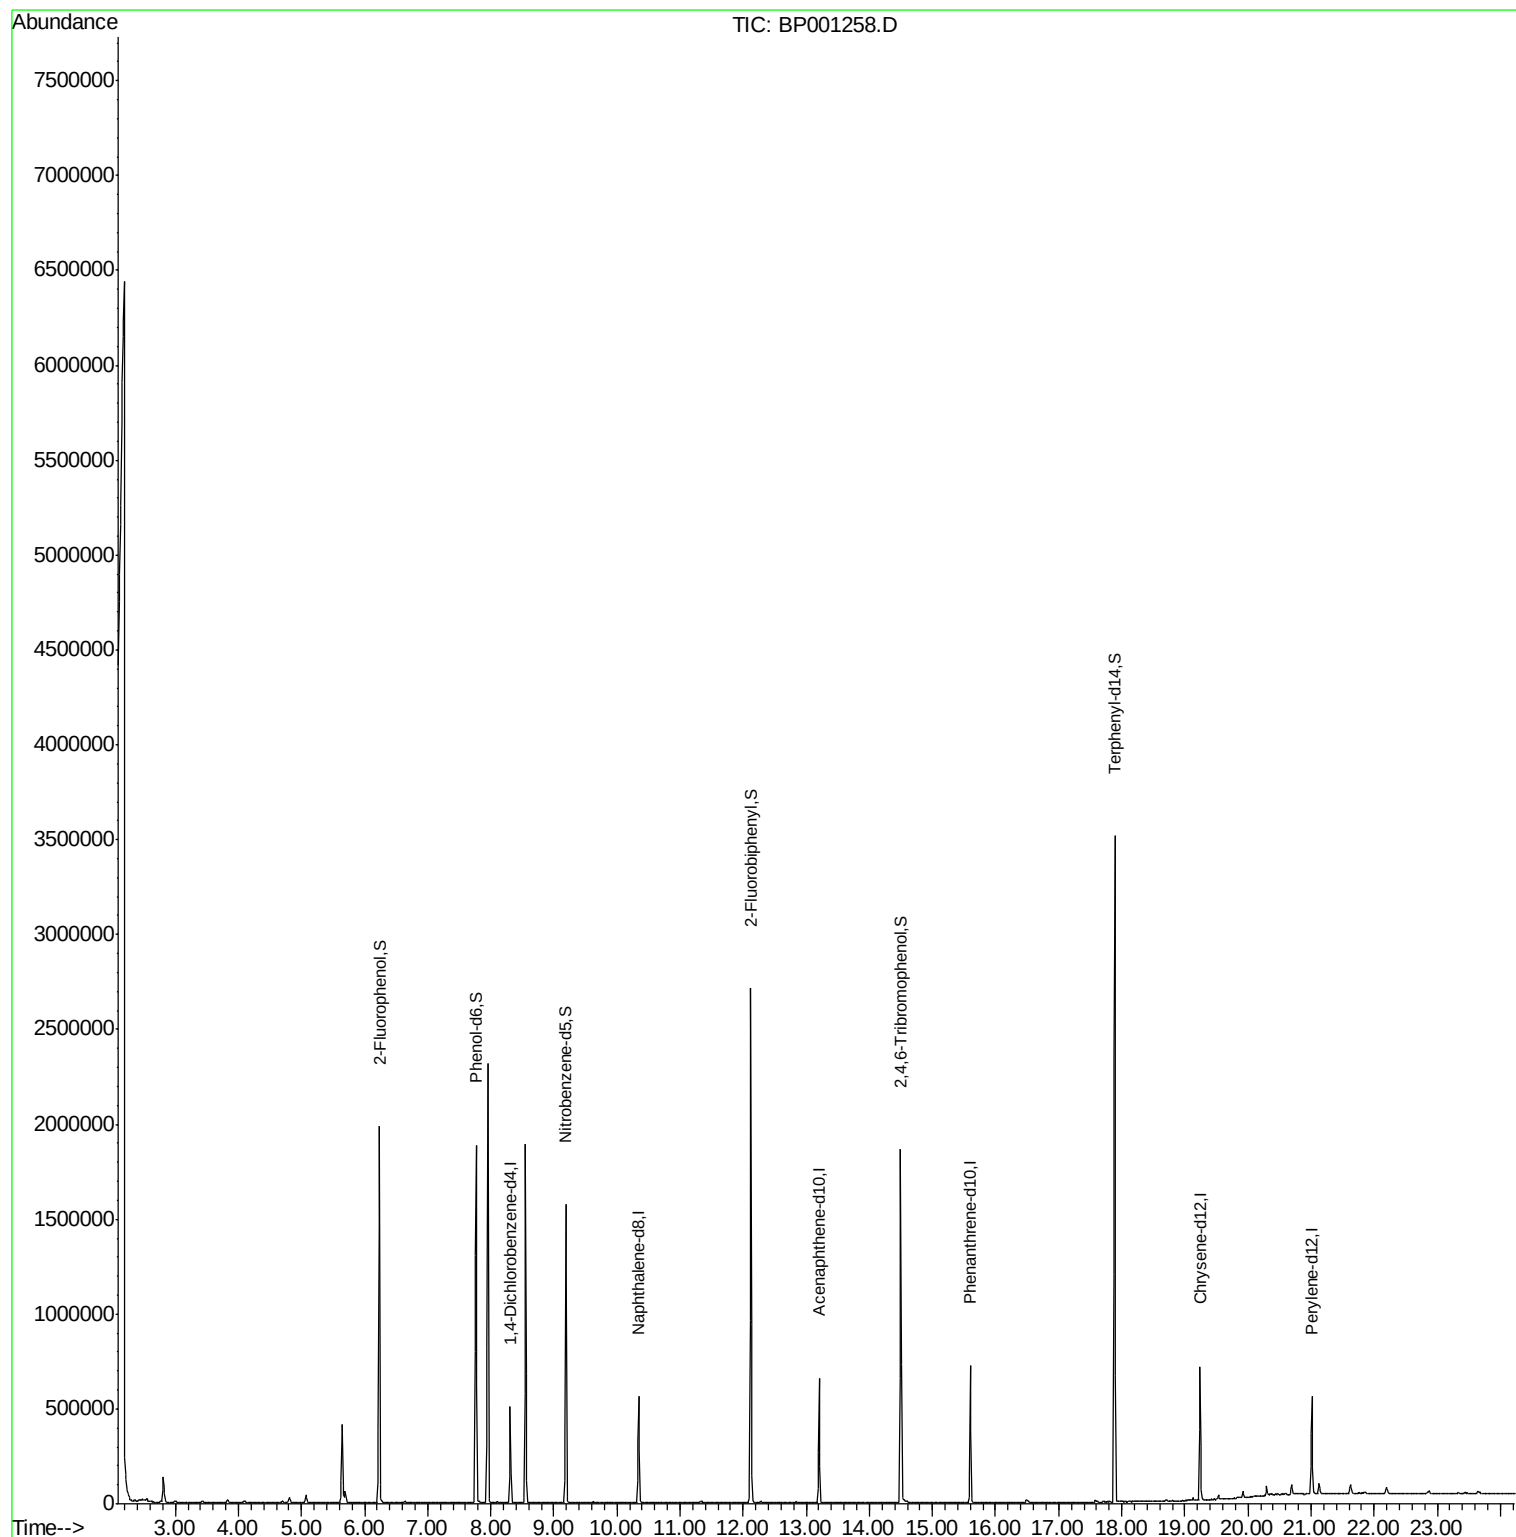

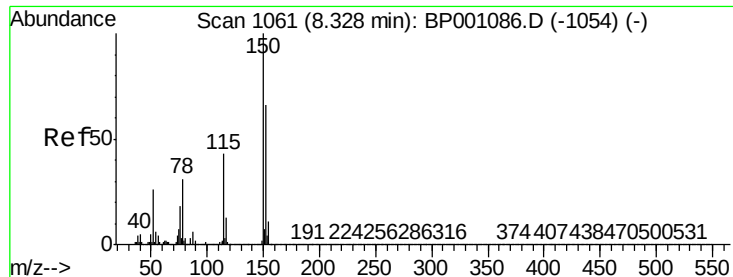

#1

1,4-Dichlorobenzene-d4

Concen: 20.000 ng

RT: 8.31 min Scan# 1058

Delta R.T. -0.00 min

Lab File: BP001258.D

Acq: 07 Dec 2019 17:05

Instrument :

BNA_P

ClientSampleId :

P001-WC003


Tot Ion:152 Resp: 82330

Ion Ratio Lower Upper

152 100

150 158.1 127.3 190.9

115 69.5 56.0 84.0



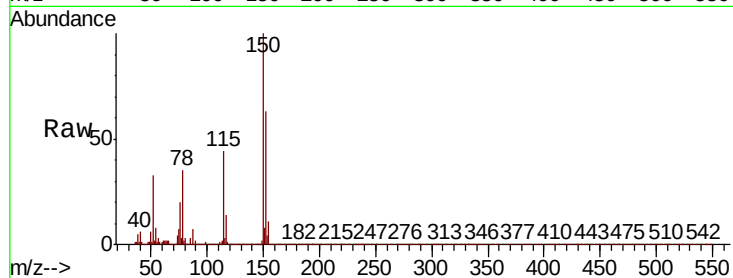


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

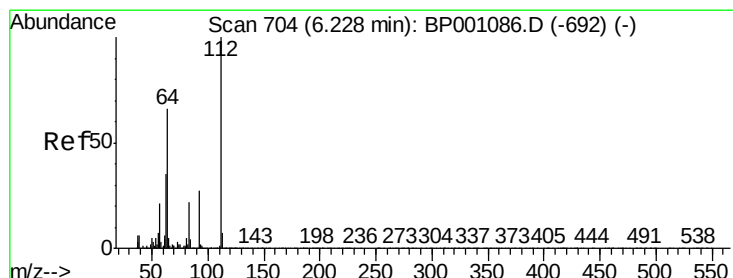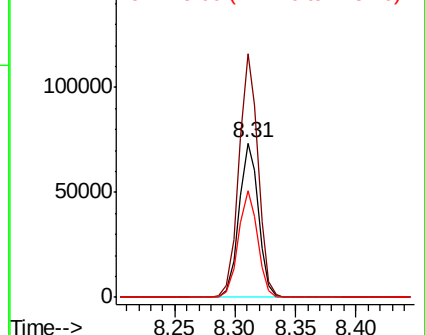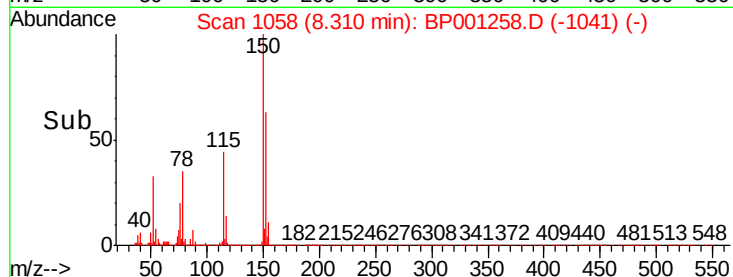

#5

2-Fluorophenol

Concen: 124.249 ng

RT: 6.23 min Scan# 705

Delta R.T. 0.02 min

Lab File: BP001258.D

Acq: 07 Dec 2019 17:05


Tgt Ion:112 Resp: 616570

Ion Ratio Lower Upper

112 100

64 71.6 56.8 85.2

63 40.9 32.2 48.2


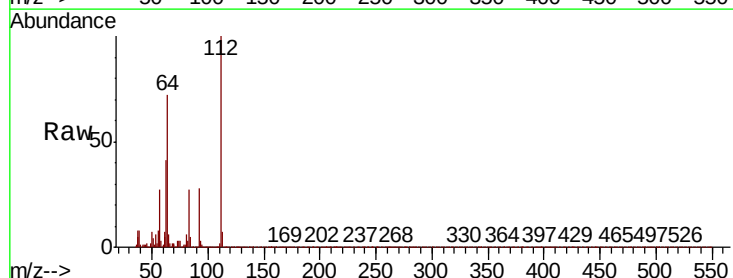



Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BP0

Ion 63.00 (62.70 to 63.70): BP0

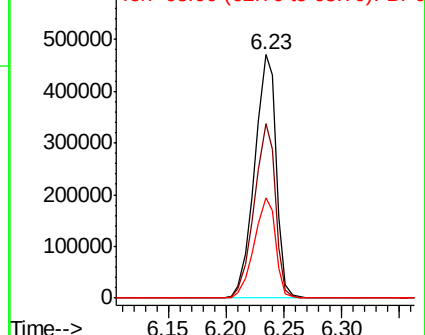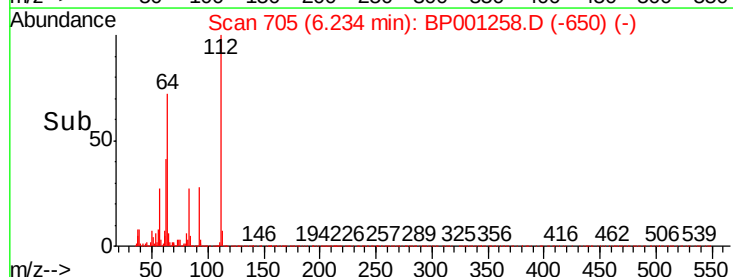

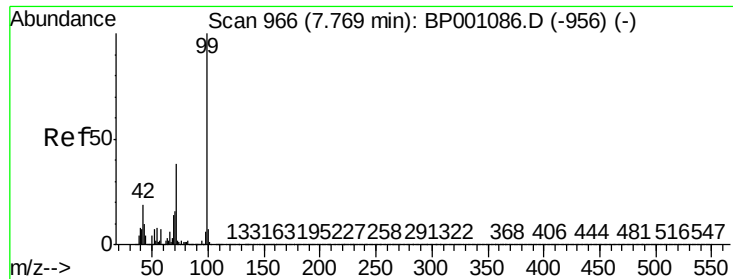

#7

Phenol-d6

Concen: 114.882 ng

RT: 7.77 min Scan# 966

Delta R.T. 0.01 min

Lab File: BP001258.D

Acq: 07 Dec 2019 17:05

Instrument :

BNA_P

ClientSampleId :

P001-WC003





Tot Ion: 99 Resp: 759496

Ion Ratio Lower Upper

99 100

42 22.7 17.6 26.4

71 44.5 33.8 50.8

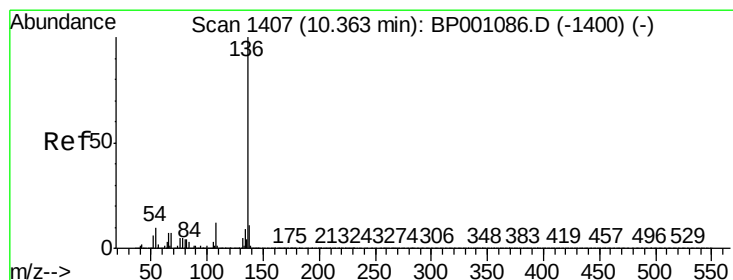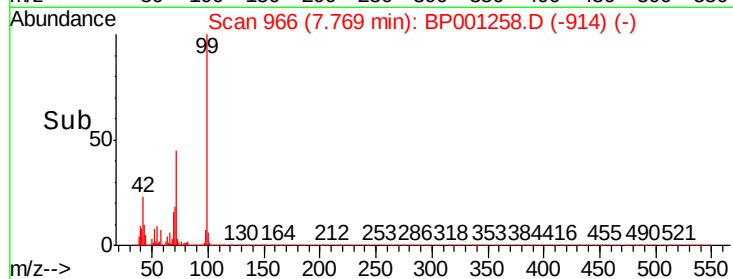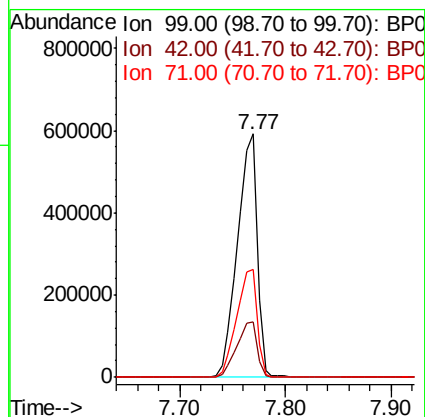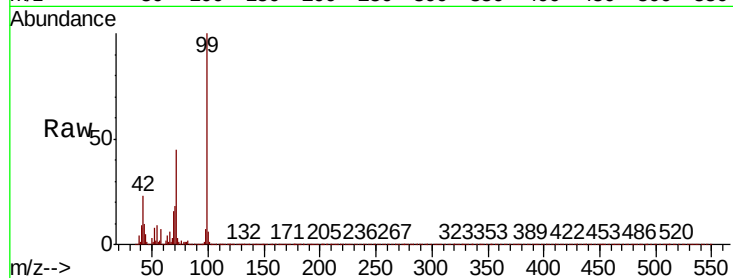

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.34 min Scan# 1403

Delta R.T. -0.01 min

Lab File: BP001258.D

Acq: 07 Dec 2019 17:05

Tgt Ion: 136 Resp: 299968




Ion Ratio Lower Upper


136 100

137 11.2 8.4 12.6

54 10.6 7.4 11.0

68 5.5 4.6 7.0

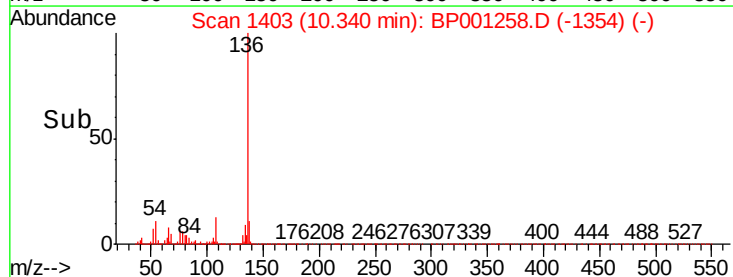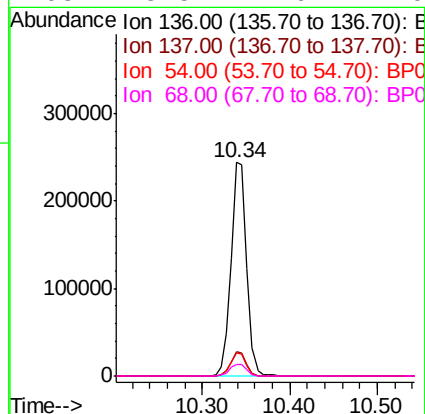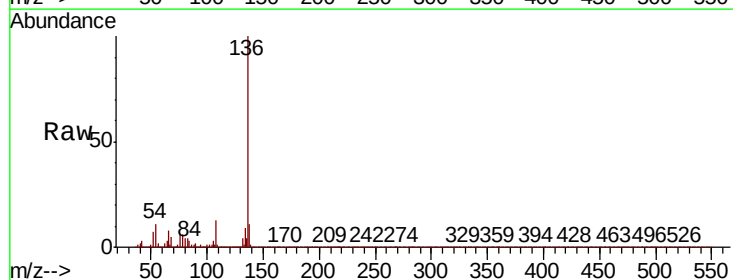

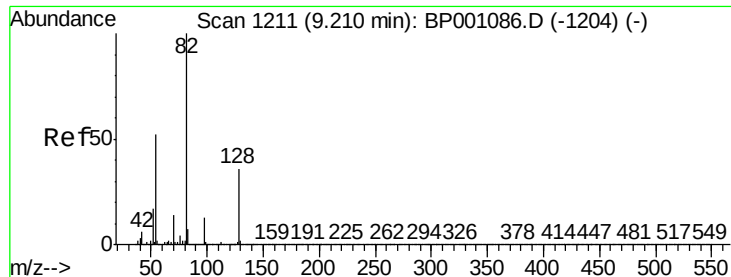

#23

Nitrobenzene-d5

Concen: 95.427 ng

RT: 9.19 min Scan# 1208

Delta R.T. -0.01 min

Lab File: BP001258.D

Acq: 07 Dec 2019 17:05

Instrument :

BNA_P

ClientSampleId :

P001-WC003





Tot Ion: 82 Resp: 659781

Ion Ratio Lower Upper

82 100

128 34.0 27.5 41.3

54 58.8 45.7 68.5

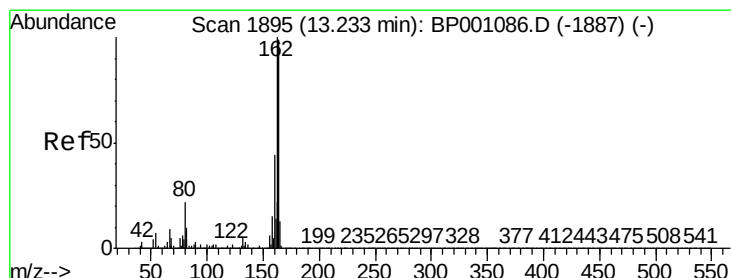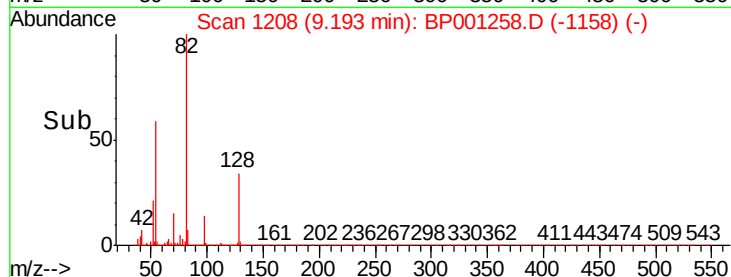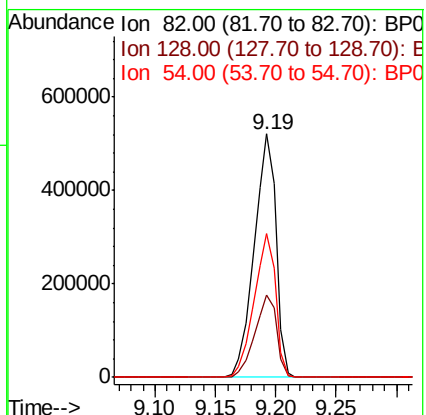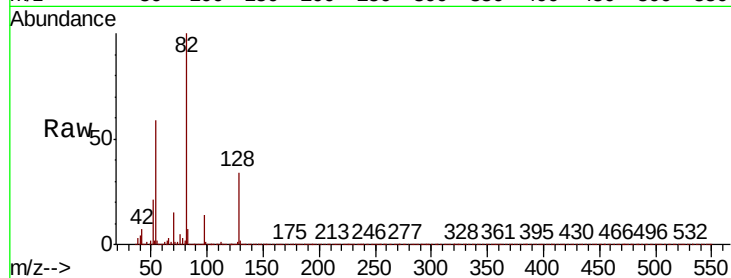

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 13.20 min Scan# 1890

Delta R.T. -0.01 min

Lab File: BP001258.D

Acq: 07 Dec 2019 17:05




Tgt Ion: 164 Resp: 170973


Ion Ratio Lower Upper

164 100

162 101.6 80.7 121.1

160 45.6 36.3 54.5

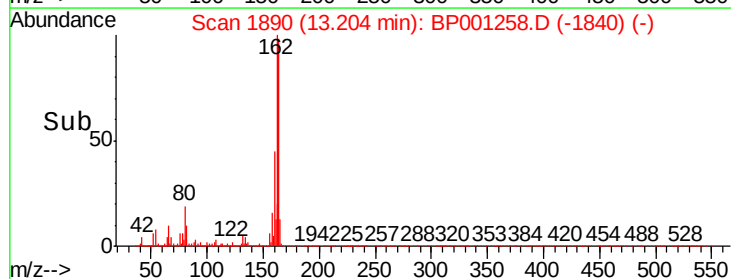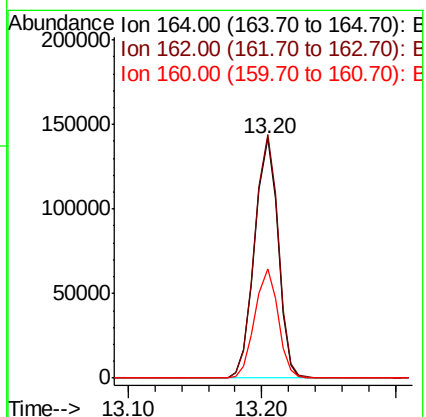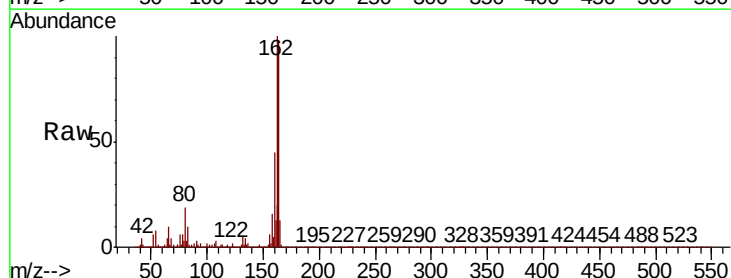

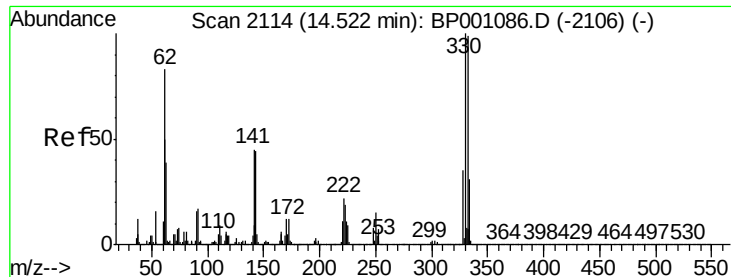

#42

2,4,6-Tribromophenol

Concen: 155.520 ng

RT: 14.50 min Scan# 2111

Delta R.T. -0.00 min

Lab File: BP001258.D

Acq: 07 Dec 2019 17:05

Instrument :

BNA_P

ClientSampleId :

P001-WC003


Tot Ion:330 Resp: 254862

Ion Ratio Lower Upper

330 100

332 95.0 79.1 118.7

141 44.6 35.9 53.9



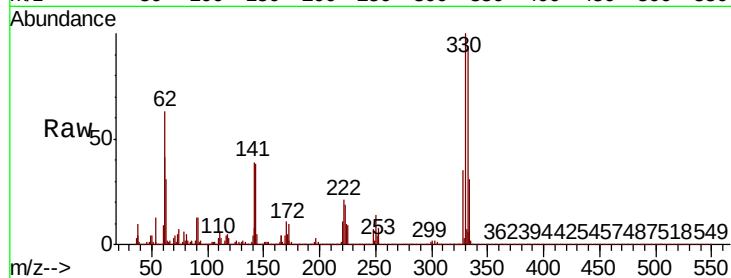


Abundance

Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

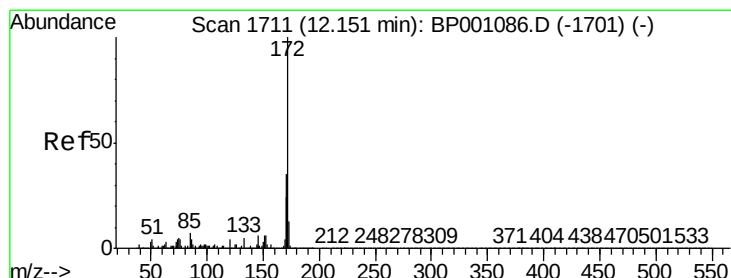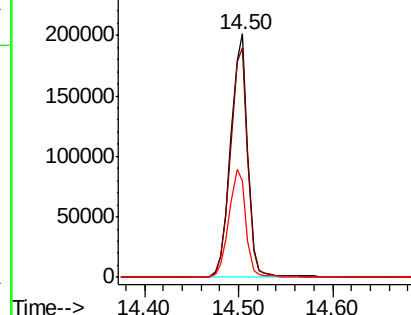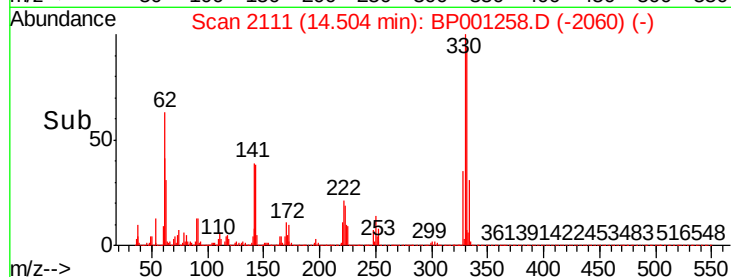

#45

2-Fluorobiphenyl

Concen: 92.304 ng

RT: 12.12 min Scan# 1706

Delta R.T. -0.01 min

Lab File: BP001258.D

Acq: 07 Dec 2019 17:05


Tgt Ion:172 Resp: 1078279

Ion Ratio Lower Upper

172 100

171 34.7 28.7 43.1

170 23.3 19.2 28.8


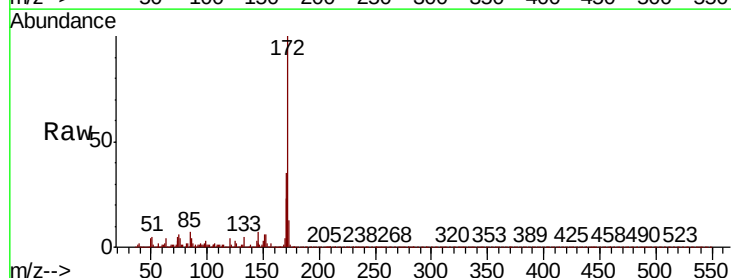



Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

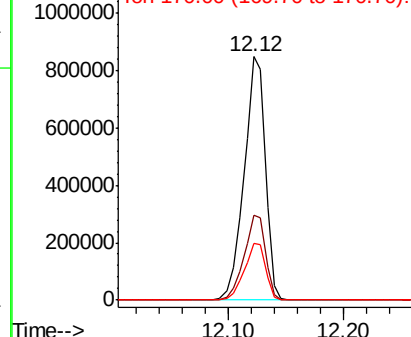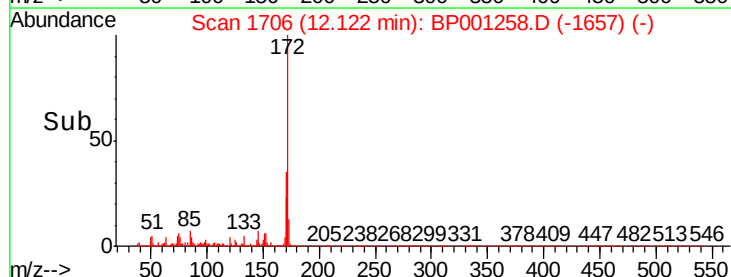

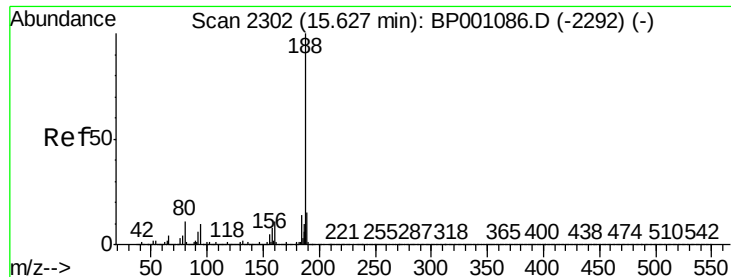

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 15.60 min Scan# 2298

Delta R.T. -0.01 min

Lab File: BP001258.D

Acq: 07 Dec 2019 17:05

Instrument :

BNA_P

ClientSampleId :

P001-WC003


Tot Ion:188 Resp: 334439

Ion Ratio Lower Upper

188 100

94 7.9 7.1 10.7




80 9.4 7.8 11.6

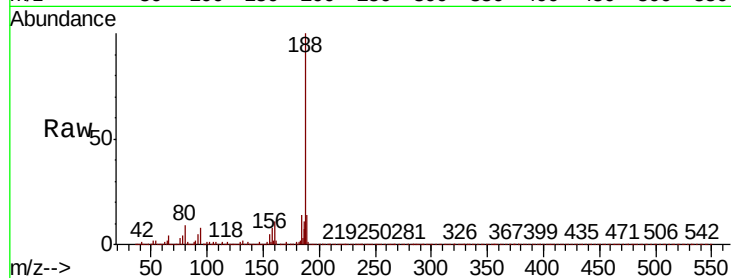

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BP0

Ion 80.00 (79.70 to 80.70): BP0

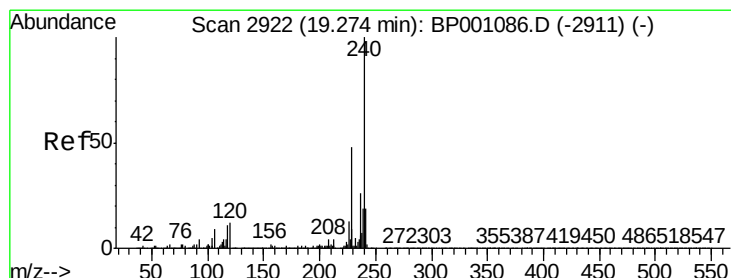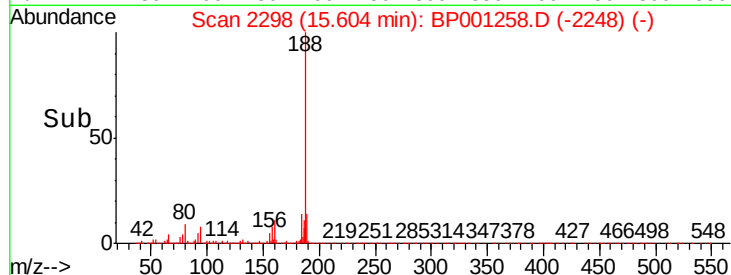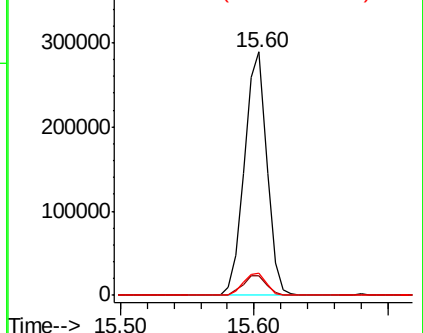

#76

Chrysene-d12

Concen: 20.000 ng

RT: 19.24 min Scan# 2916

Delta R.T. -0.02 min

Lab File: BP001258.D

Acq: 07 Dec 2019 17:05


Tgt Ion:240 Resp: 261490

Ion Ratio Lower Upper

240 100

120 10.3 7.0 10.6



236 26.1 21.7 32.5

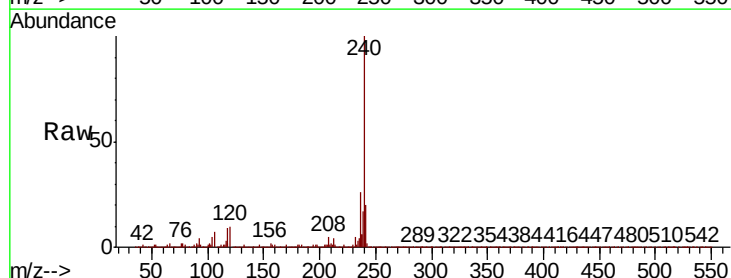


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

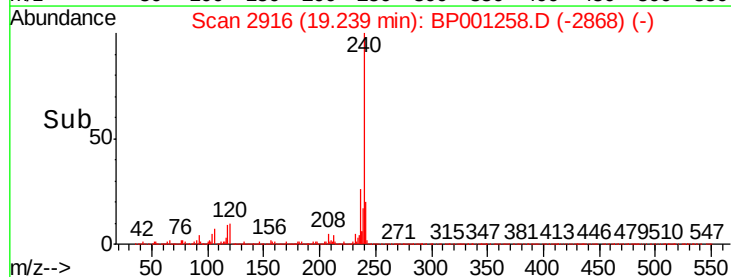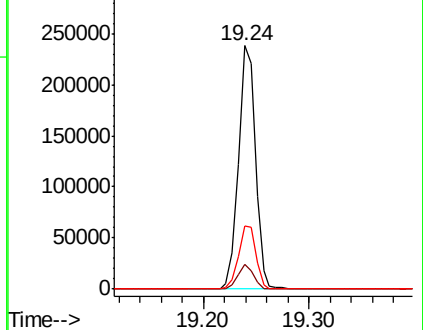

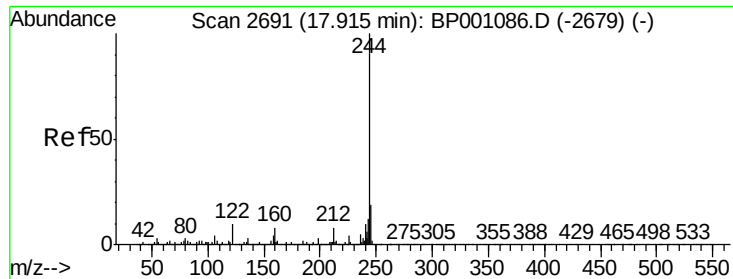

#79

Terphenyl-d14

Concen: 98.277 ng

RT: 17.89 min Scan# 2686

Delta R.T. -0.01 min

Lab File: BP001258.D

Acq: 07 Dec 2019 17:05

Instrument :

BNA_P

ClientSampleId :

P001-WC003


Tot Ion:244 Resp: 1389042

Ion Ratio Lower Upper

244 100

212 8.2 6.6 9.8




122 11.5 9.2 13.8

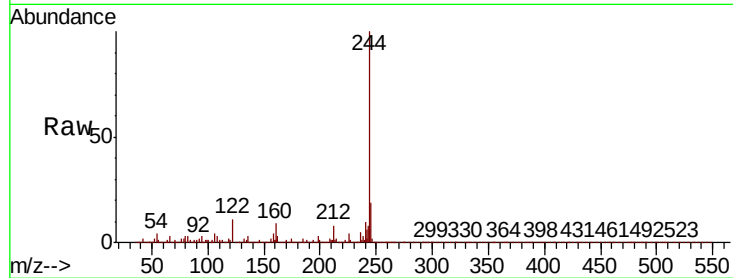

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

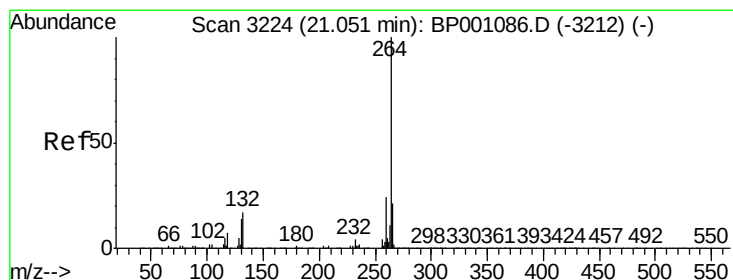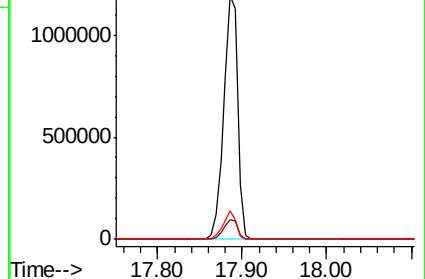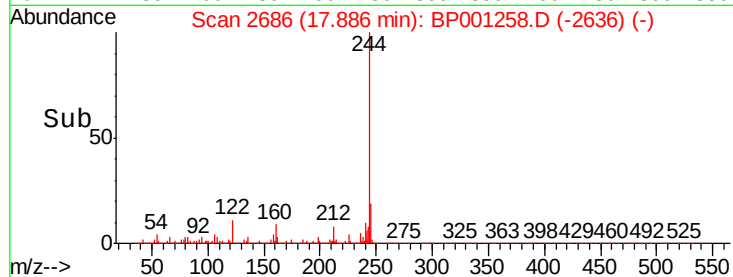

#87

Perylene-d12

Concen: 20.000 ng

RT: 21.02 min Scan# 3218

Delta R.T. -0.01 min

Lab File: BP001258.D

Acq: 07 Dec 2019 17:05


Tgt Ion:264 Resp: 263967

Ion Ratio Lower Upper

264 100

260 24.4 19.4 29.0

265 21.4 17.1 25.7

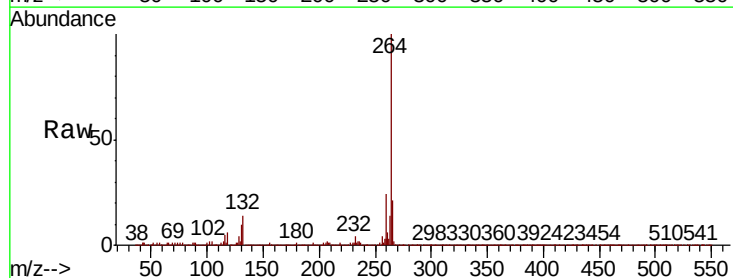

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

