


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP120719\
 Data File : BP001246.D
 Acq On : 07 Dec 2019 11:10
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP112719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Dec 05 12:34:47 2019

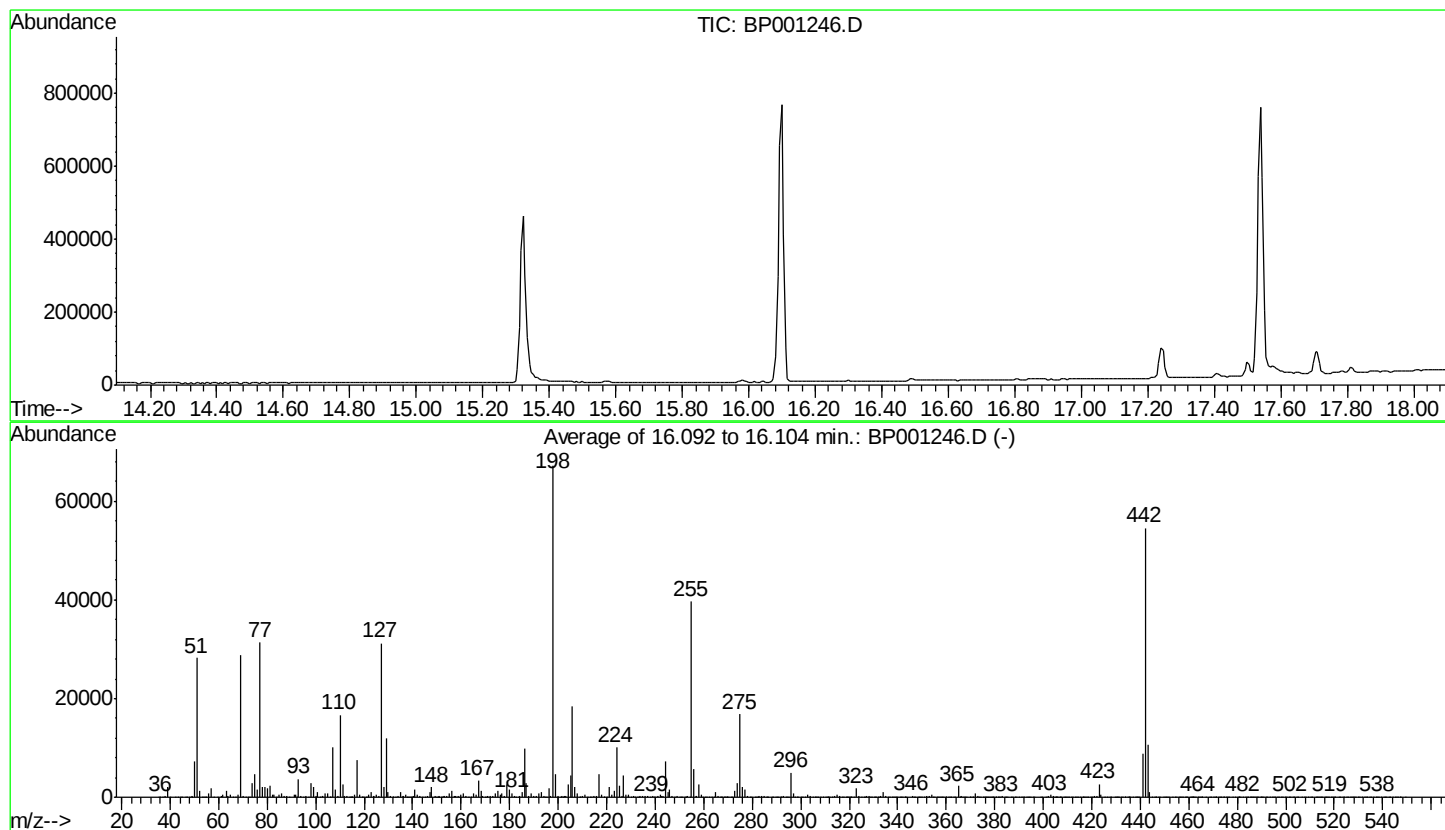

AutoFind: Scans 2381, 2382, 2383; Background Corrected with Scan 2373

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.0	28246	PASS
68	69	0.00	2	1.5	438	PASS
69	198	0.00	100	42.8	28763	PASS
70	69	0.00	2	0.7	200	PASS
127	198	10	80	46.4	31152	PASS
197	198	0.00	2	0.5	335	PASS
198	198	100	100	100.0	67202	PASS
199	198	5	9	6.8	4573	PASS
275	198	10	60	24.9	16756	PASS
365	198	1	100	3.5	2329	PASS
441	198	0.01	100	13.0	8743	PASS
442	198	50	100	81.2	54568	PASS
443	442	15	24	19.6	10692	PASS