

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120722\
 Data File : BP012974.D
 Acq On : 07 Dec 2022 17:57
 Operator : CG/JU
 Sample : PB149448BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK448

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012974.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.358	25	29	35	rVB	126973	166327	1.05%	0.111%
2	3.787	99	102	122	rBV	1551172	2586341	16.35%	1.731%
3	4.116	154	158	166	rVB	40176	62836	0.40%	0.042%
4	7.134	664	671	682	rBV	1906496	2984703	18.87%	1.998%
5	7.304	693	700	713	rVB	1703232	2632267	16.64%	1.762%
6	7.504	727	734	743	rBV	2044732	3173578	20.06%	2.124%
7	7.975	804	814	824	rBV	1869738	3023439	19.11%	2.024%
8	8.681	927	934	952	rBV	2369151	3933350	24.87%	2.633%
9	9.146	1003	1013	1022	rBV	1954796	3146439	19.89%	2.106%
10	9.869	1125	1136	1147	rBV	1600737	2633603	16.65%	1.763%
11	10.410	1220	1228	1238	rBV	2479290	4100792	25.92%	2.745%
12	10.793	1285	1293	1303	rVB	2785280	4570098	28.89%	3.059%
13	10.928	1307	1316	1327	rBV	2510266	4383729	27.71%	2.934%
14	12.375	1557	1562	1570	rBV	47305	80964	0.51%	0.054%
15	13.510	1749	1755	1760	rBV5	9366	16437	0.10%	0.011%
16	14.022	1835	1842	1854	rBV	5292054	7229778	45.71%	4.839%
17	14.310	1884	1891	1909	rBV	5875266	8328666	52.65%	5.574%
18	14.616	1935	1943	1951	rBV	4760098	6816241	43.09%	4.562%
19	14.804	1968	1975	2000	rBV	2114950	3169486	20.04%	2.121%
20	14.975	2002	2004	2008	rVV4	14436	20906	0.13%	0.014%
21	15.022	2010	2012	2018	rVB7	14285	22940	0.15%	0.015%
22	15.416	2074	2079	2086	rVB6	7111	17524	0.11%	0.012%
23	15.610	2105	2112	2125	rBV	7560882	10770446	68.09%	7.209%
24	15.722	2125	2131	2146	rVV	2580594	3462115	21.89%	2.317%
25	15.851	2148	2153	2158	rVB2	34035	58088	0.37%	0.039%
26	16.392	2240	2245	2251	rBV8	10850	20014	0.13%	0.013%
27	17.051	2353	2357	2362	rVB8	12730	22101	0.14%	0.015%
28	17.151	2370	2374	2378	rBV4	11892	20912	0.13%	0.014%
29	17.375	2403	2412	2422	rBV	5975068	8624092	54.52%	5.772%
30	17.469	2422	2428	2443	rVV	8432751	12104969	76.53%	8.102%
31	17.757	2471	2477	2483	rBV7	9359	20560	0.13%	0.014%
32	19.274	2731	2735	2740	rBV2	111037	148912	0.94%	0.100%
33	19.345	2743	2747	2752	rBV	102266	144394	0.91%	0.097%
34	19.698	2801	2807	2821	rBV	10931225	14937758	94.44%	9.998%
35	21.457	3100	3106	3117	rBV	7209794	9824013	62.11%	6.575%
36	23.786	3494	3502	3519	rBV2	7528074	15817996	100.00%	10.587%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120722\
Data File : BP012974.D
Acq On : 07 Dec 2022 17:57
Operator : CG/JU
Sample : PB149448BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK448

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Title : SVOA CALIBRATION

37 23.945 3522 3529 3543 rVB 4977126 10332324 65.32% 6.915%




Sum of corrected areas: 149409138

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120722\
Data File : BP012974.D
Acq On : 07 Dec 2022 17:57
Operator : CG/JU
Sample : PB149448BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK448

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

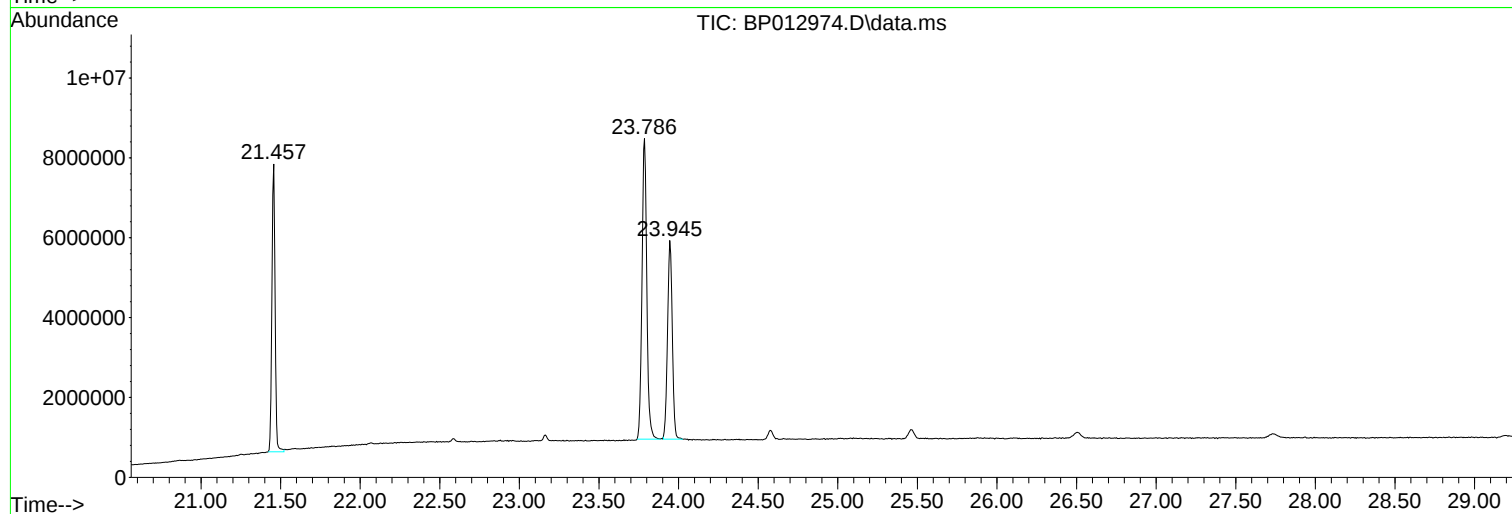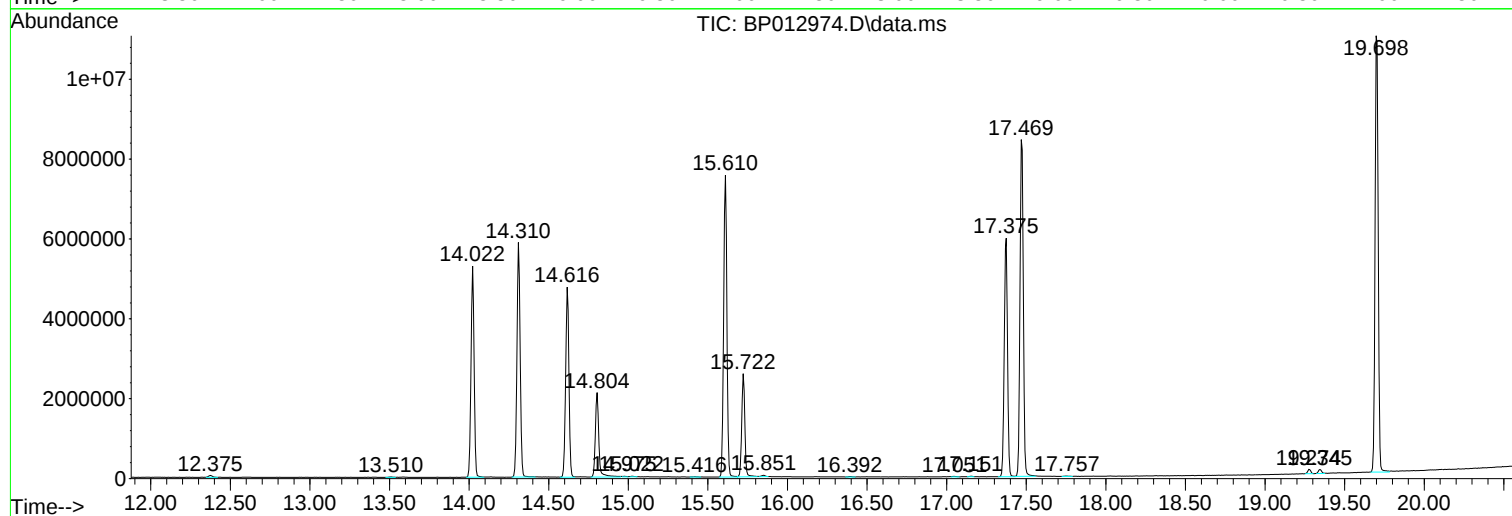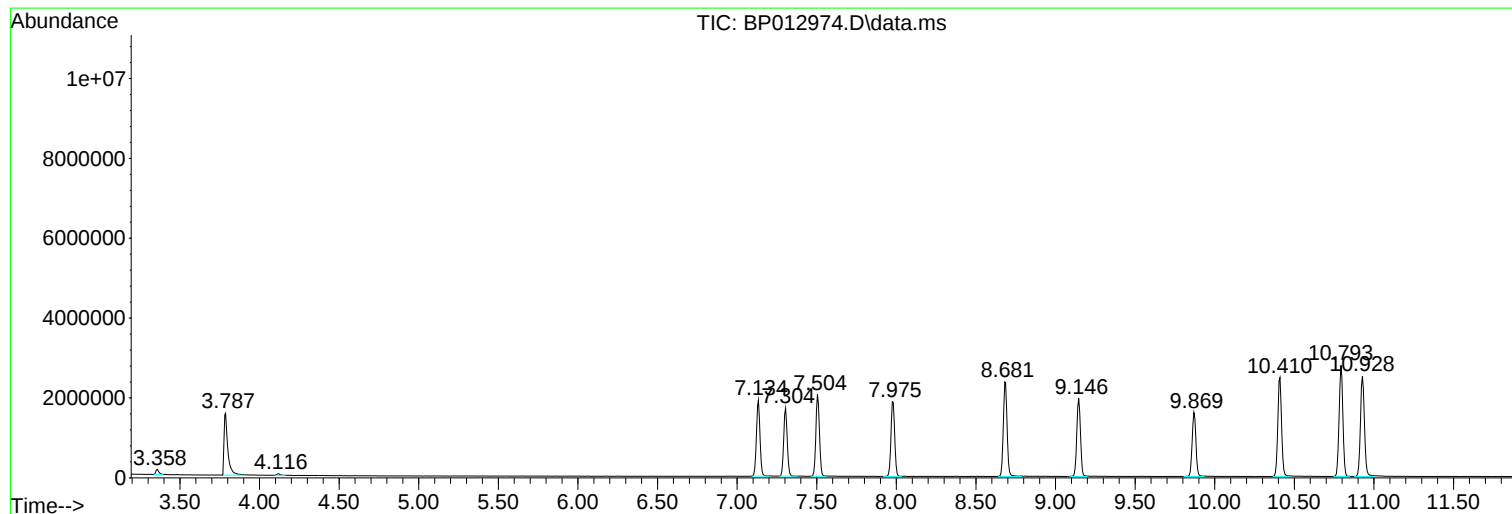

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120722\
Data File : BP012974.D
Acq On : 07 Dec 2022 17:57
Operator : CG/JU
Sample : PB149448BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK448

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120722\
Data File : BP012974.D
Acq On : 07 Dec 2022 17:57
Operator : CG/JU
Sample : PB149448BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK448

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc