
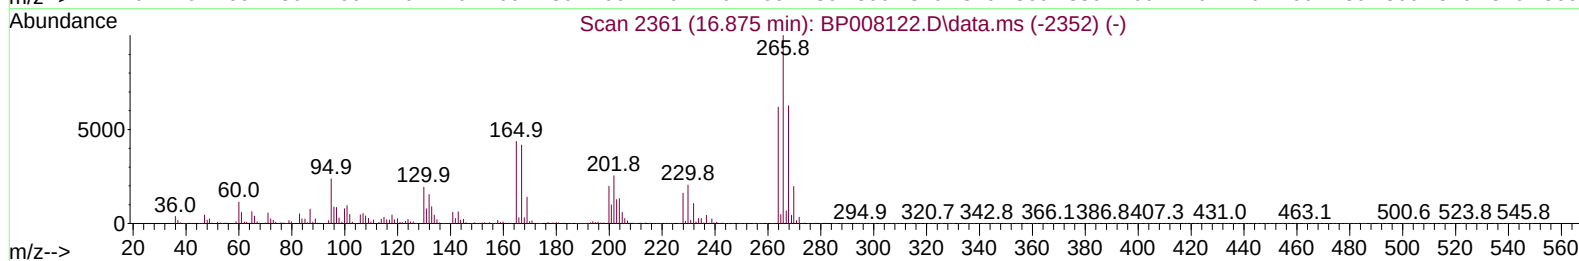
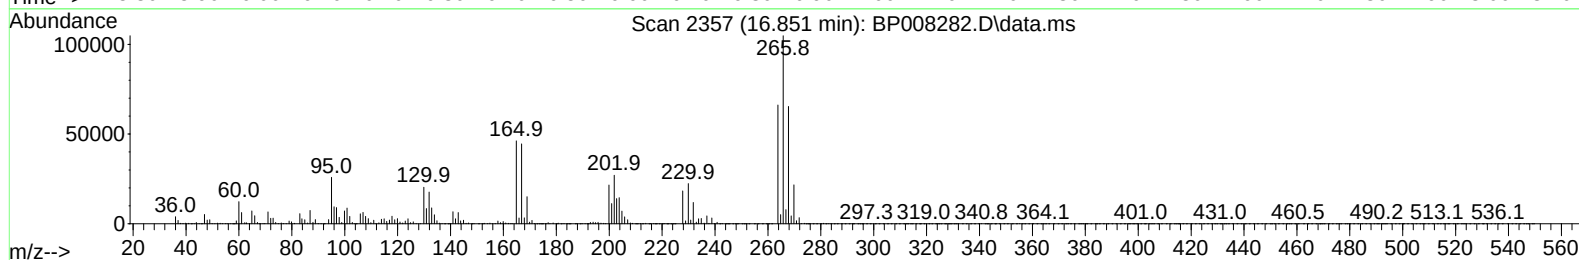


Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP120821\  
 Data File : BP008282.D  
 Acq On : 08 Dec 2021 16:54  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 09 10:19:46 2021  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP112521.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Dec 09 01:43:36 2021  
 Response via : Initial Calibration

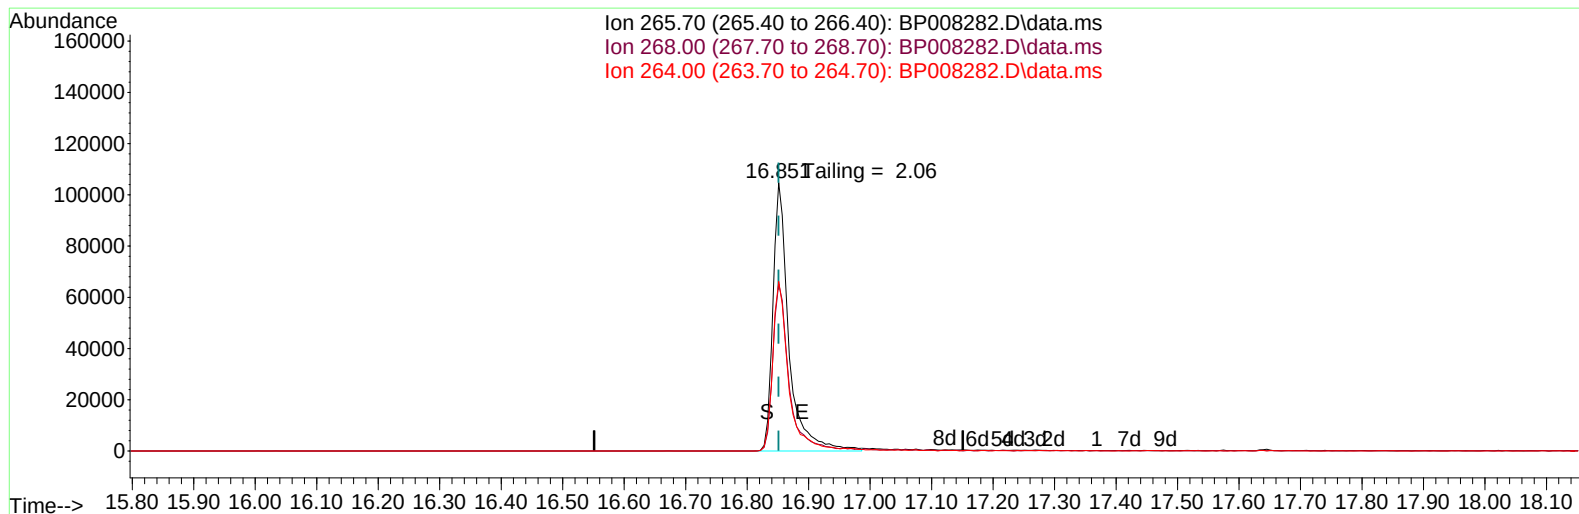

TIC: BP008282.D\data.ms

**(70) Pentachlorophenol (C)**




16.851min (+ 0.000) 22577.40 ng m

response 194686

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.60  | 62.37  |
| 264.00 | 61.90  | 63.14  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP120821\  
 Data File : BP008282.D  
 Acq On : 08 Dec 2021 16:54  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 09 10:19:46 2021  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP112521.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Dec 09 01:43:36 2021  
 Response via : Initial Calibration

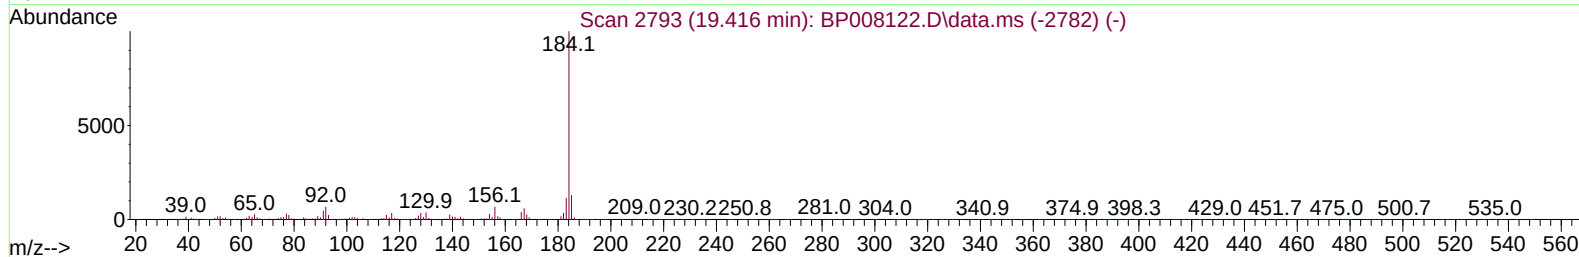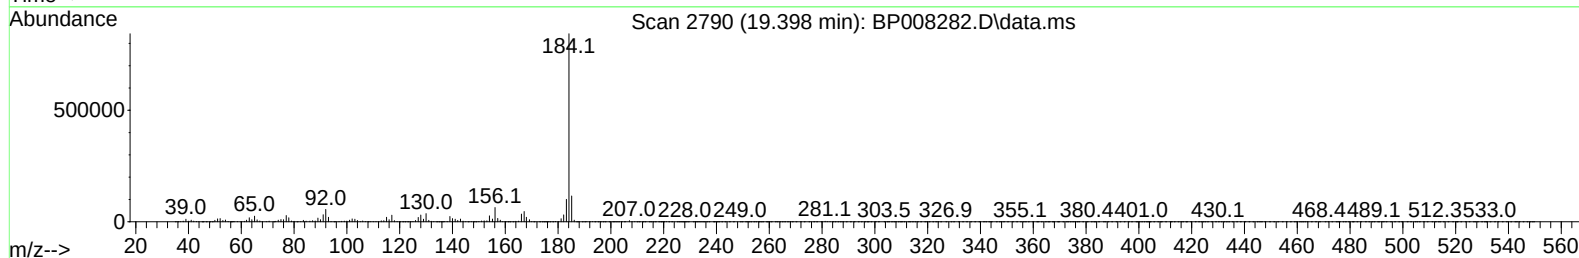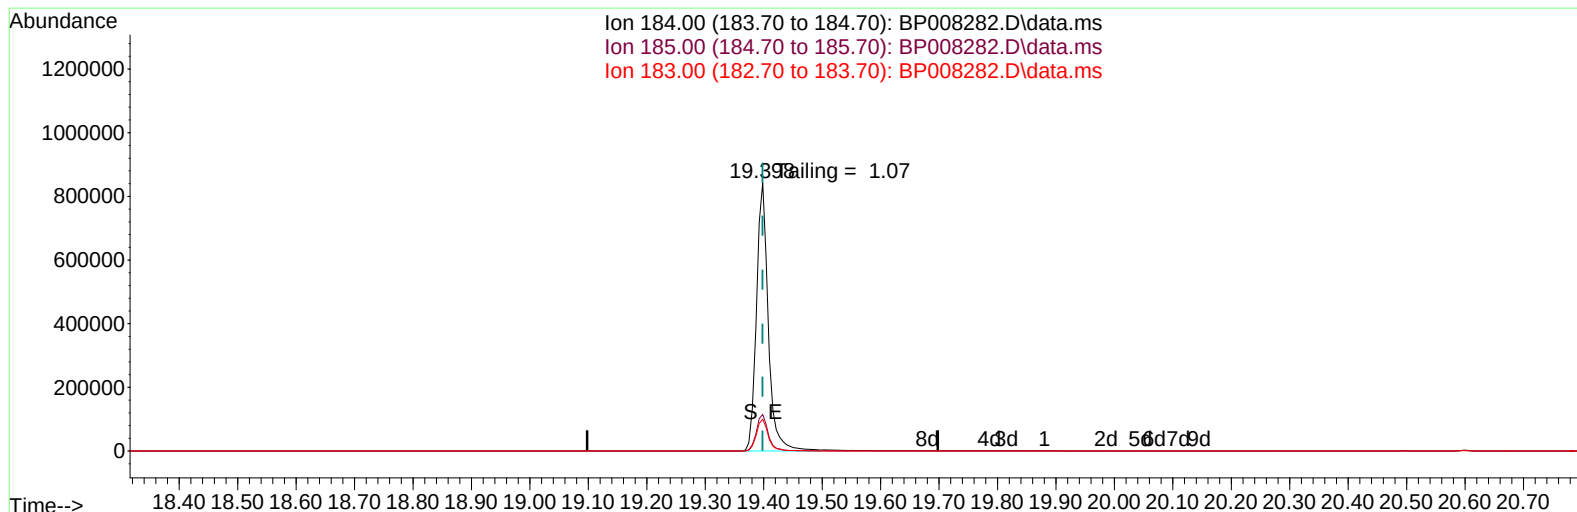

TIC: BP008282.D\data.ms

**(77) Benzidine**

19.398min (+ 0.000) 6778845.85 ng m

response 1208830

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 12.90  | 13.67  |
| 183.00 | 11.40  | 11.88  |
| 0.00   | 0.00   | 0.00   |