


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120821\
 Data File : BP008282.D
 Acq On : 08 Dec 2021 16:54
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Dec 11 03:53:01 2021

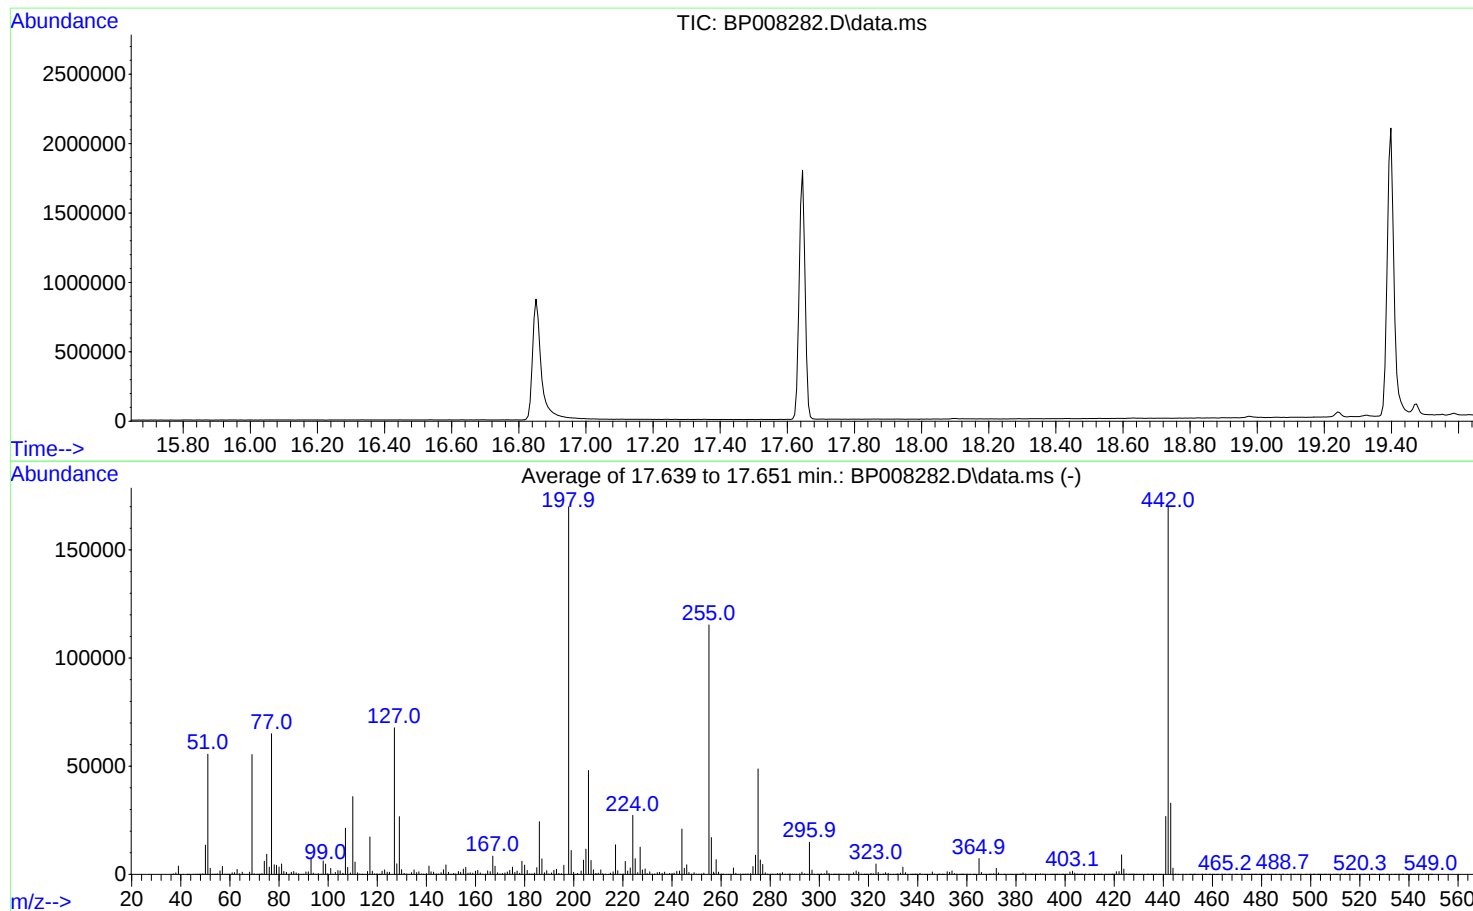




AutoFind: Scans 2491, 2492, 2493; Background Corrected with Scan 2484

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.7	55555	PASS
68	69	0.00	2	1.8	1010	PASS
69	198	0.00	100	32.6	55384	PASS
70	69	0.00	2	0.6	322	PASS
127	198	10	80	39.9	67748	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	169899	PASS
199	198	5	9	6.5	11050	PASS
275	198	10	60	28.7	48747	PASS
365	198	1	100	4.3	7325	PASS
441	198	0.01	100	15.8	26803	PASS
442	442	100	100	100.0	170084	PASS
443	442	15	24	19.3	32904	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120821\
 Data File : BP008282.D
 Acq On : 08 Dec 2021 16:54
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Dec 09 10:19:46 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 09 01:43:36 2021
 Response via : Initial Calibration

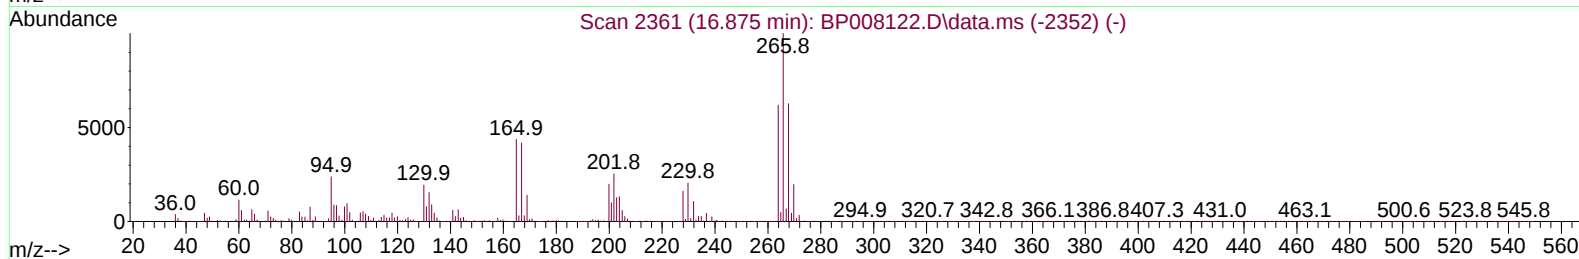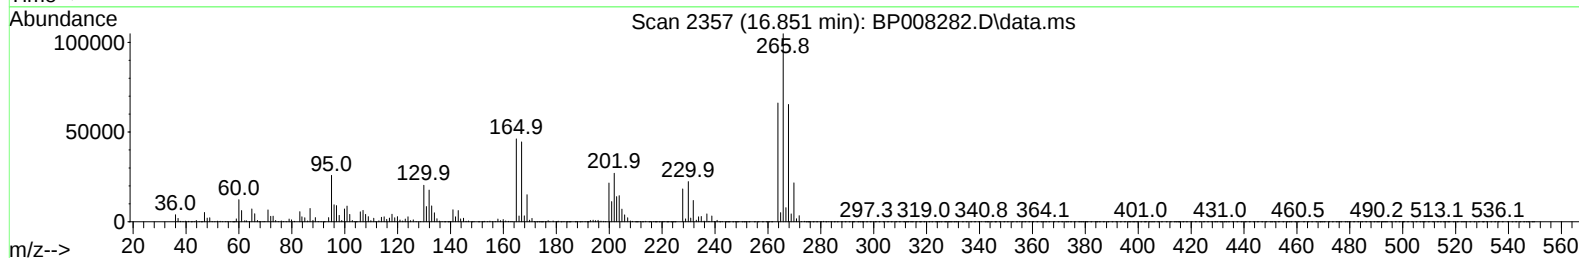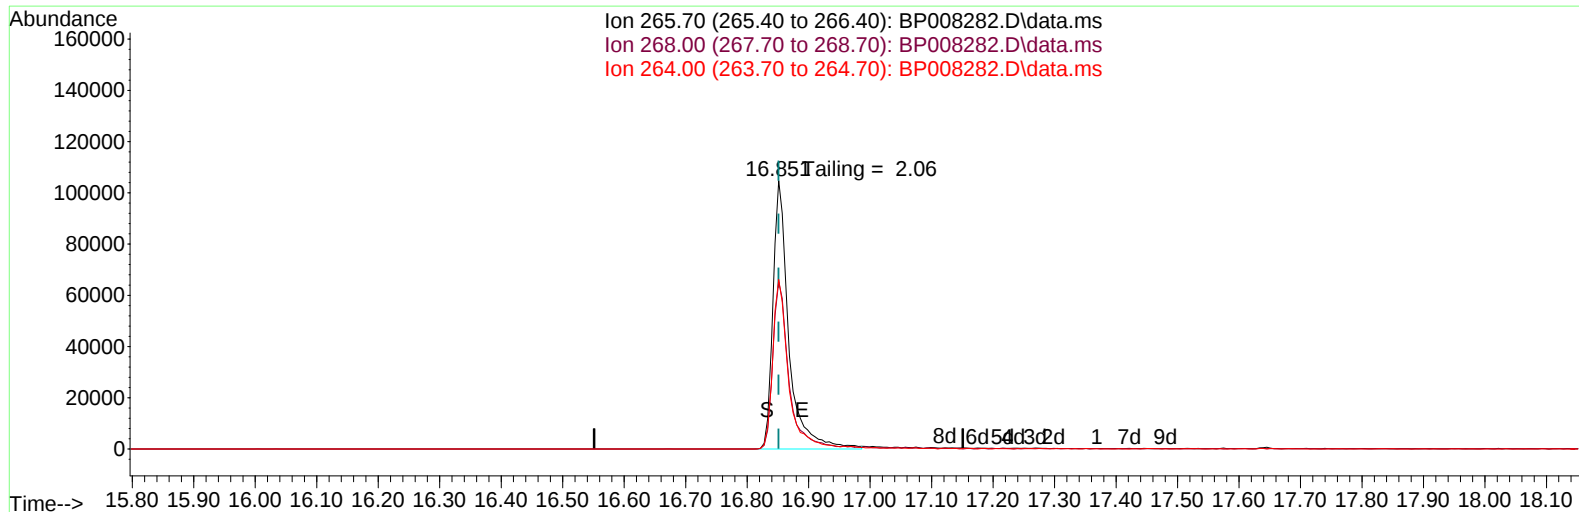

TIC: BP008282.D\data.ms

(70) Pentachlorophenol (C)

16.851min (+ 0.000) 22577.40 ng m




response 194686

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	62.37
264.00	61.90	63.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120821\
 Data File : BP008282.D
 Acq On : 08 Dec 2021 16:54
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Dec 09 10:19:46 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 09 01:43:36 2021
 Response via : Initial Calibration

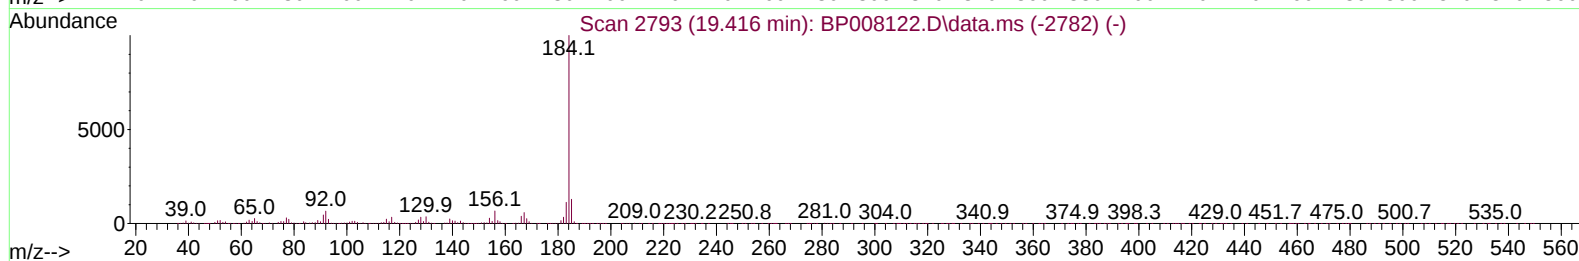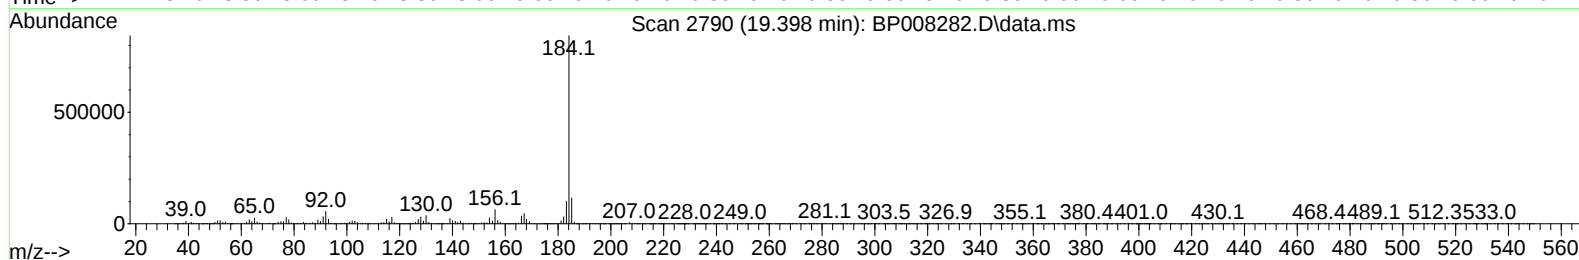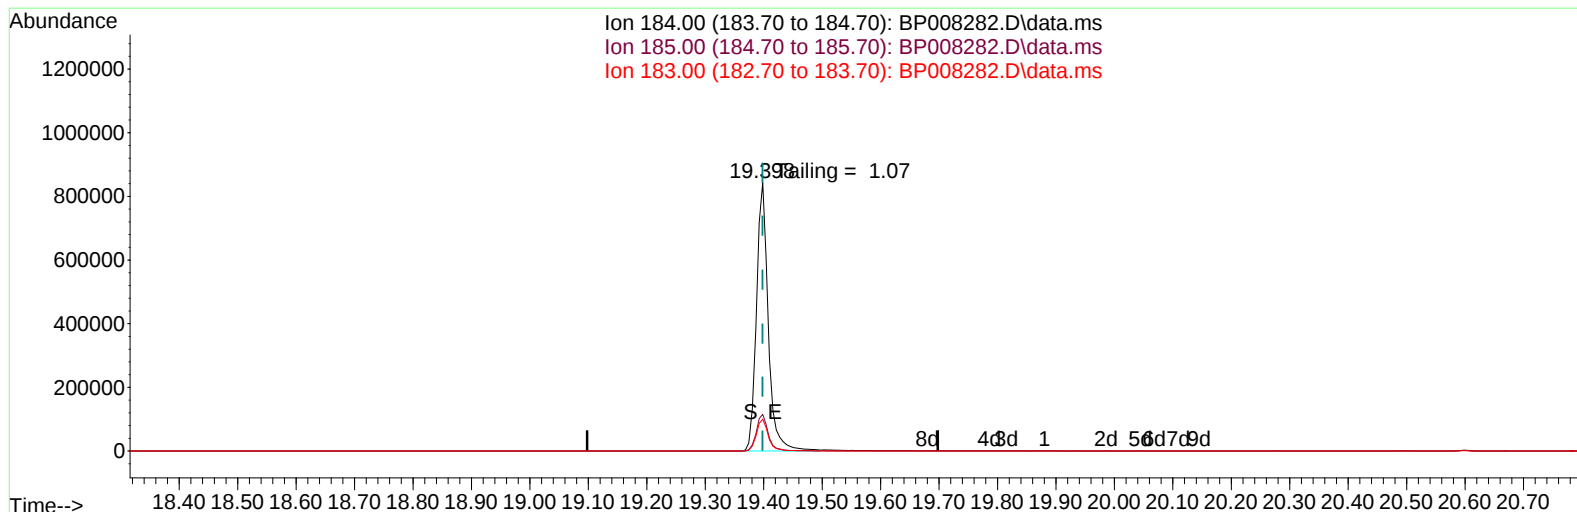

TIC: BP008282.D\data.ms

(77) Benzidine

19.398min (+ 0.000) 6778845.85 ng m

response 1208830

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	12.90	13.67
183.00	11.40	11.88
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_P
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
12/8/2021	BNA_P	BP008282.D
Compound Name	Response	Retention Time
DDT	611514	20.598
DDD	17914	20.174
DDE	2173	19.68
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
20087	631601	3.18