


Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP121019\
 Data File : BP001293.D
 Acq On : 10 Dec 2019 10:13
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP112719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Dec 05 12:34:47 2019

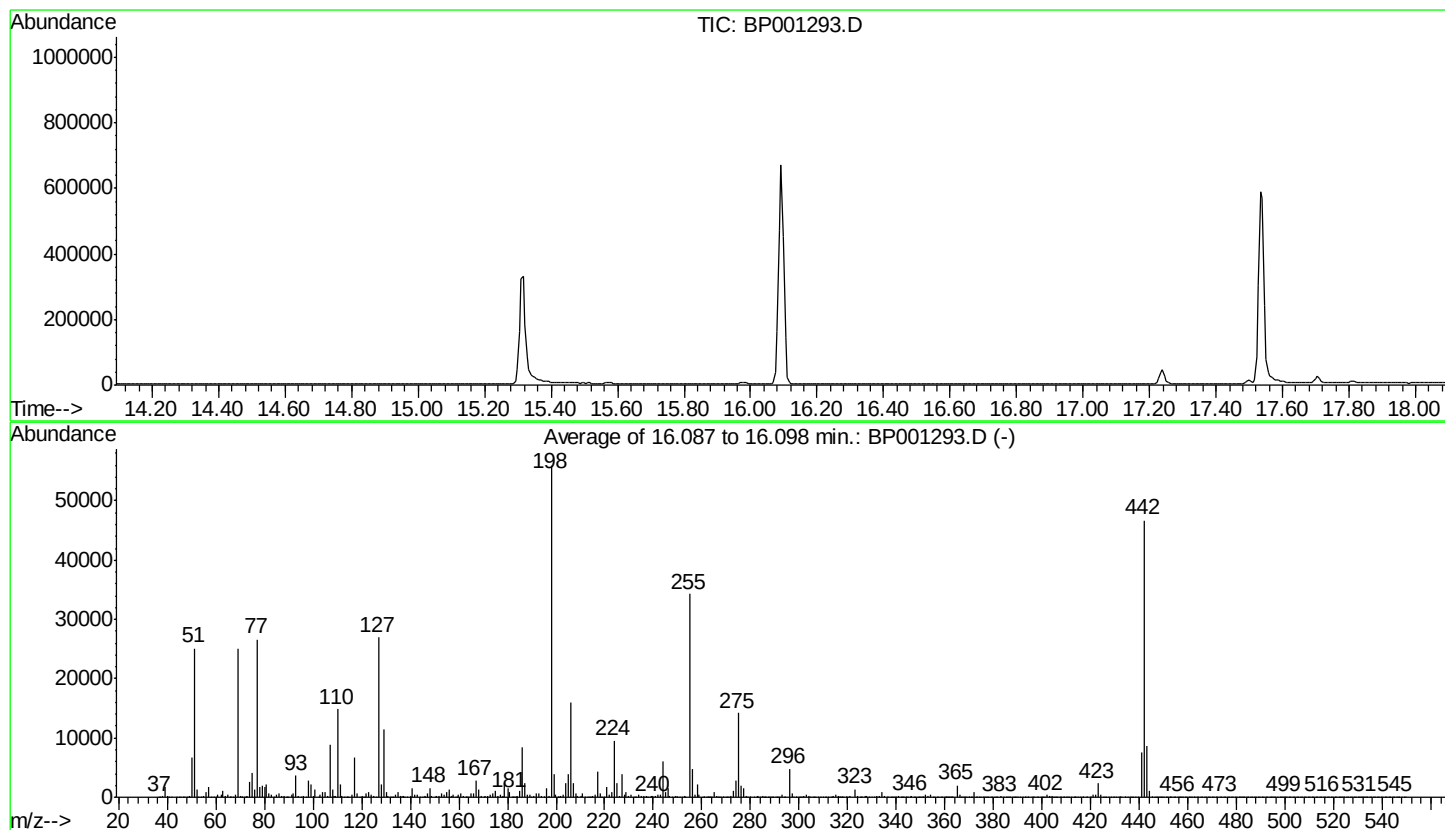

AutoFind: Scans 2380, 2381, 2382; Background Corrected with Scan 2373

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.9	25109	PASS
68	69	0.00	2	1.9	466	PASS
69	198	0.00	100	44.6	24972	PASS
70	69	0.00	2	0.5	118	PASS
127	198	10	80	48.2	26957	PASS
197	198	0.00	2	0.3	143	PASS
198	198	100	100	100.0	55938	PASS
199	198	5	9	6.9	3832	PASS
275	198	10	60	25.4	14219	PASS
365	198	1	100	3.5	1964	PASS
441	198	0.01	100	13.4	7477	PASS
442	198	50	100	83.5	46690	PASS
443	442	15	24	18.5	8650	PASS