

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
 Data File : BP013058.D
 Acq On : 11 Dec 2022 01:32
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: Dec 12 03:30:16 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Dec 12 01:32:54 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.969	152	726904	20.000	ng/u1	0.00
20) Naphthalene-d8	10.787	136	3196469	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.610	164	2151550	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.369	188	4799203	20.000	ng/u1	0.00
79) Chrysene-d12	21.451	240	4387707	20.000	ng/u1	0.00
88) Perylene-d12	23.939	264	4271034	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.352	96	125490	7.381	ng/uL	0.00
4) Pyridine-d5	3.781	84	931641	19.291	ng/u1	0.00
7) Phenol-d5	7.122	99	1166675	19.705	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.293	67	726263	20.334	ng/u1	0.00
11) 2-Chlorophenol-d4	7.499	132	944858	20.272	ng/u1	0.00
15) 4-Methylphenol-d8	8.681	113	959970	19.788	ng/u1	0.00
21) Nitrobenzene-d5	9.140	128	482177	20.531	ng/u1	0.00
24) 2-Nitrophenol-d4	9.863	143	547959	20.725	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.398	165	1043089	20.311	ng/u1	0.00
31) 4-Chloroaniline-d4	10.922	131	1461635	20.160	ng/u1	0.00
46) Dimethylphthalate-d6	14.016	166	3191921	19.303	ng/u1	0.00
49) Acenaphthylene-d8	14.304	160	3651084	20.094	ng/u1	0.00
54) 4-Nitrophenol-d4	14.804	143	583276	19.610	ng/u1	0.00
60) Fluorene-d10	15.604	176	2772628	19.820	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.722	200	583892	18.906	ng/u1	0.00
73) Anthracene-d10	17.463	188	4371004	20.188	ng/u1	0.00
81) Pyrene-d10	19.692	212	5102005	20.258	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.774	264	4248297	19.956	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.387	88	133753	7.536	ng/uL	95
5) Pyridine	3.799	79	924722	19.266	ng/u1	97
6) Benzaldehyde	7.105	77	457637	19.739	ng/u1	98
8) Phenol	7.152	94	1199266	20.033	ng/u1	99
10) Bis(2-Chloroethyl)ether	7.387	93	987621	20.100	ng/u1	98
12) 2-Chlorophenol	7.528	128	964139	20.172	ng/u1	97
13) 2-Methylphenol	8.410	108	928292	19.890	ng/u1	97
14) 2,2'-oxybis(1-Chloropr...	8.499	45	1421733	21.087	ng/u1	99
16) Acetophenone	8.799	105	1551543	20.858	ng/u1	98
17) N-Nitroso-di-n-propyla...	8.787	70	776964	20.771	ng/u1	98
18) 4-Methylphenol	8.740	108	1033065	19.984	ng/u1	98
19) Hexachloroethane	9.057	117	384538	20.133	ng/u1	98
22) Nitrobenzene	9.181	77	1135005	20.595	ng/u1	100
23) Isophorone	9.710	82	2231023	20.021	ng/u1	99
25) 2-Nitrophenol	9.893	139	588393	20.539	ng/u1	96
26) 2,4-Dimethylphenol	9.951	107	1123765	20.104	ng/u1	99
27) Bis(2-Chloroethoxy)met...	10.187	93	1409250	19.778	ng/u1	99
29) 2,4-Dichlorophenol	10.428	162	1018046	20.237	ng/u1	99
30) Naphthalene	10.834	128	3307030	19.782	ng/u1	99
32) 4-Chloroaniline	10.945	127	1459290	20.340	ng/u1	99
33) Hexachlorobutadiene	11.116	225	681506	19.730	ng/u1	97
34) Caprolactam	11.728	113	213448	12.444	ng/u1	98
35) 4-Chloro-3-methylphenol	12.063	107	1055580	20.561	ng/u1	98
36) 2-Methylnaphthalene	12.440	142	2288450	19.954	ng/u1	99

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
 Data File : BP013058.D
 Acq On : 11 Dec 2022 01:32
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: Dec 12 03:30:16 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Dec 12 01:32:54 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.657	142	2351955	19.942	ng/ul	100
39) 1,2,4,5-Tetrachloroben...	12.804	216	1369636	19.770	ng/ul	99
40) Hexachlorocyclopentadiene	12.781	237	709107	15.728	ng/ul	98
41) 2,4,6-Trichlorophenol	13.040	196	893719	20.073	ng/ul	100
42) 2,4,5-Trichlorophenol	13.110	196	972844	20.341	ng/ul	100
43) 1,1'-Biphenyl	13.445	154	3174109	19.643	ng/ul	100
44) 2-Chloronaphthalene	13.487	162	2520961	19.822	ng/ul	99
45) 2-Nitroaniline	13.692	65	672069	21.796	ng/ul	99
47) Dimethylphthalate	14.063	163	3196525	19.504	ng/ul	100
48) 2,6-Dinitrotoluene	14.187	165	635327	20.859	ng/ul	98
50) Acenaphthylene	14.334	152	3911312	20.023	ng/ul	99
51) 3-Nitroaniline	14.516	138	545587	18.970	ng/ul	98
52) Acenaphthene	14.675	153	2666031	19.695	ng/ul	100
53) 2,4-Dinitrophenol	14.722	184	362704	17.421	ng/ul	97
55) 4-Nitrophenol	14.822	109	416880	20.541	ng/ul	97
56) Dibenzofuran	15.010	168	3804695	19.768	ng/ul	99
57) 2,4-Dinitrotoluene	14.969	165	918772	20.767	ng/ul	99
58) 2,3,4,6-Tetrachlorophenol	15.234	232	873150	20.006	ng/ul#	97
59) Diethylphthalate	15.428	149	3115875	19.557	ng/ul	99
61) Fluorene	15.657	166	3102020	20.097	ng/ul	99
62) 4-Chlorophenyl-phenyle...	15.651	204	1627669	19.940	ng/ul	99
63) 4-Nitroaniline	15.681	138	512792	20.263	ng/ul	97
66) 4,6-Dinitro-2-methylph...	15.739	198	575163	19.057	ng/ul	99
67) N-Nitrosodiphenylamine	15.863	169	2662951	20.014	ng/ul	100
68) 4-Bromophenyl-phenylether	16.545	248	964516	18.506	ng/ul	96
69) Hexachlorobenzene	16.663	284	1217639	19.676	ng/ul	97
70) Atrazine	16.822	200	1029523	19.856	ng/ul	99
71) Pentachlorophenol	17.010	266	715873	19.101	ng/ul	99
72) Phenanthrene	17.410	178	5006187	20.027	ng/ul	99
74) Anthracene	17.498	178	5055009	20.253	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.410	216	1366404	19.956	ng/ul	99
76) Pentachlorobenzene	14.928	250	1379624	19.763	ng/ul	100
77) Carbazole	17.769	167	4517328	21.491	ng/ul	100
78) Di-n-butylphthalate	18.310	149	5442287	21.264	ng/ul	100
80) Fluoranthene	19.369	202	5961509	20.855	ng/ul	100
82) Pyrene	19.721	202	6158908	20.887	ng/ul	99
83) Butylbenzylphthalate	20.586	149	2425875	21.296	ng/ul	99
84) 3,3'-Dichlorobenzidine	21.363	252	1729545	17.449	ng/ul	100
85) Benzo(a)anthracene	21.433	228	5907857	20.283	ng/ul	100
86) Bis(2-ethylhexyl)phtha...	21.345	149	3516940	21.887	ng/ul	99
87) Chrysene	21.492	228	5513927	20.018	ng/ul	100
89) Di-n-octyl phthalate	22.298	149	5790764	24.201	ng/ul	100
90) Benzo(b)fluoranthene	23.174	252	5540524	20.343	ng/ul	100
91) Benzo(k)fluoranthene	23.227	252	5500904	20.369	ng/ul	99
93) Benzo(a)pyrene	23.827	252	4716349	19.888	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	26.539	276	5518444	18.682	ng/ul	99
95) Dibenzo(a,h)anthracene	26.556	278	4601015	18.813	ng/ul	100
96) Benzo(g,h,i)perylene	27.339	276	4195499	17.692	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
 Data File : BP013058.D
 Acq On : 11 Dec 2022 01:32
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :


Quant Time: Dec 12 03:30:16 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Dec 12 01:32:54 2022
 Response via : Initial Calibration

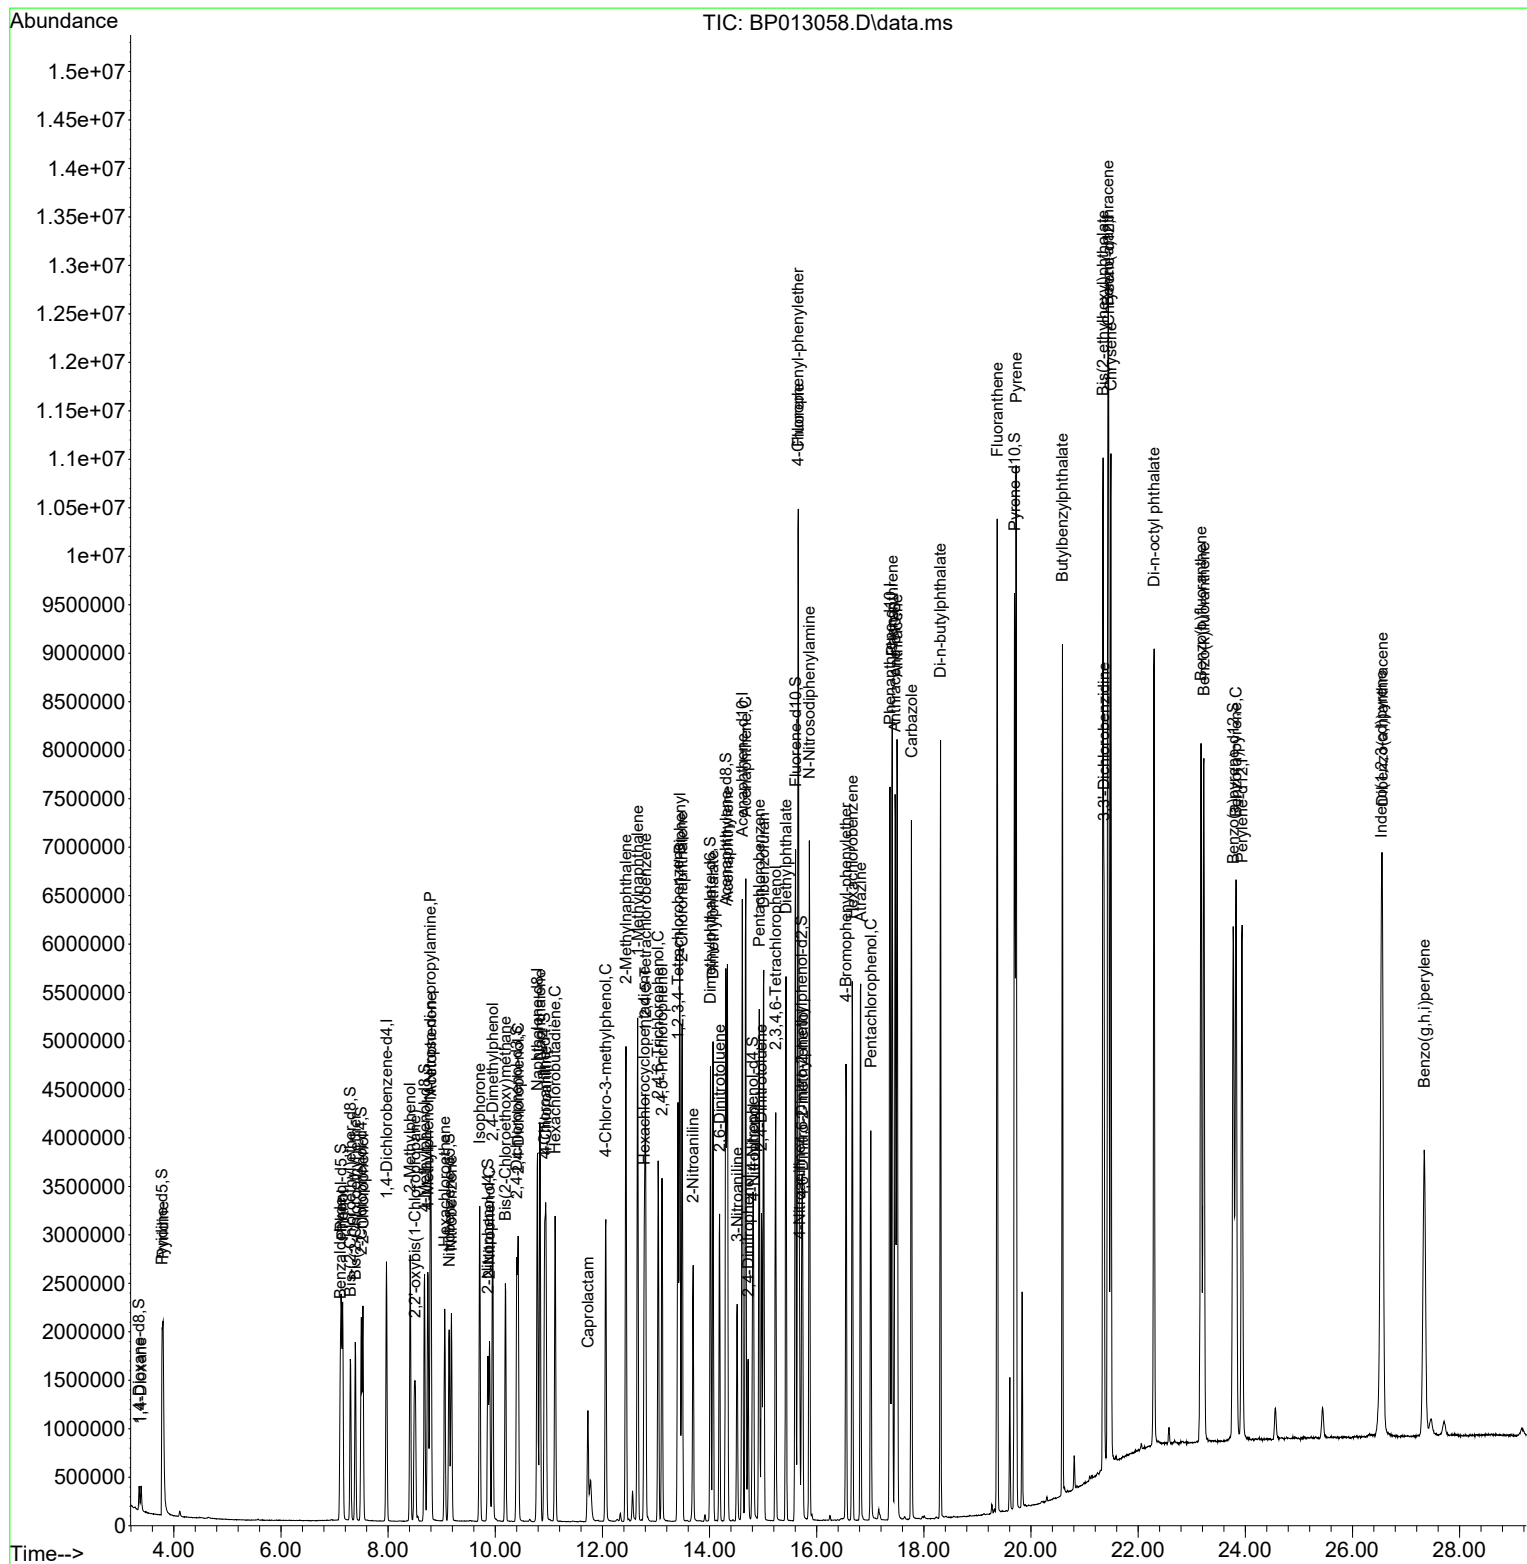



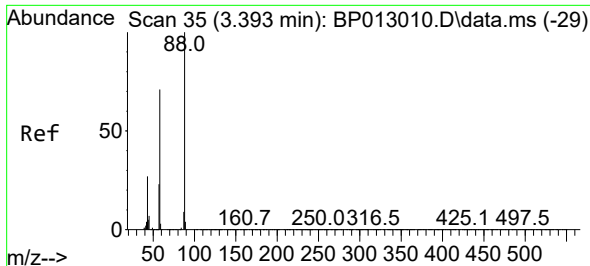


#2
 1,4-Dioxane
 Concen: 7.536 ng/uL
 RT: 3.387 min Scan# 34
 Delta R.T. -0.000 min
 Lab File: BP013058.D
 Acq: 11 Dec 2022 01:32

Instrument :
 BNA_P
 ClientSampleId :



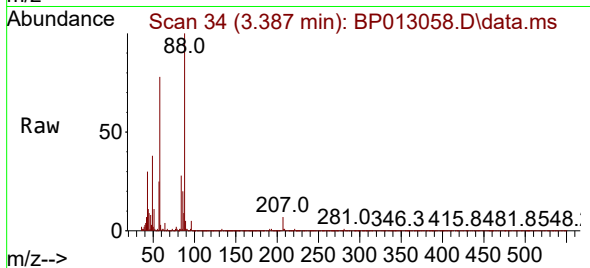



Tgt Ion: 88 Resp: 133753
 Ion Ratio Lower Upper
 88 100
 43 30.1 22.4 33.6
 58 77.7 58.2 87.4

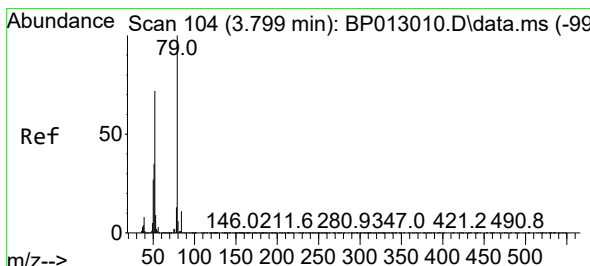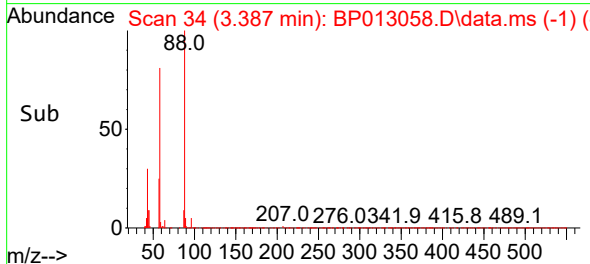

#5
 Pyridine
 Concen: 19.266 ng/uL
 RT: 3.799 min Scan# 104
 Delta R.T. -0.000 min
 Lab File: BP013058.D
 Acq: 11 Dec 2022 01:32

Tgt Ion: 79 Resp: 924722
 Ion Ratio Lower Upper
 79 100
 52 79.4 60.7 91.1
 51 37.4 28.9 43.3


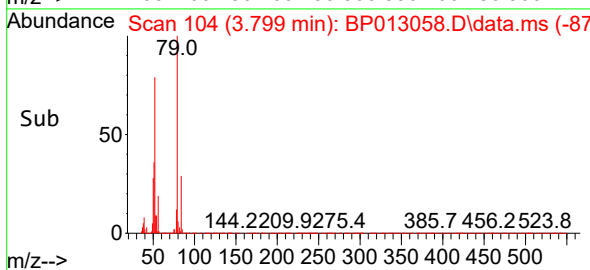

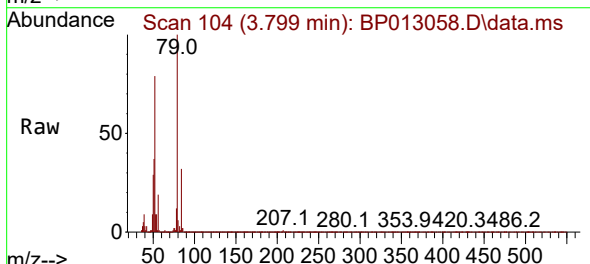


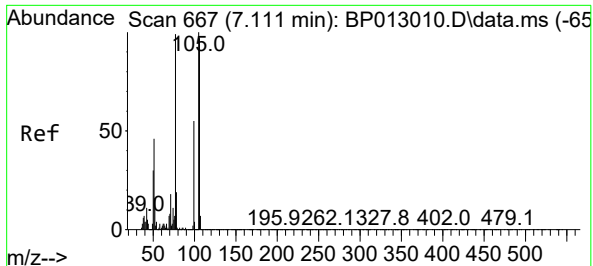

#6
Benzaldehyde
Concen: 19.739 ng/ul
RT: 7.105 min Scan# 666
Delta R.T. -0.000 min
Lab File: BP013058.D
Acq: 11 Dec 2022 01:32




Instrument :
BNA_P
ClientSampleId :


Tgt Ion: 77 Resp: 457637
Ion Ratio Lower Upper
77 100
105 99.0 81.5 122.3
106 96.2 76.9 115.3

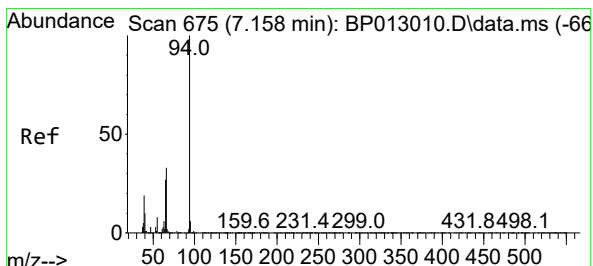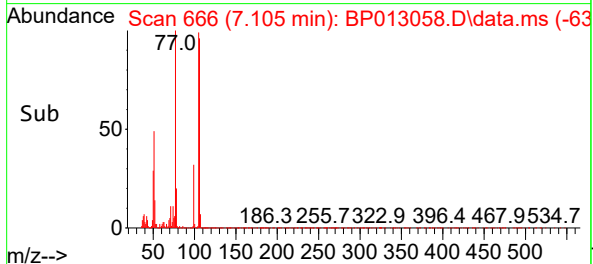

#8
Phenol
Concen: 20.033 ng/ul
RT: 7.152 min Scan# 674
Delta R.T. -0.000 min
Lab File: BP013058.D
Acq: 11 Dec 2022 01:32

Tgt Ion: 94 Resp: 1199266
Ion Ratio Lower Upper
94 100
65 28.0 21.1 31.7
66 33.8 27.0 40.6


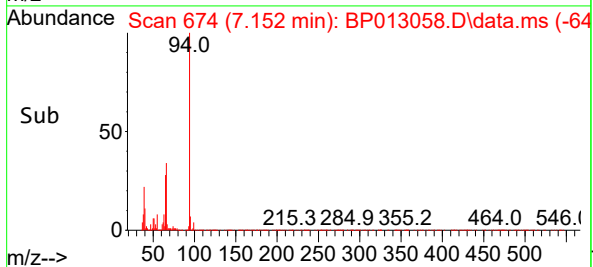

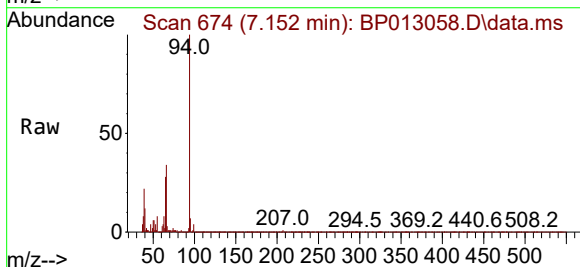




#10
Bis(2-Chloroethyl)ether
Concen: 20.100 ng/ul
RT: 7.387 min Scan# 715
Delta R.T. -0.000 min
Lab File: BP013058.D
Acq: 11 Dec 2022 01:32




Instrument :
BNA_P
ClientSampleId :


Tgt Ion: 93 Resp: 987621
Ion Ratio Lower Upper
93 100
63 77.2 59.8 89.8
95 32.9 26.4 39.6



#12
2-Chlorophenol
Concen: 20.172 ng/ul
RT: 7.528 min Scan# 738
Delta R.T. -0.006 min
Lab File: BP013058.D
Acq: 11 Dec 2022 01:32

Tgt Ion:128 Resp: 964139
Ion Ratio Lower Upper
128 100
64 47.0 34.9 52.3
130 32.4 25.8 38.6





#13

2-Methylphenol

Concen: 19.890 ng/ul

RT: 8.410 min Scan# 8

Delta R.T. -0.000 min

Lab File: BP013058.D

Acq: 11 Dec 2022 01:32

Instrument :

BNA_P





ClientSampleId :

Tgt Ion:108 Resp: 928292

Ion Ratio Lower Upper

108 100

107 89.3 69.1 103.7



#14

2,2'-oxybis(1-Chloropropane)

Concen: 21.087 ng/ul

RT: 8.499 min Scan# 903

Delta R.T. -0.006 min

Lab File: BP013058.D

Acq: 11 Dec 2022 01:32




Tgt Ion: 45 Resp: 1421733


Ion Ratio Lower Upper

45 100

77 13.8 11.0 16.6

79 10.4 9.3 13.9




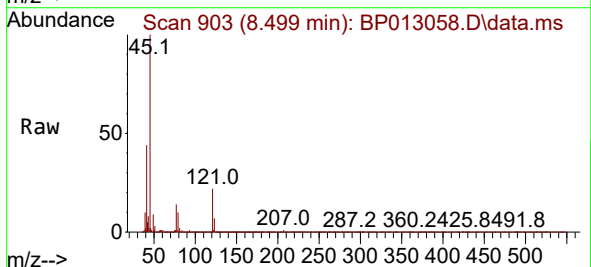




#16
Acetophenone
Concen: 20.858 ng/ul
RT: 8.799 min Scan# 91
Delta R.T. -0.000 min
Lab File: BP013058.D
Acq: 11 Dec 2022 01:32




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:105 Resp: 1551543
Ion Ratio Lower Upper
105 100
77 74.4 59.3 88.9
51 27.1 19.6 29.4



#17
N-Nitroso-di-n-propylamine
Concen: 20.771 ng/ul
RT: 8.787 min Scan# 952
Delta R.T. -0.000 min
Lab File: BP013058.D
Acq: 11 Dec 2022 01:32

Tgt Ion: 70 Resp: 776964
Ion Ratio Lower Upper
70 100
42 59.0 45.5 68.3
101 10.0 7.9 11.9
130 22.0 17.4 26.2

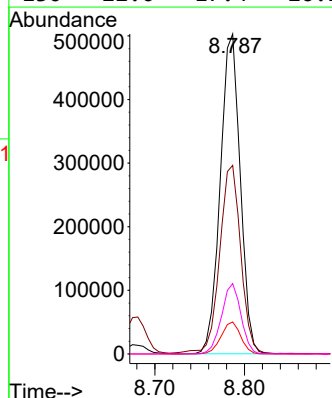



#18

4-Methylphenol

Concen: 19.984 ng/ul

RT: 8.740 min Scan# 945

Delta R.T. -0.000 min

Lab File: BP013058.D

Acq: 11 Dec 2022 01:32

Instrument :

BNA_P





ClientSampleId :

Tgt Ion:108 Resp: 1033065

Ion Ratio Lower Upper

108 100

107 111.5 87.4 131.2



#19

Hexachloroethane

Concen: 20.133 ng/ul

RT: 9.057 min Scan# 998

Delta R.T. -0.000 min

Lab File: BP013058.D

Acq: 11 Dec 2022 01:32




Tgt Ion:117 Resp: 384538


Ion Ratio Lower Upper

117 100

201 114.0 93.7 140.5

199 71.7 58.6 88.0


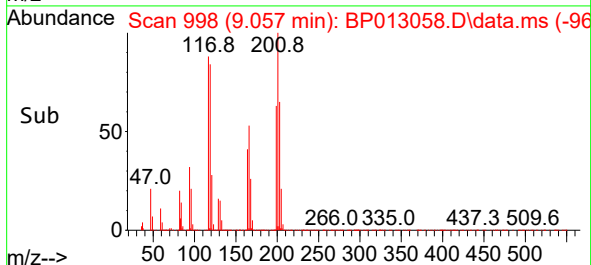
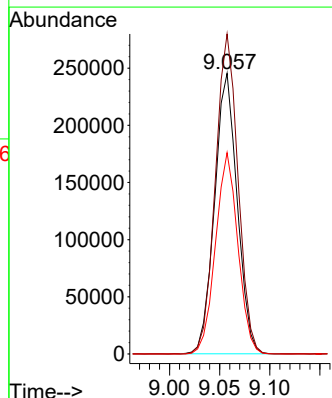
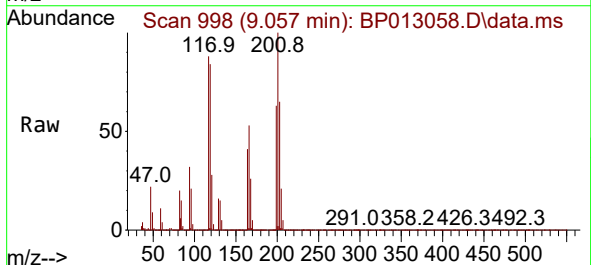




#22
Nitrobenzene
Concen: 20.595 ng/ul
RT: 9.181 min Scan# 1109
Delta R.T. -0.000 min
Lab File: BP013058.D
Acq: 11 Dec 2022 01:32




Instrument :
BNA_P
ClientSampleId :


Tgt Ion: 77 Resp: 1135005
Ion Ratio Lower Upper
77 100
123 47.6 38.3 57.5
65 12.8 10.3 15.5



#23
Isophorone
Concen: 20.021 ng/ul
RT: 9.710 min Scan# 1109
Delta R.T. -0.000 min
Lab File: BP013058.D
Acq: 11 Dec 2022 01:32

Tgt Ion: 82 Resp: 2231023
Ion Ratio Lower Upper
82 100
95 6.9 5.4 8.2
138 18.2 15.3 22.9


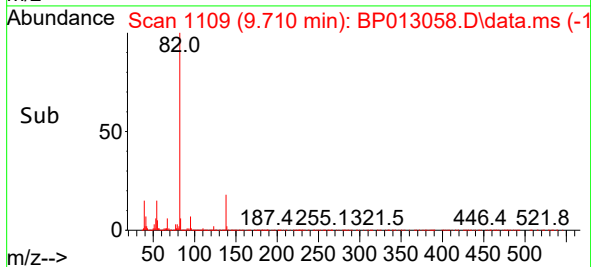

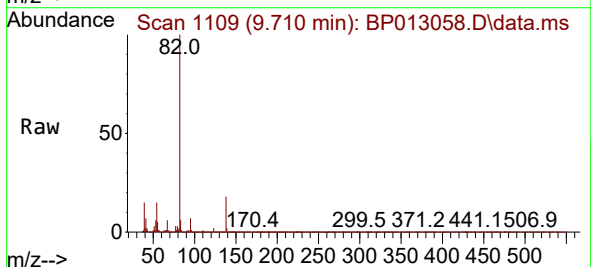




#25
2-Nitrophenol
Concen: 20.539 ng/ul
RT: 9.893 min Scan# 1141
Delta R.T. -0.000 min
Lab File: BP013058.D
Acq: 11 Dec 2022 01:32




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:139 Resp: 588393
Ion Ratio Lower Upper
139 100
65 49.4 36.6 54.8
109 27.5 21.6 32.4



#26
2,4-Dimethylphenol
Concen: 20.104 ng/ul
RT: 9.951 min Scan# 1150
Delta R.T. -0.000 min
Lab File: BP013058.D
Acq: 11 Dec 2022 01:32

Tgt Ion:107 Resp: 1123765
Ion Ratio Lower Upper
107 100
121 52.5 41.8 62.6
122 89.1 72.6 108.8









#27
Bis(2-Chloroethoxy)methane
Concen: 19.778 ng/ul
RT: 10.187 min Scan# 1190
Delta R.T. -0.006 min
Lab File: BP013058.D
Acq: 11 Dec 2022 01:32




Instrument :
BNA_P
ClientSampleId :


Tgt Ion: 93 Resp: 1409250
Ion Ratio Lower Upper
93 100
95 32.8 26.0 39.0
123 11.3 9.2 13.8



#29
2,4-Dichlorophenol
Concen: 20.237 ng/ul
RT: 10.428 min Scan# 1231
Delta R.T. -0.000 min
Lab File: BP013058.D
Acq: 11 Dec 2022 01:32

Tgt Ion:162 Resp: 1018046
Ion Ratio Lower Upper
162 100
164 65.3 52.5 78.7
98 33.8 26.6 39.8









#30
Naphthalene
Concen: 19.782 ng/ul
RT: 10.834 min Scan# 1300
Delta R.T. -0.000 min
Lab File: BP013058.D
Acq: 11 Dec 2022 01:32




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:128 Resp: 3307030
Ion Ratio Lower Upper
128 100
129 11.2 8.7 13.1
127 12.8 10.4 15.6

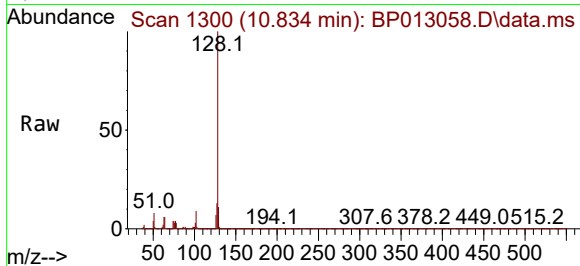

#32
4-Chloroaniline
Concen: 20.340 ng/ul
RT: 10.945 min Scan# 1319
Delta R.T. -0.000 min
Lab File: BP013058.D
Acq: 11 Dec 2022 01:32


Tgt Ion:127 Resp: 1459290
Ion Ratio Lower Upper
127 100
129 32.5 25.6 38.4

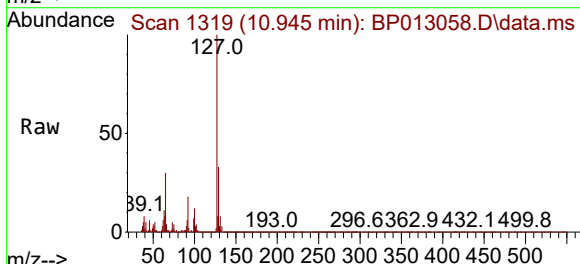






#33
Hexachlorobutadiene
Concen: 19.730 ng/ul
RT: 11.116 min Scan# 11
Delta R.T. -0.006 min
Lab File: BP013058.D
Acq: 11 Dec 2022 01:32

Instrument :
BNA_P
ClientSampleId :







Tgt Ion:225 Resp: 681506
Ion Ratio Lower Upper
225 100
223 63.2 49.2 73.8
227 65.1 50.2 75.2



#34
Caprolactam
Concen: 12.444 ng/ul
RT: 11.728 min Scan# 1452
Delta R.T. -0.000 min
Lab File: BP013058.D
Acq: 11 Dec 2022 01:32

Tgt Ion:113 Resp: 213448
Ion Ratio Lower Upper
113 100
55 173.4 141.9 212.9
56 125.6 99.6 149.4


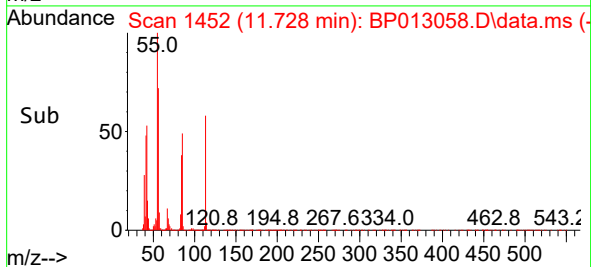

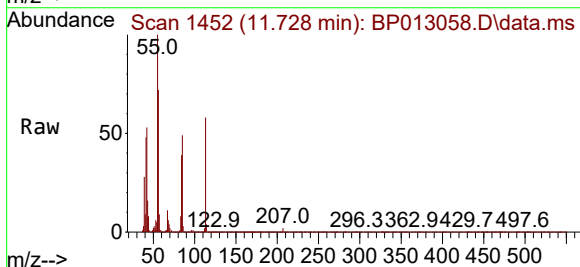




#35
4-Chloro-3-methylphenol
Concen: 20.561 ng/ul
RT: 12.063 min Scan# 1509
Delta R.T. -0.000 min
Lab File: BP013058.D
Acq: 11 Dec 2022 01:32




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:107 Resp: 1055580
Ion Ratio Lower Upper
107 100
144 27.1 21.4 32.2
142 84.6 65.8 98.6



#36
2-Methylnaphthalene
Concen: 19.954 ng/ul
RT: 12.440 min Scan# 1573
Delta R.T. -0.000 min
Lab File: BP013058.D
Acq: 11 Dec 2022 01:32

Tgt Ion:142 Resp: 2288450
Ion Ratio Lower Upper
142 100
141 89.3 70.8 106.2









#37
1-Methylnaphthalene
Concen: 19.942 ng/ul
RT: 12.657 min Scan# 1610
Delta R.T. -0.000 min
Lab File: BP013058.D
Acq: 11 Dec 2022 01:32




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:142 Resp: 2351955
Ion Ratio Lower Upper
142 100
141 91.3 72.7 109.1
116 3.5 2.7 4.1



#39
1,2,4,5-Tetrachlorobenzene
Concen: 19.770 ng/ul
RT: 12.804 min Scan# 1635
Delta R.T. -0.000 min
Lab File: BP013058.D
Acq: 11 Dec 2022 01:32

Tgt Ion:216 Resp: 1369636
Ion Ratio Lower Upper
216 100
214 77.8 61.9 92.9
179 19.5 15.0 22.6
108 14.5 11.0 16.4





#40

Hexachlorocyclopentadiene

Concen: 15.728 ng/ul

RT: 12.781 min Scan# 1631

Delta R.T. -0.006 min

Lab File: BP013058.D

Acq: 11 Dec 2022 01:32

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:237 Resp: 709107

Ion Ratio Lower Upper

237 100

235 63.4 49.7 74.5

272 13.1 10.8 16.2

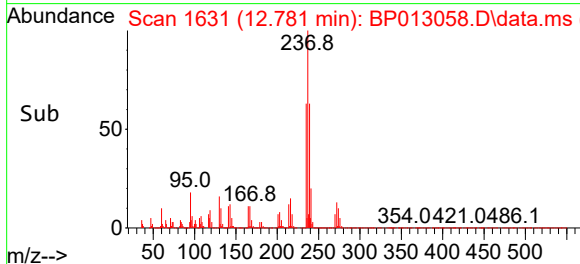

#41

2,4,6-Trichlorophenol

Concen: 20.073 ng/ul

RT: 13.040 min Scan# 1675

Delta R.T. -0.006 min

Lab File: BP013058.D

Acq: 11 Dec 2022 01:32




Tgt Ion:196 Resp: 893719


Ion Ratio Lower Upper

196 100

198 96.1 77.0 115.6

200 31.2 25.3 37.9

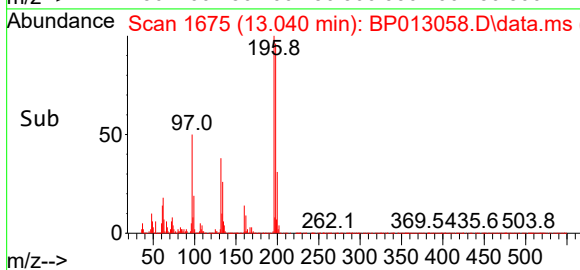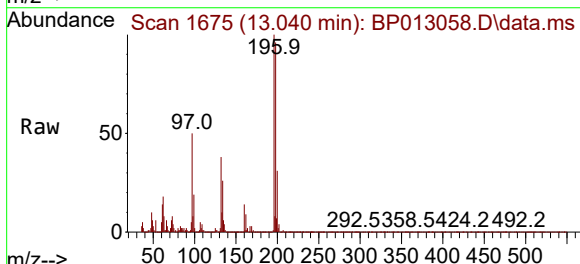



#42

2,4,5-Trichlorophenol

Concen: 20.341 ng/ul

RT: 13.110 min Scan# 1

Delta R.T. -0.006 min

Lab File: BP013058.D

Acq: 11 Dec 2022 01:32

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:196 Resp: 972844

Ion Ratio Lower Upper

196 100

198 96.8 77.1 115.7

200 31.7 25.4 38.2



#43

1,1'-Biphenyl

Concen: 19.643 ng/ul

RT: 13.445 min Scan# 1744

Delta R.T. -0.000 min

Lab File: BP013058.D

Acq: 11 Dec 2022 01:32




Tgt Ion:154 Resp: 3174109


Ion Ratio Lower Upper

154 100

153 39.8 31.5 47.3

76 12.0 9.6 14.4




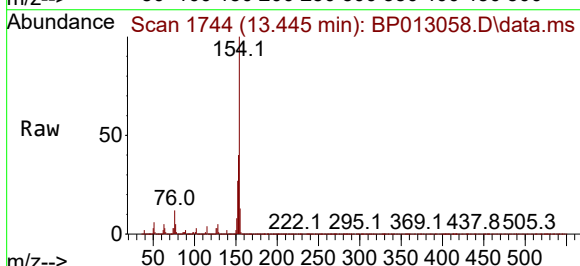




#44
2-Chloronaphthalene
Concen: 19.822 ng/ul
RT: 13.487 min Scan# 1751
Delta R.T. -0.000 min
Lab File: BP013058.D
Acq: 11 Dec 2022 01:32




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:162 Resp: 2520961
Ion Ratio Lower Upper
162 100
164 32.8 26.3 39.5
127 35.9 29.3 43.9

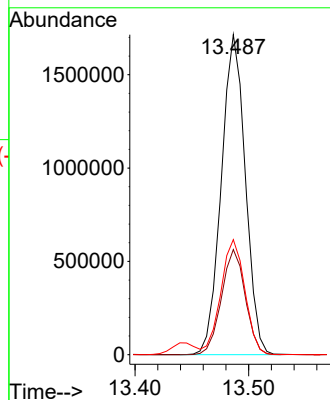

#45
2-Nitroaniline
Concen: 21.796 ng/ul
RT: 13.692 min Scan# 1786
Delta R.T. -0.000 min
Lab File: BP013058.D
Acq: 11 Dec 2022 01:32

Tgt Ion: 65 Resp: 672069
Ion Ratio Lower Upper
65 100
92 71.0 56.4 84.6
138 114.0 90.3 135.5

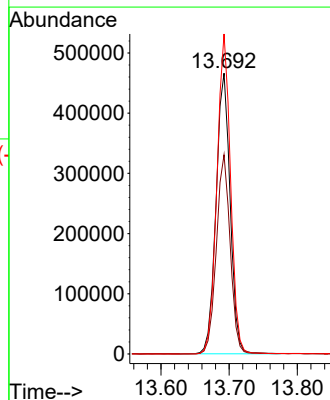



#47

Dimethylphthalate

Concen: 19.504 ng/ul

RT: 14.063 min Scan# 1849

Delta R.T. -0.000 min

Lab File: BP013058.D

Acq: 11 Dec 2022 01:32

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:163 Resp: 3196525

Ion Ratio Lower Upper

163 100

194 4.1 3.4 5.0

164 10.3 8.3 12.5



#48

2,6-Dinitrotoluene

Concen: 20.859 ng/ul

RT: 14.187 min Scan# 1870

Delta R.T. -0.000 min

Lab File: BP013058.D

Acq: 11 Dec 2022 01:32




Tgt Ion:165 Resp: 635327


Ion Ratio Lower Upper

165 100

89 52.0 43.0 64.4

121 19.5 16.1 24.1









#50
Acenaphthylene
Concen: 20.023 ng/ul
RT: 14.334 min Scan# 1895
Delta R.T. -0.000 min
Lab File: BP013058.D
Acq: 11 Dec 2022 01:32




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:152 Resp: 3911312
Ion Ratio Lower Upper
152 100
151 20.1 15.8 23.6
153 13.2 10.6 16.0

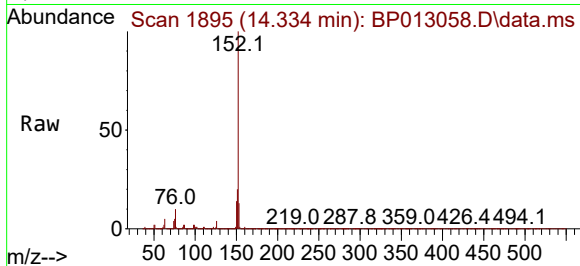

#51
3-Nitroaniline
Concen: 18.970 ng/ul
RT: 14.516 min Scan# 1926
Delta R.T. -0.000 min
Lab File: BP013058.D
Acq: 11 Dec 2022 01:32

Tgt Ion:138 Resp: 545587
Ion Ratio Lower Upper
138 100
108 10.1 8.6 13.0
92 108.9 88.4 132.6

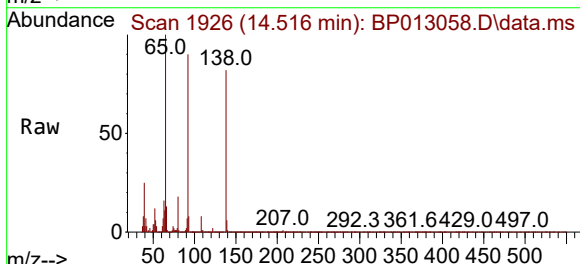



#52

Acenaphthene

Concen: 19.695 ng/ul

RT: 14.675 min Scan# 1953

Delta R.T. -0.000 min

Lab File: BP013058.D

Acq: 11 Dec 2022 01:32

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:153 Resp: 2666031

Ion Ratio Lower Upper

153 100

152 48.1 38.2 57.4

154 88.7 70.8 106.2

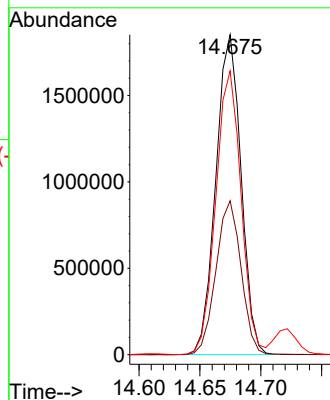

#53

2,4-Dinitrophenol

Concen: 17.421 ng/ul

RT: 14.722 min Scan# 1961

Delta R.T. -0.000 min

Lab File: BP013058.D

Acq: 11 Dec 2022 01:32




Tgt Ion:184 Resp: 362704


Ion Ratio Lower Upper

184 100

63 56.8 48.4 72.6


154 57.6 45.5 68.3

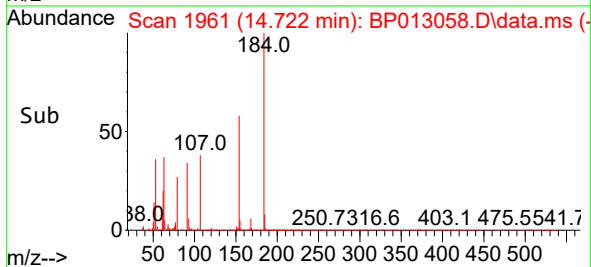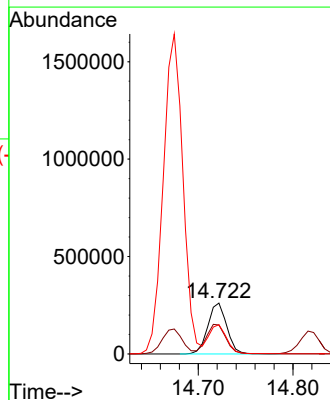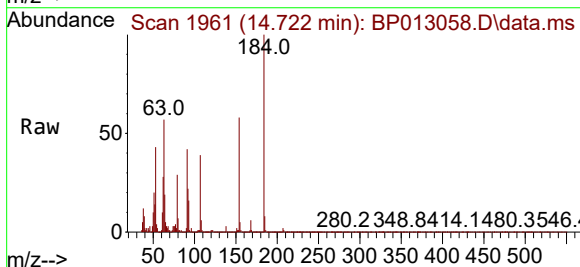






#55
4-Nitrophenol
Concen: 20.541 ng/ul
RT: 14.822 min Scan# 1978
Delta R.T. 0.006 min
Lab File: BP013058.D
Acq: 11 Dec 2022 01:32

Instrument :
BNA_P
ClientSampleId :



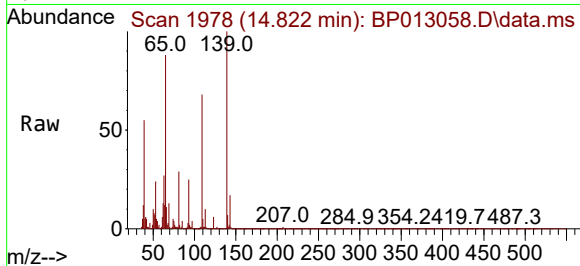



Tgt Ion:109 Resp: 416880
Ion Ratio Lower Upper
109 100
139 147.9 120.8 181.2
65 129.9 107.9 161.9



#56
Dibenzofuran
Concen: 19.768 ng/ul
RT: 15.010 min Scan# 2010
Delta R.T. -0.000 min
Lab File: BP013058.D
Acq: 11 Dec 2022 01:32

Tgt Ion:168 Resp: 3804695
Ion Ratio Lower Upper
168 100
139 34.1 27.9 41.9

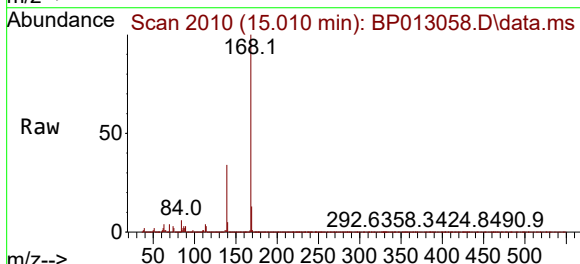



#57

2,4-Dinitrotoluene

Concen: 20.767 ng/ul

RT: 14.969 min Scan# 2003

Delta R.T. -0.006 min

Lab File: BP013058.D

Acq: 11 Dec 2022 01:32

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:165 Resp: 918772

Ion Ratio Lower Upper

165 100

63 40.3 31.8 47.6

182 2.8 2.1 3.1



#58

2,3,4,6-Tetrachlorophenol

Concen: 20.006 ng/ul

RT: 15.234 min Scan# 2048

Delta R.T. -0.000 min

Lab File: BP013058.D

Acq: 11 Dec 2022 01:32

Tgt Ion:232 Resp: 873150




Ion Ratio Lower Upper


232 100

131 37.2 31.8 47.6

130 1.8 1.8 2.6#

166 27.2 22.9 34.3


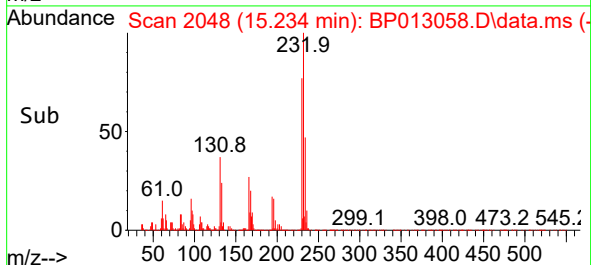
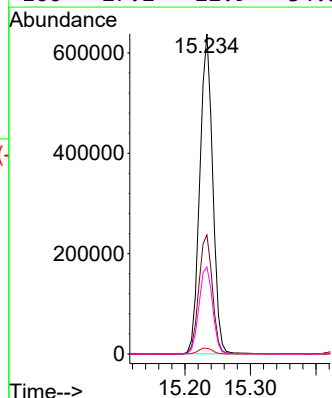
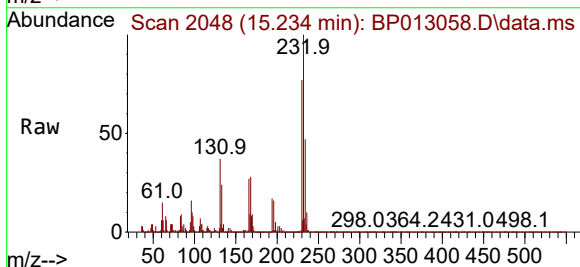




#59
Diethylphthalate
Concen: 19.557 ng/ul
RT: 15.428 min Scan# 2081
Delta R.T. -0.000 min
Lab File: BP013058.D
Acq: 11 Dec 2022 01:32




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:149 Resp: 3115875
Ion Ratio Lower Upper
149 100
177 23.4 18.4 27.6
150 12.5 9.9 14.9



#61
Fluorene
Concen: 20.097 ng/ul
RT: 15.657 min Scan# 2120
Delta R.T. -0.000 min
Lab File: BP013058.D
Acq: 11 Dec 2022 01:32

Tgt Ion:166 Resp: 3102020
Ion Ratio Lower Upper
166 100
165 96.1 77.4 116.2
167 13.7 10.6 16.0







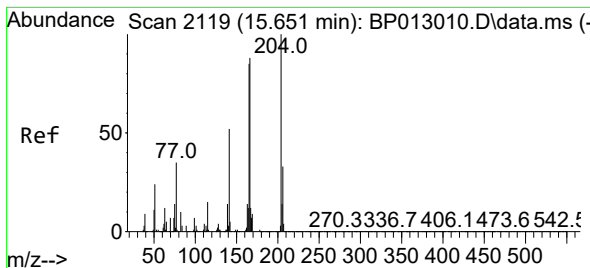

#62
4-Chlorophenyl-phenylether
Concen: 19.940 ng/ul
RT: 15.651 min Scan# 2119
Delta R.T. -0.000 min
Lab File: BP013058.D
Acq: 11 Dec 2022 01:32




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:204 Resp: 1627669
Ion Ratio Lower Upper
204 100
206 33.4 26.3 39.5
141 50.8 40.4 60.6

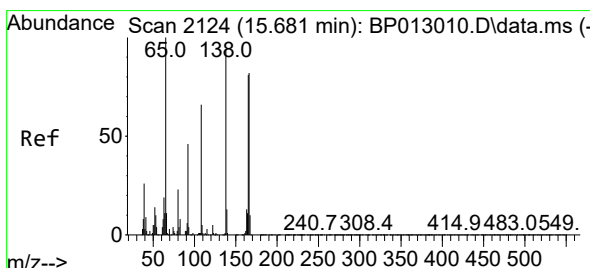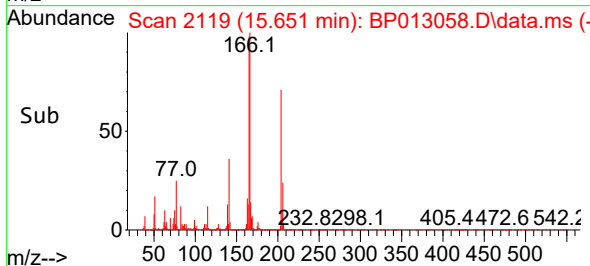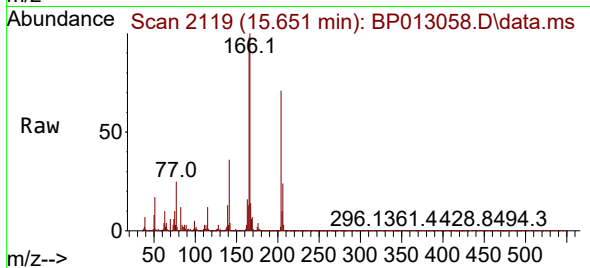

#63
4-Nitroaniline
Concen: 20.263 ng/ul
RT: 15.681 min Scan# 2124
Delta R.T. -0.000 min
Lab File: BP013058.D
Acq: 11 Dec 2022 01:32

Tgt Ion:138 Resp: 512792
Ion Ratio Lower Upper
138 100
92 48.6 39.0 58.4
108 72.8 55.1 82.7


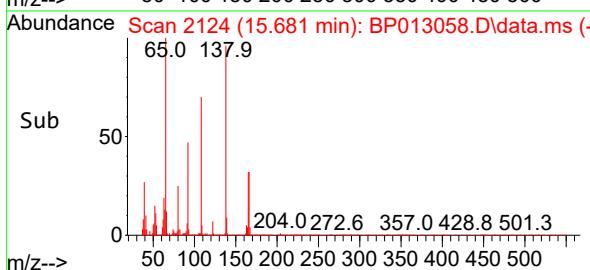

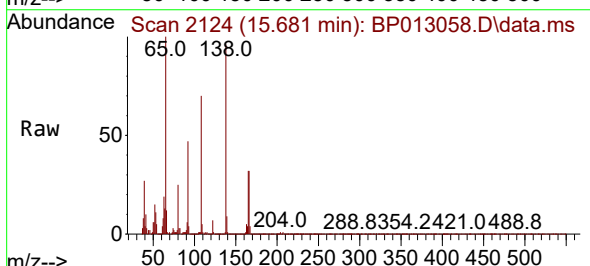




#66
4,6-Dinitro-2-methylphenol
Concen: 19.057 ng/ul
RT: 15.739 min Scan# 2134
Delta R.T. 0.006 min
Lab File: BP013058.D
Acq: 11 Dec 2022 01:32




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:198 Resp: 575163
Ion Ratio Lower Upper
198 100
182 4.1 3.3 4.9
77 20.4 16.6 25.0



#67
N-Nitrosodiphenylamine
Concen: 20.014 ng/ul
RT: 15.863 min Scan# 2155
Delta R.T. -0.006 min
Lab File: BP013058.D
Acq: 11 Dec 2022 01:32

Tgt Ion:169 Resp: 2662951
Ion Ratio Lower Upper
169 100
168 66.3 53.0 79.6
167 36.7 29.1 43.7









#68
4-Bromophenyl-phenylether
Concen: 18.506 ng/ul
RT: 16.545 min Scan# 21
Delta R.T. -0.006 min
Lab File: BP013058.D
Acq: 11 Dec 2022 01:32




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:248 Resp: 964516
Ion Ratio Lower Upper
248 100
250 98.9 77.4 116.0
141 64.7 48.3 72.5



#69
Hexachlorobenzene
Concen: 19.676 ng/ul
RT: 16.663 min Scan# 2291
Delta R.T. -0.006 min
Lab File: BP013058.D
Acq: 11 Dec 2022 01:32

Tgt Ion:284 Resp: 1217639
Ion Ratio Lower Upper
284 100
142 31.1 22.6 34.0
249 30.4 24.6 37.0





#70

Atrazine

Concen: 19.856 ng/ul

RT: 16.822 min Scan# 21

Delta R.T. -0.000 min

Lab File: BP013058.D

Acq: 11 Dec 2022 01:32

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:200 Resp: 1029523

Ion Ratio Lower Upper

200 100

173 24.2 20.5 30.7

215 49.7 39.9 59.9



#71

Pentachlorophenol

Concen: 19.101 ng/ul

RT: 17.010 min Scan# 2350

Delta R.T. -0.000 min

Lab File: BP013058.D

Acq: 11 Dec 2022 01:32




Tgt Ion:266 Resp: 715873


Ion Ratio Lower Upper

266 100

264 64.1 50.9 76.3

268 65.3 51.4 77.2

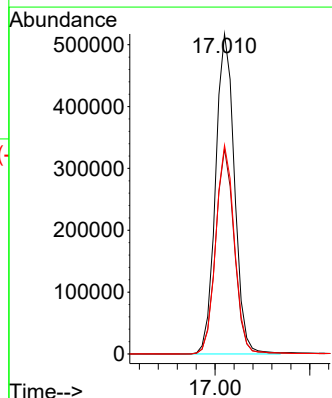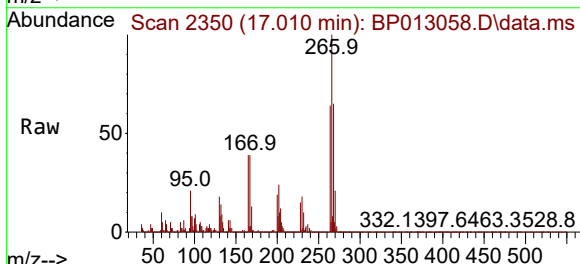



#72

Phenanthrene

Concen: 20.027 ng/ul

RT: 17.410 min Scan# 2419

Delta R.T. -0.000 min

Lab File: BP013058.D

Acq: 11 Dec 2022 01:32

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:178 Resp: 5006187

Ion Ratio Lower Upper

178 100

179 15.3 12.5 18.7

176 19.0 15.4 23.0



#74

Anthracene

Concen: 20.253 ng/ul

RT: 17.498 min Scan# 2433

Delta R.T. -0.006 min

Lab File: BP013058.D

Acq: 11 Dec 2022 01:32




Tgt Ion:178 Resp: 5055009


Ion Ratio Lower Upper

178 100

179 15.8 12.5 18.7

176 18.8 14.8 22.2




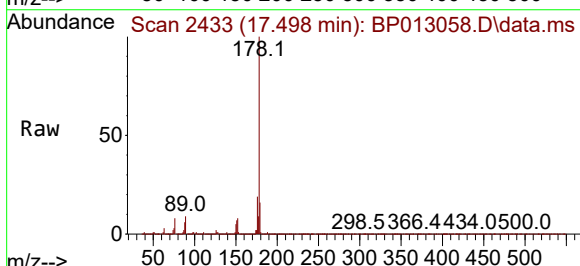




#75
1,2,3,4-Tetrachlorobenzene
Concen: 19.956 ng/uL
RT: 13.410 min Scan# 1739
Delta R.T. -0.000 min
Lab File: BP013058.D
Acq: 11 Dec 2022 01:32




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:216 Resp: 1366404
Ion Ratio Lower Upper
216 100
214 78.5 62.2 93.2
218 48.9 38.9 58.3

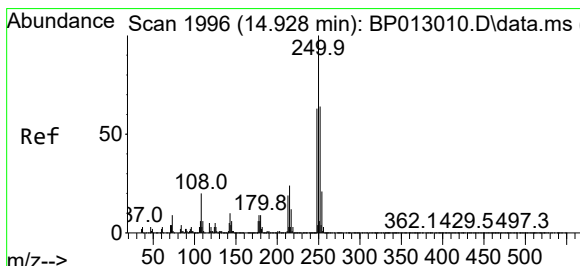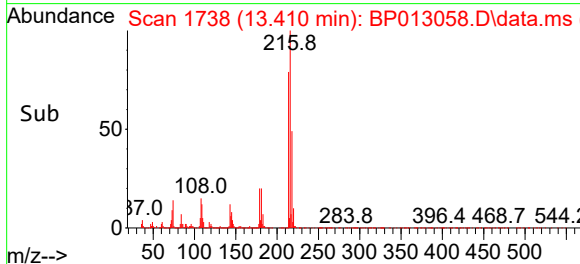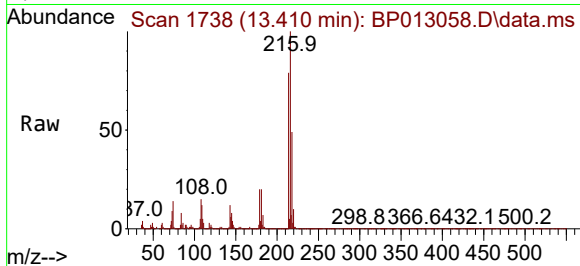

#76
Pentachlorobenzene
Concen: 19.763 ng/uL
RT: 14.928 min Scan# 1996
Delta R.T. -0.000 min
Lab File: BP013058.D
Acq: 11 Dec 2022 01:32

Tgt Ion:250 Resp: 1379624
Ion Ratio Lower Upper
250 100
248 63.1 50.6 76.0
252 63.8 51.1 76.7

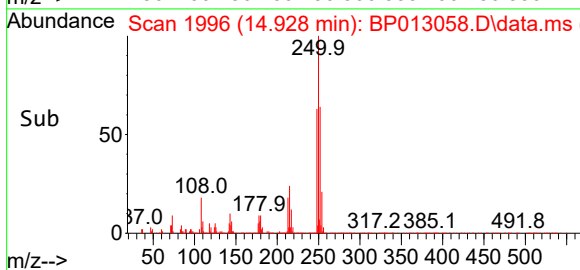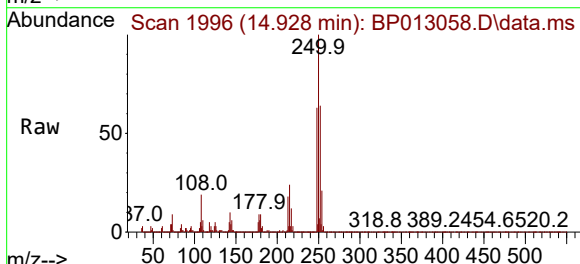



#77

Carbazole

Concen: 21.491 ng/ul

RT: 17.769 min Scan# 2480

Delta R.T. -0.000 min

Lab File: BP013058.D

Acq: 11 Dec 2022 01:32

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:167 Resp: 4517328

Ion Ratio Lower Upper

167 100

166 21.5 17.2 25.8

139 12.2 9.4 14.2



#78

Di-n-butylphthalate

Concen: 21.264 ng/ul

RT: 18.310 min Scan# 2571

Delta R.T. -0.000 min

Lab File: BP013058.D

Acq: 11 Dec 2022 01:32




Tgt Ion:149 Resp: 5442287


Ion Ratio Lower Upper

149 100

150 9.3 7.5 11.3

104 4.7 3.8 5.6

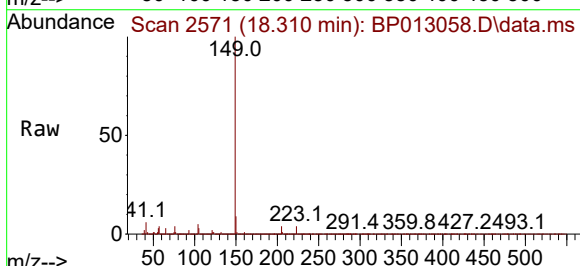



#80

Fluoranthene

Concen: 20.855 ng/ul

RT: 19.369 min Scan# 21

Delta R.T. -0.000 min

Lab File: BP013058.D

Acq: 11 Dec 2022 01:32

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:202 Resp: 5961509

Ion Ratio Lower Upper

202 100

101 10.1 8.2 12.2

100 7.7 6.1 9.1

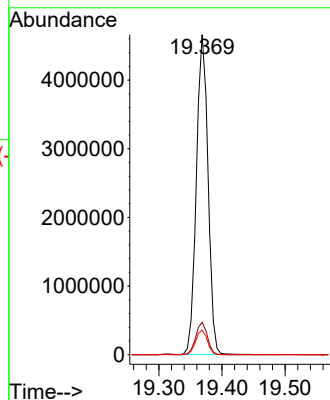

#82

Pyrene

Concen: 20.887 ng/ul

RT: 19.721 min Scan# 2811

Delta R.T. -0.006 min

Lab File: BP013058.D

Acq: 11 Dec 2022 01:32




Tgt Ion:202 Resp: 6158908


Ion Ratio Lower Upper

202 100

101 12.2 9.4 14.2

100 9.9 7.8 11.8

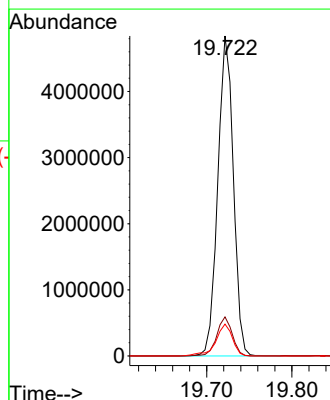

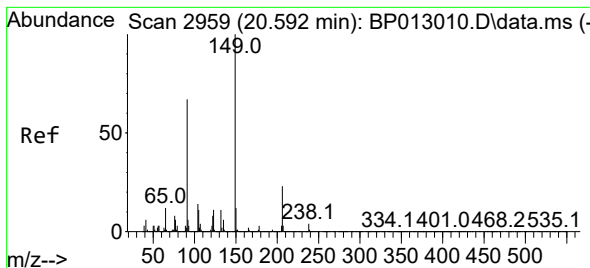

#83

Butylbenzylphthalate

Concen: 21.296 ng/ul

RT: 20.586 min Scan# 2958

Delta R.T. -0.000 min

Lab File: BP013058.D

Acq: 11 Dec 2022 01:32

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:149 Resp: 2425875

Ion Ratio Lower Upper

149 100

91 65.9 53.4 80.0

206 22.7 17.9 26.9

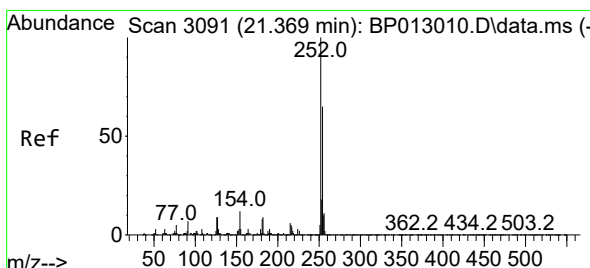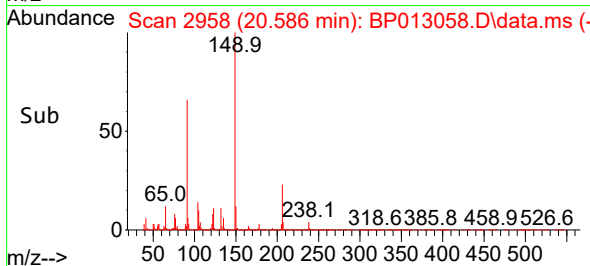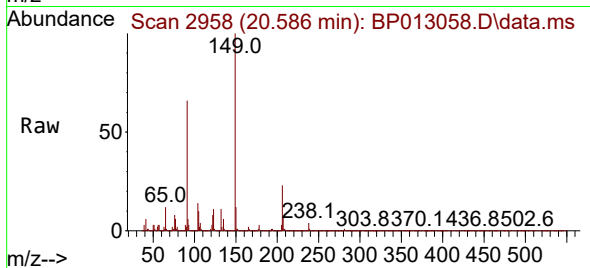

#84

3,3'-Dichlorobenzidine

Concen: 17.449 ng/ul

RT: 21.363 min Scan# 3090

Delta R.T. -0.000 min

Lab File: BP013058.D

Acq: 11 Dec 2022 01:32




Tgt Ion:252 Resp: 1729545


Ion Ratio Lower Upper

252 100

254 65.1 51.8 77.8

126 9.5 7.4 11.2


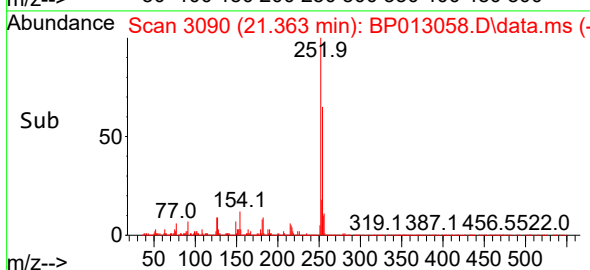

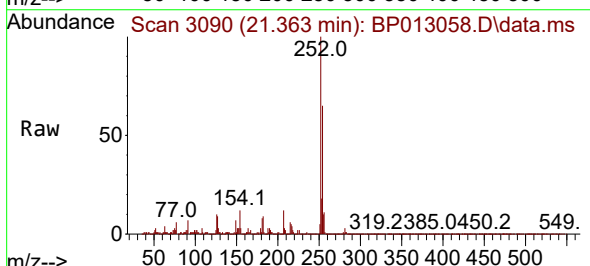




#85
Benzo(a)anthracene
Concen: 20.283 ng/ul
RT: 21.433 min Scan# 3103
Delta R.T. -0.000 min
Lab File: BP013058.D
Acq: 11 Dec 2022 01:32




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:228 Resp: 5907857
Ion Ratio Lower Upper
228 100
229 20.0 16.1 24.1
226 27.4 22.0 33.0



#86
Bis(2-ethylhexyl)phthalate
Concen: 21.887 ng/ul
RT: 21.345 min Scan# 3087
Delta R.T. -0.000 min
Lab File: BP013058.D
Acq: 11 Dec 2022 01:32

Tgt Ion:149 Resp: 3516940
Ion Ratio Lower Upper
149 100
167 28.9 22.5 33.7
279 5.1 3.8 5.8





#87

Chrysene

Concen: 20.018 ng/ul

RT: 21.492 min Scan# 3113

Delta R.T. -0.000 min

Lab File: BP013058.D

Acq: 11 Dec 2022 01:32

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:228 Resp: 5513927

Ion Ratio Lower Upper

228 100

226 30.6 24.5 36.7

229 19.8 16.0 24.0

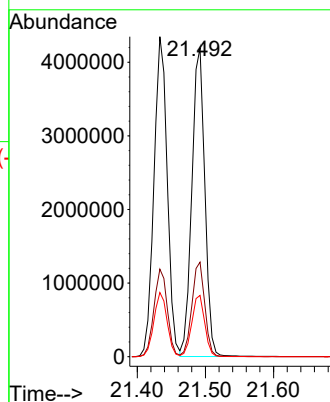

#89

Di-n-octyl phthalate

Concen: 24.201 ng/ul




RT: 22.298 min Scan# 3249


Delta R.T. -0.000 min

Lab File: BP013058.D

Acq: 11 Dec 2022 01:32


Tgt Ion:149 Resp: 5790764

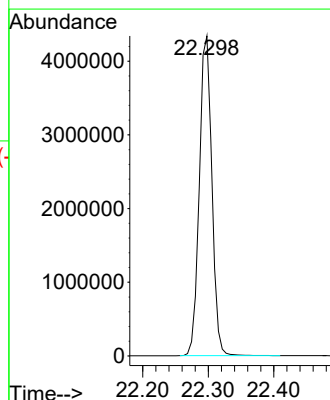






#90
Benzo(b)fluoranthene
Concen: 20.343 ng/ul
RT: 23.174 min Scan# 31
Delta R.T. -0.000 min
Lab File: BP013058.D
Acq: 11 Dec 2022 01:32

Instrument :
BNA_P
ClientSampleId :







Tgt Ion:252 Resp: 5540524
Ion Ratio Lower Upper
252 100
253 22.2 17.7 26.5
125 8.8 6.8 10.2

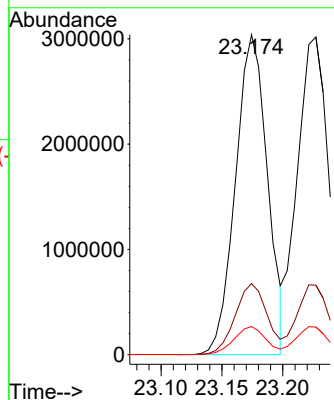

#91
Benzo(k)fluoranthene
Concen: 20.369 ng/ul
RT: 23.227 min Scan# 3407
Delta R.T. -0.000 min
Lab File: BP013058.D
Acq: 11 Dec 2022 01:32

Tgt Ion:252 Resp: 5500904
Ion Ratio Lower Upper
252 100
253 21.8 17.7 26.5
125 8.7 6.8 10.2

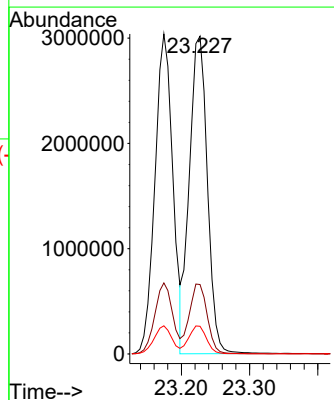



#93

Benzo(a)pyrene

Concen: 19.888 ng/ul

RT: 23.827 min Scan# 3

Delta R.T. -0.006 min

Lab File: BP013058.D

Acq: 11 Dec 2022 01:32

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:252 Resp: 4716349

Ion Ratio Lower Upper

252 100

253 22.0 17.5 26.3

125 9.9 7.5 11.3



#94

Indeno(1,2,3-cd)pyrene

Concen: 18.682 ng/ul

RT: 26.539 min Scan# 3970

Delta R.T. -0.006 min

Lab File: BP013058.D

Acq: 11 Dec 2022 01:32




Tgt Ion:276 Resp: 5518444


Ion Ratio Lower Upper

276 100

138 20.9 17.1 25.7


277 24.9 20.0 30.0

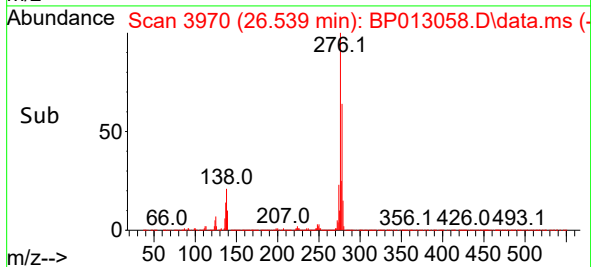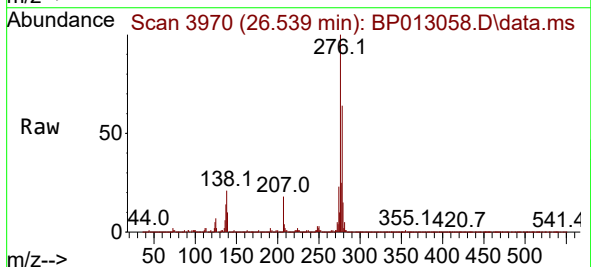






#95
Dibenzo(a,h)anthracene
Concen: 18.813 ng/ul
RT: 26.556 min Scan# 3975
Delta R.T. -0.000 min
Lab File: BP013058.D
Acq: 11 Dec 2022 01:32

Instrument :
BNA_P
ClientSampleId :



Tgt Ion:278 Resp: 4601015
Ion Ratio Lower Upper
278 100
139 13.6 11.1 16.7
279 23.8 19.0 28.6



#96
Benzo(g,h,i)perylene
Concen: 17.692 ng/ul
RT: 27.339 min Scan# 4106
Delta R.T. -0.006 min
Lab File: BP013058.D
Acq: 11 Dec 2022 01:32

Tgt Ion:276 Resp: 4195499
Ion Ratio Lower Upper
276 100
138 18.7 15.4 23.2
277 24.4 19.1 28.7

