

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP121022\  
 Data File : BP013068.D  
 Acq On : 11 Dec 2022 07:47  
 Operator : CG/JU  
 Sample : N5927-15  
 Misc :  
 ALS Vial : 39 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :

Quant Time: Dec 12 03:32:41 2022  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\SFAM-EPA-BP120722.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Mon Dec 12 01:32:54 2022  
 Response via : Initial Calibration


| Compound                      | R.T.   | QIon | Response | Conc   | Units  | Dev(Min) |
|-------------------------------|--------|------|----------|--------|--------|----------|
| -----                         |        |      |          |        |        |          |
| Internal Standards            |        |      |          |        |        |          |
| 1) 1,4-Dichlorobenzene-d4     | 7.969  | 152  | 455173   | 20.000 | ng/ul  | 0.00     |
| 20) Naphthalene-d8            | 10.781 | 136  | 1995441  | 20.000 | ng/ul  | 0.00     |
| 38) Acenaphthene-d10          | 14.610 | 164  | 1352599  | 20.000 | ng/ul  | 0.00     |
| 64) Phenanthrene-d10          | 17.363 | 188  | 3199885  | 20.000 | ng/ul  | 0.00     |
| 79) Chrysene-d12              | 21.445 | 240  | 3226739  | 20.000 | ng/ul  | 0.00     |
| 88) Perylene-d12              | 23.933 | 264  | 3502483  | 20.000 | ng/ul  | 0.00     |
|                               |        |      |          |        |        |          |
| System Monitoring Compounds   |        |      |          |        |        |          |
| 3) 1,4-Dioxane-d8             | 3.352  | 96   | 52876    | 4.967  | ng/uL  | 0.00     |
| 4) Pyridine-d5                | 3.781  | 84   | 284818   | 9.418  | ng/ul  | 0.00     |
| 7) Phenol-d5                  | 7.122  | 99   | 312573   | 8.431  | ng/ul  | 0.00     |
| 9) Bis-(2-Chloroethyl)eth...  | 7.293  | 67   | 919339   | 41.106 | ng/ul  | 0.00     |
| 11) 2-Chlorophenol-d4         | 7.493  | 132  | 937989   | 32.139 | ng/ul  | 0.00     |
| 15) 4-Methylphenol-d8         | 8.675  | 113  | 614081   | 20.215 | ng/ul  | 0.00     |
| 21) Nitrobenzene-d5           | 9.134  | 128  | 605237   | 41.282 | ng/ul  | 0.00     |
| 24) 2-Nitrophenol-d4          | 9.863  | 143  | 680476   | 41.227 | ng/ul  | 0.00     |
| 28) 2,4-Dichlorophenol-d3     | 10.399 | 165  | 1201024  | 37.462 | ng/ul  | 0.00     |
| 31) 4-Chloroaniline-d4        | 10.916 | 131  | 1351000  | 29.850 | ng/ul  | 0.00     |
| 46) Dimethylphthalate-d6      | 14.016 | 166  | 4414629  | 42.467 | ng/ul  | 0.00     |
| 49) Acenaphthylene-d8         | 14.304 | 160  | 4793682  | 41.966 | ng/ul  | 0.00     |
| 54) 4-Nitrophenol-d4          | 14.798 | 143  | 120291   | 6.433  | ng/ul  | 0.00     |
| 60) Fluorene-d10              | 15.598 | 176  | 3847240  | 43.746 | ng/ul  | 0.00     |
| 65) 4,6-Dinitro-2-methylph... | 15.716 | 200  | 704726   | 34.223 | ng/ul  | 0.00     |
| 73) Anthracene-d10            | 17.463 | 188  | 6349319  | 43.982 | ng/ul  | 0.00     |
| 81) Pyrene-d10                | 19.692 | 212  | 7824698  | 42.247 | ng/ul  | 0.00     |
| 92) Benzo(a)pyrene-d12        | 23.774 | 264  | 7798949  | 44.673 | ng/ul  | 0.00     |
|                               |        |      |          |        |        |          |
| Target Compounds              |        |      |          |        |        |          |
| 2) 1,4-Dioxane                | 3.387  | 88   | 13482    | 1.213  | ng/uL# | 87       |
| 59) Diethylphthalate          | 15.422 | 149  | 117756   | 1.176  | ng/ul  | 99       |
| -----                         |        |      |          |        |        |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP121022\  
Data File : BP013068.D  
Acq On : 11 Dec 2022 07:47  
Operator : CG/JU  
Sample : N5927-15  
Misc :  
ALS Vial : 39 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :

Quant Time: Dec 12 03:32:41 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\SFAM-EPA-BP120722.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Mon Dec 12 01:32:54 2022  
Response via : Initial Calibration




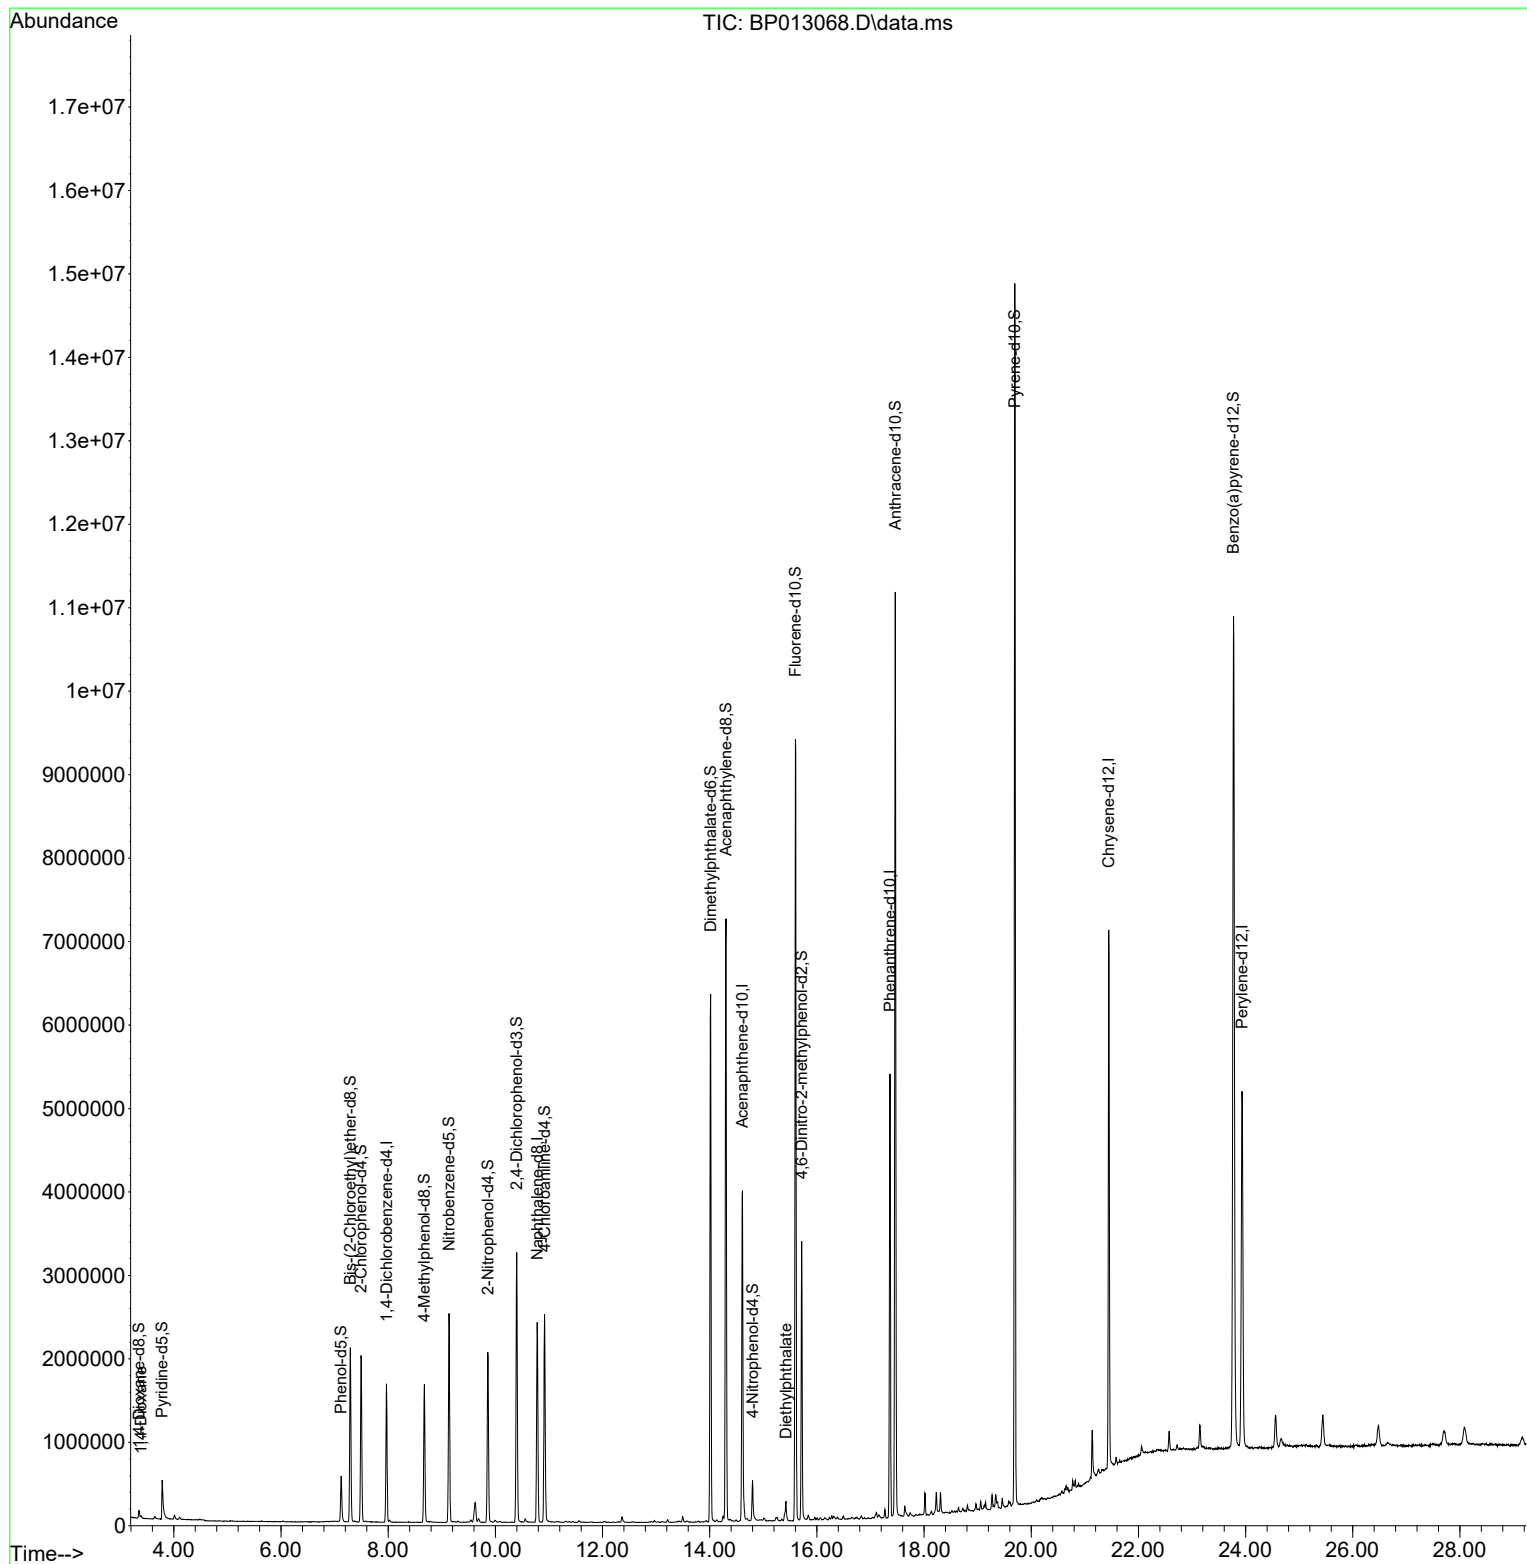


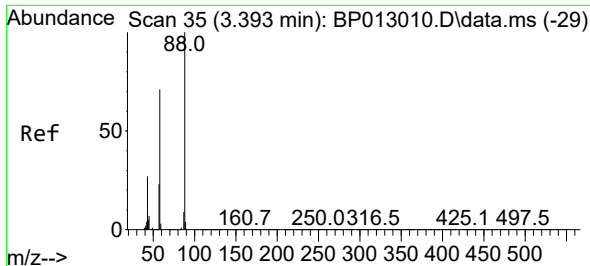

#2  
1,4-Dioxane  
Concen: 1.213 ng/uL  
RT: 3.387 min Scan# 34  
Delta R.T. 0.000 min  
Lab File: BP013068.D  
Acq: 11 Dec 2022 07:47

Instrument :  
BNA\_P  
ClientSampleId :

Tgt Ion: 88 Resp: 13482  
Ion Ratio Lower Upper  
88 100  
43 38.8 22.4 33.6#  
58 64.8 58.2 87.4

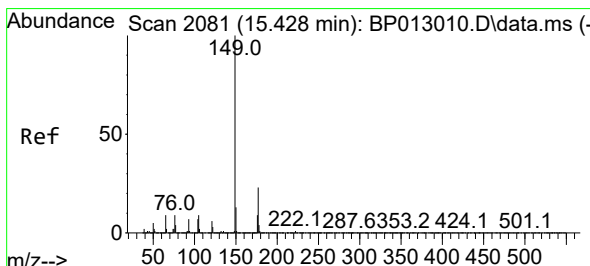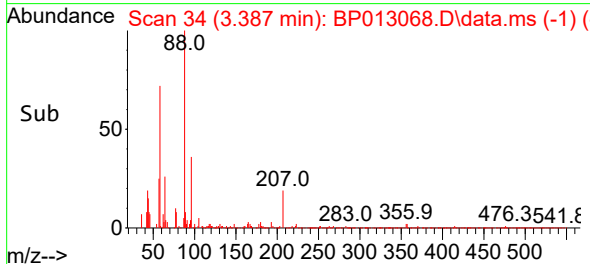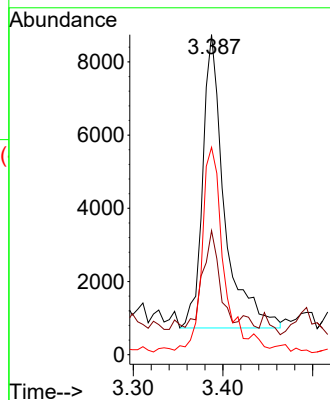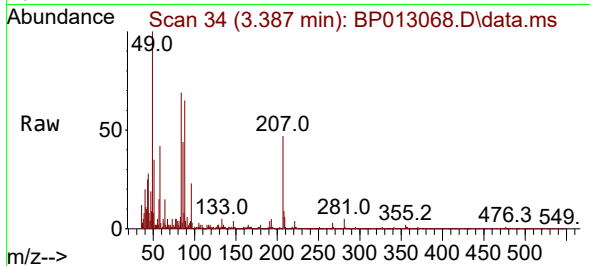

#59  
Diethylphthalate  
Concen: 1.176 ng/uL  
RT: 15.422 min Scan# 2080  
Delta R.T. -0.006 min  
Lab File: BP013068.D  
Acq: 11 Dec 2022 07:47

Tgt Ion: 149 Resp: 117756  
Ion Ratio Lower Upper  
149 100  
177 24.0 18.4 27.6  
150 12.6 9.9 14.9

