




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
 Data File : BP013066.D
 Acq On : 11 Dec 2022 06:39
 Operator : CG/JU
 Sample : N5927-09
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXZ97

Manual IntegrationsAPPROVED

Quant Time: Dec 12 03:32:20 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Dec 12 01:32:54 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/12/2022
 Supervised By :mohammad ahmed 12/12/2022

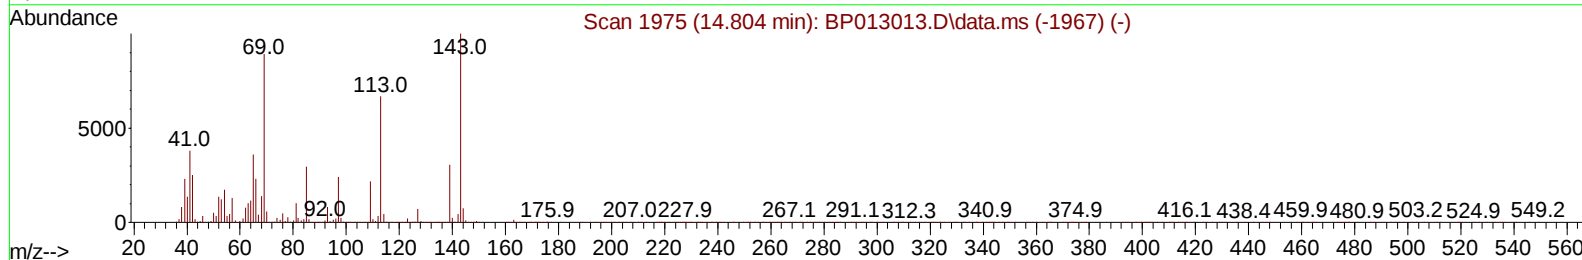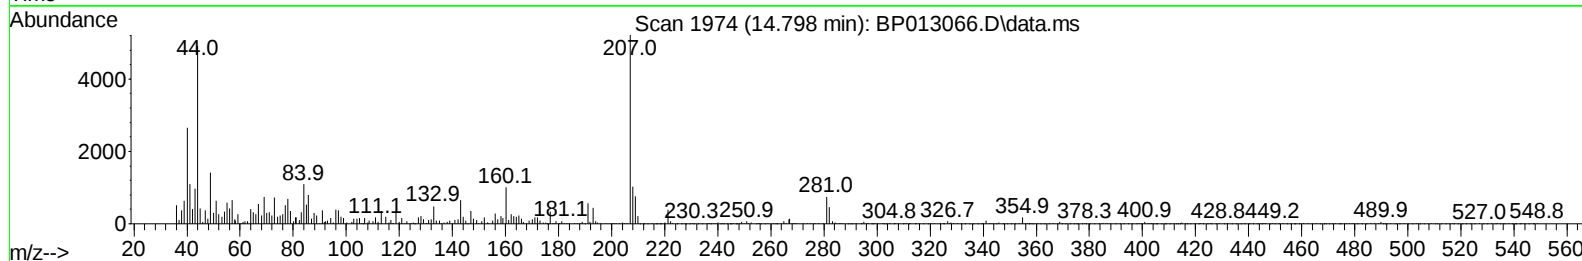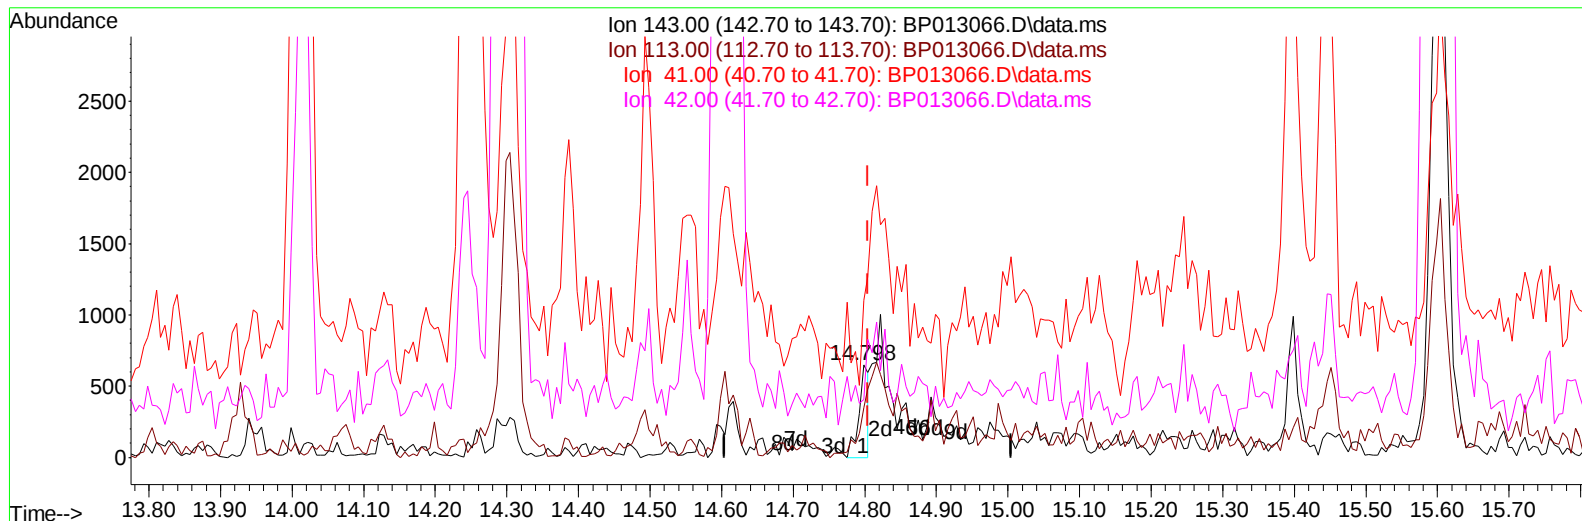

TIC: BP013066.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.798min (-0.006) 0.02 ng/u1

response 638

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	65.80	53.38
41.00	35.70	169.54#
42.00	24.70	62.62#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
 Data File : BP013066.D
 Acq On : 11 Dec 2022 06:39
 Operator : CG/JU
 Sample : N5927-09
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXZ97

Manual IntegrationsAPPROVED

Quant Time: Dec 12 03:32:20 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Dec 12 01:32:54 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/12/2022
 Supervised By :mohammad ahmed 12/12/2022

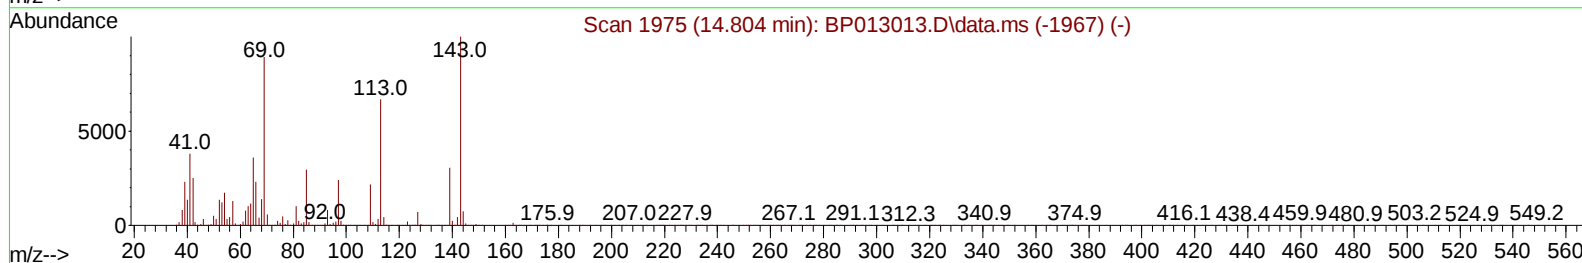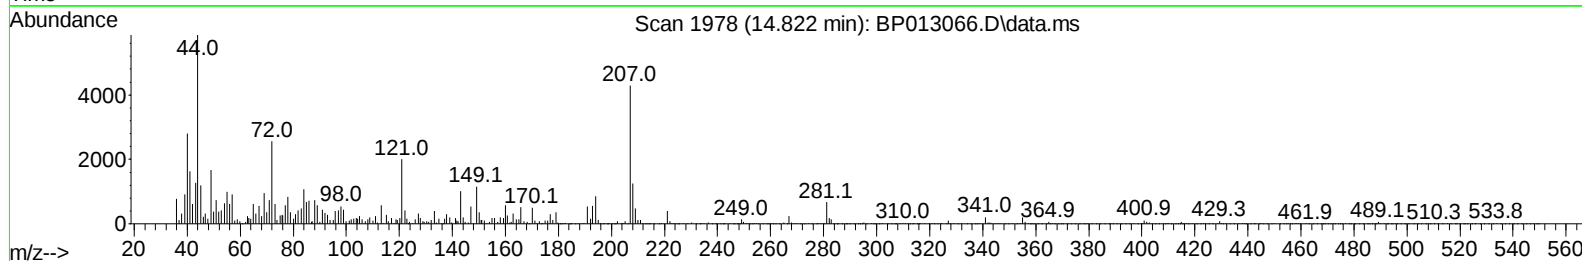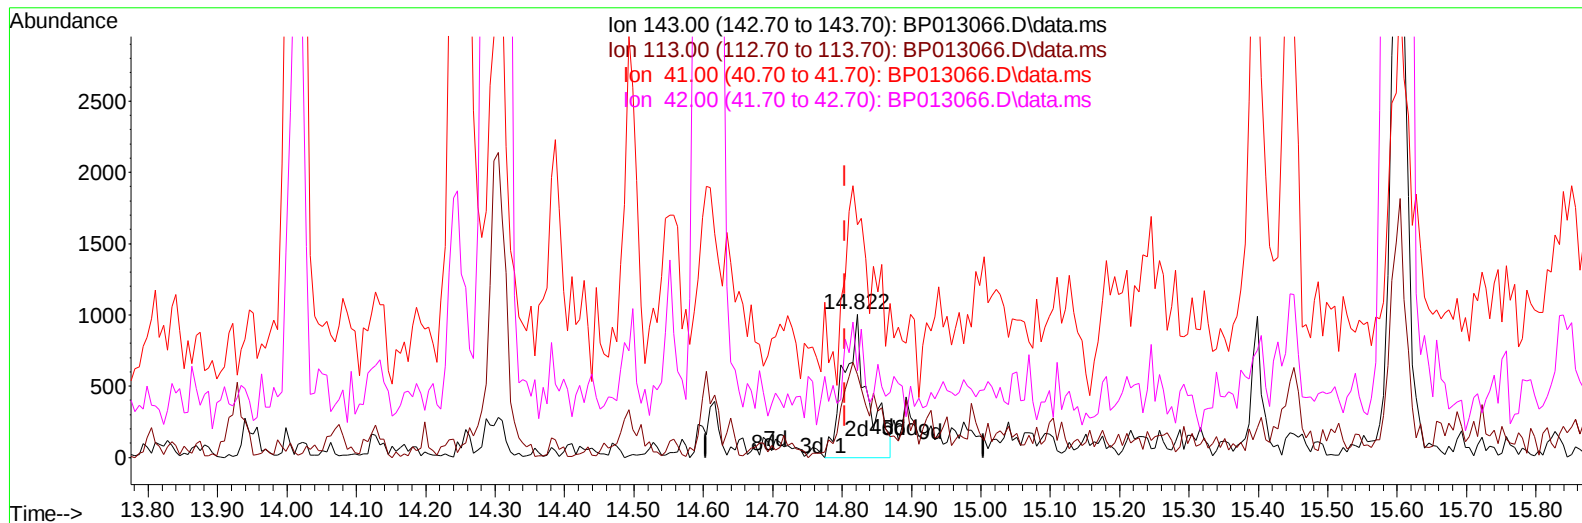

TIC: BP013066.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.822min (+ 0.018) 0.09 ng/ul m

response 2400

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	65.80	58.01
41.00	35.70	162.49#
42.00	24.70	60.60#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
Data File : BP013066.D
Acq On : 11 Dec 2022 06:39
Operator : CG/JU
Sample : N5927-09
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXZ97

Manual IntegrationsAPPROVED

Quant Time: Dec 12 03:32:20 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Dec 12 01:32:54 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/12/2022
Supervised By :mohammad ahmed 12/12/2022

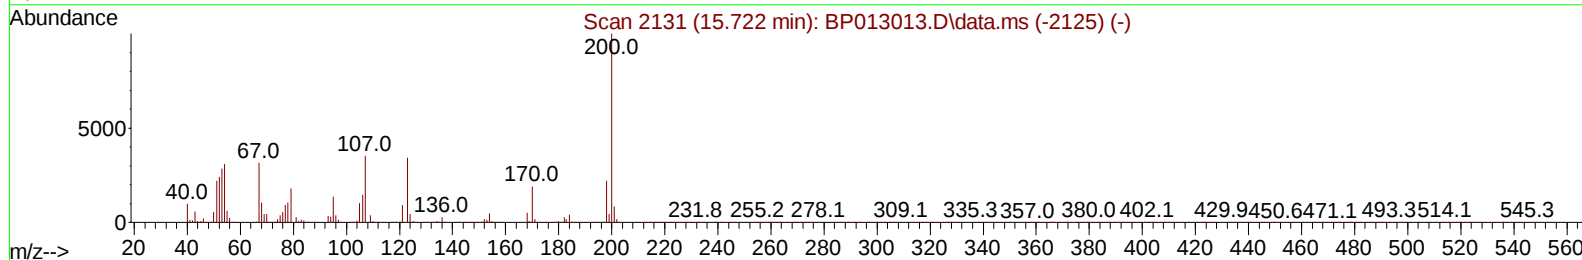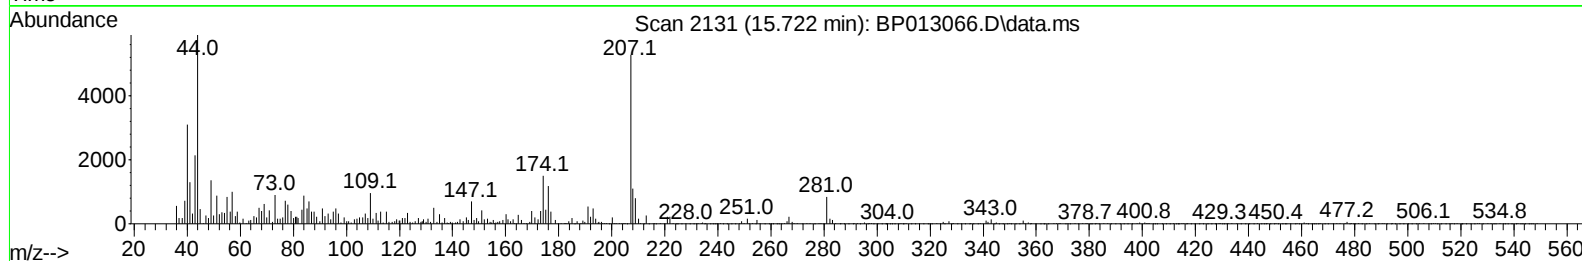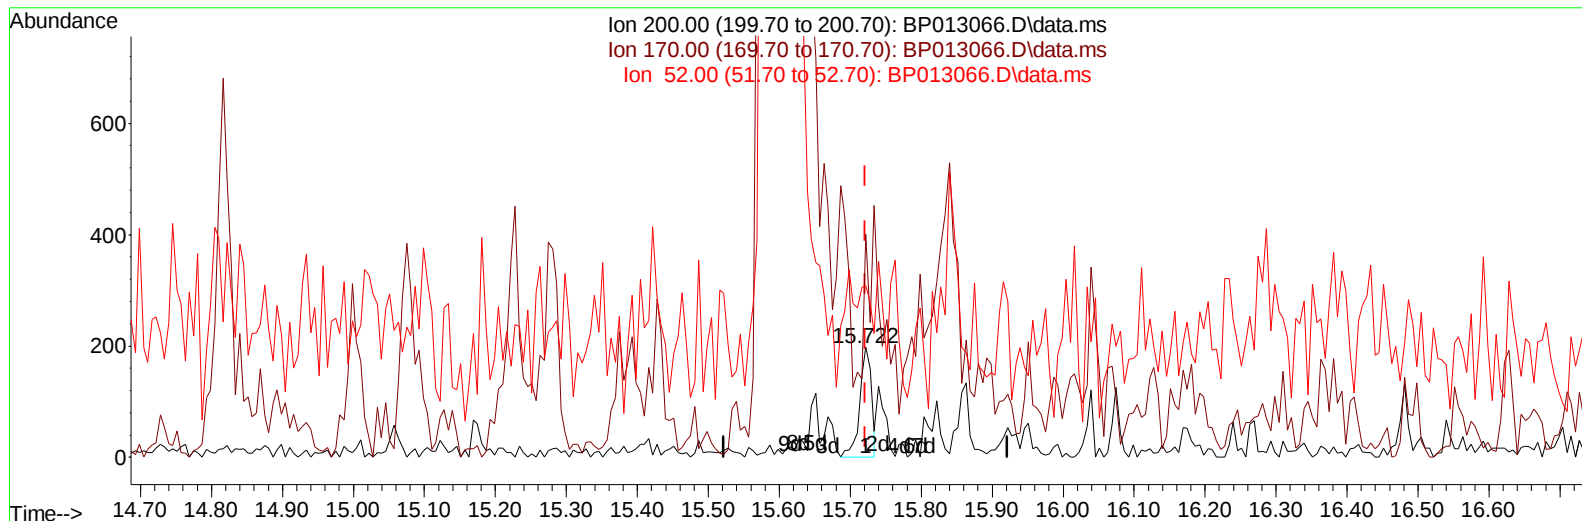

TIC: BP013066.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.722min (+ 0.000) 0.01 ng/u1

response 228

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	18.90	202.53#
52.00	37.00	156.06#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
 Data File : BP013066.D
 Acq On : 11 Dec 2022 06:39
 Operator : CG/JU
 Sample : N5927-09
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXZ97

Manual IntegrationsAPPROVED

Quant Time: Dec 12 03:32:20 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Dec 12 01:32:54 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/12/2022
 Supervised By :mohammad ahmed 12/12/2022

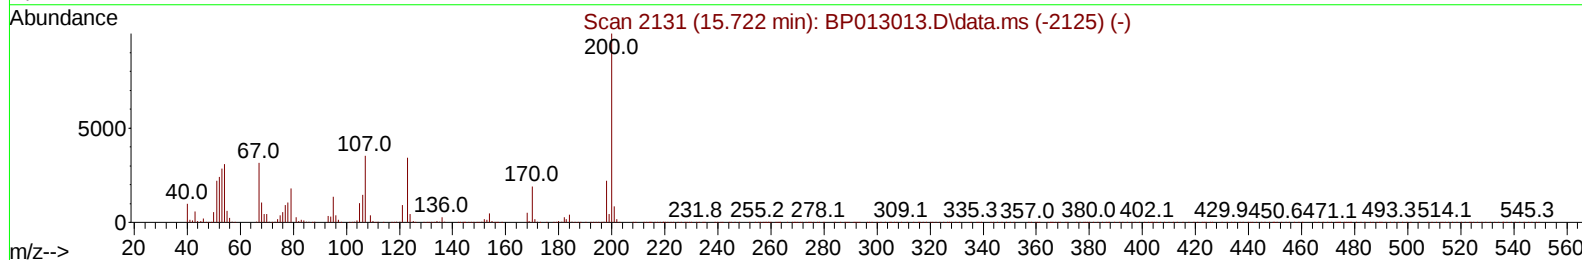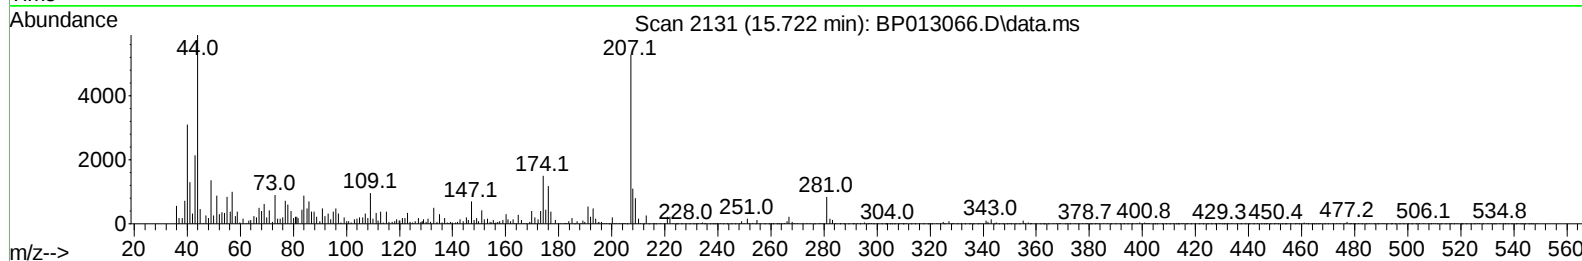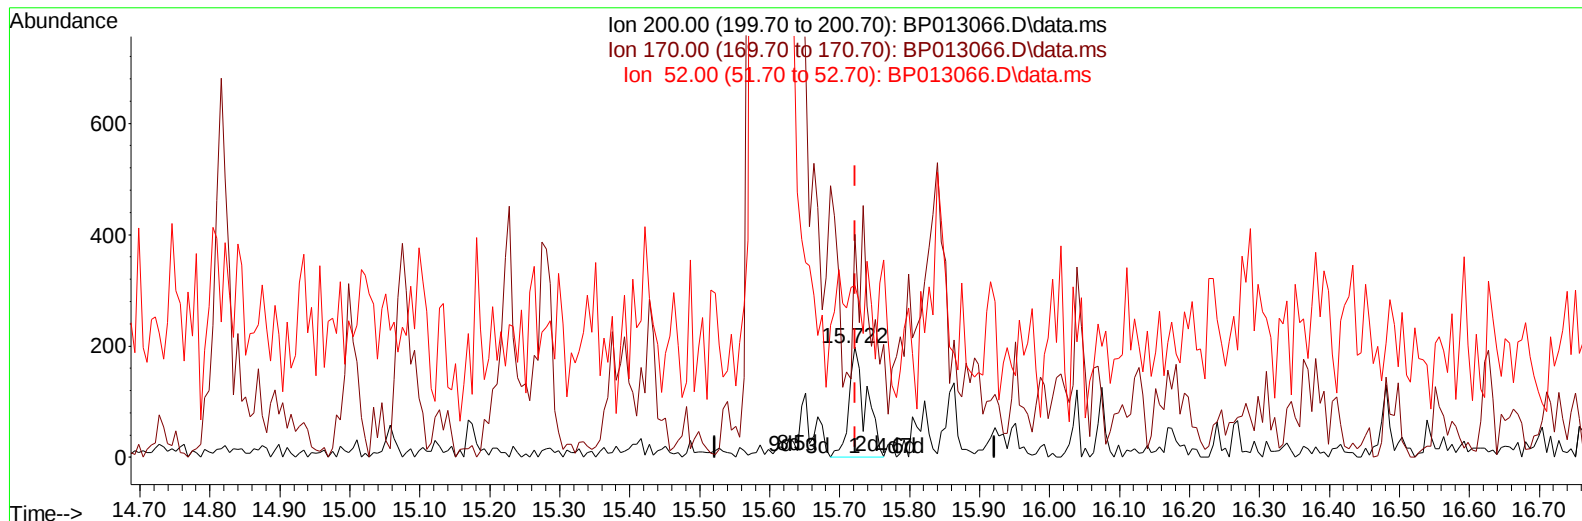

TIC: BP013066.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.722min (+ 0.000) 0.01 ng/ul m

response 335

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	18.90	202.53#
52.00	37.00	156.06#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
 Data File : BP013066.D
 Acq On : 11 Dec 2022 06:39
 Operator : CG/JU
 Sample : N5927-09
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXZ97

Manual IntegrationsAPPROVED

Quant Time: Dec 12 03:32:20 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Dec 12 01:32:54 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/12/2022
 Supervised By :mohammad ahmed 12/12/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.969	152	631320	20.000	ng/ul	0.00
20) Naphthalene-d8	10.781	136	2757183	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.610	164	1879409	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.363	188	4405576	20.000	ng/ul	0.00
79) Chrysene-d12	21.451	240	4200387	20.000	ng/ul	0.00
88) Perylene-d12	23.933	264	4347182	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.352	96	69379	4.699	ng/uL	0.00
4) Pyridine-d5	3.781	84	396701	9.458	ng/ul	0.00
7) Phenol-d5	7.122	99	46985	0.914	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.293	67	1074560	34.641	ng/ul	0.00
11) 2-Chlorophenol-d4	7.499	132	432432	10.683	ng/ul	0.00
15) 4-Methylphenol-d8	8.675	113	130318	3.093	ng/ul	0.00
21) Nitrobenzene-d5	9.134	128	711090	35.102	ng/ul	0.00
24) 2-Nitrophenol-d4	9.863	143	50428	2.211	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.399	165	503145	11.358	ng/ul	0.00
31) 4-Chloroaniline-d4	10.916	131	1702244	27.220	ng/ul	0.00
46) Dimethylphthalate-d6	14.016	166	4746707	32.863	ng/ul	0.00
49) Acenaphthylene-d8	14.304	160	5532127	34.855	ng/ul	0.00
54) 4-Nitrophenol-d4	14.822	143	2400m	0.092	ng/ul	0.02
60) Fluorene-d10	15.604	176	4330935	35.442	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.722	200	335m	0.012	ng/ul	0.00
73) Anthracene-d10	17.463	188	7005622	35.247	ng/ul	0.00
81) Pyrene-d10	19.692	212	8421305	34.928	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.774	264	7652945	35.319	ng/ul	0.00
Target Compounds						
2) 1,4-Dioxane	3.387	88	39839	2.585	ng/uL	Qvalue 93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
Data File : BP013066.D
Acq On : 11 Dec 2022 06:39
Operator : CG/JU
Sample : N5927-09
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXZ97

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 12/12/2022
Supervised By :mohammad ahmed 12/12/2022

Quant Time: Dec 12 03:32:20 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Dec 12 01:32:54 2022
Response via : Initial Calibration

