

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
 Data File : BP013062.D
 Acq On : 11 Dec 2022 04:23
 Operator : CG/JU
 Sample : N5927-19
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXZA4

Quant Time: Dec 12 03:31:37 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Dec 12 01:32:54 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.969	152	591366	20.000	ng/u1	0.00
20) Naphthalene-d8	10.781	136	2622942	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.610	164	1789854	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.363	188	4089515	20.000	ng/u1	0.00
79) Chrysene-d12	21.451	240	3745715	20.000	ng/u1	0.00
88) Perylene-d12	23.939	264	3744183	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.352	96	65504	4.736	ng/uL	0.00
4) Pyridine-d5	3.781	84	366917	9.339	ng/u1	0.00
7) Phenol-d5	7.122	99	358118	7.435	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.293	67	1060451	36.496	ng/u1	0.00
11) 2-Chlorophenol-d4	7.499	132	1059241	27.935	ng/u1	0.00
15) 4-Methylphenol-d8	8.675	113	712684	18.057	ng/u1	0.00
21) Nitrobenzene-d5	9.140	128	702333	36.444	ng/u1	0.00
24) 2-Nitrophenol-d4	9.863	143	778982	35.904	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.399	165	1377222	32.681	ng/u1	0.00
31) 4-Chloroaniline-d4	10.922	131	1552647	26.098	ng/u1	0.00
46) Dimethylphthalate-d6	14.016	166	5408292	39.316	ng/u1	0.00
49) Acenaphthylene-d8	14.304	160	5694234	37.672	ng/u1	0.00
54) 4-Nitrophenol-d4	14.798	143	150210	6.071	ng/u1	0.00
60) Fluorene-d10	15.604	176	4571404	39.282	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.716	200	917981	34.882	ng/u1	0.00
73) Anthracene-d10	17.463	188	7608079	41.237	ng/u1	0.00
81) Pyrene-d10	19.692	212	8896304	41.377	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.780	264	7875882	42.202	ng/u1	0.00


Target Compounds					Qvalue
2) 1,4-Dioxane	3.387	88	106603	7.383	ng/uL 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
Data File : BP013062.D
Acq On : 11 Dec 2022 04:23
Operator : CG/JU
Sample : N5927-19
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXZA4

Quant Time: Dec 12 03:31:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Dec 12 01:32:54 2022
Response via : Initial Calibration

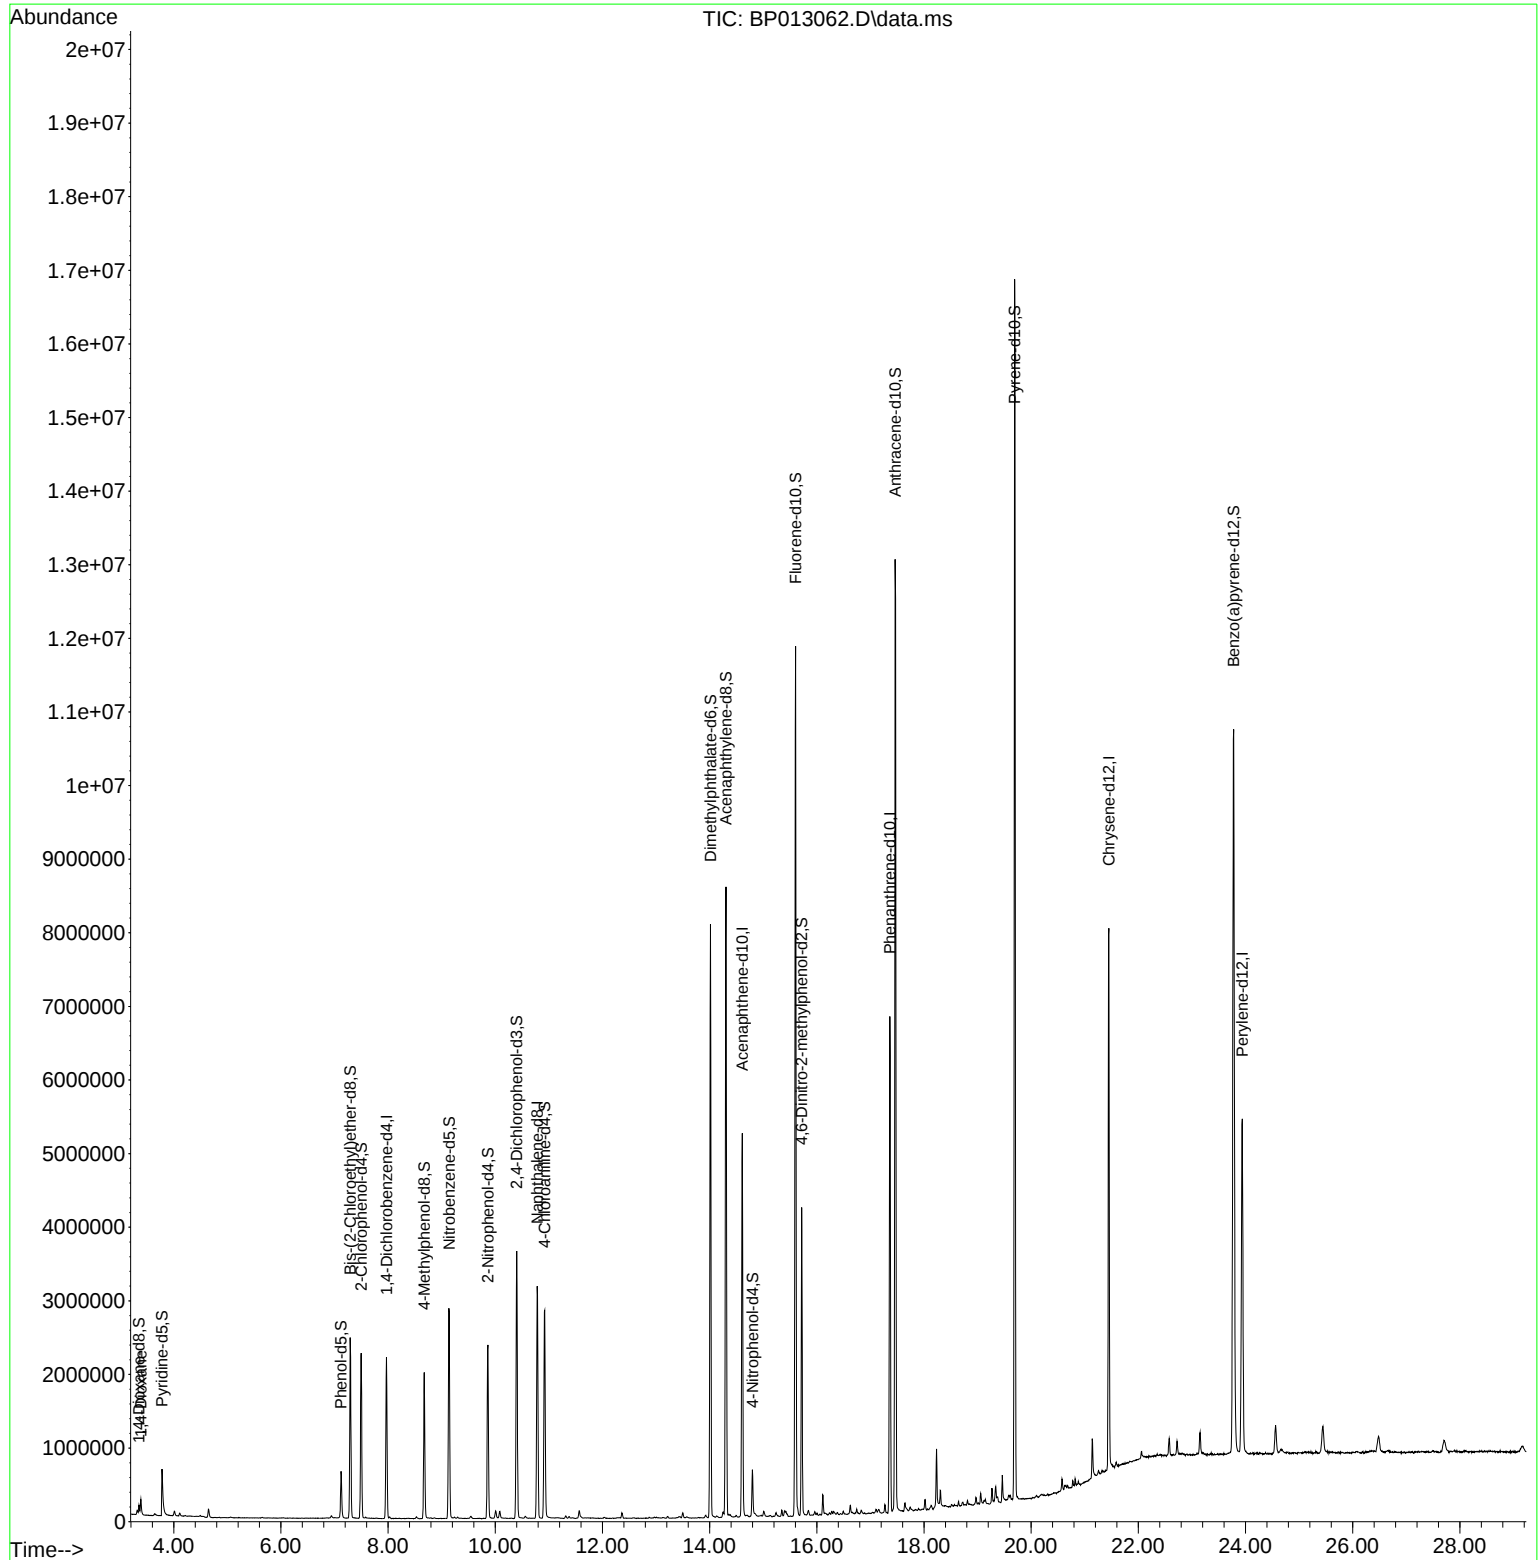

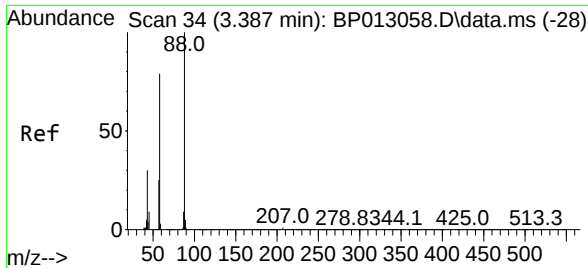

#2
 1,4-Dioxane
 Concen: 7.383 ng/uL
 RT: 3.387 min Scan# 34
 Delta R.T. -0.000 min
 Lab File: BP013062.D
 Acq: 11 Dec 2022 04:23

Instrument :
 BNA_P
 ClientSampleId :
 EXZA4

Tgt Ion: 88 Resp: 106603
 Ion Ratio Lower Upper
 88 100
 43 32.7 22.4 33.6
 58 78.6 58.2 87.4

