

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
 Data File : BP013068.D
 Acq On : 11 Dec 2022 07:47
 Operator : CG/JU
 Sample : N5927-15
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXZA2

Quant Time: Dec 12 03:32:41 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Dec 12 01:32:54 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.969	152	455173	20.000	ng/u1	0.00
20) Naphthalene-d8	10.781	136	1995441	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.610	164	1352599	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.363	188	3199885	20.000	ng/u1	0.00
79) Chrysene-d12	21.445	240	3226739	20.000	ng/u1	0.00
88) Perylene-d12	23.933	264	3502483	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.352	96	52876	4.967	ng/uL	0.00
4) Pyridine-d5	3.781	84	284818	9.418	ng/u1	0.00
7) Phenol-d5	7.122	99	312573	8.431	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.293	67	919339	41.106	ng/u1	0.00
11) 2-Chlorophenol-d4	7.493	132	937989	32.139	ng/u1	0.00
15) 4-Methylphenol-d8	8.675	113	614081	20.215	ng/u1	0.00
21) Nitrobenzene-d5	9.134	128	605237	41.282	ng/u1	0.00
24) 2-Nitrophenol-d4	9.863	143	680476	41.227	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.399	165	1201024	37.462	ng/u1	0.00
31) 4-Chloroaniline-d4	10.916	131	1351000	29.850	ng/u1	0.00
46) Dimethylphthalate-d6	14.016	166	4414629	42.467	ng/u1	0.00
49) Acenaphthylene-d8	14.304	160	4793682	41.966	ng/u1	0.00
54) 4-Nitrophenol-d4	14.798	143	120291	6.433	ng/u1	0.00
60) Fluorene-d10	15.598	176	3847240	43.746	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.716	200	704726	34.223	ng/u1	0.00
73) Anthracene-d10	17.463	188	6349319	43.982	ng/u1	0.00
81) Pyrene-d10	19.692	212	7824698	42.247	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.774	264	7798949	44.673	ng/u1	0.00


Target Compounds					Qvalue	
2) 1,4-Dioxane	3.387	88	13482	1.213	ng/uL#	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
Data File : BP013068.D
Acq On : 11 Dec 2022 07:47
Operator : CG/JU
Sample : N5927-15
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXZA2

Quant Time: Dec 12 03:32:41 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Dec 12 01:32:54 2022
Response via : Initial Calibration

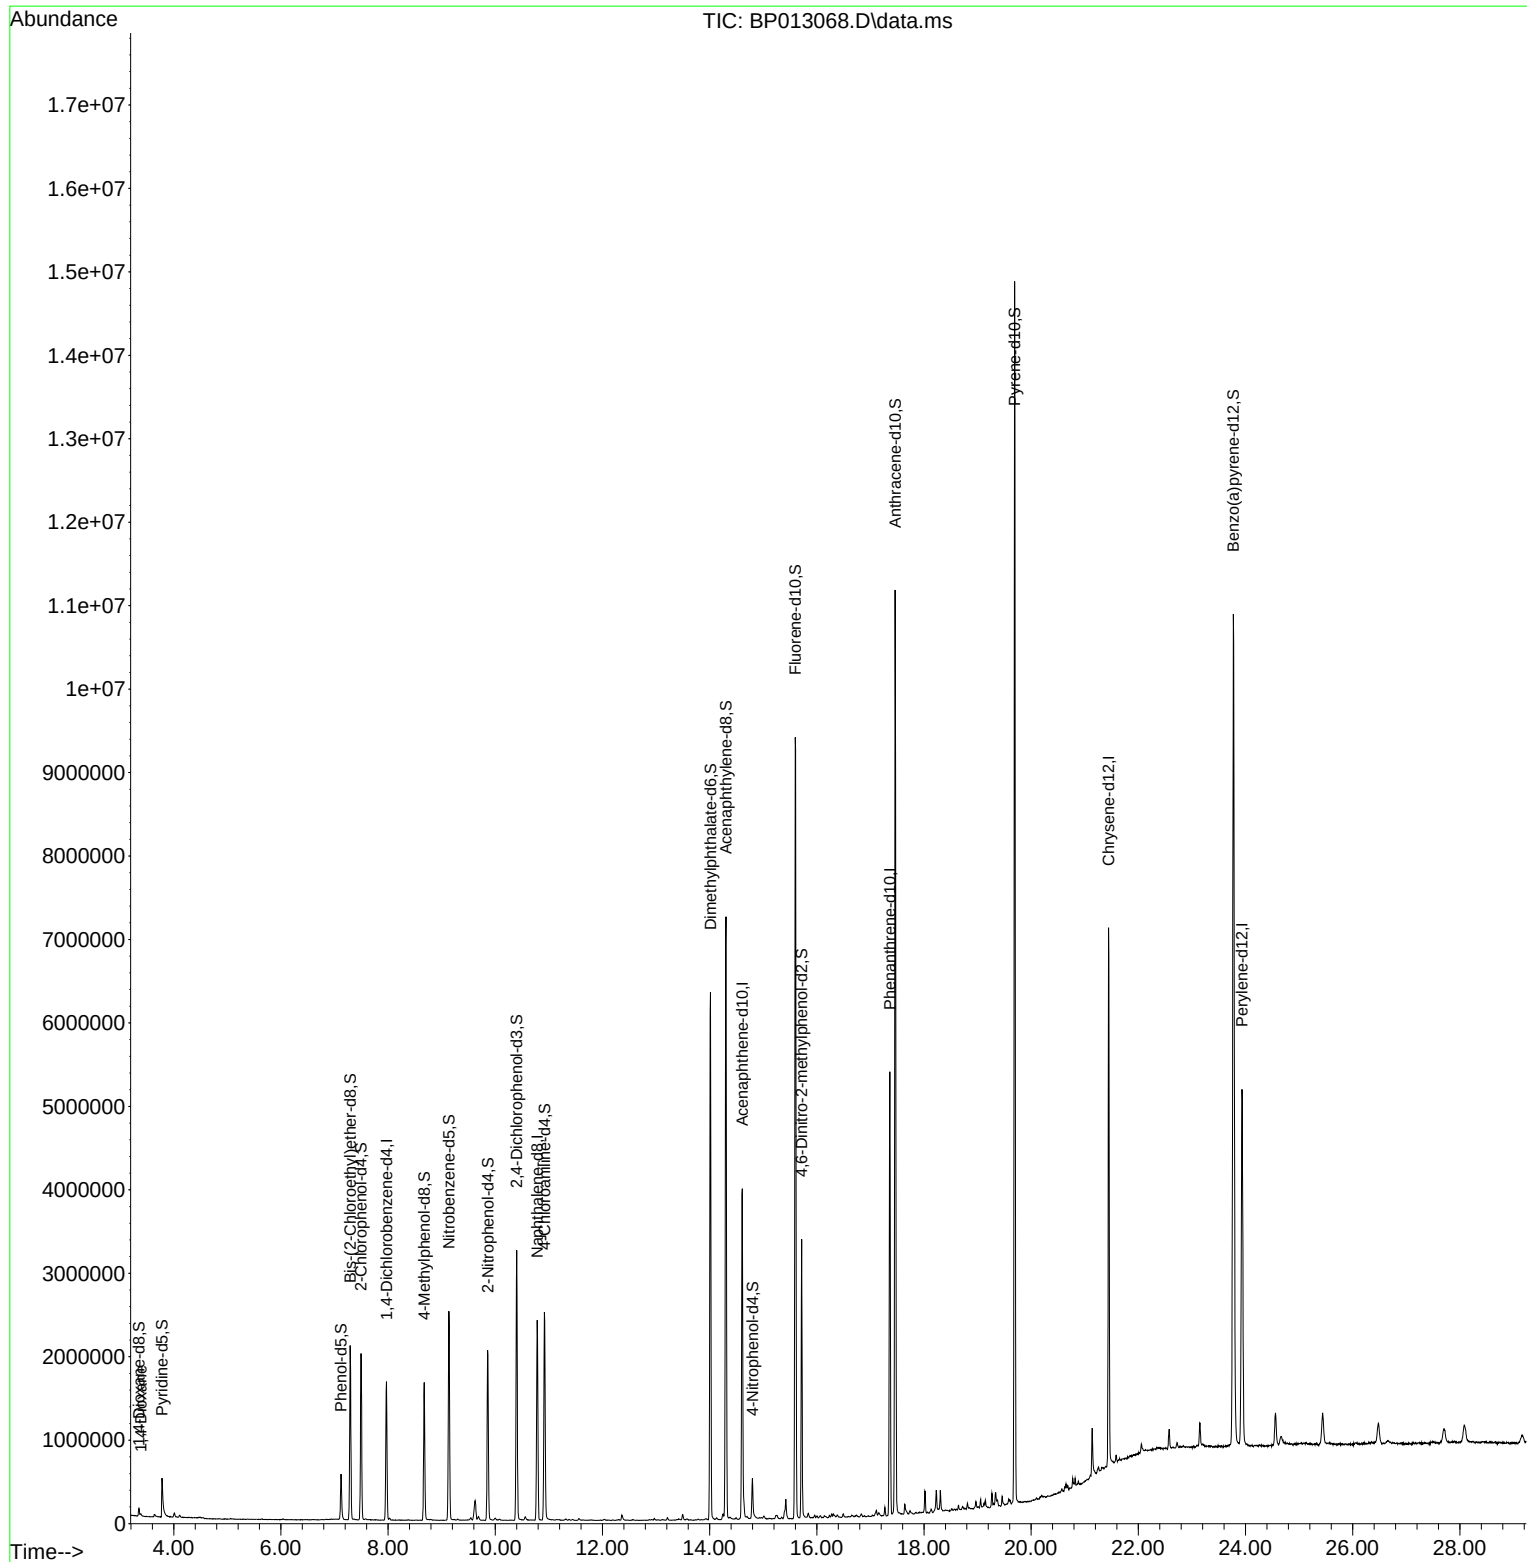

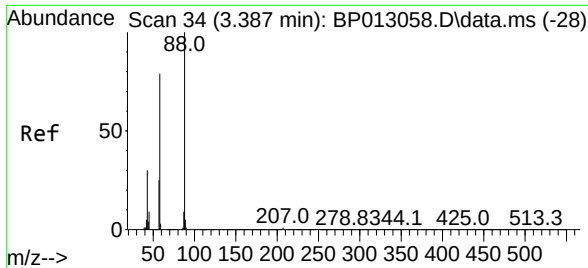

#2
 1,4-Dioxane
 Concen: 1.213 ng/uL
 RT: 3.387 min Scan# 34
 Delta R.T. 0.000 min
 Lab File: BP013068.D
 Acq: 11 Dec 2022 07:47

Instrument :
 BNA_P
 ClientSampleId :
 EXZA2

Tgt Ion:	88	Resp:	13482
Ion	Ratio	Lower	Upper
88	100		
43	38.8	22.4	33.6#
58	64.8	58.2	87.4

