

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
 Data File : BP013032.D
 Acq On : 10 Dec 2022 10:35
 Operator : CG/JU
 Sample : PB149532BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK532

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013032.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.352	24	28	39	rVB	145562	211212	1.39%	0.139%
2	3.781	98	101	118	rBV	1703354	2692486	17.66%	1.775%
3	4.111	154	157	162	rVB	37783	52466	0.34%	0.035%
4	7.128	662	670	681	rBV	2186486	3448885	22.62%	2.274%
5	7.299	692	699	708	rVB	1823592	2842909	18.65%	1.875%
6	7.499	726	733	744	rBV	2247526	3549598	23.28%	2.341%
7	7.969	806	813	822	rBV	2162830	3374592	22.13%	2.225%
8	8.675	924	933	943	rBV	2800372	4452792	29.20%	2.936%
9	9.140	1004	1012	1023	rBV	2200203	3497450	22.94%	2.306%
10	9.716	1103	1110	1114	rBV8	8003	16962	0.11%	0.011%
11	9.863	1126	1135	1145	rBV	1816548	2985655	19.58%	1.969%
12	10.404	1218	1227	1241	rBV	2889110	4763188	31.24%	3.141%
13	10.787	1283	1292	1300	rBV	3102583	5202778	34.12%	3.431%
14	10.922	1307	1315	1328	rBV	2744020	4729881	31.02%	3.119%
15	12.369	1554	1561	1568	rBV2	51303	90732	0.60%	0.060%
16	12.657	1605	1610	1618	rBV9	9190	21482	0.14%	0.014%
17	13.410	1731	1738	1742	rBV9	11834	26095	0.17%	0.017%
18	13.487	1749	1751	1759	rVB7	11225	20428	0.13%	0.013%
19	13.581	1764	1767	1772	rVB7	11088	16916	0.11%	0.011%
20	14.016	1832	1841	1848	rBV	5540159	7579765	49.71%	4.998%
21	14.304	1883	1890	1903	rBV	6162416	9056097	59.40%	5.971%
22	14.610	1935	1942	1950	rBV	5098283	7492500	49.14%	4.940%
23	14.675	1950	1953	1957	rVB4	11792	16647	0.11%	0.011%
24	14.798	1968	1974	1992	rBV	2156951	3407756	22.35%	2.247%
25	14.928	1993	1996	2000	rVV5	24956	44397	0.29%	0.029%
26	14.969	2000	2003	2006	rVV5	20344	31297	0.21%	0.021%
27	15.010	2007	2010	2018	rVB3	22900	37835	0.25%	0.025%
28	15.428	2077	2081	2087	rVB3	15506	23070	0.15%	0.015%
29	15.604	2104	2111	2118	rBV	8097260	11507636	75.48%	7.588%
30	15.657	2118	2120	2125	rVV3	35523	53113	0.35%	0.035%
31	15.722	2125	2131	2147	rVV	2511105	3540346	23.22%	2.334%
32	15.845	2148	2152	2161	rVB2	41343	85389	0.56%	0.056%
33	16.663	2287	2291	2296	rVB6	13494	20530	0.13%	0.014%
34	16.828	2312	2319	2321	rBV8	11917	21408	0.14%	0.014%
35	17.039	2353	2355	2361	rVB7	10828	15337	0.10%	0.010%
36	17.151	2370	2374	2378	rBV3	15069	20448	0.13%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
Data File : BP013032.D
Acq On : 10 Dec 2022 10:35
Operator : CG/JU
Sample : PB149532BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK532

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Title : SVOA CALIBRATION

37	17.369	2404	2411	2421	rBV	6450010	9278341	60.85%	6.118%
38	17.469	2421	2428	2448	rVB	9114554	13138331	86.17%	8.663%
39	18.016	2516	2521	2524	rBV7	8378	15247	0.10%	0.010%
40	18.310	2568	2571	2575	rBV	19018	24520	0.16%	0.016%
41	19.269	2731	2734	2740	rVB3	102740	149298	0.98%	0.098%
42	19.339	2742	2746	2749	rBV	106636	139094	0.91%	0.092%
43	19.698	2800	2807	2819	rBV	11687103	15246808	100.00%	10.053%
44	21.451	3100	3105	3115	rBV	6741272	8823435	57.87%	5.818%
45	23.780	3494	3501	3514	rVB2	5918267	12212022	80.10%	8.052%
46	23.939	3522	3528	3538	rVB2	3760127	7680492	50.37%	5.064%




Sum of corrected areas: 151657666

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
Data File : BP013032.D
Acq On : 10 Dec 2022 10:35
Operator : CG/JU
Sample : PB149532BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK532

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

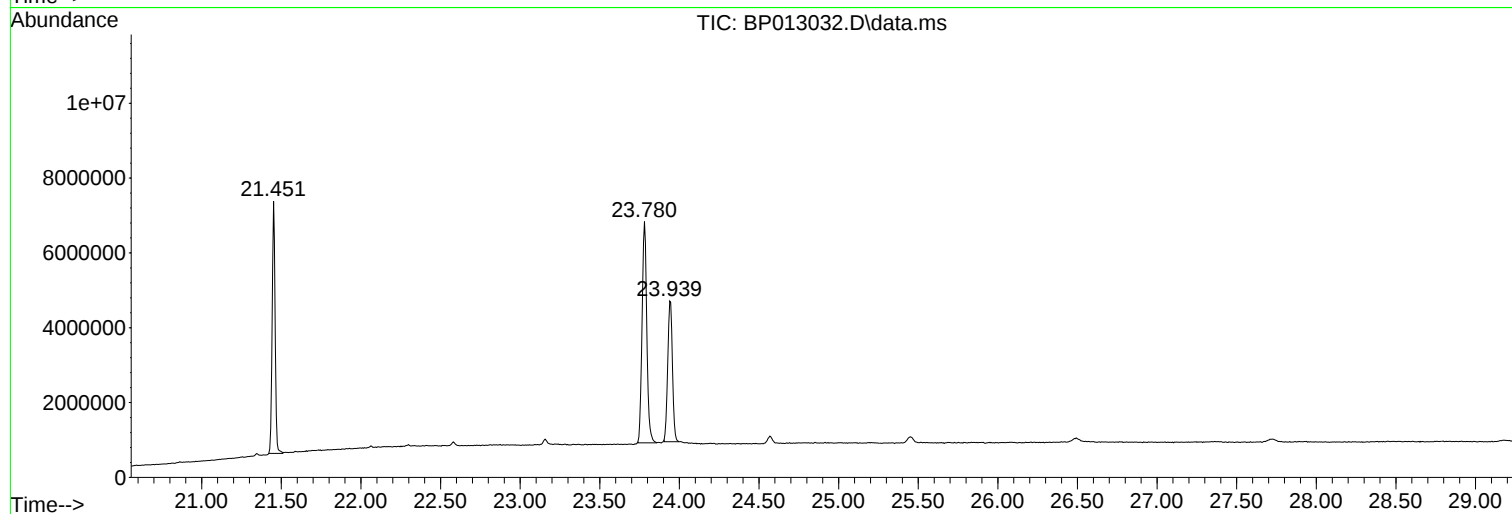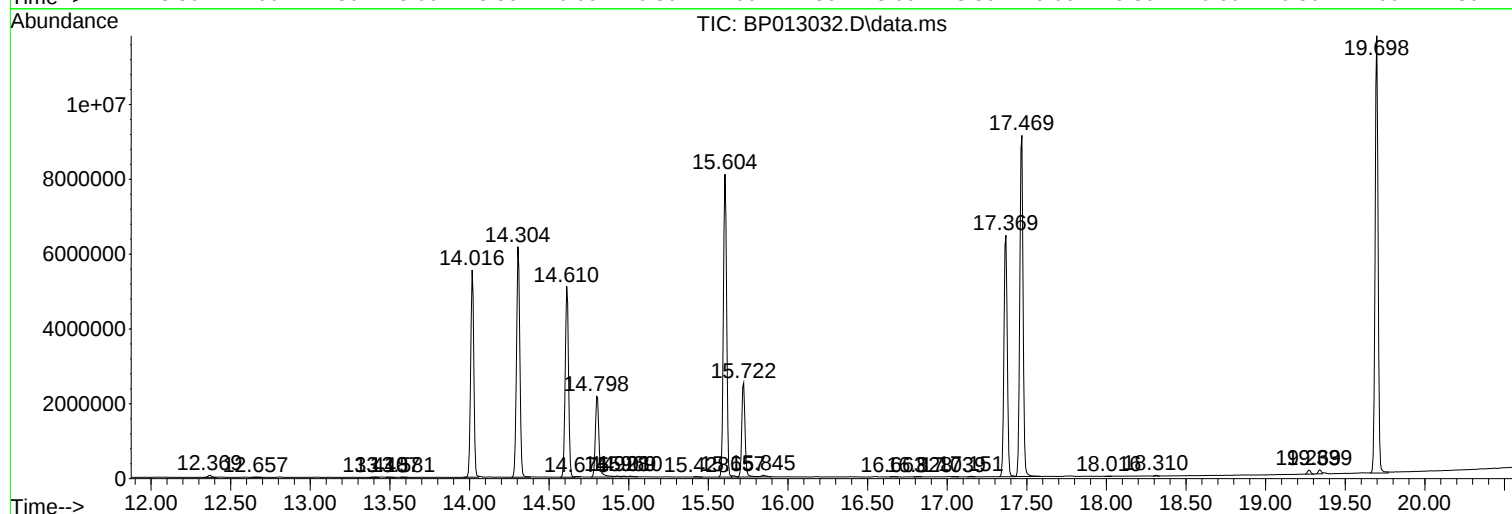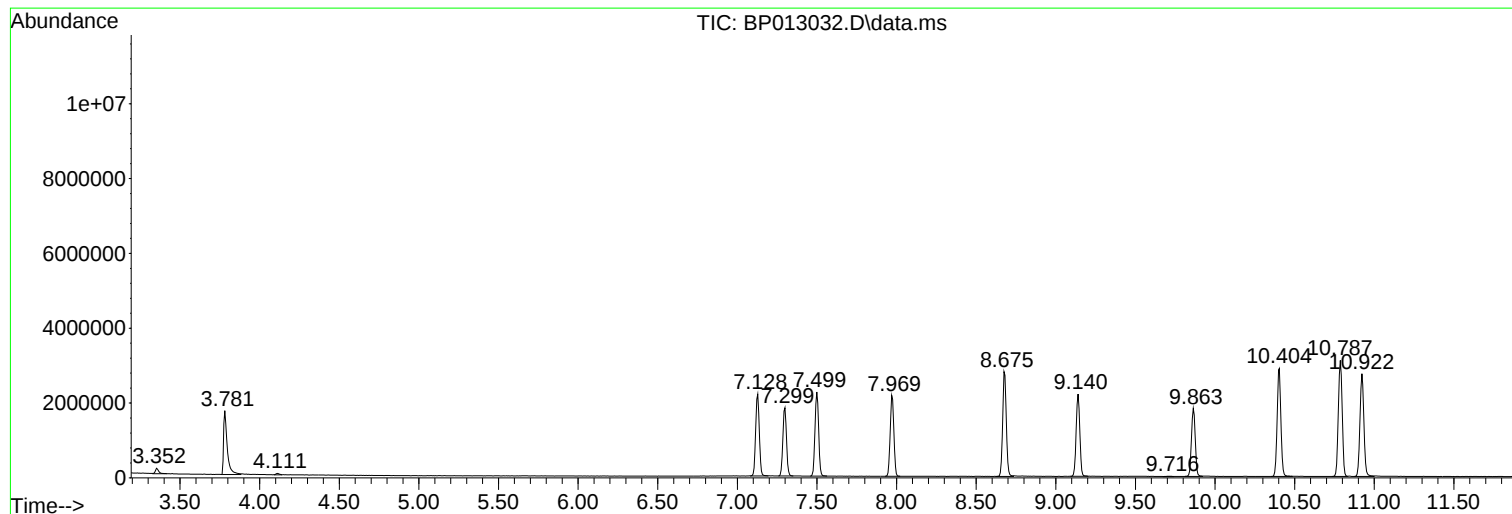

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
Data File : BP013032.D
Acq On : 10 Dec 2022 10:35
Operator : CG/JU
Sample : PB149532BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK532

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
Data File : BP013032.D
Acq On : 10 Dec 2022 10:35
Operator : CG/JU
Sample : PB149532BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK532

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
