

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
 Data File : BP013041.D
 Acq On : 10 Dec 2022 15:53
 Operator : CG/JU
 Sample : PB149500BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK500

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013041.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.352	24	28	39	rVB	163696	238966	1.40%	0.148%
2	3.781	97	101	119	rBV	2042910	3374654	19.82%	2.096%
3	4.116	154	158	164	rVB	28673	41832	0.25%	0.026%
4	7.128	660	670	683	rBV	2739252	4294061	25.22%	2.668%
5	7.299	691	699	709	rVB	2270028	3523423	20.69%	2.189%
6	7.499	725	733	744	rBV	2733933	4277397	25.12%	2.657%
7	7.969	807	813	821	rBV	1653846	2610466	15.33%	1.622%
8	8.675	926	933	951	rBV	3379835	5469373	32.12%	3.398%
9	9.140	1003	1012	1025	rBV	2622591	4311516	25.32%	2.678%
10	9.863	1125	1135	1148	rBV	2265492	3671880	21.57%	2.281%
11	10.399	1219	1226	1244	rBV	3414200	5835598	34.27%	3.625%
12	10.787	1283	1292	1301	rBV	2417775	4070151	23.90%	2.528%
13	10.922	1306	1315	1329	rBV	3366902	5744057	33.74%	3.568%
14	12.369	1555	1561	1569	rVB2	60324	100060	0.59%	0.062%
15	13.498	1749	1753	1760	rVV3	22753	37850	0.22%	0.024%
16	13.581	1763	1767	1772	rVB3	13450	22557	0.13%	0.014%
17	14.016	1834	1841	1853	rBV	6648941	8867154	52.08%	5.508%
18	14.304	1883	1890	1904	rBV	7475794	10855727	63.76%	6.744%
19	14.610	1935	1942	1953	rBV	4053645	5819554	34.18%	3.615%
20	14.798	1966	1974	1995	rBV	2708108	4257466	25.00%	2.645%
21	15.016	2007	2011	2018	rVB8	16348	27845	0.16%	0.017%
22	15.604	2102	2111	2122	rBV	9453962	13718542	80.57%	8.522%
23	15.722	2124	2131	2147	rVV	2836115	4027725	23.66%	2.502%
24	15.845	2147	2152	2159	rVB	46050	81054	0.48%	0.050%
25	16.386	2240	2244	2251	rVB9	11476	20943	0.12%	0.013%
26	17.039	2352	2355	2360	rVB6	15436	22491	0.13%	0.014%
27	17.145	2368	2373	2379	rBV4	10621	23655	0.14%	0.015%
28	17.369	2401	2411	2420	rBV	4876980	7096088	41.68%	4.408%
29	17.469	2420	2428	2449	rVV	10444883	15209186	89.33%	9.448%
30	17.739	2471	2474	2483	rBV4	11637	22278	0.13%	0.014%
31	19.269	2730	2734	2740	rBV	128674	185779	1.09%	0.115%
32	19.339	2742	2746	2750	rVV	120578	159120	0.93%	0.099%
33	19.698	2800	2807	2815	rBV	12512194	17026776	100.00%	10.577%
34	21.345	3084	3087	3091	rBV	117118	134756	0.79%	0.084%
35	21.451	3100	3105	3113	rBV	4896761	6540216	38.41%	4.063%
36	23.780	3493	3501	3516	rVB	6616341	13569133	79.69%	8.429%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
Data File : BP013041.D
Acq On : 10 Dec 2022 15:53
Operator : CG/JU
Sample : PB149500BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK500

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Title : SVOA CALIBRATION

37	23.939	3521	3528	3538	rVB2	2800588	5686699	33.40%	3.533%
----	--------	------	------	------	------	---------	---------	--------	--------




Sum of corrected areas: 160976028

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
Data File : BP013041.D
Acq On : 10 Dec 2022 15:53
Operator : CG/JU
Sample : PB149500BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK500

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

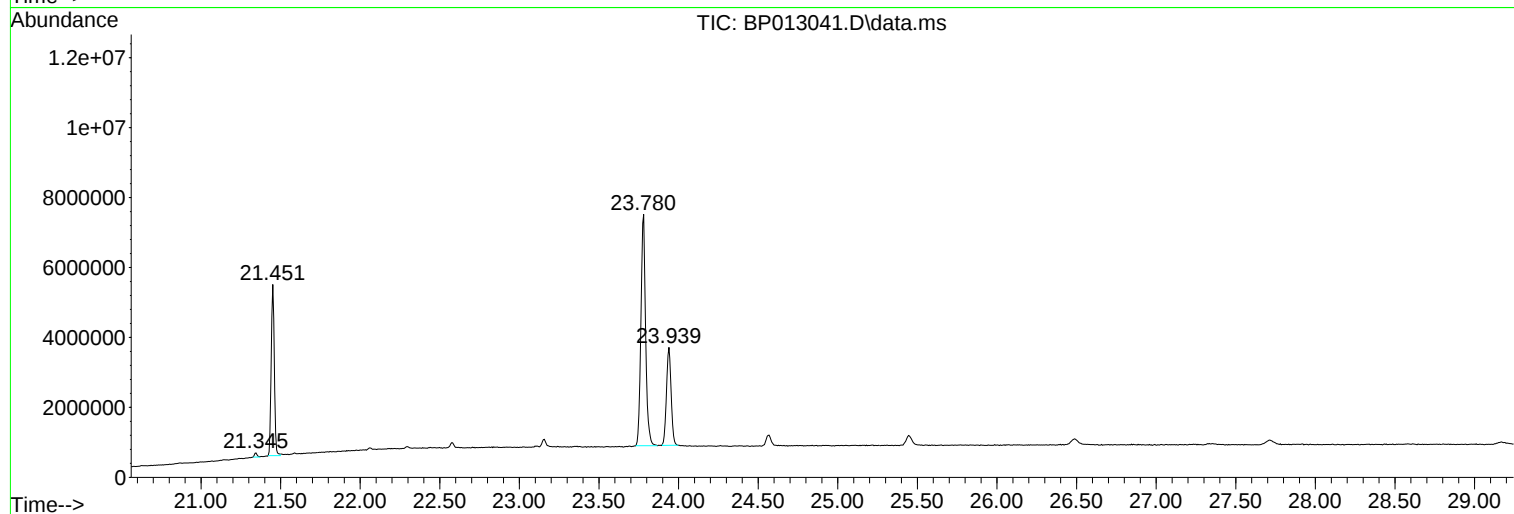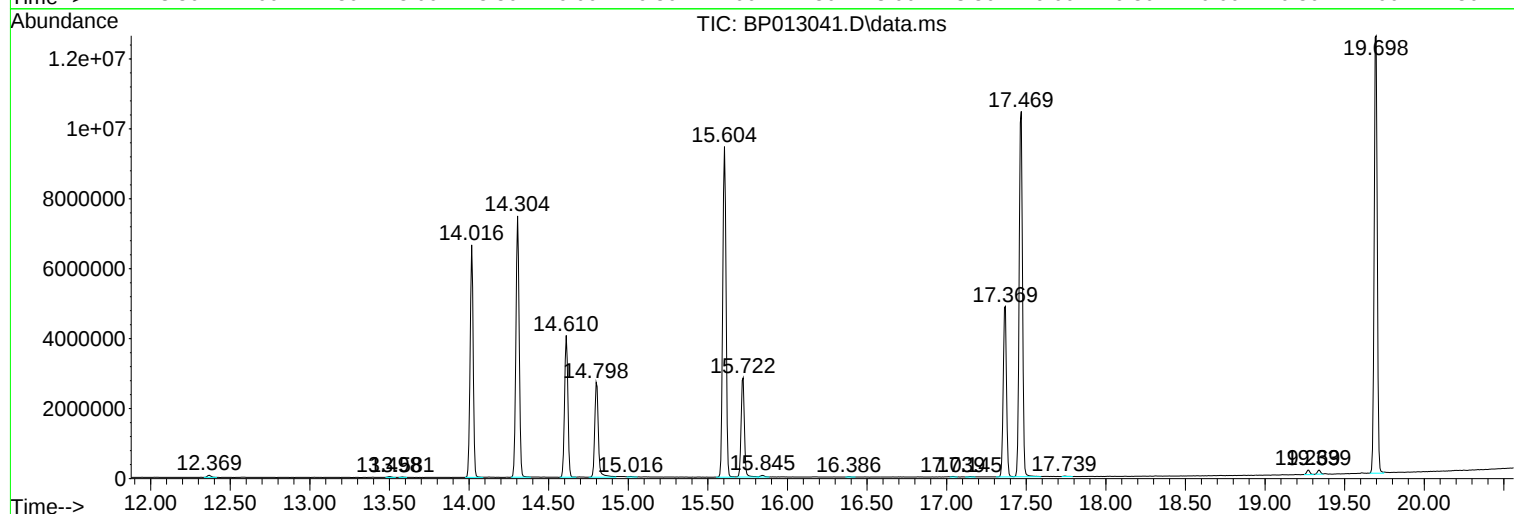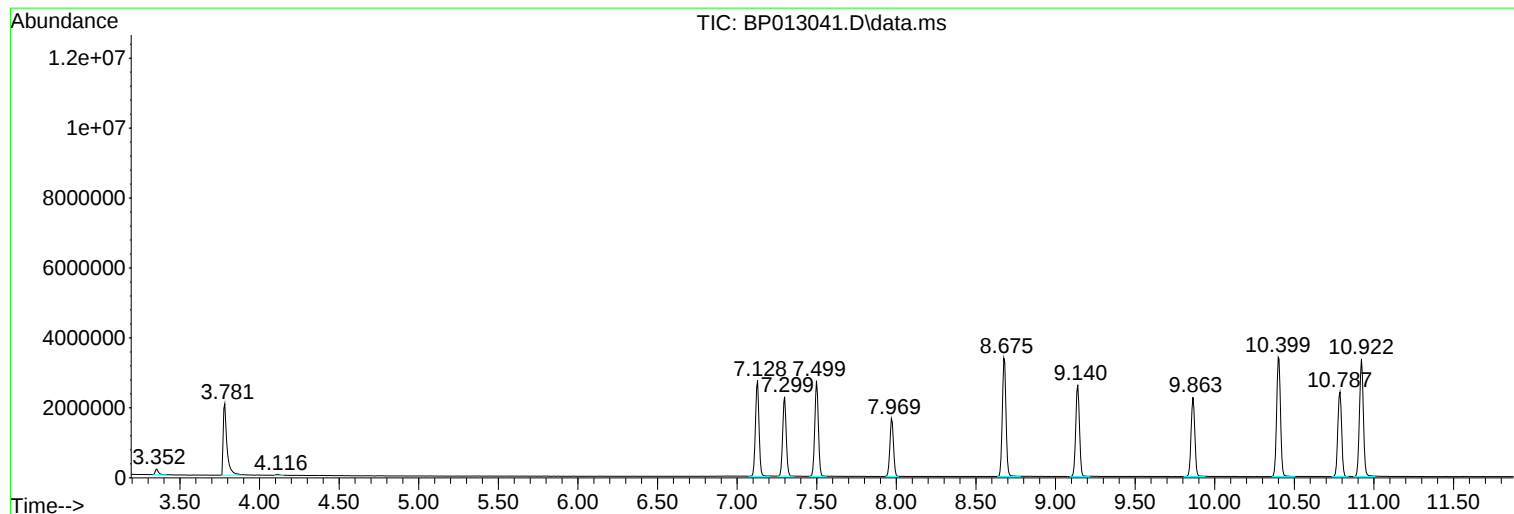

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
Data File : BP013041.D
Acq On : 10 Dec 2022 15:53
Operator : CG/JU
Sample : PB149500BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK500

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
Data File : BP013041.D
Acq On : 10 Dec 2022 15:53
Operator : CG/JU
Sample : PB149500BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK500

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc